

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011722\
 Data File : PS018039.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jan 2022 08:44
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 17 14:33:14 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 06 10:21:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.049	6.646	734.7E6	307.5E6	508.267	529.888
Target Compounds							
9) T	2,4-D	8.216f	0.000	14849858	0	8.155	N.D. #
11) T	2,4,5-TP ...	0.000	8.442	0	9851184	N.D.	2.764
12) T	2,4,5-T	9.293	0.000	11494647	0	1.297	N.D. #
13) T	2,4-DB	9.842	0.000	12760067	0	7.719	N.D. #
14) T	DINOSEB	10.977	0.000	4151056	0	<MDL	N.D. #
15) T	Picloram	10.815	10.672	246.2E6	89713619	20.625	19.185
16) T	DCPA	11.248	0.000	3981069	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011722\
Data File : PS018039.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jan 2022 08:44
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 17 14:33:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
Quant Title : 8080.M
QLast Update : Thu Jan 06 10:21:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

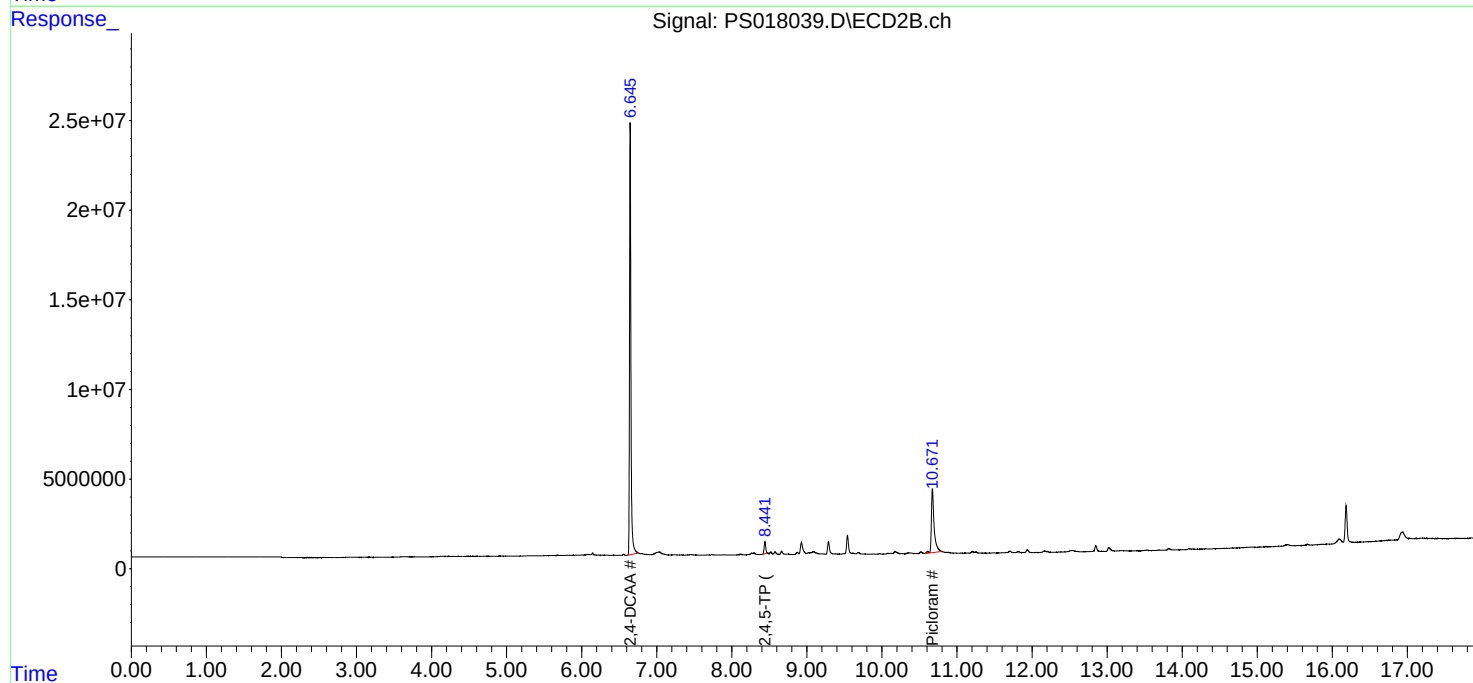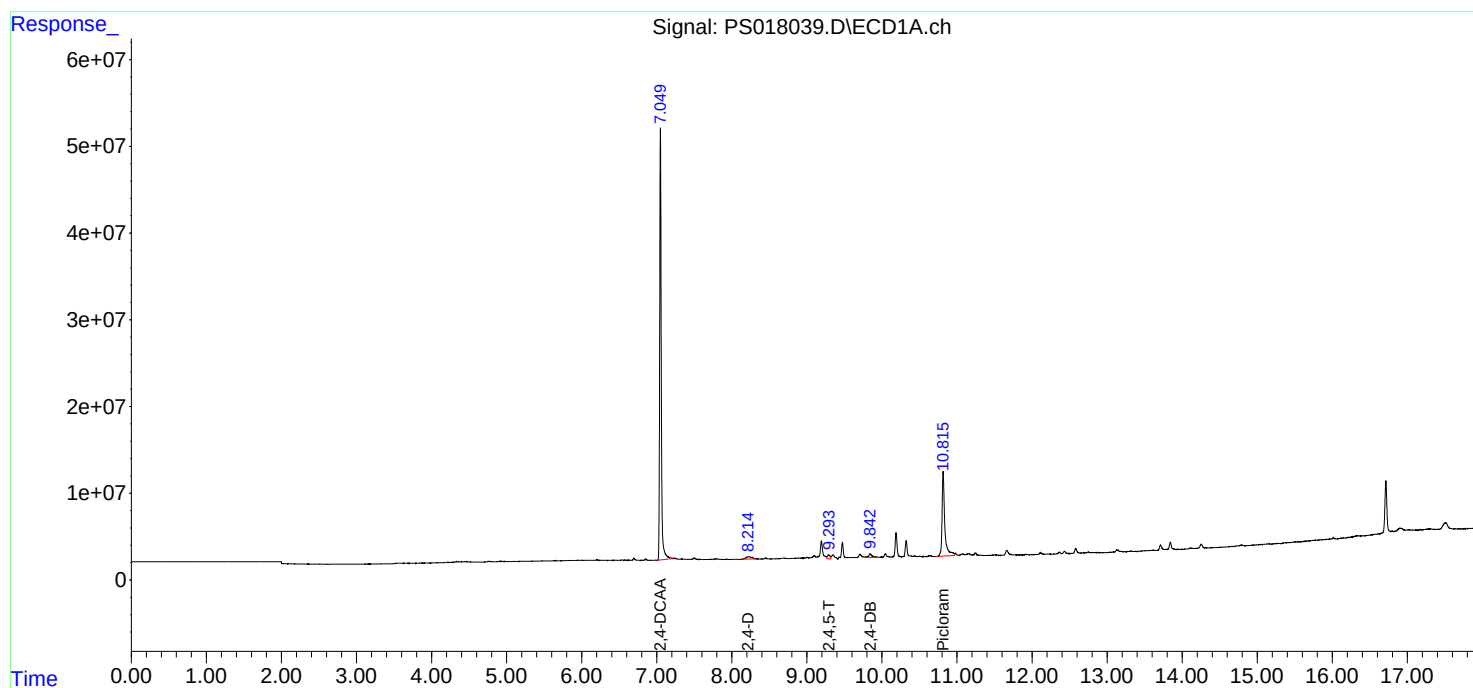


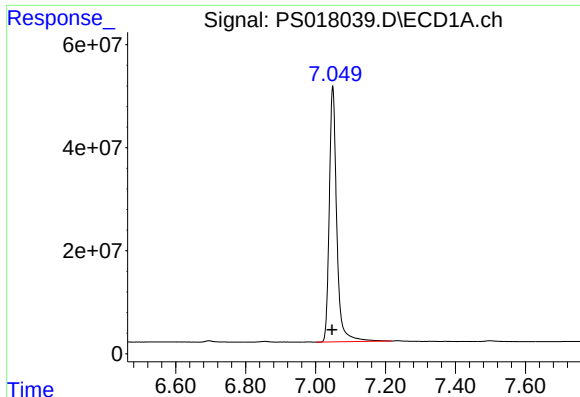

#4 2,4-DCAA


R.T.: 7.049 min
Delta R.T.: 0.002 min
Response: 734693547
Conc: 508.27 ng/ml

Instrument :
ECD_S
ClientSampleId :

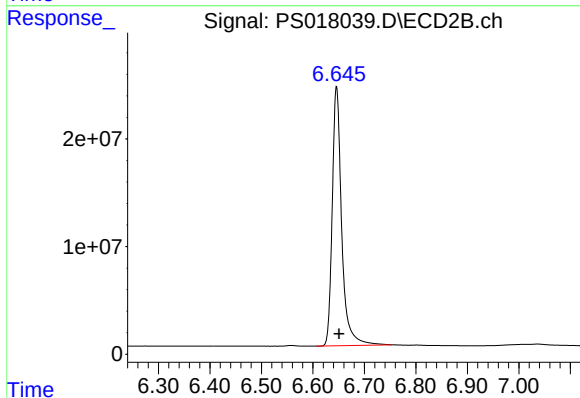


#4 2,4-DCAA

R.T.: 6.646 min
Delta R.T.: -0.005 min
Response: 307466847
Conc: 529.89 ng/ml

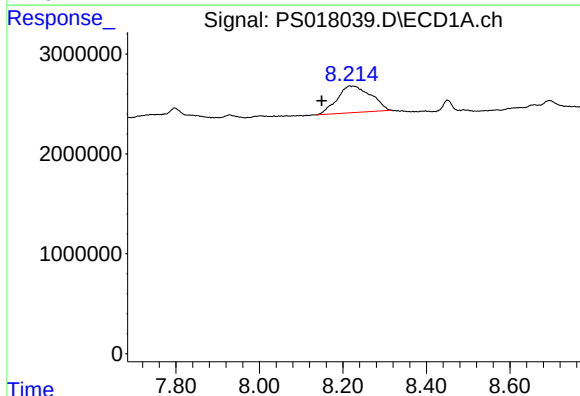


#9 2,4-D

R.T.: 8.216 min
Delta R.T.: 0.067 min
Response: 14849858
Conc: 8.16 ng/ml

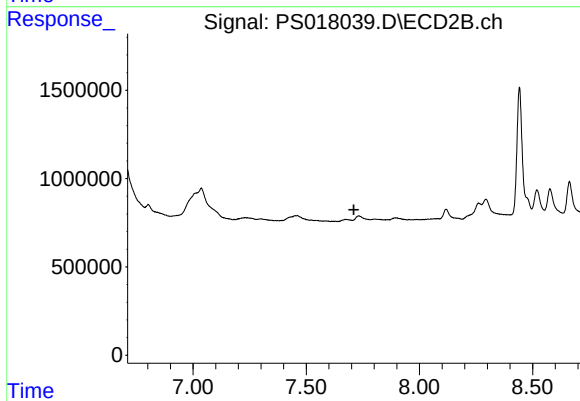

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.710 min
Response: 0
Conc: N.D.

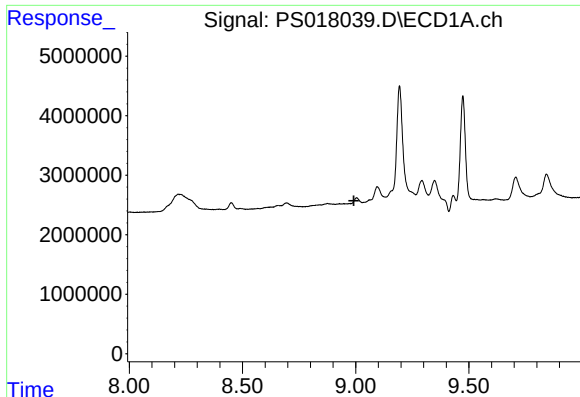

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 8.992 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

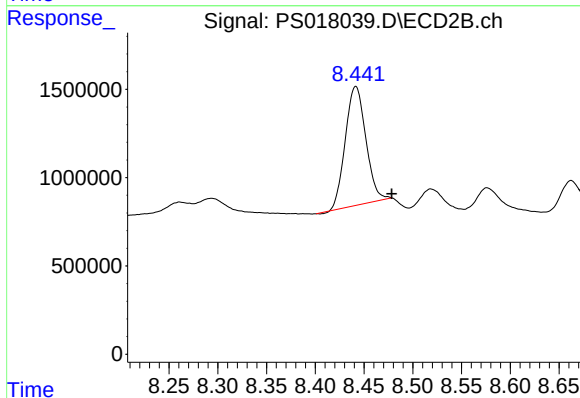


#11 2,4,5-TP (SILVEX)

R.T.: 8.442 min
Delta R.T.: -0.037 min
Response: 9851184
Conc: 2.76 ng/ml

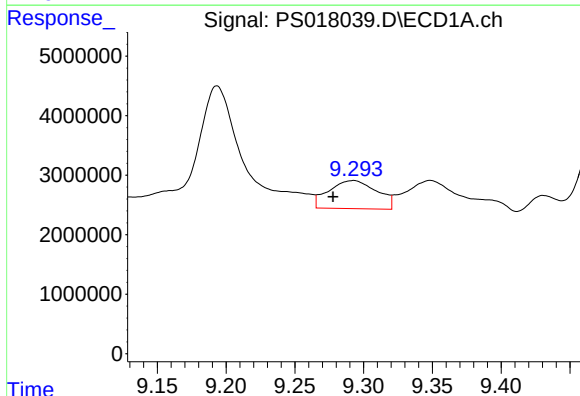


#12 2,4,5-T

R.T.: 9.293 min
Delta R.T.: 0.015 min
Response: 11494647
Conc: 1.30 ng/ml

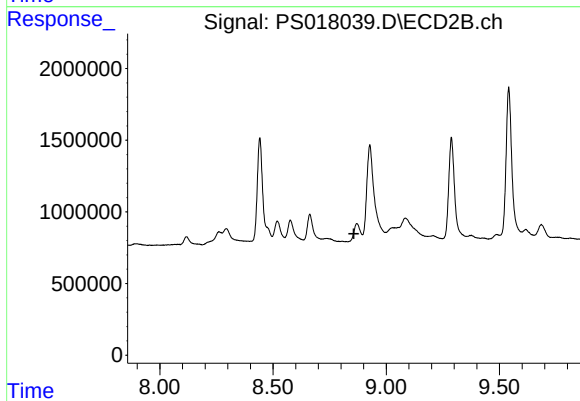

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 8.857 min
Response: 0
Conc: N.D.

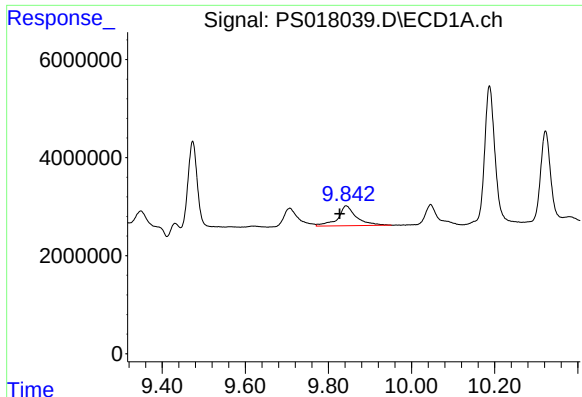

#13 2,4-DB


R.T.: 9.842 min
Delta R.T.: 0.015 min
Response: 12760067
Conc: 7.72 ng/ml

Instrument :
ECD_S
ClientSampleId :

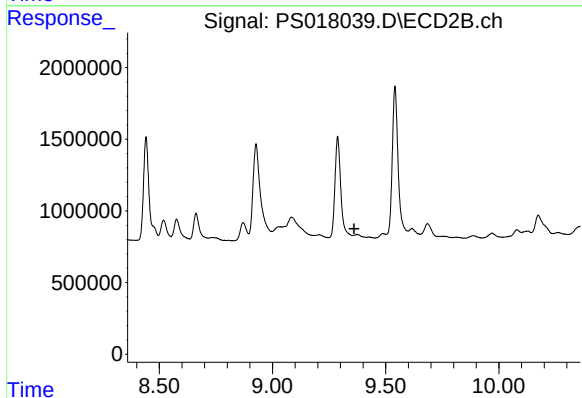


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.360 min
Response: 0
Conc: N.D.

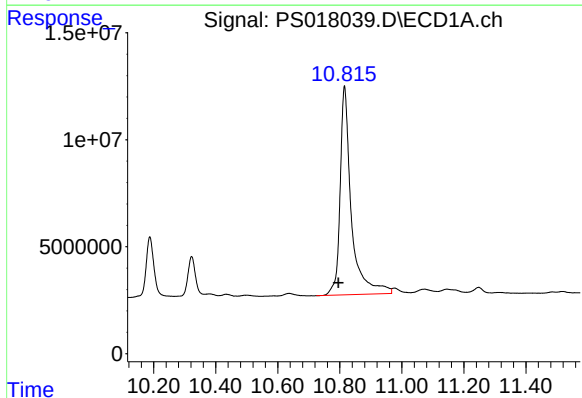

#15 Picloram

R.T.: 10.815 min
Delta R.T.: 0.019 min
Response: 246181077
Conc: 20.63 ng/ml

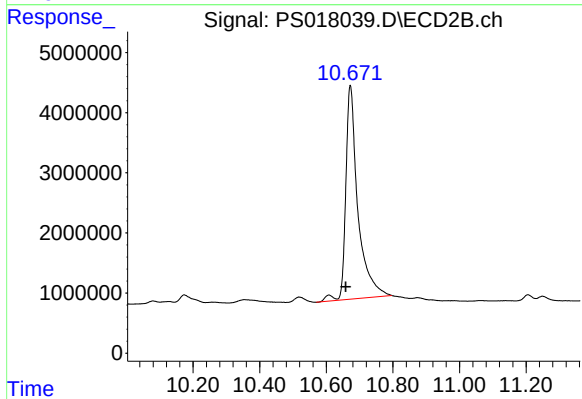

#15 Picloram

R.T.: 10.672 min
Delta R.T.: 0.013 min
Response: 89713619
Conc: 19.19 ng/ml