

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011722\
 Data File : PS018043.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jan 2022 11:36
 Operator : AJ\MA
 Sample : N1121-03MSD
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 WASTE-CLASS-LAUNDRY-PITMSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 17 14:34:01 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 06 10:21:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.043	6.643	327.9E6	167.9E6	226.865	289.343 #
Target Compounds							
1) T	Dalapon	2.907	2.407	713.3E6	894.7E6	290.748	1170.012 #
2) T	3,5-DICHL...	6.284	5.859	685.7E6	264.7E6	318.759	299.278
3) T	4-Nitroph...	6.869	6.323	217.5E6	57302773	269.302	186.945 #
5) T	DICAMBA	7.232	6.799	2789.4E6	1185.2E6	446.709	450.793
6) T	MCPD	7.402	6.904	85471203	113.2E6	18.306	52.620 #
7) T	MCPA	7.556	7.104	401.5E6	194.9E6	60.185	65.300
8) T	DICHLORPROP	7.919	7.410	801.0E6	432.5E6	509.229	647.954 #
9) T	2,4-D	8.144	7.695	1110.0E6	311.8E6	609.563	423.702 #
10) T	Pentachlo...	8.445	8.112	3868.7E6	1416.4E6	183.126	168.167
11) T	2,4,5-TP ...	8.996	8.464	4786.8E6	3936.7E6	565.676	1104.364 #
12) T	2,4,5-T	9.281	8.875	4544.9E6	2521.2E6	512.724	770.763 #
13) T	2,4-DB	9.827	9.368	1459.4E6	1188.3E6	882.835	2685.722 #
14) T	DINOSEB	10.911f	9.720f	24829.0E6	4616.7E6	3780.907	1850.362 #
15) T	Picloram	10.772	10.667	30303.1E6	6379.7E6	2538.816	1364.302 #
16) T	DCPA	11.243	10.603	4416.7E6	2684.1E6	408.775	607.884 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011722\
Data File : PS018043.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jan 2022 11:36
Operator : AJ\MA
Sample : N1121-03MSD
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
WASTE-CLASS-LAUNDRY-PITMSD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 17 14:34:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
Quant Title : 8080.M
QLast Update : Thu Jan 06 10:21:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

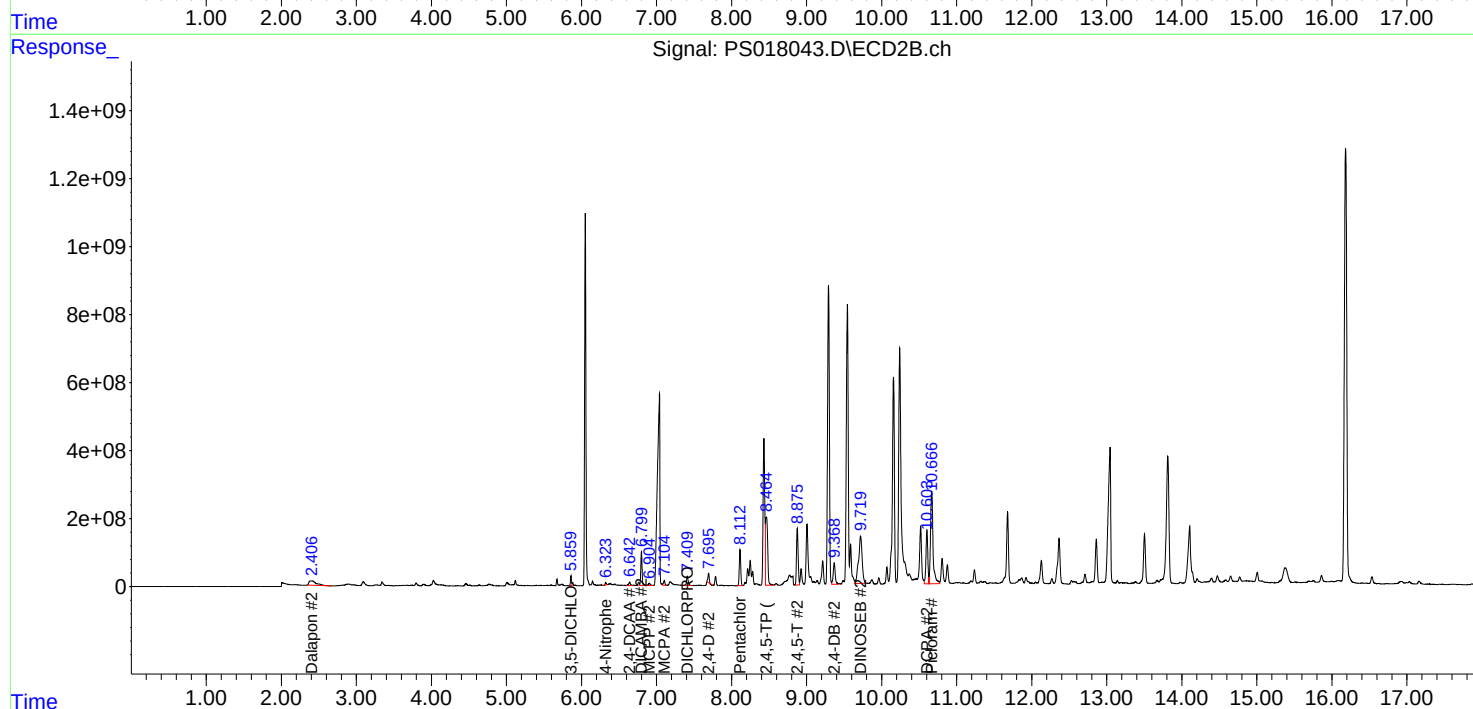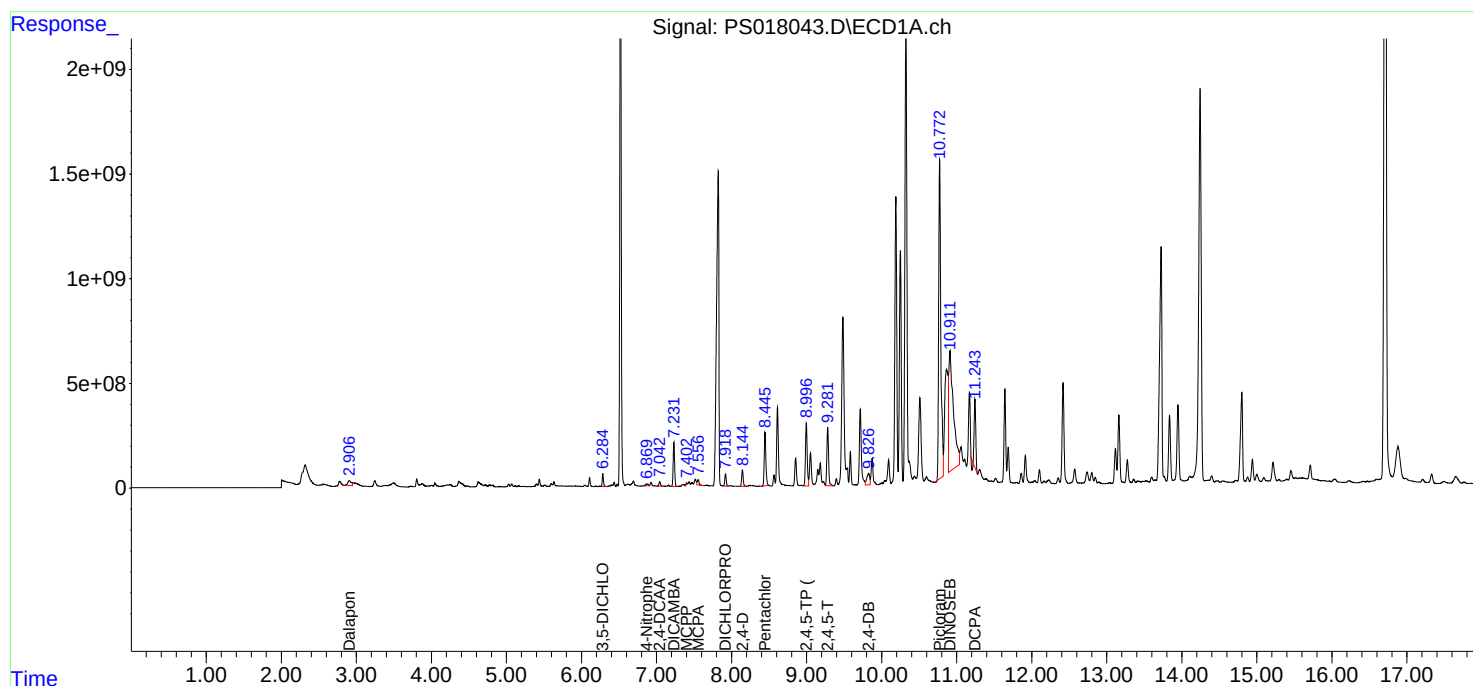


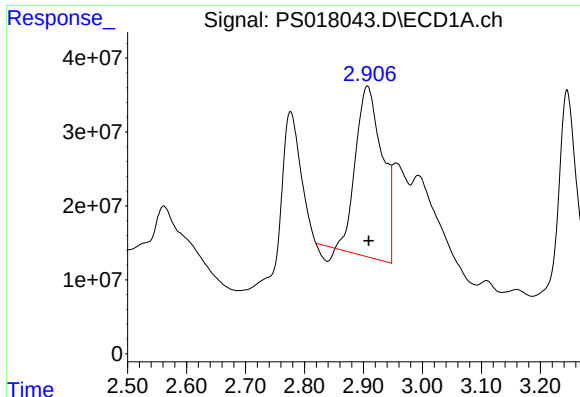

#1 Dalapon


R.T.: 2.907 min
Delta R.T.: -0.002 min
Response: 713270758
Conc: 290.75 ng/ml

Instrument :
ECD_S
ClientSampleId :
WASTE-CLASS-LAUNDRY-PITMSD

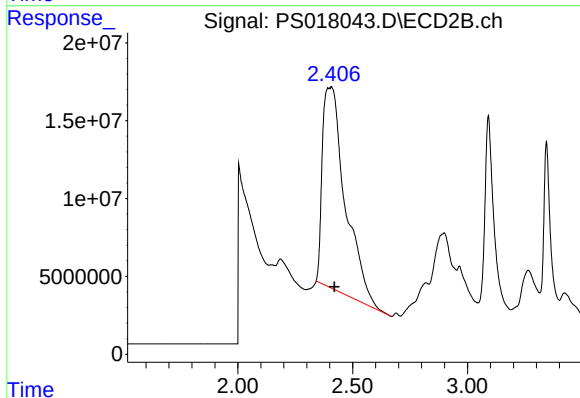


#1 Dalapon

R.T.: 2.407 min
Delta R.T.: -0.014 min
Response: 894694560
Conc: 1170.01 ng/ml

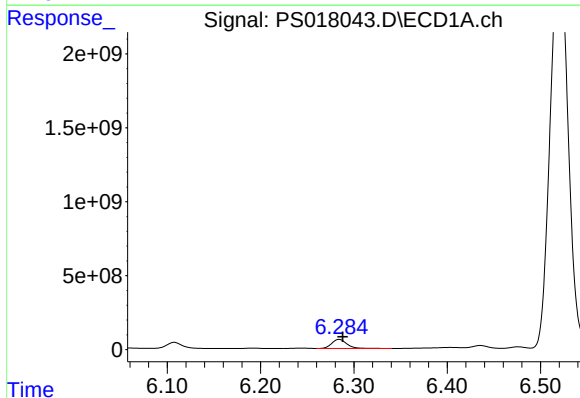


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.284 min
Delta R.T.: -0.004 min
Response: 685728973
Conc: 318.76 ng/ml

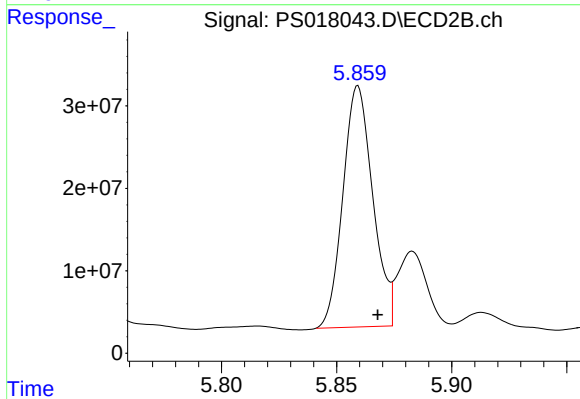

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.859 min
Delta R.T.: -0.009 min
Response: 264749991
Conc: 299.28 ng/ml

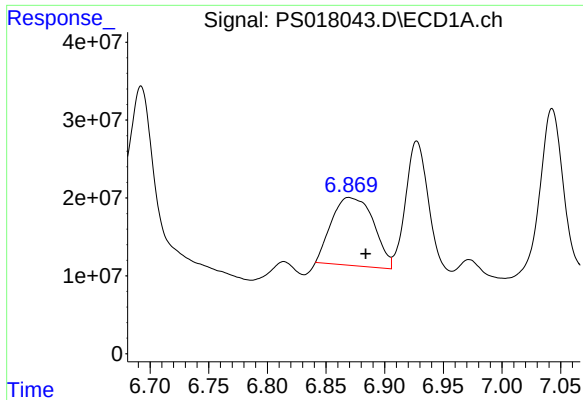

#3 4-Nitrophenol


R.T.: 6.869 min
Delta R.T.: -0.015 min
Response: 217511195
Conc: 269.30 ng/ml

Instrument :
ECD_S
ClientSampleId :
WASTE-CLASS-LAUNDRY-PITMSD

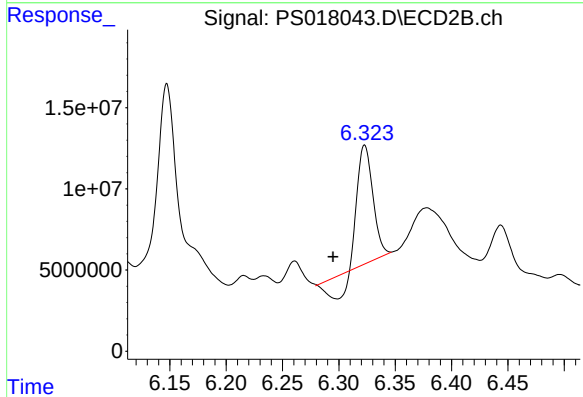


#3 4-Nitrophenol

R.T.: 6.323 min
Delta R.T.: 0.028 min
Response: 57302773
Conc: 186.94 ng/ml

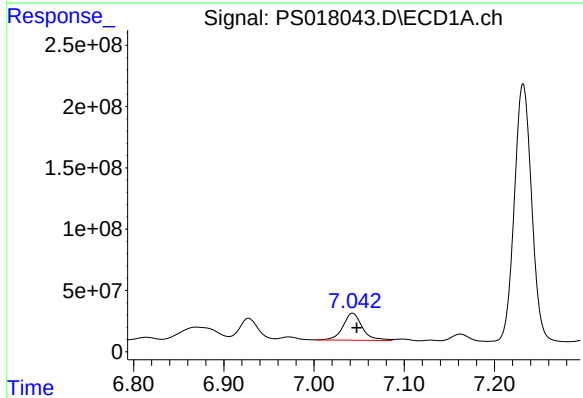


#4 2,4-DCAA

R.T.: 7.043 min
Delta R.T.: -0.005 min
Response: 327930646
Conc: 226.87 ng/ml

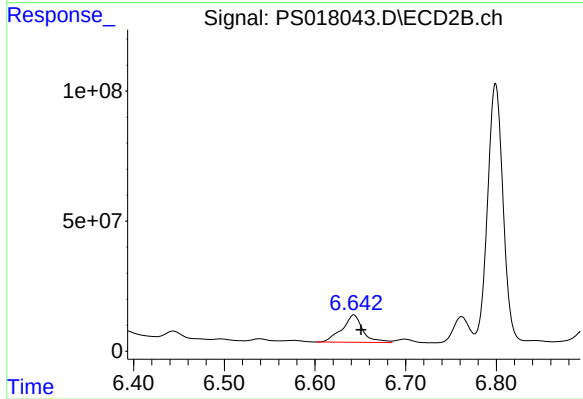

#4 2,4-DCAA


R.T.: 6.643 min
Delta R.T.: -0.008 min
Response: 167890691
Conc: 289.34 ng/ml

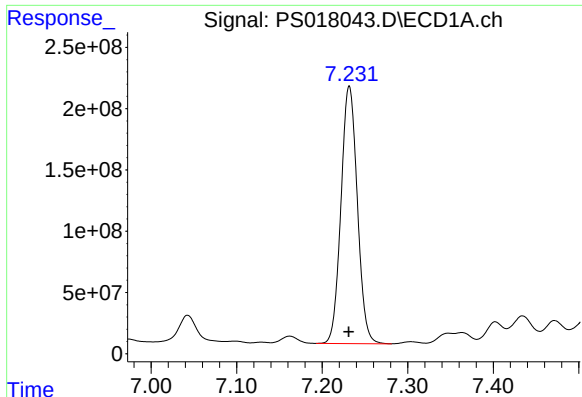

#5 DICAMBA


R.T.: 7.232 min
Delta R.T.: 0.000 min
Response: 2789433644
Conc: 446.71 ng/ml

Instrument :
ECD_S
ClientSampleId :
WASTE-CLASS-LAUNDRY-PITMSD

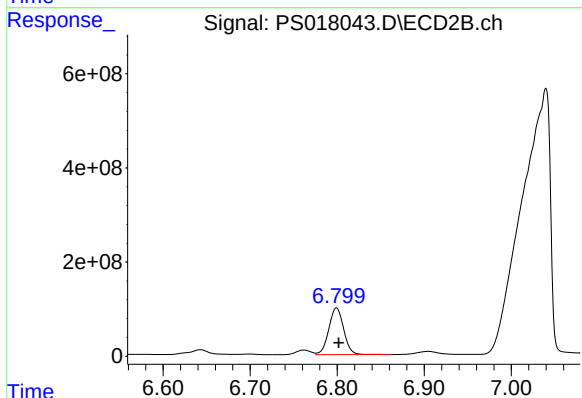


#5 DICAMBA

R.T.: 6.799 min
Delta R.T.: -0.003 min
Response: 1185159930
Conc: 450.79 ng/ml

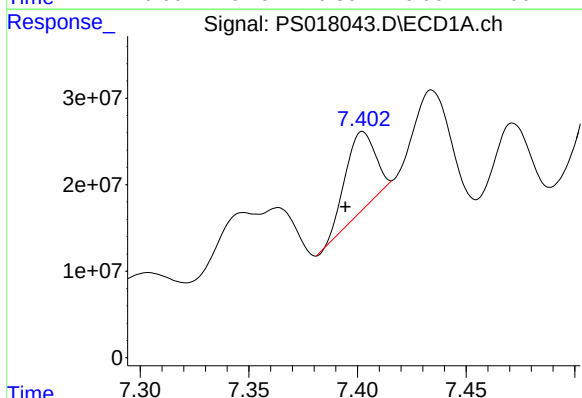


#6 MCPP

R.T.: 7.402 min
Delta R.T.: 0.008 min
Response: 85471203
Conc: 18.31 ug/ml

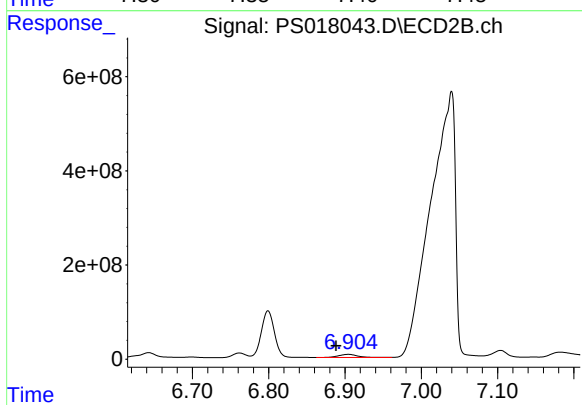

#6 MCPP


R.T.: 6.904 min
Delta R.T.: 0.016 min
Response: 113181507
Conc: 52.62 ug/ml

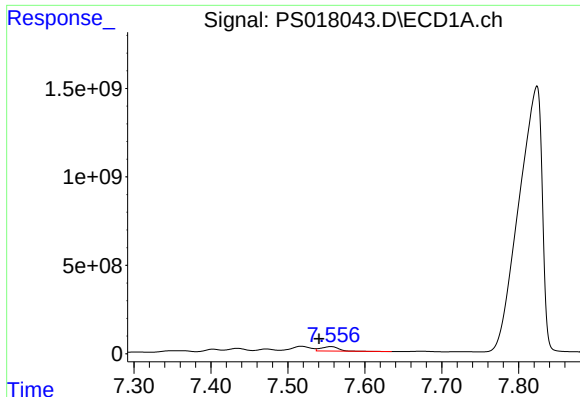

#7 MCPA


R.T.: 7.556 min
Delta R.T.: 0.016 min
Response: 401536807
Conc: 60.18 ug/ml

Instrument :
ECD_S
ClientSampleId :
WASTE-CLASS-LAUNDRY-PITMSD

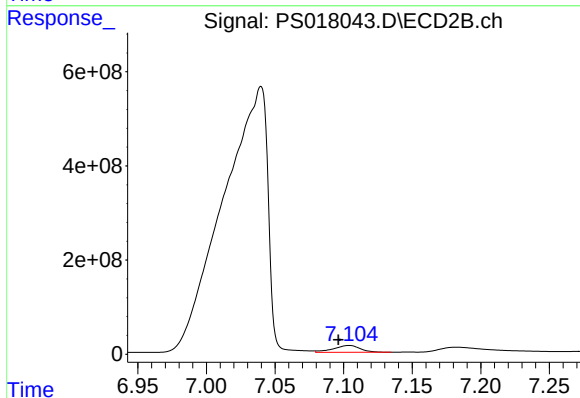


#7 MCPA

R.T.: 7.104 min
Delta R.T.: 0.008 min
Response: 194850900
Conc: 65.30 ug/ml

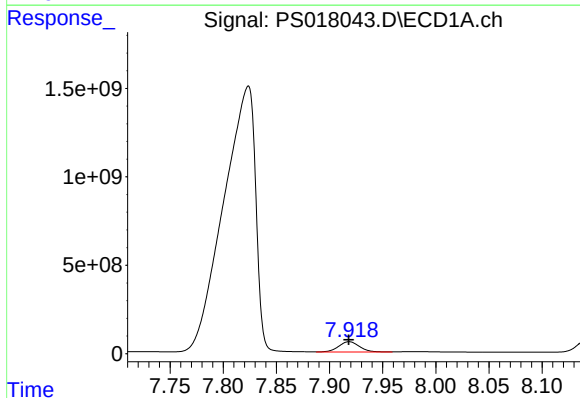


#8 DICHLORPROP

R.T.: 7.919 min
Delta R.T.: 0.000 min
Response: 801040305
Conc: 509.23 ng/ml

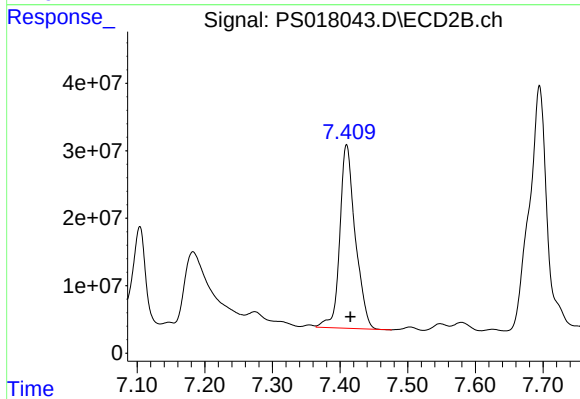

#8 DICHLORPROP


R.T.: 7.410 min
Delta R.T.: -0.005 min
Response: 432460108
Conc: 647.95 ng/ml

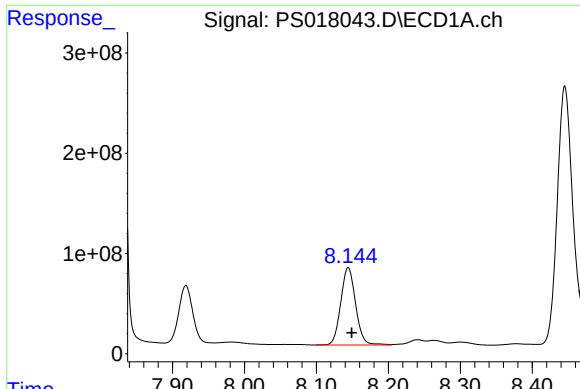

#9 2,4-D


R.T.: 8.144 min
Delta R.T.: -0.005 min
Response: 1109975132
Conc: 609.56 ng/ml

Instrument :
ECD_S
ClientSampleId :
WASTE-CLASS-LAUNDRY-PITMSD

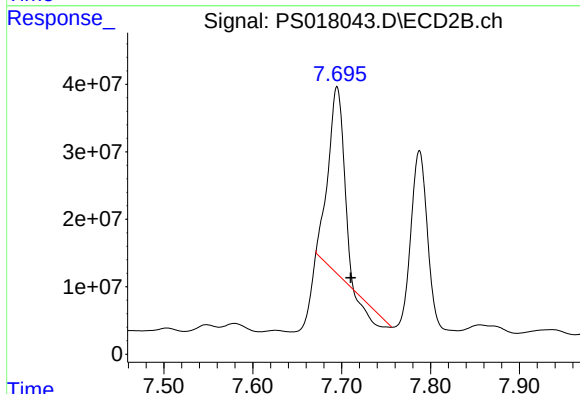


#9 2,4-D

R.T.: 7.695 min
Delta R.T.: -0.015 min
Response: 311821879
Conc: 423.70 ng/ml

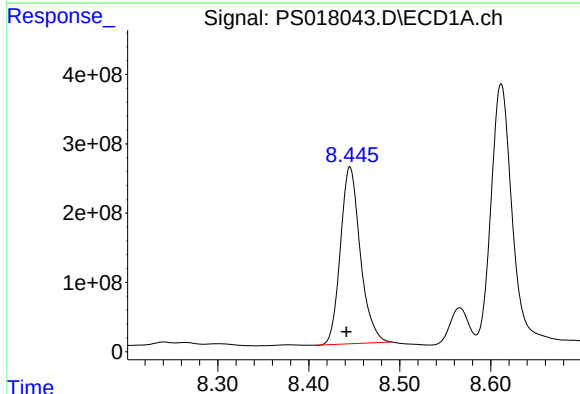


#10 Pentachlorophenol

R.T.: 8.445 min
Delta R.T.: 0.004 min
Response: 3868728366
Conc: 183.13 ng/ml

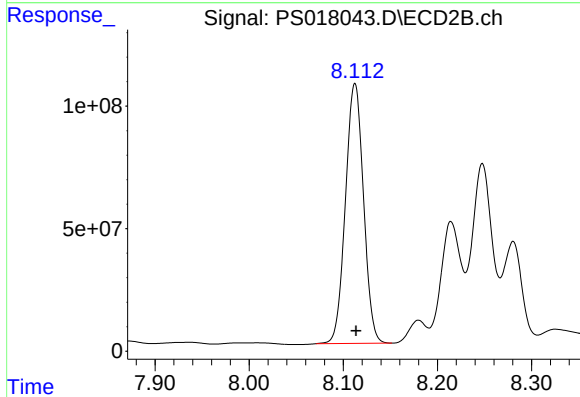

#10 Pentachlorophenol


R.T.: 8.112 min
Delta R.T.: -0.001 min
Response: 1416365158
Conc: 168.17 ng/ml

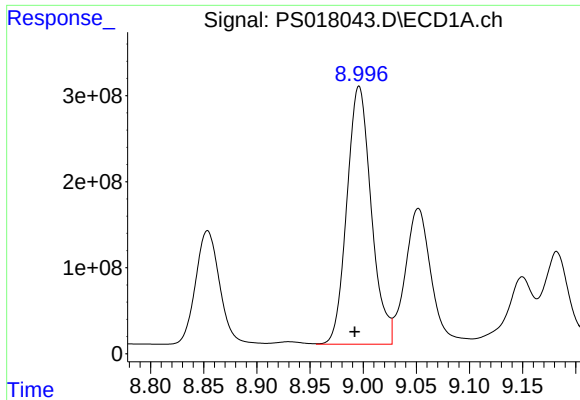

#11 2,4,5-TP (SILVEX)


R.T.: 8.996 min
Delta R.T.: 0.004 min
Response: 4786826131
Conc: 565.68 ng/ml

Instrument :
ECD_S
ClientSampleId :
WASTE-CLASS-LAUNDRY-PITMSD

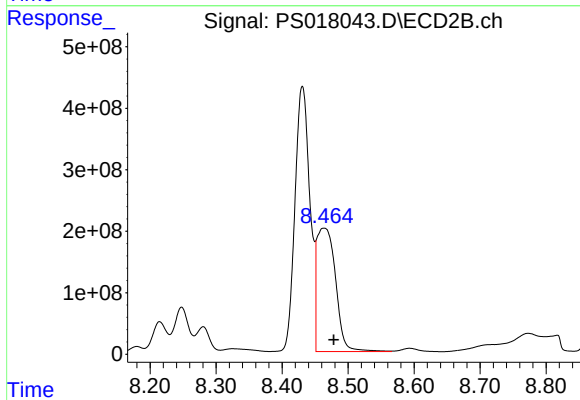


#11 2,4,5-TP (SILVEX)

R.T.: 8.464 min
Delta R.T.: -0.015 min
Response: 3936719053
Conc: 1104.36 ng/ml

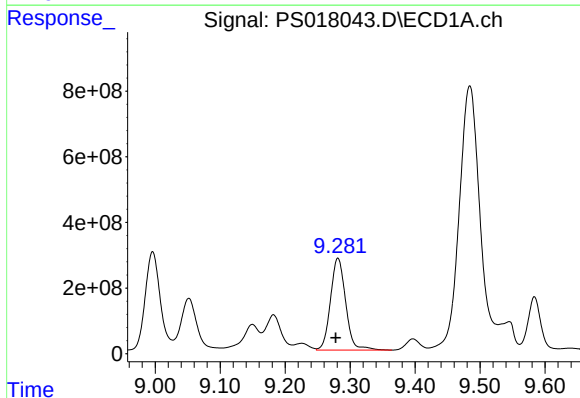


#12 2,4,5-T

R.T.: 9.281 min
Delta R.T.: 0.003 min
Response: 4544853739
Conc: 512.72 ng/ml

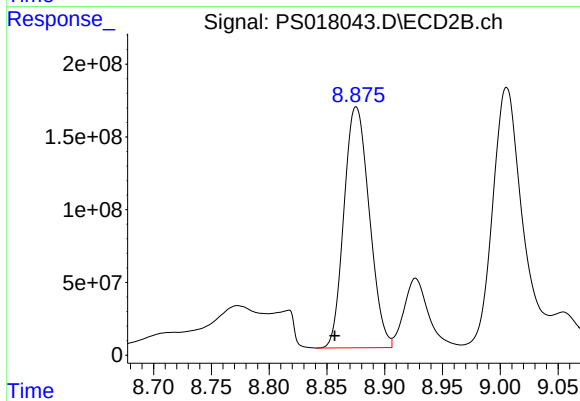

#12 2,4,5-T


R.T.: 8.875 min
Delta R.T.: 0.019 min
Response: 2521177124
Conc: 770.76 ng/ml

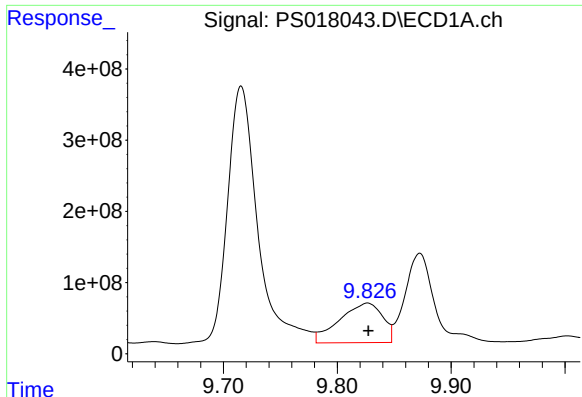

#13 2,4-DB


R.T.: 9.827 min
Delta R.T.: 0.000 min
Response: 1459356518
Conc: 882.84 ng/ml

Instrument :
ECD_S
ClientSampleId :
WASTE-CLASS-LAUNDRY-PITMSD

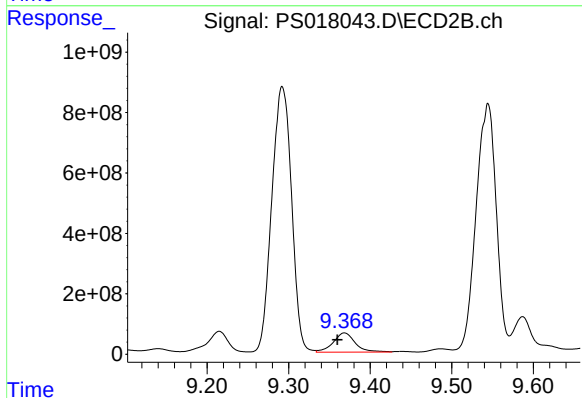


#13 2,4-DB

R.T.: 9.368 min
Delta R.T.: 0.009 min
Response: 1188317000
Conc: 2685.72 ng/ml

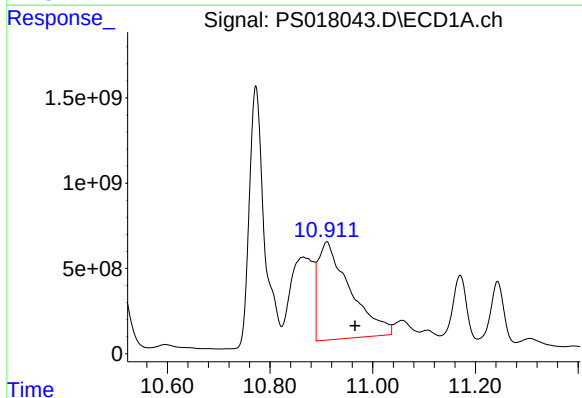


#14 DINOSEB

R.T.: 10.911 min
Delta R.T.: -0.055 min
Response: 24829008429
Conc: 3780.91 ng/ml

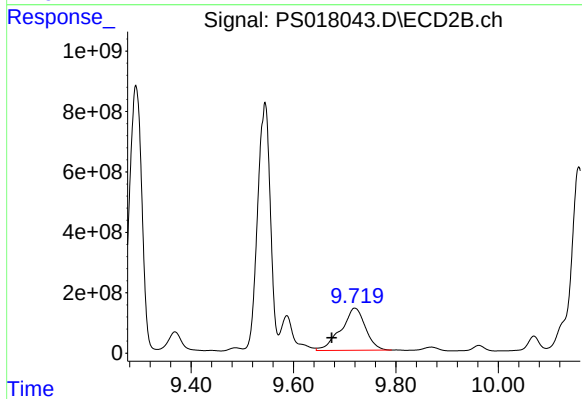

#14 DINOSEB


R.T.: 9.720 min
Delta R.T.: 0.045 min
Response: 4616682678
Conc: 1850.36 ng/ml

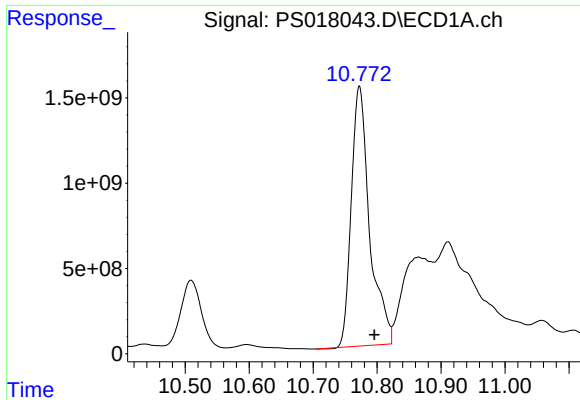

#15 Picloram


R.T.: 10.772 min
Delta R.T.: -0.024 min
Response: 30303087282
Conc: 2538.82 ng/ml

Instrument :
ECD_S
ClientSampleId :
WASTE-CLASS-LAUNDRY-PITMSD

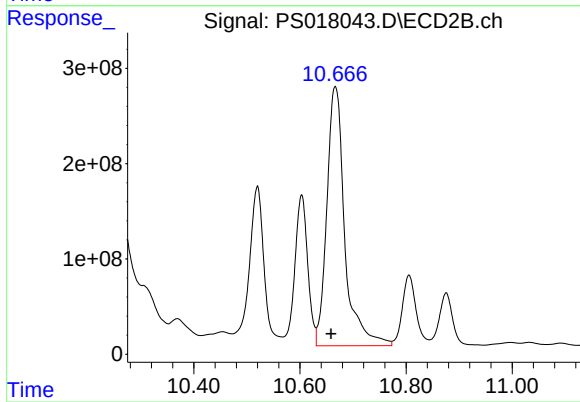


#15 Picloram

R.T.: 10.667 min
Delta R.T.: 0.008 min
Response: 6379676017
Conc: 1364.30 ng/ml

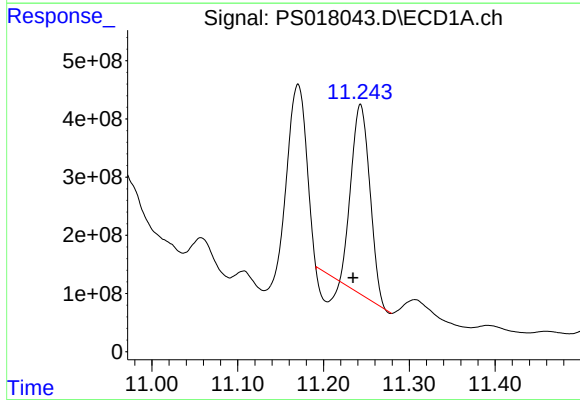

#16 DCPA

R.T.: 11.243 min
Delta R.T.: 0.009 min
Response: 4416725871
Conc: 408.77 ng/ml

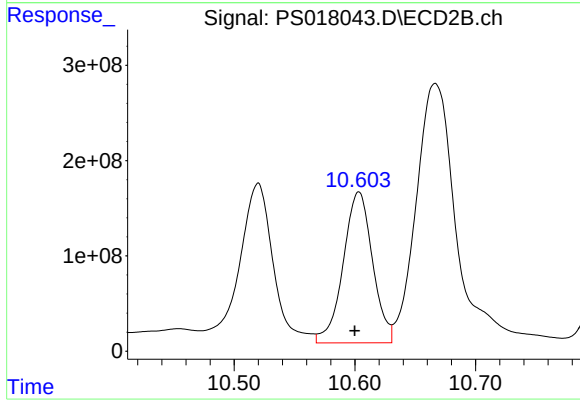

#16 DCPA

R.T.: 10.603 min
Delta R.T.: 0.003 min
Response: 2684100692
Conc: 607.88 ng/ml