

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011722\
 Data File : PS018048.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jan 2022 15:02
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 17 16:25:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 06 10:21:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.046	6.644	706.7E6	309.8E6	488.889	533.990
Target Compounds							
7) T	MCPA	7.488f	0.000	14539626	0	2.179	N.D. #
9) T	2,4-D	8.200f	0.000	10386479	0	5.704	N.D. #
10) T	Pentachlo...	8.446	0.000	3666142	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.056f	8.433f	26906566	9084122	3.180	2.548
12) T	2,4,5-T	9.284	0.000	8441409	0	<MDL	N.D. #
14) T	DINOSEB	10.982	0.000	544964	0	<MDL	N.D. #
15) T	Picloram	10.805	10.673	20353041	34130275	1.705	7.299 #
16) T	DCPA	11.231	0.000	10869149	0	1.006	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011722\
Data File : PS018048.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jan 2022 15:02
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 17 16:25:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
Quant Title : 8080.M
QLast Update : Thu Jan 06 10:21:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

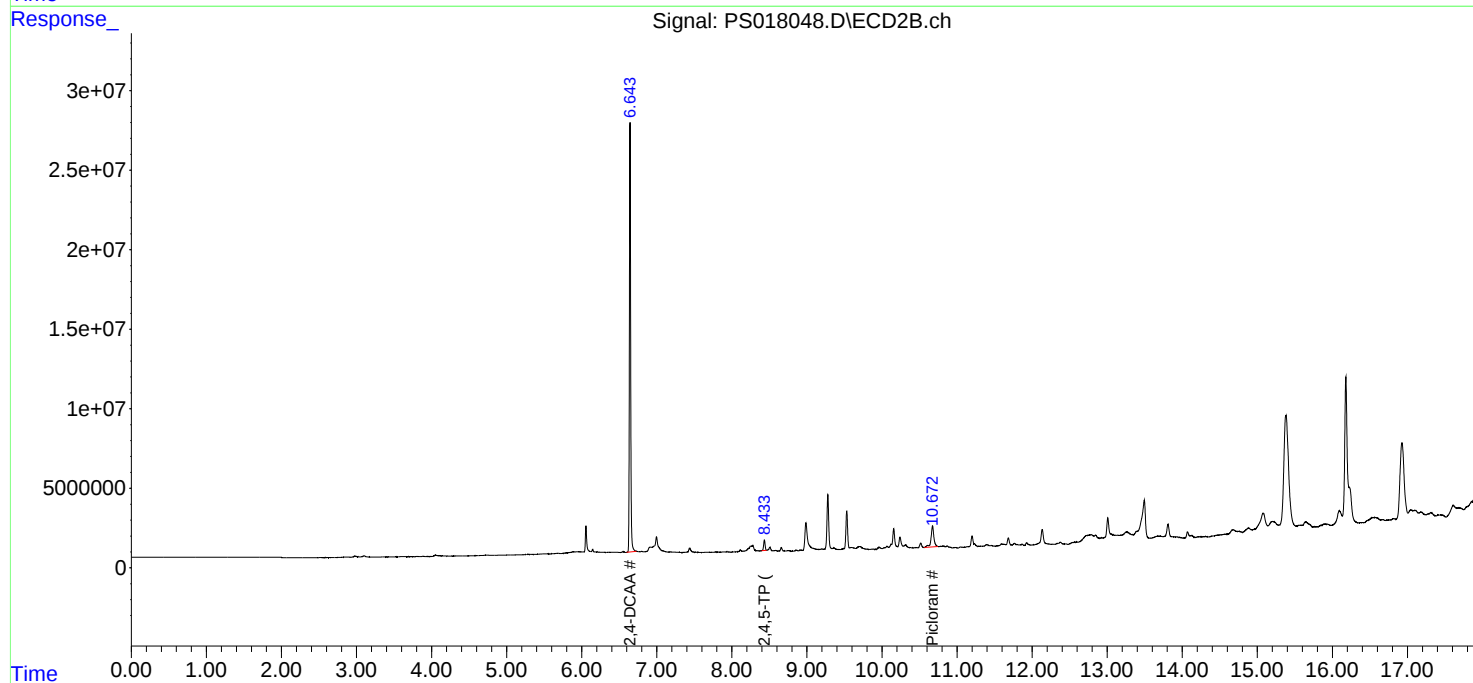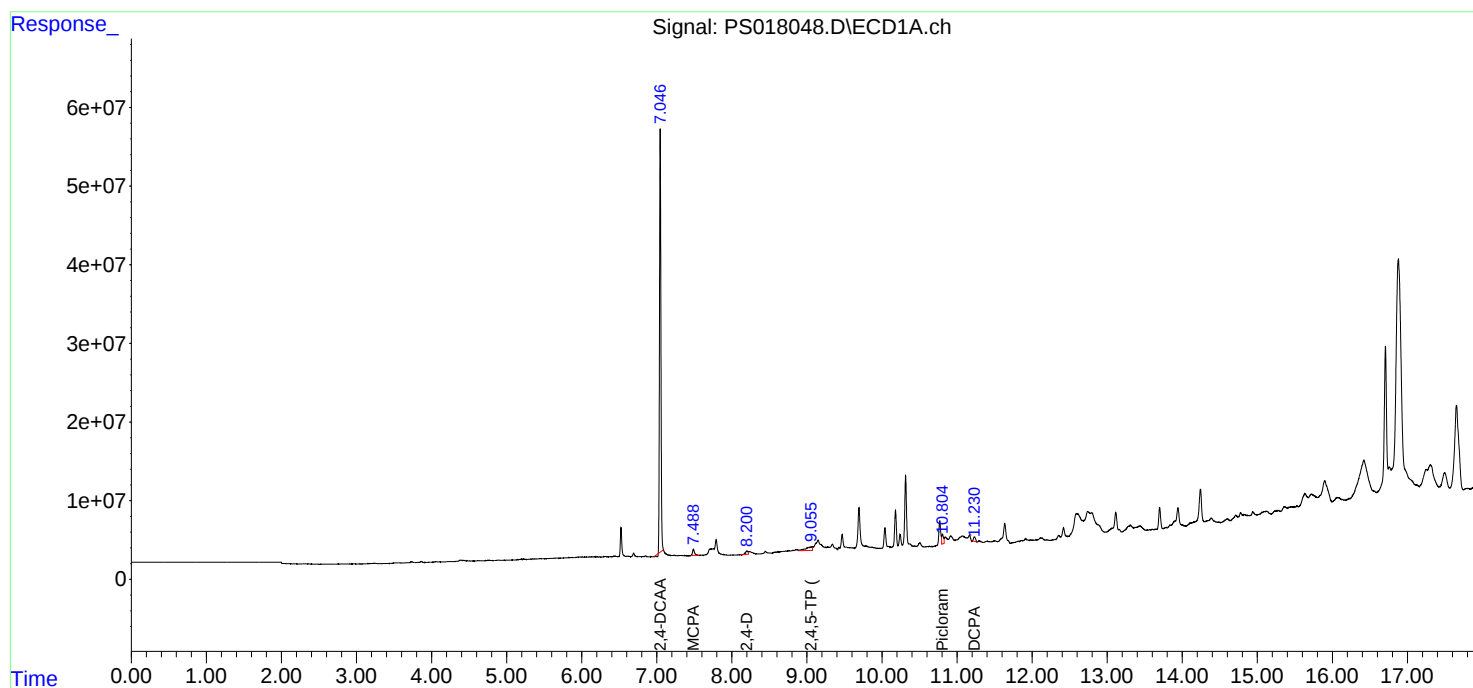


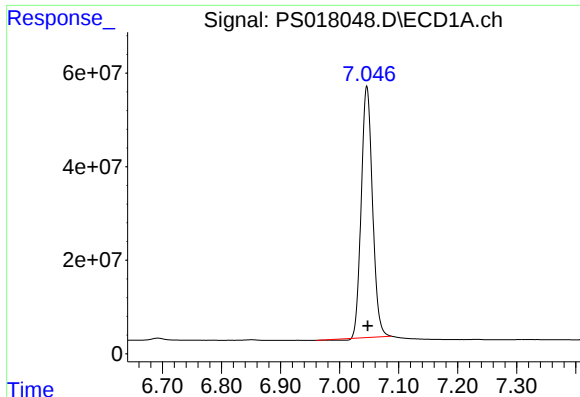

#4 2,4-DCAA


R.T.: 7.046 min
Delta R.T.: -0.001 min
Response: 706683417
Conc: 488.89 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

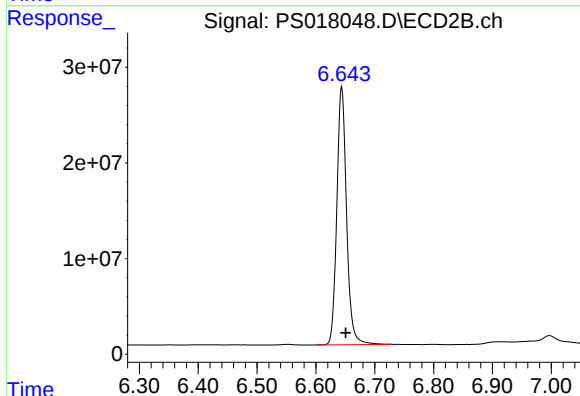


#4 2,4-DCAA

R.T.: 6.644 min
Delta R.T.: -0.007 min
Response: 309846830
Conc: 533.99 ng/ml

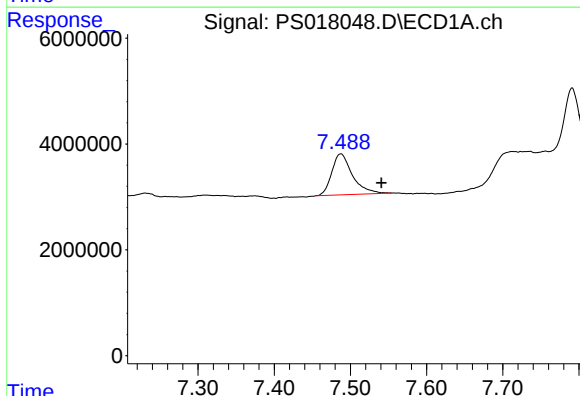


#7 MCPA

R.T.: 7.488 min
Delta R.T.: -0.053 min
Response: 14539626
Conc: 2.18 ug/ml

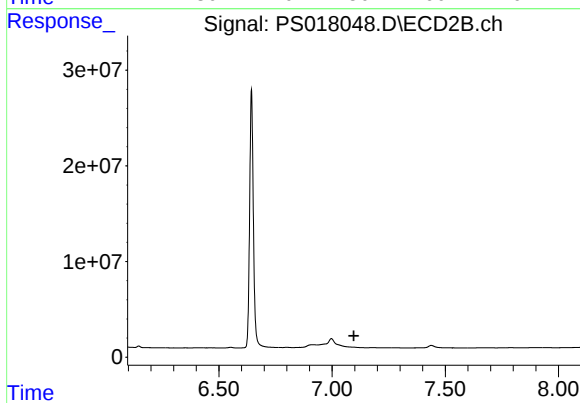

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.096 min
Response: 0
Conc: N.D.

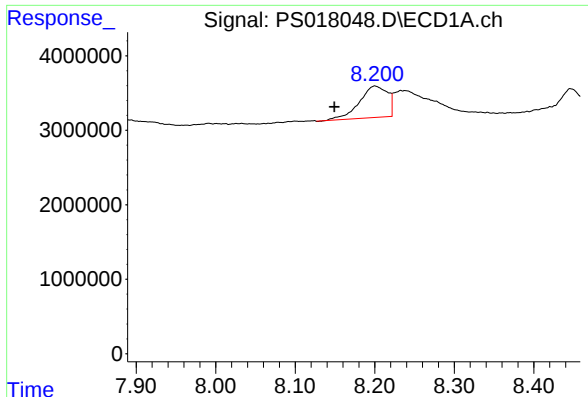

#9 2,4-D


R.T.: 8.200 min
Delta R.T.: 0.051 min
Response: 10386479
Conc: 5.70 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

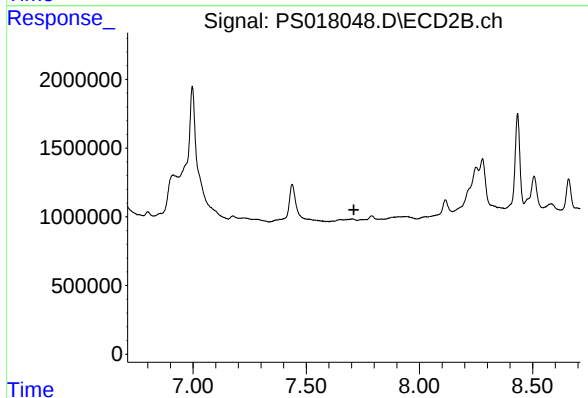


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.710 min
Response: 0
Conc: N.D.

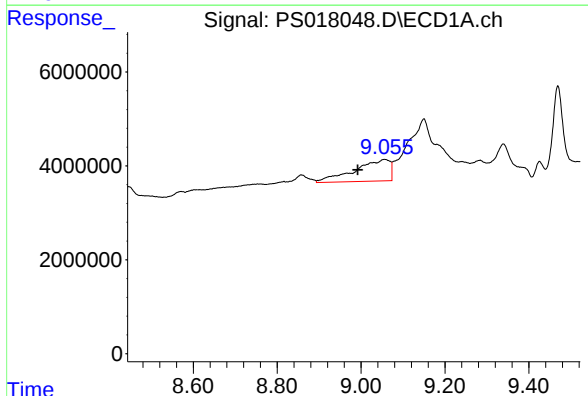


#11 2,4,5-TP (SILVEX)

R.T.: 9.056 min
Delta R.T.: 0.064 min
Response: 26906566
Conc: 3.18 ng/ml

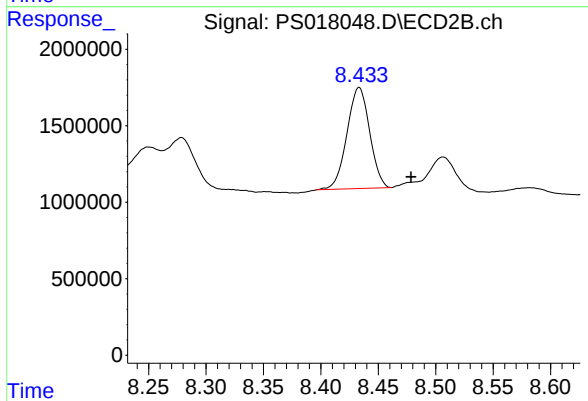

#11 2,4,5-TP (SILVEX)


R.T.: 8.433 min
Delta R.T.: -0.045 min
Response: 9084122
Conc: 2.55 ng/ml

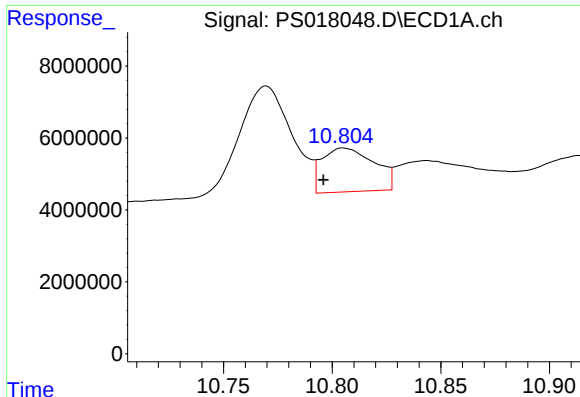

#15 Picloram


R.T.: 10.805 min
Delta R.T.: 0.009 min
Response: 20353041
Conc: 1.71 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

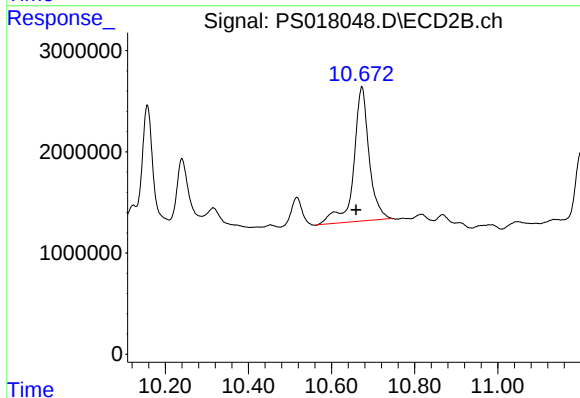


#15 Picloram

R.T.: 10.673 min
Delta R.T.: 0.014 min
Response: 34130275
Conc: 7.30 ng/ml

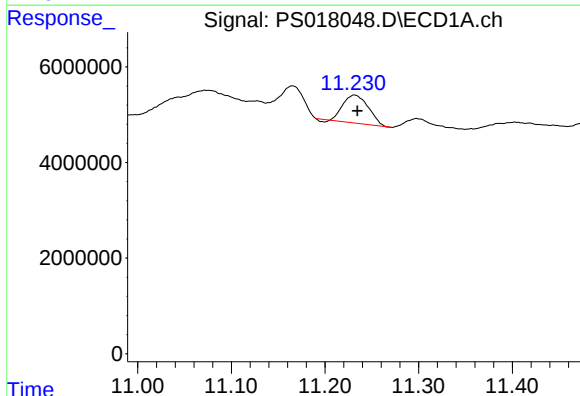

#16 DCPA

R.T.: 11.231 min
Delta R.T.: -0.003 min
Response: 10869149
Conc: 1.01 ng/ml

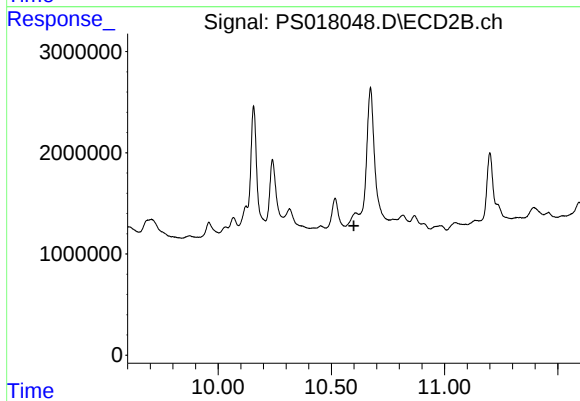

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.600 min
Response: 0
Conc: N.D.