

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011819\
 Data File : PS002851.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jan 2019 08:01
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 18 11:19:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS011719.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 17 13:42:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.336	10.827	188.0E6	175.5E6	521.156	435.067
Target Compounds							
7) T	MCPA	0.000	11.720	0	5044072	N.D.	2.886 #
8) T	DICHLORPROP	0.000	12.139	0	4278457	N.D.	11.384 #
10) T	Pentachlo...	13.567	13.242	1293557	766383	0.236	0.138 #
11) T	2,4,5-TP ...	0.000	13.873	0	3920353	N.D.	1.809 #
12) T	2,4,5-T	0.000	14.453	0	11396853	N.D.	6.747 #
15) T	Picloram	0.000	16.684	0	580983	N.D.	0.198 #
16) T	DCPA	17.400	16.684	1345866	580983	0.502	0.202 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011819\
Data File : PS002851.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jan 2019 08:01
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 18 11:19:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS011719.M
Quant Title : 8080.M
QLast Update : Thu Jan 17 13:42:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

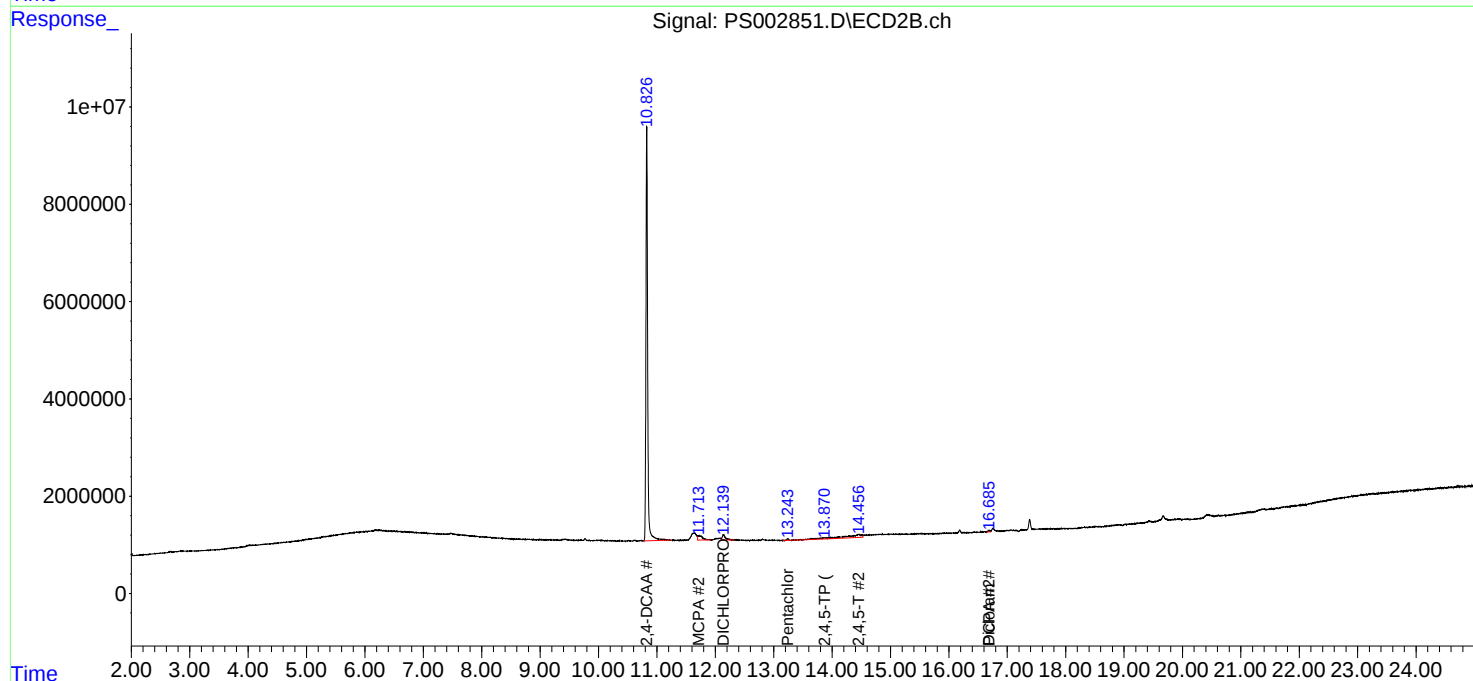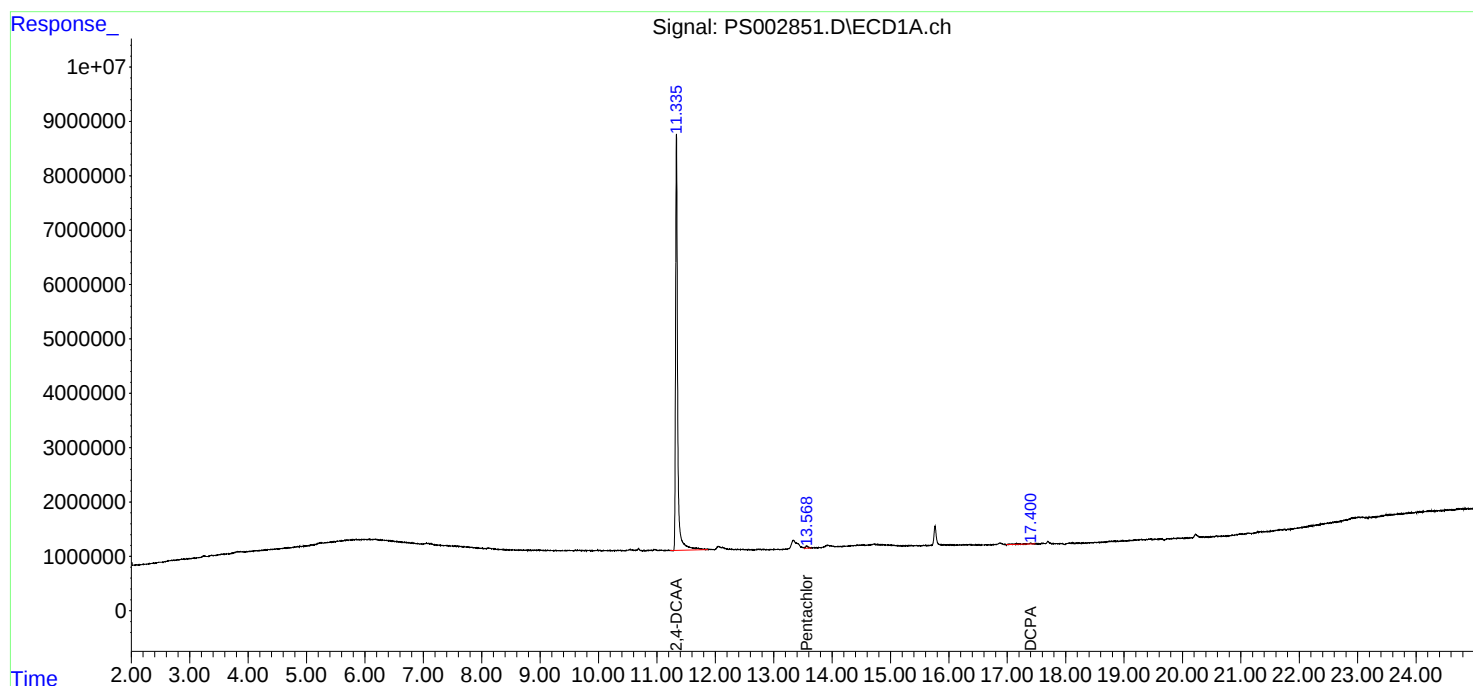


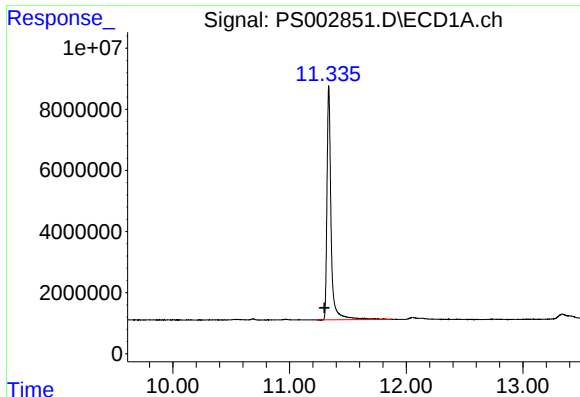

#4 2,4-DCAA


R.T.: 11.336 min
Delta R.T.: 0.037 min
Response: 187973290
Conc: 521.16 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

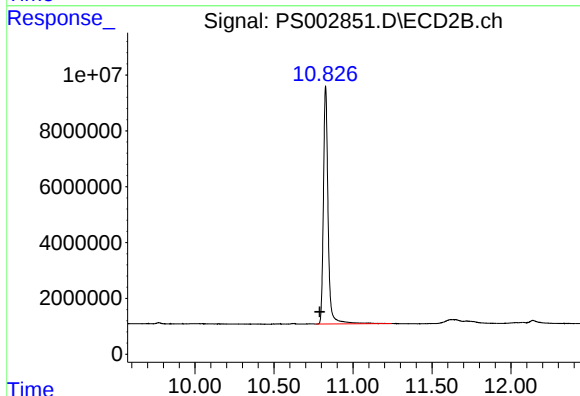


#4 2,4-DCAA

R.T.: 10.827 min
Delta R.T.: 0.037 min
Response: 175470615
Conc: 435.07 ng/ml

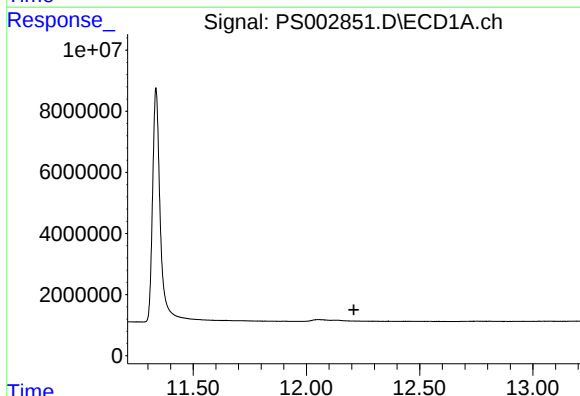


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.210 min
Response: 0
Conc: N.D.

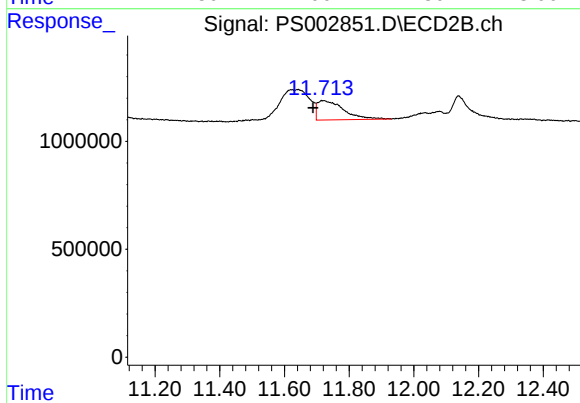

#7 MCPA


R.T.: 11.720 min
Delta R.T.: 0.031 min
Response: 5044072
Conc: 2.89 ug/ml

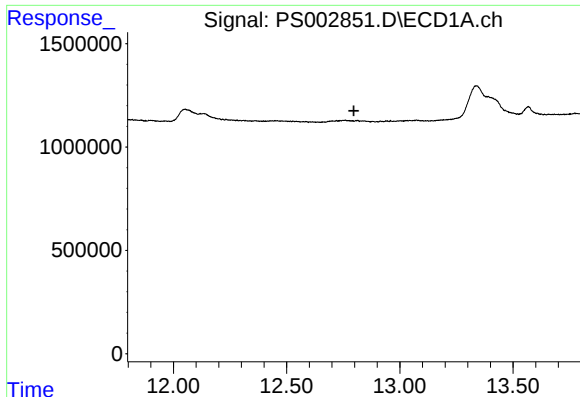

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 12.797 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

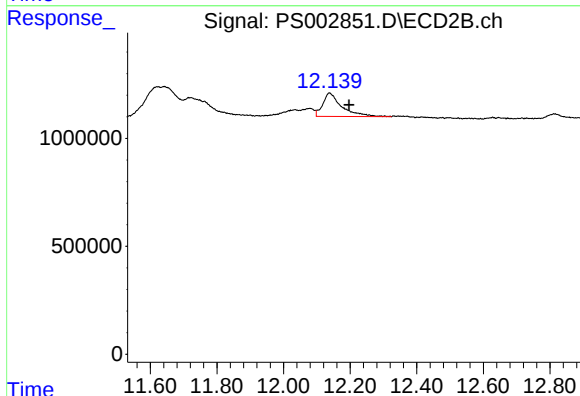


#8 DICHLORPROP

R.T.: 12.139 min
Delta R.T.: -0.058 min
Response: 4278457
Conc: 11.38 ng/ml

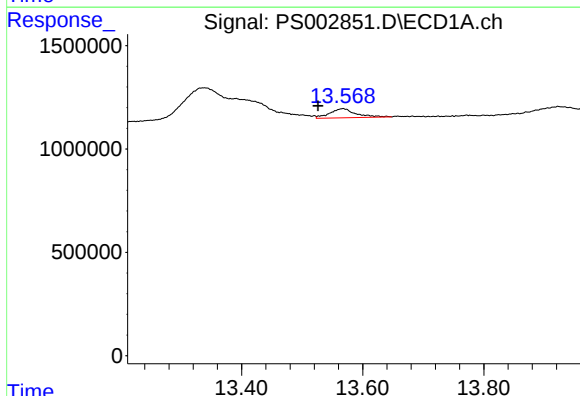


#10 Pentachlorophenol

R.T.: 13.567 min
Delta R.T.: 0.040 min
Response: 1293557
Conc: 0.24 ng/ml

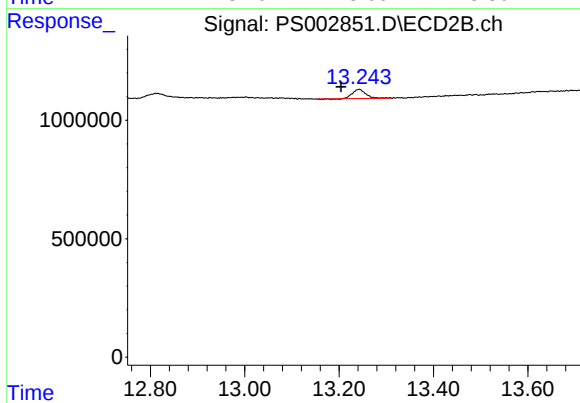

#10 Pentachlorophenol


R.T.: 13.242 min
Delta R.T.: 0.038 min
Response: 766383
Conc: 0.14 ng/ml

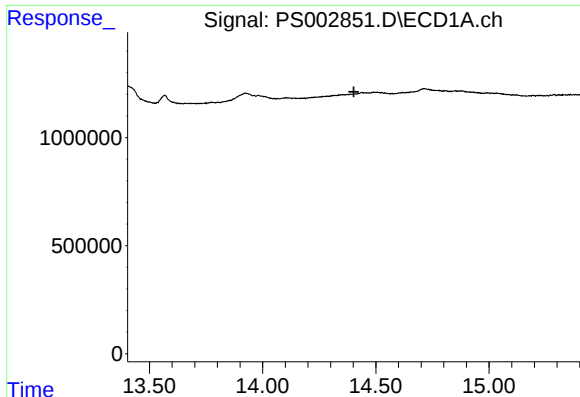

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.403 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

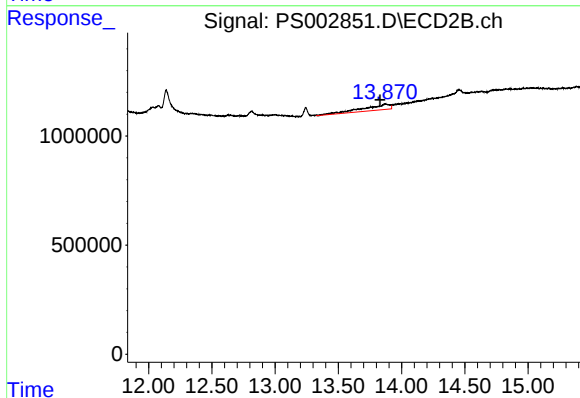


#11 2,4,5-TP (SILVEX)

R.T.: 13.873 min
Delta R.T.: 0.043 min
Response: 3920353
Conc: 1.81 ng/ml

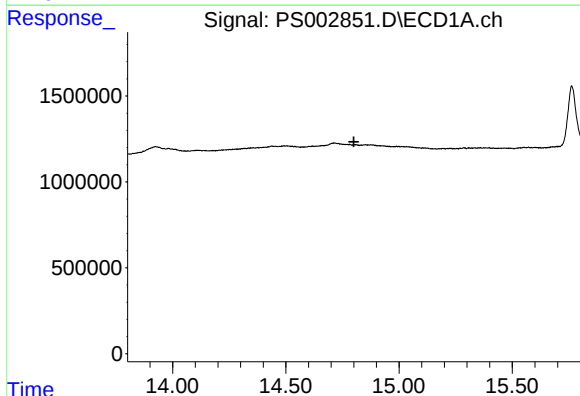


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.800 min
Response: 0
Conc: N.D.

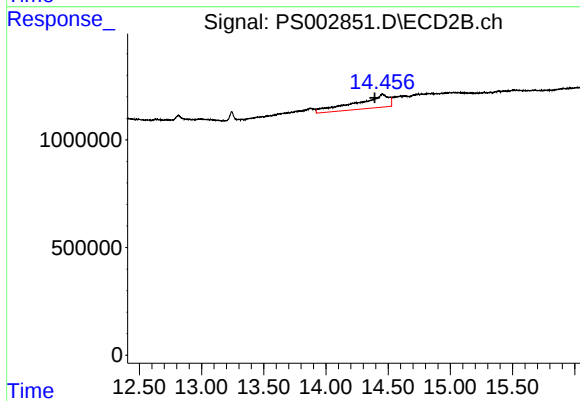

#12 2,4,5-T


R.T.: 14.453 min
Delta R.T.: 0.062 min
Response: 11396853
Conc: 6.75 ng/ml

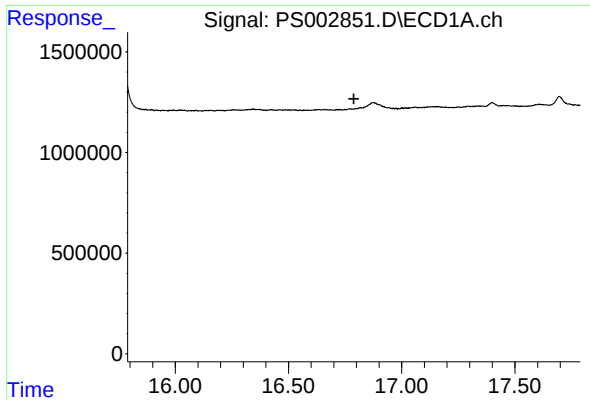

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 16.789 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

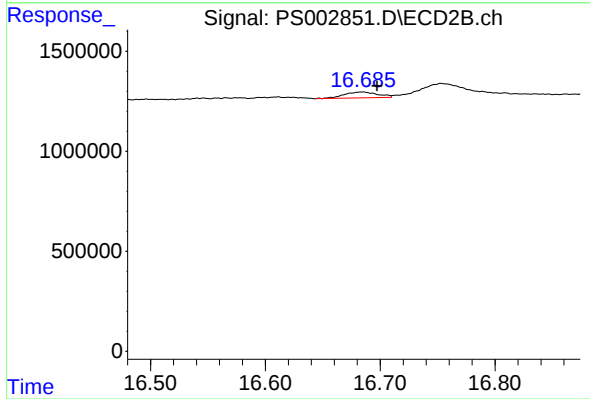


#15 Picloram

R.T.: 16.684 min
Delta R.T.: -0.013 min
Response: 580983
Conc: 0.20 ng/ml

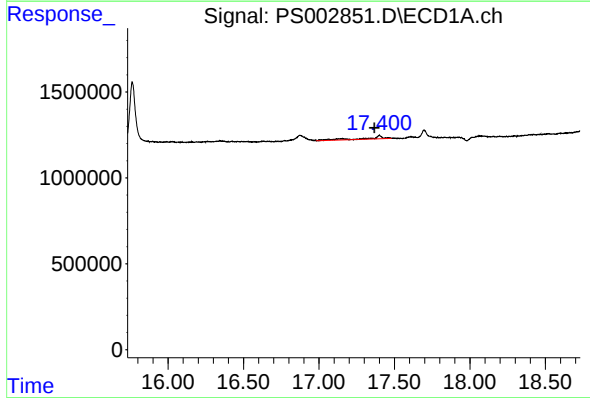

#16 DCPA

R.T.: 17.400 min
Delta R.T.: 0.031 min
Response: 1345866
Conc: 0.50 ng/ml

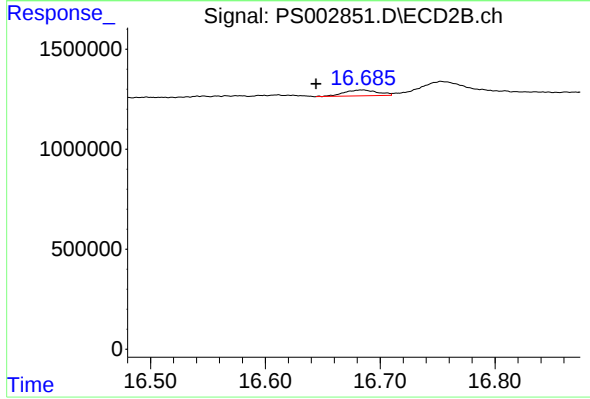

#16 DCPA

R.T.: 16.684 min
Delta R.T.: 0.040 min
Response: 580983
Conc: 0.20 ng/ml