

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011821\
 Data File : PS013803.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jan 2021 19:07
 Operator : DD\AJ
 Sample : M1141-23
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 ETGI-354

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 19 01:47:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010421.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 05 01:51:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.208	6.910	490.1E6	216.6E6	512.872	538.582
Target Compounds							
1) T	Dalapon	2.986f	2.588	77292005	87649928	71.065	168.574 #
2) T	3,5-DICHL...	0.000	6.093	0	46707860	N.D.	74.139
3) T	4-Nitroph...	7.102f	6.539	26293962	6835471	55.305	26.953 #
5) T	DICAMBA	7.383	7.043	10146435	8203639	2.635	4.777 #
6) T	MCP	7.617f	7.142	8832753	4686445	3.083	3.316
7) T	MCPA	7.673f	0.000	6901749	0	1.679	N.D. #
8) T	DICHLORPROP	8.033f	7.748f	8130030	-163824	8.399	N.D. #
10) T	Pentachlo...	8.680f	0.000	10432207	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	8.756	0	8166081	N.D.	3.419
12) T	2,4,5-T	9.395f	0.000	27678148	0	4.895	N.D. #
13) T	2,4-DB	9.978	0.000	21335765	0	21.835	N.D. #
14) T	DINOSEB	11.141	10.043f	19638360	15826426	4.451	9.458 #
15) T	Picloram	10.974	0.000	25596893	0	3.544	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011821\
Data File : PS013803.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jan 2021 19:07
Operator : DD\AJ
Sample : M1141-23
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
ETGI-354

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 19 01:47:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010421.M
Quant Title : 8080.M
QLast Update : Tue Jan 05 01:51:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

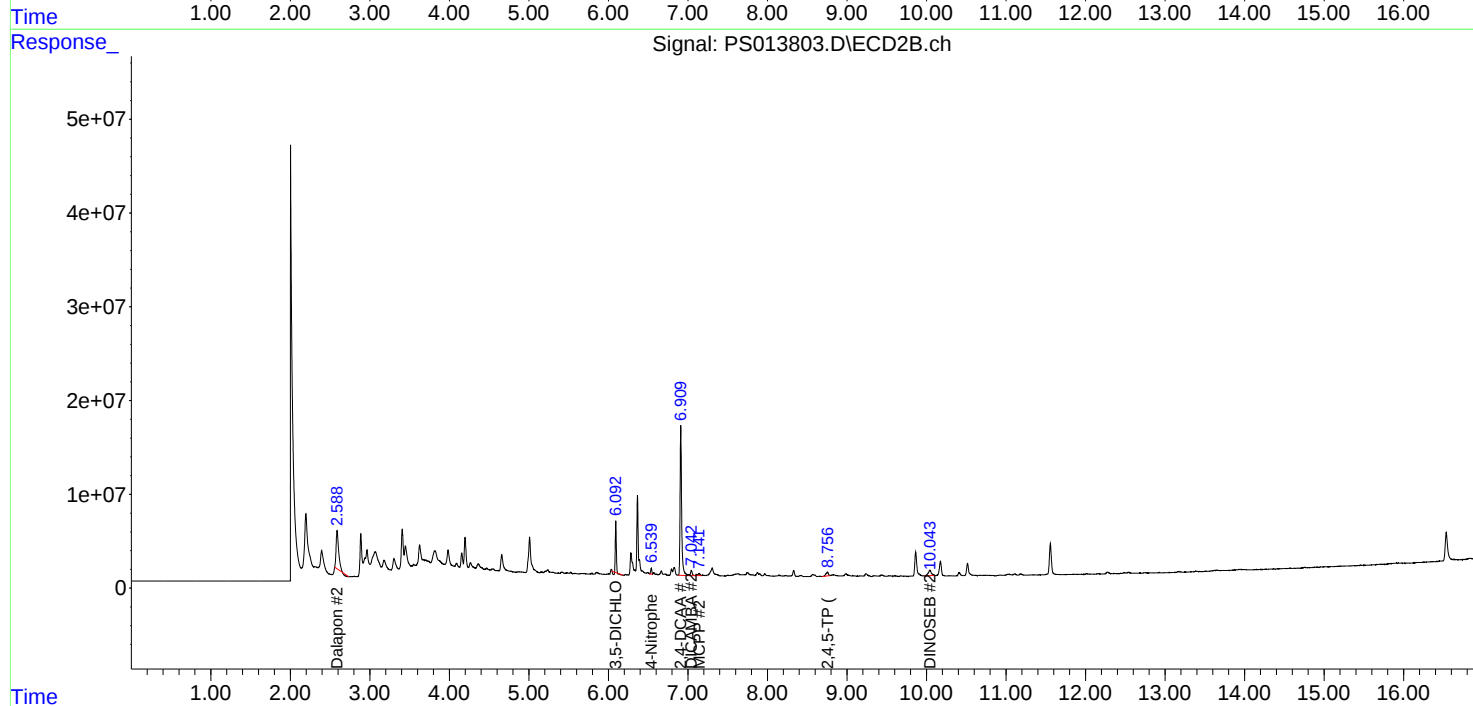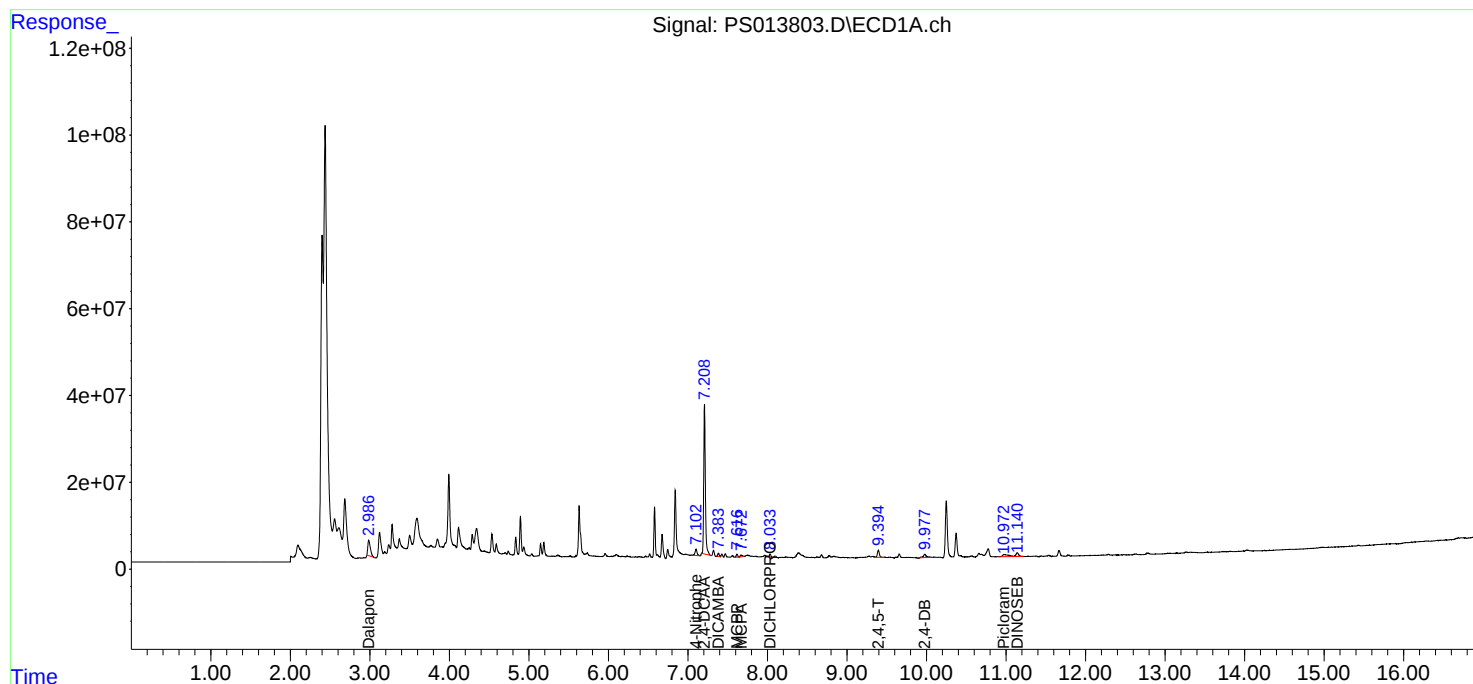


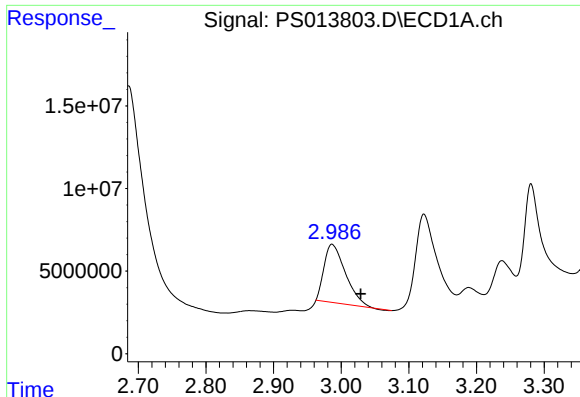

#1 Dalapon


R.T.: 2.986 min
Delta R.T.: -0.043 min
Response: 77292005
Conc: 71.06 ng/ml

Instrument :
ECD_S
ClientSampleId :
ETGI-354

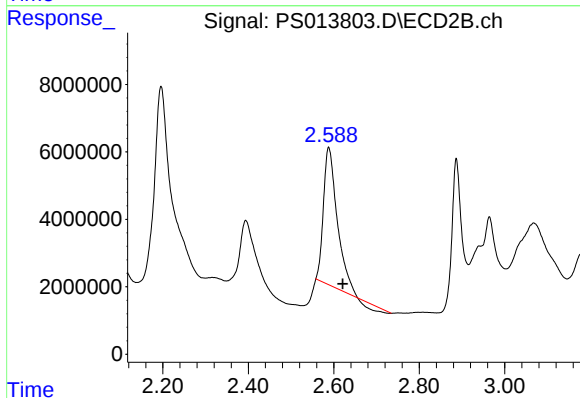


#1 Dalapon

R.T.: 2.588 min
Delta R.T.: -0.033 min
Response: 87649928
Conc: 168.57 ng/ml

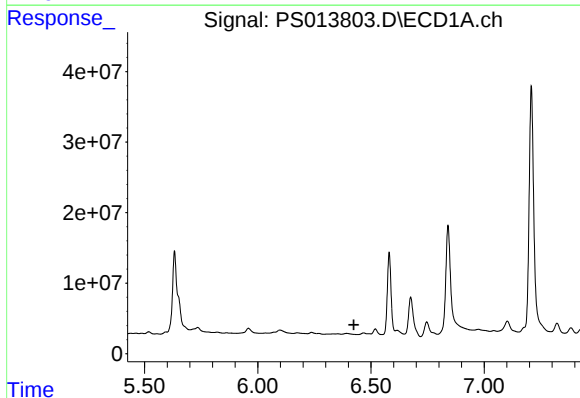


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.425 min
Response: 0
Conc: N.D.

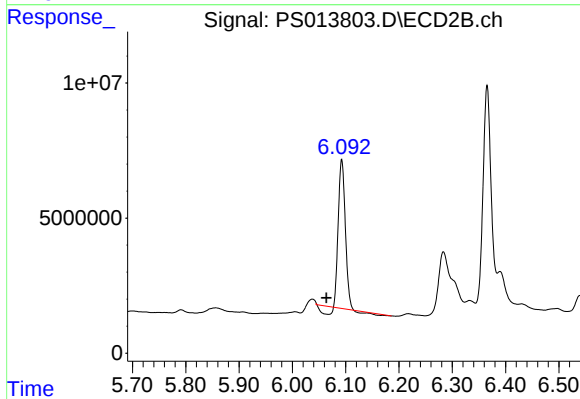

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.093 min
Delta R.T.: 0.028 min
Response: 46707860
Conc: 74.14 ng/ml

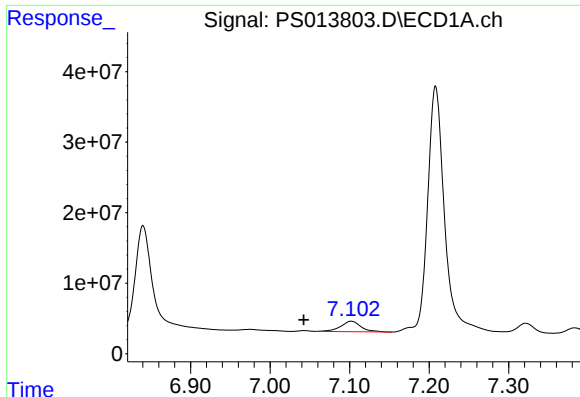

#3 4-Nitrophenol


R.T.: 7.102 min
Delta R.T.: 0.060 min
Response: 26293962
Conc: 55.31 ng/ml

Instrument :
ECD_S
ClientSampleId :
ETGI-354

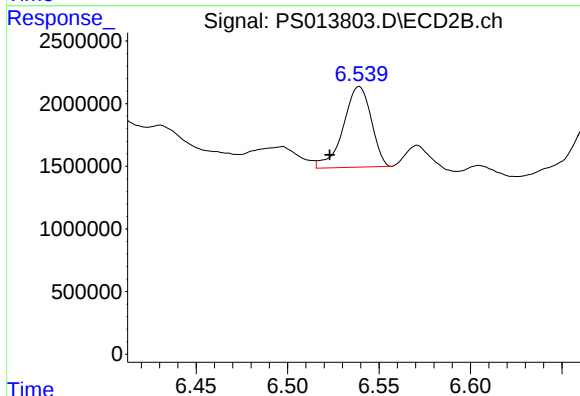


#3 4-Nitrophenol

R.T.: 6.539 min
Delta R.T.: 0.016 min
Response: 6835471
Conc: 26.95 ng/ml

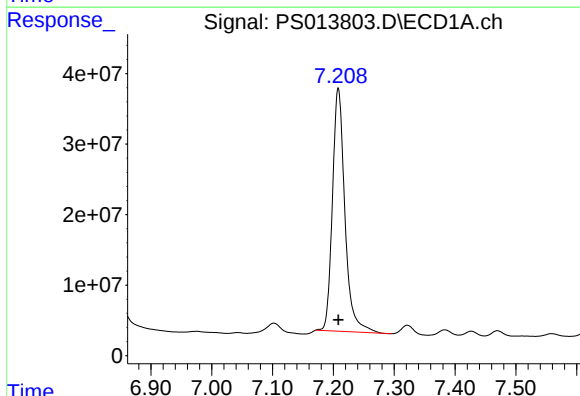


#4 2,4-DCAA

R.T.: 7.208 min
Delta R.T.: 0.000 min
Response: 490097134
Conc: 512.87 ng/ml

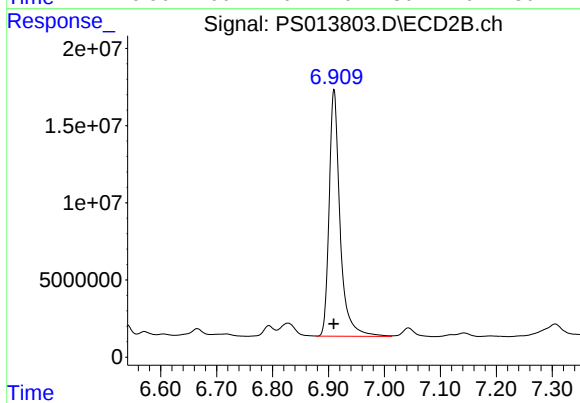

#4 2,4-DCAA


R.T.: 6.910 min
Delta R.T.: 0.000 min
Response: 216571826
Conc: 538.58 ng/ml

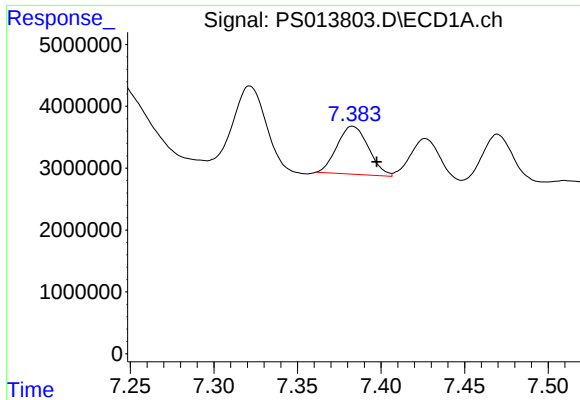

#5 DICAMBA


R.T.: 7.383 min
Delta R.T.: -0.014 min
Response: 10146435
Conc: 2.63 ng/ml

Instrument :
ECD_S
ClientSampleId :
ETGI-354

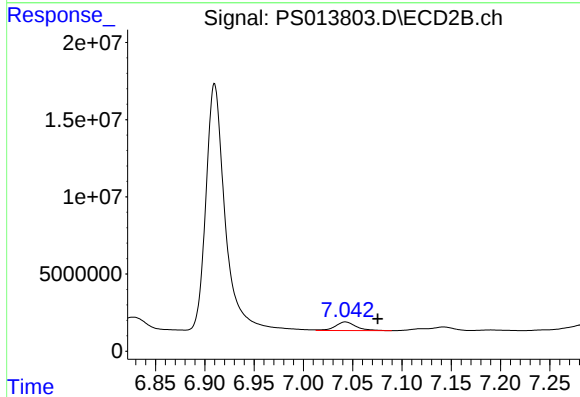


#5 DICAMBA

R.T.: 7.043 min
Delta R.T.: -0.033 min
Response: 8203639
Conc: 4.78 ng/ml

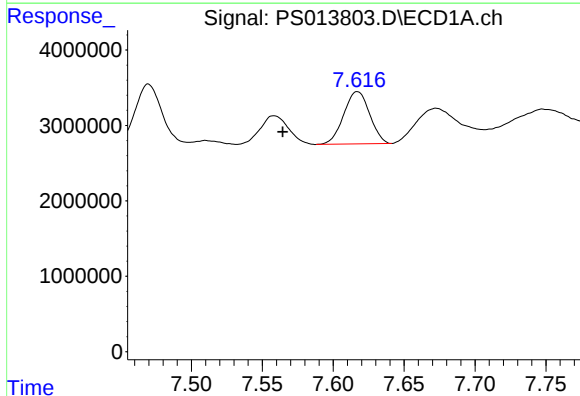


#6 MCP

R.T.: 7.617 min
Delta R.T.: 0.053 min
Response: 8832753
Conc: 3.08 ug/ml

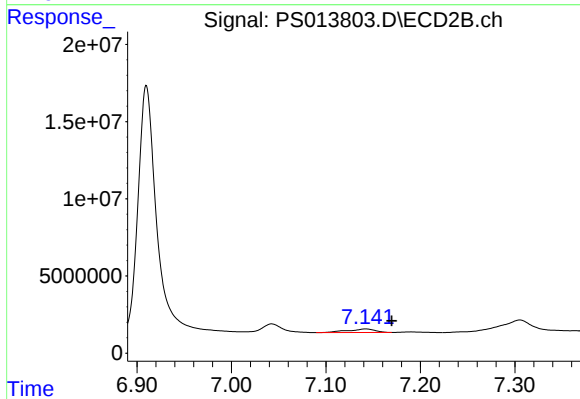

#6 MCP


R.T.: 7.142 min
Delta R.T.: -0.028 min
Response: 4686445
Conc: 3.32 ug/ml

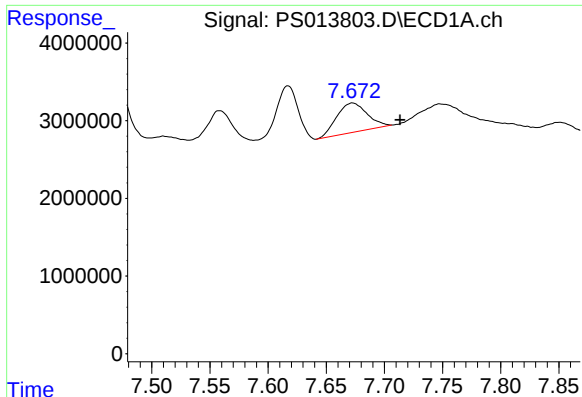

#7 MCPA


R.T.: 7.673 min
Delta R.T.: -0.041 min
Response: 6901749
Conc: 1.68 ug/ml

Instrument :
ECD_S
ClientSampleId :
ETGI-354

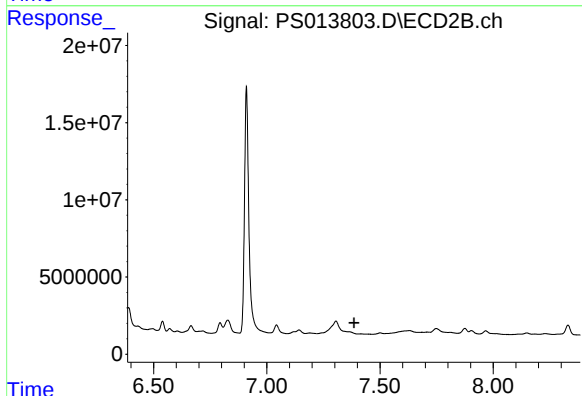


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.385 min
Response: 0
Conc: N.D.

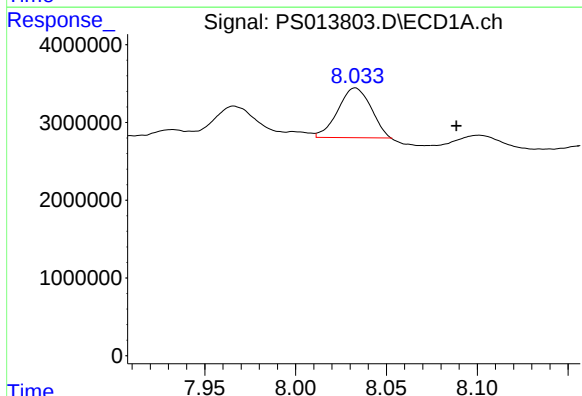


#8 DICHLORPROP

R.T.: 8.033 min
Delta R.T.: -0.056 min
Response: 8130030
Conc: 8.40 ng/ml

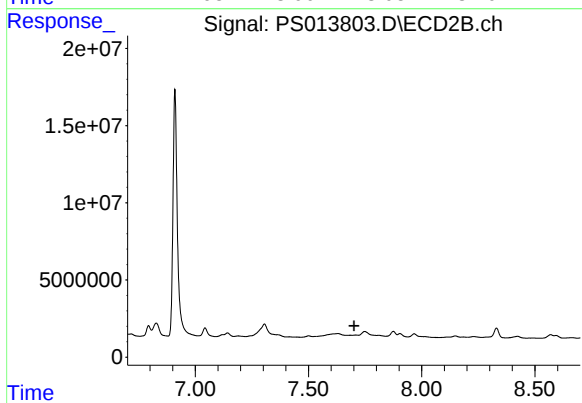

#8 DICHLORPROP


R.T.: 7.748 min
Delta R.T.: 0.048 min
Response: -163824
Conc: N.D.

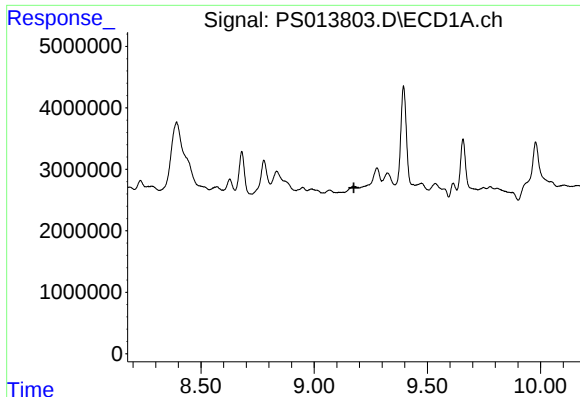

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.175 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
ETGI-354

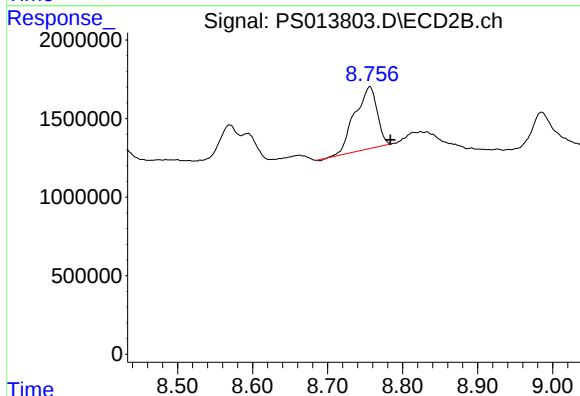


#11 2,4,5-TP (SILVEX)

R.T.: 8.756 min
Delta R.T.: -0.027 min
Response: 8166081
Conc: 3.42 ng/ml

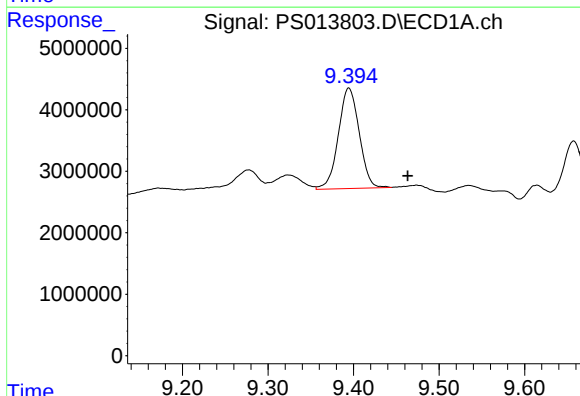


#12 2,4,5-T

R.T.: 9.395 min
Delta R.T.: -0.069 min
Response: 27678148
Conc: 4.89 ng/ml

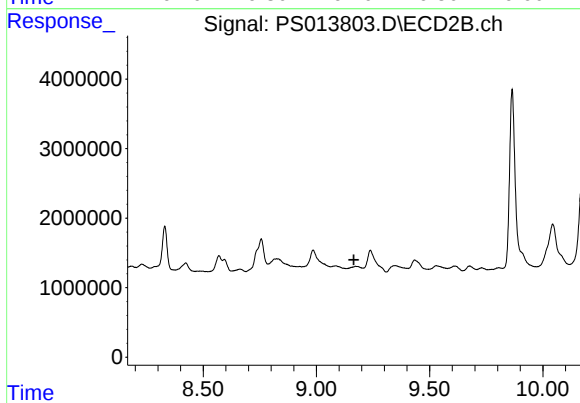

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.165 min
Response: 0
Conc: N.D.

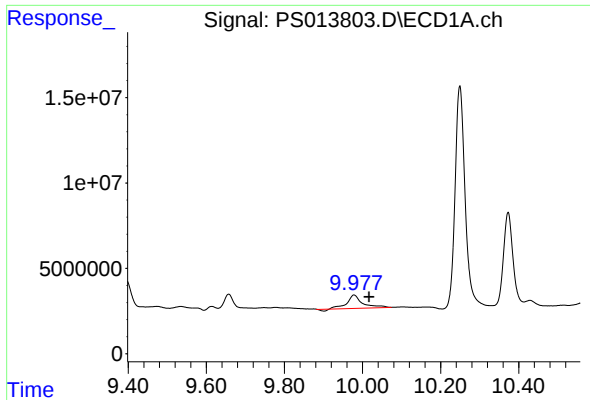

#13 2,4-DB


R.T.: 9.978 min
Delta R.T.: -0.039 min
Response: 21335765
Conc: 21.83 ng/ml

Instrument :
ECD_S
ClientSampleId :
ETGI-354

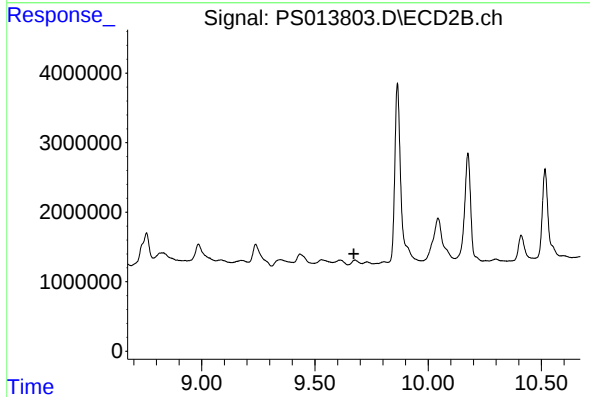


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.672 min
Response: 0
Conc: N.D.

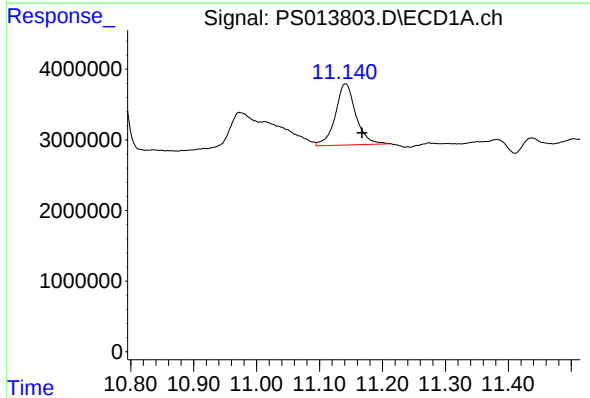


#14 DINOSEB

R.T.: 11.141 min
Delta R.T.: -0.026 min
Response: 19638360
Conc: 4.45 ng/ml

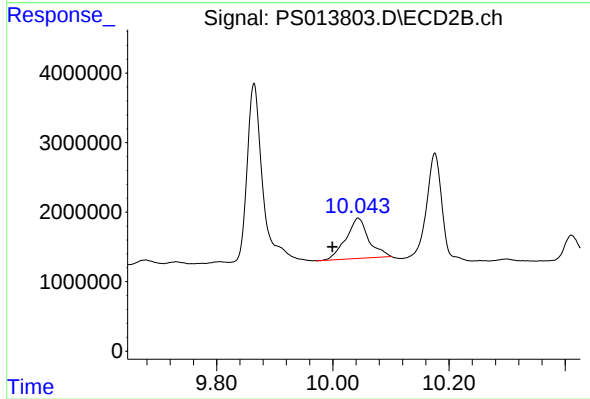

#14 DINOSEB


R.T.: 10.043 min
Delta R.T.: 0.044 min
Response: 15826426
Conc: 9.46 ng/ml

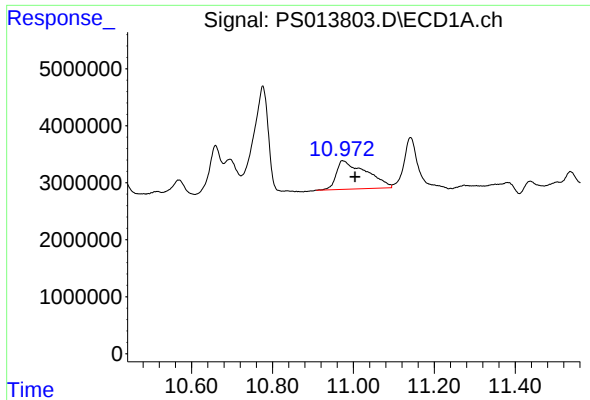

#15 Picloram

R.T.: 10.974 min
Delta R.T.: -0.030 min
Response: 25596893
Conc: 3.54 ng/ml

Instrument :
ECD_S
ClientSampleId :
ETGI-354

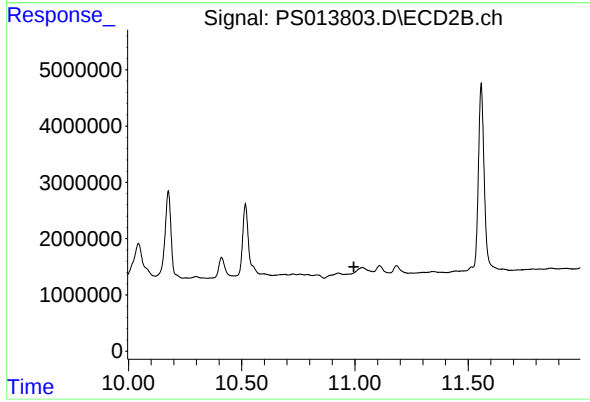

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.995 min
Response: 0
Conc: N.D.