

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011822\
 Data File : PS018055.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jan 2022 08:58
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 18 15:03:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 06 10:21:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.047	6.645	719.7E6	298.9E6	497.925	515.053
Target Compounds							
5) T	DICAMBA	7.234	0.000	2587522	0	<MDL	N.D. #
9) T	2,4-D	8.210f	0.000	11668831	0	6.408	N.D. #
11) T	2,4,5-TP ...	0.000	8.439	0	11312057	N.D.	3.173
12) T	2,4,5-T	9.288	8.925f	13918319	15342535	1.570	4.690 #
13) T	2,4-DB	9.838	0.000	14139295	0	8.554	N.D. #
14) T	DINOSEB	10.974	0.000	4649099	0	<MDL	N.D. #
15) T	Picloram	10.812	10.669	264.9E6	93316561	22.193	19.956
16) T	DCPA	11.242	10.669f	4625263	93316561	<MDL	21.134 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011822\
Data File : PS018055.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jan 2022 08:58
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 18 15:03:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
Quant Title : 8080.M
QLast Update : Thu Jan 06 10:21:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

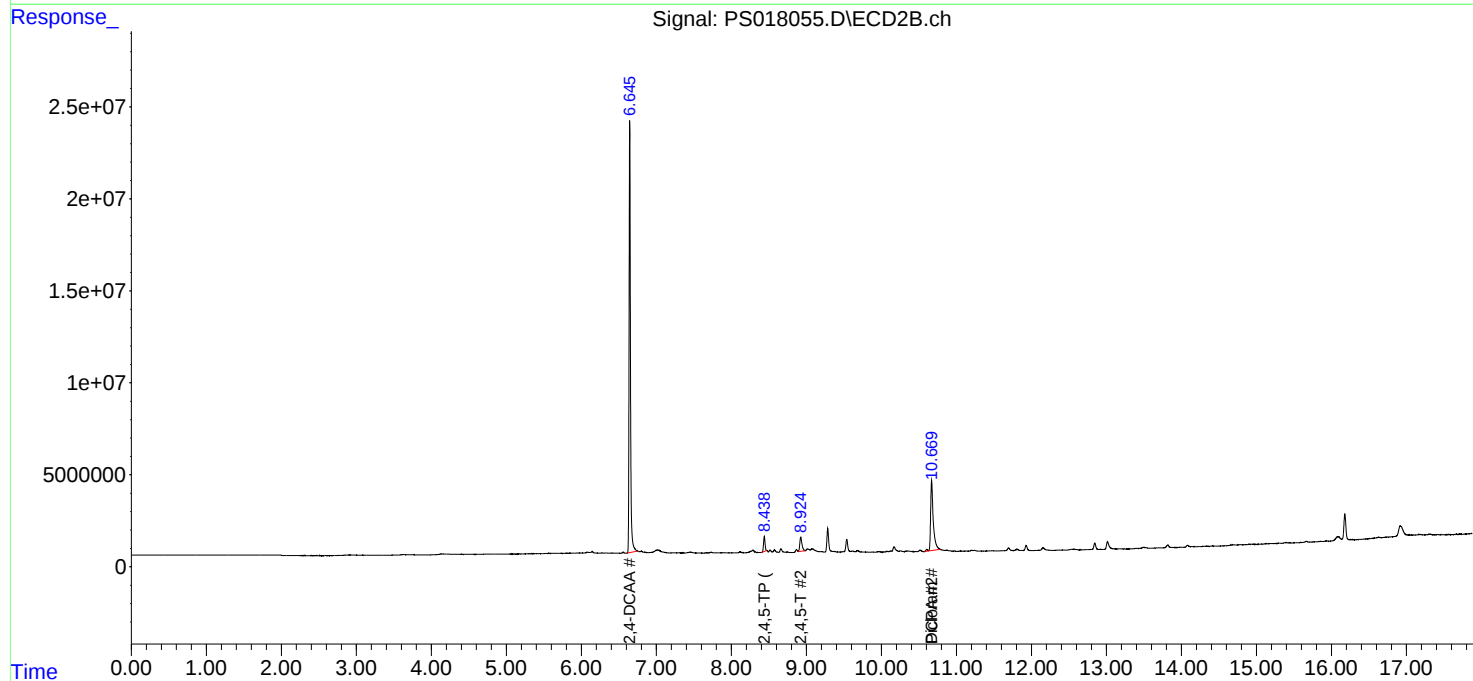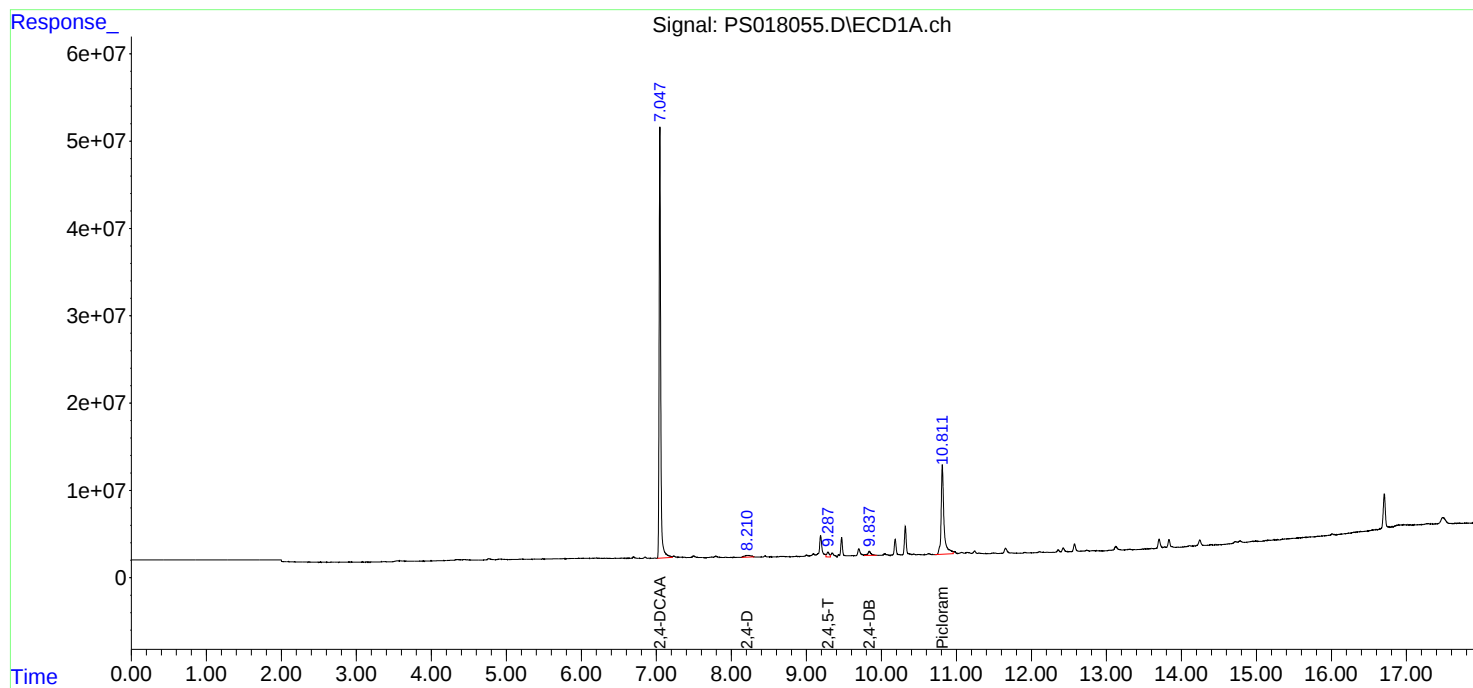


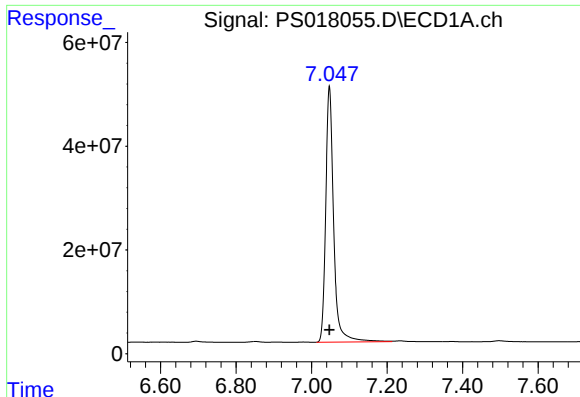

#4 2,4-DCAA


R.T.: 7.047 min
Delta R.T.: 0.000 min
Response: 719744458
Conc: 497.92 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

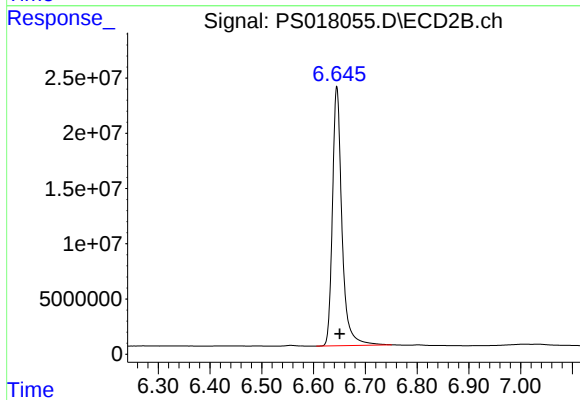


#4 2,4-DCAA

R.T.: 6.645 min
Delta R.T.: -0.006 min
Response: 298858885
Conc: 515.05 ng/ml

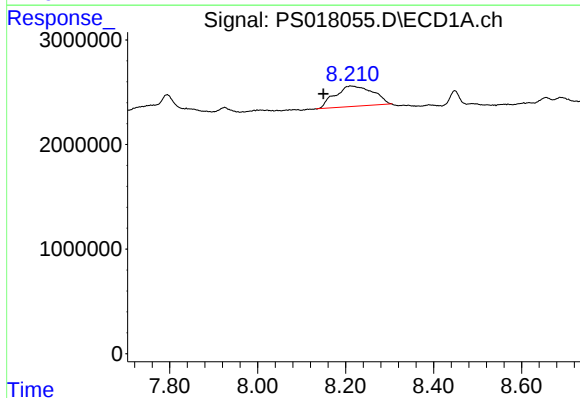


#9 2,4-D

R.T.: 8.210 min
Delta R.T.: 0.061 min
Response: 11668831
Conc: 6.41 ng/ml

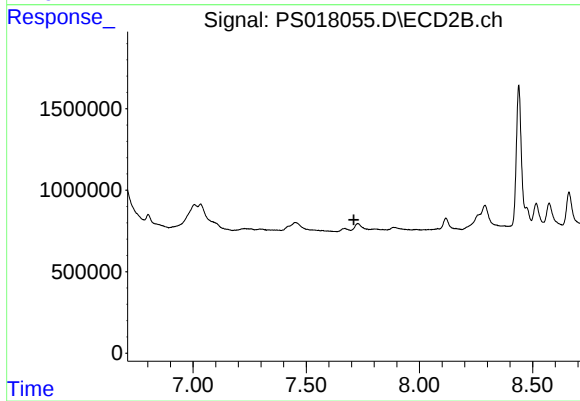

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.710 min
Response: 0
Conc: N.D.

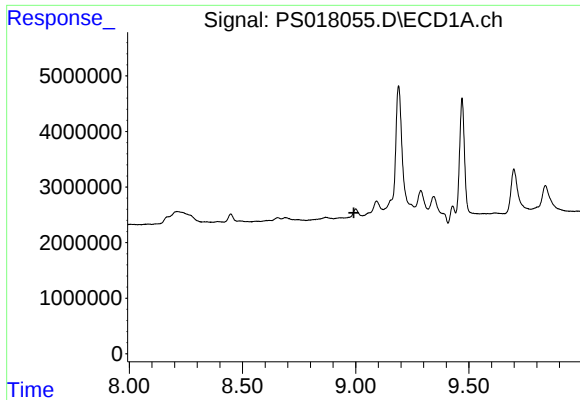

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 8.992 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

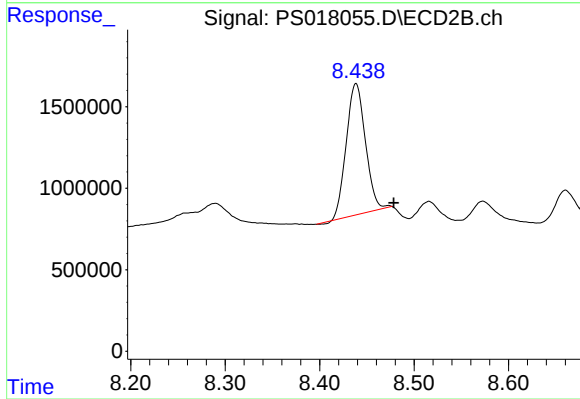


#11 2,4,5-TP (SILVEX)

R.T.: 8.439 min
Delta R.T.: -0.040 min
Response: 11312057
Conc: 3.17 ng/ml

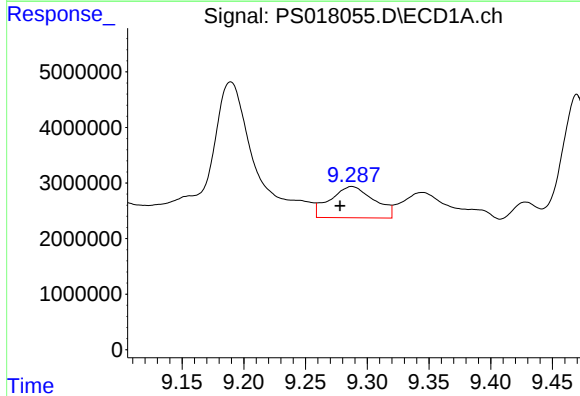


#12 2,4,5-T

R.T.: 9.288 min
Delta R.T.: 0.010 min
Response: 13918319
Conc: 1.57 ng/ml

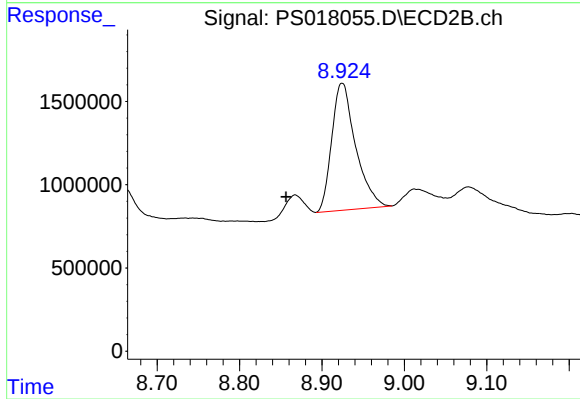

#12 2,4,5-T


R.T.: 8.925 min
Delta R.T.: 0.068 min
Response: 15342535
Conc: 4.69 ng/ml

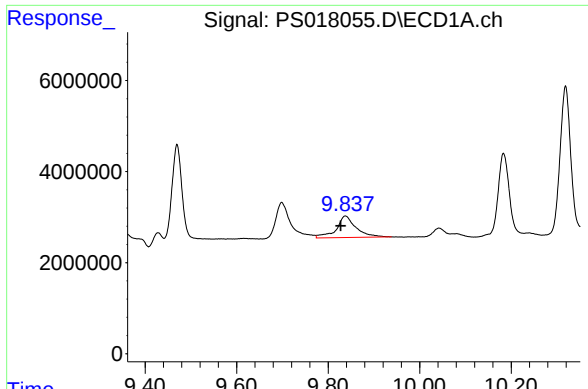

#13 2,4-DB


R.T.: 9.838 min
Delta R.T.: 0.010 min
Response: 14139295
Conc: 8.55 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

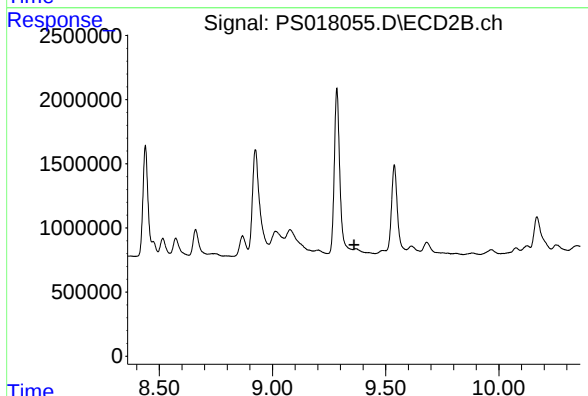


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.360 min
Response: 0
Conc: N.D.

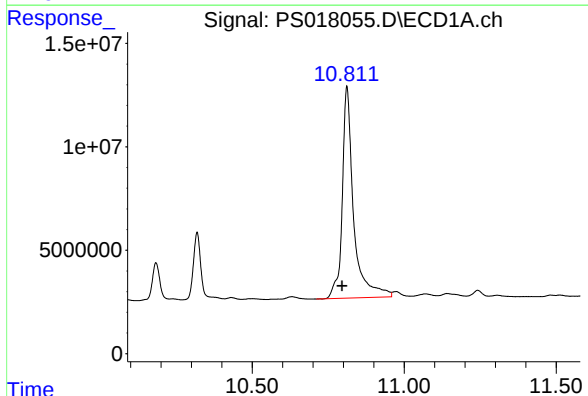


#15 Picloram

R.T.: 10.812 min
Delta R.T.: 0.016 min
Response: 264891778
Conc: 22.19 ng/ml

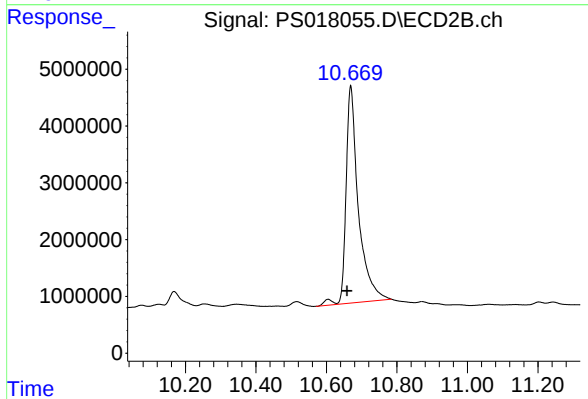

#15 Picloram


R.T.: 10.669 min
Delta R.T.: 0.010 min
Response: 93316561
Conc: 19.96 ng/ml

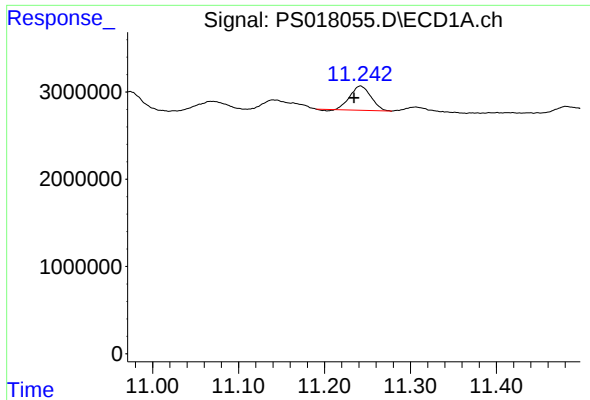

#16 DCPA

R.T.: 11.242 min
Delta R.T.: 0.007 min
Response: 4625263
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

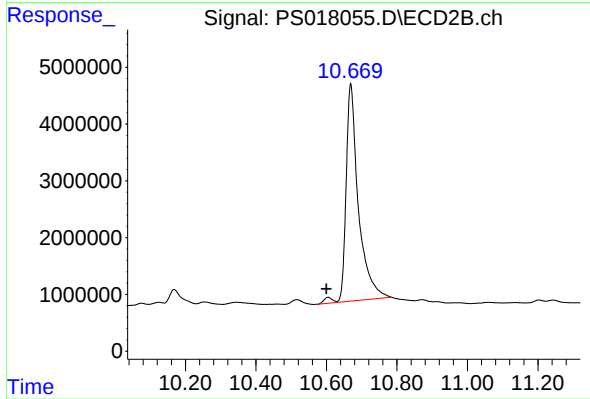

#16 DCPA

R.T.: 10.669 min
Delta R.T.: 0.069 min
Response: 93316561
Conc: 21.13 ng/ml