

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011822\
 Data File : PS018067.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jan 2022 16:06
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 18 23:58:31 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 06 10:21:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.048	6.646	675.1E6	303.1E6	467.060	522.378
Target Compounds							
5) T	DICAMBA	7.235	0.000	8420223	0	1.348	N.D. #
7) T	MCPA	7.492f	0.000	4436412	0	<MDL	N.D. #
9) T	2,4-D	8.159	0.000	3620678	0	1.988	N.D. #
10) T	Pentachlo...	8.449	8.117	20865743	8592166	<MDL	1.020 #
11) T	2,4,5-TP ...	9.000	8.437f	19939128	24349278	2.356	6.831 #
12) T	2,4,5-T	9.285	8.861	29497108	6353140	3.328	1.942 #
13) T	2,4-DB	9.831	0.000	30765239	0	18.611	N.D. #
14) T	DINOSEB	10.977	0.000	15481580	0	2.358	N.D. #
15) T	Picloram	10.807	10.664	401.0E6	148.4E6	33.595	31.745
16) T	DCPA	11.245	10.604	18246154	8183964	1.689	1.853



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011822\
Data File : PS018067.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jan 2022 16:06
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 18 23:58:31 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
Quant Title : 8080.M
QLast Update : Thu Jan 06 10:21:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

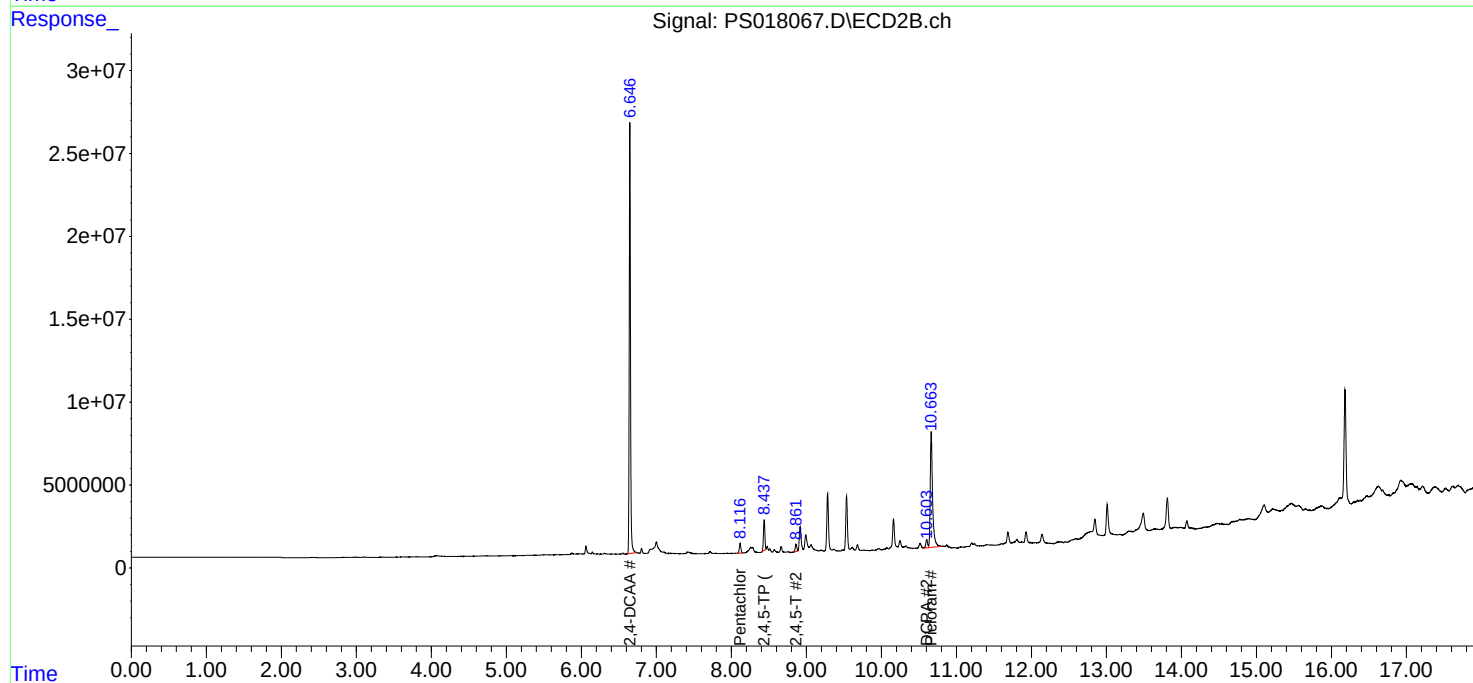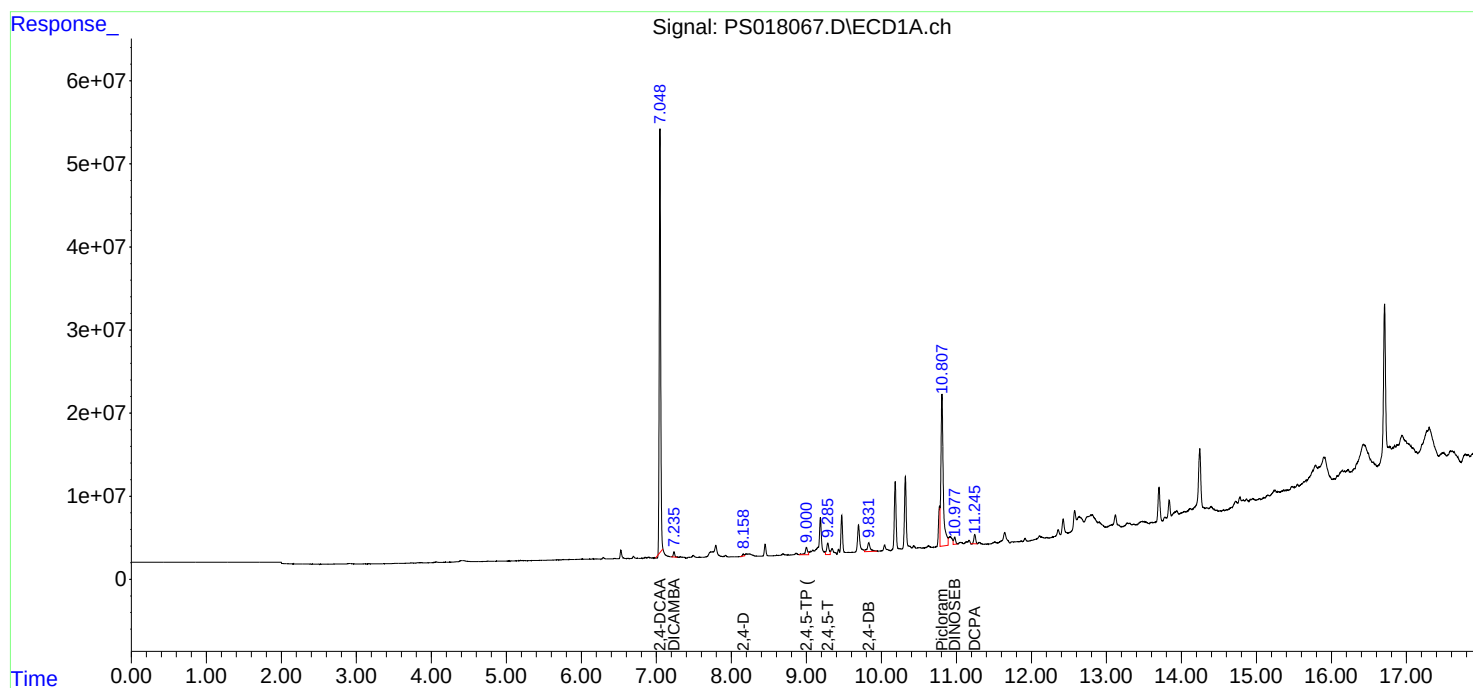


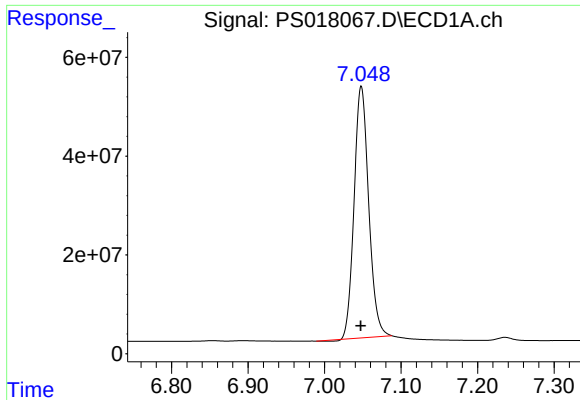

#4 2,4-DCAA


R.T.: 7.048 min
Delta R.T.: 0.000 min
Response: 675128984
Conc: 467.06 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

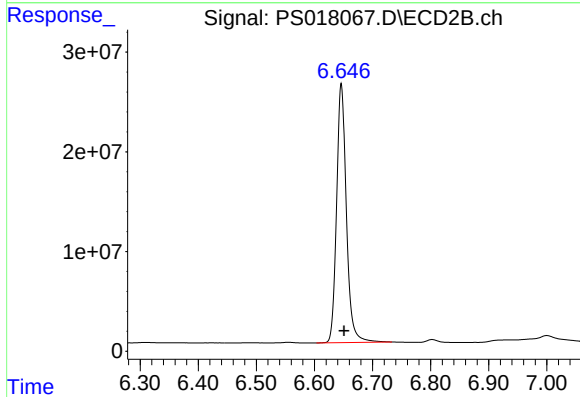


#4 2,4-DCAA

R.T.: 6.646 min
Delta R.T.: -0.005 min
Response: 303109212
Conc: 522.38 ng/ml

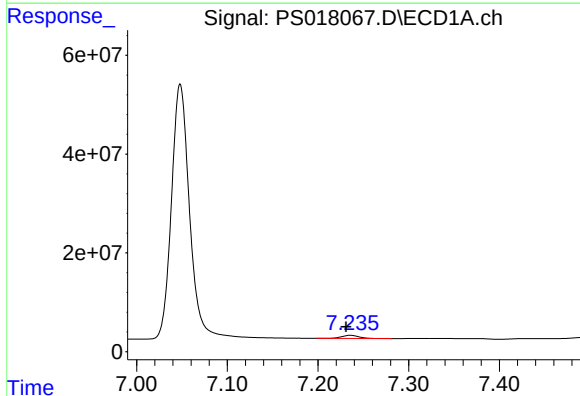


#5 DICAMBA

R.T.: 7.235 min
Delta R.T.: 0.005 min
Response: 8420223
Conc: 1.35 ng/ml

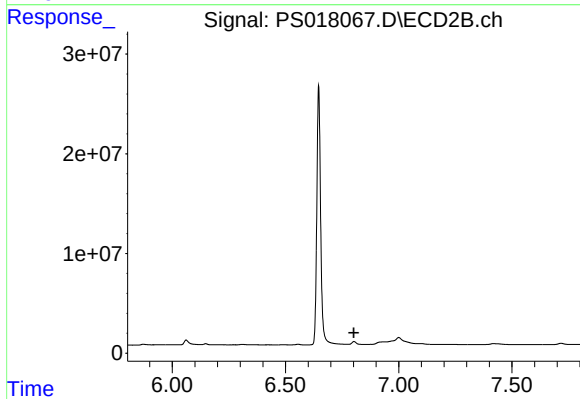

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 6.802 min
Response: 0
Conc: N.D.

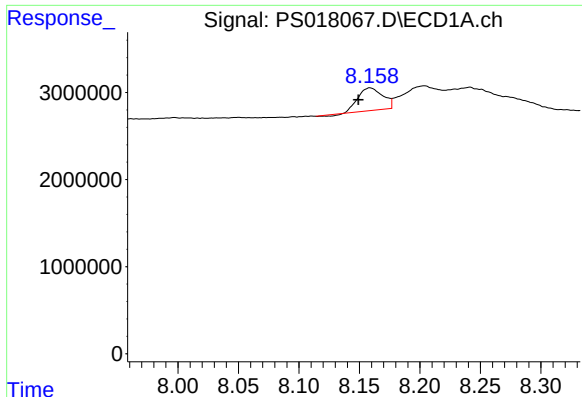

#9 2,4-D


R.T.: 8.159 min
Delta R.T.: 0.010 min
Response: 3620678
Conc: 1.99 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

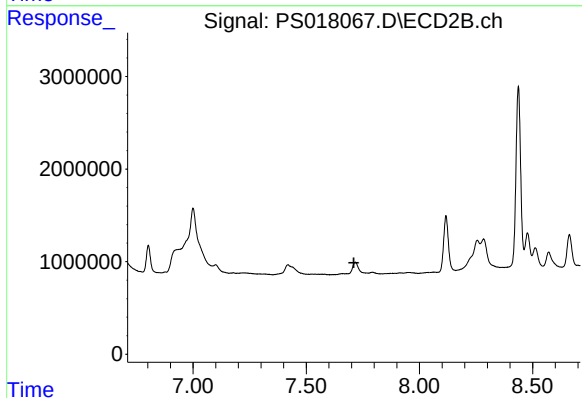


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.710 min
Response: 0
Conc: N.D.

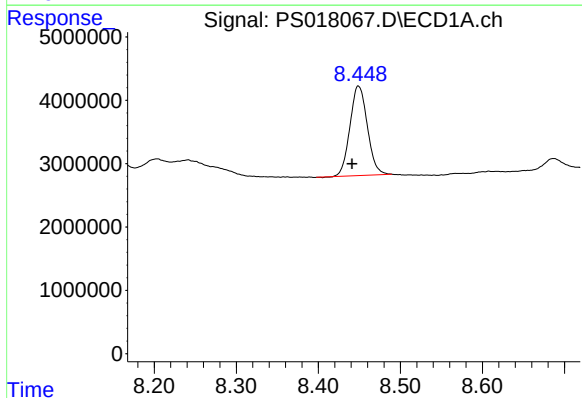


#10 Pentachlorophenol

R.T.: 8.449 min
Delta R.T.: 0.008 min
Response: 20865743
Conc: N.D.

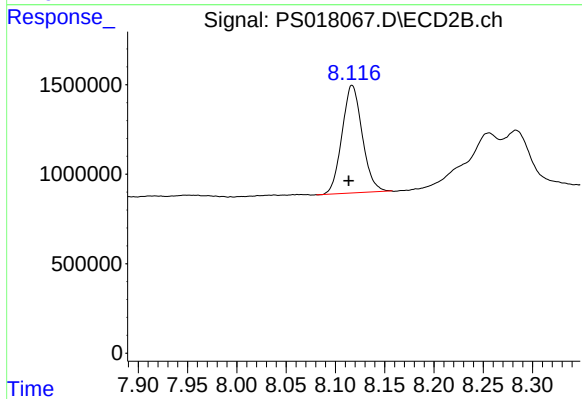

#10 Pentachlorophenol


R.T.: 8.117 min
Delta R.T.: 0.003 min
Response: 8592166
Conc: 1.02 ng/ml

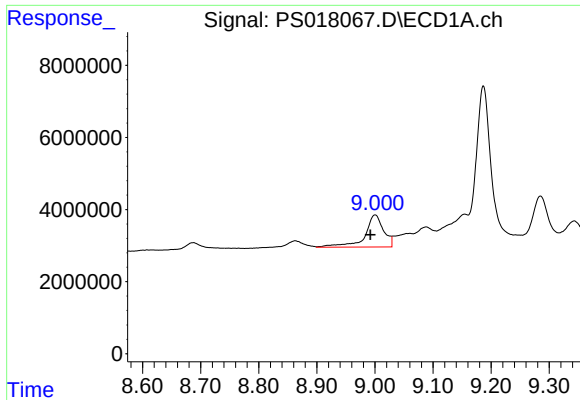

#11 2,4,5-TP (SILVEX)


R.T.: 9.000 min
Delta R.T.: 0.008 min
Response: 19939128
Conc: 2.36 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

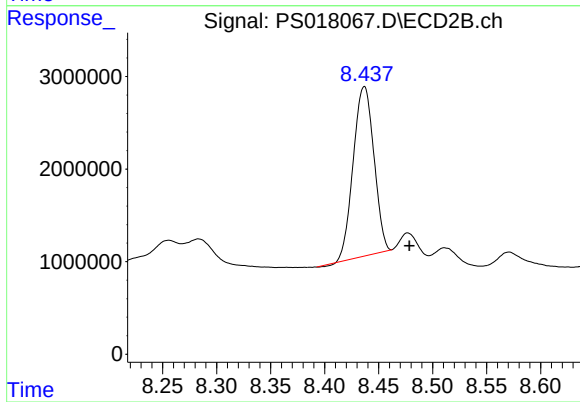


#11 2,4,5-TP (SILVEX)

R.T.: 8.437 min
Delta R.T.: -0.042 min
Response: 24349278
Conc: 6.83 ng/ml

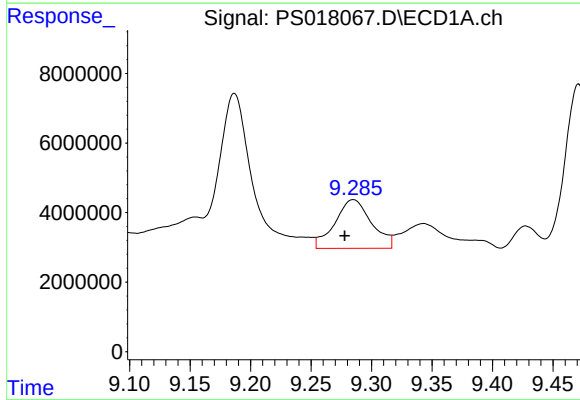


#12 2,4,5-T

R.T.: 9.285 min
Delta R.T.: 0.007 min
Response: 29497108
Conc: 3.33 ng/ml

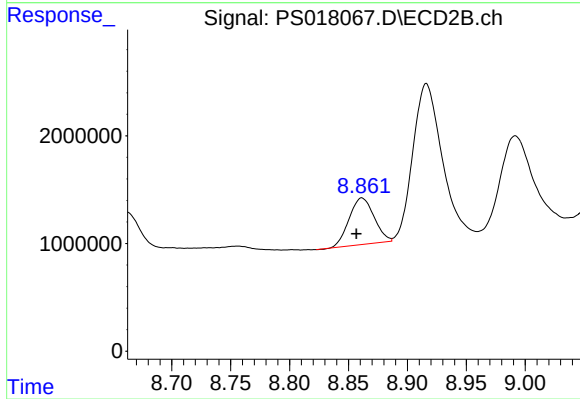

#12 2,4,5-T


R.T.: 8.861 min
Delta R.T.: 0.005 min
Response: 6353140
Conc: 1.94 ng/ml

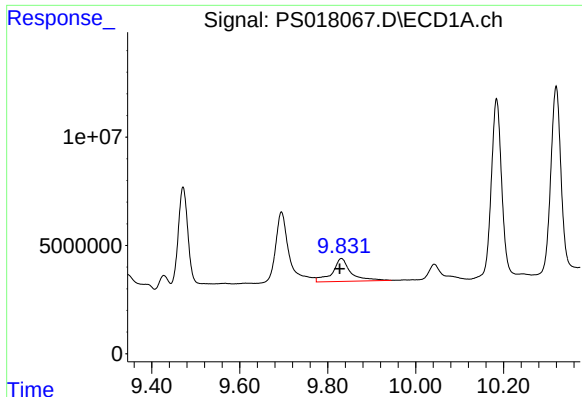

#13 2,4-DB


R.T.: 9.831 min
Delta R.T.: 0.004 min
Response: 30765239
Conc: 18.61 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

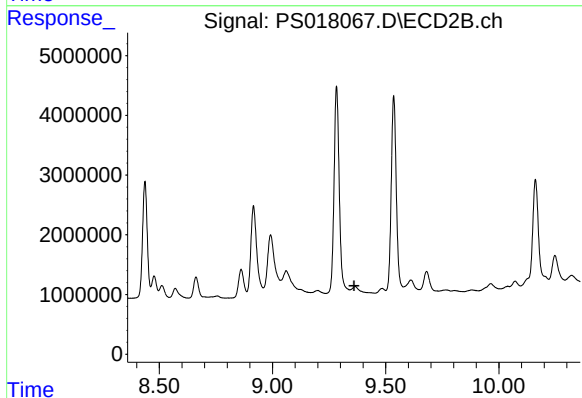


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.360 min
Response: 0
Conc: N.D.

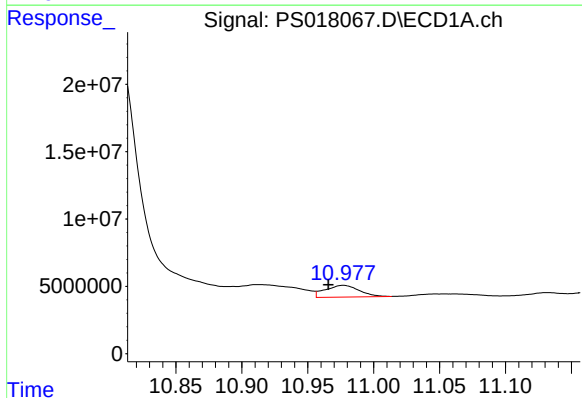


#14 DINOSEB

R.T.: 10.977 min
Delta R.T.: 0.011 min
Response: 15481580
Conc: 2.36 ng/ml

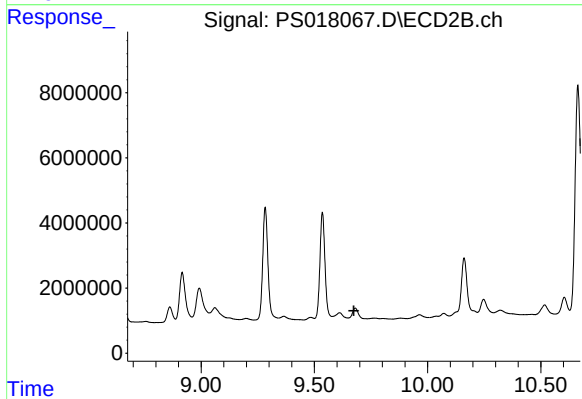

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.675 min
Response: 0
Conc: N.D.

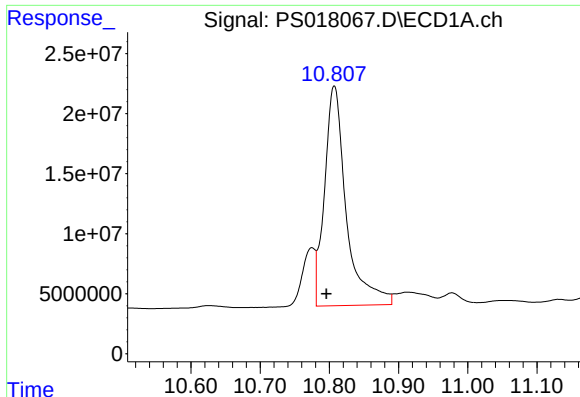

#15 Picloram


R.T.: 10.807 min
Delta R.T.: 0.011 min
Response: 400983807
Conc: 33.59 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

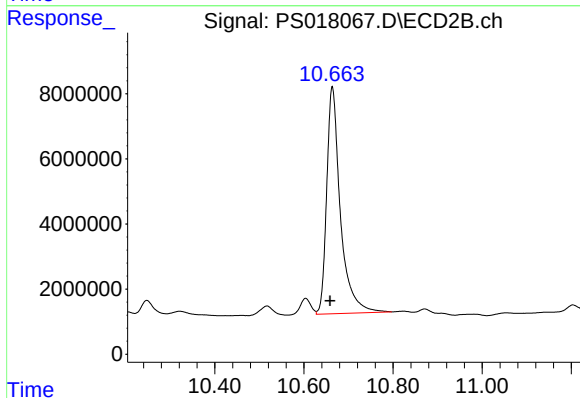


#15 Picloram

R.T.: 10.664 min
Delta R.T.: 0.005 min
Response: 148442690
Conc: 31.74 ng/ml

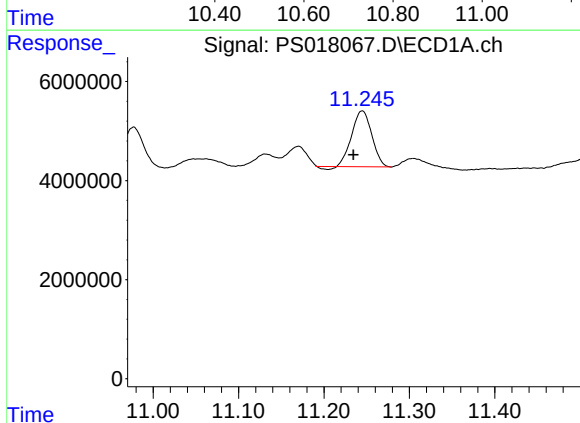

#16 DCPA

R.T.: 11.245 min
Delta R.T.: 0.010 min
Response: 18246154
Conc: 1.69 ng/ml

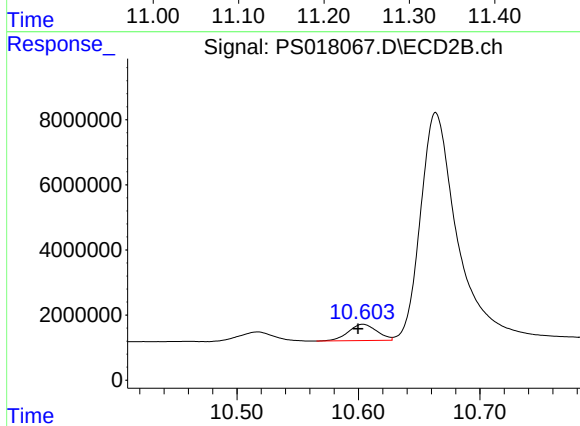

#16 DCPA

R.T.: 10.604 min
Delta R.T.: 0.004 min
Response: 8183964
Conc: 1.85 ng/ml