

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011823\
 Data File : PS021796.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jan 2023 09:04
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 18 20:26:56 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010923.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 10 10:34:52 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.379	6.811	1423.7E6	1099.4E6	511.459	611.920
Target Compounds							
1) T	Dalapon	2.512	0.000	88597	0	<MDL	N.D. #
3) T	4-Nitroph...	6.227	0.000	7123775	0	4.887	N.D. #
6) T	MCP	0.000	7.120f	0	3118271	N.D.	<MDL
7) T	MCPA	6.763	7.219f	452782	30590348	<MDL	3.373 #
10) T	Pentachlo...	7.555	0.000	931418	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.088	0.000	561982	0	<MDL	N.D. #
12) T	2,4,5-T	8.346	9.098f	19462469	334000	1.010	<MDL #
14) T	DINOSEB	9.844f	0.000	82037138	0	4.998	N.D. #
15) T	Picloram	9.756	10.818f	15976415	9242689	<MDL	<MDL #
16) T	DCPA	10.165	10.818	1132990	9242689	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011823\
Data File : PS021796.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jan 2023 09:04
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 18 20:26:56 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010923.M
Quant Title : 8080.M
QLast Update : Tue Jan 10 10:34:52 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

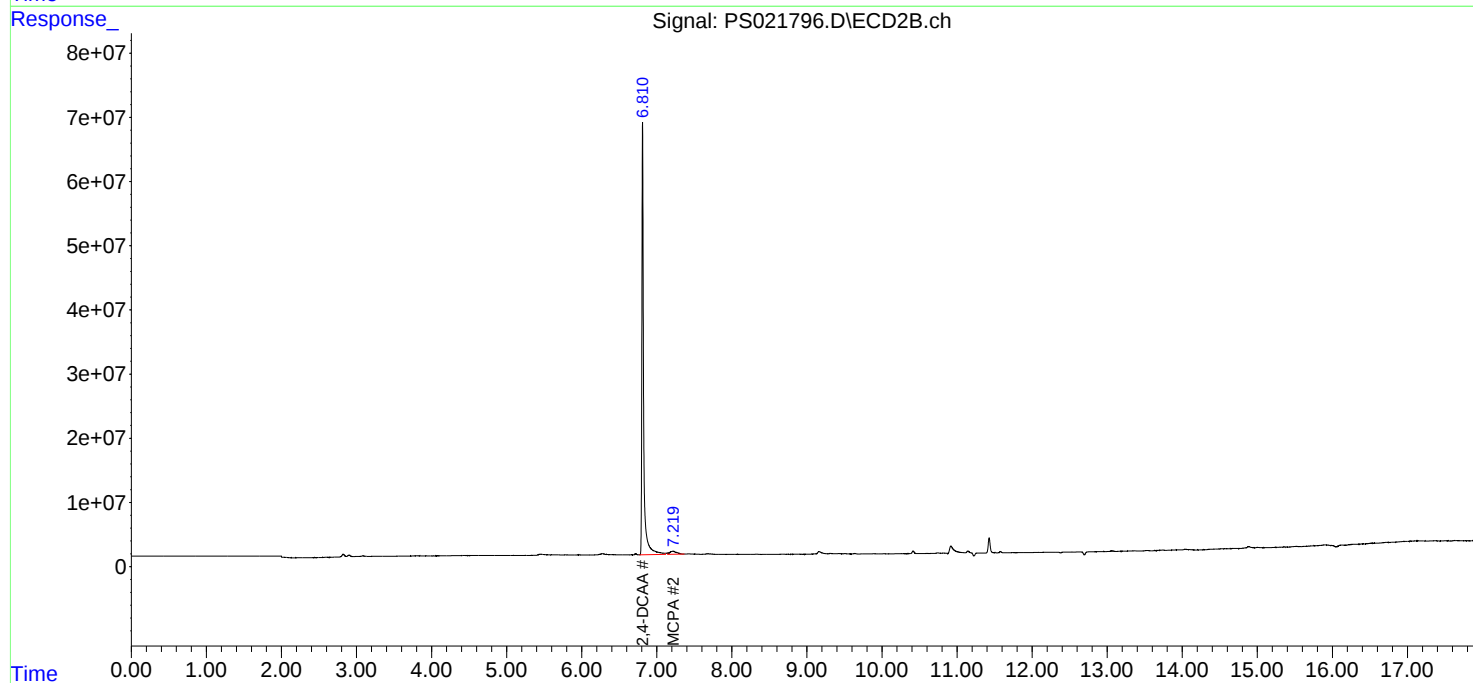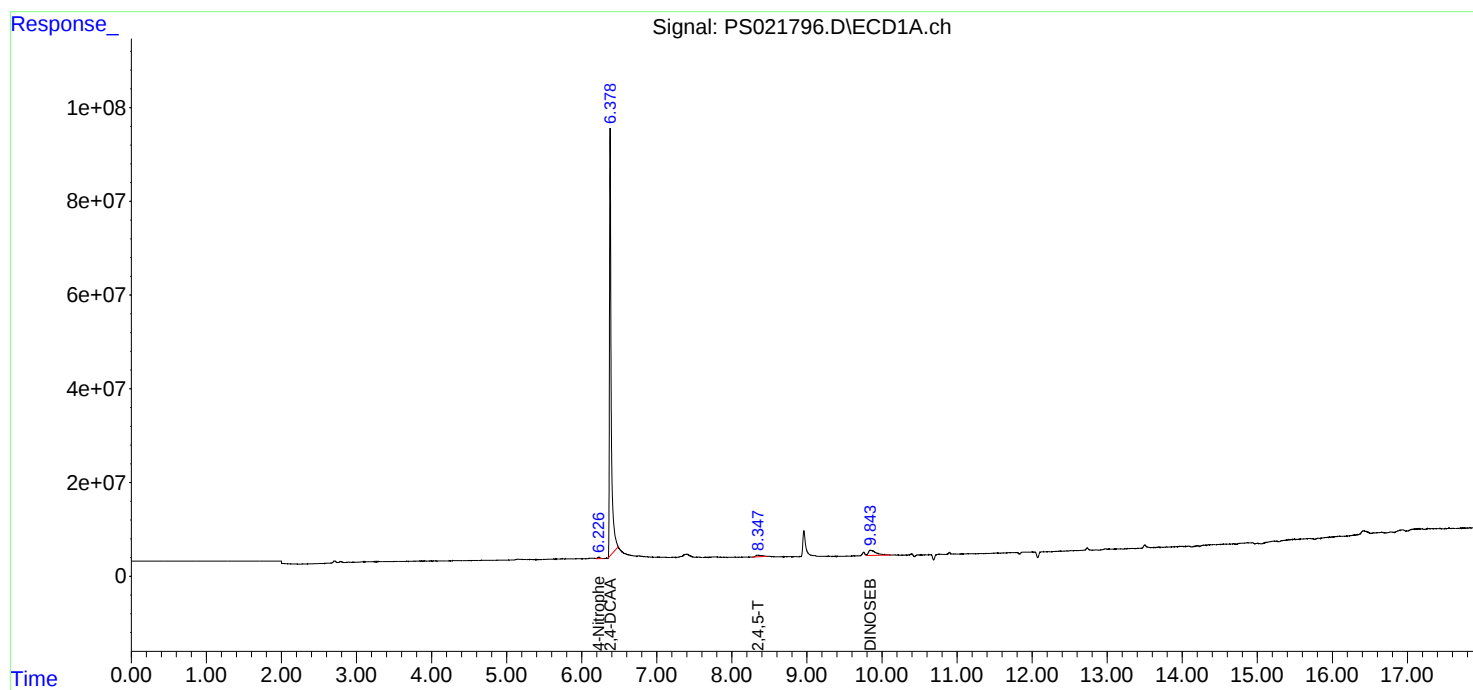


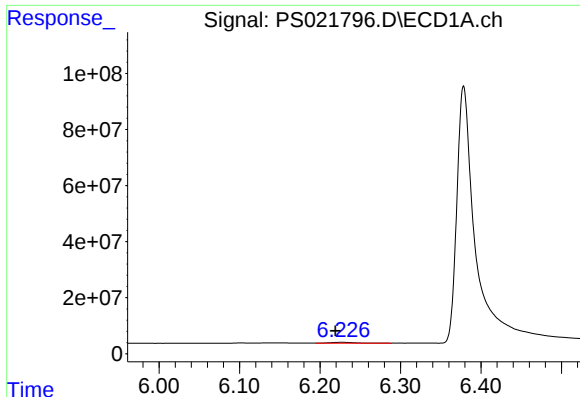

#3 4-Nitrophenol


R.T.: 6.227 min
Delta R.T.: 0.008 min
Response: 7123775
Conc: 4.89 ng/ml

Instrument :
ECD_S
ClientSampleId :

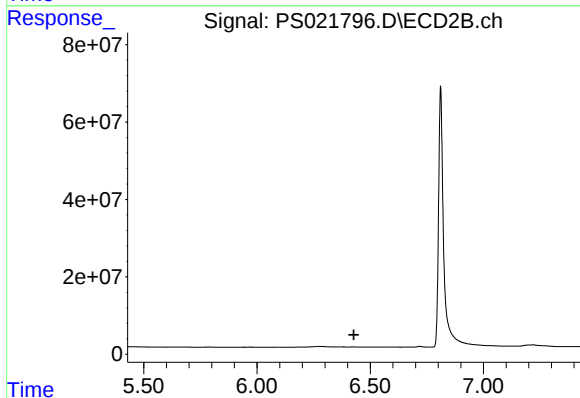


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.428 min
Response: 0
Conc: N.D.

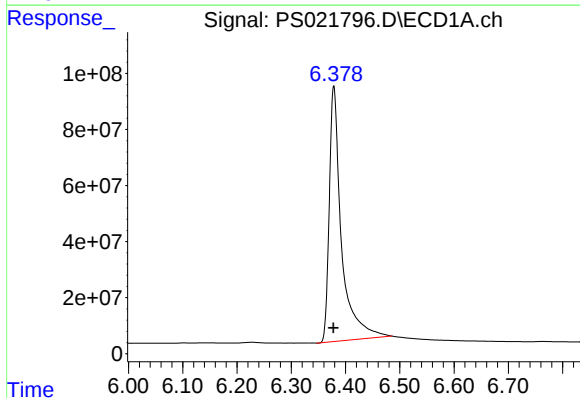


#4 2,4-DCAA

R.T.: 6.379 min
Delta R.T.: 0.001 min
Response: 1423679209
Conc: 511.46 ng/ml

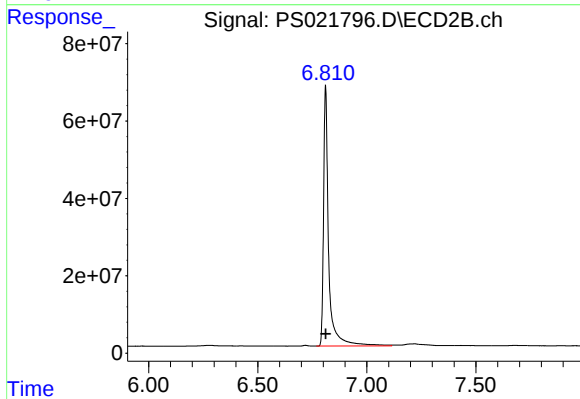

#4 2,4-DCAA


R.T.: 6.811 min
Delta R.T.: 0.000 min
Response: 1099429673
Conc: 611.92 ng/ml

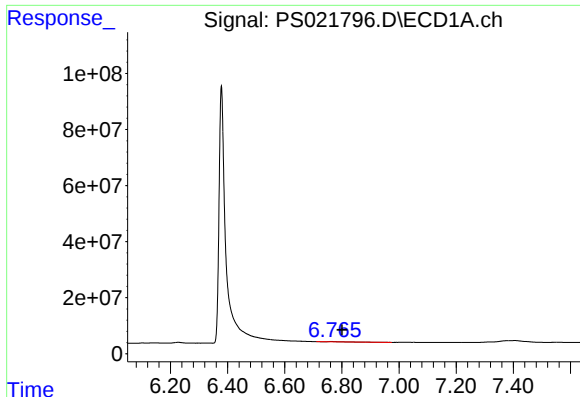

#7 MCPA


R.T.: 6.763 min
Delta R.T.: -0.038 min
Response: 452782
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

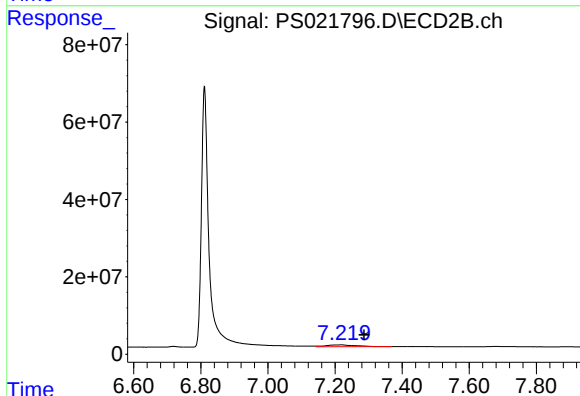


#7 MCPA

R.T.: 7.219 min
Delta R.T.: -0.068 min
Response: 30590348
Conc: 3.37 ug/ml

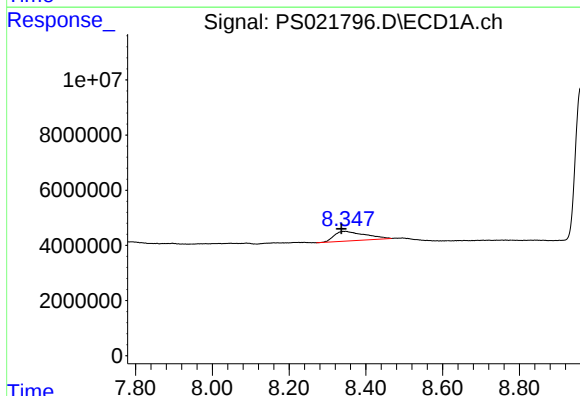


#12 2,4,5-T

R.T.: 8.346 min
Delta R.T.: 0.009 min
Response: 19462469
Conc: 1.01 ng/ml

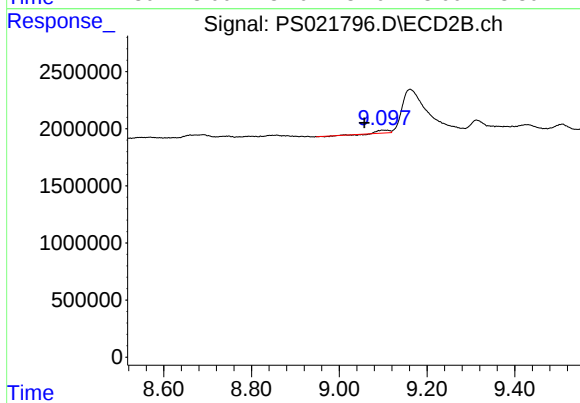

#12 2,4,5-T


R.T.: 9.098 min
Delta R.T.: 0.040 min
Response: 334000
Conc: N.D.

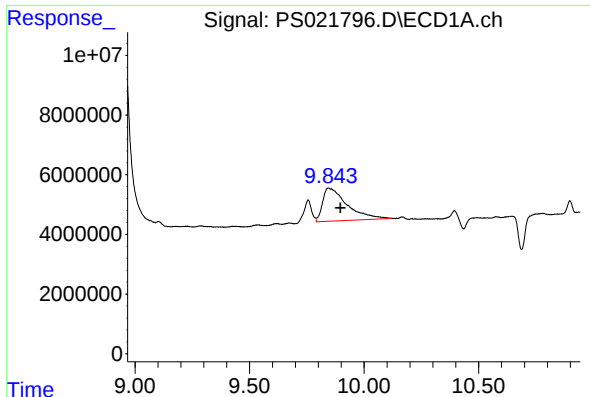

#14 DINOSEB

R.T.: 9.844 min
Delta R.T.: -0.052 min
Response: 82037138
Conc: 5.00 ng/ml

Instrument :
ECD_S
ClientSampleId :

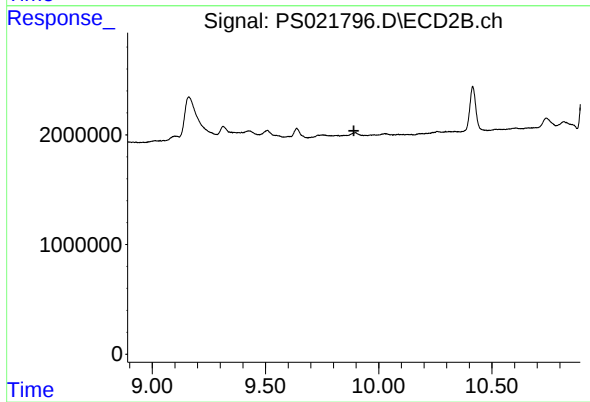

#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.890 min
Response: 0
Conc: N.D.