

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011823\
 Data File : PS021799.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jan 2023 10:49
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 18 20:28:08 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010923.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 10 10:34:52 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.379	6.811	1442.6E6	1099.7E6	518.247	612.077
Target Compounds							
1) T	Dalapon	2.515	2.590	357149	404587	<MDL	<MDL #
3) T	4-Nitroph...	6.226	0.000	6901135	0	4.735	N.D. #
6) T	MCP	0.000	7.115f	0	3980381	N.D.	<MDL
7) T	MCPA	6.764	0.000	3188306	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.668f	0	1748727	N.D.	<MDL
10) T	Pentachlo...	7.556	0.000	1318951	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.094	8.657	3320822	2771165	<MDL	<MDL #
12) T	2,4,5-T	8.333	9.092	9626160	2822088	<MDL	<MDL #
13) T	2,4-DB	8.842	9.502f	426153	2435401	<MDL	1.625 #
14) T	DINOSEB	9.863	0.000	62218791	0	3.791	N.D. #
15) T	Picloram	9.755	10.821f	20571518	10396117	<MDL	<MDL #
16) T	DCPA	10.165	10.821	1184008	10396117	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011823\
Data File : PS021799.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jan 2023 10:49
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 18 20:28:08 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010923.M
Quant Title : 8080.M
QLast Update : Tue Jan 10 10:34:52 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

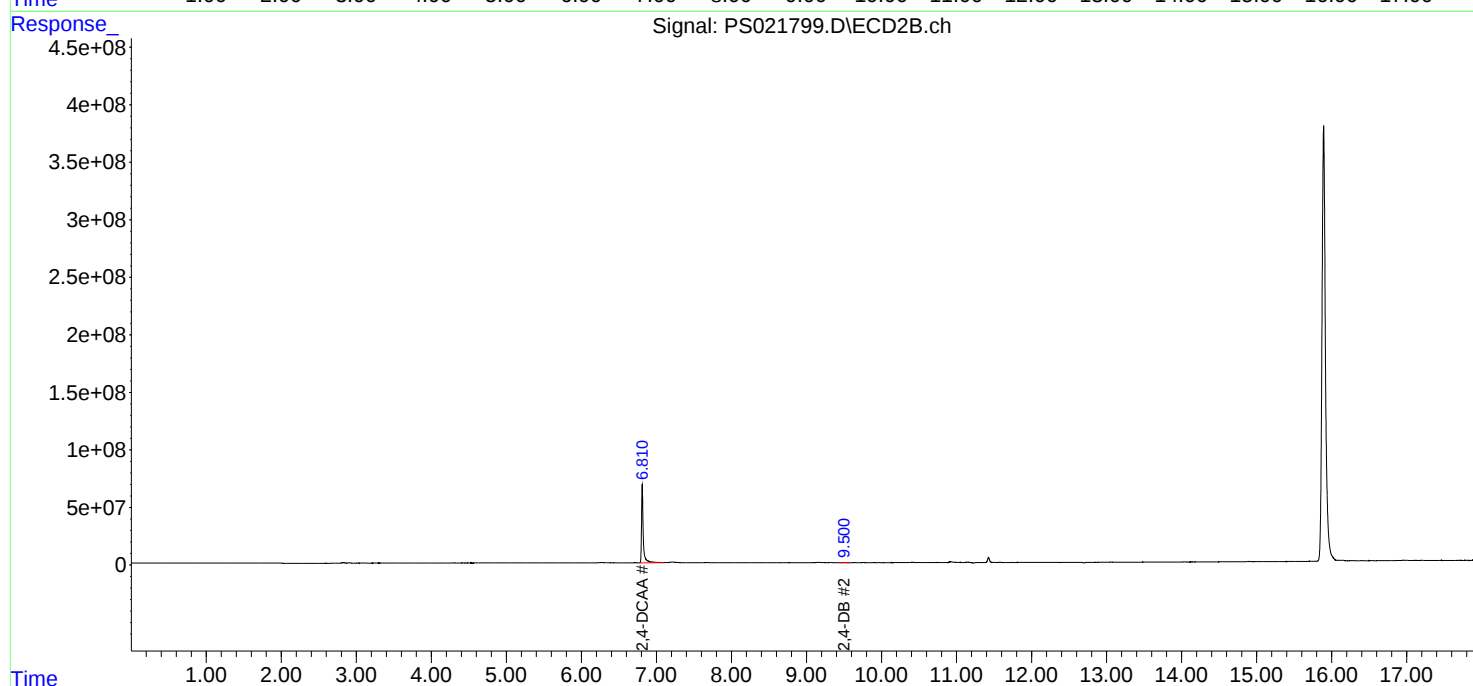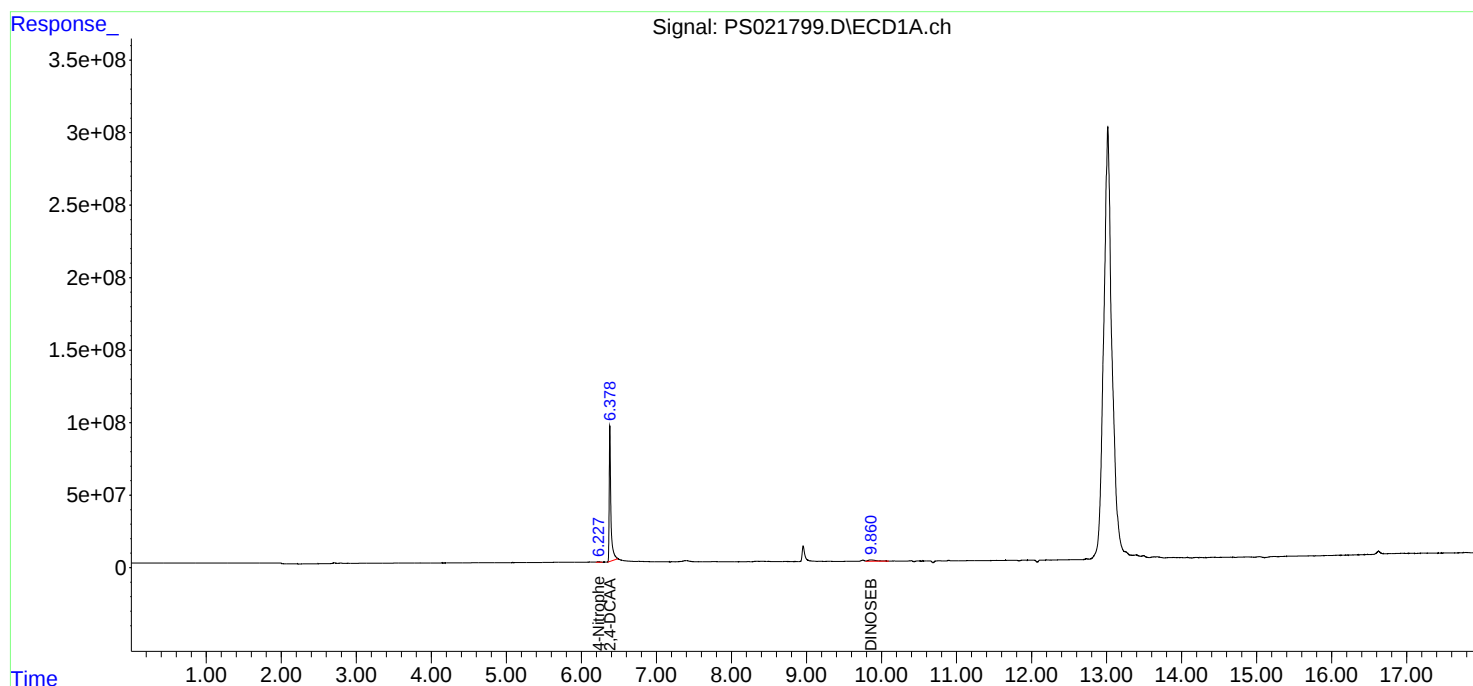


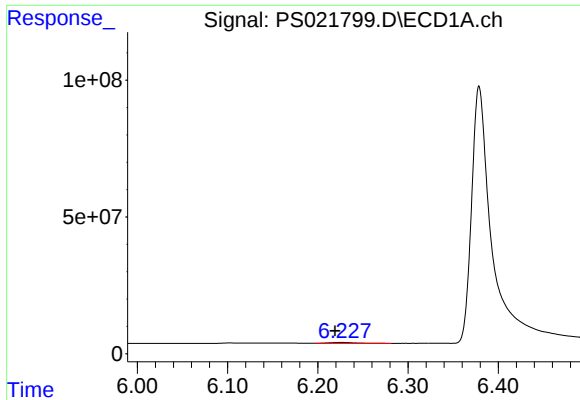

#3 4-Nitrophenol


R.T.: 6.226 min
Delta R.T.: 0.007 min
Response: 6901135
Conc: 4.73 ng/ml

Instrument :
ECD_S
ClientSampleId :

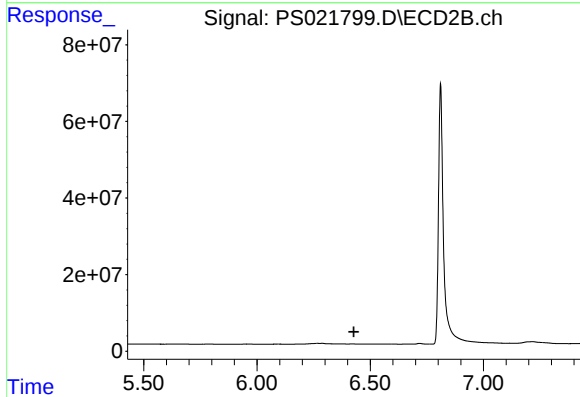


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.428 min
Response: 0
Conc: N.D.

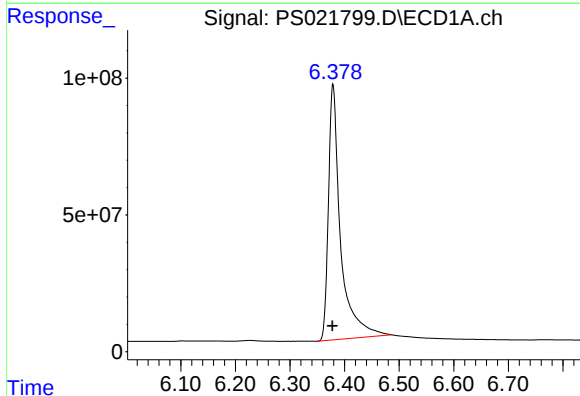


#4 2,4-DCAA

R.T.: 6.379 min
Delta R.T.: 0.002 min
Response: 1442574192
Conc: 518.25 ng/ml

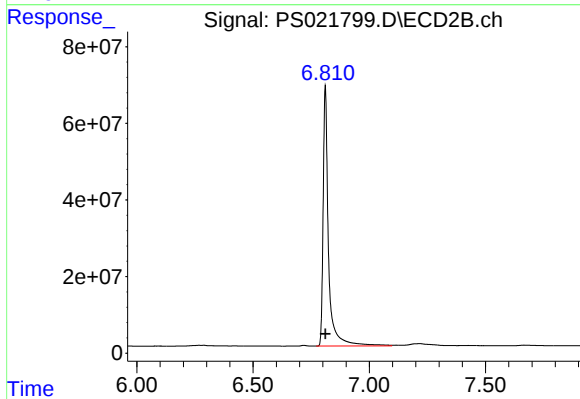

#4 2,4-DCAA


R.T.: 6.811 min
Delta R.T.: 0.000 min
Response: 1099712431
Conc: 612.08 ng/ml

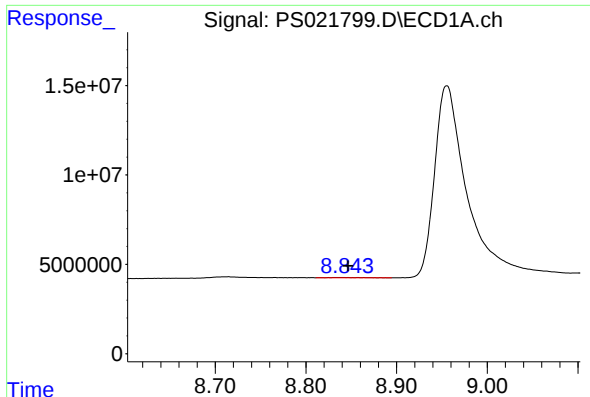

#13 2,4-DB


R.T.: 8.842 min
Delta R.T.: -0.005 min
Response: 426153
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

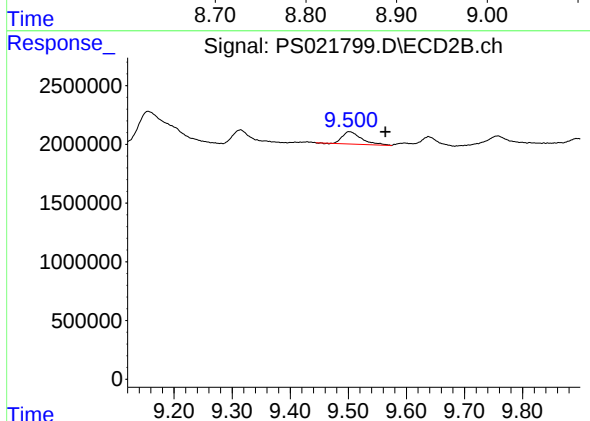


#13 2,4-DB

R.T.: 9.502 min
Delta R.T.: -0.062 min
Response: 2435401
Conc: 1.63 ng/ml

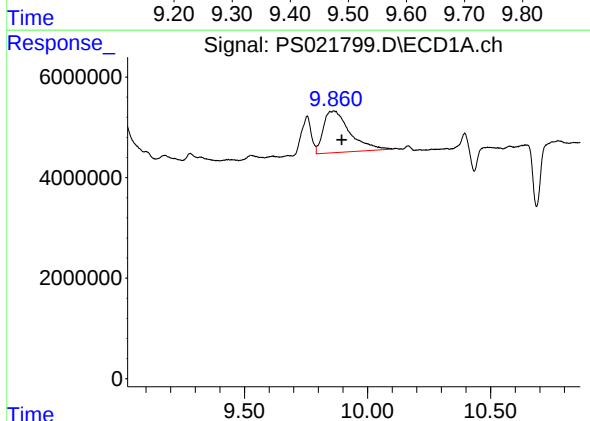

#14 DINOSEB

R.T.: 9.863 min
Delta R.T.: -0.033 min
Response: 62218791
Conc: 3.79 ng/ml

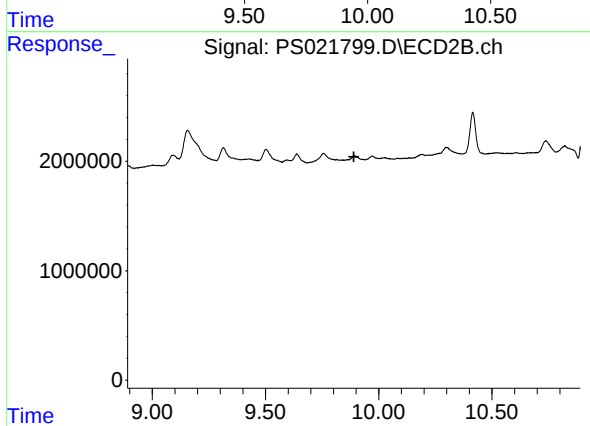

#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 9.890 min
Response: 0
Conc: N.D.