

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011824\
 Data File : PS025583.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jan 2024 20:28
 Operator : AR\AJ
 Sample : I,BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 19 00:11:46 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS011124.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 11 16:45:24 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	6.351	6.760	758.1E6	397.0E6	508.998	517.080
Target Compounds						
1) T Dalapon	0.000	2.557	0	3107344	N.D.	2.645
2) T 3,5-DICHL...	5.693	0.000	1020090	0	<MDL	N.D. #
5) T DICAMBA	0.000	6.957	0	1698934	N.D.	<MDL
6) T MCPP	0.000	6.957f	0	1698934	N.D.	<MDL
7) T MCPA	0.000	7.231	0	2971763	N.D.	<MDL
8) T DICHLORPROP	0.000	7.566	0	2990904	N.D.	3.460
9) T 2,4-D	7.250	0.000	17273516	0	9.381	N.D. #
12) T 2,4,5-T	0.000	8.987	0	628429	N.D.	<MDL
15) T Picloram	9.662	10.722	25638032	9023879	2.478	1.697 #
16) T DCPA	0.000	10.722	0	9023879	N.D.	1.552



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011824\
Data File : PS025583.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jan 2024 20:28
Operator : AR\AJ
Sample : I,BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 19 00:11:46 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS011124.M
Quant Title : 8080.M
QLast Update : Thu Jan 11 16:45:24 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

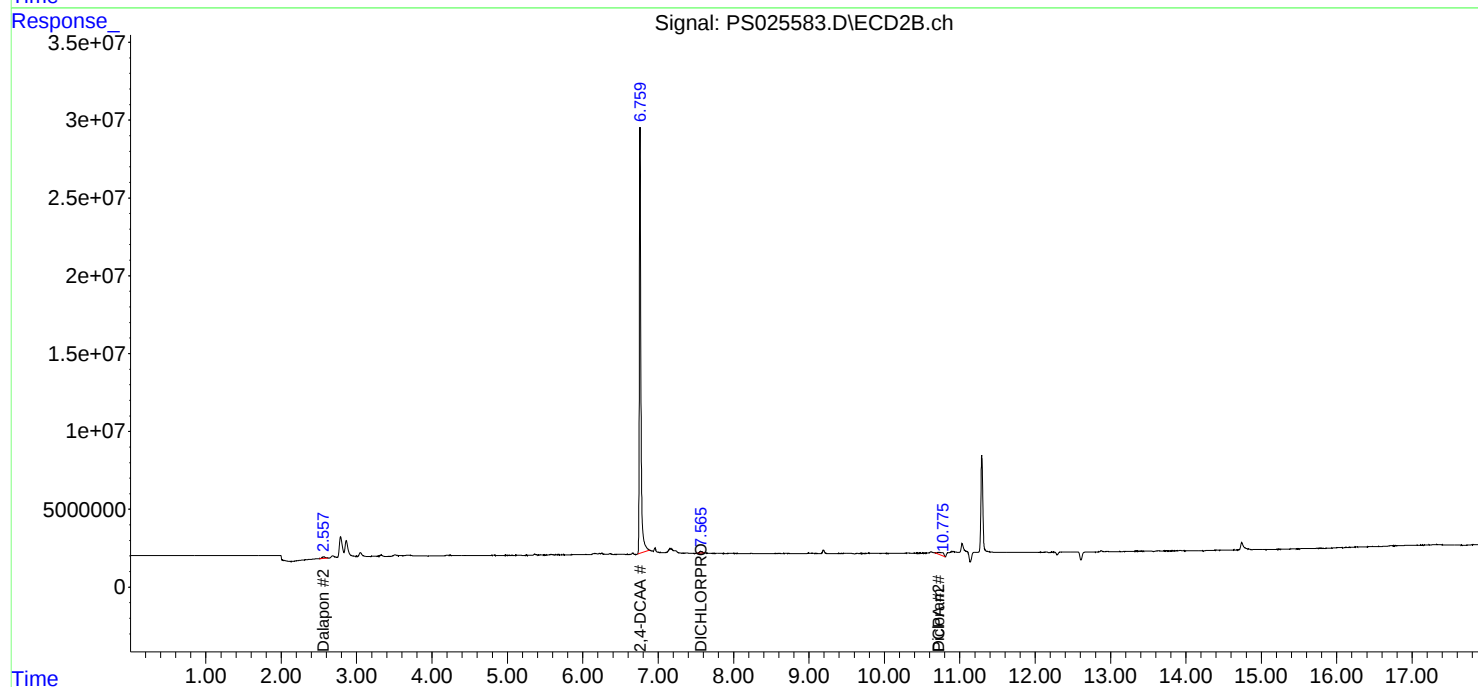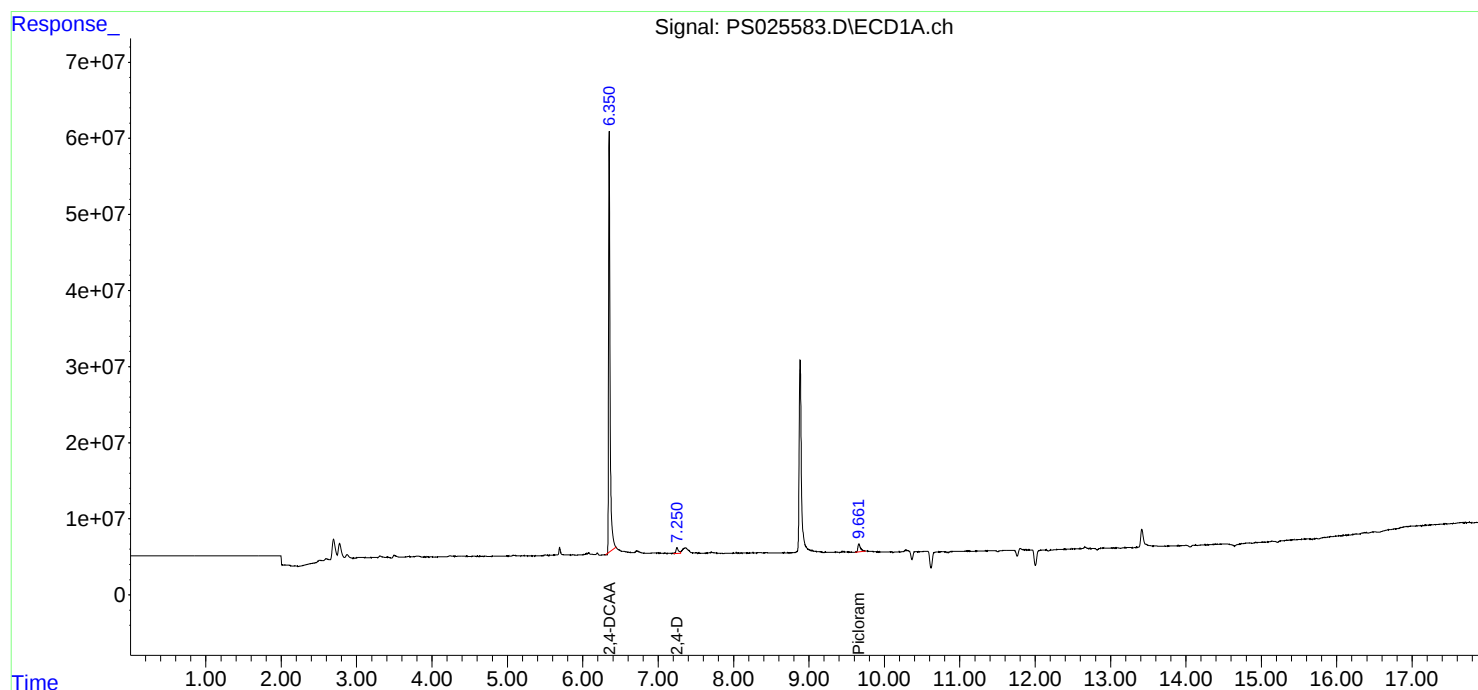

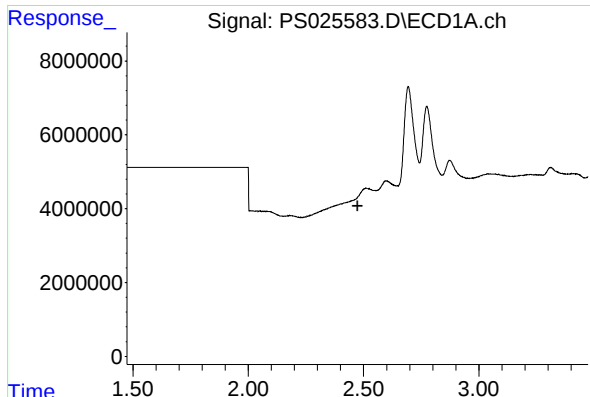

#1 Dalapon

R.T.: 0.000 min
Exp R.T.: 2.474 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

#1 Dalapon


R.T.: 2.557 min
Delta R.T.: 0.028 min
Response: 3107344
Conc: 2.64 ng/ml

#4 2,4-DCAA

R.T.: 6.351 min
Delta R.T.: 0.000 min
Response: 758133589
Conc: 509.00 ng/ml

#4 2,4-DCAA


R.T.: 6.760 min
Delta R.T.: -0.001 min
Response: 397014129
Conc: 517.08 ng/ml

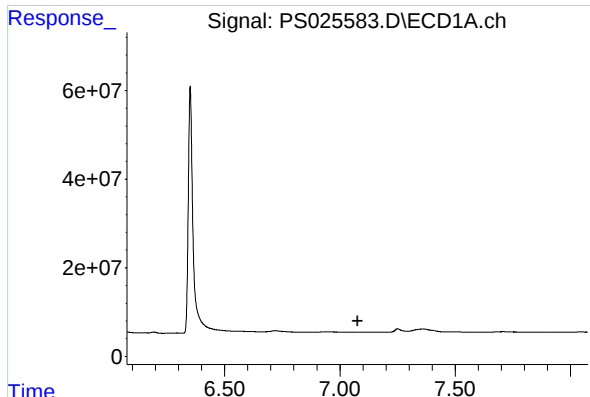

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.077 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

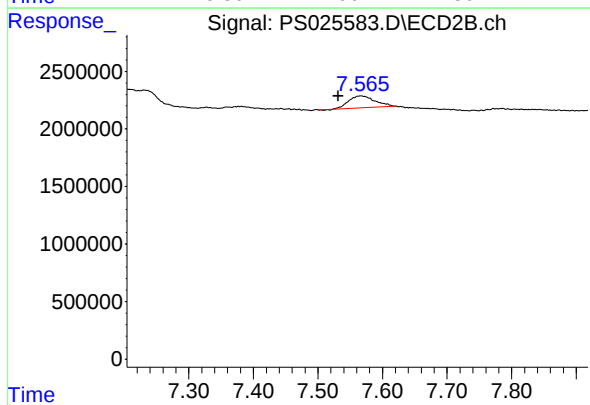


#8 DICHLORPROP

R.T.: 7.566 min
Delta R.T.: 0.035 min
Response: 2990904
Conc: 3.46 ng/ml

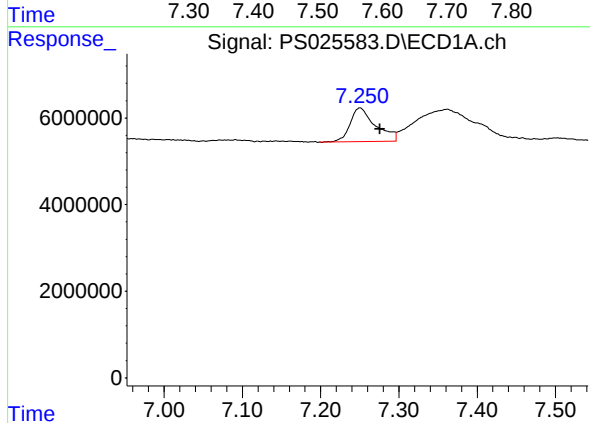


#9 2,4-D

R.T.: 7.250 min
Delta R.T.: -0.025 min
Response: 17273516
Conc: 9.38 ng/ml

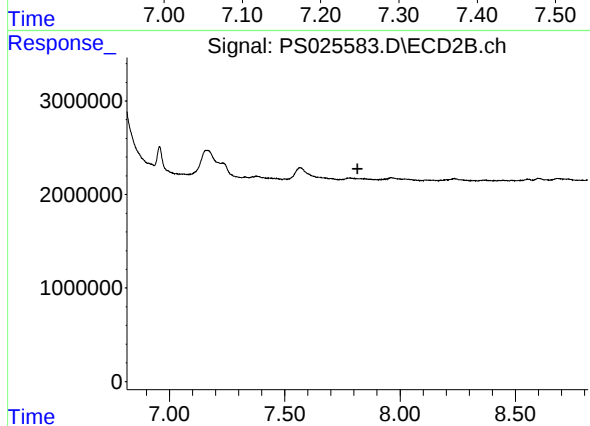

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.815 min
Response: 0
Conc: N.D.

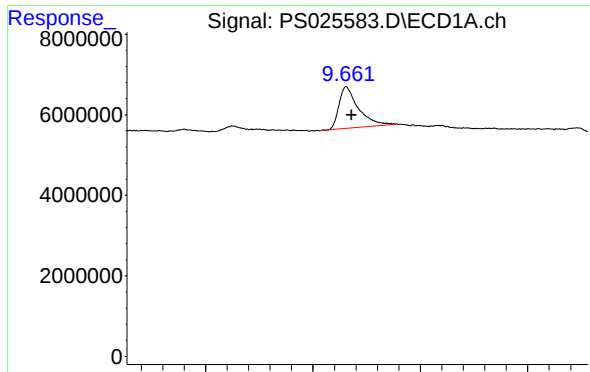

#15 Picloram


R.T.: 9.662 min
Delta R.T.: -0.011 min
Response: 25638032
Conc: 2.48 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

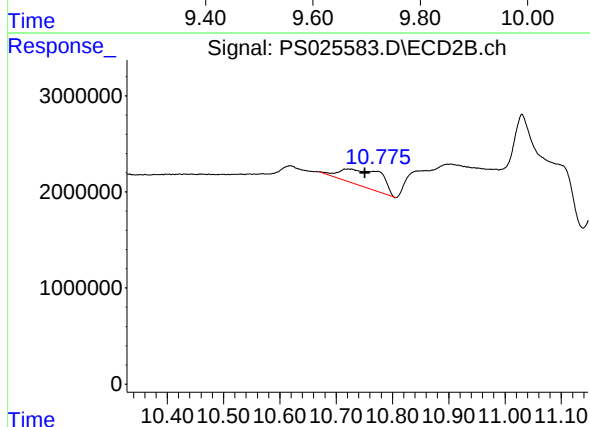


#15 Picloram

R.T.: 10.722 min
Delta R.T.: -0.029 min
Response: 9023879
Conc: 1.70 ng/ml

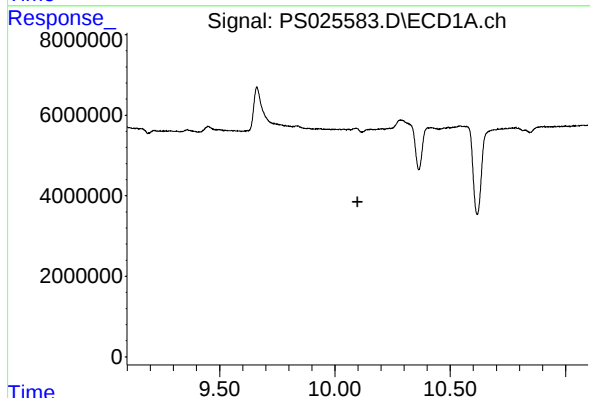

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.098 min
Response: 0
Conc: N.D.

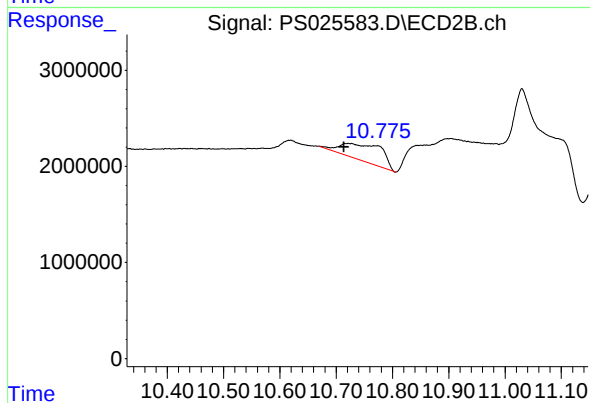

#16 DCPA

R.T.: 10.722 min
Delta R.T.: 0.008 min
Response: 9023879
Conc: 1.55 ng/ml