

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011922\
 Data File : PS018069.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jan 2022 08:41
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 20 00:47:14 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 06 10:21:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
5) T	DICAMBA	7.235	0.000	7750673	0	1.241	N.D. #
8) T	DICHLORPROP	7.922	0.000	2883259	0	1.833	N.D. #
9) T	2,4-D	8.149	0.000	10375592	0	5.698	N.D. #
10) T	Pentachlo...	8.448	8.112	22553427	9006751	1.068	1.069
11) T	2,4,5-TP ...	8.998	8.473	25904852	3742500	3.061	1.050 #
12) T	2,4,5-T	9.283	8.853	44024080	11782227	4.967	3.602 #
13) T	2,4-DB	9.821	0.000	31743744	0	19.203	N.D. #
14) T	DINOSEB	10.976	9.675	11699737	7451937	1.782	2.987 #
15) T	Picloram	10.801	10.655	493.6E6	174.1E6	41.353	37.239
16) T	DCPA	11.244	10.599	27383002	12673835	2.534	2.870



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011922\
Data File : PS018069.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jan 2022 08:41
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 20 00:47:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
Quant Title : 8080.M
QLast Update : Thu Jan 06 10:21:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

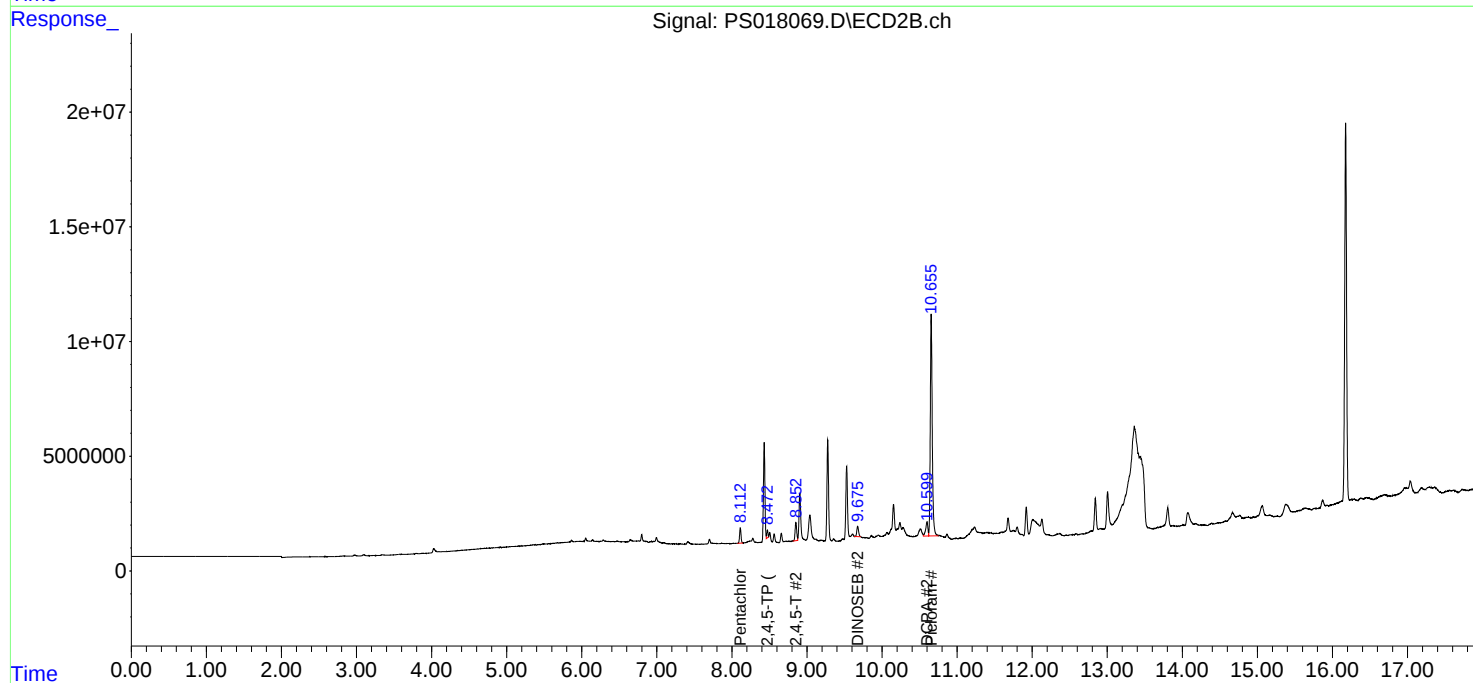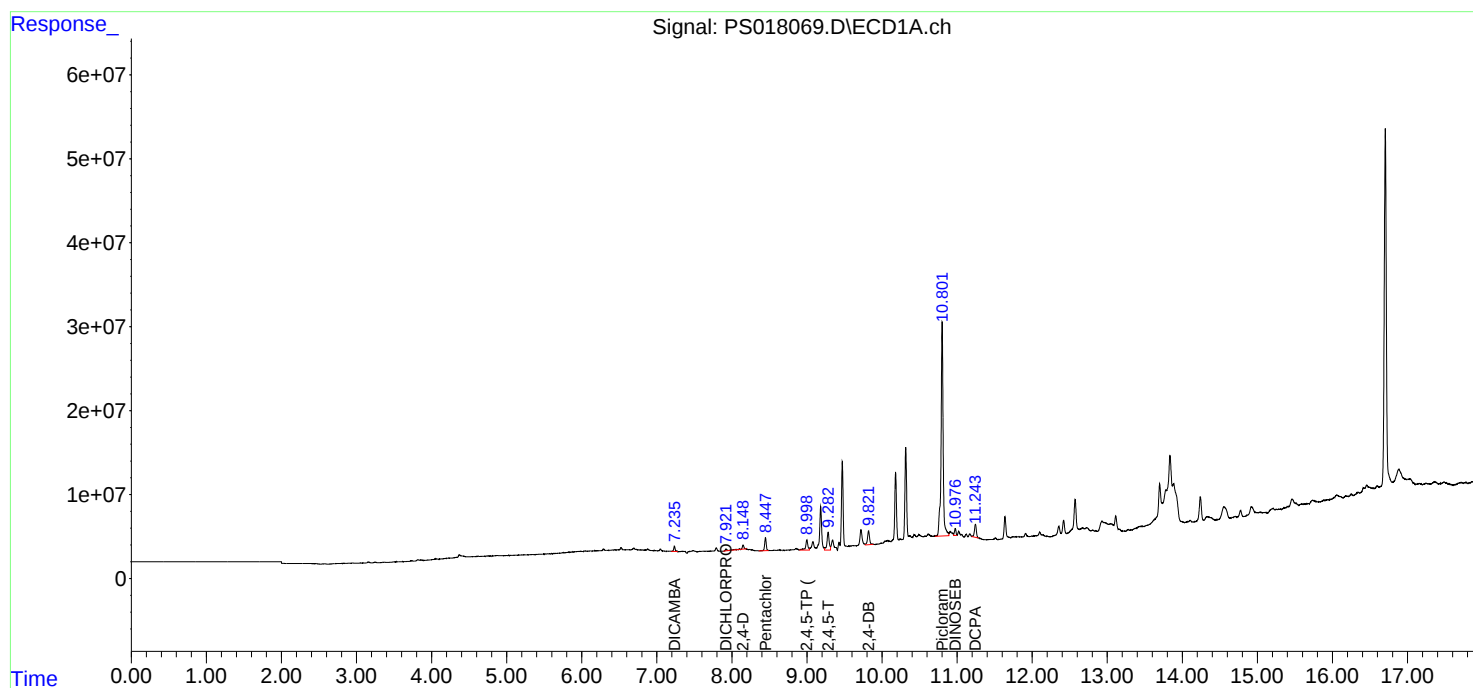


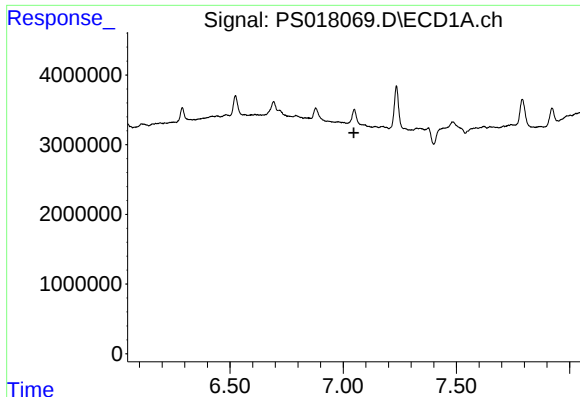

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 7.047 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

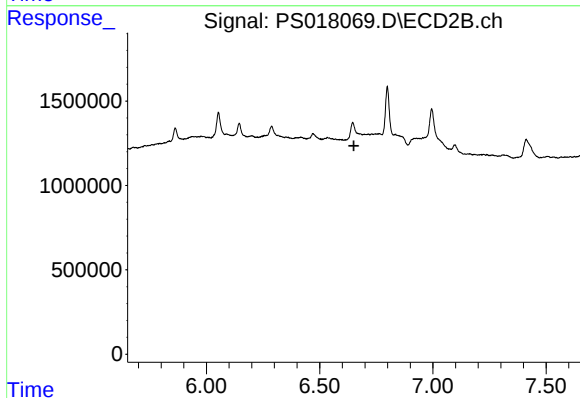


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.651 min
Response: 0
Conc: N.D.

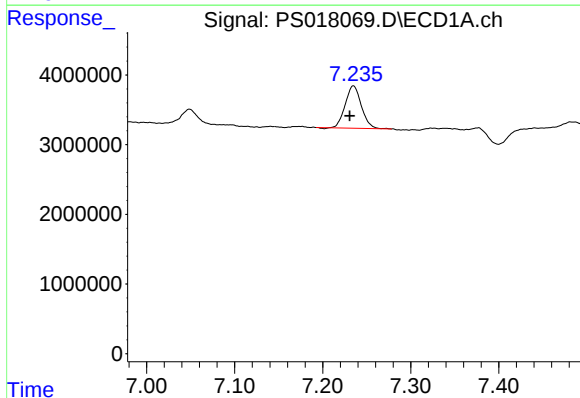


#5 DICAMBA

R.T.: 7.235 min
Delta R.T.: 0.004 min
Response: 7750673
Conc: 1.24 ng/ml

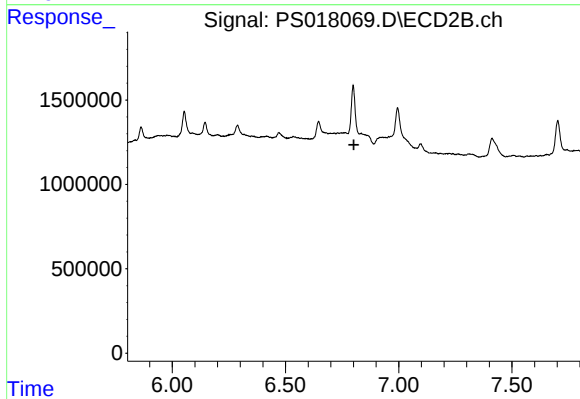

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 6.802 min
Response: 0
Conc: N.D.

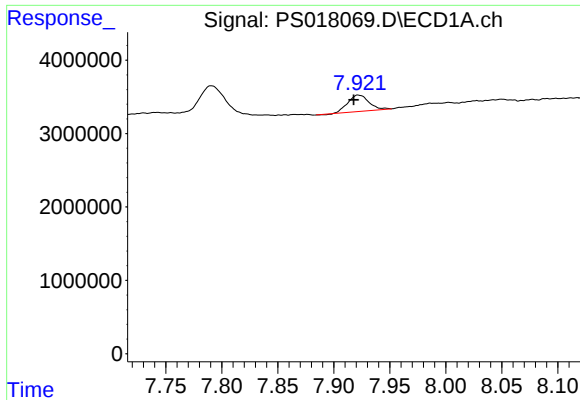

#8 DICHLORPROP


R.T.: 7.922 min
Delta R.T.: 0.004 min
Response: 2883259
Conc: 1.83 ng/ml

Instrument :
ECD_S
ClientSampleId :

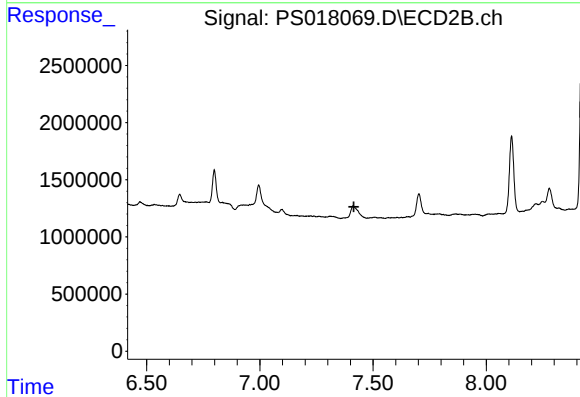


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 7.415 min
Response: 0
Conc: N.D.

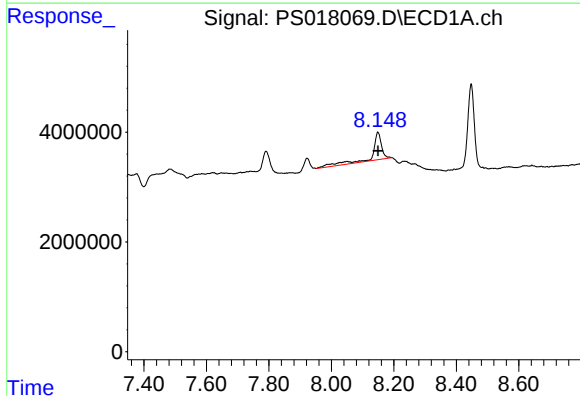


#9 2,4-D

R.T.: 8.149 min
Delta R.T.: 0.000 min
Response: 10375592
Conc: 5.70 ng/ml

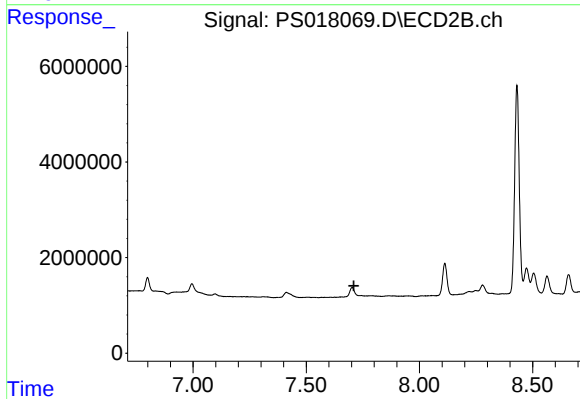

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.710 min
Response: 0
Conc: N.D.

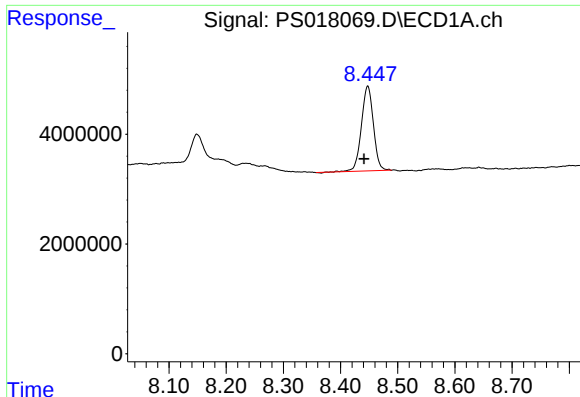

#10 Pentachlorophenol


R.T.: 8.448 min
Delta R.T.: 0.006 min
Response: 22553427
Conc: 1.07 ng/ml

Instrument :
ECD_S
ClientSampleId :

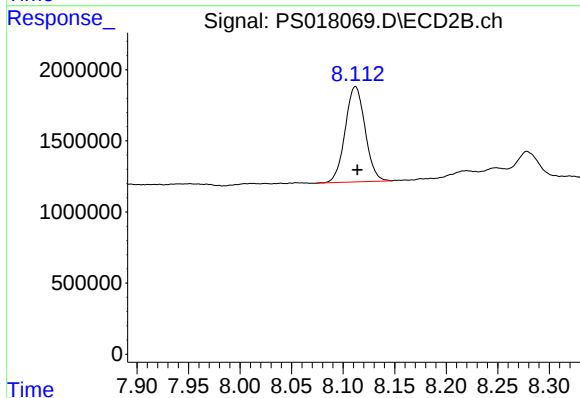


#10 Pentachlorophenol

R.T.: 8.112 min
Delta R.T.: -0.002 min
Response: 9006751
Conc: 1.07 ng/ml

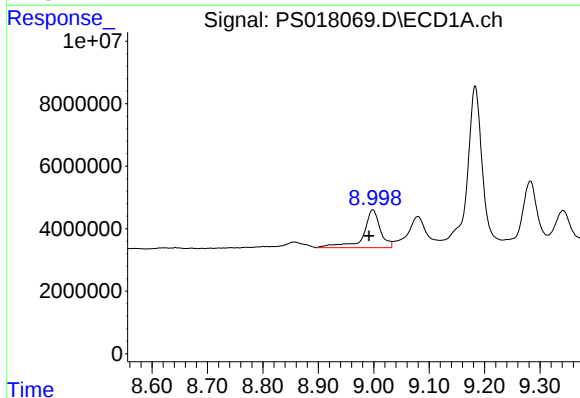


#11 2,4,5-TP (SILVEX)

R.T.: 8.998 min
Delta R.T.: 0.006 min
Response: 25904852
Conc: 3.06 ng/ml

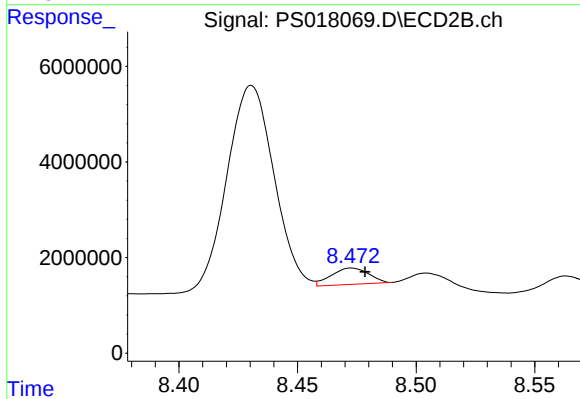

#11 2,4,5-TP (SILVEX)


R.T.: 8.473 min
Delta R.T.: -0.006 min
Response: 3742500
Conc: 1.05 ng/ml

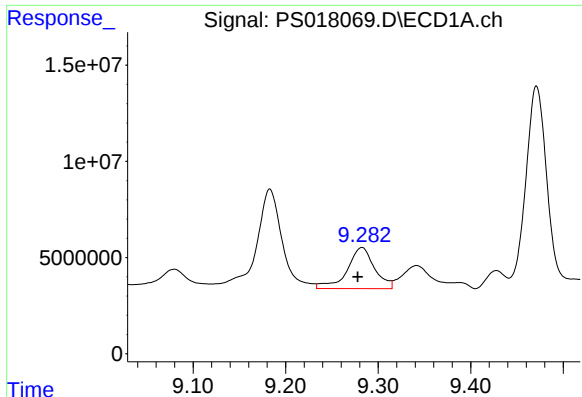

#12 2,4,5-T


R.T.: 9.283 min
Delta R.T.: 0.005 min
Response: 44024080
Conc: 4.97 ng/ml

Instrument :
ECD_S
ClientSampleId :

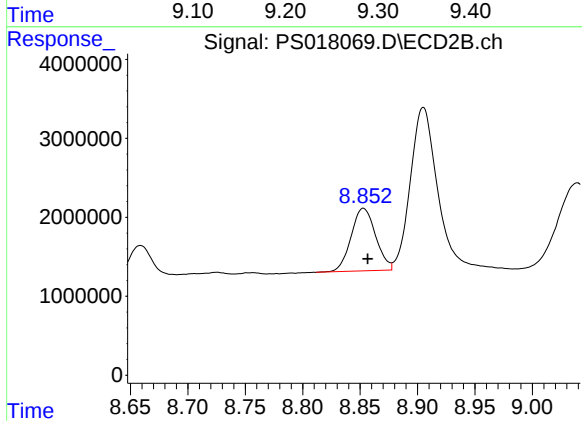


#12 2,4,5-T

R.T.: 8.853 min
Delta R.T.: -0.004 min
Response: 11782227
Conc: 3.60 ng/ml

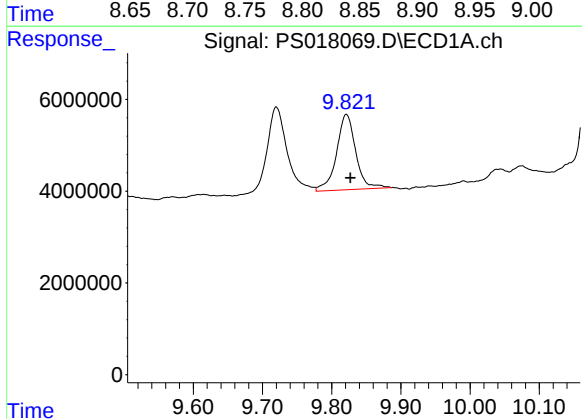


#13 2,4-DB

R.T.: 9.821 min
Delta R.T.: -0.006 min
Response: 31743744
Conc: 19.20 ng/ml

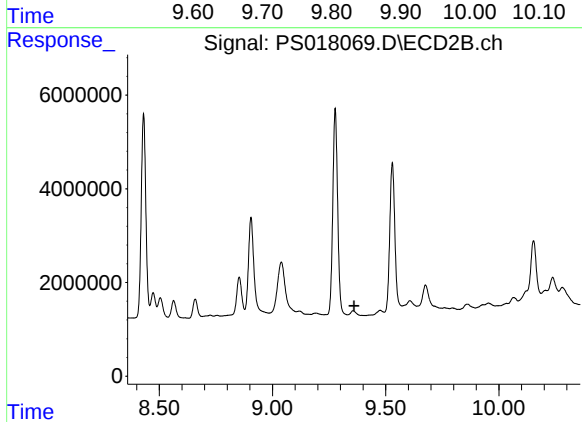

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.360 min
Response: 0
Conc: N.D.

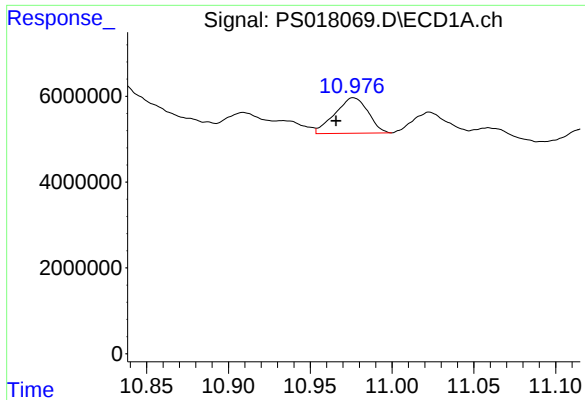

#14 DINOSEB


R.T.: 10.976 min
Delta R.T.: 0.011 min
Response: 11699737
Conc: 1.78 ng/ml

Instrument :
ECD_S
ClientSampleId :

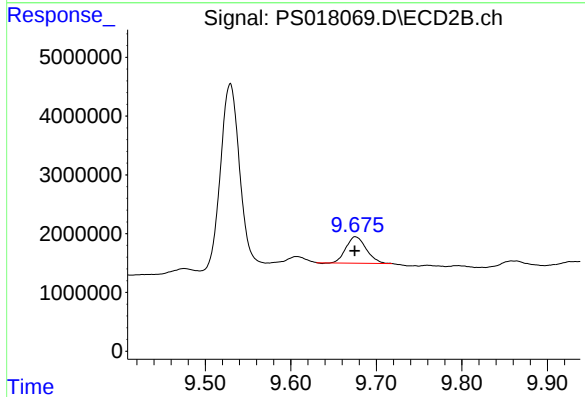


#14 DINOSEB

R.T.: 9.675 min
Delta R.T.: 0.000 min
Response: 7451937
Conc: 2.99 ng/ml

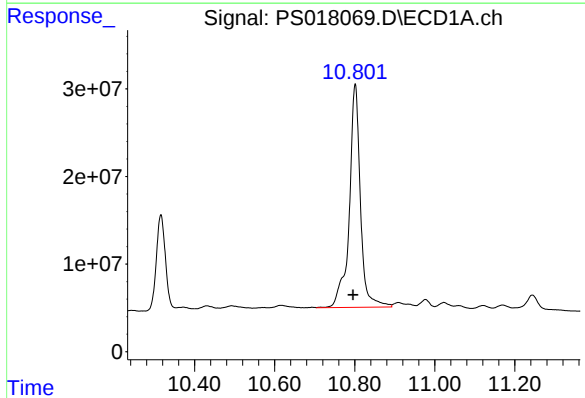


#15 Picloram

R.T.: 10.801 min
Delta R.T.: 0.005 min
Response: 493589583
Conc: 41.35 ng/ml

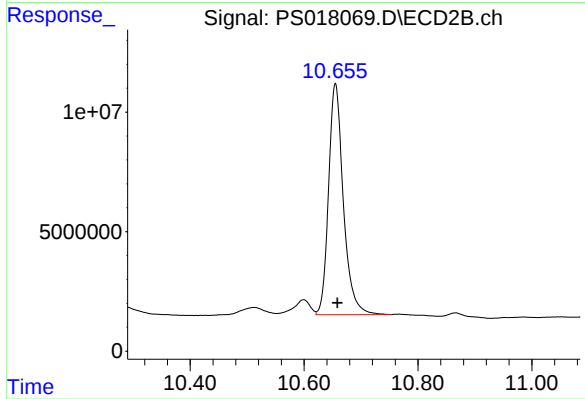

#15 Picloram


R.T.: 10.655 min
Delta R.T.: -0.004 min
Response: 174134496
Conc: 37.24 ng/ml

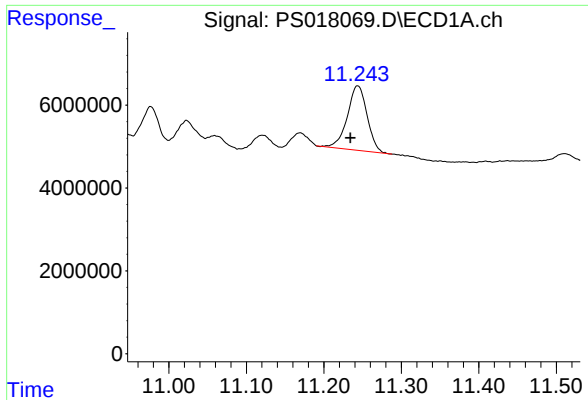

#16 DCPA

R.T.: 11.244 min
Delta R.T.: 0.009 min
Response: 27383002
Conc: 2.53 ng/ml

Instrument :
ECD_S
ClientSampleId :

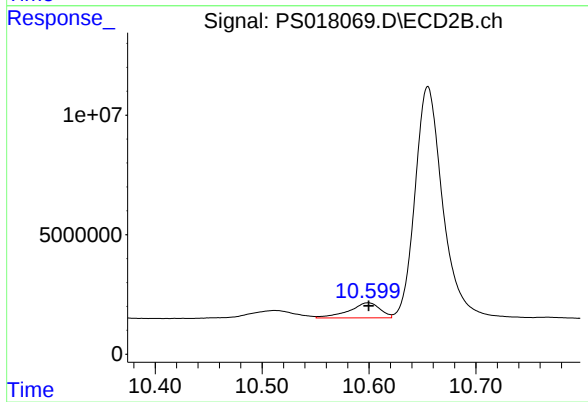

#16 DCPA

R.T.: 10.599 min
Delta R.T.: 0.000 min
Response: 12673835
Conc: 2.87 ng/ml