

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011923\
 Data File : PS021802.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jan 2023 08:54
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 19 20:37:48 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010923.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 10 10:34:52 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.379	6.811	1416.8E6	1098.5E6	508.984	611.401
Target Compounds							
1) T	Dalapon	2.507	0.000	437637	0	<MDL	N.D. #
3) T	4-Nitroph...	6.228	0.000	6781769	0	4.653	N.D. #
6) T	MCP	0.000	7.114	0	4594563	N.D.	<MDL
7) T	MCPA	6.766	7.218f	118523	32356570	<MDL	3.568 #
10) T	Pentachlo...	7.556	0.000	729268	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.090	0.000	754479	0	<MDL	N.D. #
12) T	2,4,5-T	8.350	0.000	12279740	0	<MDL	N.D. #
13) T	2,4-DB	8.834	0.000	375718	0	<MDL	N.D. #
14) T	DINOSEB	9.866	0.000	44268044	0	2.697	N.D. #
15) T	Picloram	9.755	10.925f	20970796	59666472	<MDL	3.369 #
16) T	DCPA	10.165	0.000	1183762	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS011923\
Data File : PS021802.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jan 2023 08:54
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 19 20:37:48 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010923.M
Quant Title : 8080.M
QLast Update : Tue Jan 10 10:34:52 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

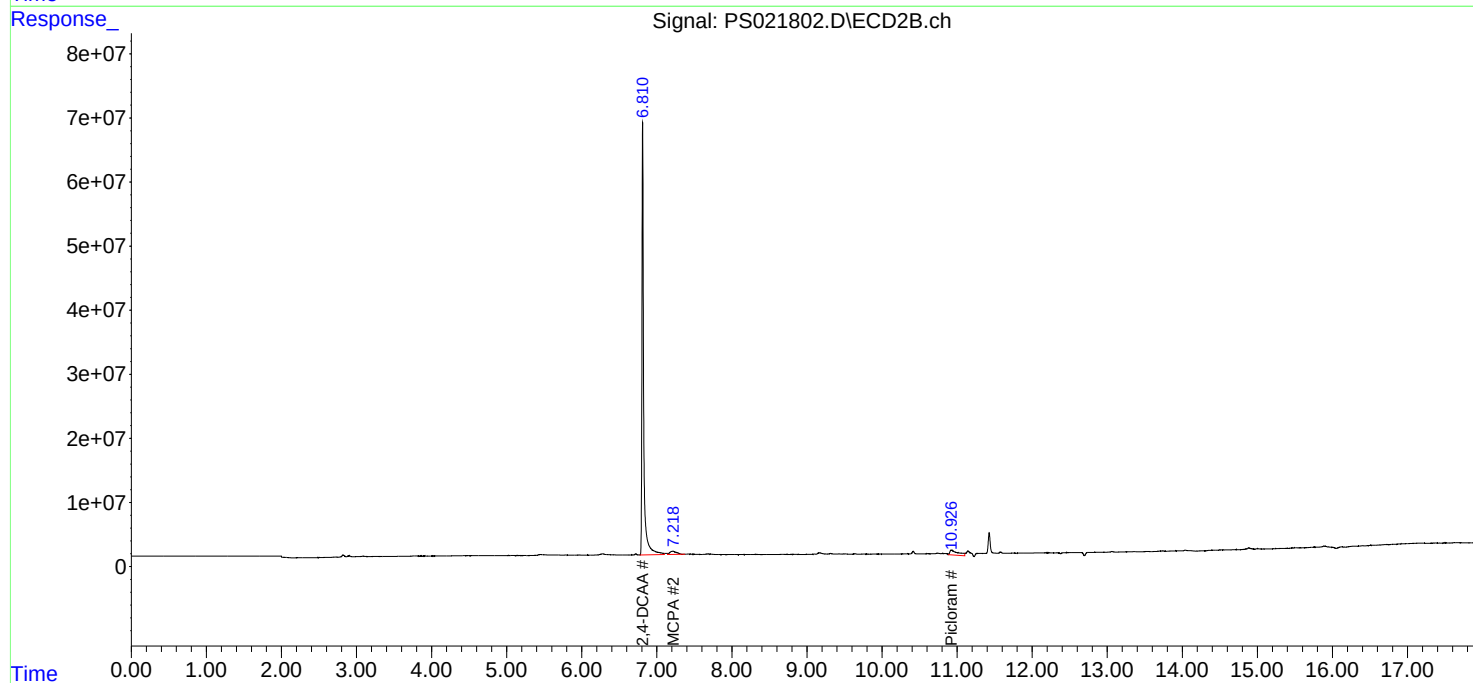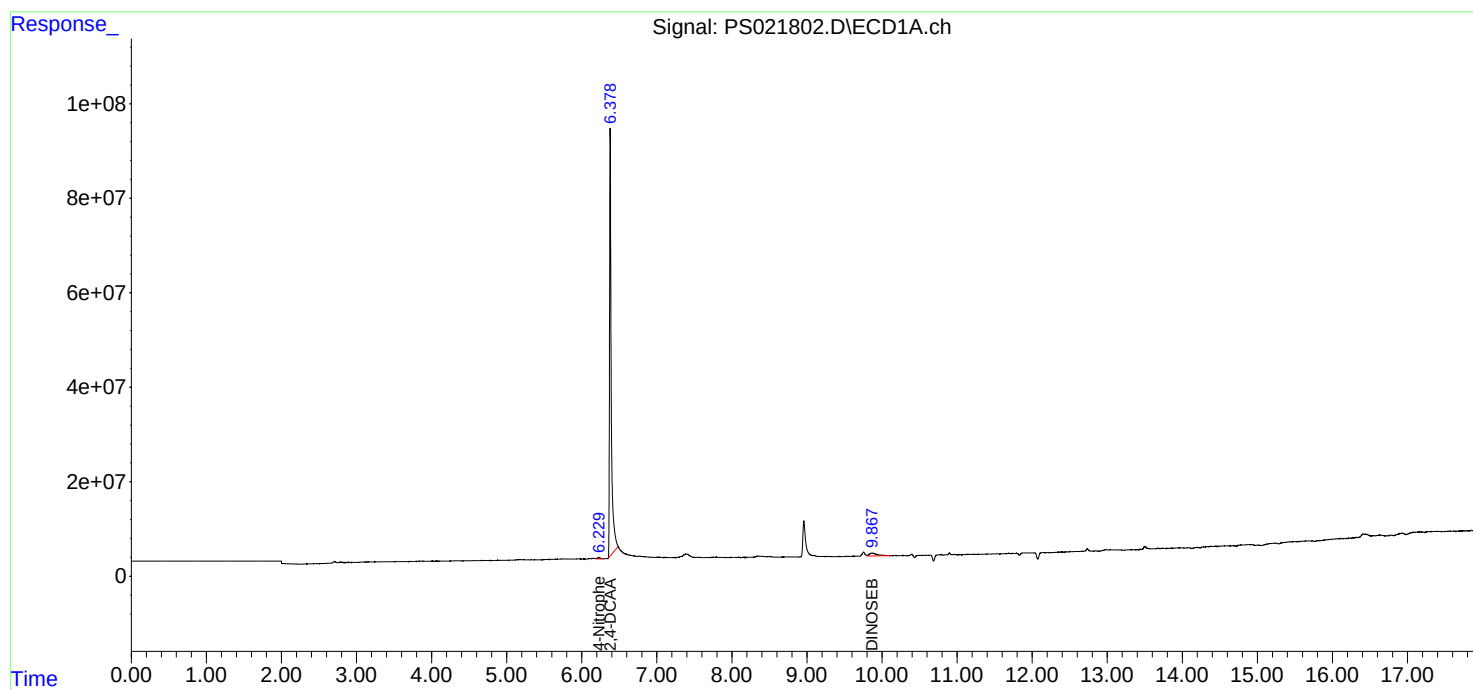


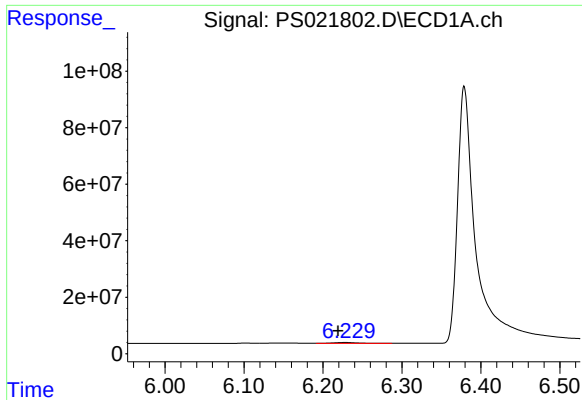

#3 4-Nitrophenol


R.T.: 6.228 min
Delta R.T.: 0.009 min
Response: 6781769
Conc: 4.65 ng/ml

Instrument :
ECD_S
ClientSampleId :

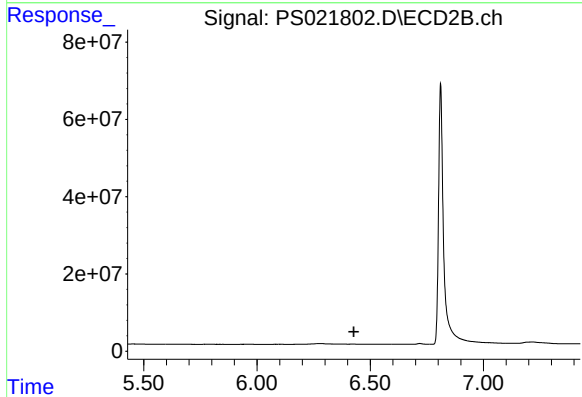


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.428 min
Response: 0
Conc: N.D.

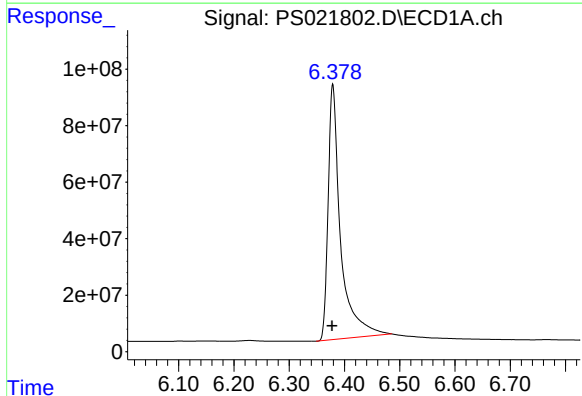


#4 2,4-DCAA

R.T.: 6.379 min
Delta R.T.: 0.002 min
Response: 1416790510
Conc: 508.98 ng/ml

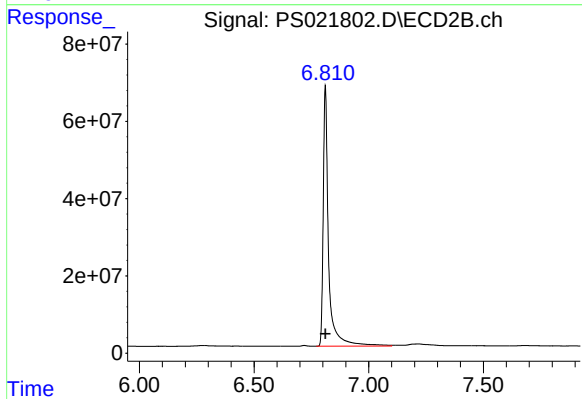

#4 2,4-DCAA


R.T.: 6.811 min
Delta R.T.: 0.000 min
Response: 1098497443
Conc: 611.40 ng/ml

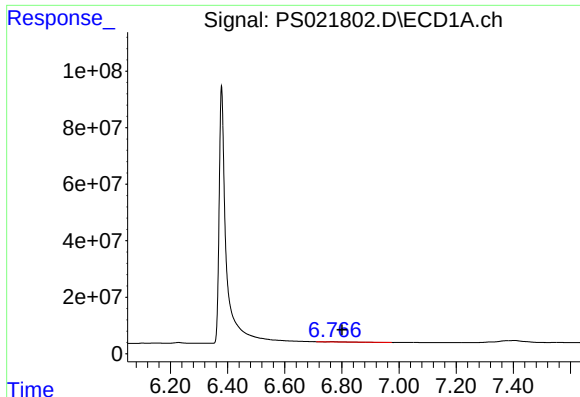

#7 MCPA


R.T.: 6.766 min
Delta R.T.: -0.036 min
Response: 118523
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

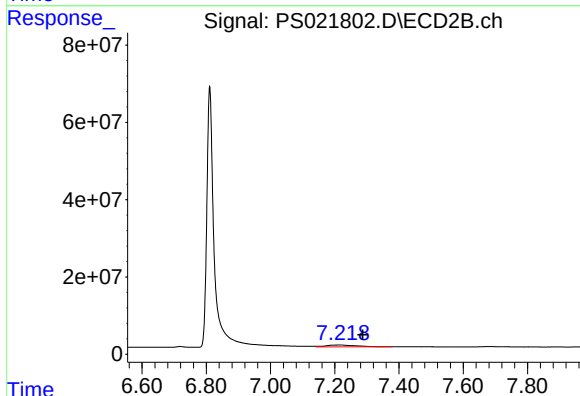


#7 MCPA

R.T.: 7.218 min
Delta R.T.: -0.069 min
Response: 32356570
Conc: 3.57 ug/ml

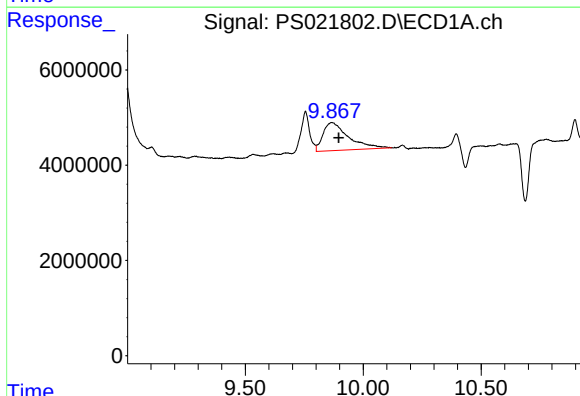


#14 DINOSEB

R.T.: 9.866 min
Delta R.T.: -0.030 min
Response: 44268044
Conc: 2.70 ng/ml

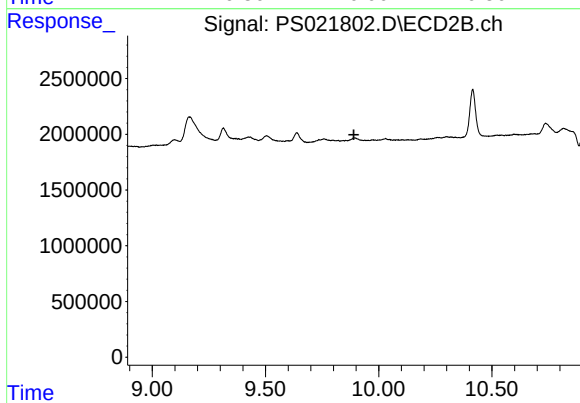

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 9.890 min
Response: 0
Conc: N.D.

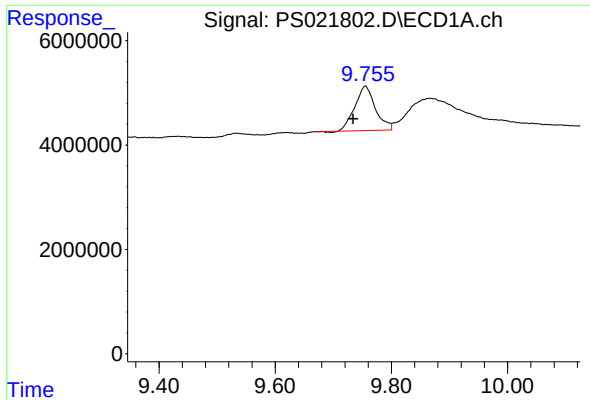

#15 Picloram

R.T.: 9.755 min
Delta R.T.: 0.021 min
Response: 20970796
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

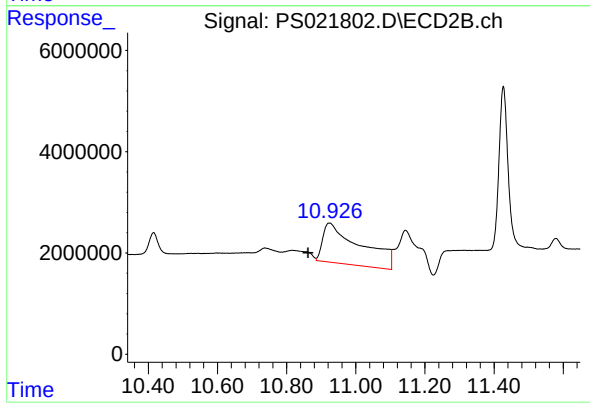

#15 Picloram

R.T.: 10.925 min
Delta R.T.: 0.063 min
Response: 59666472
Conc: 3.37 ng/ml