

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012020\
 Data File : PS008464.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jan 2020 09:18
 Operator : DD\AJ
 Sample : BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 20 10:13:05 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 08 11:00:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.278	5.971	871.8E6	478.6E6	493.767	505.176
Target Compounds							
5) T	DICAMBA	6.470	6.141	16930379	10450321	2.463	2.613
10) T	Pentachlo...	7.702	7.494	52201326	31118792	2.147	2.304
11) T	2,4,5-TP ...	8.250	7.853	23139944	14163782	2.478	2.710
12) T	2,4,5-T	8.533	8.232	31650466	20072164	3.430	3.796
14) T	DINOSEB	0.000	9.076	0	11166569	N.D.	2.956
15) T	Picloram	10.064	10.057	329.8E6	217.8E6	26.421	29.311
16) T	DCPA	10.516	10.007	31807734	19490658	2.680	2.991



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012020\
Data File : PS008464.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jan 2020 09:18
Operator : DD\AJ
Sample : BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 20 10:13:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
Quant Title : 8080.M
QLast Update : Wed Jan 08 11:00:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

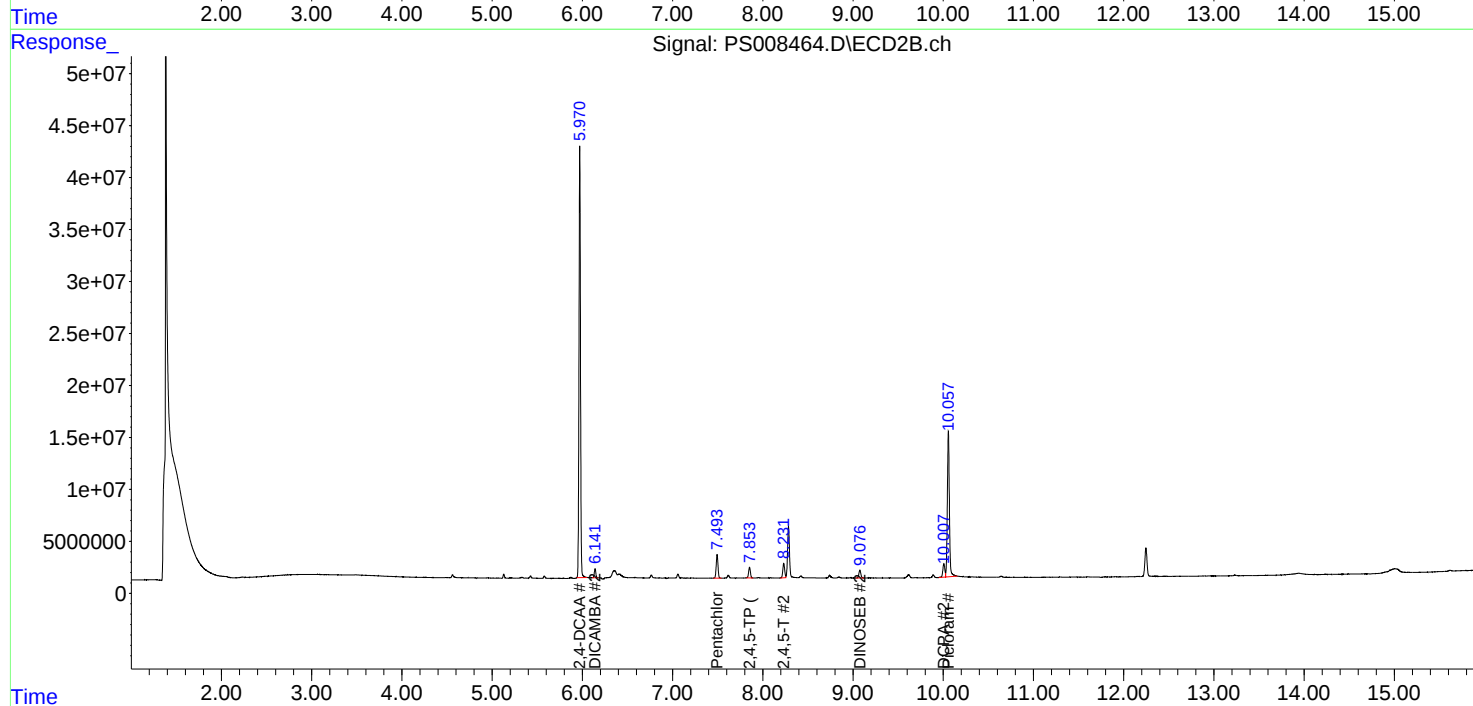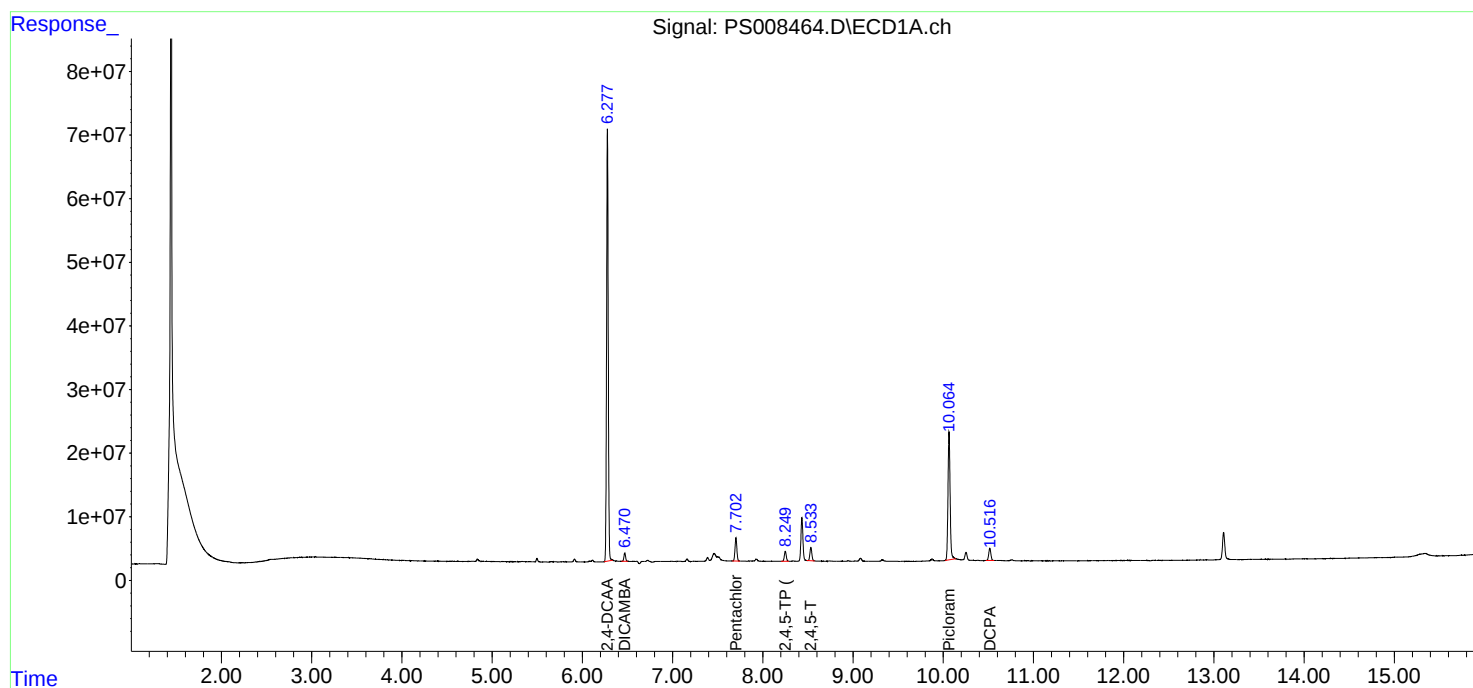


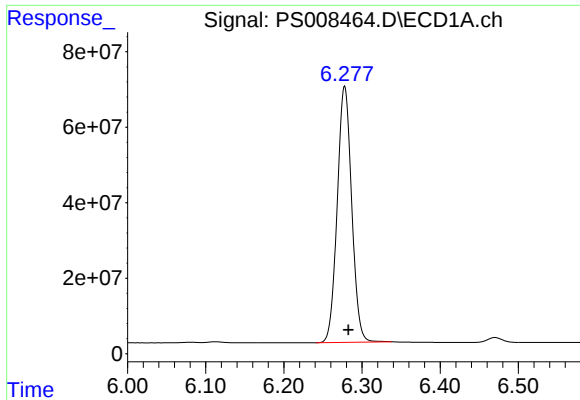

#4 2,4-DCAA


R.T.: 6.278 min
Delta R.T.: -0.005 min
Response: 871846020
Conc: 493.77 ng/ml

Instrument :
ECD_S
ClientSampleId :

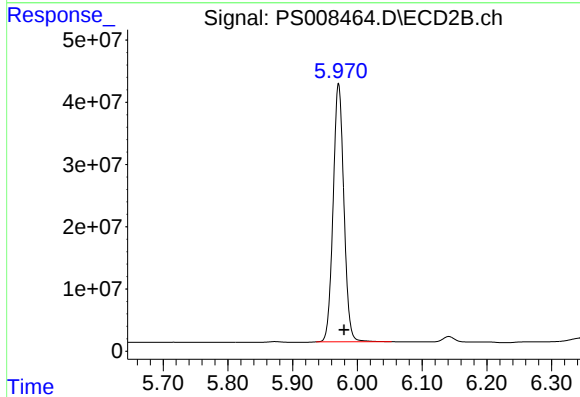


#4 2,4-DCAA

R.T.: 5.971 min
Delta R.T.: -0.008 min
Response: 478635348
Conc: 505.18 ng/ml

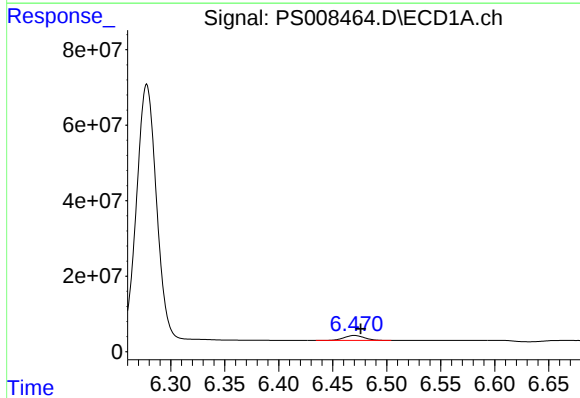


#5 DICAMBA

R.T.: 6.470 min
Delta R.T.: -0.006 min
Response: 16930379
Conc: 2.46 ng/ml

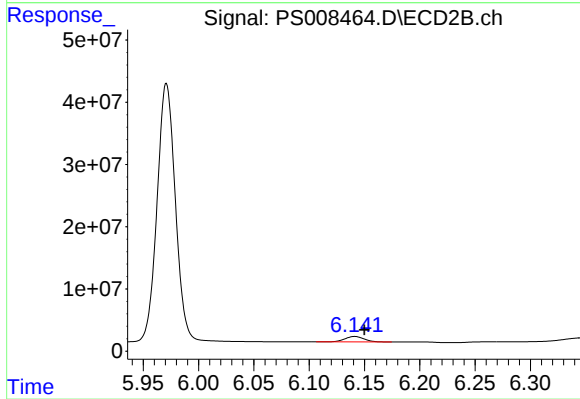

#5 DICAMBA


R.T.: 6.141 min
Delta R.T.: -0.009 min
Response: 10450321
Conc: 2.61 ng/ml

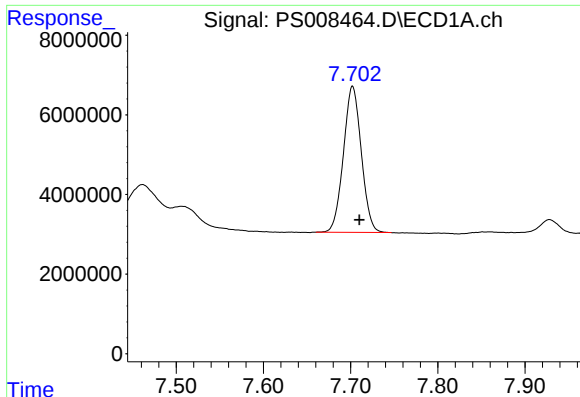

#10 Pentachlorophenol


R.T.: 7.702 min
Delta R.T.: -0.008 min
Response: 52201326
Conc: 2.15 ng/ml

Instrument :
ECD_S
ClientSampleId :

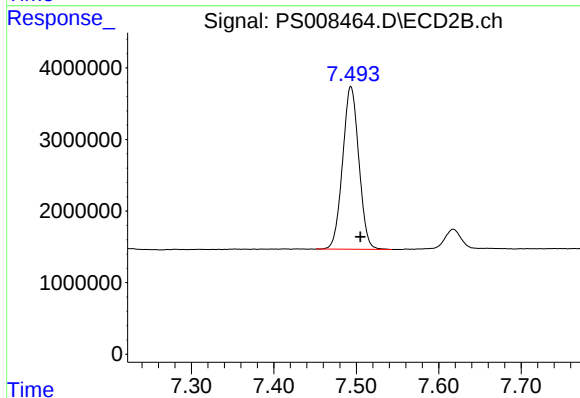


#10 Pentachlorophenol

R.T.: 7.494 min
Delta R.T.: -0.011 min
Response: 31118792
Conc: 2.30 ng/ml

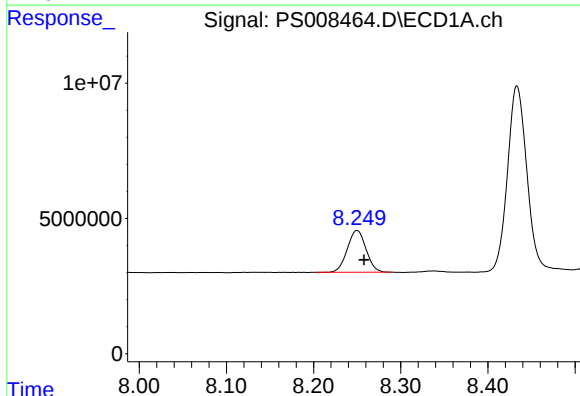


#11 2,4,5-TP (SILVEX)

R.T.: 8.250 min
Delta R.T.: -0.008 min
Response: 23139944
Conc: 2.48 ng/ml

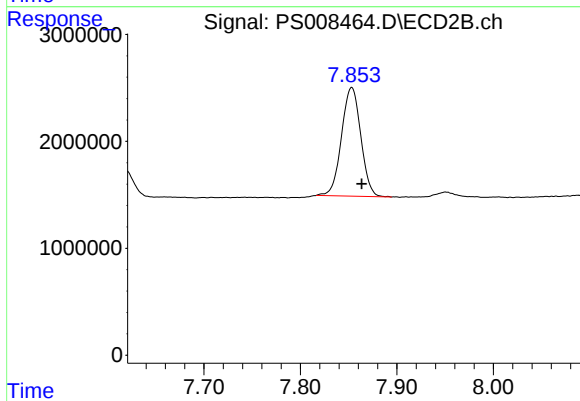

#11 2,4,5-TP (SILVEX)


R.T.: 7.853 min
Delta R.T.: -0.011 min
Response: 14163782
Conc: 2.71 ng/ml

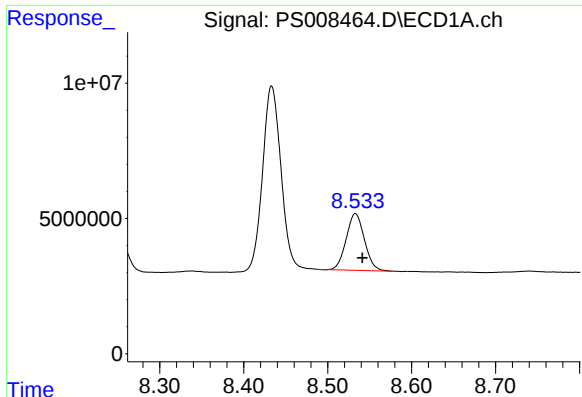

#12 2,4,5-T


R.T.: 8.533 min
Delta R.T.: -0.008 min
Response: 31650466
Conc: 3.43 ng/ml

Instrument :
ECD_S
ClientSampleId :

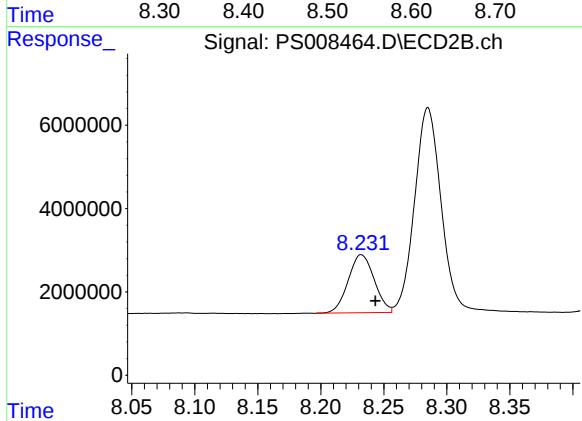


#12 2,4,5-T

R.T.: 8.232 min
Delta R.T.: -0.011 min
Response: 20072164
Conc: 3.80 ng/ml

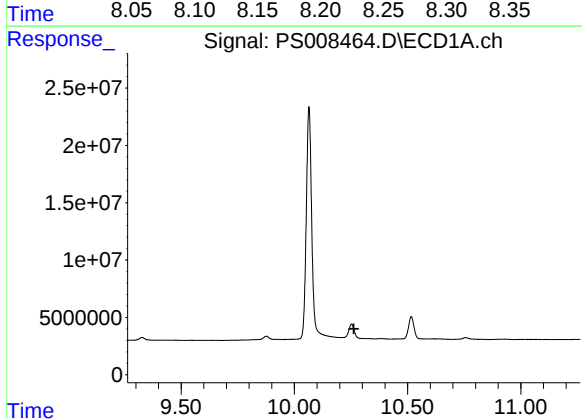


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 10.263 min
Response: 0
Conc: N.D.

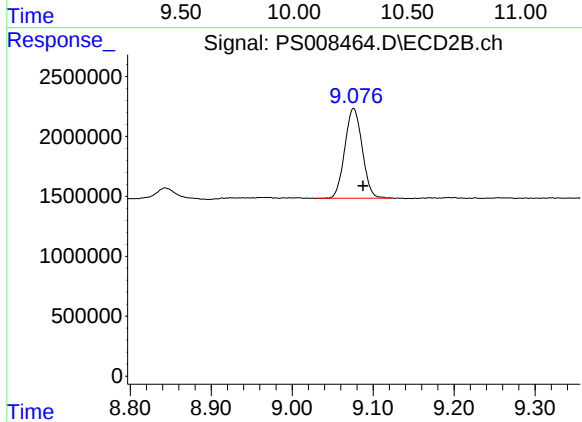

#14 DINOSEB


R.T.: 9.076 min
Delta R.T.: -0.012 min
Response: 11166569
Conc: 2.96 ng/ml

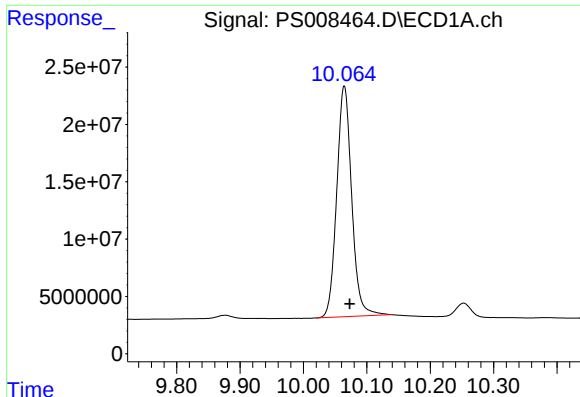

#15 Picloram


R.T.: 10.064 min
Delta R.T.: -0.009 min
Response: 329783601
Conc: 26.42 ng/ml

Instrument :
ECD_S
ClientSampleId :

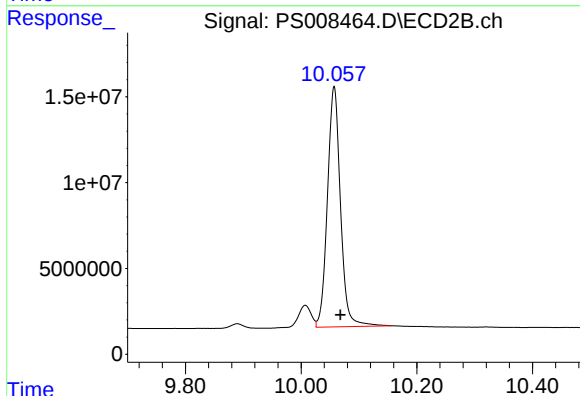


#15 Picloram

R.T.: 10.057 min
Delta R.T.: -0.011 min
Response: 217761469
Conc: 29.31 ng/ml

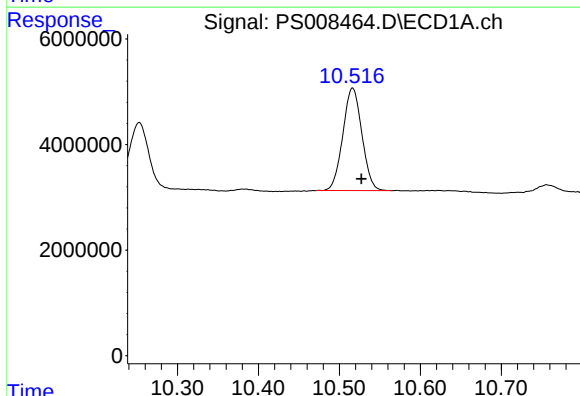

#16 DCPA

R.T.: 10.516 min
Delta R.T.: -0.011 min
Response: 31807734
Conc: 2.68 ng/ml

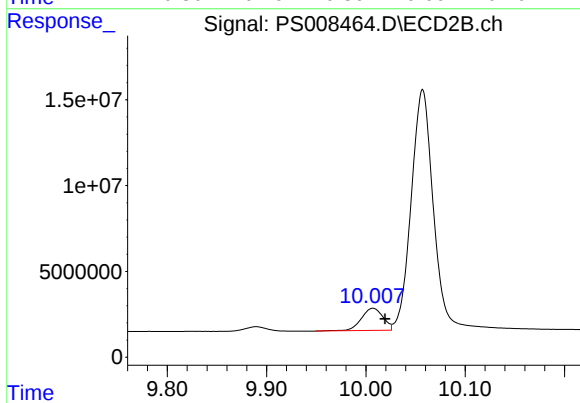

#16 DCPA

R.T.: 10.007 min
Delta R.T.: -0.012 min
Response: 19490658
Conc: 2.99 ng/ml