

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012020\
 Data File : PS008468.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jan 2020 10:46
 Operator : DD\AJ
 Sample : PB126179BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 20 11:16:13 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 08 11:00:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.273	5.967	879.8E6	479.8E6	498.258	506.414
Target Compounds							
9) T	2,4-D	7.456	0.000	16762182	0	9.215	N.D. #
10) T	Pentachlo...	0.000	7.489	0	9393298	N.D.	<MDL
12) T	2,4,5-T	0.000	8.281	0	13518484	N.D.	2.556
15) T	Picloram	10.059	10.052	35529104	24313948	2.846	3.273
16) T	DCPA	0.000	10.052	0	24313948	N.D.	3.731



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012020\
Data File : PS008468.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jan 2020 10:46
Operator : DD\AJ
Sample : PB126179BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 20 11:16:13 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
Quant Title : 8080.M
QLast Update : Wed Jan 08 11:00:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

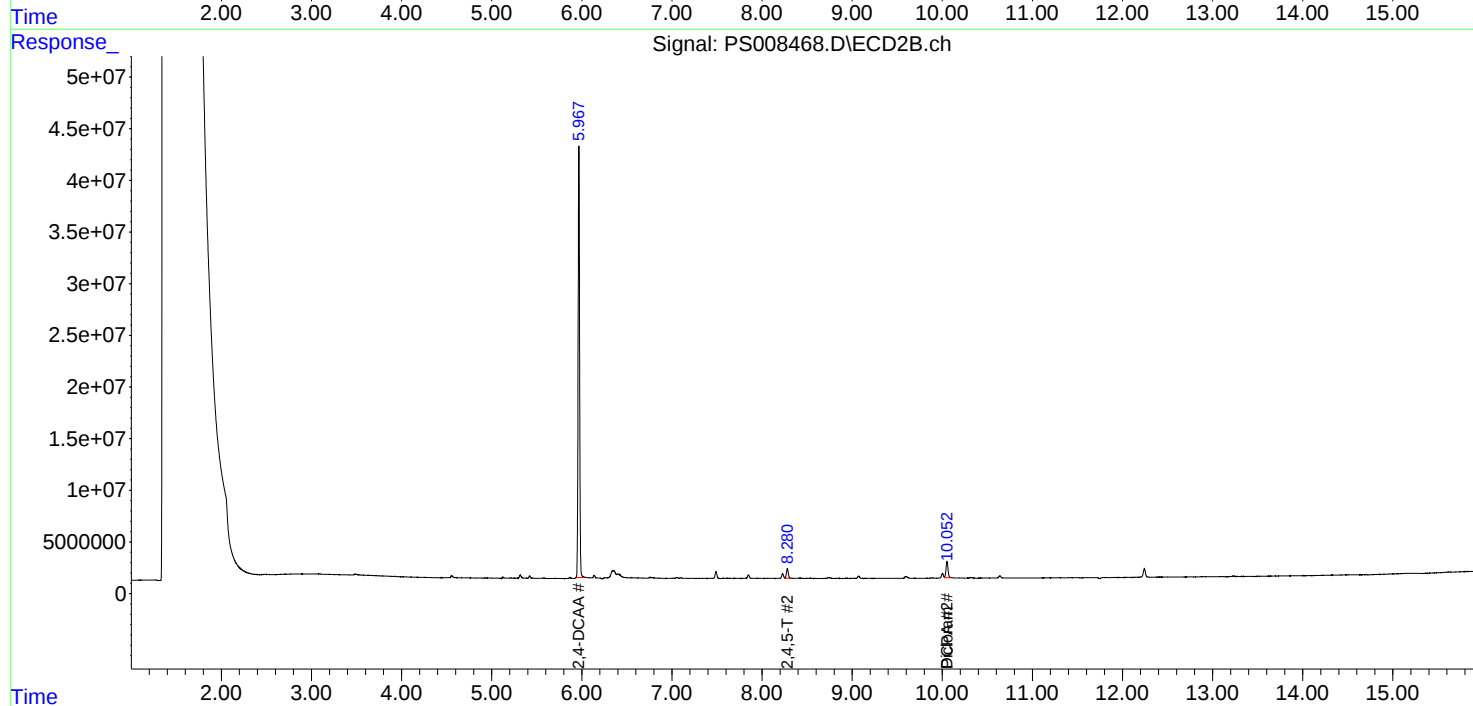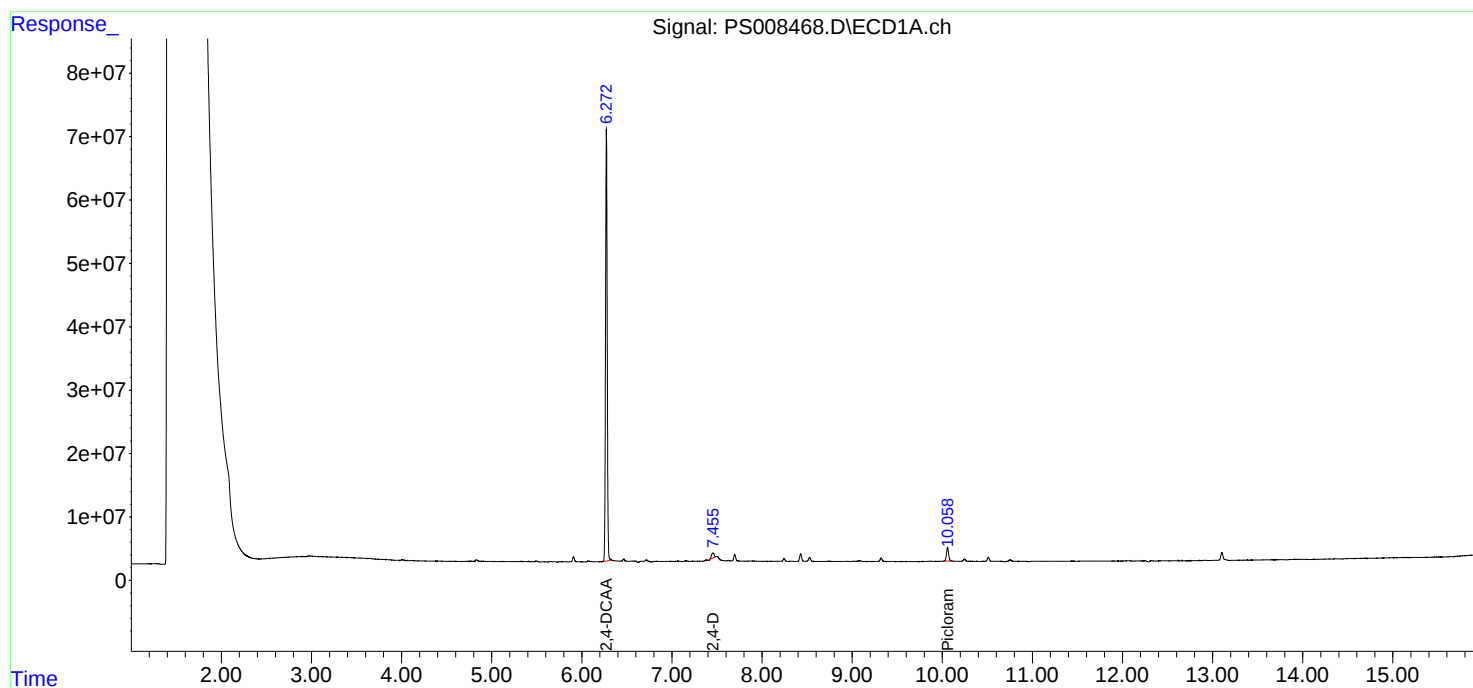


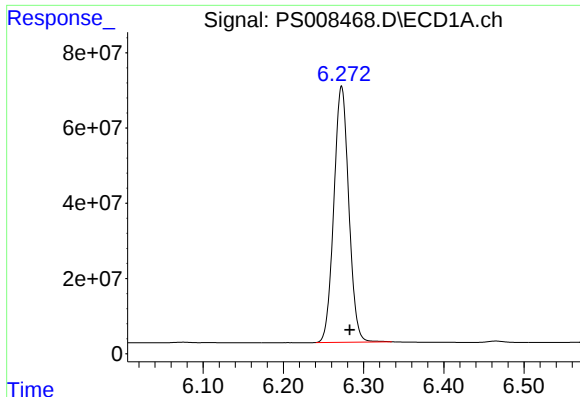

#4 2,4-DCAA


R.T.: 6.273 min
Delta R.T.: -0.010 min
Response: 879775891
Conc: 498.26 ng/ml

Instrument :
ECD_S
ClientSampleId :

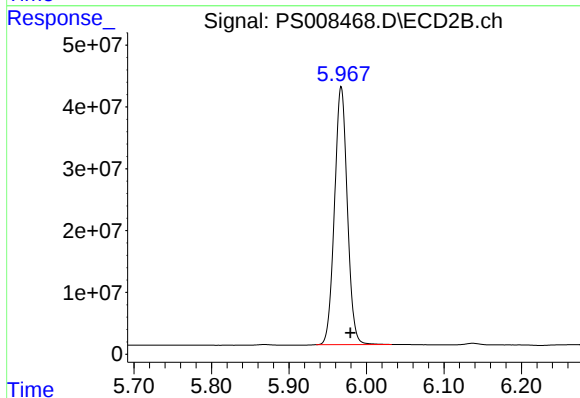


#4 2,4-DCAA

R.T.: 5.967 min
Delta R.T.: -0.012 min
Response: 479808548
Conc: 506.41 ng/ml

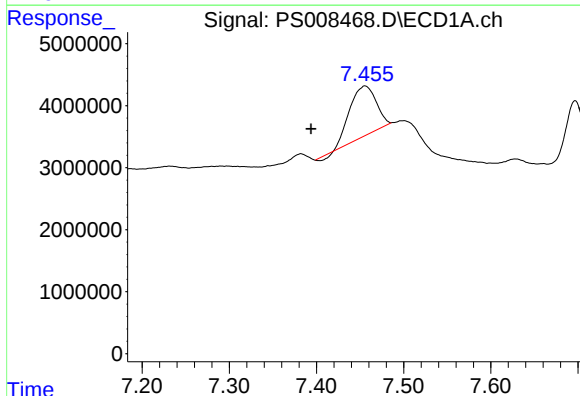


#9 2,4-D

R.T.: 7.456 min
Delta R.T.: 0.062 min
Response: 16762182
Conc: 9.21 ng/ml

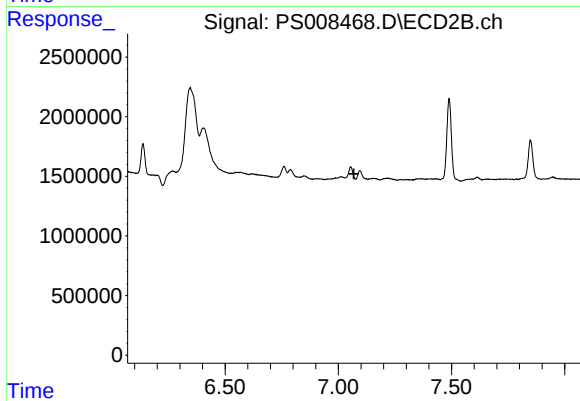

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.069 min
Response: 0
Conc: N.D.

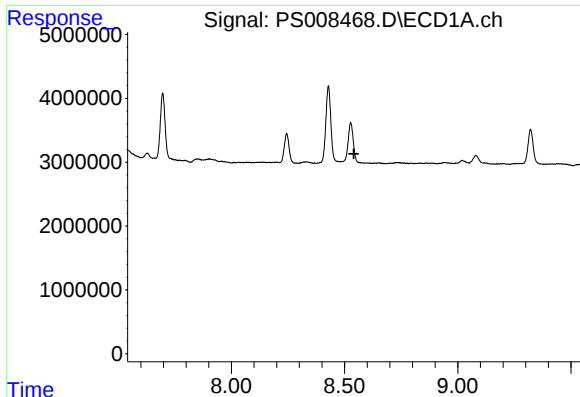

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 8.541 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

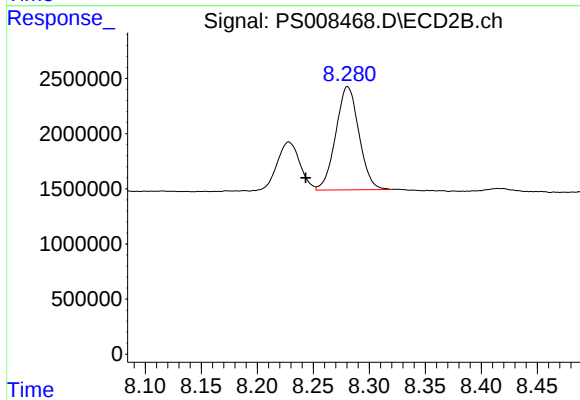


#12 2,4,5-T

R.T.: 8.281 min
Delta R.T.: 0.037 min
Response: 13518484
Conc: 2.56 ng/ml

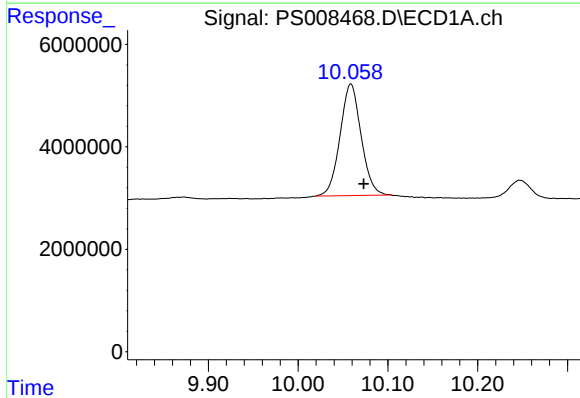


#15 Picloram

R.T.: 10.059 min
Delta R.T.: -0.014 min
Response: 35529104
Conc: 2.85 ng/ml

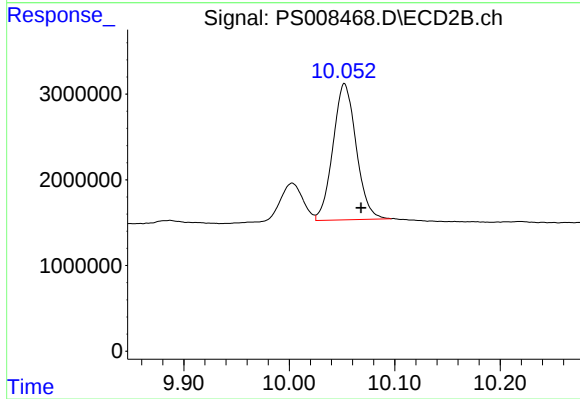

#15 Picloram


R.T.: 10.052 min
Delta R.T.: -0.015 min
Response: 24313948
Conc: 3.27 ng/ml

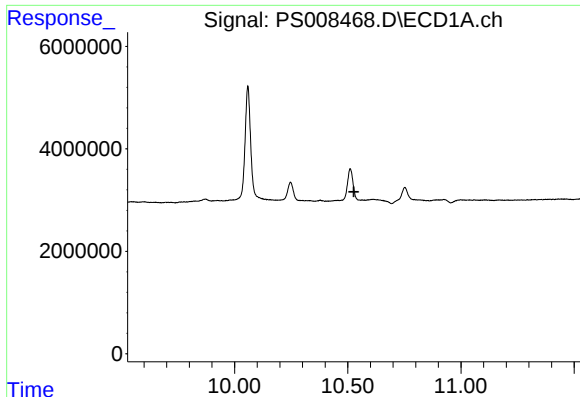

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.527 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

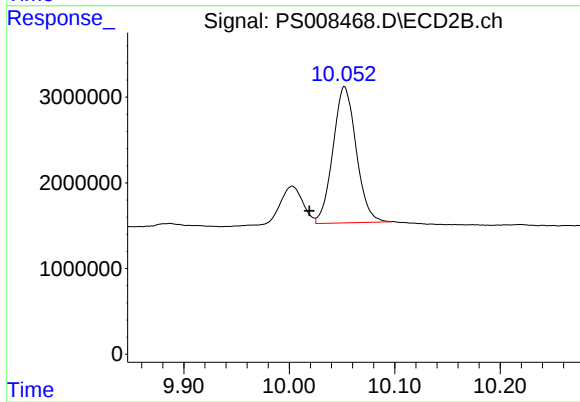

#16 DCPA

R.T.: 10.052 min
Delta R.T.: 0.033 min
Response: 24313948
Conc: 3.73 ng/ml