

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012120\
 Data File : PS008477.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jan 2020 01:18
 Operator : DD\AJ
 Sample : PB126207BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB126207BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 04:19:26 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 08 11:00:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.276	5.969	868.2E6	484.1E6	491.726	510.894
Target Compounds							
9) T	2,4-D	7.460	0.000	18507366	0	10.174	N.D. #
10) T	Pentachlo...	0.000	7.491	0	8452117	N.D.	<MDL
15) T	Picloram	0.000	10.055	0	10510841	N.D.	1.415
16) T	DCPA	0.000	10.055	0	10510841	N.D.	1.613



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012120\
Data File : PS008477.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jan 2020 01:18
Operator : DD\AJ
Sample : PB126207BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB126207BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 04:19:26 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
Quant Title : 8080.M
QLast Update : Wed Jan 08 11:00:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

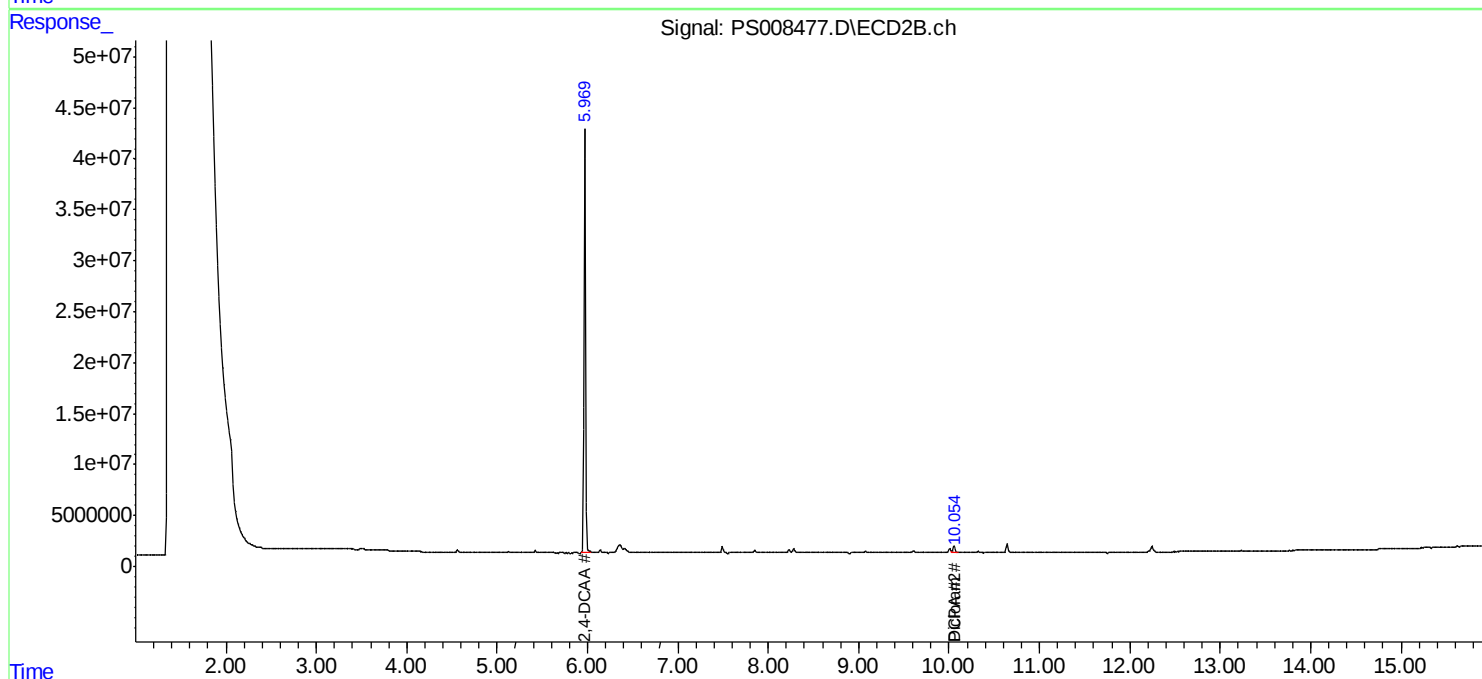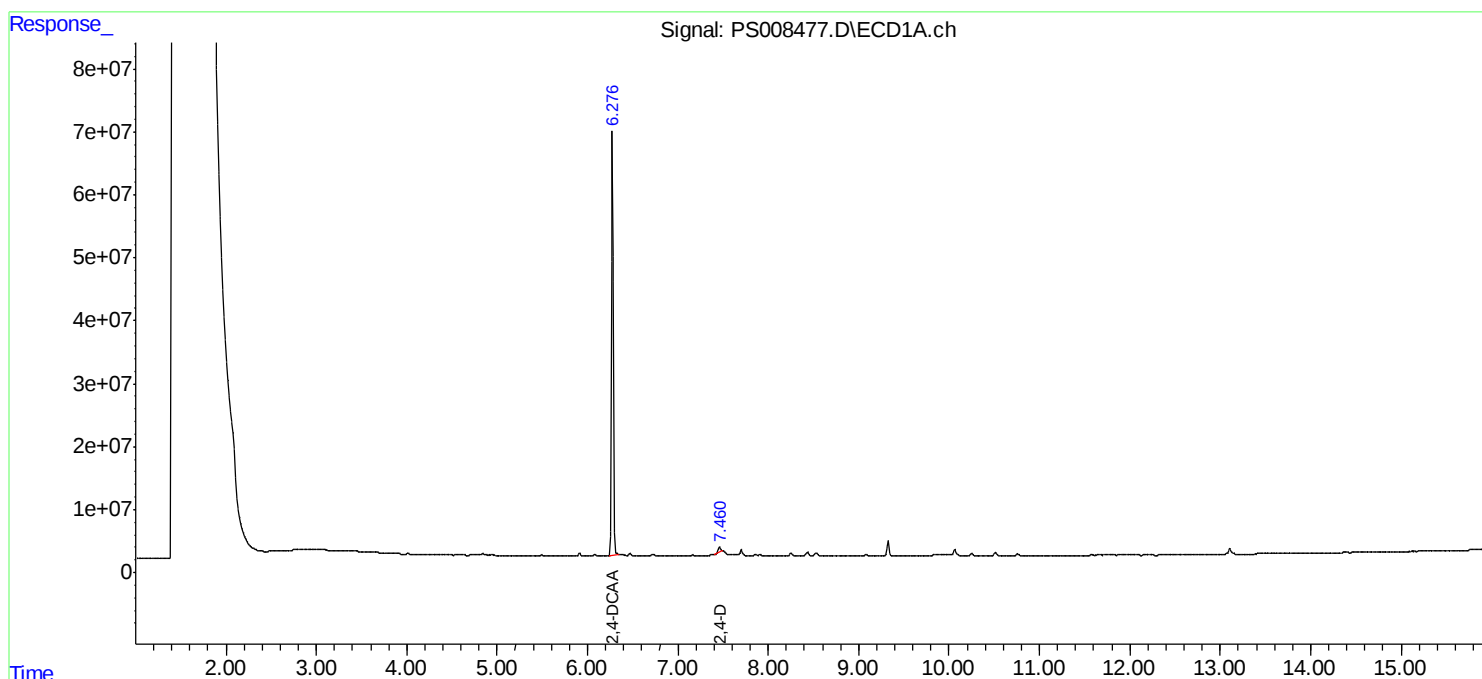


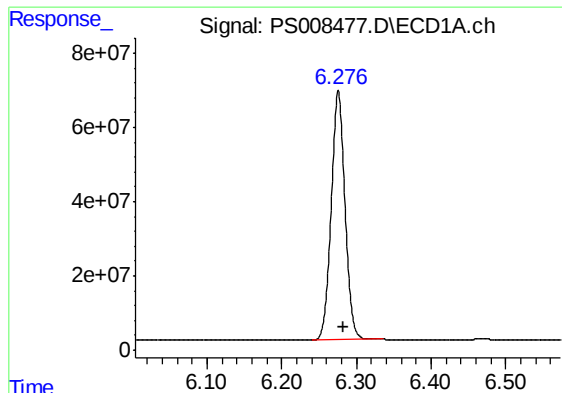

#4 2,4-DCAA


R.T.: 6.276 min
Delta R.T.: -0.007 min
Response: 868241978
Conc: 491.73 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB126207BL

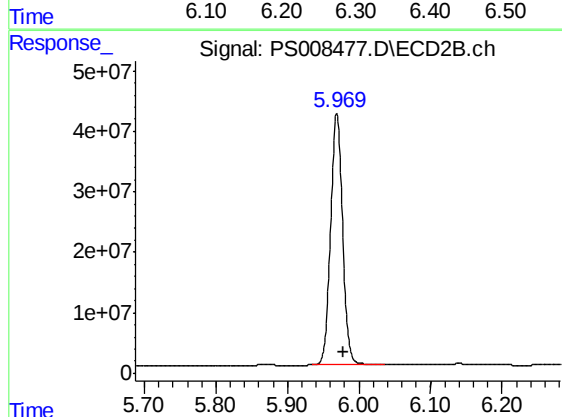


#4 2,4-DCAA

R.T.: 5.969 min
Delta R.T.: -0.010 min
Response: 484053140
Conc: 510.89 ng/ml

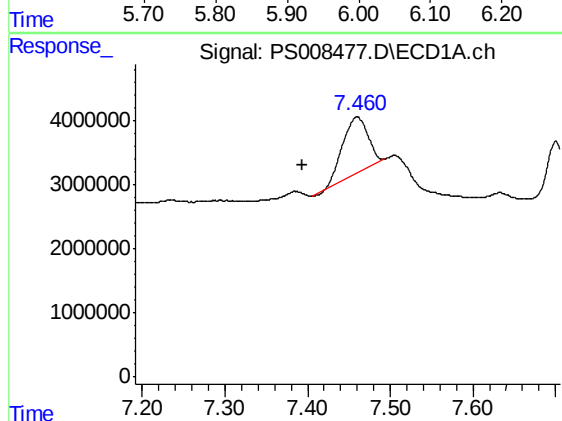


#9 2,4-D

R.T.: 7.460 min
Delta R.T.: 0.066 min
Response: 18507366
Conc: 10.17 ng/ml

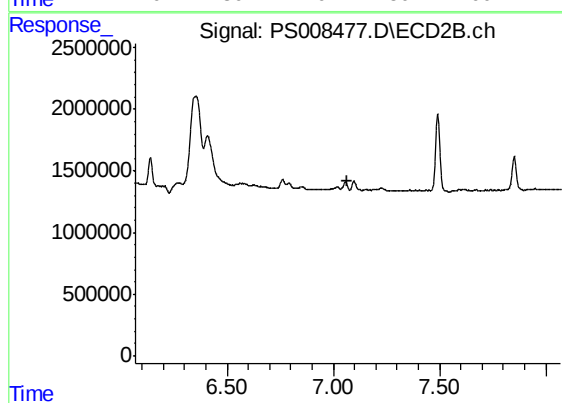

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.069 min
Response: 0
Conc: N.D.

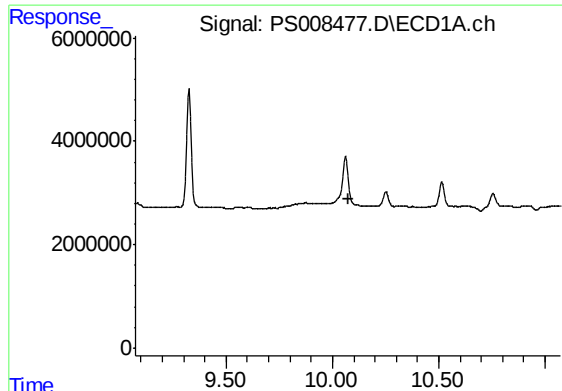

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 10.073 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB126207BL

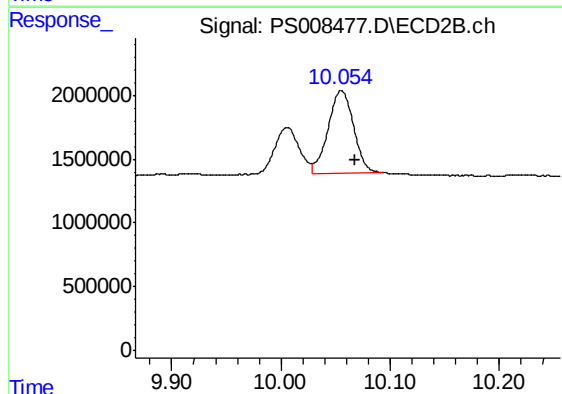


#15 Picloram

R.T.: 10.055 min
Delta R.T.: -0.013 min
Response: 10510841
Conc: 1.41 ng/ml

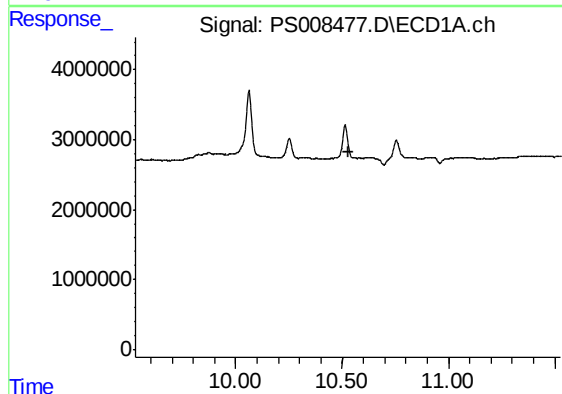

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.527 min
Response: 0
Conc: N.D.

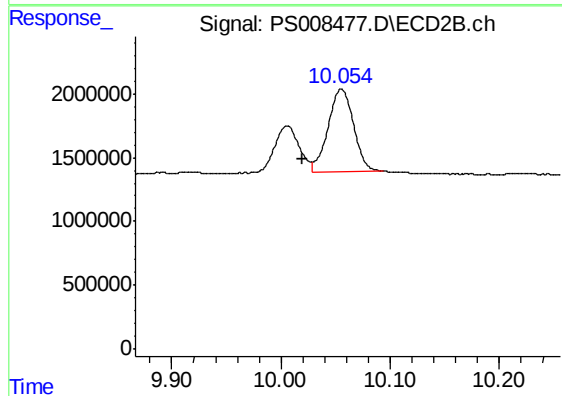

#16 DCPA

R.T.: 10.055 min
Delta R.T.: 0.036 min
Response: 10510841
Conc: 1.61 ng/ml