

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012121\
 Data File : PS013829.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jan 2021 15:58
 Operator : DD\AJ
 Sample : PB134253BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 18:02:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010421.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 05 01:51:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.210	6.912	534.0E6	232.4E6	558.776	577.864
Target Compounds							
1) T	Dalapon	2.986f	2.588	65609821	142.7E6	60.324	274.489 #
2) T	3,5-DICHL...	0.000	6.094	0	44506767	N.D.	70.645
3) T	4-Nitroph...	6.982f	0.000	9529349	0	20.043	N.D. #
5) T	DICAMBA	0.000	7.045	0	4670539	N.D.	2.720
6) T	MCP	7.559	0.000	10977337	0	3.832	N.D. #
7) T	MCPA	7.694	7.368	10712752	29269147	2.606	14.478 #
10) T	Pentachlo...	8.680f	0.000	18467632	0	1.304	N.D. #
11) T	2,4,5-TP ...	0.000	8.761	0	20772542	N.D.	8.696
12) T	2,4,5-T	9.396f	0.000	21402214	0	3.785	N.D. #
14) T	DINOSEB	11.151	0.000	41771327	0	9.468	N.D. #
15) T	Picloram	0.000	10.929f	0	4341357	N.D.	1.249
16) T	DCPA	11.442	10.929	-3634897	4341357	N.D.	1.403



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012121\
Data File : PS013829.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jan 2021 15:58
Operator : DD\AJ
Sample : PB134253BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 18:02:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010421.M
Quant Title : 8080.M
QLast Update : Tue Jan 05 01:51:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

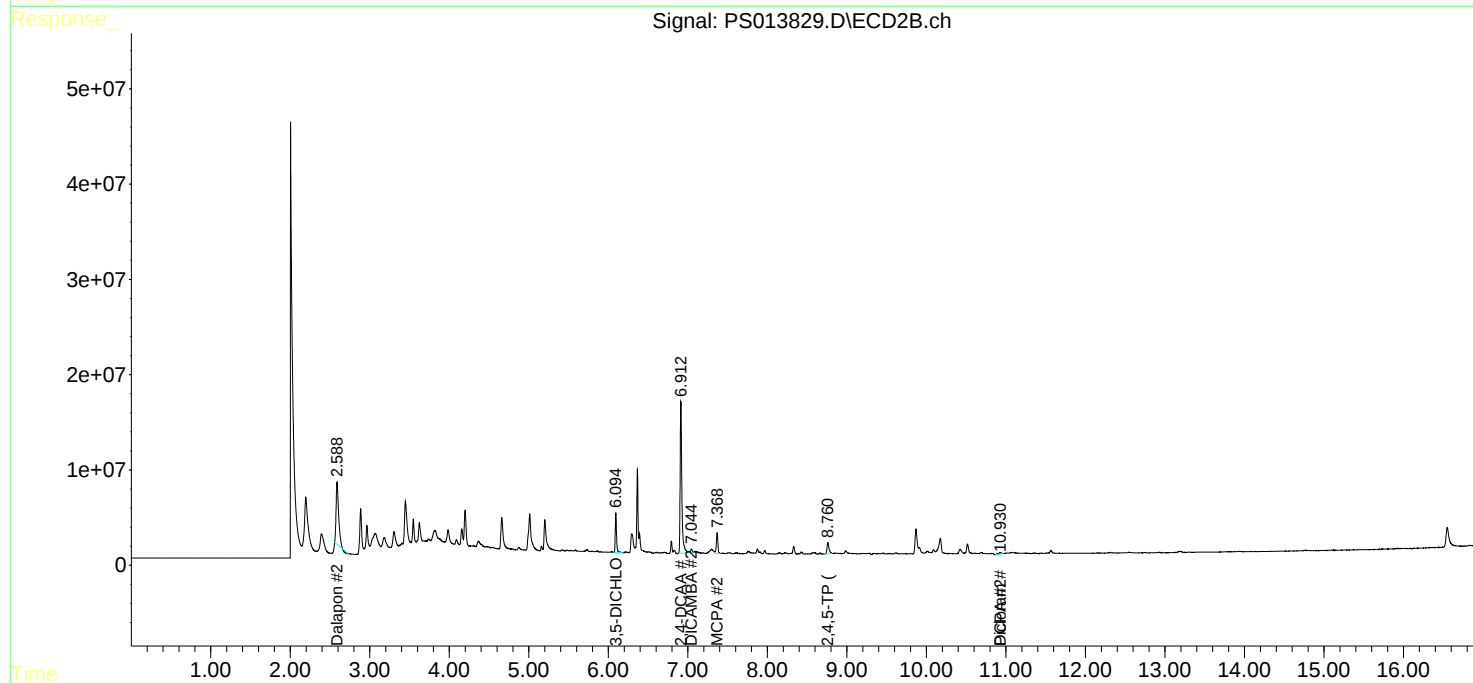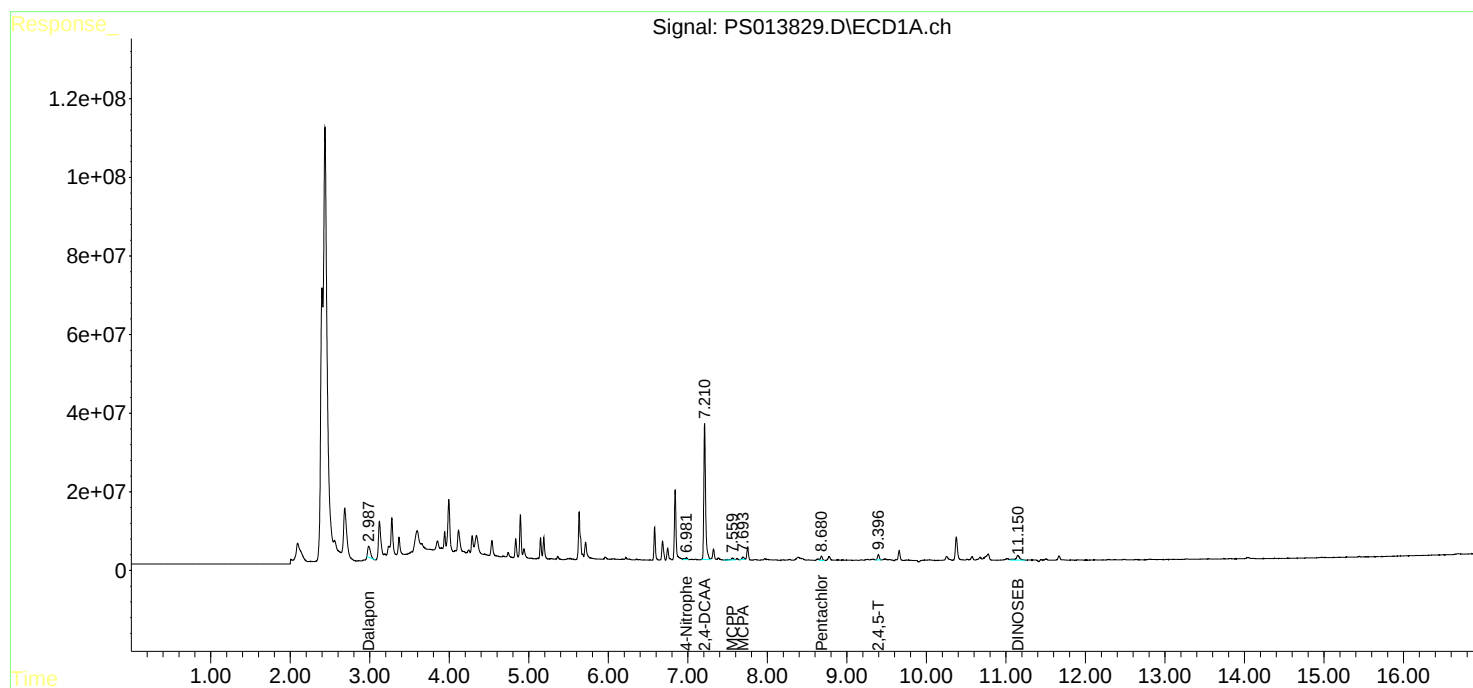


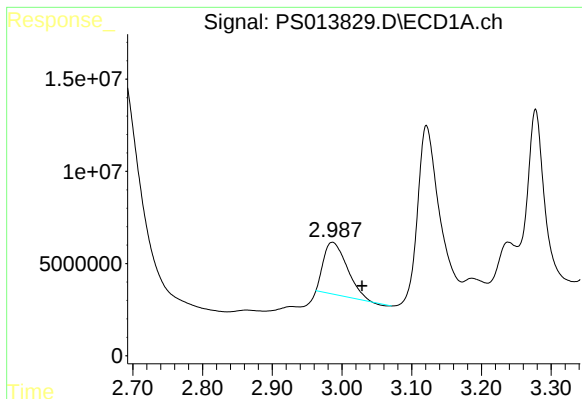

#1 Dalapon


R.T.: 2.986 min
Delta R.T.: -0.043 min
Response: 65609821
Conc: 60.32 ng/ml

Instrument :
ECD_S
ClientSampleId :

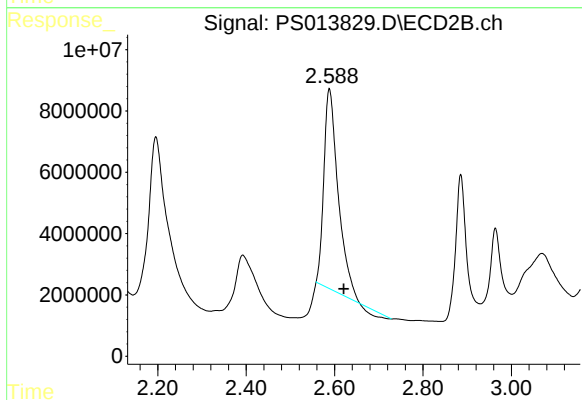


#1 Dalapon

R.T.: 2.588 min
Delta R.T.: -0.033 min
Response: 142720498
Conc: 274.49 ng/ml

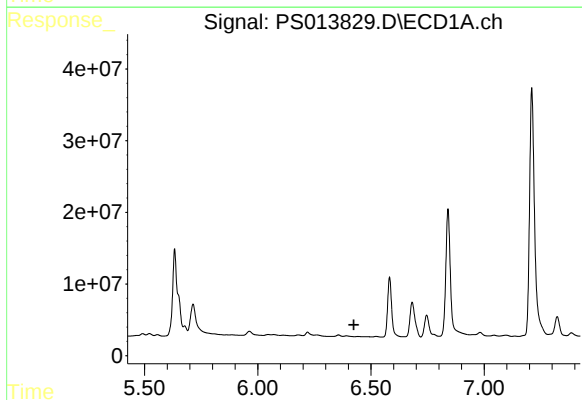


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.425 min
Response: 0
Conc: N.D.

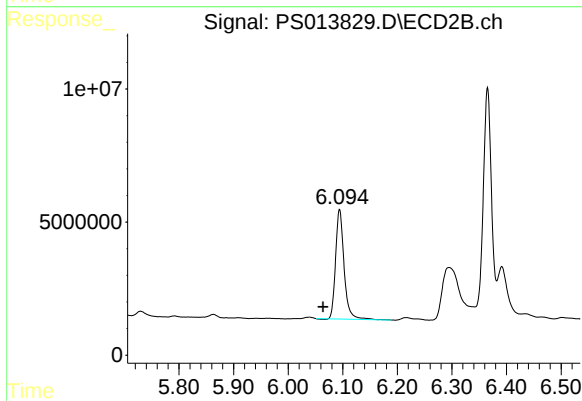

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.094 min
Delta R.T.: 0.030 min
Response: 44506767
Conc: 70.65 ng/ml

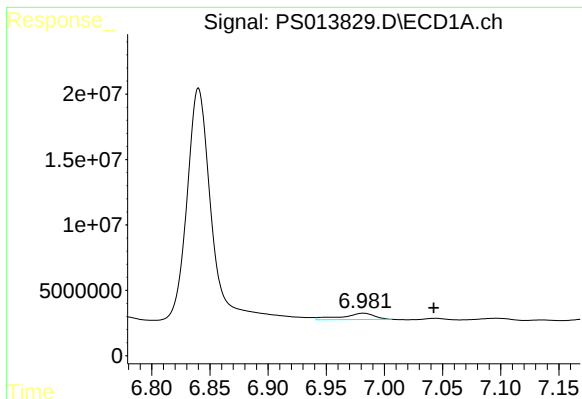

#3 4-Nitrophenol


R.T.: 6.982 min
Delta R.T.: -0.061 min
Response: 9529349
Conc: 20.04 ng/ml

Instrument :
ECD_S
ClientSampleId :

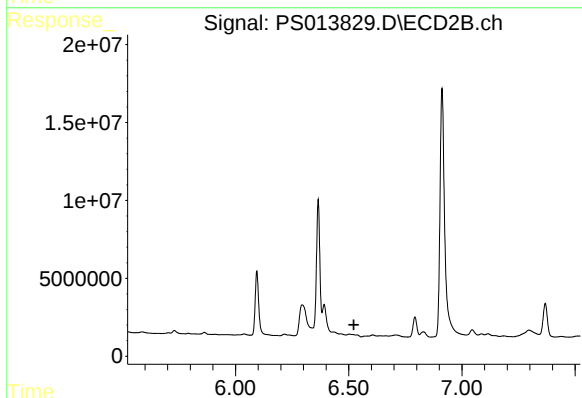


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.523 min
Response: 0
Conc: N.D.

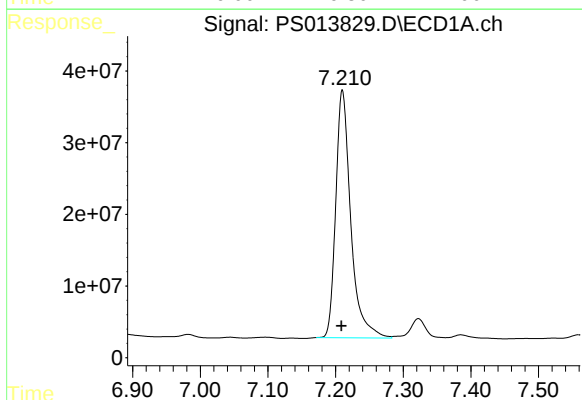


#4 2,4-DCAA

R.T.: 7.210 min
Delta R.T.: 0.002 min
Response: 533962404
Conc: 558.78 ng/ml

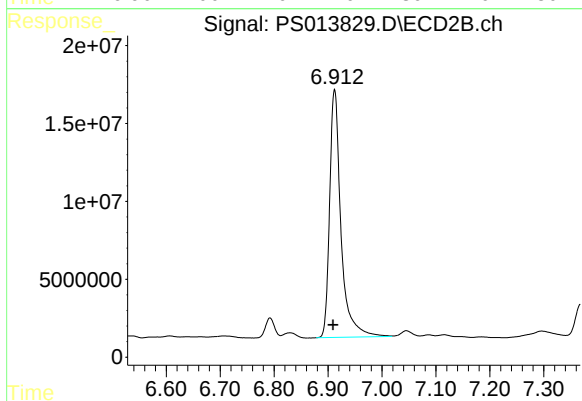

#4 2,4-DCAA


R.T.: 6.912 min
Delta R.T.: 0.003 min
Response: 232367760
Conc: 577.86 ng/ml

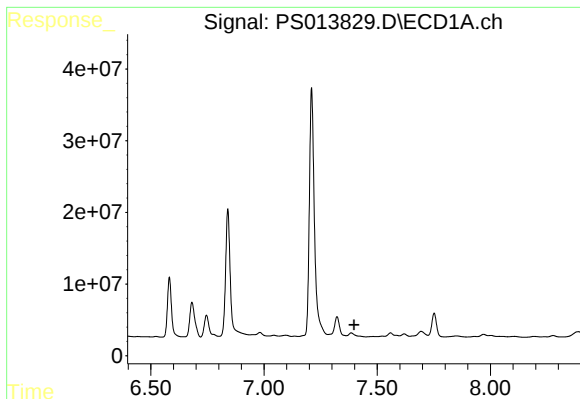

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.397 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

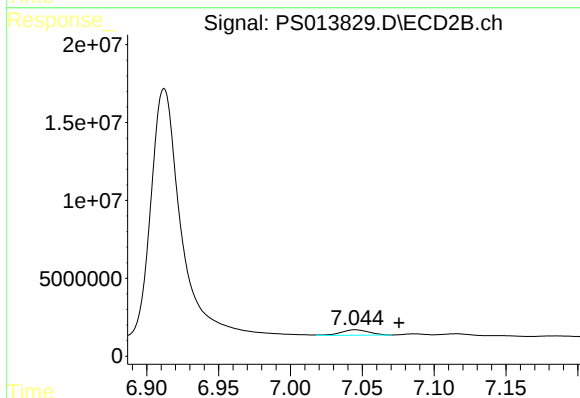


#5 DICAMBA

R.T.: 7.045 min
Delta R.T.: -0.030 min
Response: 4670539
Conc: 2.72 ng/ml

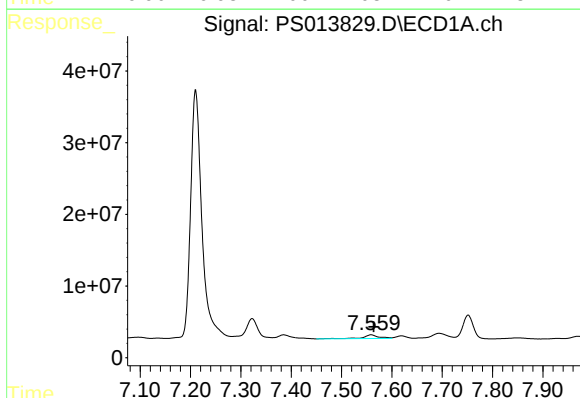


#6 MCP

R.T.: 7.559 min
Delta R.T.: -0.006 min
Response: 10977337
Conc: 3.83 ug/ml

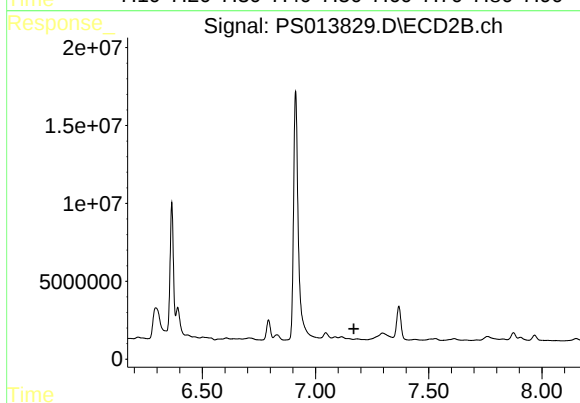

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.170 min
Response: 0
Conc: N.D.

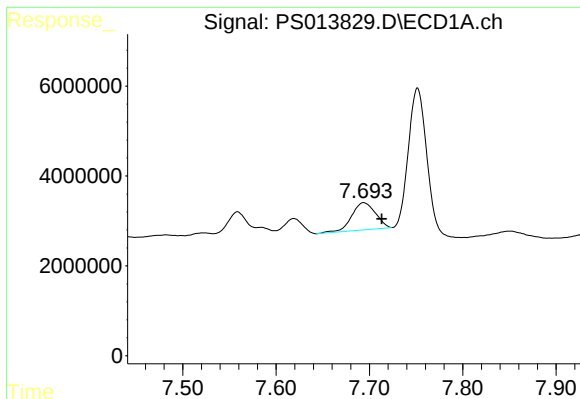

#7 MCPA


R.T.: 7.694 min
Delta R.T.: -0.019 min
Response: 10712752
Conc: 2.61 ug/ml

Instrument :
ECD_S
ClientSampleId :

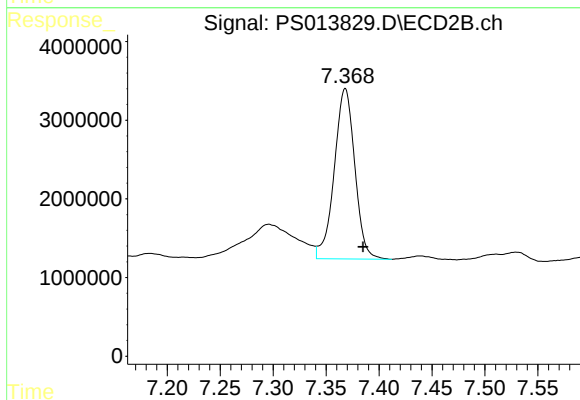


#7 MCPA

R.T.: 7.368 min
Delta R.T.: -0.017 min
Response: 29269147
Conc: 14.48 ug/ml

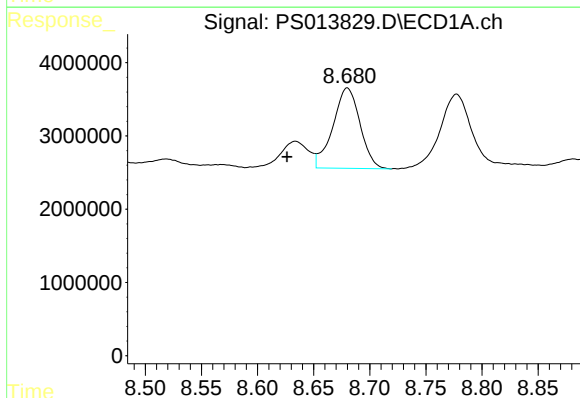


#10 Pentachlorophenol

R.T.: 8.680 min
Delta R.T.: 0.054 min
Response: 18467632
Conc: 1.30 ng/ml

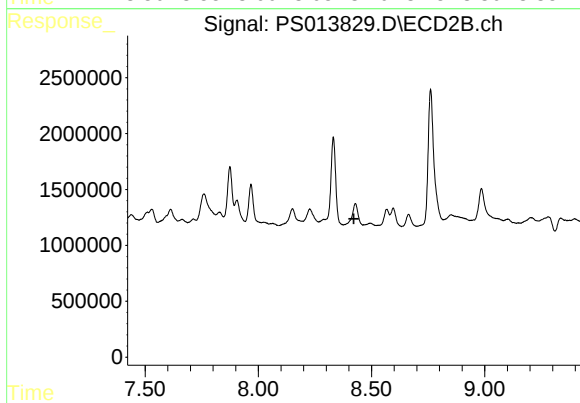

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 8.422 min
Response: 0
Conc: N.D.

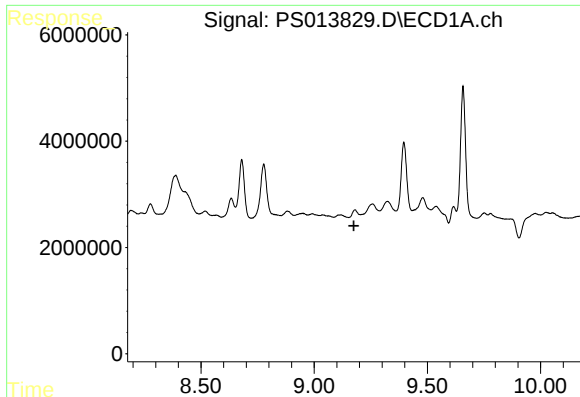

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.175 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

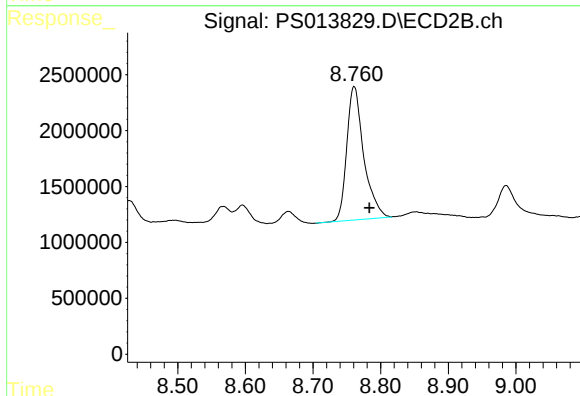


#11 2,4,5-TP (SILVEX)

R.T.: 8.761 min
Delta R.T.: -0.023 min
Response: 20772542
Conc: 8.70 ng/ml

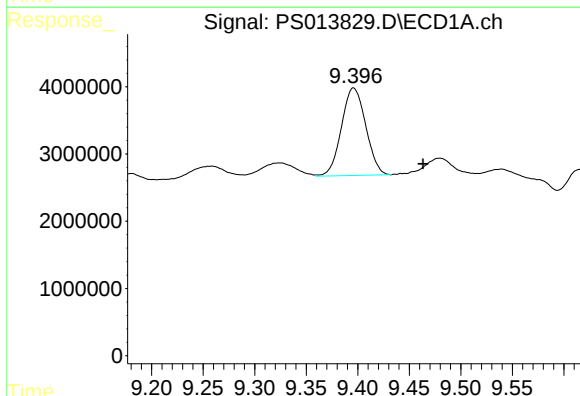


#12 2,4,5-T

R.T.: 9.396 min
Delta R.T.: -0.067 min
Response: 21402214
Conc: 3.78 ng/ml

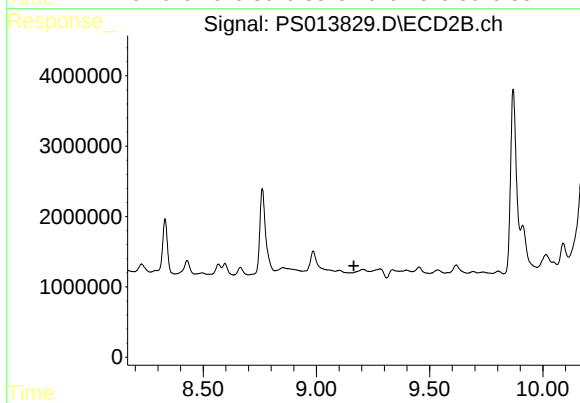

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.165 min
Response: 0
Conc: N.D.

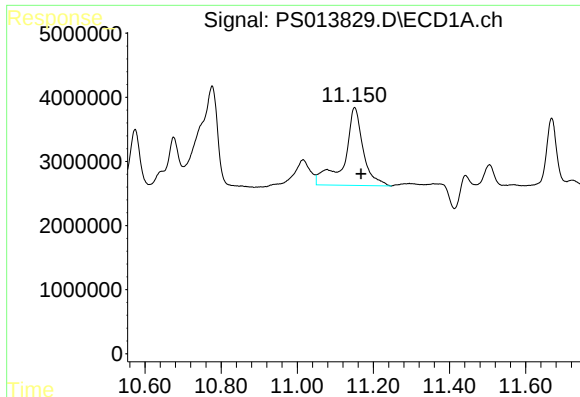

#14 DINOSEB


R.T.: 11.151 min
Delta R.T.: -0.017 min
Response: 41771327
Conc: 9.47 ng/ml

Instrument :
ECD_S
ClientSampleId :

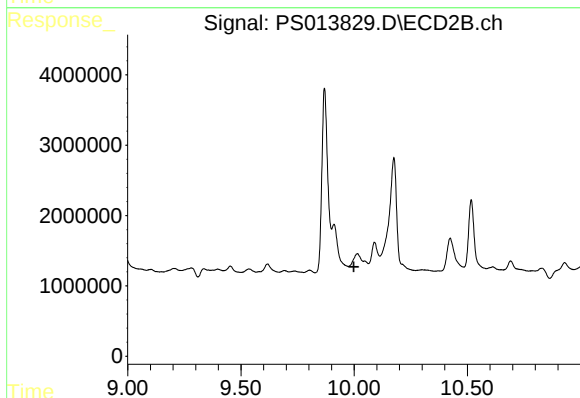


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.999 min
Response: 0
Conc: N.D.

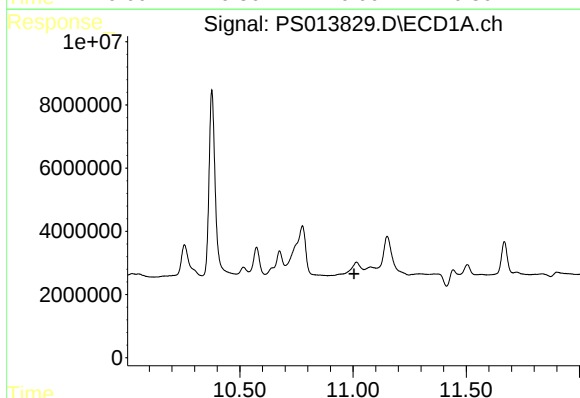


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.004 min
Response: 0
Conc: N.D.

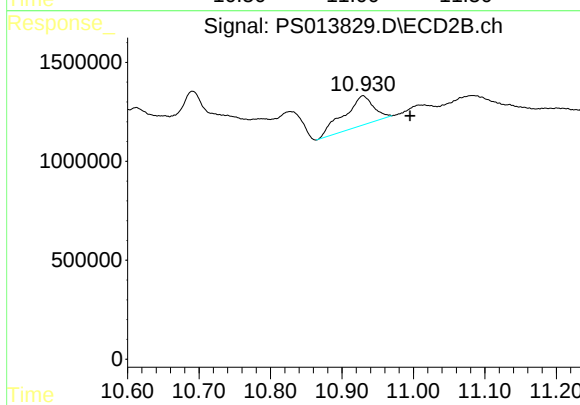

#15 Picloram


R.T.: 10.929 min
Delta R.T.: -0.066 min
Response: 4341357
Conc: 1.25 ng/ml

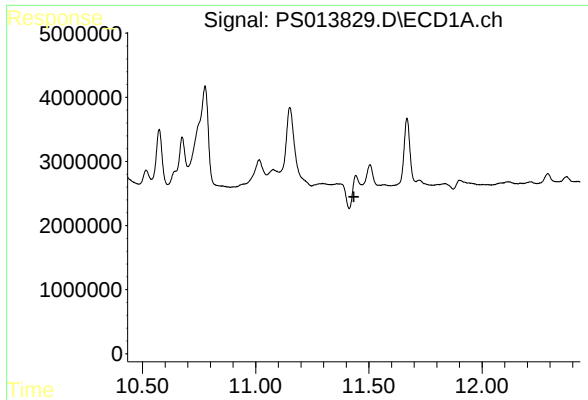

#16 DCPA

R.T.: 11.442 min
Delta R.T.: 0.009 min
Response: -3634897
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

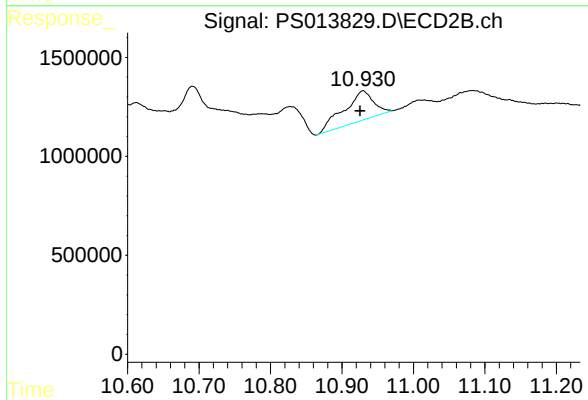

#16 DCPA

R.T.: 10.929 min
Delta R.T.: 0.004 min
Response: 4341357
Conc: 1.40 ng/ml