

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012122\
 Data File : PS018088.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jan 2022 08:42
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 21:30:46 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 06 10:21:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

2) T	3,5-DICHL...	6.316	0.000	93668409	0	43.542	N.D.	#
5) T	DICAMBA	0.000	6.848f	0	46660006	N.D.	17.748	
6) T	MCPD	0.000	6.848f	0	46660006	N.D.	21.693	
7) T	MCPA	7.491f	0.000	4152617	0	<MDL	N.D.	#
9) T	2,4-D	8.200f	0.000	182.1E6	0	99.978	N.D.	#
11) T	2,4,5-TP ...	0.000	8.437f	0	16873797	N.D.	4.734	
15) T	Picloram	10.811	10.670	50396795	20711076	4.222	4.429	
16) T	DCPA	11.244	10.670f	2304429	20711076	<MDL	4.691	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012122\
Data File : PS018088.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jan 2022 08:42
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 21:30:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
Quant Title : 8080.M
QLast Update : Thu Jan 06 10:21:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

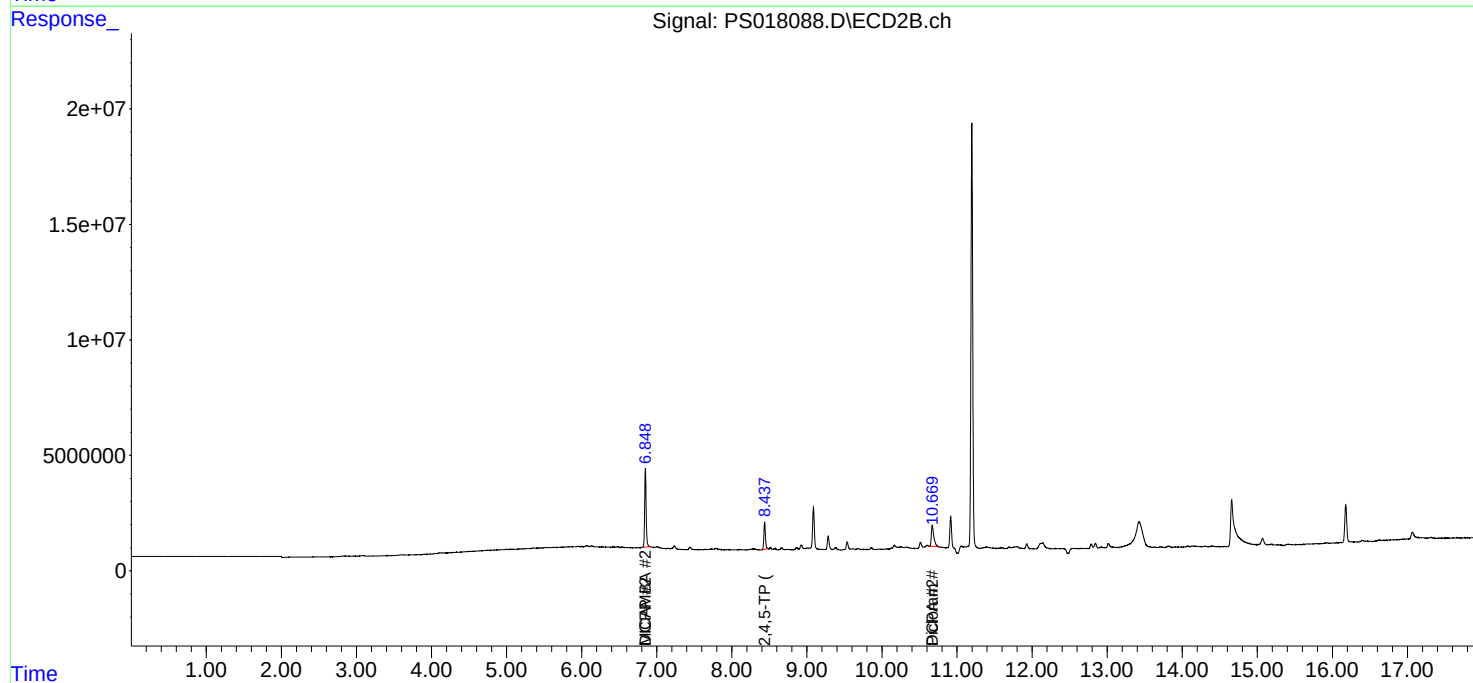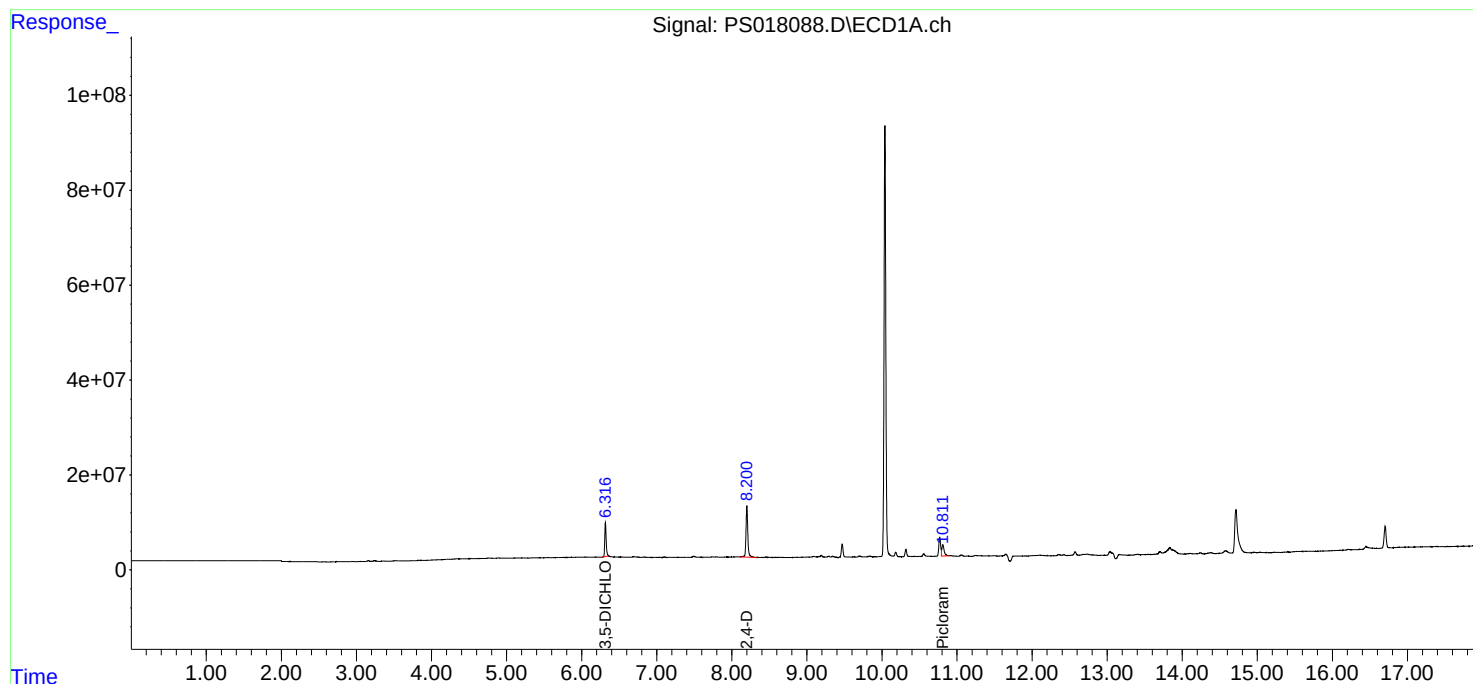


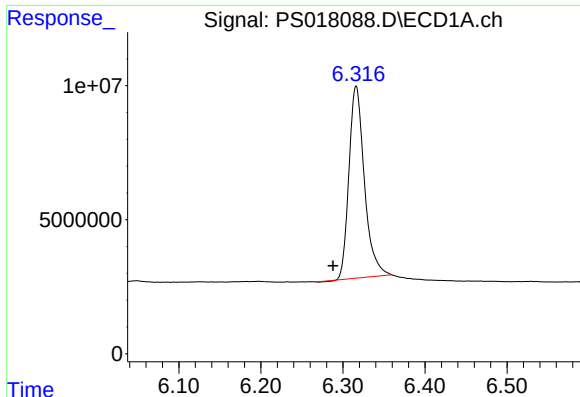

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.316 min
Delta R.T.: 0.028 min
Response: 93668409
Conc: 43.54 ng/ml

Instrument :
ECD_S
ClientSampleId :

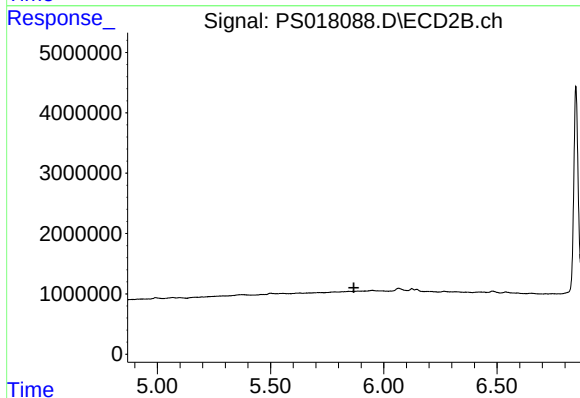


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.868 min
Response: 0
Conc: N.D.

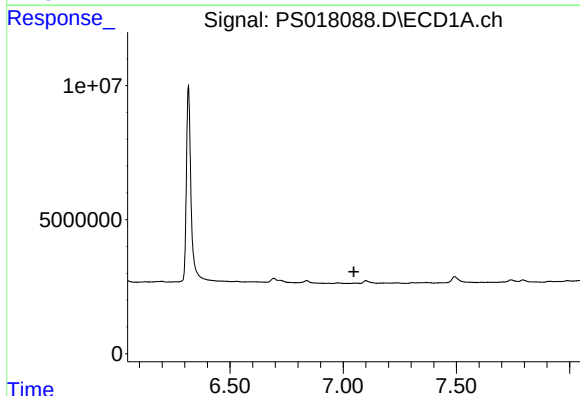


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.047 min
Response: 0
Conc: N.D.

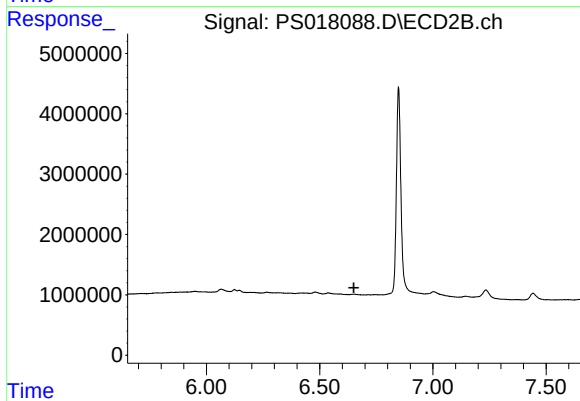

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.651 min
Response: 0
Conc: N.D.

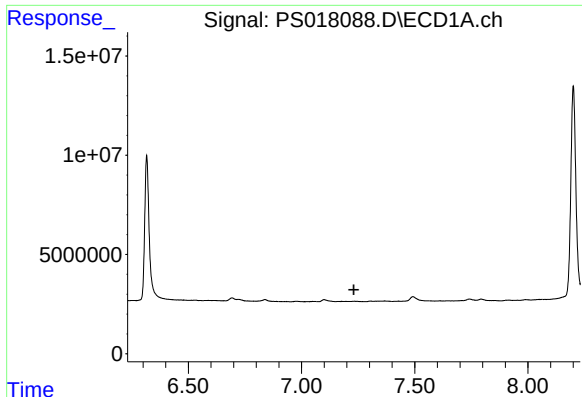

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.231 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

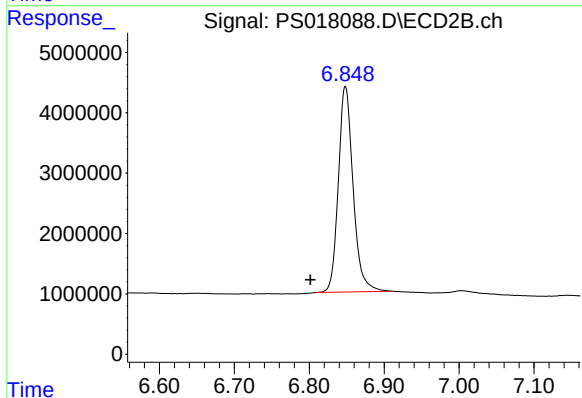


#5 DICAMBA

R.T.: 6.848 min
Delta R.T.: 0.046 min
Response: 46660006
Conc: 17.75 ng/ml

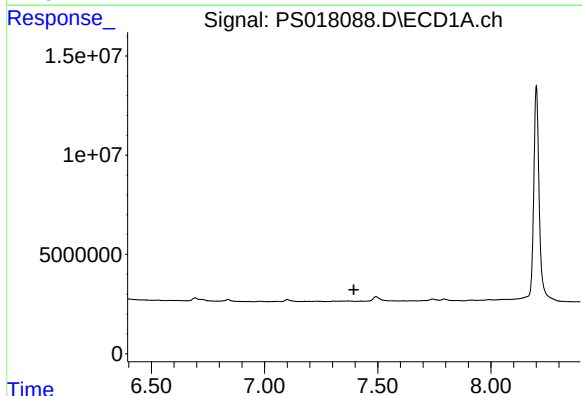


#6 MCP

R.T.: 0.000 min
Exp R.T.: 7.395 min
Response: 0
Conc: N.D.

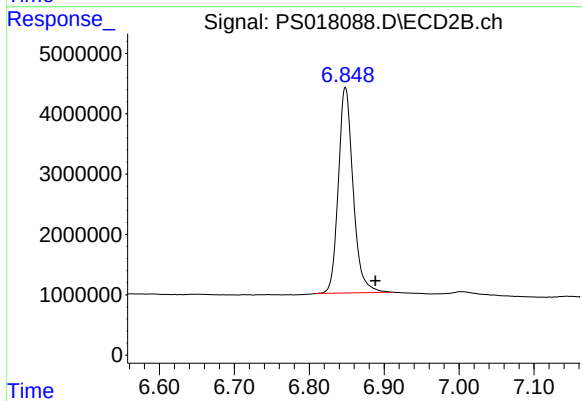

#6 MCP


R.T.: 6.848 min
Delta R.T.: -0.040 min
Response: 46660006
Conc: 21.69 ug/ml

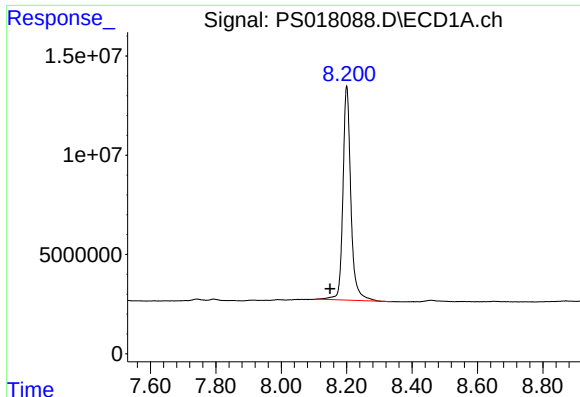

#9 2,4-D


R.T.: 8.200 min
Delta R.T.: 0.051 min
Response: 182053618
Conc: 99.98 ng/ml

Instrument :
ECD_S
ClientSampleId :

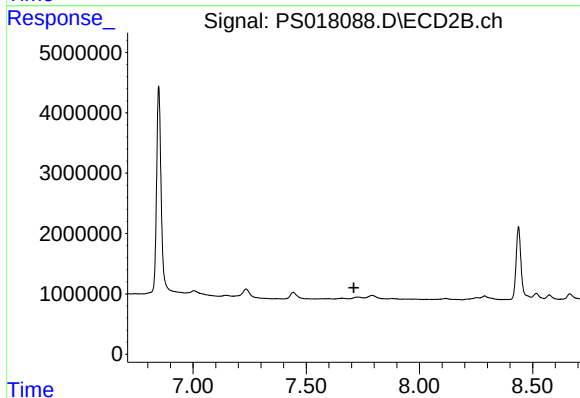


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.710 min
Response: 0
Conc: N.D.

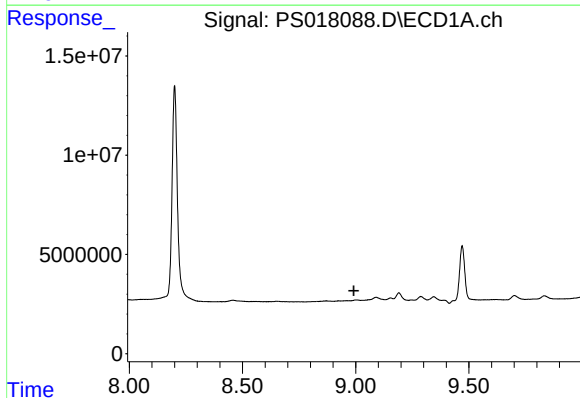


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 8.992 min
Response: 0
Conc: N.D.

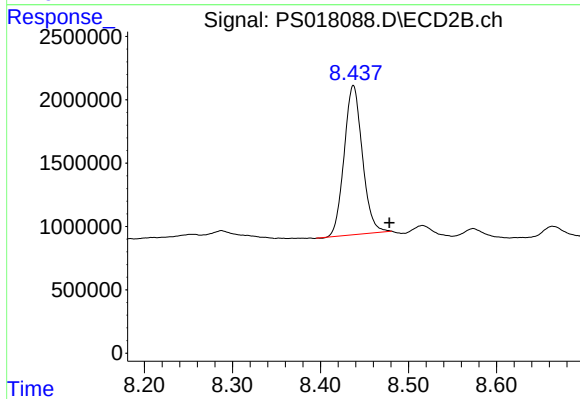

#11 2,4,5-TP (SILVEX)


R.T.: 8.437 min
Delta R.T.: -0.041 min
Response: 16873797
Conc: 4.73 ng/ml

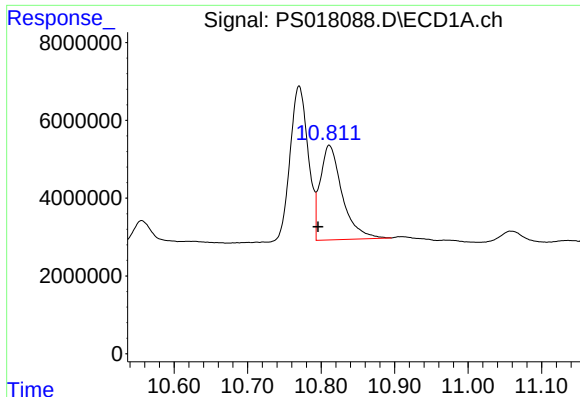

#15 Picloram


R.T.: 10.811 min
Delta R.T.: 0.015 min
Response: 50396795
Conc: 4.22 ng/ml

Instrument :
ECD_S
ClientSampleId :

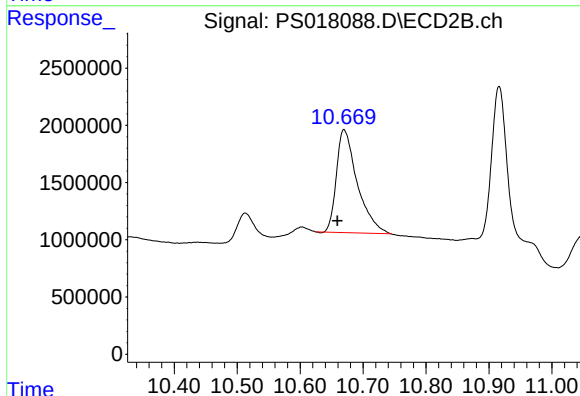


#15 Picloram

R.T.: 10.670 min
Delta R.T.: 0.011 min
Response: 20711076
Conc: 4.43 ng/ml

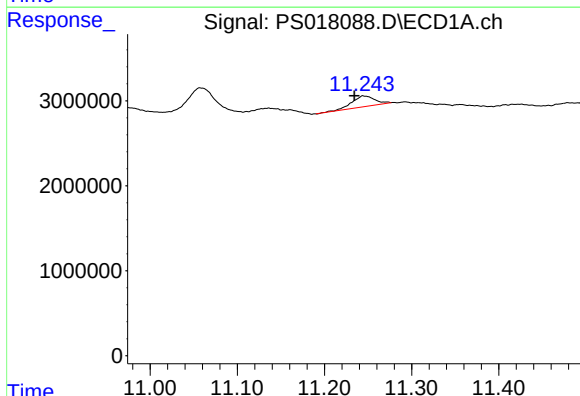

#16 DCPA

R.T.: 11.244 min
Delta R.T.: 0.010 min
Response: 2304429
Conc: N.D.

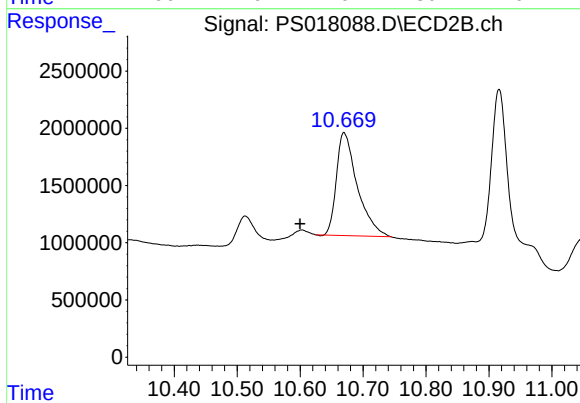

#16 DCPA

R.T.: 10.670 min
Delta R.T.: 0.070 min
Response: 20711076
Conc: 4.69 ng/ml