

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012122\
 Data File : PS018095.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jan 2022 18:40
 Operator : AJ\MA
 Sample : PB142176BS
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 21:33:52 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 06 10:21:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.046	6.645	825.9E6	322.6E6	571.386	555.884
Target Compounds							
1) T	Dalapon	2.910	2.419	1153.8E6	352.6E6	470.326	461.162
2) T	3,5-DICHL...	6.287	5.861	1095.3E6	459.0E6	509.140	518.858
3) T	4-Nitroph...	6.874	6.281	460.9E6	175.7E6	570.695	573.190
5) T	DICAMBA	7.233	6.800	3160.4E6	1322.6E6	506.122	503.085
6) T	MCPD	7.401	6.893	229.9E6	98972873	49.233	46.014
7) T	MCPA	7.549	7.102	326.4E6	145.7E6	48.922	48.825
8) T	DICHLORPROP	7.919	7.410	782.3E6	331.5E6	497.330	496.677
9) T	2,4-D	8.146	7.699	947.0E6	395.3E6	520.047	537.119
10) T	Pentachlo...	8.445	8.113	11172.7E6	4413.8E6	528.858	524.063
11) T	2,4,5-TP ...	8.995	8.475	4369.7E6	1842.9E6	516.379	516.983
12) T	2,4,5-T	9.277	8.851	4513.1E6	1774.7E6	509.147	542.563
13) T	2,4-DB	9.824	9.354	901.5E6	228.3E6	545.347	516.065
14) T	DINOSEB	10.972	9.675	3295.7E6	1266.5E6	501.866	507.622
15) T	Picloram	10.796	10.653	6212.9E6	2404.0E6	520.519	514.101
16) T	DCPA	11.241	10.601	5668.1E6	2283.8E6	524.595	517.233



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012122\
Data File : PS018095.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jan 2022 18:40
Operator : AJ\MA
Sample : PB142176BS
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 21:33:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
Quant Title : 8080.M
QLast Update : Thu Jan 06 10:21:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

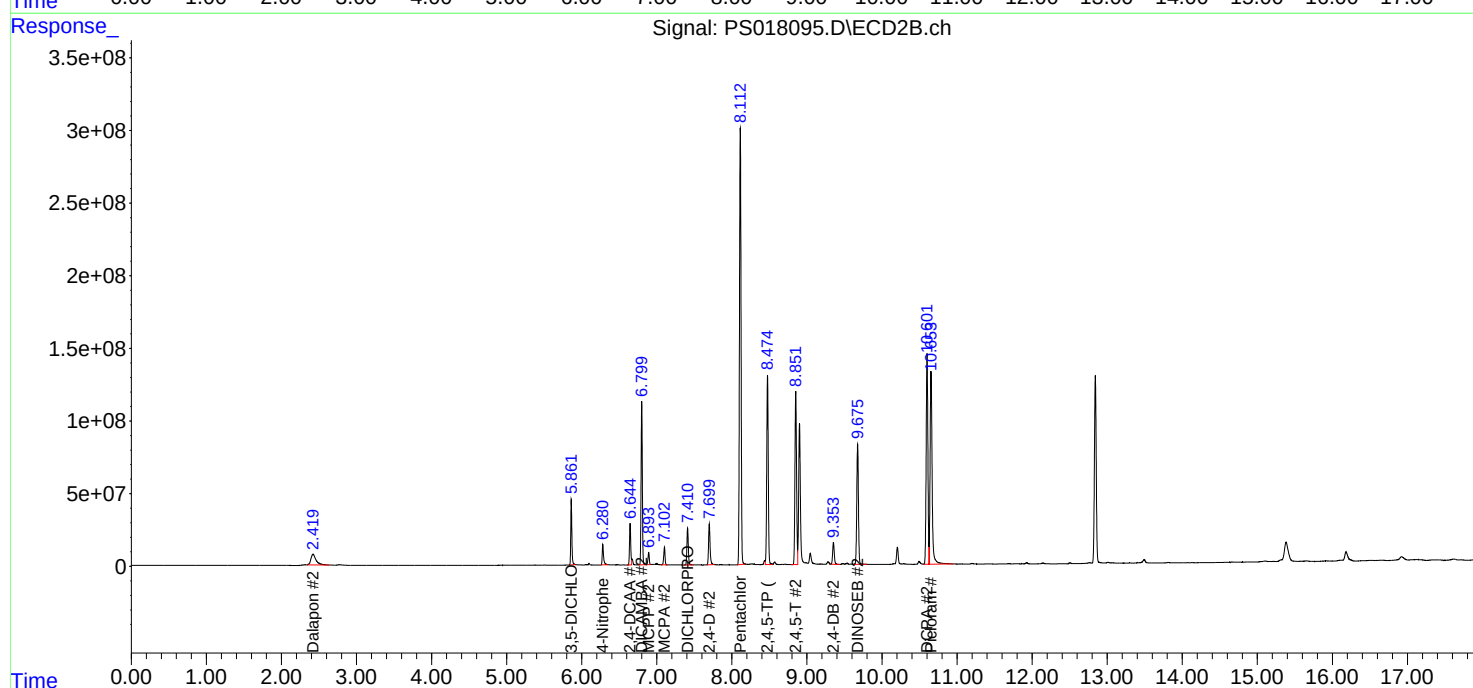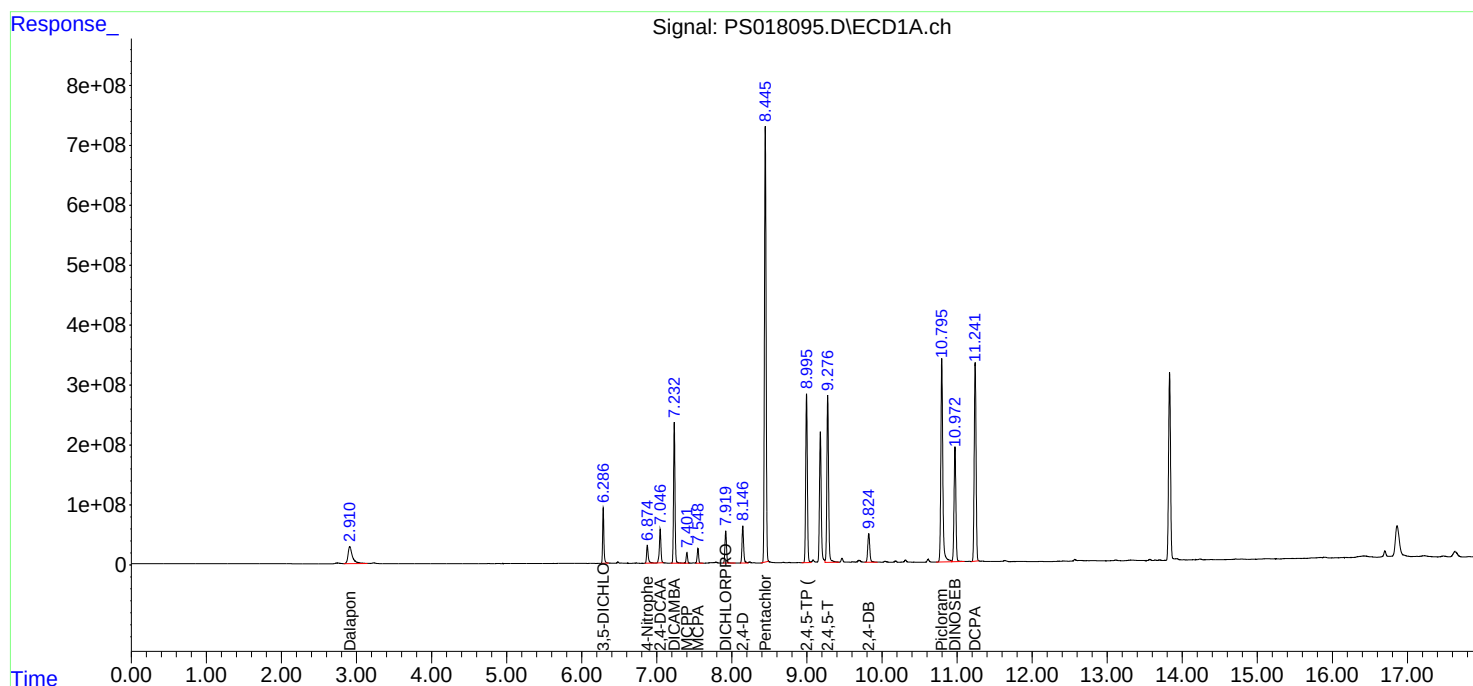


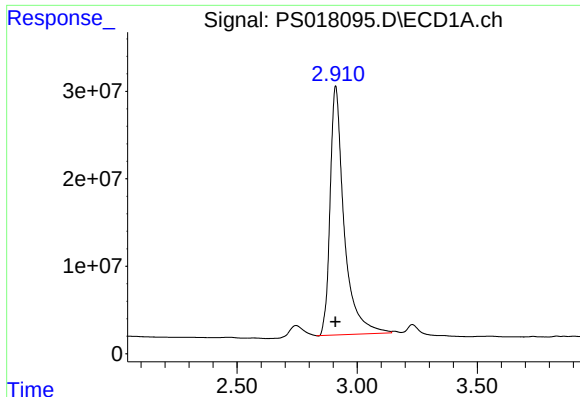

#1 Dalapon


R.T.: 2.910 min
Delta R.T.: 0.001 min
Response: 1153814200
Conc: 470.33 ng/ml

Instrument :
ECD_S
ClientSampleId :

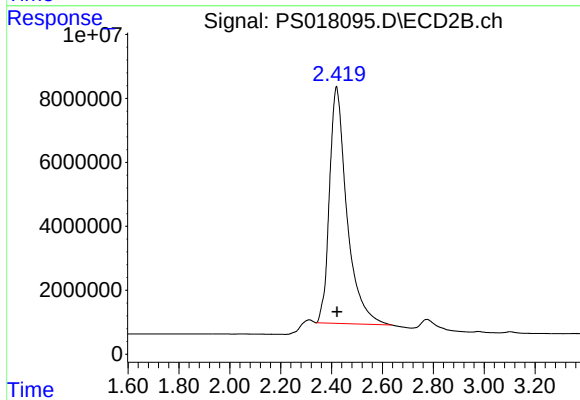


#1 Dalapon

R.T.: 2.419 min
Delta R.T.: -0.001 min
Response: 352645046
Conc: 461.16 ng/ml

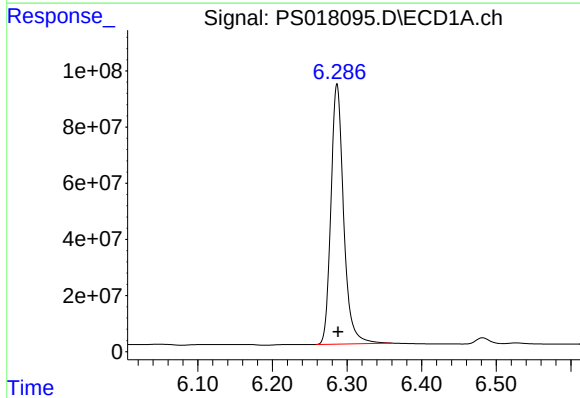


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.287 min
Delta R.T.: -0.002 min
Response: 1095284701
Conc: 509.14 ng/ml

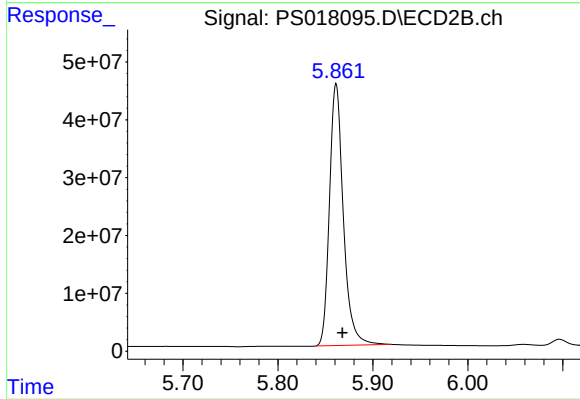

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.861 min
Delta R.T.: -0.007 min
Response: 458997608
Conc: 518.86 ng/ml

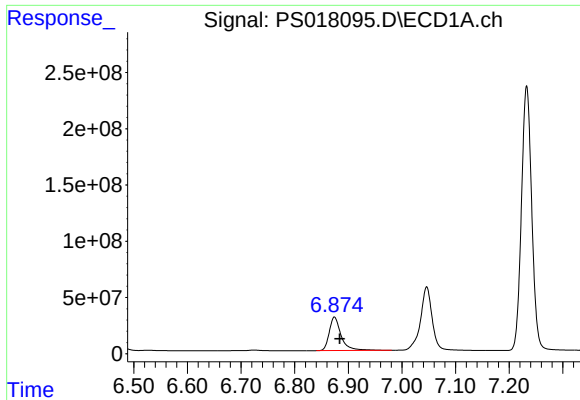

#3 4-Nitrophenol


R.T.: 6.874 min
Delta R.T.: -0.010 min
Response: 460941293
Conc: 570.70 ng/ml

Instrument :
ECD_S
ClientSampleId :

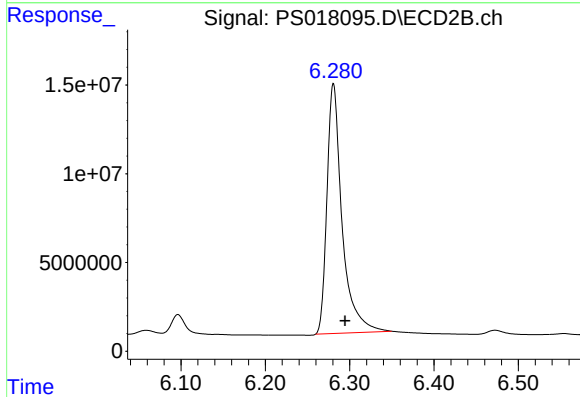


#3 4-Nitrophenol

R.T.: 6.281 min
Delta R.T.: -0.014 min
Response: 175695560
Conc: 573.19 ng/ml

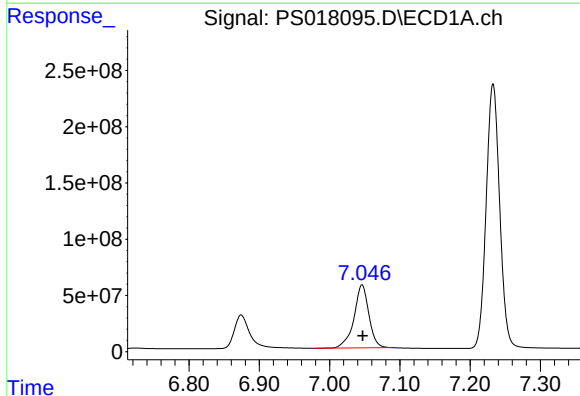


#4 2,4-DCAA

R.T.: 7.046 min
Delta R.T.: -0.001 min
Response: 825931484
Conc: 571.39 ng/ml

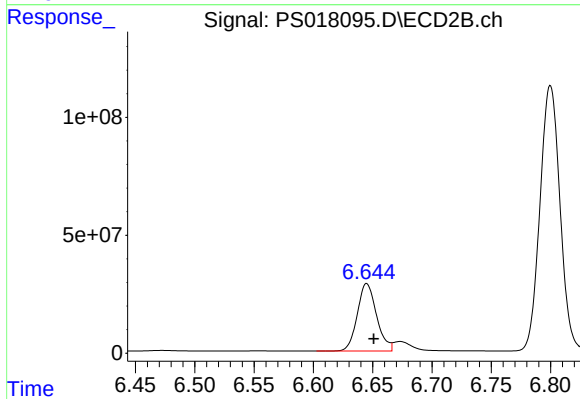

#4 2,4-DCAA


R.T.: 6.645 min
Delta R.T.: -0.006 min
Response: 322551067
Conc: 555.88 ng/ml

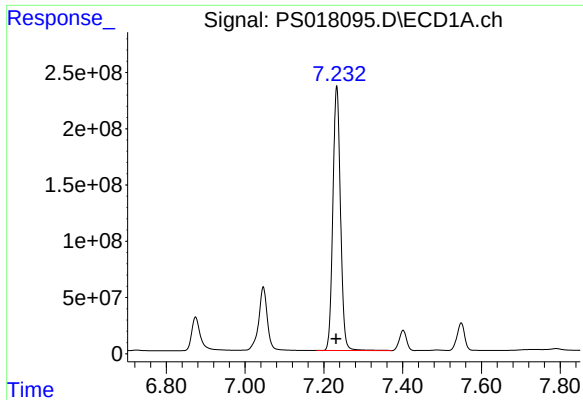

#5 DICAMBA


R.T.: 7.233 min
Delta R.T.: 0.002 min
Response: 3160436731
Conc: 506.12 ng/ml

Instrument :
ECD_S
ClientSampleId :

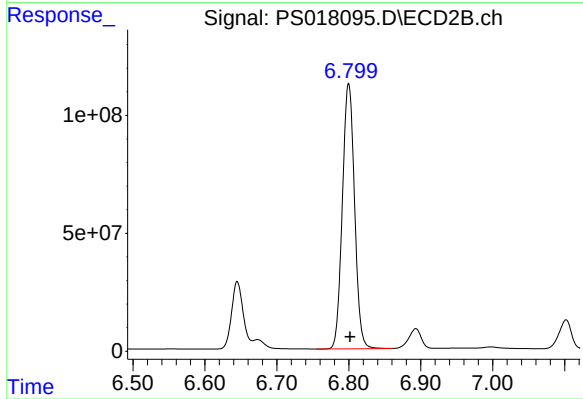


#5 DICAMBA

R.T.: 6.800 min
Delta R.T.: -0.002 min
Response: 1322636300
Conc: 503.08 ng/ml

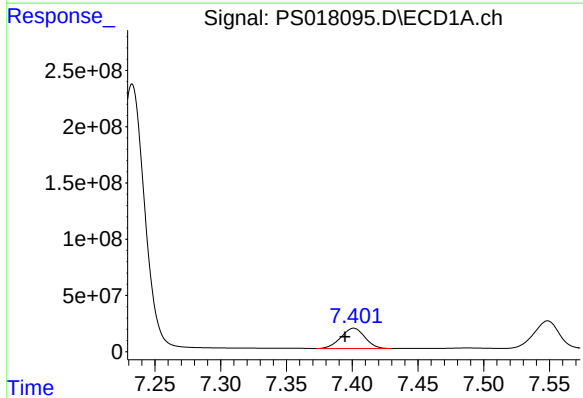


#6 MCP

R.T.: 7.401 min
Delta R.T.: 0.007 min
Response: 229864945
Conc: 49.23 ug/ml

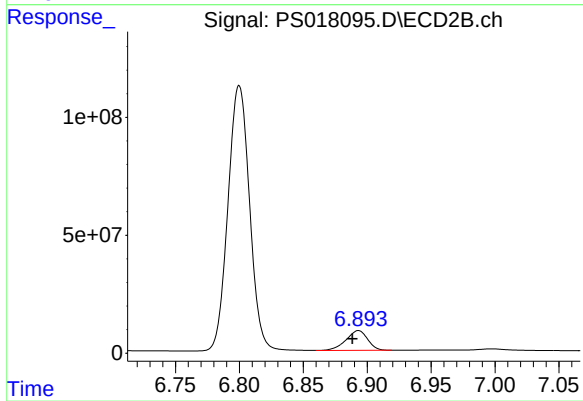

#6 MCP


R.T.: 6.893 min
Delta R.T.: 0.005 min
Response: 98972873
Conc: 46.01 ug/ml

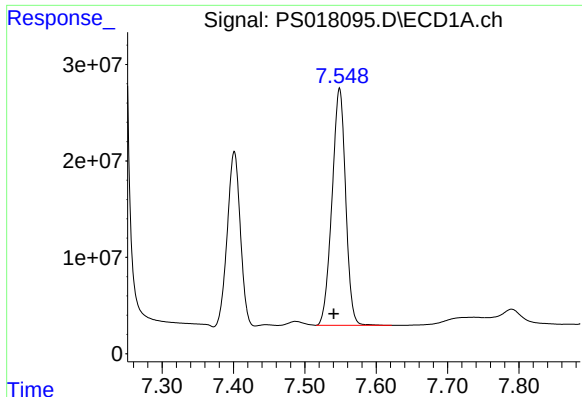

#7 MCPA


R.T.: 7.549 min
Delta R.T.: 0.008 min
Response: 326396818
Conc: 48.92 ug/ml

Instrument :
ECD_S
ClientSampleId :

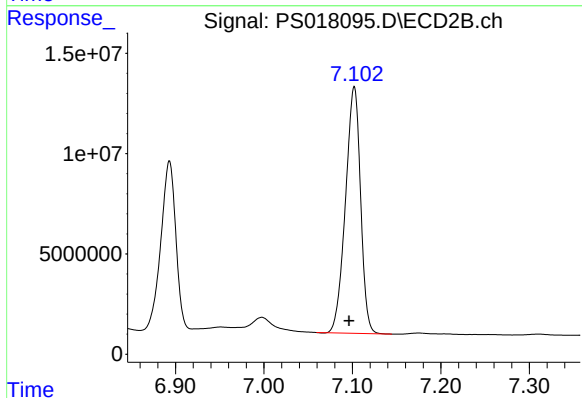


#7 MCPA

R.T.: 7.102 min
Delta R.T.: 0.006 min
Response: 145691883
Conc: 48.83 ug/ml

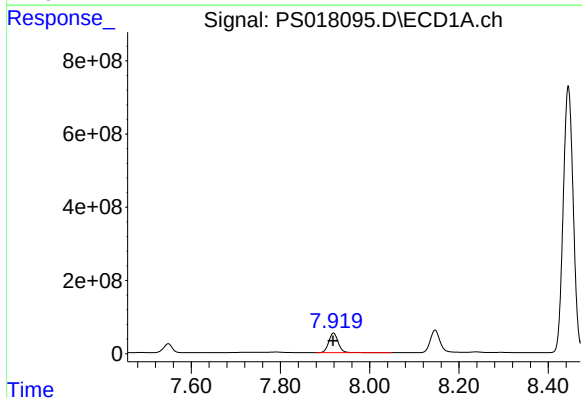


#8 DICHLORPROP

R.T.: 7.919 min
Delta R.T.: 0.001 min
Response: 782323535
Conc: 497.33 ng/ml

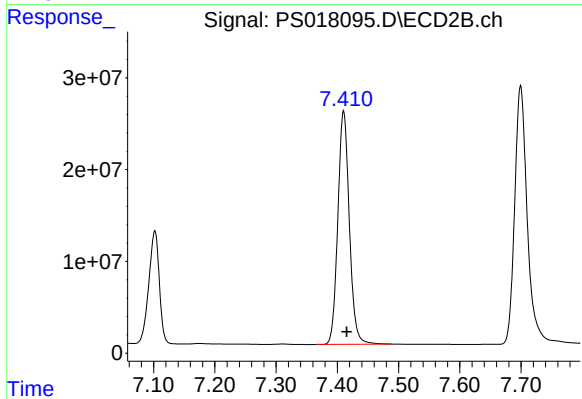

#8 DICHLORPROP


R.T.: 7.410 min
Delta R.T.: -0.005 min
Response: 331493906
Conc: 496.68 ng/ml

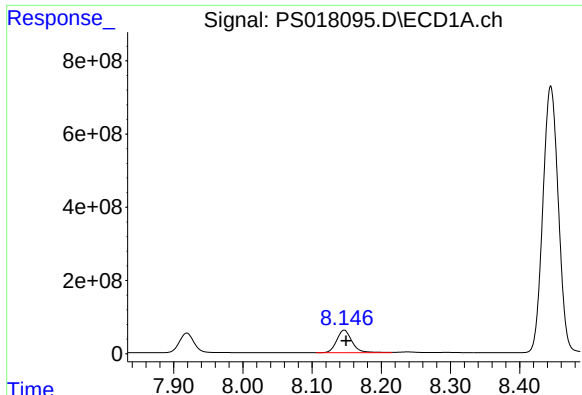

#9 2,4-D


R.T.: 8.146 min
Delta R.T.: -0.003 min
Response: 946971327
Conc: 520.05 ng/ml

Instrument :
ECD_S
ClientSampleId :

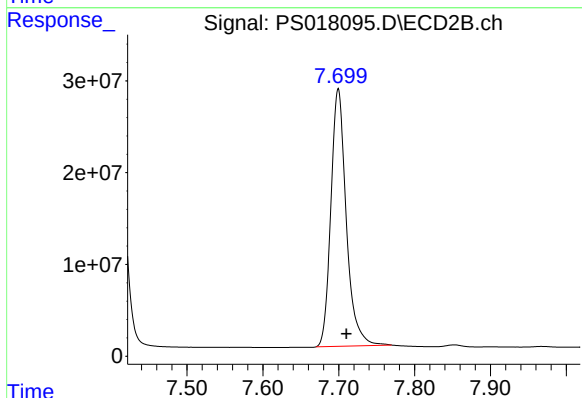


#9 2,4-D

R.T.: 7.699 min
Delta R.T.: -0.011 min
Response: 395290060
Conc: 537.12 ng/ml

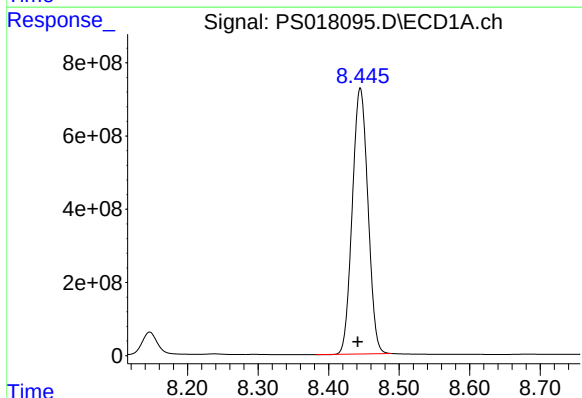


#10 Pentachlorophenol

R.T.: 8.445 min
Delta R.T.: 0.004 min
Response: 11172676473
Conc: 528.86 ng/ml

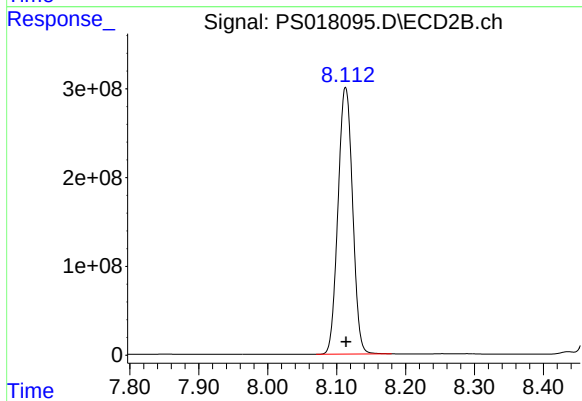

#10 Pentachlorophenol


R.T.: 8.113 min
Delta R.T.: 0.000 min
Response: 4413845246
Conc: 524.06 ng/ml

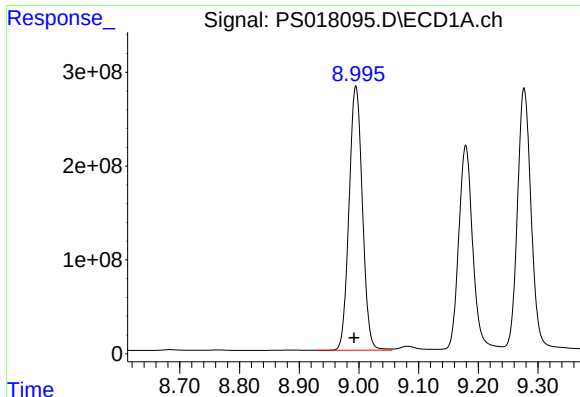

#11 2,4,5-TP (SILVEX)


R.T.: 8.995 min
Delta R.T.: 0.003 min
Response: 4369670153
Conc: 516.38 ng/ml

Instrument :
ECD_S
ClientSampleId :

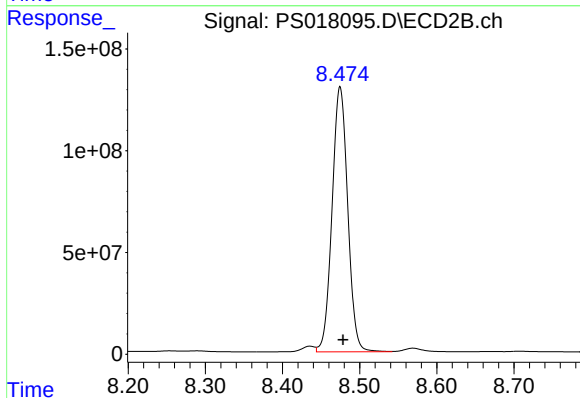


#11 2,4,5-TP (SILVEX)

R.T.: 8.475 min
Delta R.T.: -0.004 min
Response: 1842884398
Conc: 516.98 ng/ml

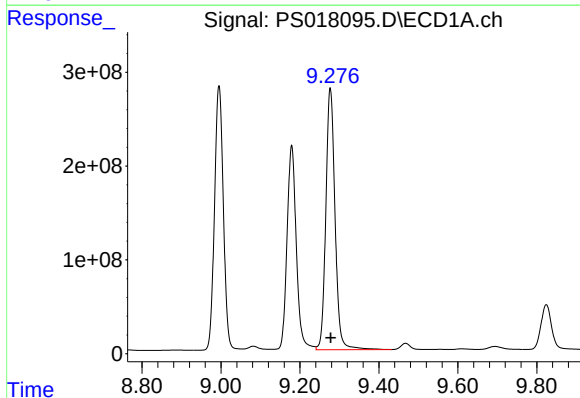


#12 2,4,5-T

R.T.: 9.277 min
Delta R.T.: -0.001 min
Response: 4513146863
Conc: 509.15 ng/ml

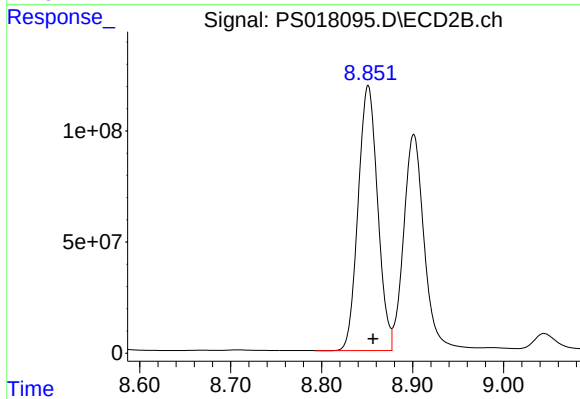

#12 2,4,5-T


R.T.: 8.851 min
Delta R.T.: -0.006 min
Response: 1774734111
Conc: 542.56 ng/ml

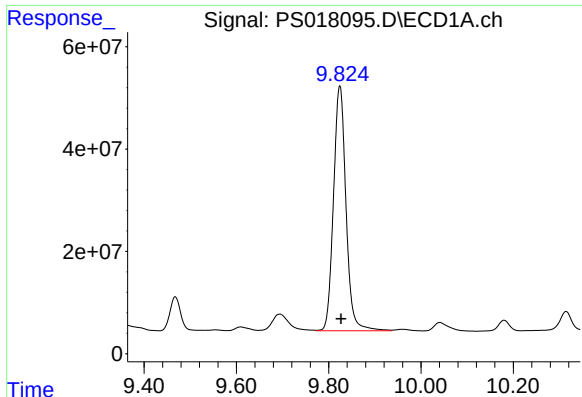

#13 2,4-DB


R.T.: 9.824 min
Delta R.T.: -0.003 min
Response: 901477788
Conc: 545.35 ng/ml

Instrument :
ECD_S
ClientSampleId :

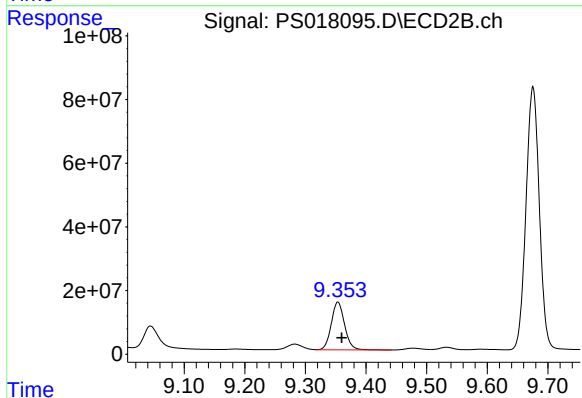


#13 2,4-DB

R.T.: 9.354 min
Delta R.T.: -0.006 min
Response: 228336682
Conc: 516.06 ng/ml

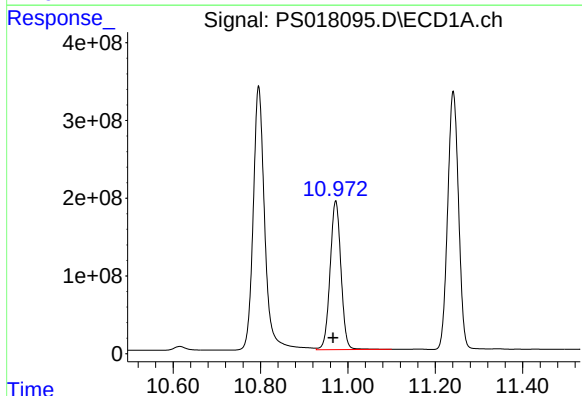


#14 DINOSEB

R.T.: 10.972 min
Delta R.T.: 0.006 min
Response: 3295728231
Conc: 501.87 ng/ml

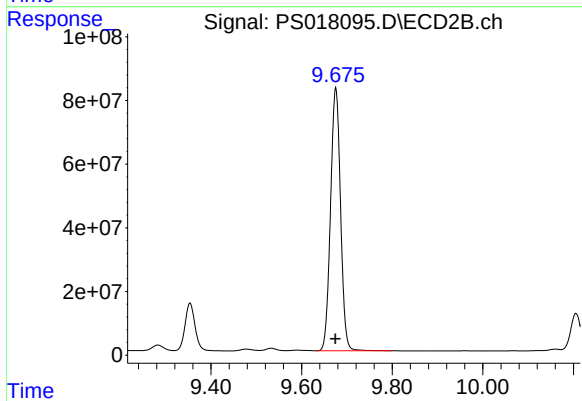

#14 DINOSEB


R.T.: 9.675 min
Delta R.T.: 0.000 min
Response: 1266524220
Conc: 507.62 ng/ml

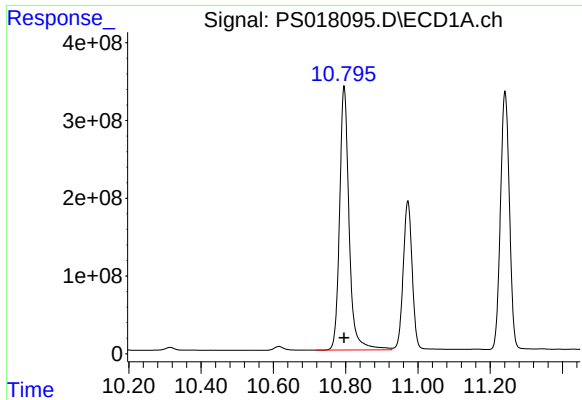

#15 Picloram


R.T.: 10.796 min
Delta R.T.: 0.000 min
Response: 6212864293
Conc: 520.52 ng/ml

Instrument :
ECD_S
ClientSampleId :

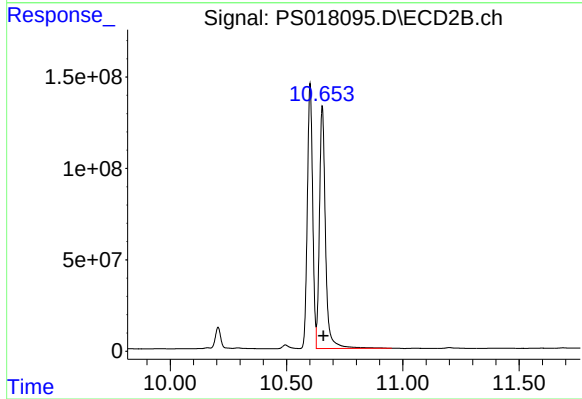


#15 Picloram

R.T.: 10.653 min
Delta R.T.: -0.006 min
Response: 2404014081
Conc: 514.10 ng/ml

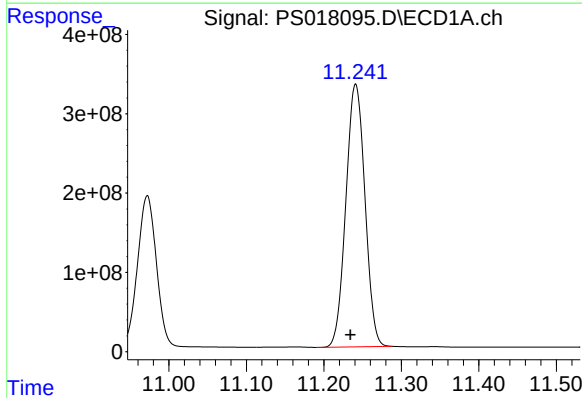

#16 DCPA

R.T.: 11.241 min
Delta R.T.: 0.007 min
Response: 5668135374
Conc: 524.59 ng/ml

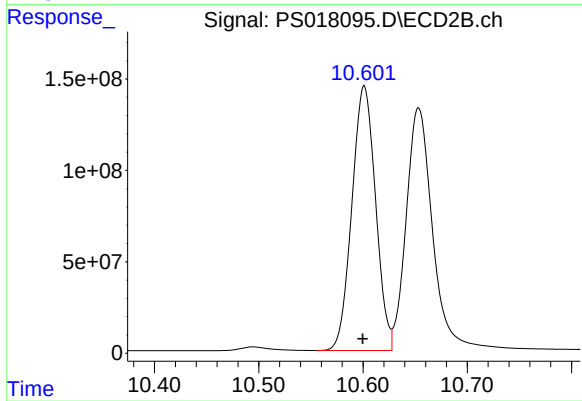

#16 DCPA

R.T.: 10.601 min
Delta R.T.: 0.001 min
Response: 2283833092
Conc: 517.23 ng/ml