

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS012122\  
 Data File : PS018097.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 21 Jan 2022 19:33  
 Operator : AJ\MA  
 Sample : N1218-01  
 Misc :  
 ALS Vial : 10 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 EAST-BOILER-PIT-WASTE-CLASS

Manual Integrations  
 APPROVED

Reviewed By : Abdul Mirza 01/24/2022  
 Supervised By : Ankita Jodhani 01/25/2022

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Jan 21 21:34:56 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS010522.M  
 Quant Title : 8080.M  
 QLast Update : Thu Jan 06 10:21:08 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1  | RT#2  | Resp#1  | Resp#2  | ng/ml    | ng/ml   |
|-----------------------------|-------|-------|---------|---------|----------|---------|
| -----                       |       |       |         |         |          |         |
| System Monitoring Compounds |       |       |         |         |          |         |
| 4) S 2,4-DCAA               | 7.045 | 6.644 | 311.0E6 | 139.3E6 | 215.175m | 240.110 |

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS012122\  
Data File : PS018097.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 21 Jan 2022 19:33  
Operator : AJ\MA  
Sample : N1218-01  
Misc :  
ALS Vial : 10 Sample Multiplier: 1



Instrument :  
ECD\_S  
ClientSampleId :  
EAST-BOILER-PIT-WASTE-CLASS


Manual Integrations  
APPROVED

Reviewed By : Abdul Mirza 01/24/2022  
Supervised By : Ankita Jodhani 01/25/2022

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jan 21 21:34:56 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS010522.M  
Quant Title : 8080.M  
QLast Update : Thu Jan 06 10:21:08 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

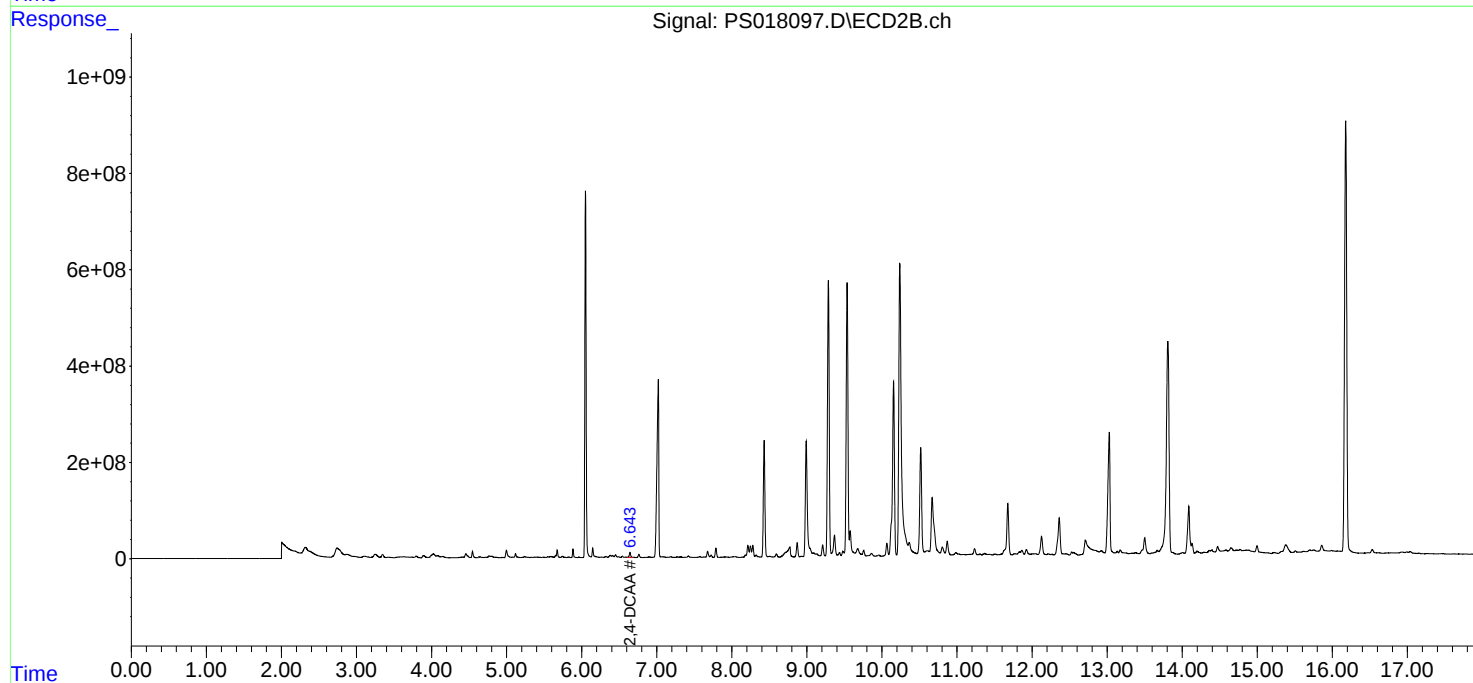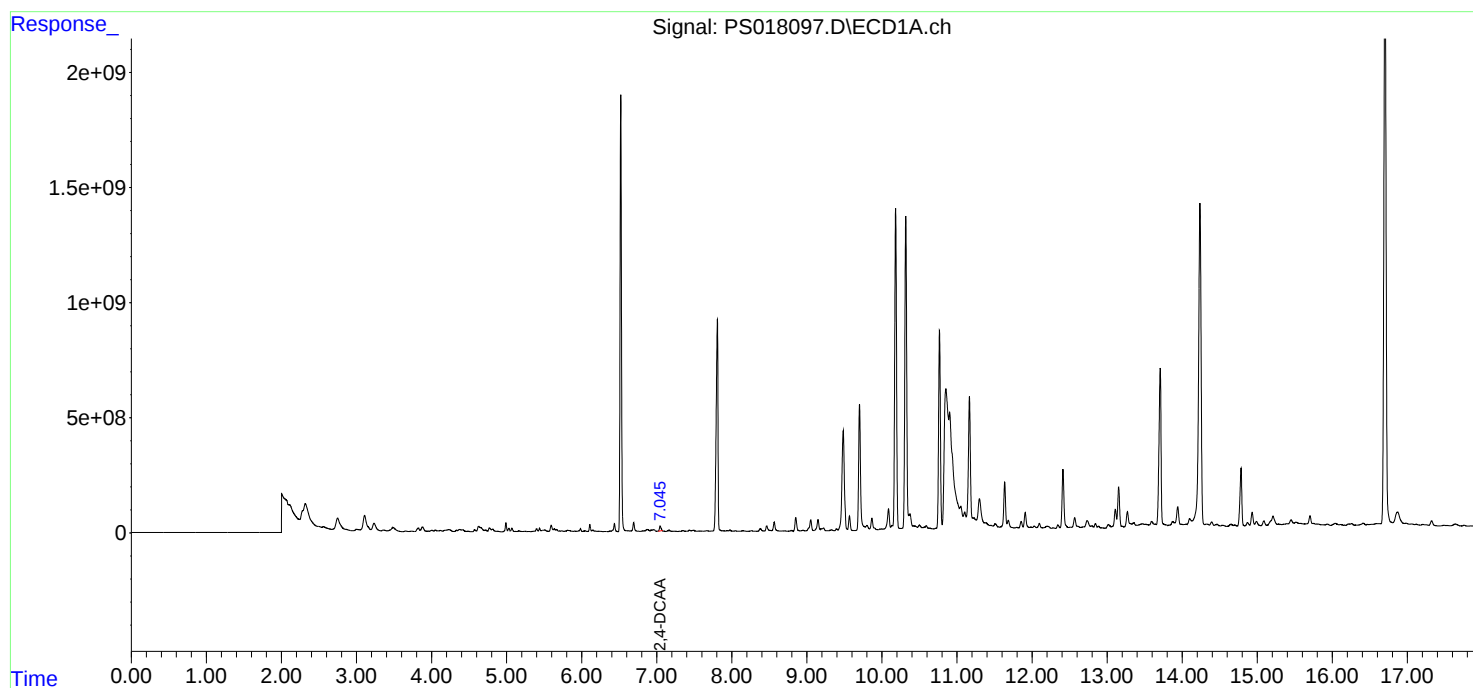

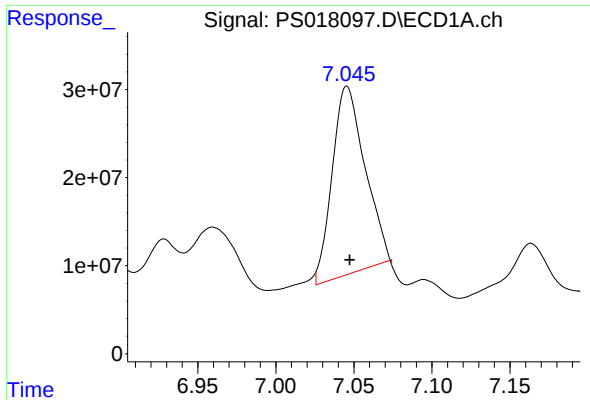


#4 2,4-DCAA

R.T.: 7.045 min  
Delta R.T.: -0.002 min  
Response: 311033206  
Conc: 215.18 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :  
EAST-BOILER-PIT-WASTE-CLASS

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 01/24/2022  
Supervised By :Ankita Jodhani 01/25/2022

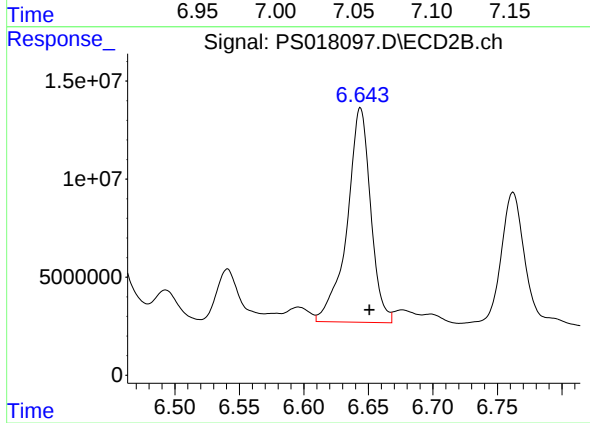

#4 2,4-DCAA

R.T.: 6.644 min  
Delta R.T.: -0.007 min  
Response: 139323680  
Conc: 240.11 ng/ml