

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012125\
 Data File : PS028933.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jan 2025 10:32
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 22 00:24:01 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS011425.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 14 12:25:39 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.170f	0.000	402769	0	<MDL	N.D. #
Target Compounds							
1) T	Dalapon	2.660f	0.000	2984907	0	1.001	N.D. #
2) T	3,5-DICHL...	6.355	6.643	1103962	2847847	<MDL	1.723 #
3) T	4-Nitroph...	6.979	0.000	5521055	0	3.116	N.D. #
5) T	DICAMBA	7.413f	0.000	81109	0	<MDL	N.D. #
7) T	MCPA	7.754f	8.202	599328	3680684	<MDL	<MDL #
8) T	DICHLORPROP	8.089	0.000	1064727	0	<MDL	N.D. #
10) T	Pentachlo...	8.601	0.000	149952	0	<MDL	N.D. #
12) T	2,4,5-T	9.482	0.000	942374	0	<MDL	N.D. #
13) T	2,4-DB	10.008f	0.000	1191775	0	<MDL	N.D. #
14) T	DINOSEB	11.227f	0.000	3901307	0	<MDL	N.D. #
15) T	Picloram	11.083	12.264	34038568	10705786	1.079	<MDL #
16) T	DCPA	11.528	0.000	6198112	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012125\
Data File : PS028933.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jan 2025 10:32
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 22 00:24:01 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS011425.M
Quant Title : 8080.M
QLast Update : Tue Jan 14 12:25:39 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

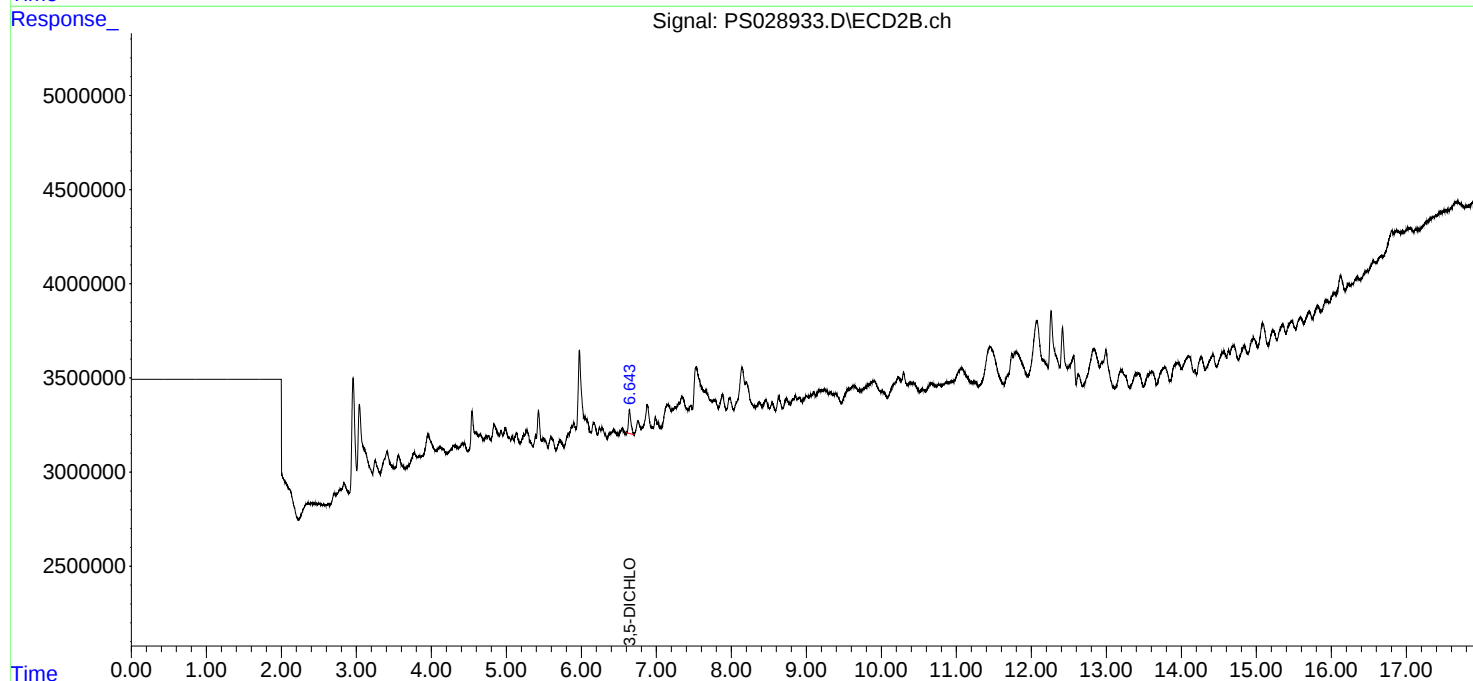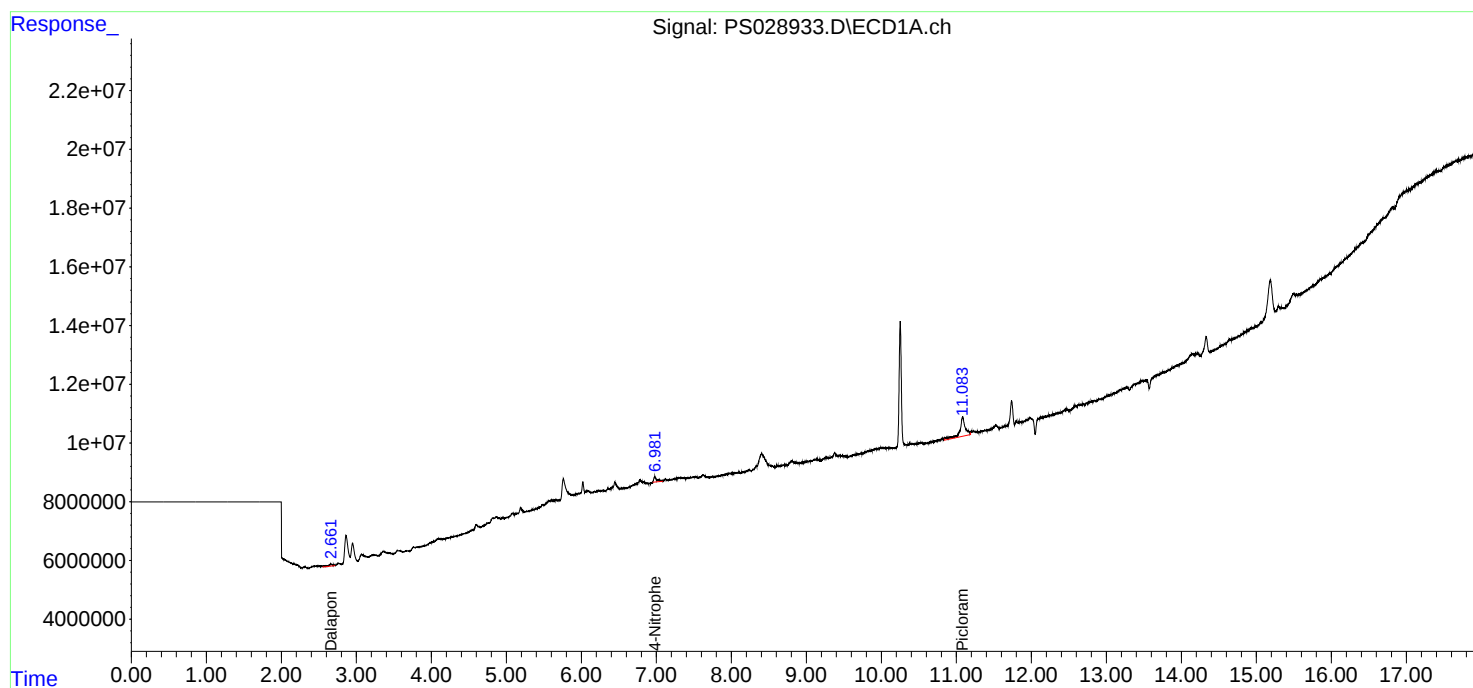


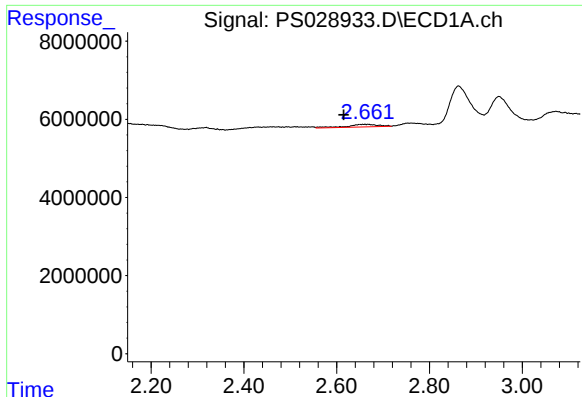

#1 Dalapon


R.T.: 2.660 min
Delta R.T.: 0.045 min
Response: 2984907
Conc: 1.00 ng/ml

Instrument :
ECD_S
ClientSampleId :

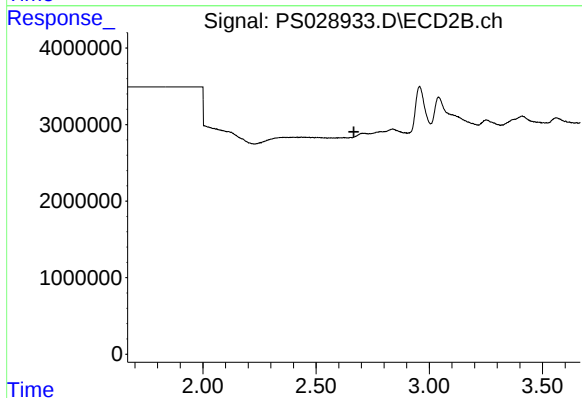


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.667 min
Response: 0
Conc: N.D.

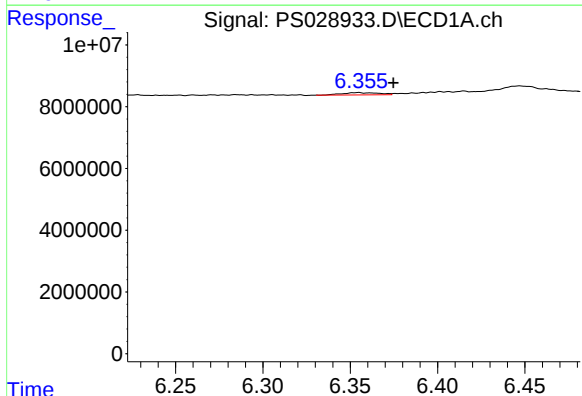


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.355 min
Delta R.T.: -0.020 min
Response: 1103962
Conc: N.D.

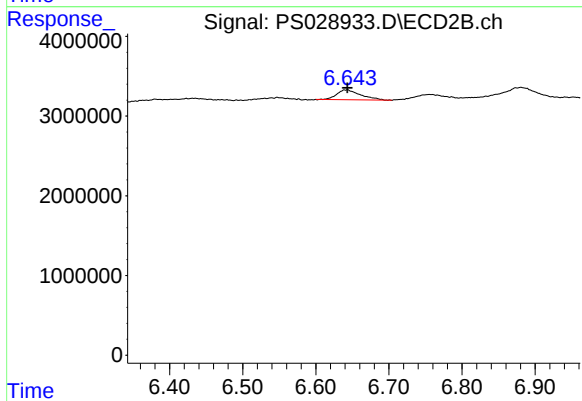

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.643 min
Delta R.T.: 0.000 min
Response: 2847847
Conc: 1.72 ng/ml

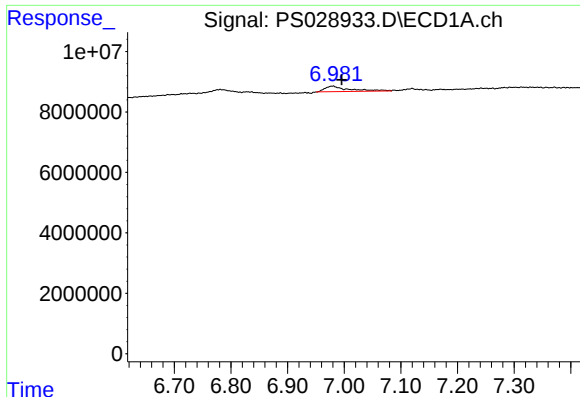

#3 4-Nitrophenol


R.T.: 6.979 min
Delta R.T.: -0.017 min
Response: 5521055
Conc: 3.12 ng/ml

Instrument :
ECD_S
ClientSampleId :

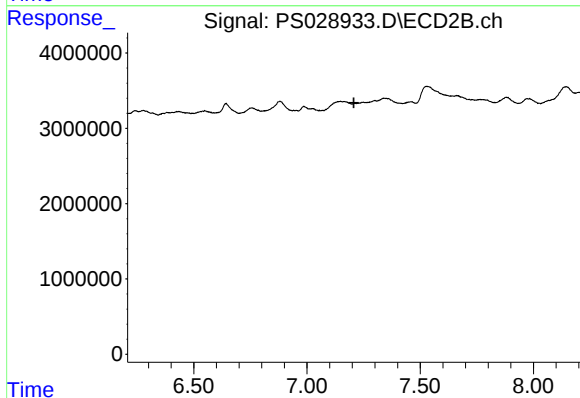


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.207 min
Response: 0
Conc: N.D.

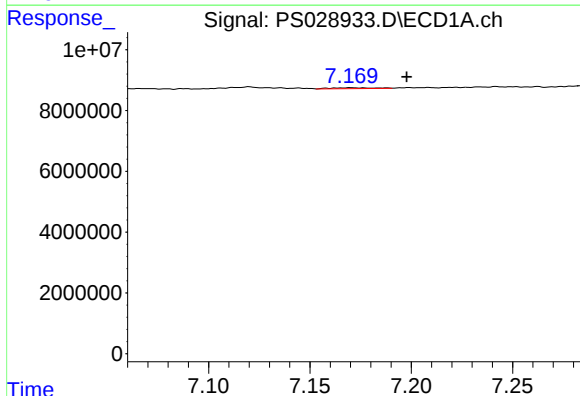


#4 2,4-DCAA

R.T.: 7.170 min
Delta R.T.: -0.027 min
Response: 402769
Conc: N.D.

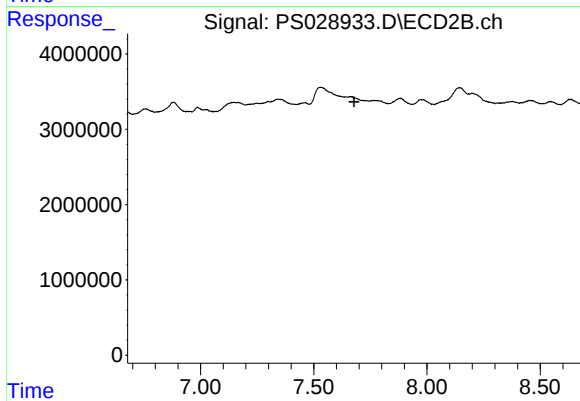

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 7.678 min
Response: 0
Conc: N.D.

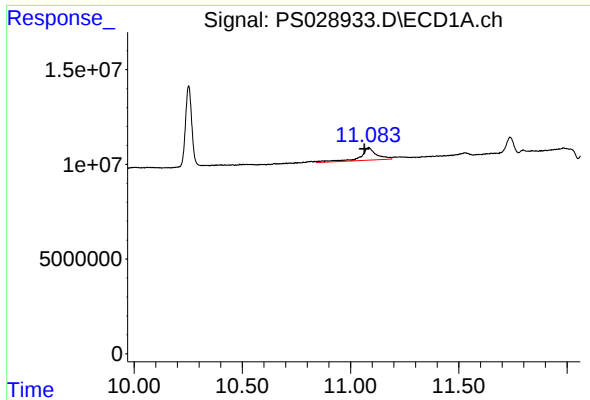

#15 Picloram

R.T.: 11.083 min
Delta R.T.: 0.019 min
Response: 34038568
Conc: 1.08 ng/ml

Instrument :
ECD_S
ClientSampleId :

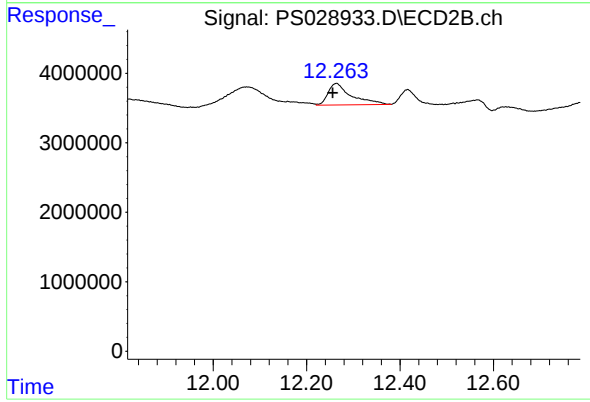

#15 Picloram

R.T.: 12.264 min
Delta R.T.: 0.008 min
Response: 10705786
Conc: N.D.