

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012219\
 Data File : PS002924.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jan 2019 11:31
 Operator : EI\SJ
 Sample : HSTDICC1500
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDICC1500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 23 07:55:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012219.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 23 07:53:15 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.284	10.783	309.1E6	392.7E6	924.419	1011.129
Target Compounds							
1) T	Dalapon	2.841	2.308	643.6E6	611.2E6	1349.176	1309.641
2) T	3,5-DICHL...	9.712	8.941	509.9E6	318.2E6	976.073	647.972 #
7) T	MCPA	0.000	11.684	0	227.0E6	N.D.	149.140 #
8) T	DICHLORPROP	12.783	12.190	517.9E6	250.0E6	1408.219	670.735 #
10) T	Pentachlo...	0.000	13.199	0	1573.8E6	N.D.	271.148 #
14) T	DINOSEB	0.000	15.464	0	1185.2E6	N.D.	710.168 #
15) T	Picloram	0.000	16.693	0	1020.7E6	N.D.	339.380 #
16) T	DCPA	0.000	16.693	0	1020.7E6	N.D.	343.882 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012219\
Data File : PS002924.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jan 2019 11:31
Operator : EI\SJ
Sample : HSTDICC1500
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDICC1500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 23 07:55:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012219.M
Quant Title : 8080.M
QLast Update : Wed Jan 23 07:53:15 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

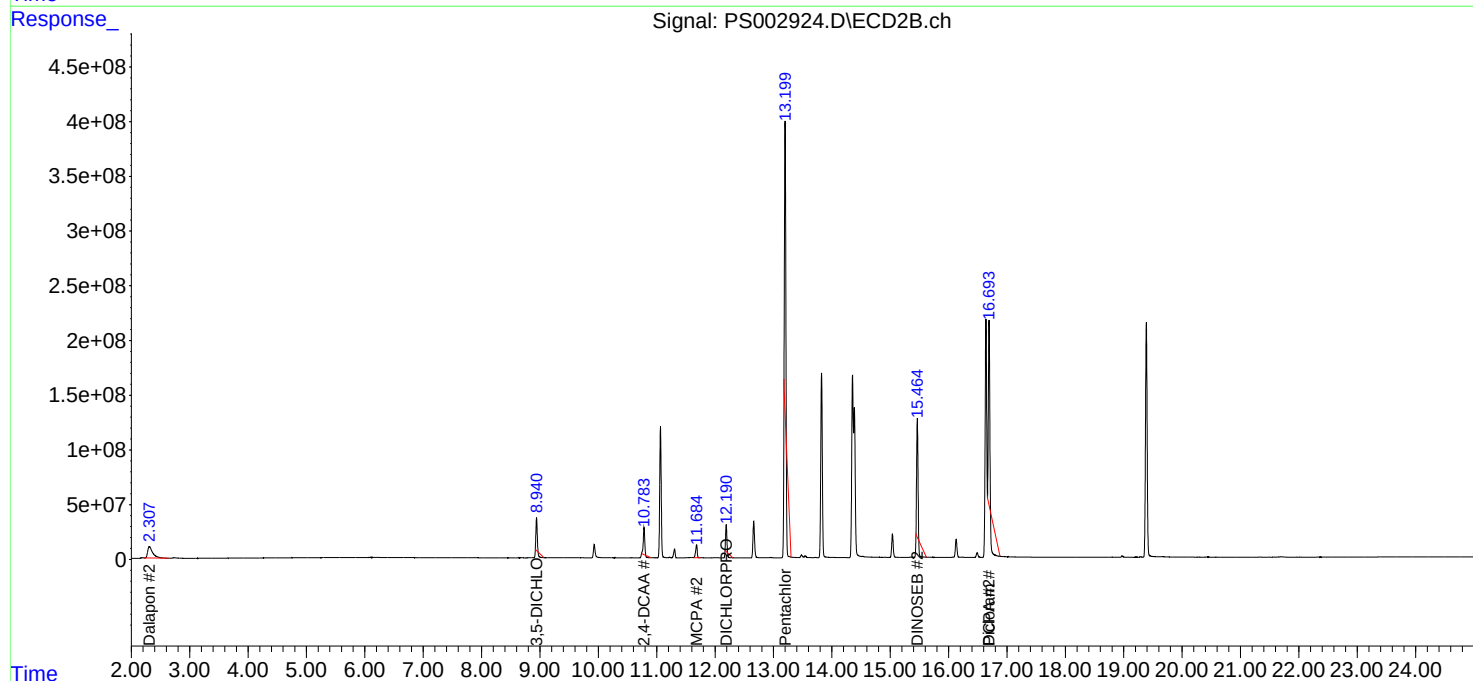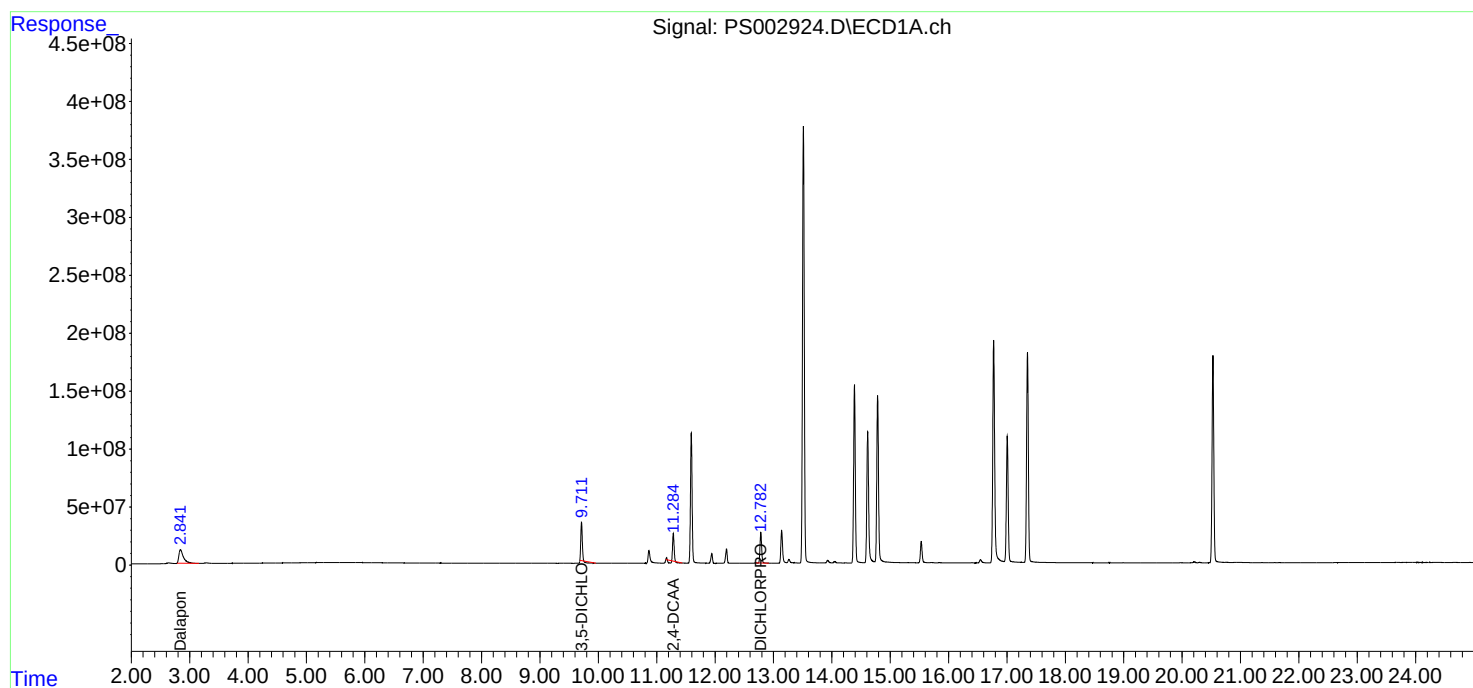


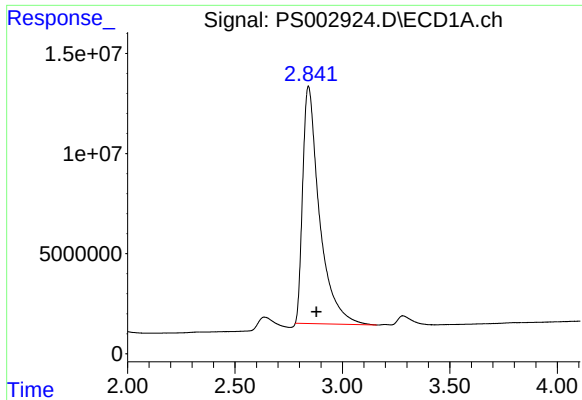

#1 Dalapon


R.T.: 2.841 min
Delta R.T.: -0.038 min
Response: 643572321
Conc: 1349.18 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC1500

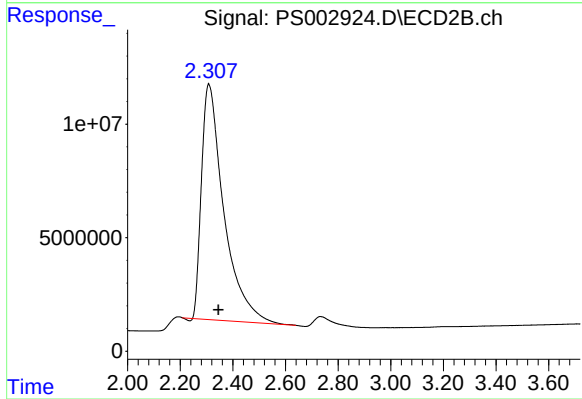


#1 Dalapon

R.T.: 2.308 min
Delta R.T.: -0.038 min
Response: 611187866
Conc: 1309.64 ng/ml

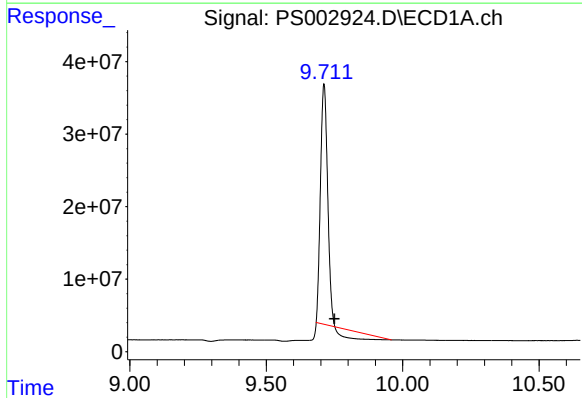


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.712 min
Delta R.T.: -0.038 min
Response: 509870808
Conc: 976.07 ng/ml

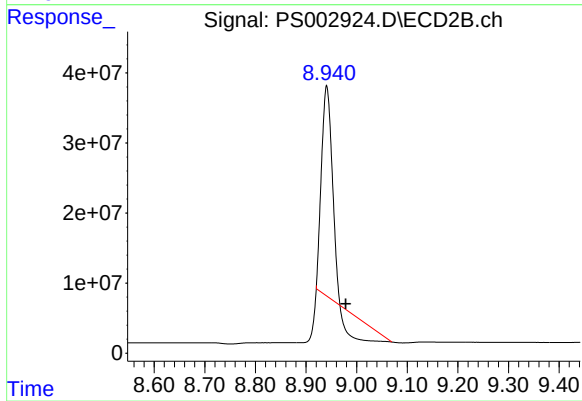

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.941 min
Delta R.T.: -0.038 min
Response: 318186276
Conc: 647.97 ng/ml

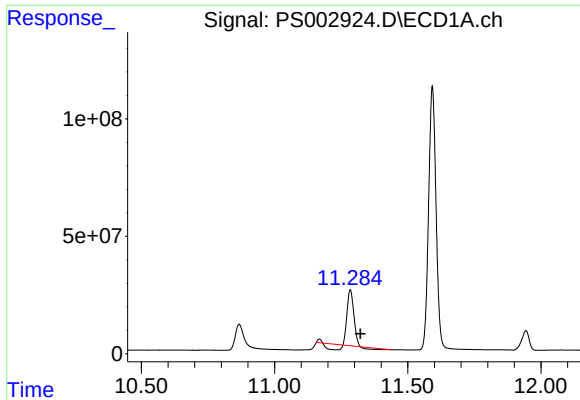

#4 2,4-DCAA


R.T.: 11.284 min
Delta R.T.: -0.038 min
Response: 309148184
Conc: 924.42 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC1500

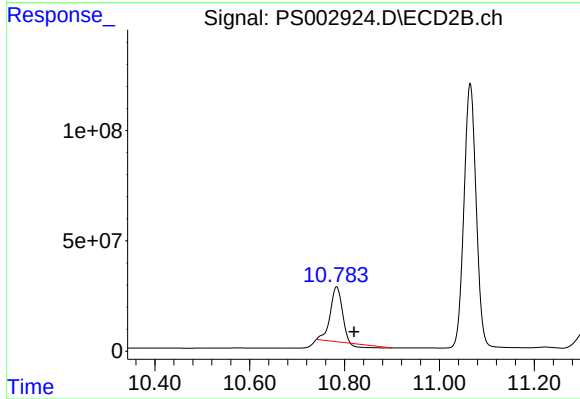


#4 2,4-DCAA

R.T.: 10.783 min
Delta R.T.: -0.037 min
Response: 392728349
Conc: 1011.13 ng/ml

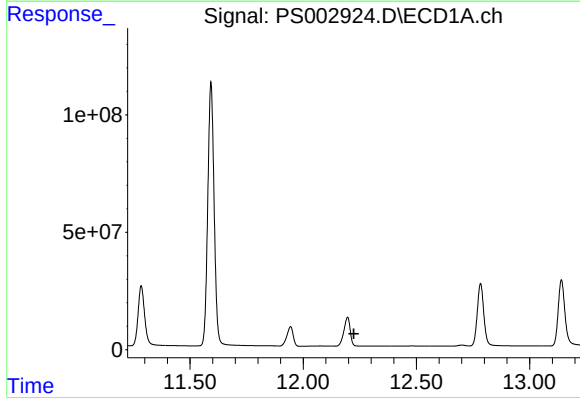


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.224 min
Response: 0
Conc: N.D.

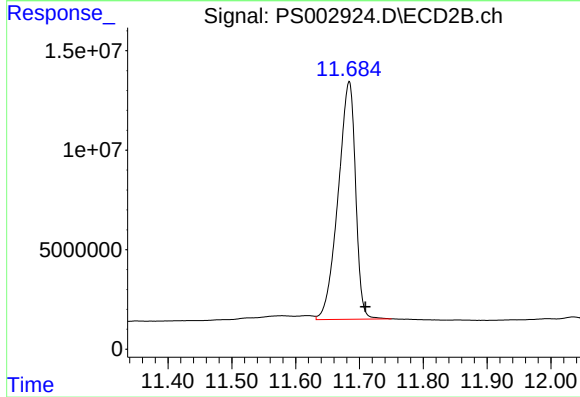

#7 MCPA


R.T.: 11.684 min
Delta R.T.: -0.026 min
Response: 226983261
Conc: 149.14 ug/ml

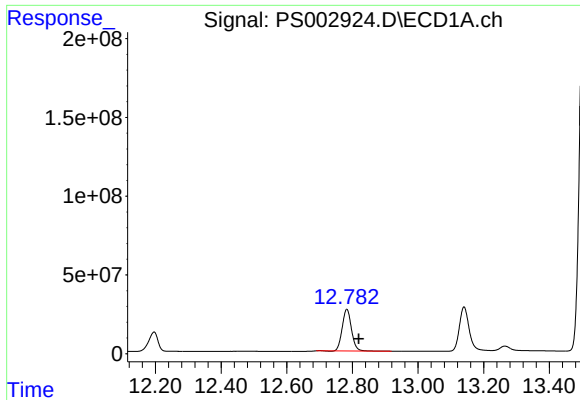

#8 DICHLORPROP


R.T.: 12.783 min
Delta R.T.: -0.037 min
Response: 517903237
Conc: 1408.22 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC1500

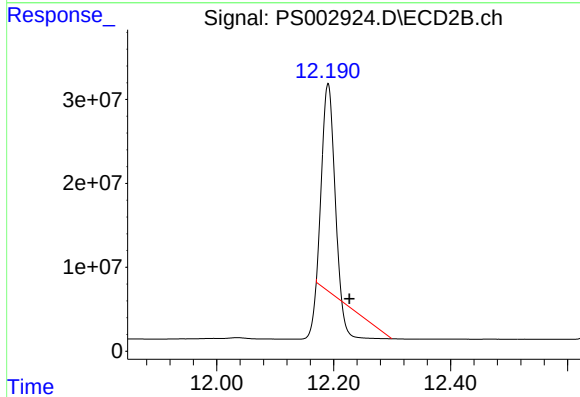


#8 DICHLORPROP

R.T.: 12.190 min
Delta R.T.: -0.037 min
Response: 249979839
Conc: 670.74 ng/ml

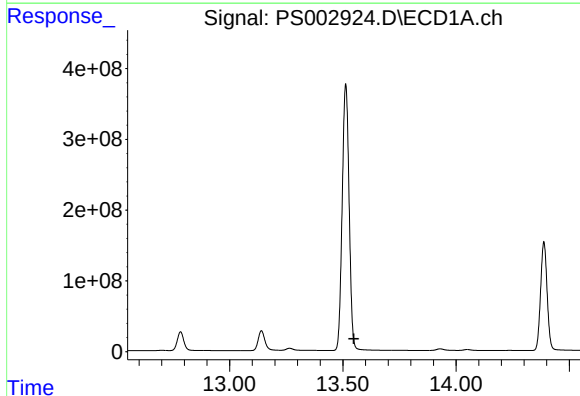


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.548 min
Response: 0
Conc: N.D.

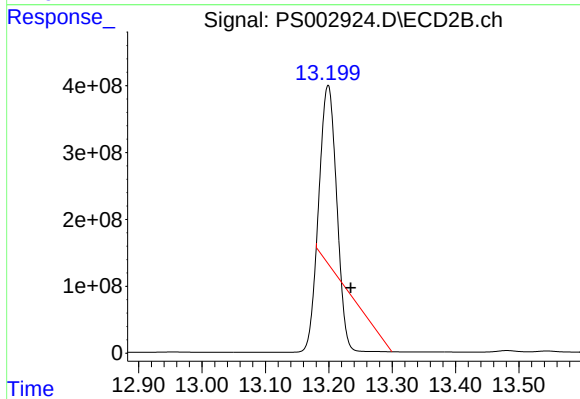

#10 Pentachlorophenol


R.T.: 13.199 min
Delta R.T.: -0.036 min
Response: 1573757698
Conc: 271.15 ng/ml

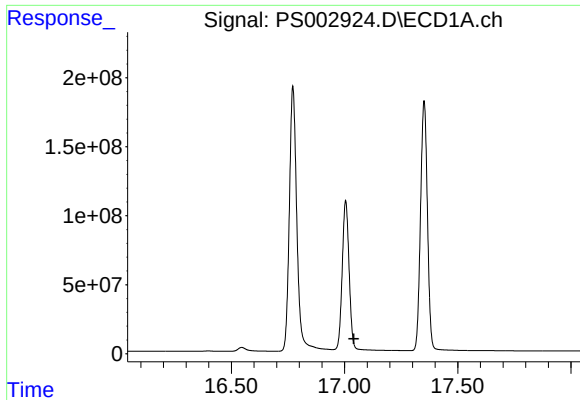

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 17.041 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HSTDICC1500

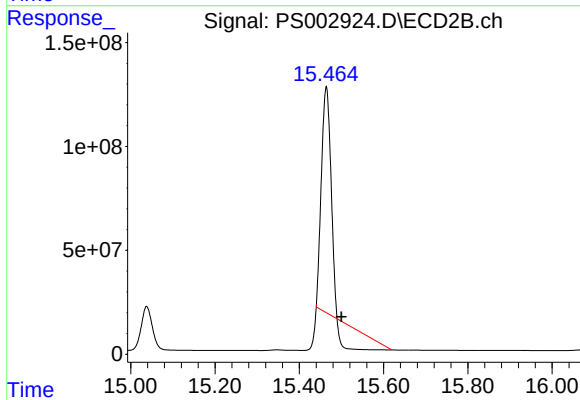


#14 DINOSEB

R.T.: 15.464 min
Delta R.T.: -0.036 min
Response: 1185202871
Conc: 710.17 ng/ml

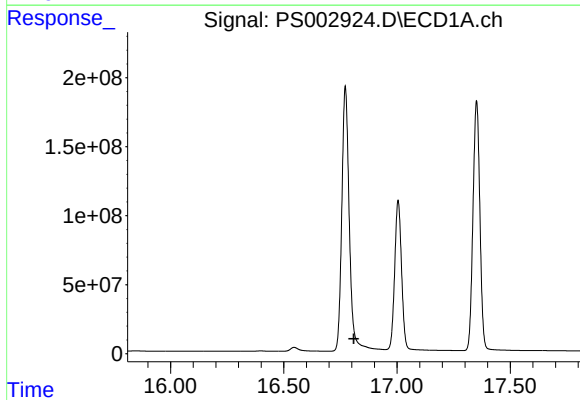


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.810 min
Response: 0
Conc: N.D.

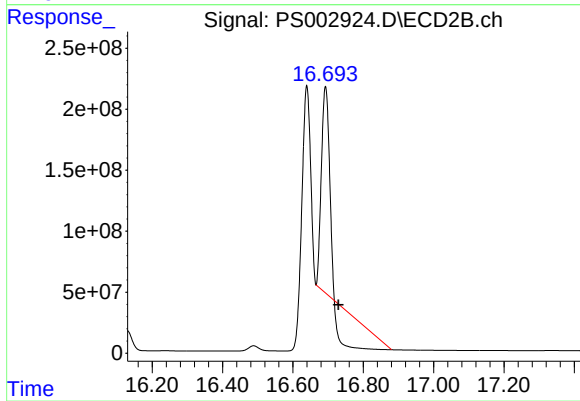

#15 Picloram


R.T.: 16.693 min
Delta R.T.: -0.036 min
Response: 1020655541
Conc: 339.38 ng/ml

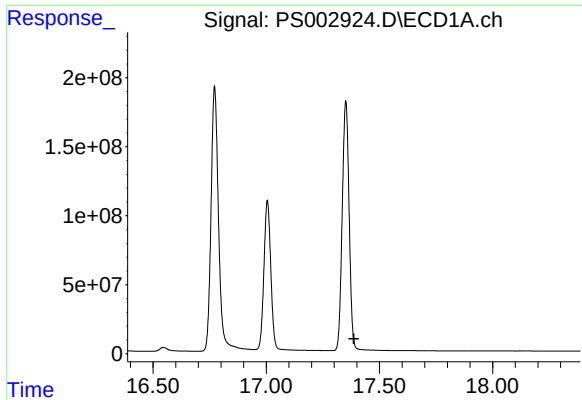

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.387 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HSTDICC1500

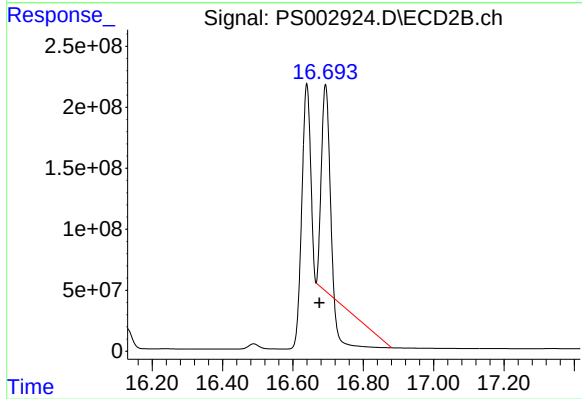

#16 DCPA

R.T.: 16.693 min
Delta R.T.: 0.017 min
Response: 102065541
Conc: 343.88 ng/ml