

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012219\
 Data File : PS002931.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jan 2019 17:44
 Operator : EI\SJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 141 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDCCC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 23 08:18:34 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012219.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 23 08:15:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.288	10.787	207.4E6	218.3E6	614.809	556.527
Target Compounds							
1) T	Dalapon	2.845	2.313	342.6E6	318.7E6	704.447	673.741
2) T	3,5-DICHL...	9.715	8.944	354.2E6	231.6E6	683.110	473.419 #
5) T	DICAMBA	0.000	11.068	0	138.0E6	N.D.	93.429 #
7) T	MCPA	0.000	11.677	0	119.0E6	N.D.	80.172 #
8) T	DICHLORPROP	12.786	12.194	275.3E6	172.4E6	740.974	458.558 #
10) T	Pentachlo...	0.000	13.201	0	1639.8E6	N.D.	285.410 #
11) T	2,4,5-TP ...	0.000	13.826	0	287.6E6	N.D.	130.271 #
12) T	2,4,5-T	14.787	14.389	991.8E6	19434107	485.774	11.211 #
14) T	DINOSEB	0.000	15.467	0	814.0E6	N.D.	488.262 #
15) T	Picloram	0.000	16.695	0	596.1E6	N.D.	202.152 #
16) T	DCPA	0.000	16.642	0	1362.1E6	N.D.	463.448 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012219\
Data File : PS002931.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jan 2019 17:44
Operator : EI\SJ
Sample : HSTDCCC750
Misc :
ALS Vial : 141 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 23 08:18:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012219.M
Quant Title : 8080.M
QLast Update : Wed Jan 23 08:15:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

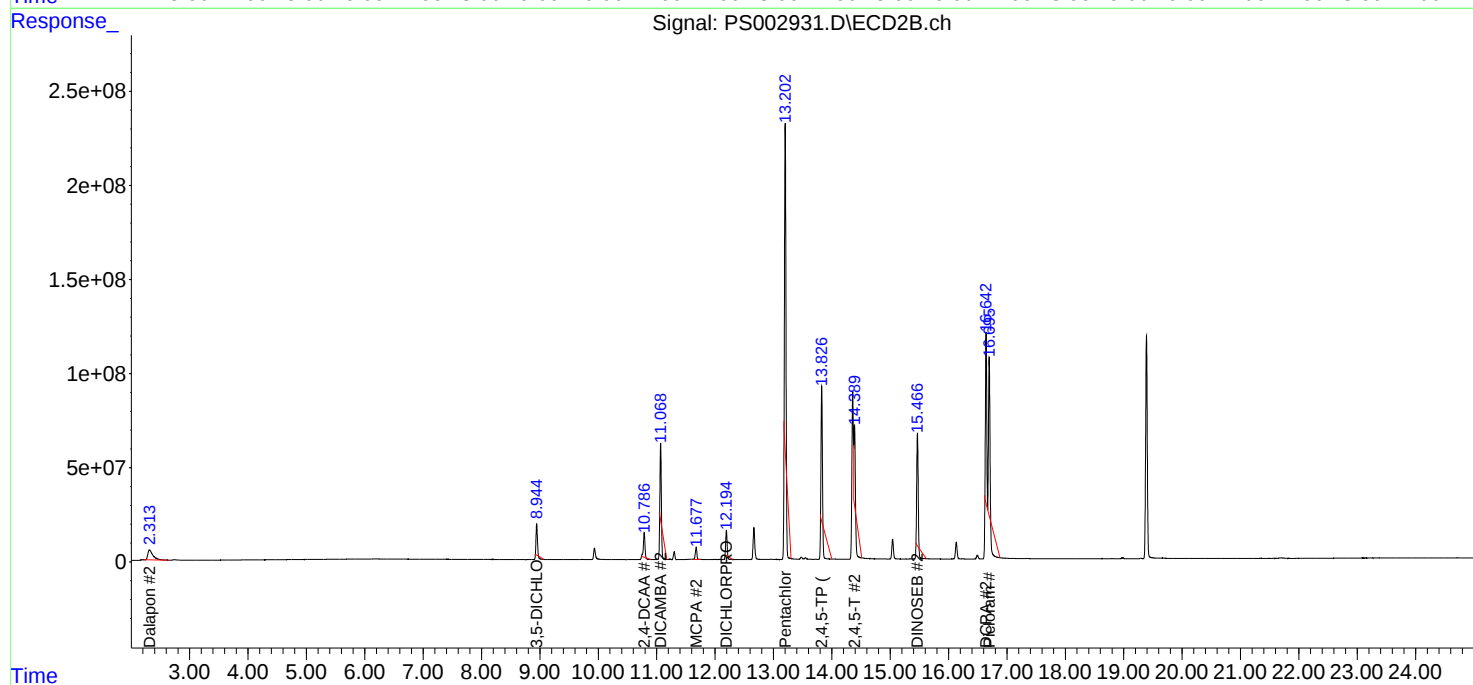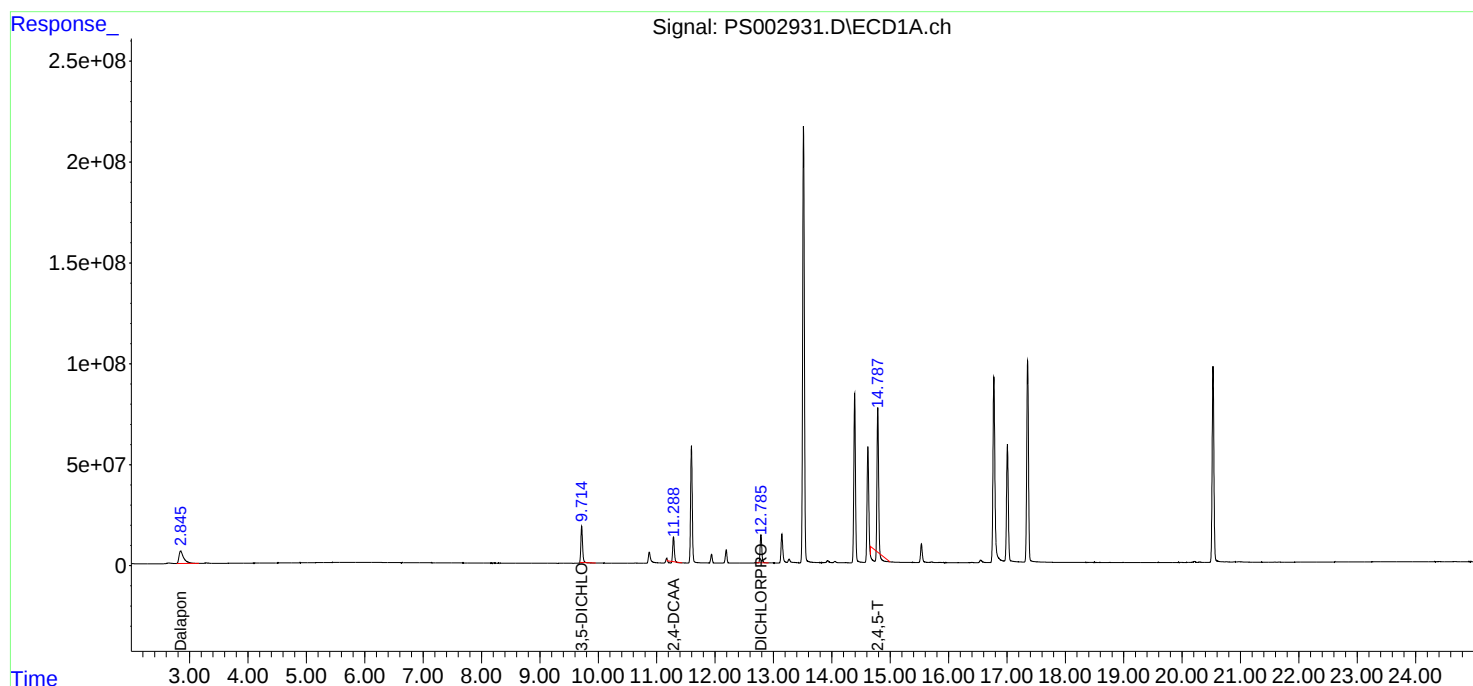


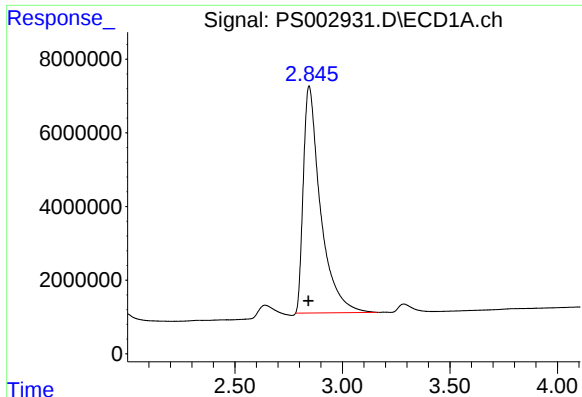

#1 Dalapon


R.T.: 2.845 min
Delta R.T.: 0.004 min
Response: 342605893
Conc: 704.45 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

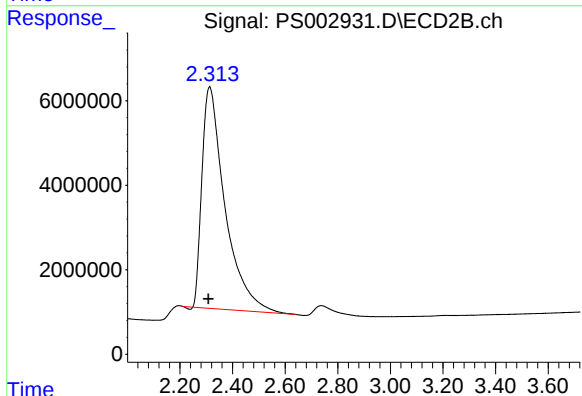


#1 Dalapon

R.T.: 2.313 min
Delta R.T.: 0.005 min
Response: 318694654
Conc: 673.74 ng/ml

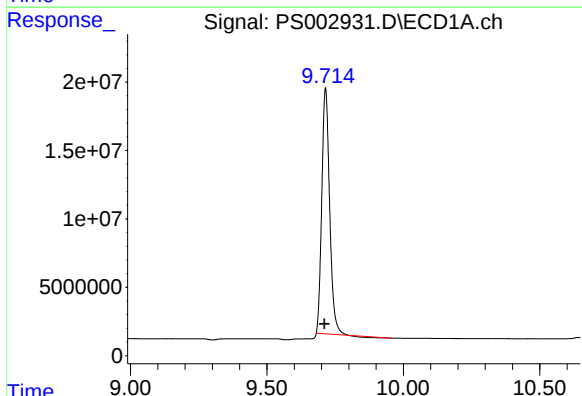


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.715 min
Delta R.T.: 0.004 min
Response: 354235347
Conc: 683.11 ng/ml

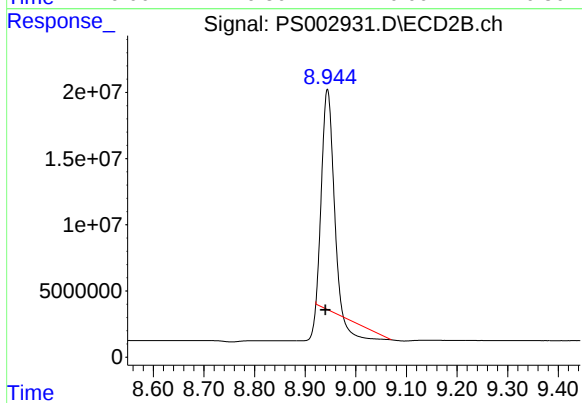

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.944 min
Delta R.T.: 0.004 min
Response: 231600393
Conc: 473.42 ng/ml

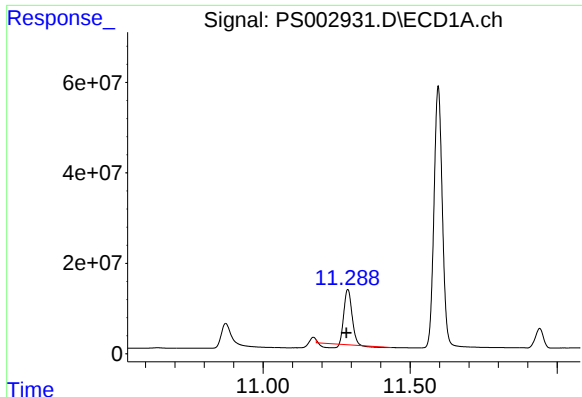

#4 2,4-DCAA


R.T.: 11.288 min
Delta R.T.: 0.004 min
Response: 207374239
Conc: 614.81 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

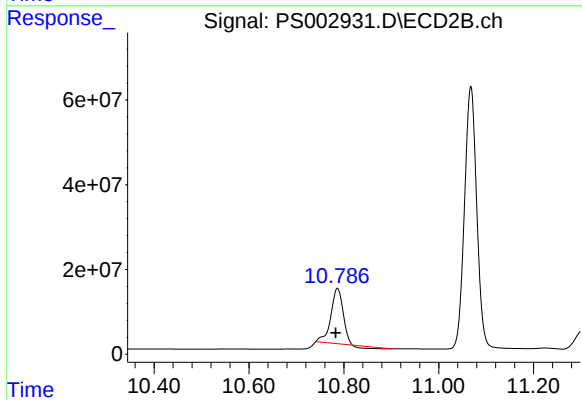


#4 2,4-DCAA

R.T.: 10.787 min
Delta R.T.: 0.004 min
Response: 218278009
Conc: 556.53 ng/ml

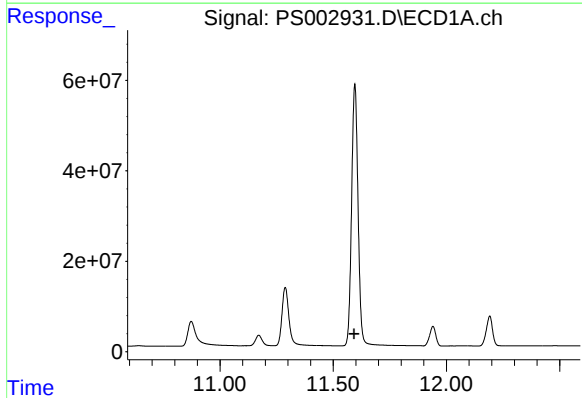


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.592 min
Response: 0
Conc: N.D.

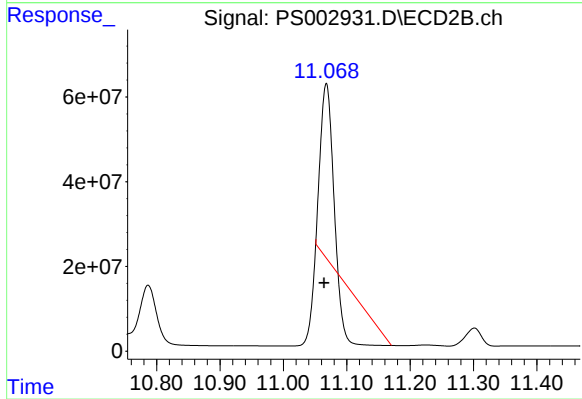

#5 DICAMBA


R.T.: 11.068 min
Delta R.T.: 0.003 min
Response: 137972629
Conc: 93.43 ng/ml

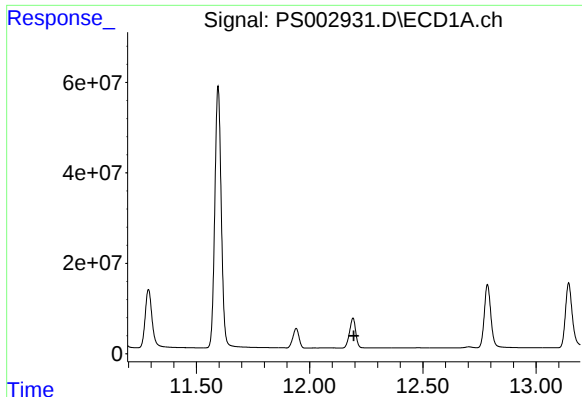

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.196 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

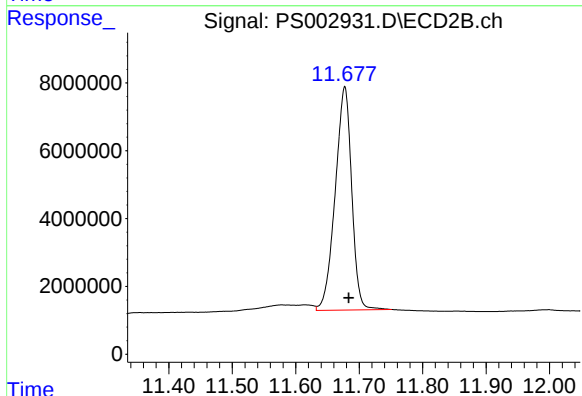


#7 MCPA

R.T.: 11.677 min
Delta R.T.: -0.006 min
Response: 119037615
Conc: 80.17 ug/ml

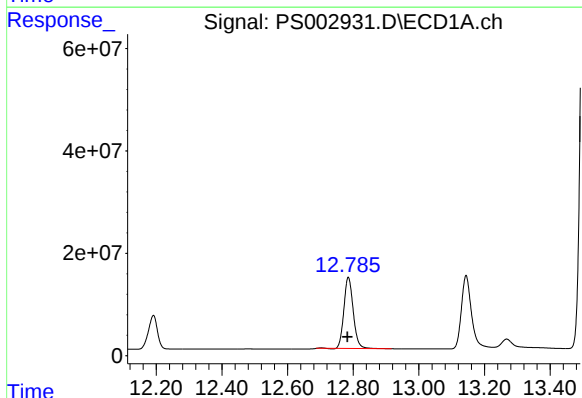


#8 DICHLORPROP

R.T.: 12.786 min
Delta R.T.: 0.003 min
Response: 275265147
Conc: 740.97 ng/ml

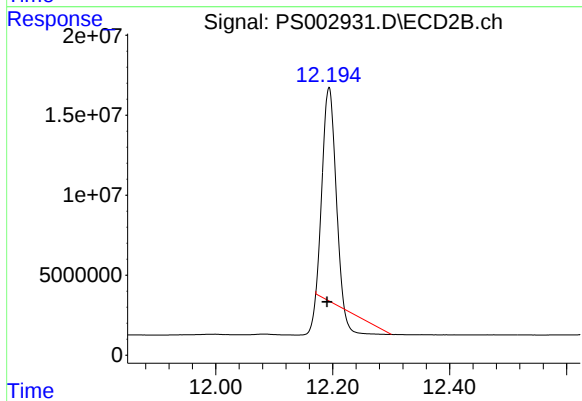

#8 DICHLORPROP


R.T.: 12.194 min
Delta R.T.: 0.003 min
Response: 172409941
Conc: 458.56 ng/ml

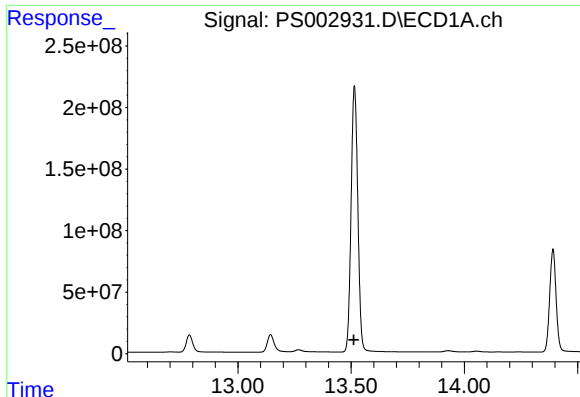

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.512 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

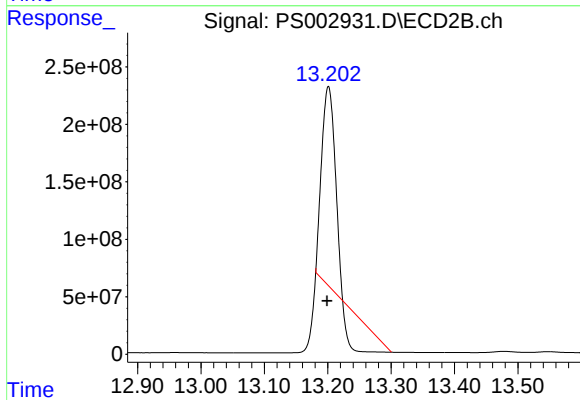


#10 Pentachlorophenol

R.T.: 13.201 min
Delta R.T.: 0.002 min
Response: 1639794061
Conc: 285.41 ng/ml

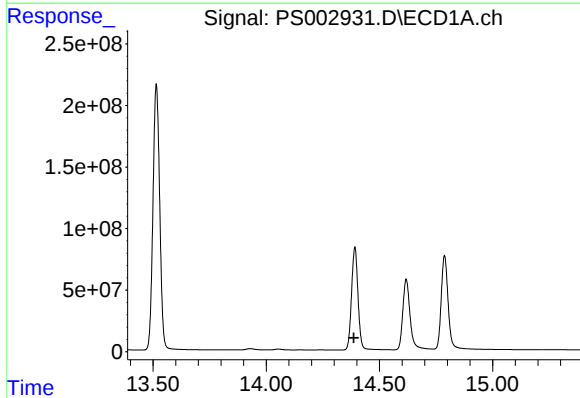


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.387 min
Response: 0
Conc: N.D.

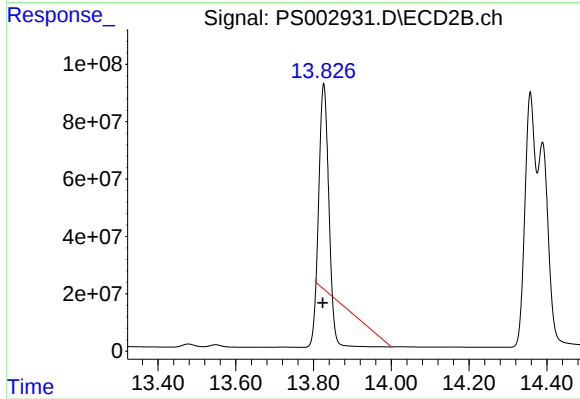

#11 2,4,5-TP (SILVEX)


R.T.: 13.826 min
Delta R.T.: 0.003 min
Response: 287565886
Conc: 130.27 ng/ml

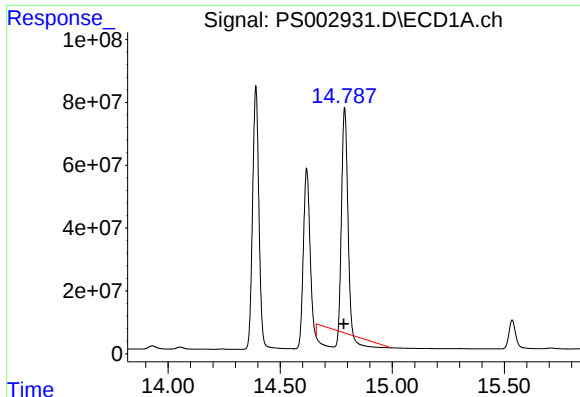

#12 2,4,5-T


R.T.: 14.787 min
Delta R.T.: 0.003 min
Response: 991793126
Conc: 485.77 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

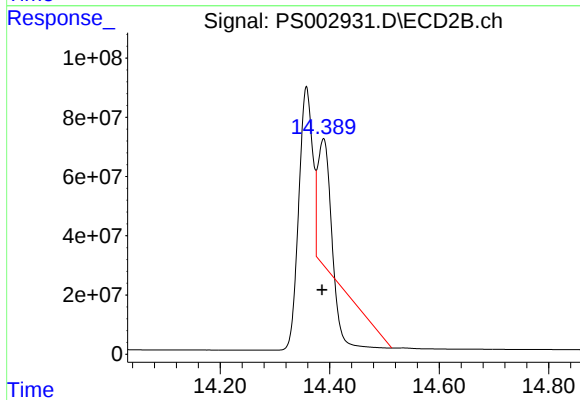


#12 2,4,5-T

R.T.: 14.389 min
Delta R.T.: 0.003 min
Response: 19434107
Conc: 11.21 ng/ml

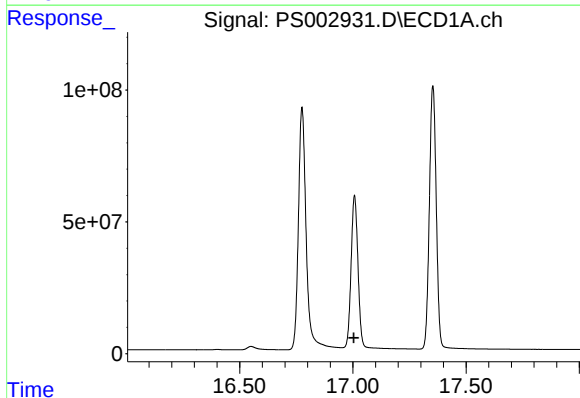


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 17.004 min
Response: 0
Conc: N.D.

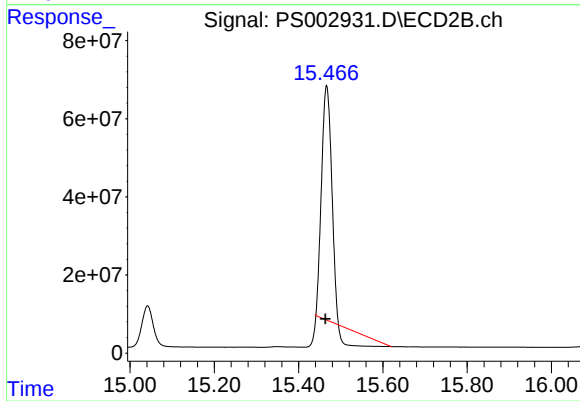

#14 DINOSEB


R.T.: 15.467 min
Delta R.T.: 0.003 min
Response: 814030538
Conc: 488.26 ng/ml

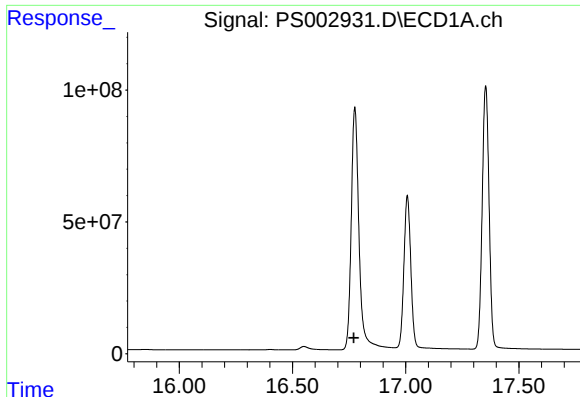

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 16.771 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

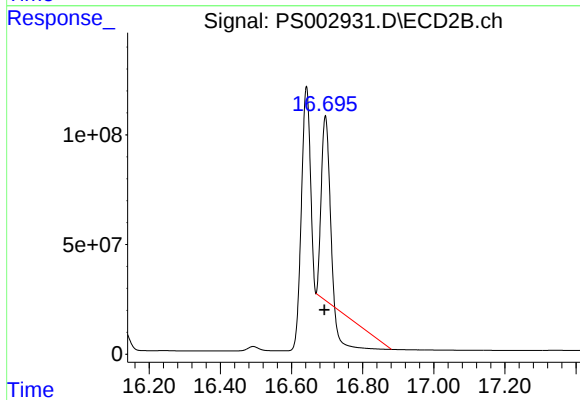


#15 Picloram

R.T.: 16.695 min
Delta R.T.: 0.003 min
Response: 596050194
Conc: 202.15 ng/ml

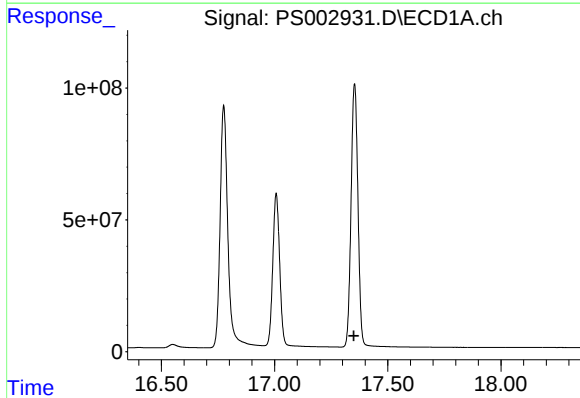

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.351 min
Response: 0
Conc: N.D.

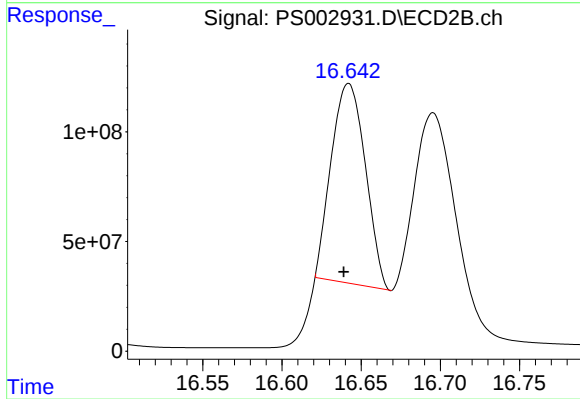

#16 DCPA

R.T.: 16.642 min
Delta R.T.: 0.003 min
Response: 1362139857
Conc: 463.45 ng/ml