

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012219\
 Data File : PS002932.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jan 2019 18:15
 Operator : EI\SJ
 Sample : K1009-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CL-01-011819-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 23 08:18:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012219.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 23 08:15:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.287	10.786	180.2E6	172.2E6	534.361	439.044
Target Compounds							
1) T	Dalapon	2.802	2.290	7523692	78419414	15.470	165.784 #
2) T	3,5-DICHL...	0.000	8.952	0	6412024	N.D.	13.107 #
5) T	DICAMBA	0.000	11.027	0	2801644	N.D.	1.897 #
6) T	MCP	0.000	11.346	0	27219634	N.D.	28.663 #
7) T	MCPA	12.145	11.733	14002540	6500514	8.835	4.378 #
10) T	Pentachlo...	13.515	13.200	3454849	2658191	0.603	0.463
12) T	2,4,5-T	0.000	14.395	0	5018120	N.D.	2.895 #
13) T	2,4-DB	0.000	14.972	0	3207752	N.D.	12.489 #
14) T	DINOSEB	0.000	15.495	0	7846013	N.D.	4.706 #
15) T	Picloram	0.000	16.699	0	41005345	N.D.	13.907 #
16) T	DCPA	0.000	16.699	0	41005345	N.D.	13.951 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012219\
Data File : PS002932.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jan 2019 18:15
Operator : EI\SJ
Sample : K1009-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
CL-01-011819-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 23 08:18:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012219.M
Quant Title : 8080.M
QLast Update : Wed Jan 23 08:15:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

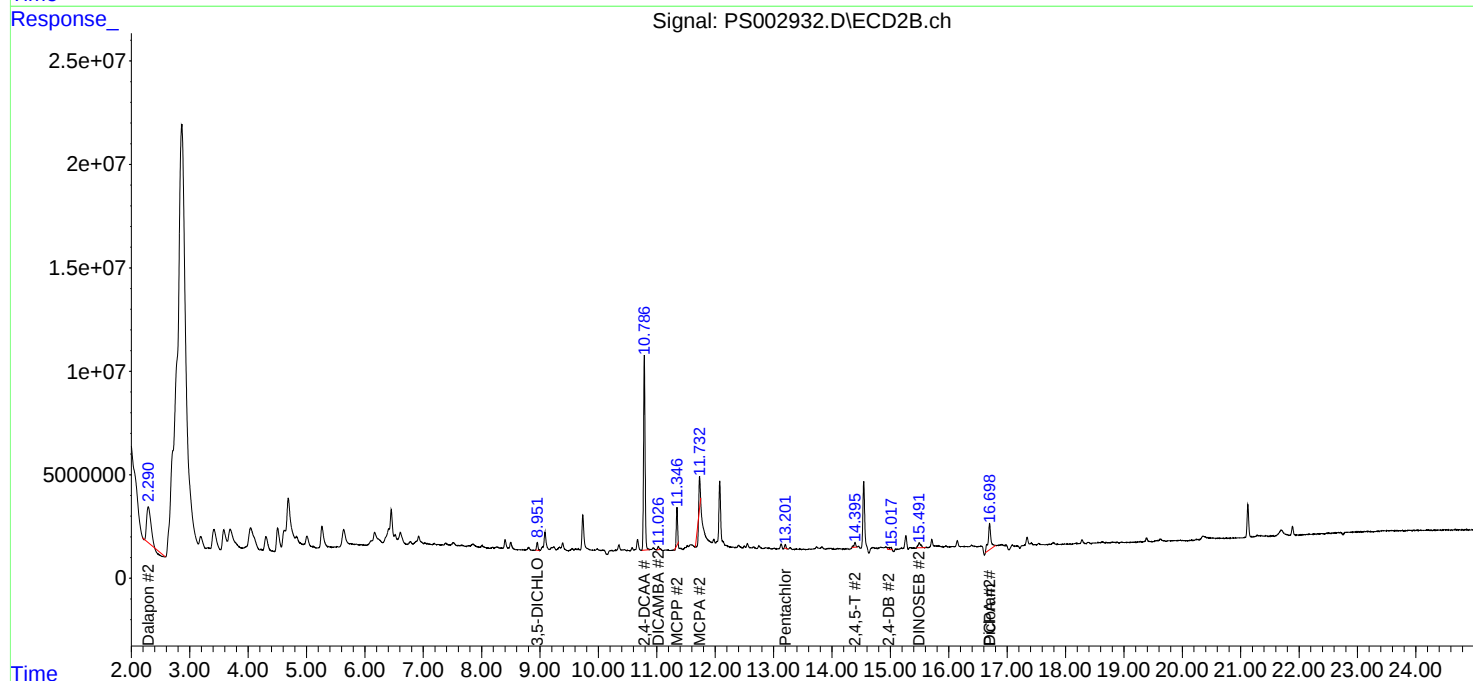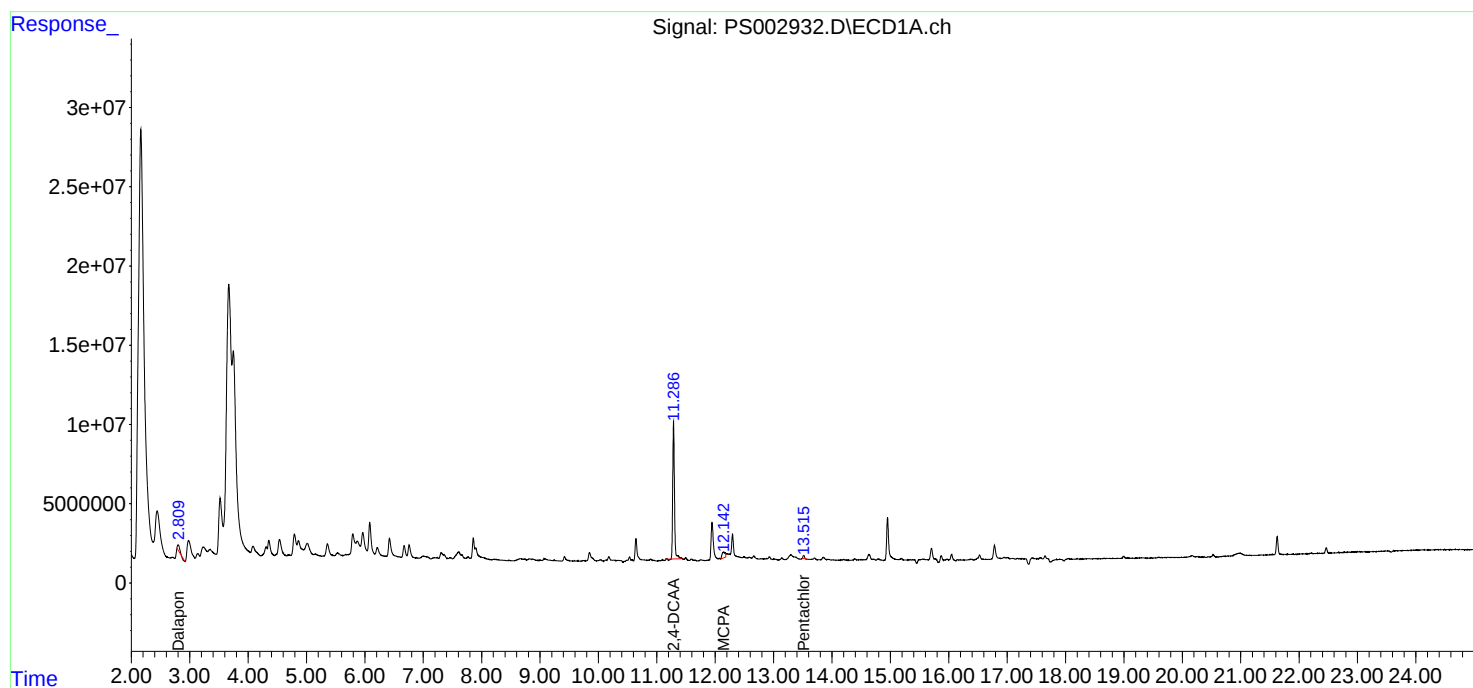


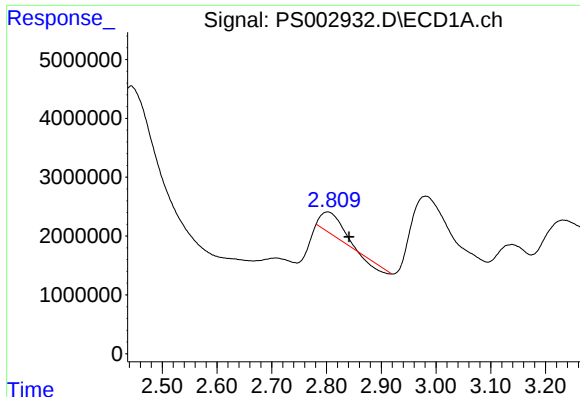

#1 Dalapon


R.T.: 2.802 min
Delta R.T.: -0.039 min
Response: 7523692
Conc: 15.47 ng/ml

Instrument :
ECD_S
ClientSampleId :
CL-01-011819-A

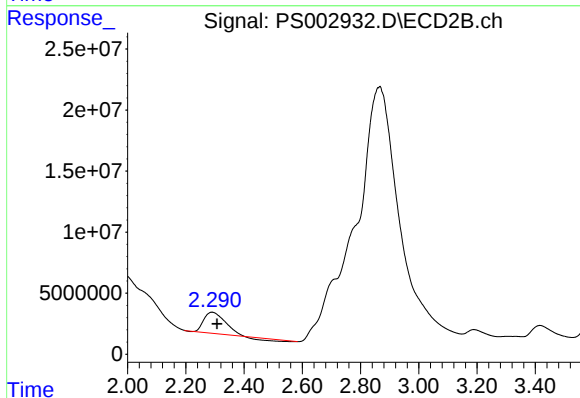


#1 Dalapon

R.T.: 2.290 min
Delta R.T.: -0.018 min
Response: 78419414
Conc: 165.78 ng/ml

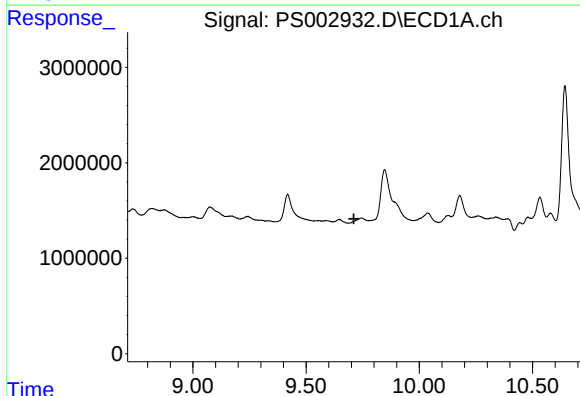


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.711 min
Response: 0
Conc: N.D.

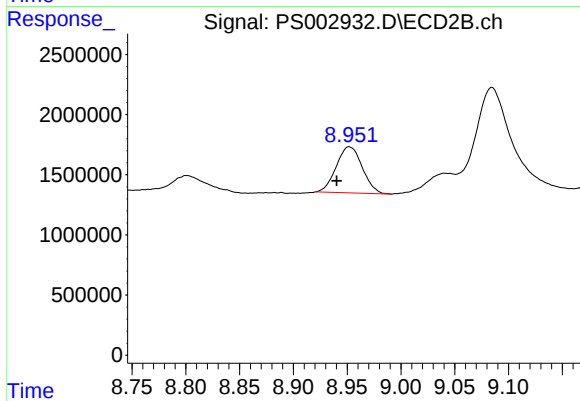

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.952 min
Delta R.T.: 0.012 min
Response: 6412024
Conc: 13.11 ng/ml

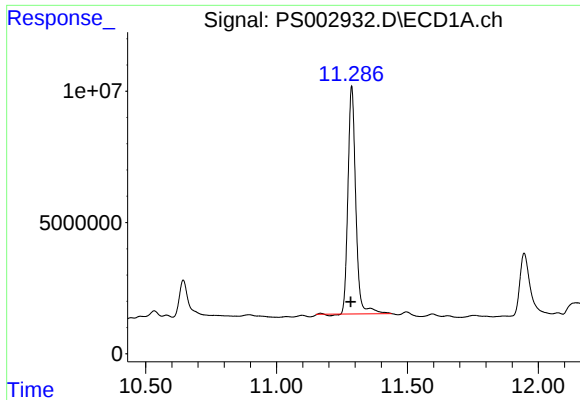

#4 2,4-DCAA


R.T.: 11.287 min
Delta R.T.: 0.003 min
Response: 180239229
Conc: 534.36 ng/ml

Instrument :
ECD_S
ClientSampleId :
CL-01-011819-A

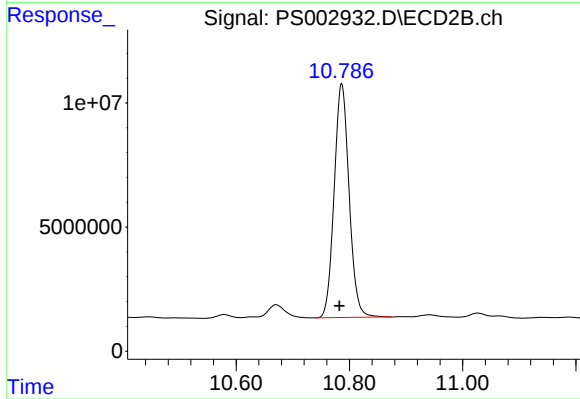


#4 2,4-DCAA

R.T.: 10.786 min
Delta R.T.: 0.004 min
Response: 172199558
Conc: 439.04 ng/ml

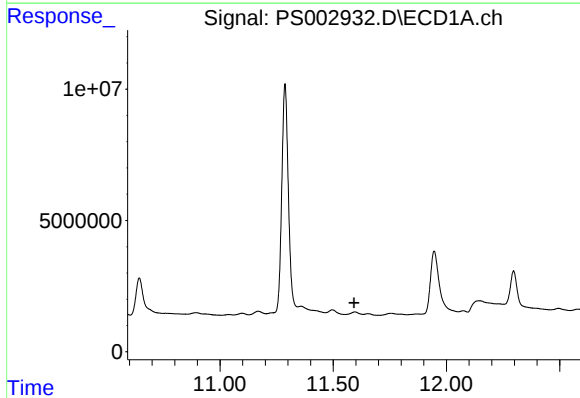


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.592 min
Response: 0
Conc: N.D.

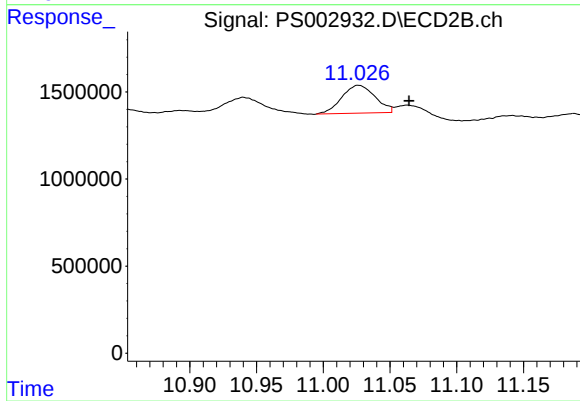

#5 DICAMBA


R.T.: 11.027 min
Delta R.T.: -0.038 min
Response: 2801644
Conc: 1.90 ng/ml

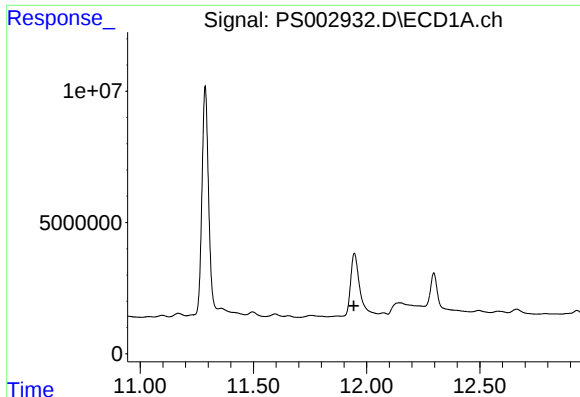

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 11.944 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-01-011819-A

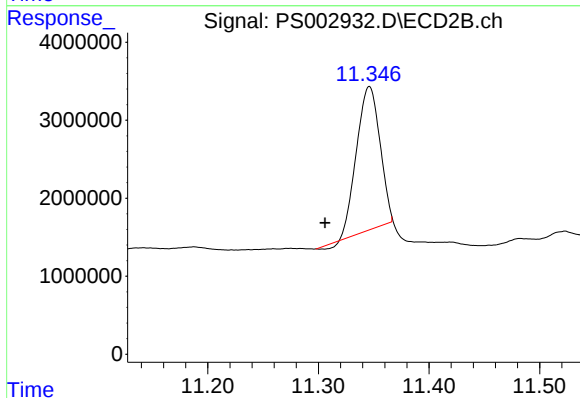


#6 MCPP

R.T.: 11.346 min
Delta R.T.: 0.040 min
Response: 27219634
Conc: 28.66 ug/ml

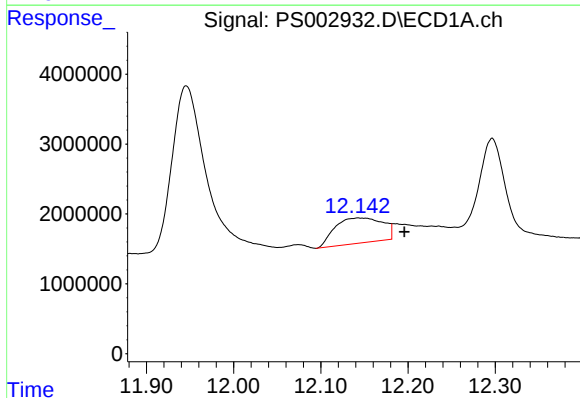


#7 MCPA

R.T.: 12.145 min
Delta R.T.: -0.051 min
Response: 14002540
Conc: 8.84 ug/ml

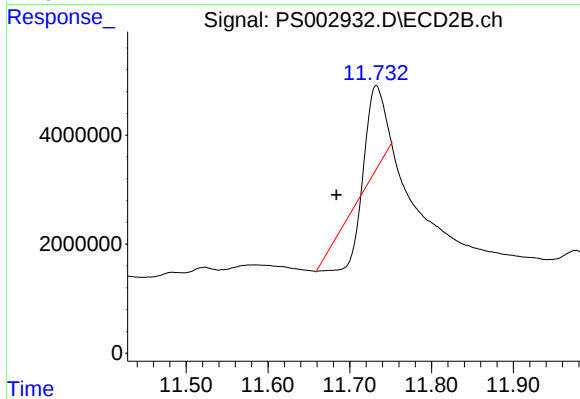

#7 MCPA


R.T.: 11.733 min
Delta R.T.: 0.049 min
Response: 6500514
Conc: 4.38 ug/ml

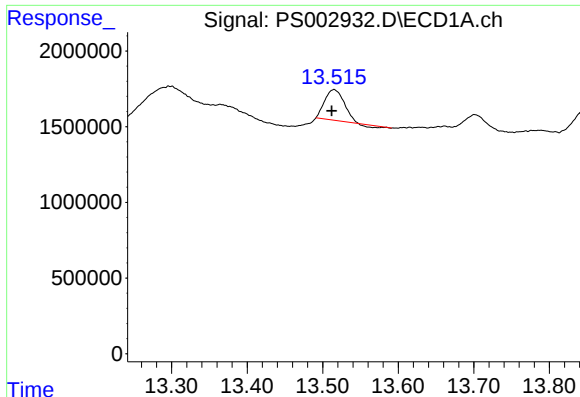

#10 Pentachlorophenol


R.T.: 13.515 min
Delta R.T.: 0.003 min
Response: 3454849
Conc: 0.60 ng/ml

Instrument :
ECD_S
ClientSampleId :
CL-01-011819-A

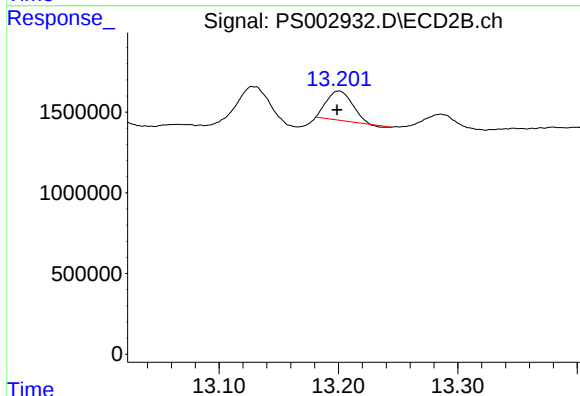


#10 Pentachlorophenol

R.T.: 13.200 min
Delta R.T.: 0.002 min
Response: 2658191
Conc: 0.46 ng/ml

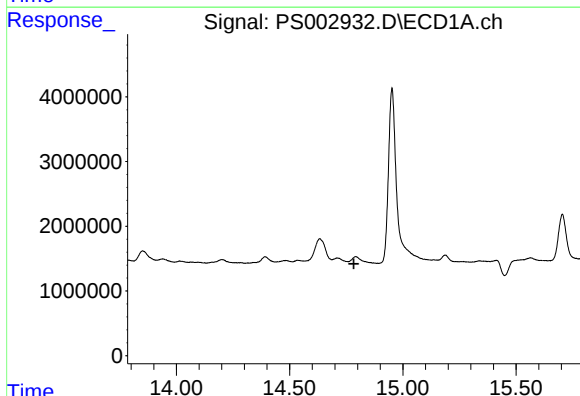


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 14.784 min
Response: 0
Conc: N.D.

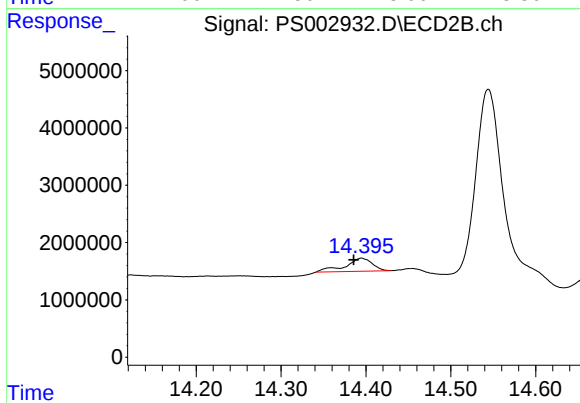

#12 2,4,5-T


R.T.: 14.395 min
Delta R.T.: 0.009 min
Response: 5018120
Conc: 2.89 ng/ml

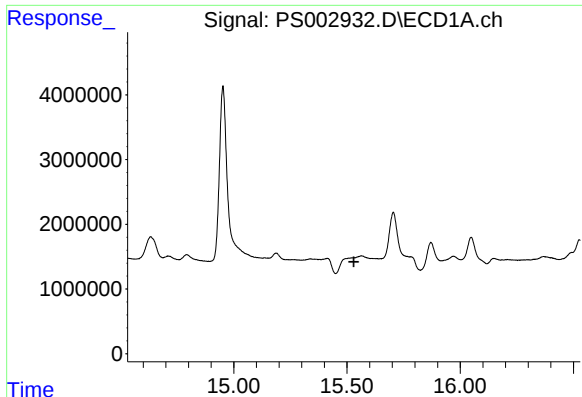

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.531 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-01-011819-A

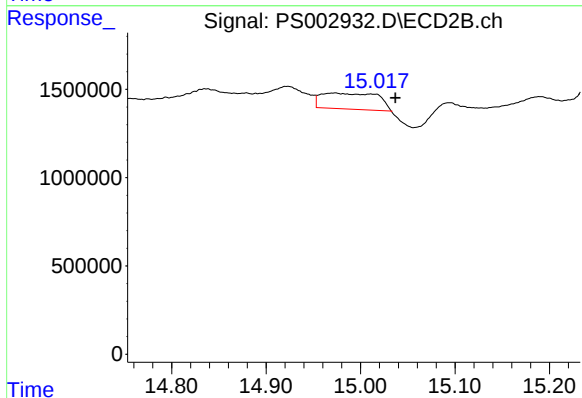


#13 2,4-DB

R.T.: 14.972 min
Delta R.T.: -0.065 min
Response: 3207752
Conc: 12.49 ng/ml

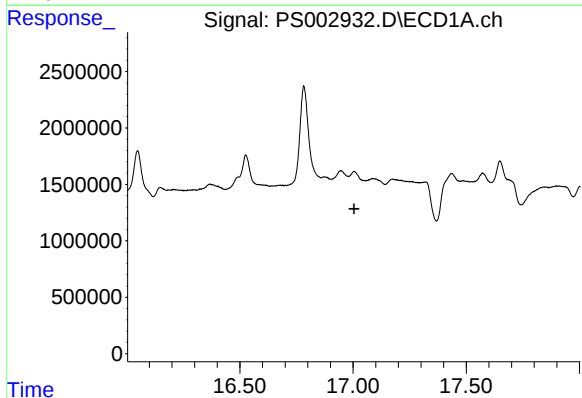


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 17.004 min
Response: 0
Conc: N.D.

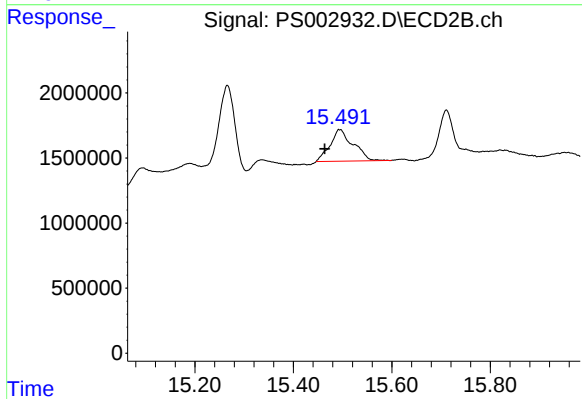

#14 DINOSEB


R.T.: 15.495 min
Delta R.T.: 0.031 min
Response: 7846013
Conc: 4.71 ng/ml

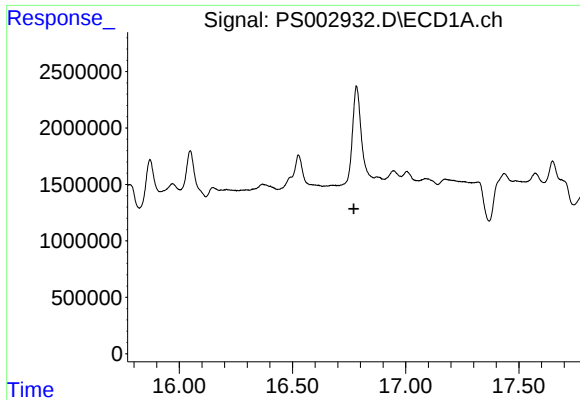

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.771 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-01-011819-A

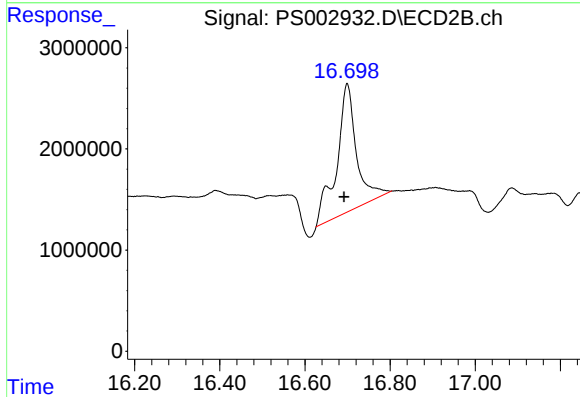


#15 Picloram

R.T.: 16.699 min
Delta R.T.: 0.007 min
Response: 41005345
Conc: 13.91 ng/ml

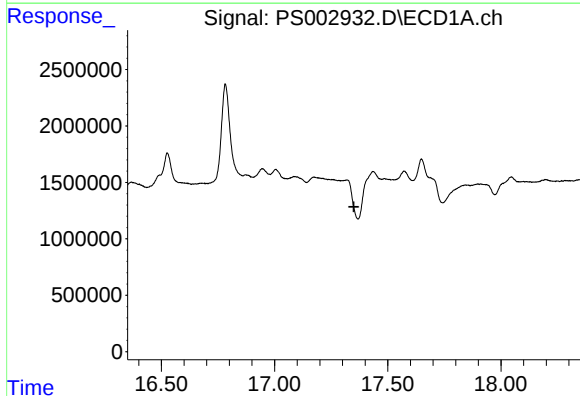

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.351 min
Response: 0
Conc: N.D.

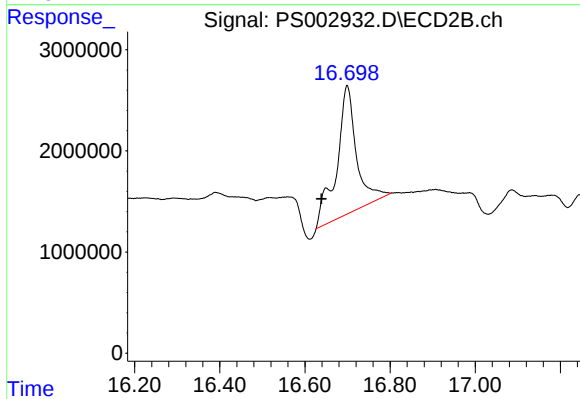

#16 DCPA

R.T.: 16.699 min
Delta R.T.: 0.061 min
Response: 41005345
Conc: 13.95 ng/ml