

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012219\
 Data File : PS002934.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jan 2019 19:17
 Operator : EI\SJ
 Sample : K1009-06
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CL-01-011819-C

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 23 08:19:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012219.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 23 08:15:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.283	10.782	138.3E6	134.3E6	409.952	342.509
Target Compounds							
1) T	Dalapon	0.000	2.284	0 63537660	N.D.	134.323	#
2) T	3,5-DICHL...	0.000	8.947	0 5090444	N.D.	10.405	#
5) T	DICAMBA	0.000	11.023	0 2720783	N.D.	1.842	#
7) T	MCPA	0.000	11.728	0 29740400	N.D.	20.030	#
13) T	2,4-DB	0.000	15.008	0 1820262	N.D.	7.087	#
14) T	DINOSEB	0.000	15.491	0 7119037	N.D.	4.270	#
15) T	Picloram	0.000	16.704	0 16615799	N.D.	5.635	#
16) T	DCPA	0.000	16.704	0 16615799	N.D.	5.653	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012219\
Data File : PS002934.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jan 2019 19:17
Operator : EI\SJ
Sample : K1009-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
CL-01-011819-C

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 23 08:19:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012219.M
Quant Title : 8080.M
QLast Update : Wed Jan 23 08:15:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

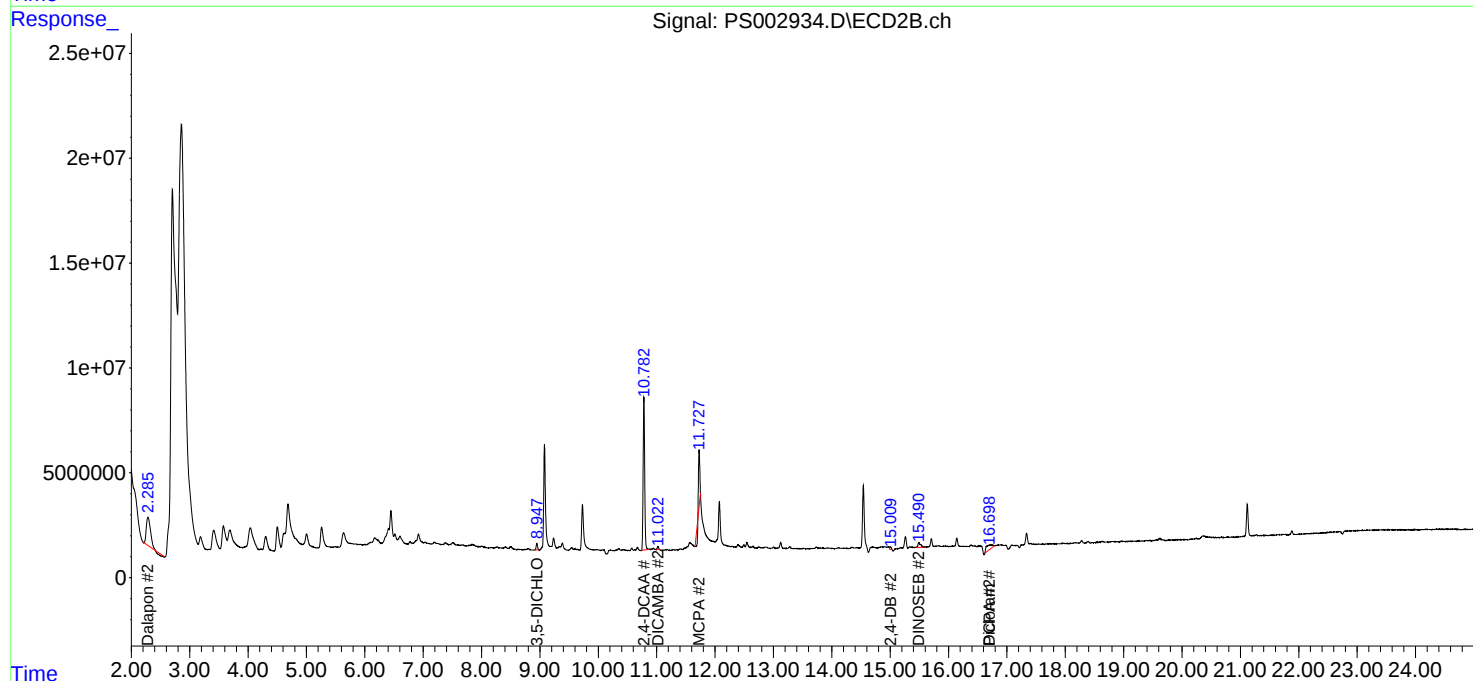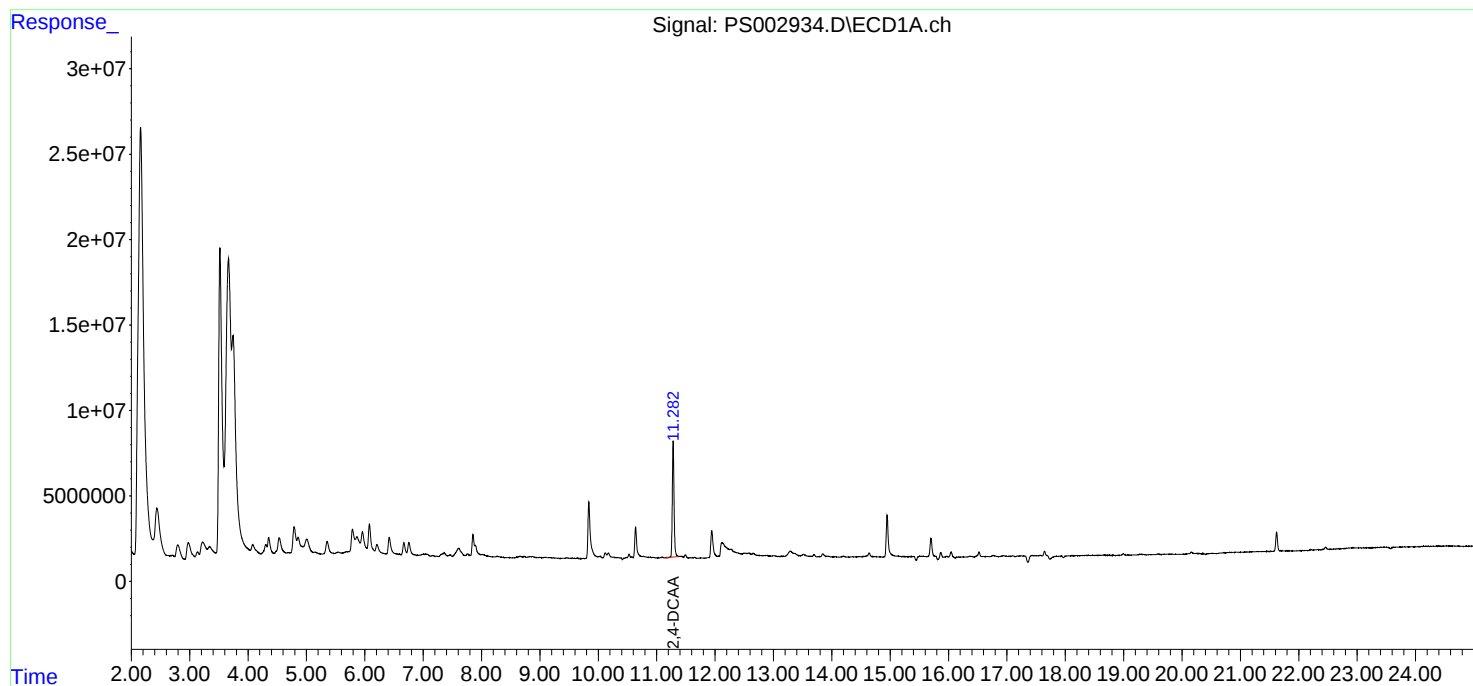


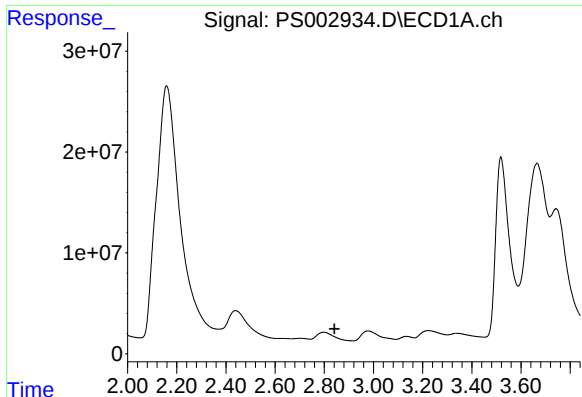

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 2.841 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-01-011819-C

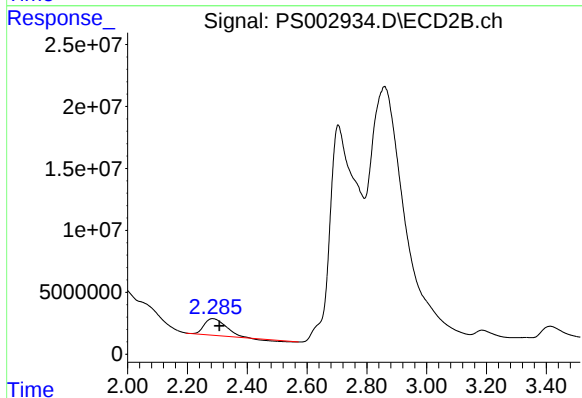


#1 Dalapon

R.T.: 2.284 min
Delta R.T.: -0.024 min
Response: 63537660
Conc: 134.32 ng/ml

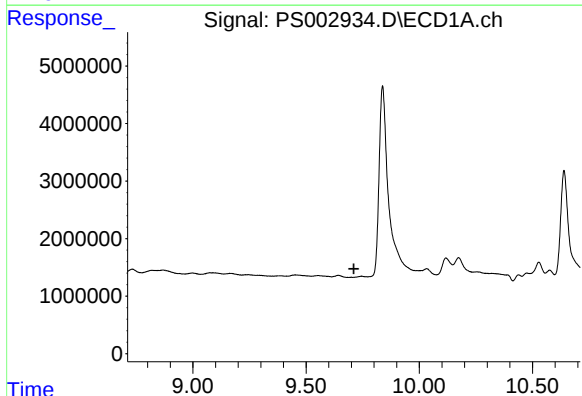


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.711 min
Response: 0
Conc: N.D.

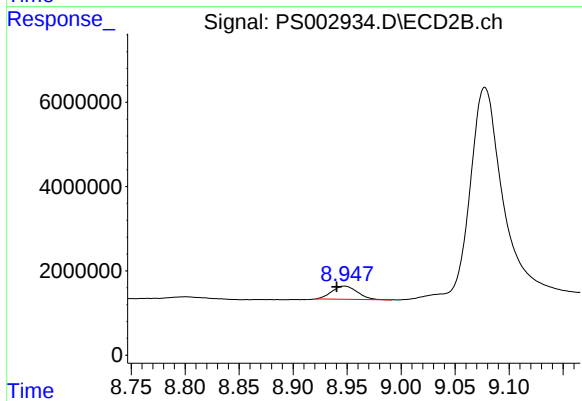

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.947 min
Delta R.T.: 0.007 min
Response: 5090444
Conc: 10.41 ng/ml

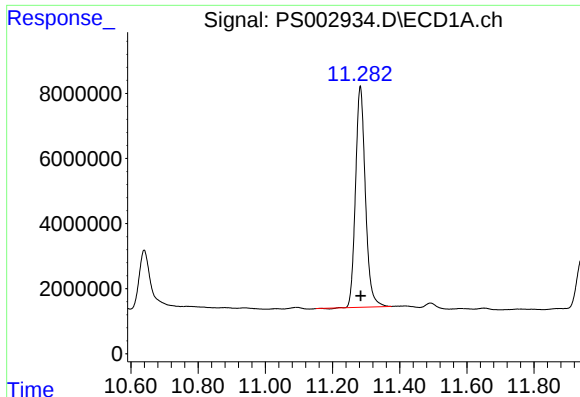

#4 2,4-DCAA


R.T.: 11.283 min
Delta R.T.: 0.000 min
Response: 138276500
Conc: 409.95 ng/ml

Instrument :
ECD_S
ClientSampleId :
CL-01-011819-C

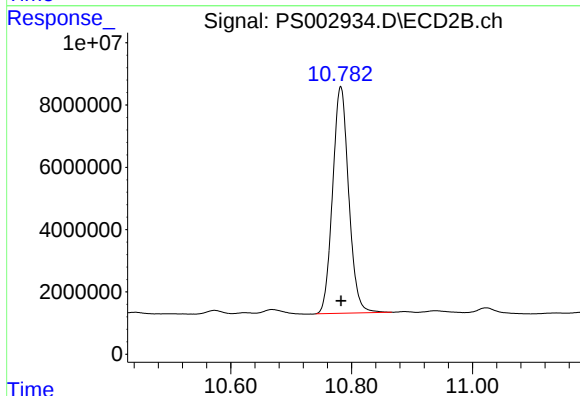


#4 2,4-DCAA

R.T.: 10.782 min
Delta R.T.: 0.000 min
Response: 134337236
Conc: 342.51 ng/ml

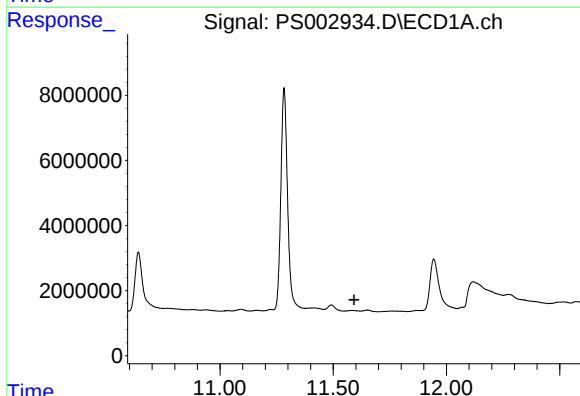


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.592 min
Response: 0
Conc: N.D.

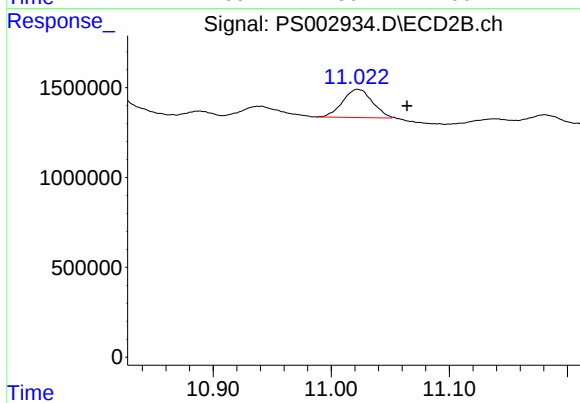

#5 DICAMBA


R.T.: 11.023 min
Delta R.T.: -0.042 min
Response: 2720783
Conc: 1.84 ng/ml

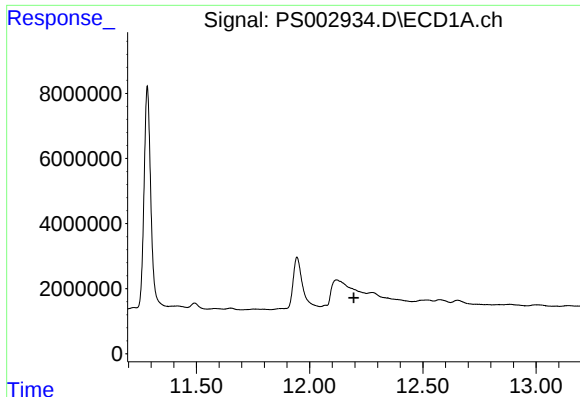

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.196 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-01-011819-C

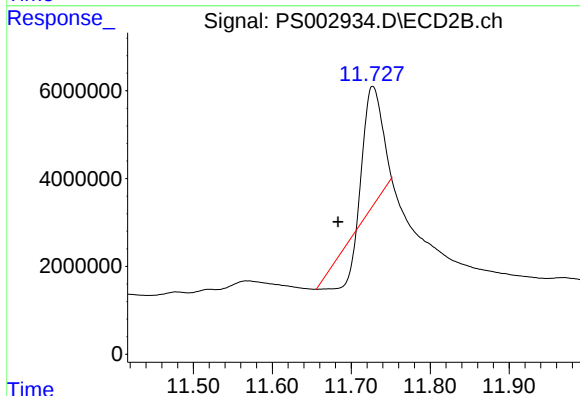


#7 MCPA

R.T.: 11.728 min
Delta R.T.: 0.044 min
Response: 29740400
Conc: 20.03 ug/ml

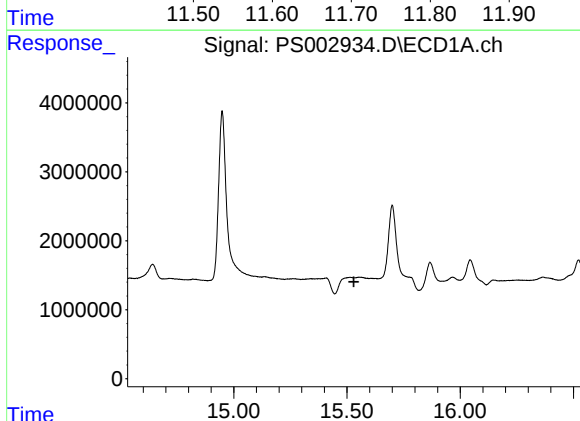


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.531 min
Response: 0
Conc: N.D.

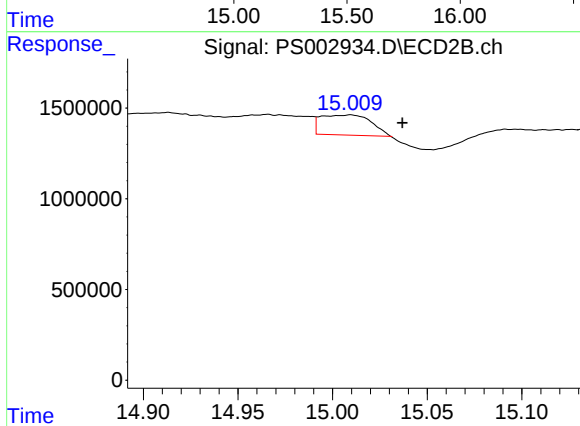

#13 2,4-DB


R.T.: 15.008 min
Delta R.T.: -0.029 min
Response: 1820262
Conc: 7.09 ng/ml

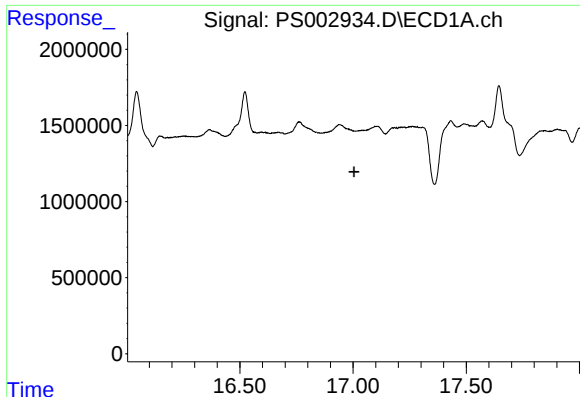

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.004 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-01-011819-C

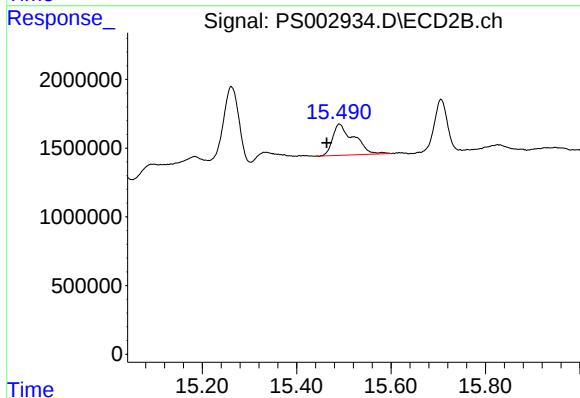


#14 DINOSEB

R.T.: 15.491 min
Delta R.T.: 0.027 min
Response: 7119037
Conc: 4.27 ng/ml

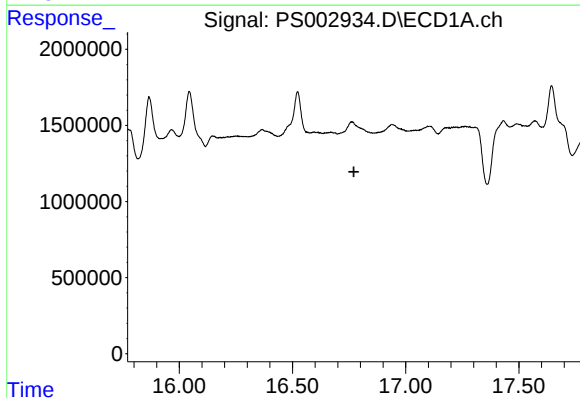


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.771 min
Response: 0
Conc: N.D.

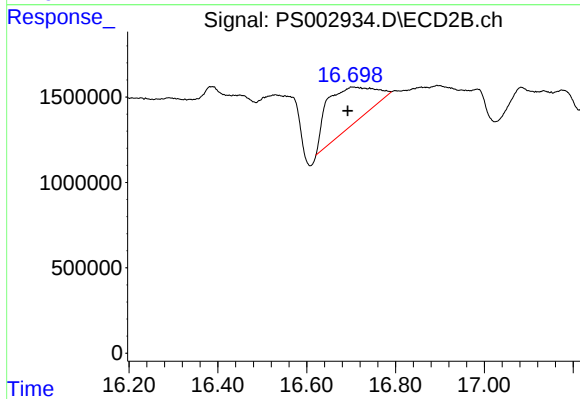

#15 Picloram


R.T.: 16.704 min
Delta R.T.: 0.011 min
Response: 16615799
Conc: 5.64 ng/ml

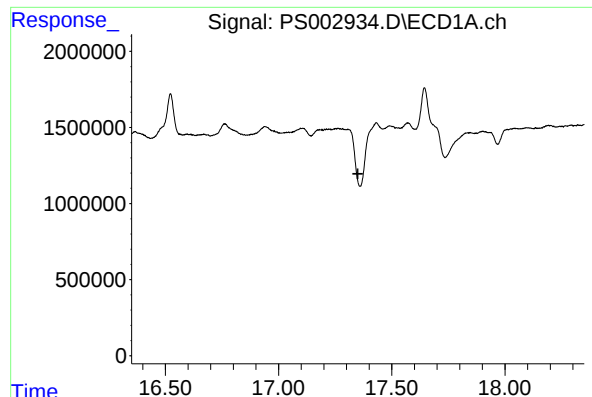

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.351 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-01-011819-C

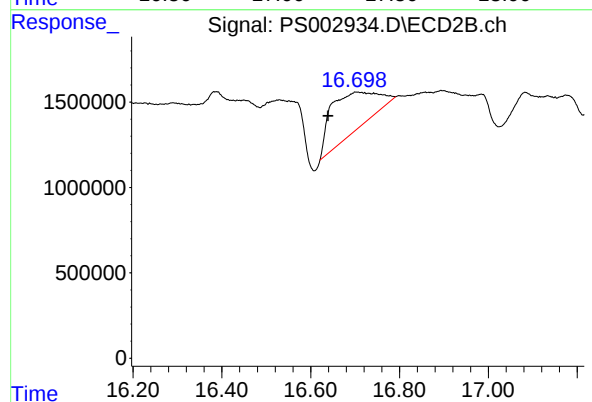

#16 DCPA

R.T.: 16.704 min
Delta R.T.: 0.065 min
Response: 16615799
Conc: 5.65 ng/ml