

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012219\
 Data File : PS002938.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jan 2019 21:21
 Operator : EI\SJ
 Sample : K1013-08
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PL-01-011819-D

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 23 08:20:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012219.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 23 08:15:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.297	10.796	155.2E6	150.4E6	459.991	383.395
Target Compounds							
1) T	Dalapon	2.812	2.297	17600525	52366167	36.189	110.705 #
2) T	3,5-DICHL...	0.000	8.962	0	6303360	N.D.	12.885 #
5) T	DICAMBA	0.000	11.036	0	2294423	N.D.	1.554 #
6) T	MCP	11.961	0.000	18127215	0	17.624	N.D. #
7) T	MCPA	12.160	0.000	11435559	0	7.216	N.D. #
10) T	Pentachlo...	0.000	13.139	0	5268288	N.D.	0.917 #
14) T	DINOSEB	0.000	15.507	0	4506475	N.D.	2.703 #
15) T	Picloram	0.000	16.725	0	17993970	N.D.	6.103 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012219\
Data File : PS002938.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jan 2019 21:21
Operator : EI\SJ
Sample : K1013-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PL-01-011819-D

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 23 08:20:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012219.M
Quant Title : 8080.M
QLast Update : Wed Jan 23 08:15:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

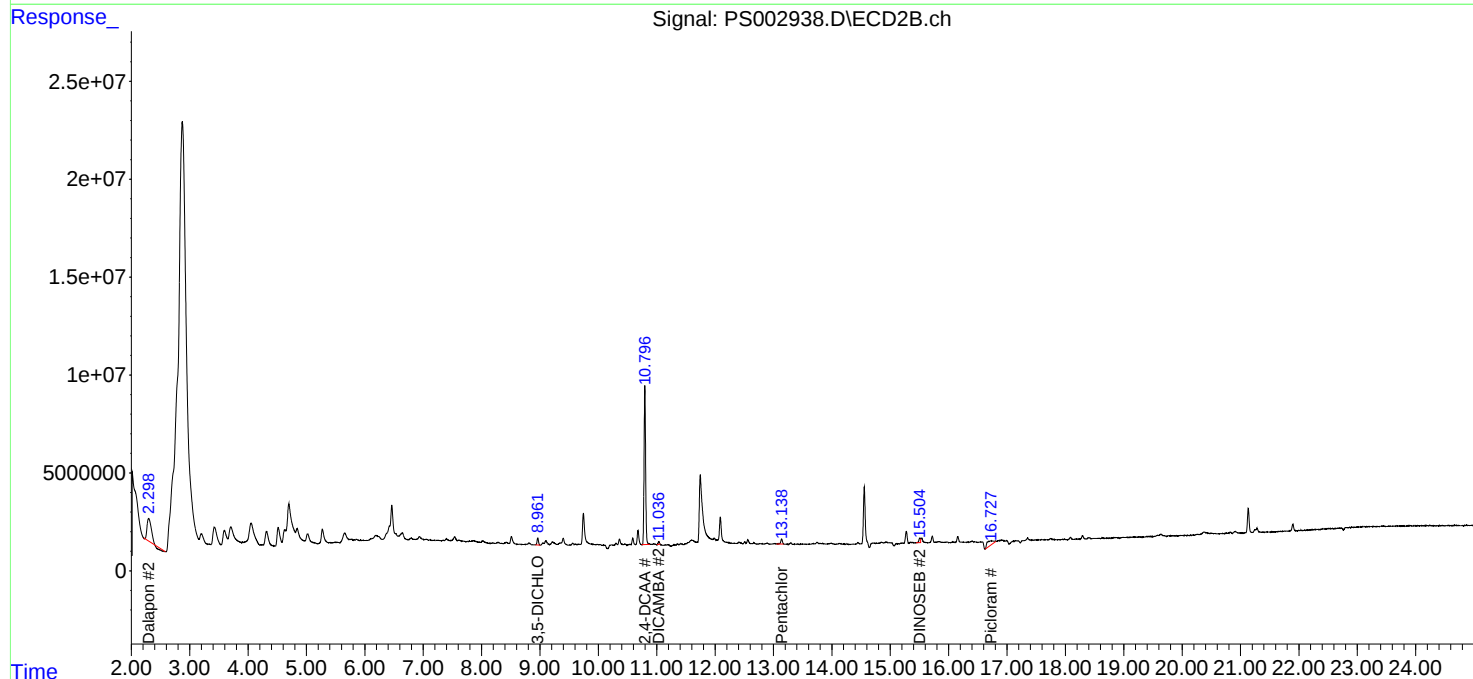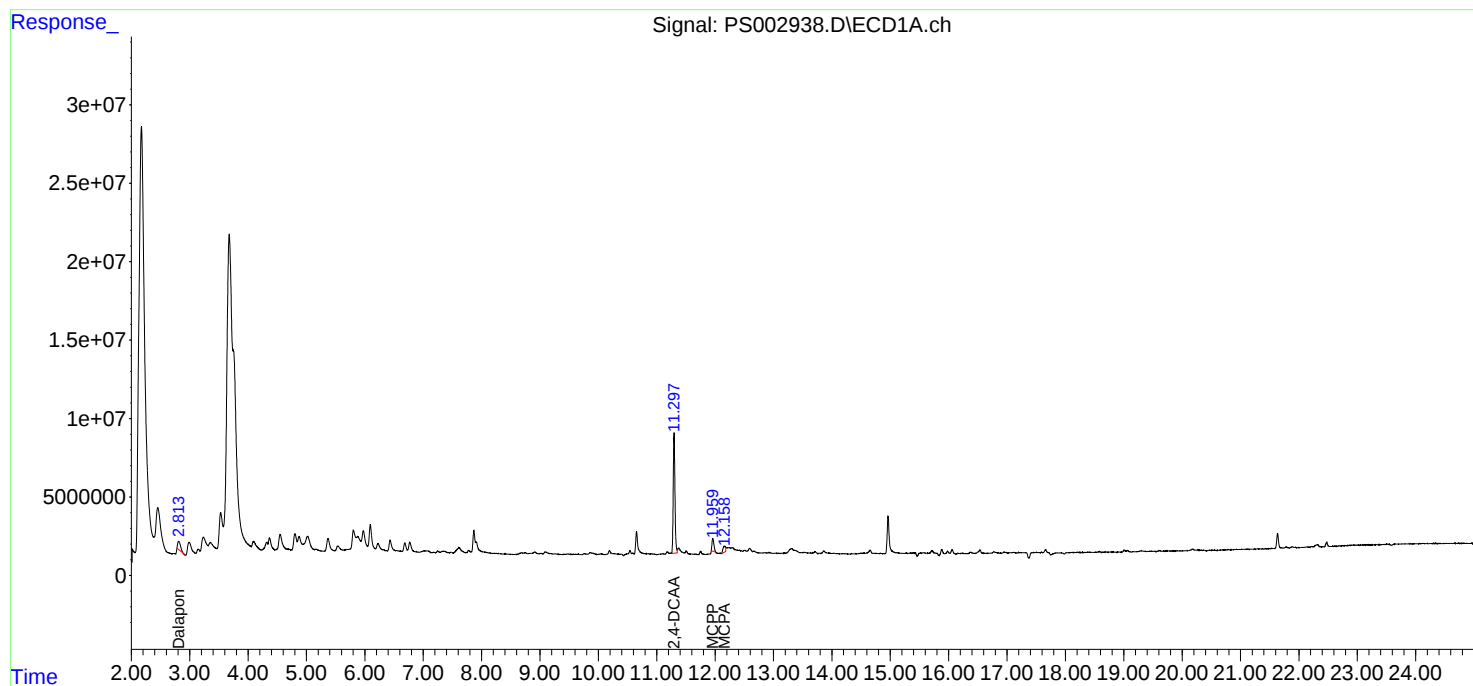


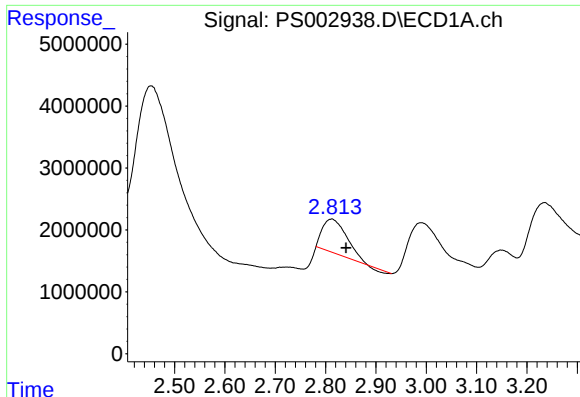

#1 Dalapon


R.T.: 2.812 min
Delta R.T.: -0.029 min
Response: 17600525
Conc: 36.19 ng/ml

Instrument :
ECD_S
ClientSampleId :
PL-01-011819-D

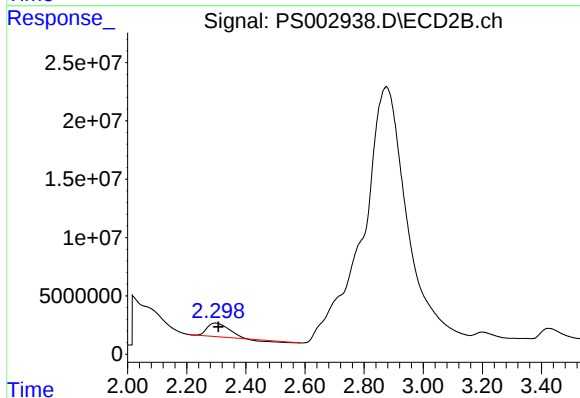


#1 Dalapon

R.T.: 2.297 min
Delta R.T.: -0.010 min
Response: 52366167
Conc: 110.71 ng/ml

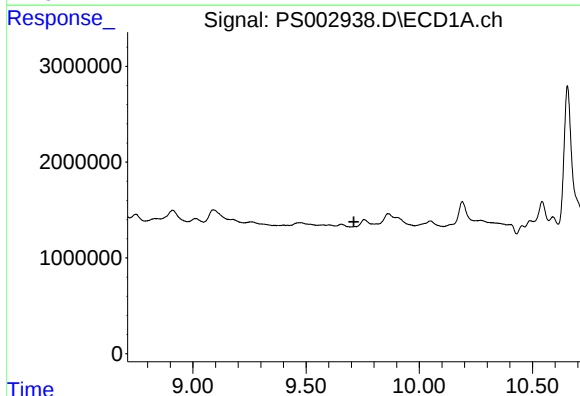


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.711 min
Response: 0
Conc: N.D.

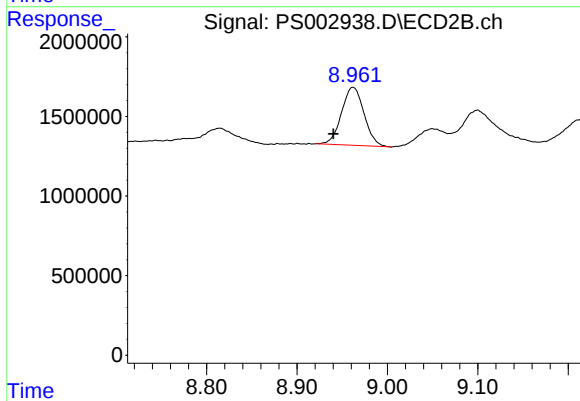

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.962 min
Delta R.T.: 0.022 min
Response: 6303360
Conc: 12.88 ng/ml

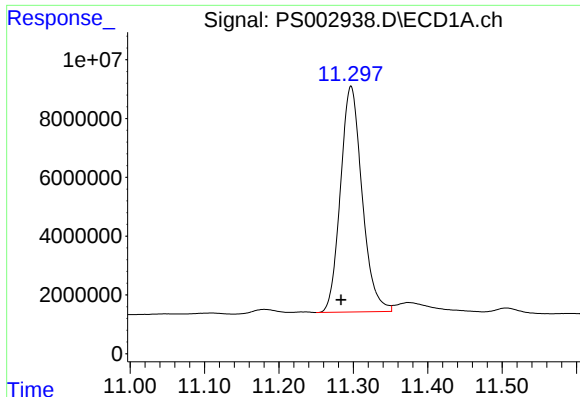

#4 2,4-DCAA


R.T.: 11.297 min
Delta R.T.: 0.013 min
Response: 155154505
Conc: 459.99 ng/ml

Instrument :
ECD_S
ClientSampleId :
PL-01-011819-D

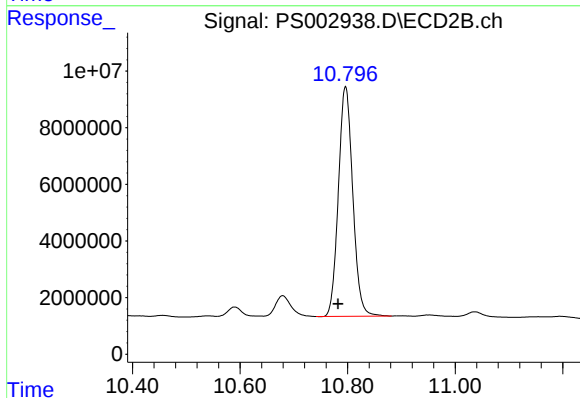


#4 2,4-DCAA

R.T.: 10.796 min
Delta R.T.: 0.013 min
Response: 150373154
Conc: 383.40 ng/ml

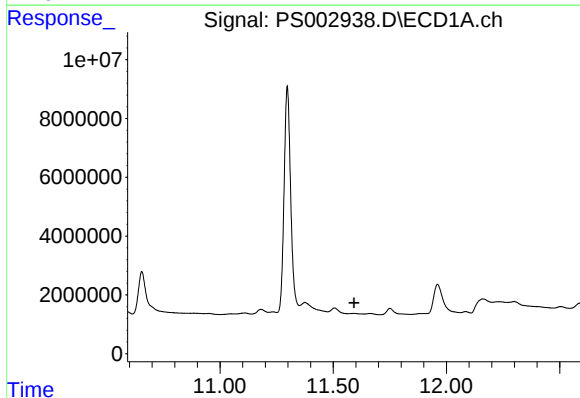


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.592 min
Response: 0
Conc: N.D.

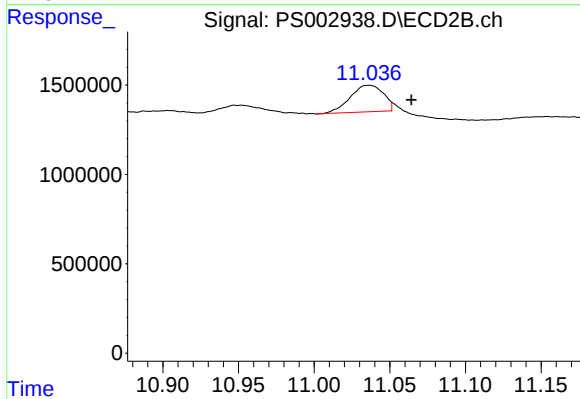

#5 DICAMBA


R.T.: 11.036 min
Delta R.T.: -0.028 min
Response: 2294423
Conc: 1.55 ng/ml

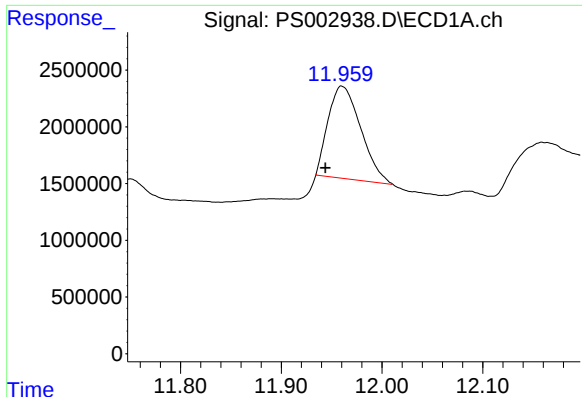

#6 MCPP


R.T.: 11.961 min
Delta R.T.: 0.017 min
Response: 18127215
Conc: 17.62 ug/ml

Instrument :
ECD_S
ClientSampleId :
PL-01-011819-D

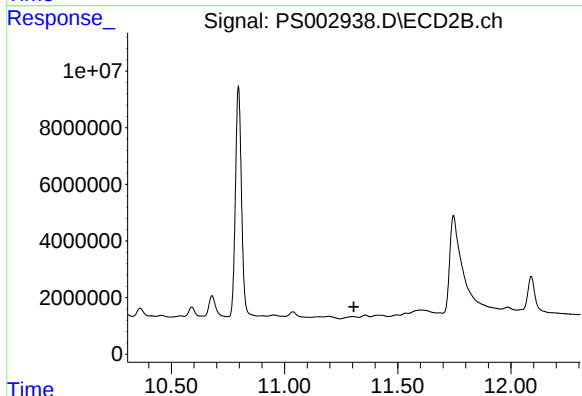


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.306 min
Response: 0
Conc: N.D.

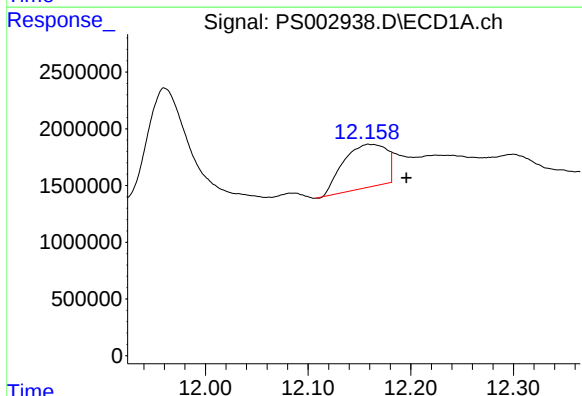


#7 MCPA

R.T.: 12.160 min
Delta R.T.: -0.035 min
Response: 11435559
Conc: 7.22 ug/ml

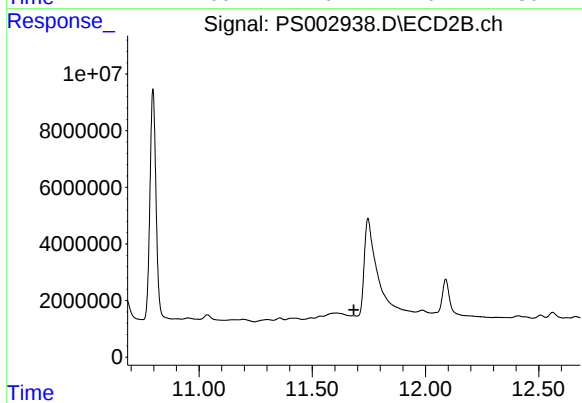

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 11.684 min
Response: 0
Conc: N.D.

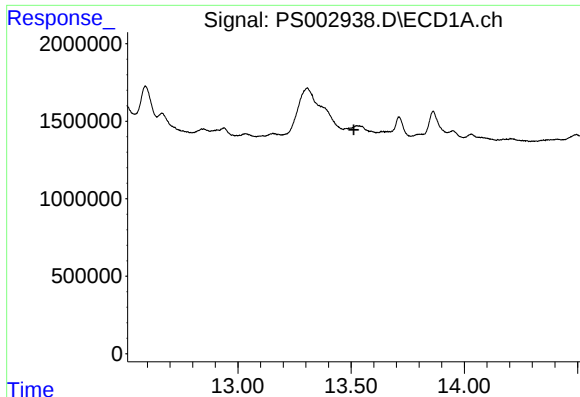

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 13.512 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PL-01-011819-D

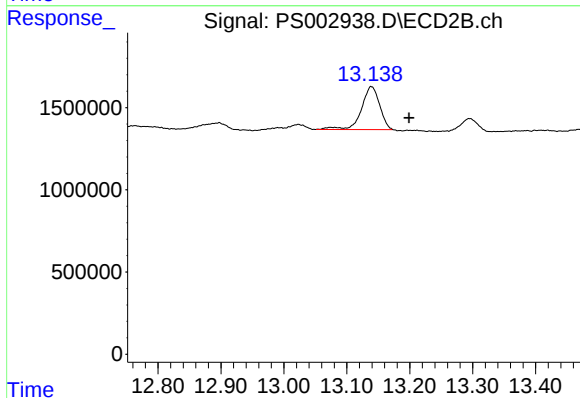


#10 Pentachlorophenol

R.T.: 13.139 min
Delta R.T.: -0.060 min
Response: 5268288
Conc: 0.92 ng/ml

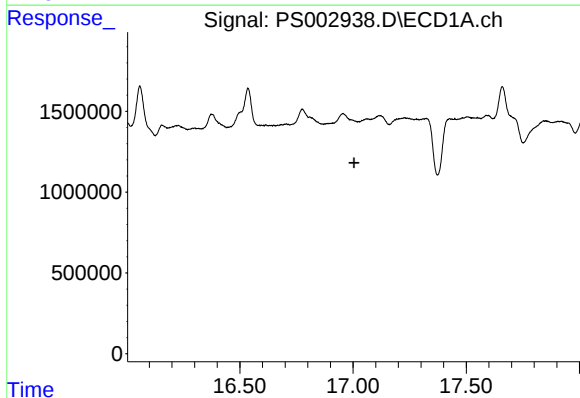


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 17.004 min
Response: 0
Conc: N.D.

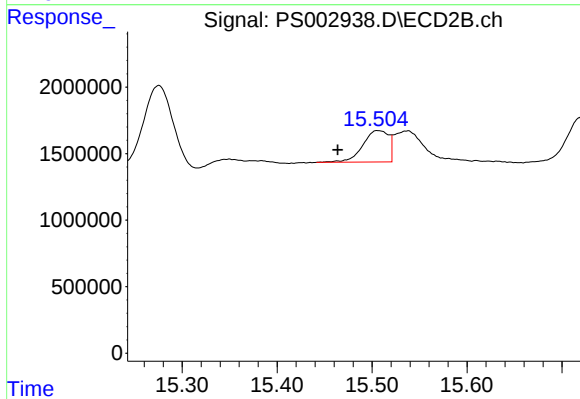

#14 DINOSEB


R.T.: 15.507 min
Delta R.T.: 0.043 min
Response: 4506475
Conc: 2.70 ng/ml

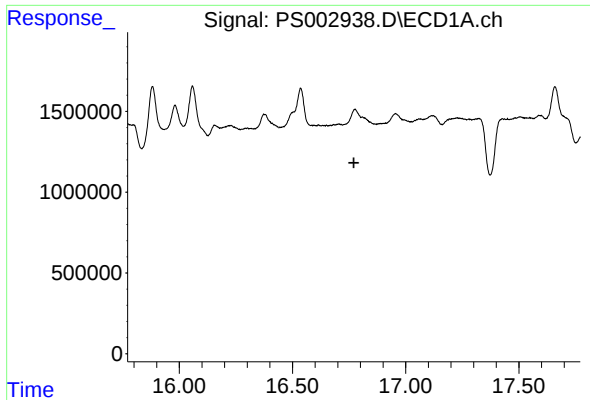

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.771 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PL-01-011819-D

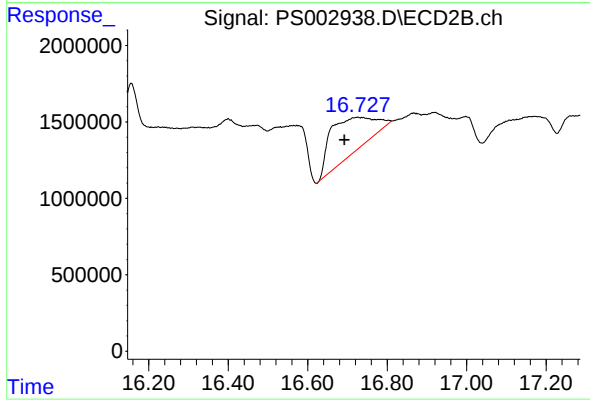

#15 Picloram

R.T.: 16.725 min
Delta R.T.: 0.033 min
Response: 17993970
Conc: 6.10 ng/ml