

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012219\
 Data File : PS002941.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jan 2019 22:55
 Operator : EI\SJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDCCC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 23 08:21:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012219.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 23 08:15:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.282	10.781	221.2E6	174.3E6	655.795	444.457 #
Target Compounds							
1) T	Dalapon	2.839	2.307	311.0E6	305.8E6	639.533	646.376
2) T	3,5-DICHL...	9.709	8.939	234.3E6	63984654	451.833	130.792 #
7) T	MCPA	0.000	11.671	0	116.5E6	N.D.	78.495 #
8) T	DICHLORPROP	12.779	12.188	263.3E6	-8353202	708.881	N.D. #
12) T	2,4,5-T	14.781	14.383	1500.8E6	-1157043813	735.092	N.D. #
14) T	DINOSEB	17.001	15.461	220.5E6	-36158934	141.029	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012219\
Data File : PS002941.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jan 2019 22:55
Operator : EI\SJ
Sample : HSTDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 23 08:21:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012219.M
Quant Title : 8080.M
QLast Update : Wed Jan 23 08:15:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

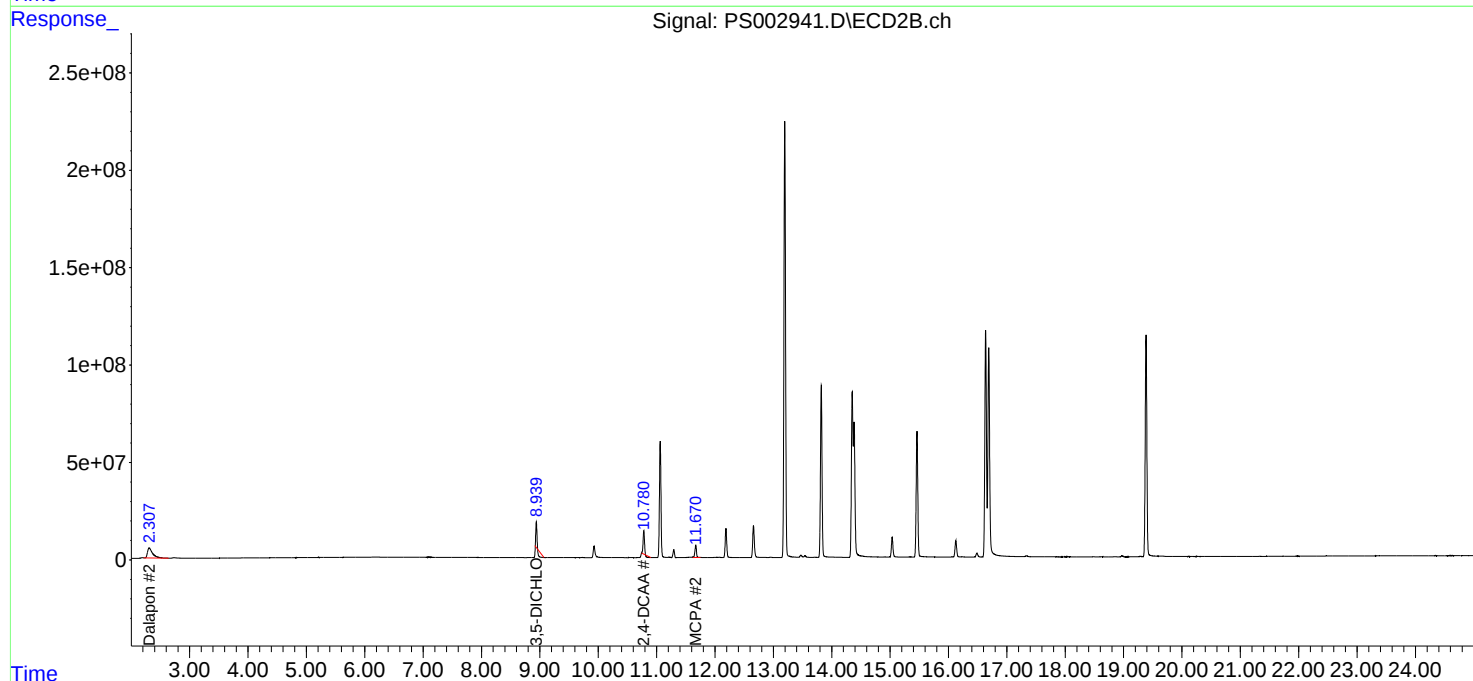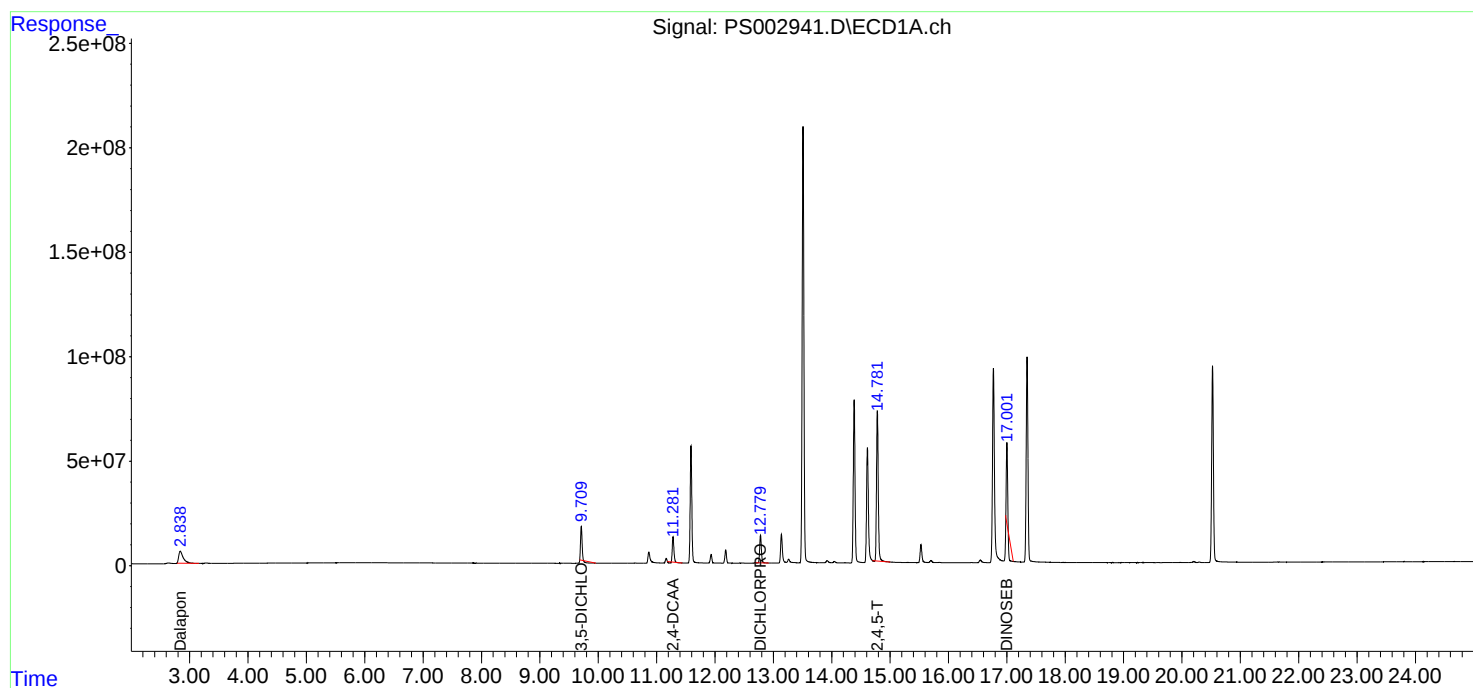


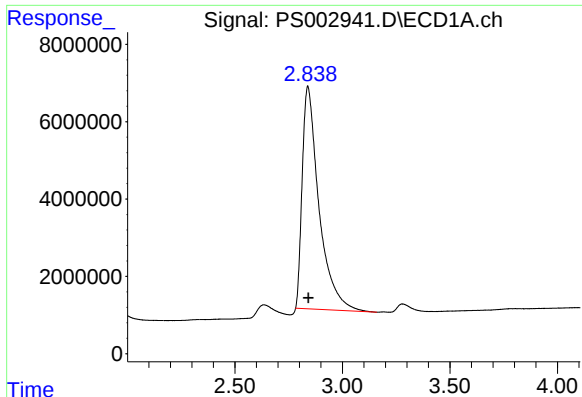

#1 Dalapon


R.T.: 2.839 min
Delta R.T.: -0.002 min
Response: 311035198
Conc: 639.53 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

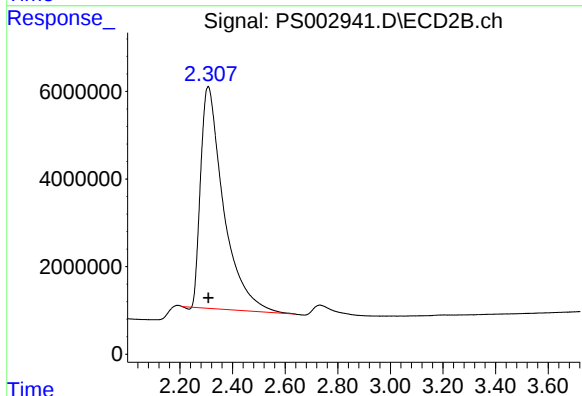


#1 Dalapon

R.T.: 2.307 min
Delta R.T.: 0.000 min
Response: 305750253
Conc: 646.38 ng/ml

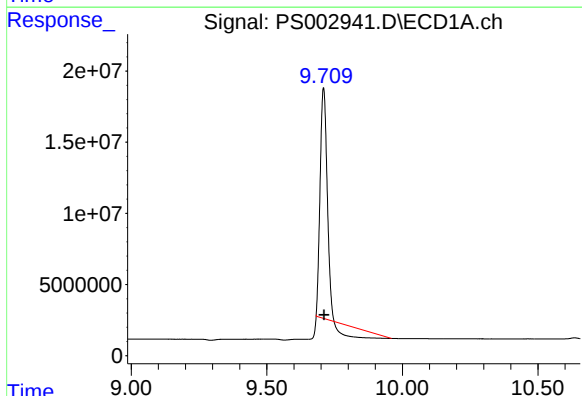


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.709 min
Delta R.T.: -0.002 min
Response: 234303880
Conc: 451.83 ng/ml

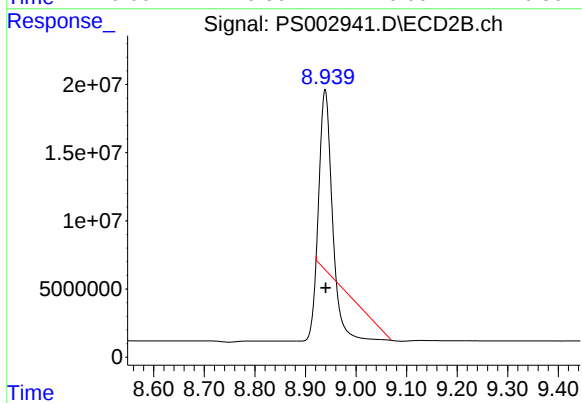

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.939 min
Delta R.T.: -0.001 min
Response: 63984654
Conc: 130.79 ng/ml

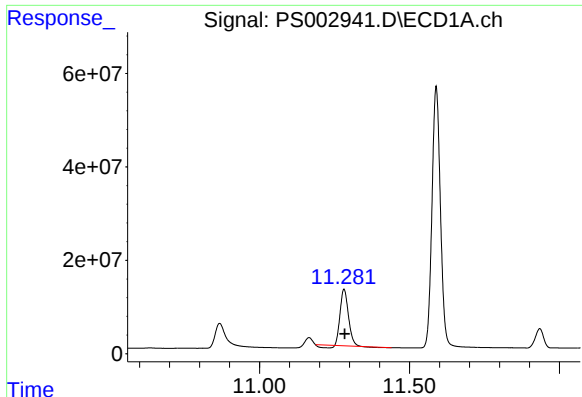

#4 2,4-DCAA


R.T.: 11.282 min
Delta R.T.: -0.002 min
Response: 221199041
Conc: 655.80 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

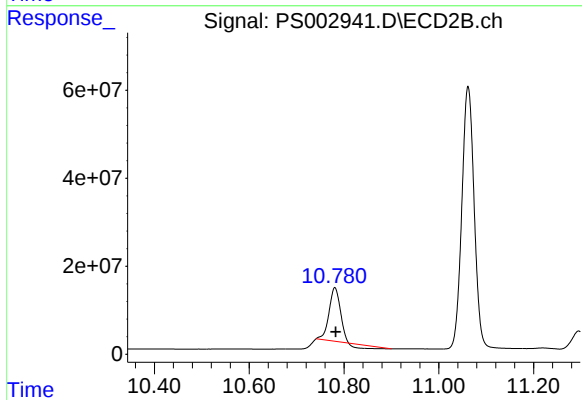


#4 2,4-DCAA

R.T.: 10.781 min
Delta R.T.: -0.002 min
Response: 174322357
Conc: 444.46 ng/ml

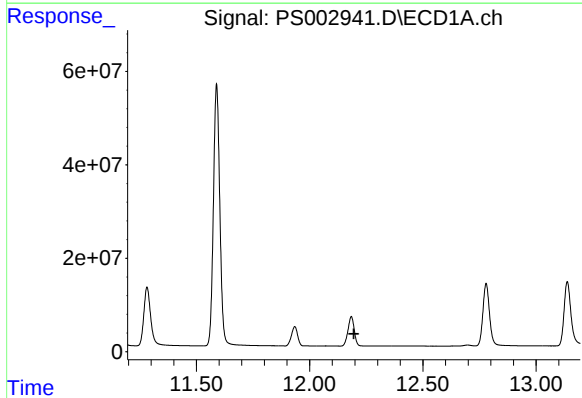


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.196 min
Response: 0
Conc: N.D.

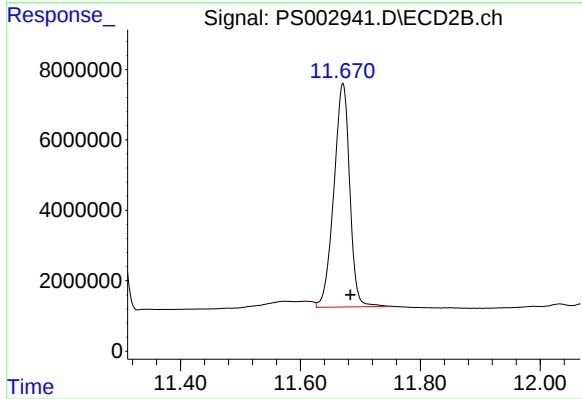

#7 MCPA


R.T.: 11.671 min
Delta R.T.: -0.013 min
Response: 116547892
Conc: 78.50 ug/ml

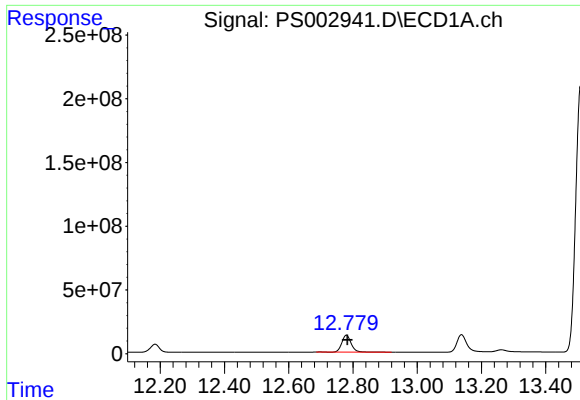

#8 DICHLORPROP


R.T.: 12.779 min
Delta R.T.: -0.003 min
Response: 263343070
Conc: 708.88 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

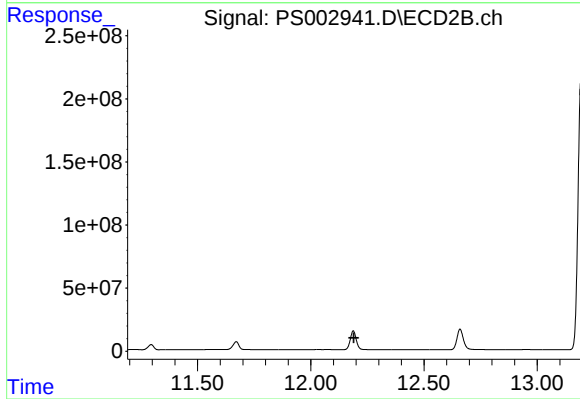


#8 DICHLORPROP

R.T.: 12.188 min
Delta R.T.: -0.003 min
Response: -8353202
Conc: N.D.

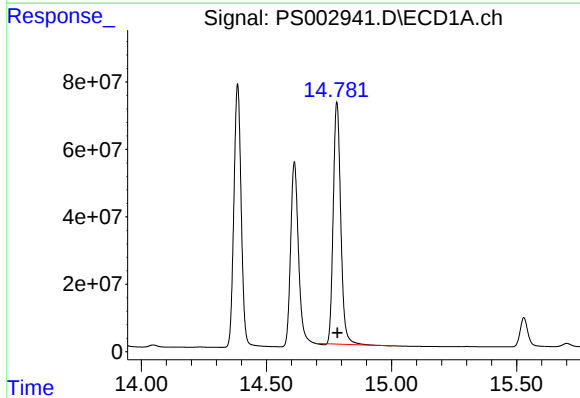


#12 2,4,5-T

R.T.: 14.781 min
Delta R.T.: -0.003 min
Response: 1500820648
Conc: 735.09 ng/ml

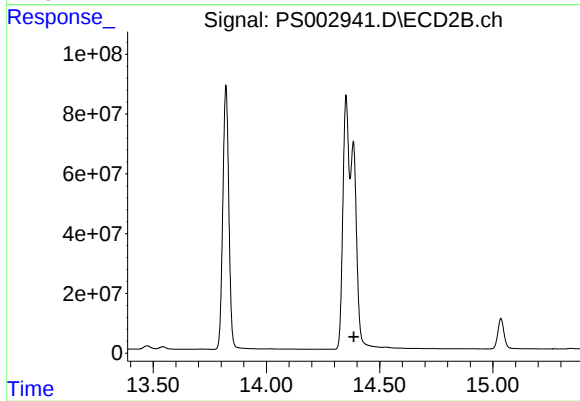

#12 2,4,5-T


R.T.: 14.383 min
Delta R.T.: -0.003 min
Response: -1157043813
Conc: N.D.

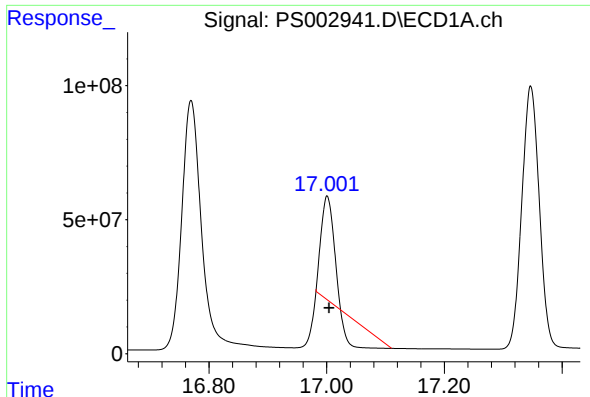

#14 DINOSEB

R.T.: 17.001 min
Delta R.T.: -0.003 min
Response: 220463439
Conc: 141.03 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

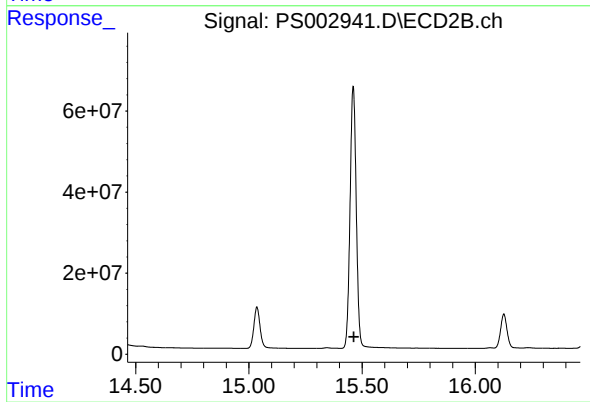

#14 DINOSEB

R.T.: 15.461 min
Delta R.T.: -0.003 min
Response: -36158934
Conc: N.D.