

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012220\
 Data File : PS008495.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jan 2020 18:10
 Operator : DD\AJ
 Sample : L1004-15
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 BU-03-012020

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 22 00:54:16 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 08 11:00:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.289	5.983	629.4E6	349.0E6	356.431	368.360
Target Compounds							
1) T	Dalapon	2.524	2.206	36734837	19133888	14.328	15.093
2) T	3,5-DICHL...	0.000	5.170	0	112.9E6	N.D.	80.771
6) T	MCP	6.703	0.000	33167285	0	6.507	N.D. #
7) T	MCPA	6.733	0.000	99889590	0	13.670	N.D. #
8) T	DICHLORPROP	0.000	6.803	0	19095052	N.D.	19.764
10) T	Pentachlo...	7.772	0.000	24566583	0	1.011	N.D. #
12) T	2,4,5-T	8.489	8.312	112.6E6	13623140	12.205	2.576 #
13) T	2,4-DB	9.052	0.000	22285760	0	16.076	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012220\
Data File : PS008495.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jan 2020 18:10
Operator : DD\AJ
Sample : L1004-15
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
BU-03-012020

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 22 00:54:16 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
Quant Title : 8080.M
QLast Update : Wed Jan 08 11:00:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

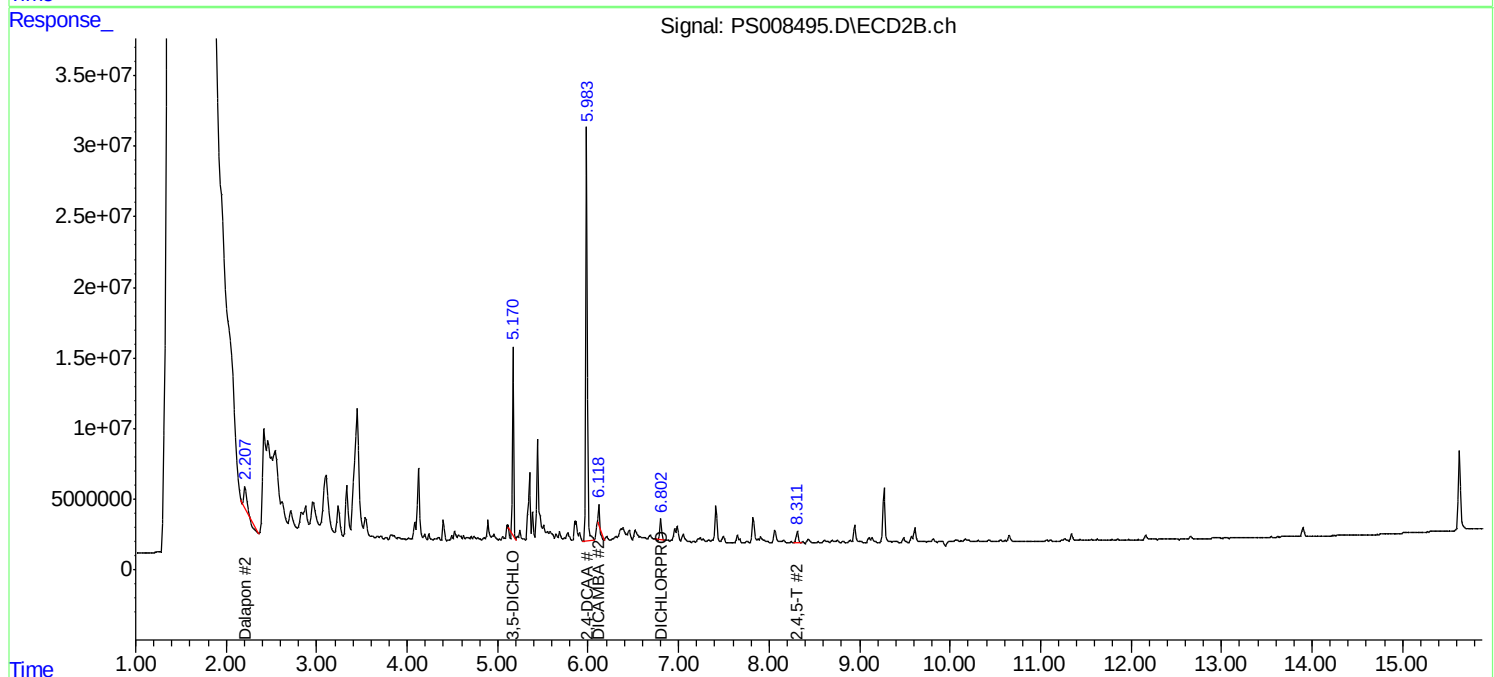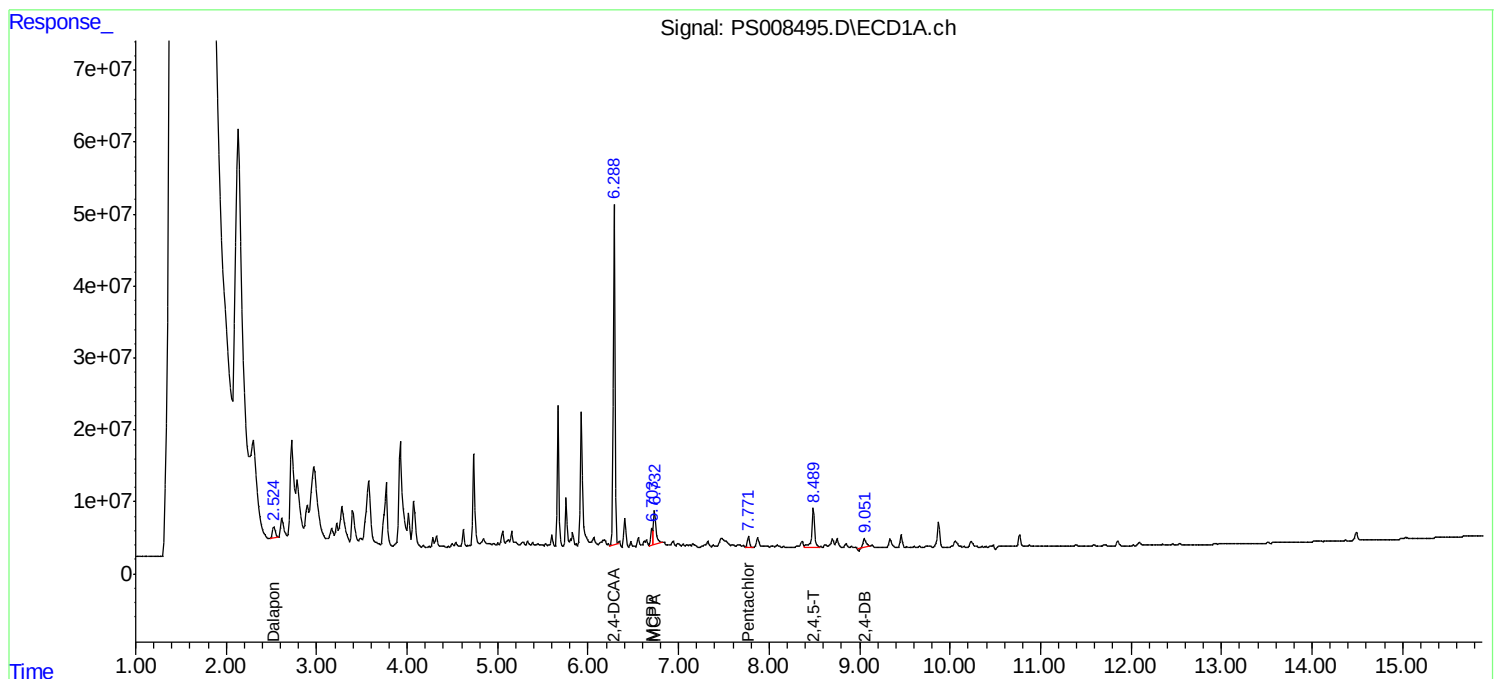


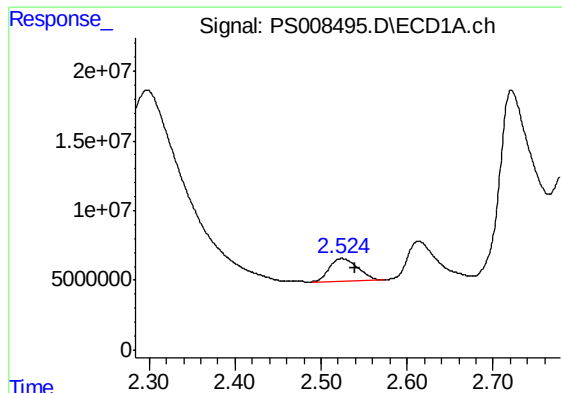

#1 Dalapon


R.T.: 2.524 min
Delta R.T.: -0.016 min
Response: 36734837
Conc: 14.33 ng/ml

Instrument :
ECD_S
ClientSampleId :
BU-03-012020

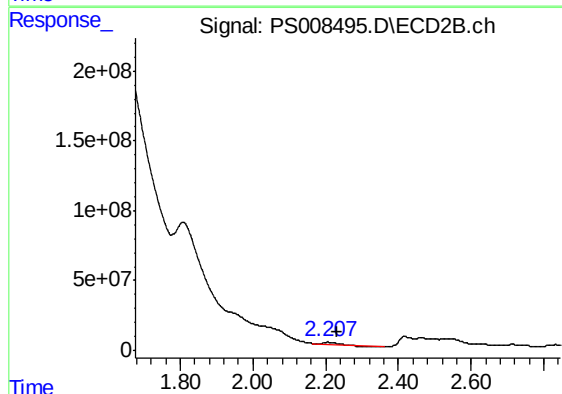


#1 Dalapon

R.T.: 2.206 min
Delta R.T.: -0.025 min
Response: 19133888
Conc: 15.09 ng/ml

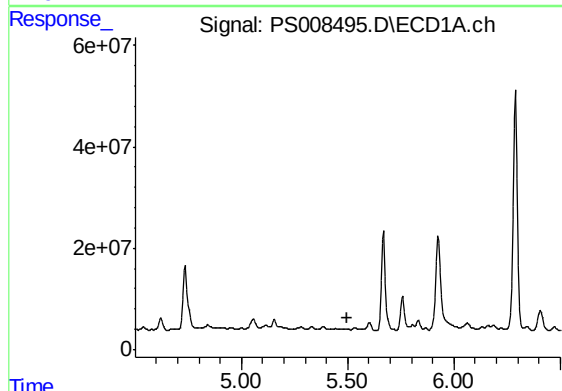


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.501 min
Response: 0
Conc: N.D.

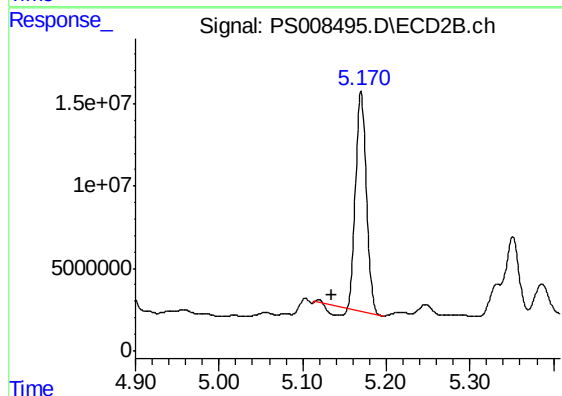

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.170 min
Delta R.T.: 0.036 min
Response: 112851851
Conc: 80.77 ng/ml

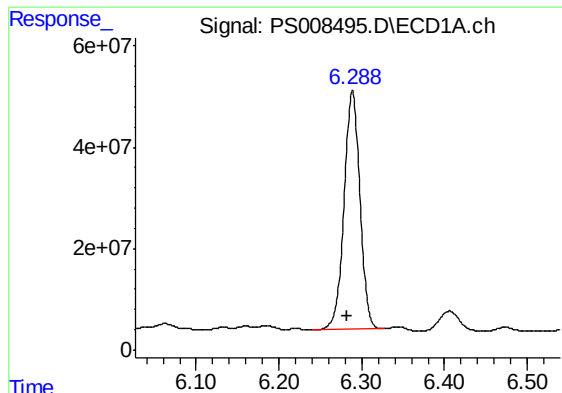

#4 2,4-DCAA


R.T.: 6.289 min
Delta R.T.: 0.006 min
Response: 629352408
Conc: 356.43 ng/ml

Instrument :
ECD_S
ClientSampleId :
BU-03-012020

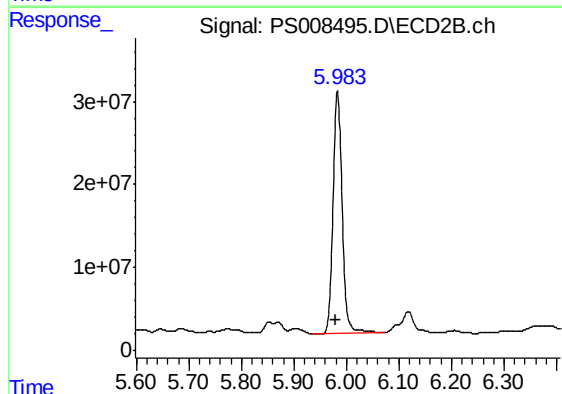


#4 2,4-DCAA

R.T.: 5.983 min
Delta R.T.: 0.004 min
Response: 349007285
Conc: 368.36 ng/ml

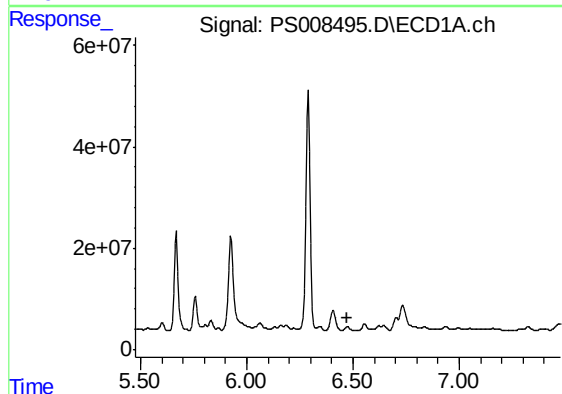


#5 DICAMBA

R.T.: 6.406 min
Delta R.T.: -0.070 min
Response: -26234354
Conc: N.D.

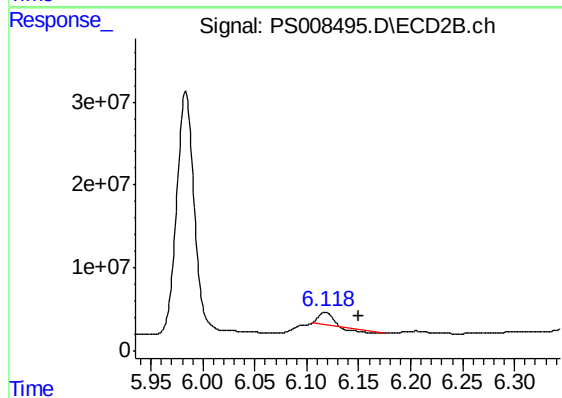

#5 DICAMBA


R.T.: 6.118 min
Delta R.T.: -0.032 min
Response: 10017004
Conc: 2.50 ng/ml

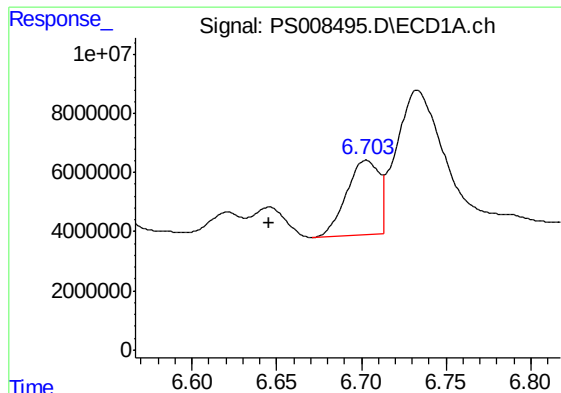

#6 MCPP


R.T.: 6.703 min
Delta R.T.: 0.057 min
Response: 33167285
Conc: 6.51 ug/ml

Instrument :
ECD_S
ClientSampleId :
BU-03-012020

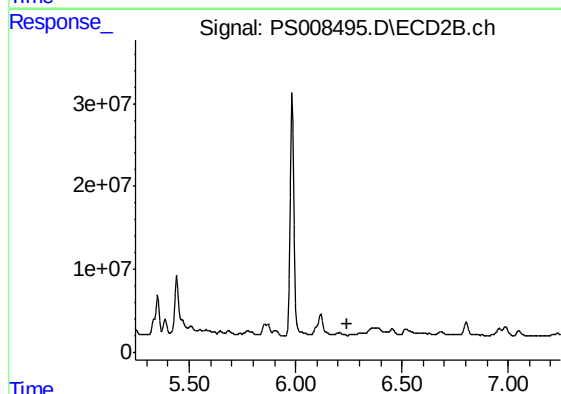


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 6.246 min
Response: 0
Conc: N.D.

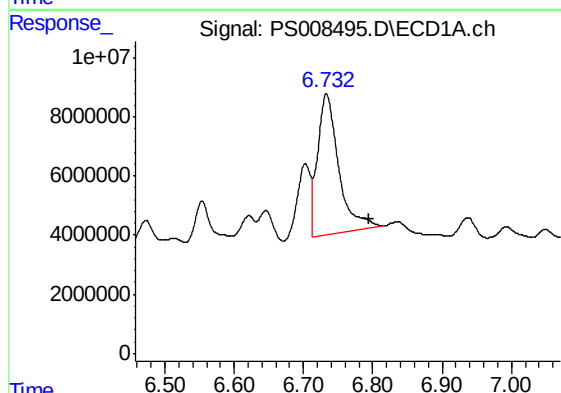


#7 MCPA

R.T.: 6.733 min
Delta R.T.: -0.061 min
Response: 99889590
Conc: 13.67 ug/ml

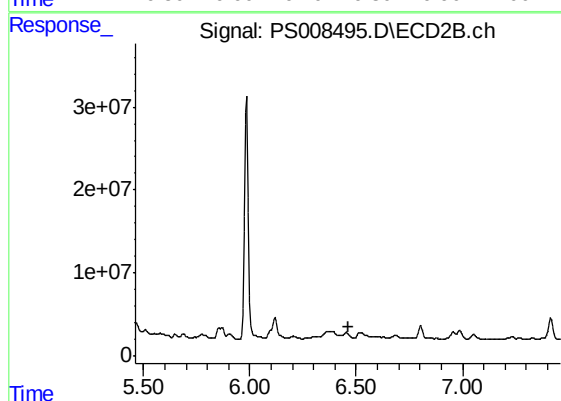

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 6.462 min
Response: 0
Conc: N.D.

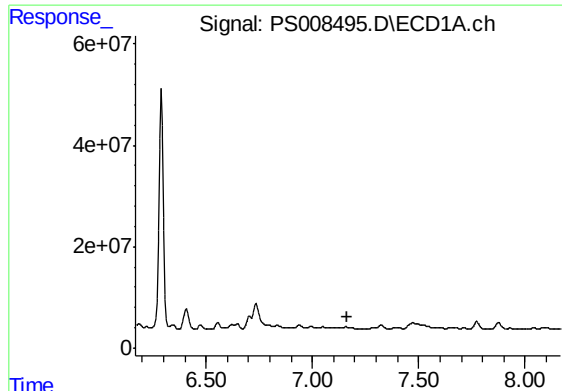

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 7.167 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
BU-03-012020

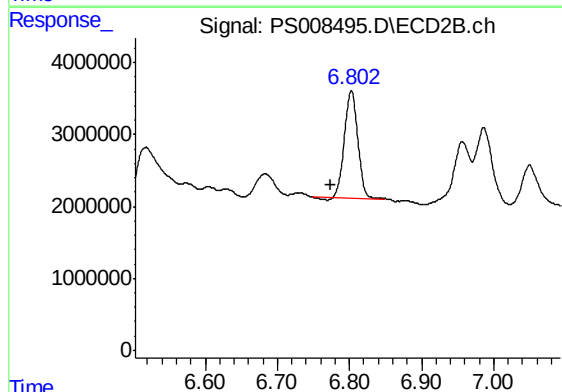


#8 DICHLORPROP

R.T.: 6.803 min
Delta R.T.: 0.028 min
Response: 19095052
Conc: 19.76 ng/ml

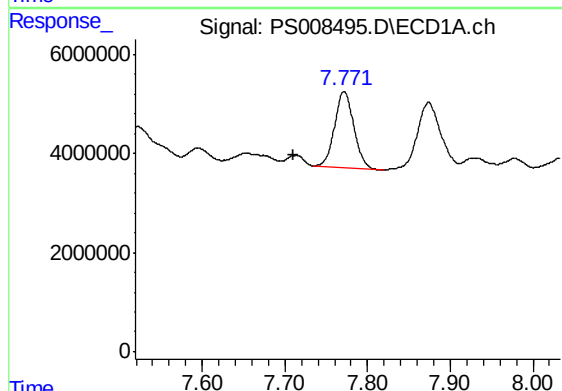


#10 Pentachlorophenol

R.T.: 7.772 min
Delta R.T.: 0.061 min
Response: 24566583
Conc: 1.01 ng/ml

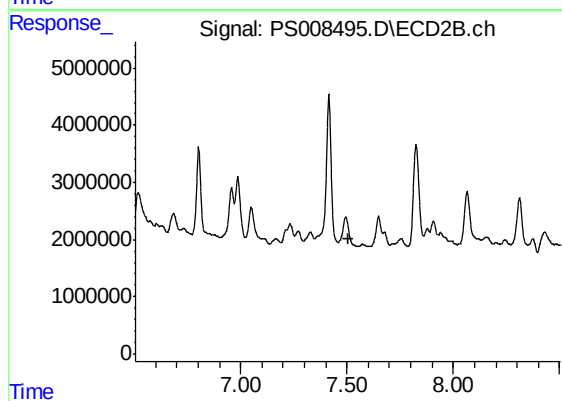

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 7.505 min
Response: 0
Conc: N.D.

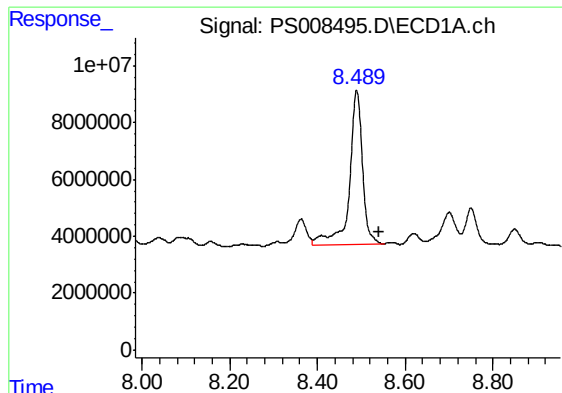

#12 2,4,5-T


R.T.: 8.489 min
Delta R.T.: -0.052 min
Response: 112613170
Conc: 12.21 ng/ml

Instrument :
ECD_S
ClientSampleId :
BU-03-012020

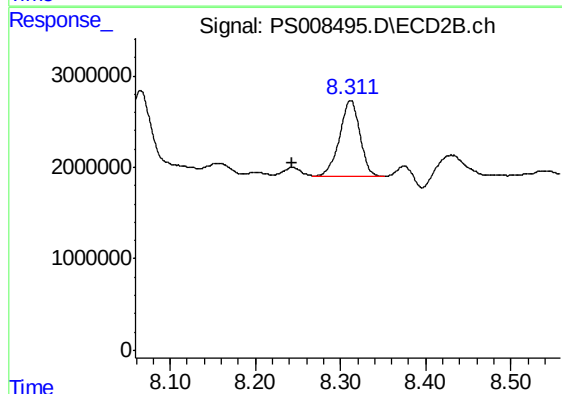


#12 2,4,5-T

R.T.: 8.312 min
Delta R.T.: 0.068 min
Response: 13623140
Conc: 2.58 ng/ml

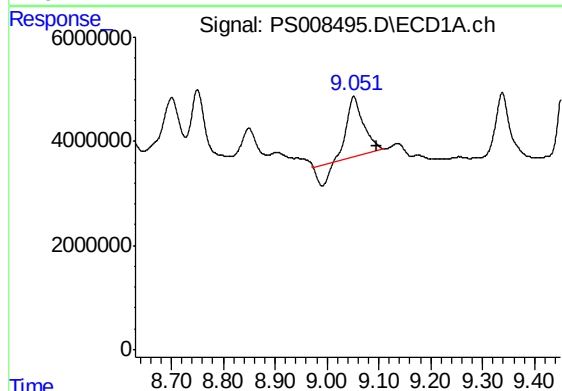

#13 2,4-DB

R.T.: 9.052 min
Delta R.T.: -0.043 min
Response: 22285760
Conc: 16.08 ng/ml

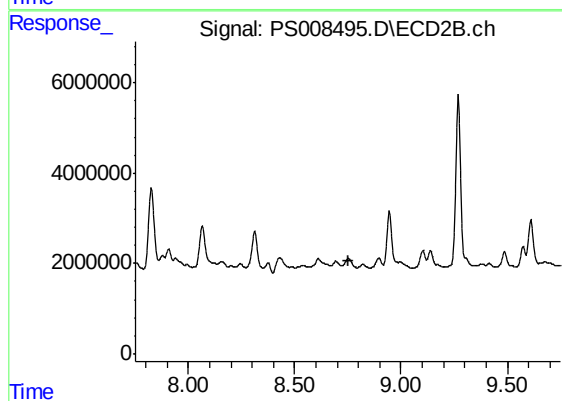

#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 8.751 min
Response: 0
Conc: N.D.