

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012220\
 Data File : PS008515.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jan 2020 01:28
 Operator : DD\AJ
 Sample : L1181-05
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 93OAK-AVE-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 22 02:32:03 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 08 11:00:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.302	5.995	478.9E6	260.0E6	271.214	274.447
Target Compounds							
2) T	3,5-DICHL...	0.000	5.117	0 10686148		N.D.	7.648
3) T	4-Nitroph...	6.079	0.000	21622521	0	22.201	N.D. #
5) T	DICAMBA	0.000	6.129	0 23102665		N.D.	5.777
6) T	MCPD	6.661	0.000	23554966	0	4.621	N.D. #
7) T	MCPA	6.795	6.459	66765665	24666175	9.137	5.777 #
8) T	DICHLORPROP	0.000	6.747	0 35593677		N.D.	36.841
9) T	2,4-D	0.000	7.063	0 19118153		N.D.	16.309
11) T	2,4,5-TP ...	0.000	7.844	0 21584093		N.D.	4.130
12) T	2,4,5-T	8.504	0.000	95998010	0	10.405	N.D. #
13) T	2,4-DB	9.064	0.000	58919149	0	42.503	N.D. #
14) T	DINOSEB	0.000	9.111	0 29145358		N.D.	7.715
15) T	Picloram	0.000	10.077	0 28177539		N.D.	3.793
16) T	DCPA	0.000	10.077	0 28177539		N.D.	4.324



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012220\
Data File : PS008515.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jan 2020 01:28
Operator : DD\AJ
Sample : L1181-05
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
93OAK-AVE-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 22 02:32:03 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
Quant Title : 8080.M
QLast Update : Wed Jan 08 11:00:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

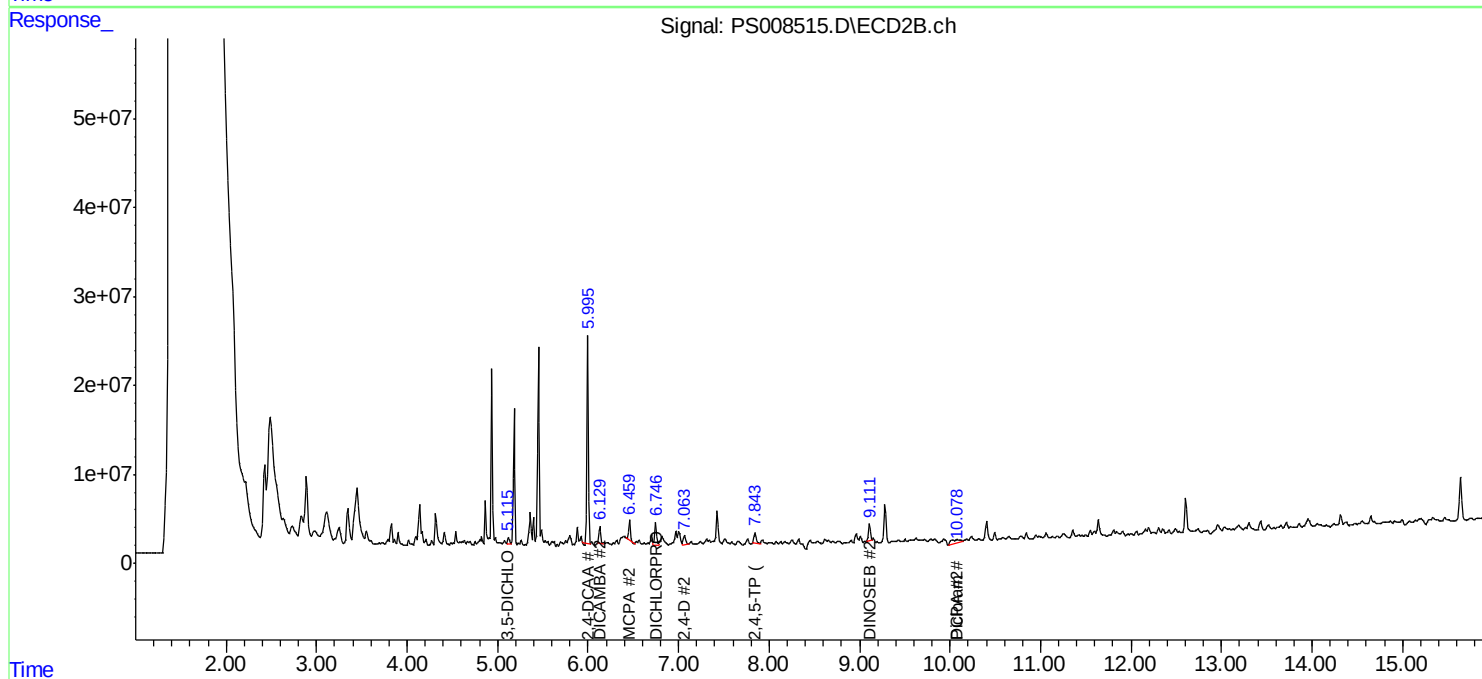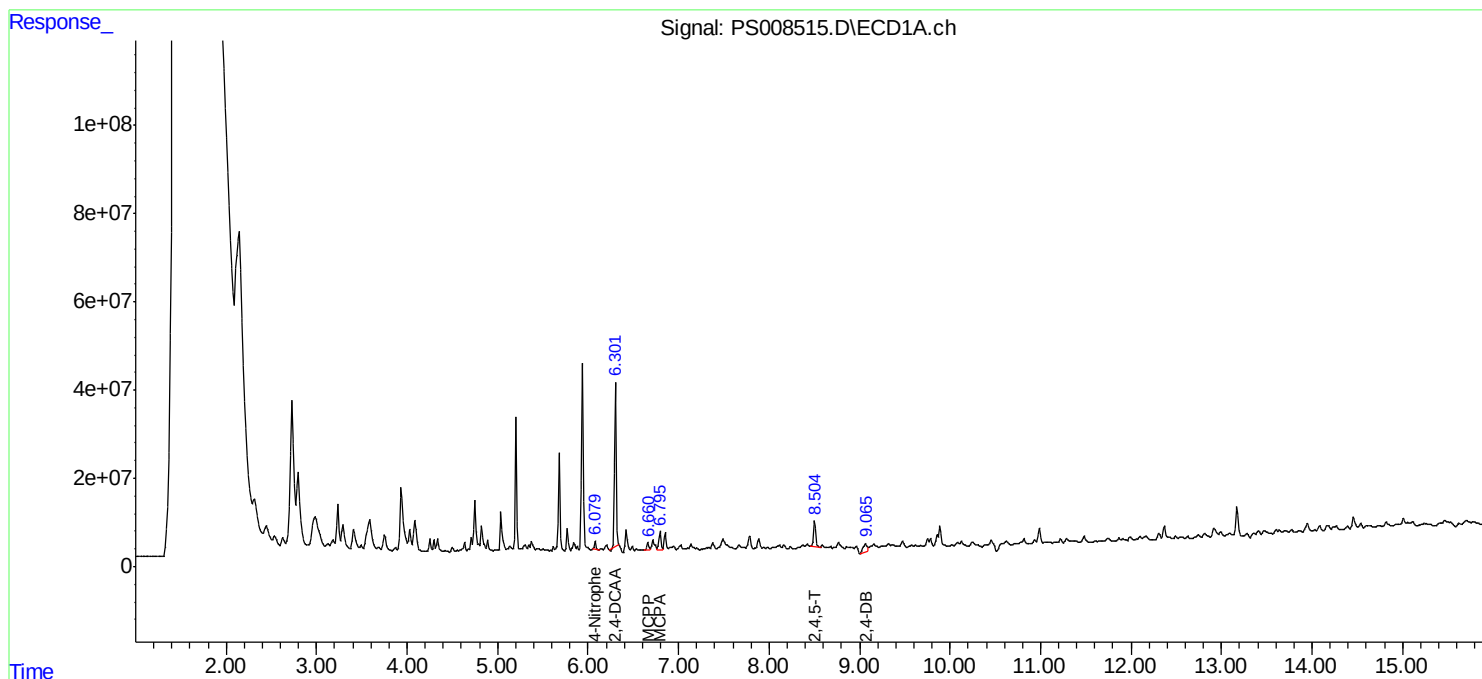


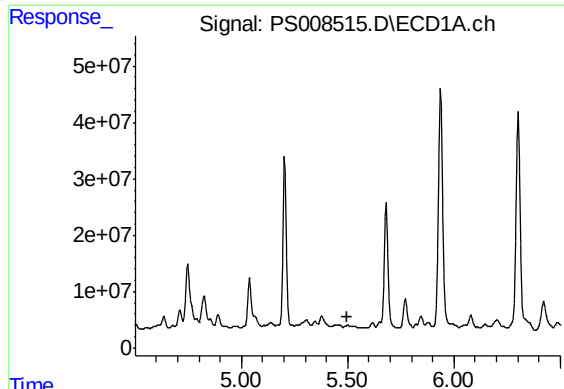

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 5.501 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
93OAK-AVE-COMP

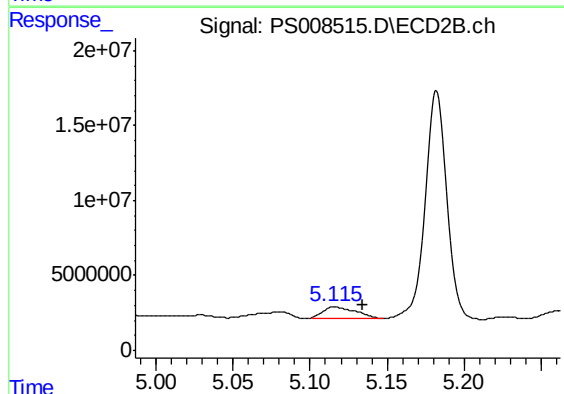


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.117 min
Delta R.T.: -0.018 min
Response: 10686148
Conc: 7.65 ng/ml

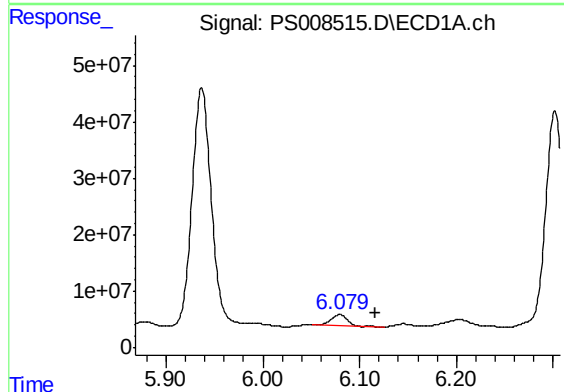


#3 4-Nitrophenol

R.T.: 6.079 min
Delta R.T.: -0.037 min
Response: 21622521
Conc: 22.20 ng/ml

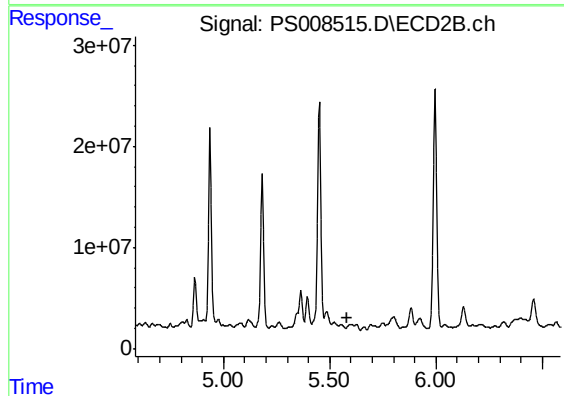

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 5.585 min
Response: 0
Conc: N.D.

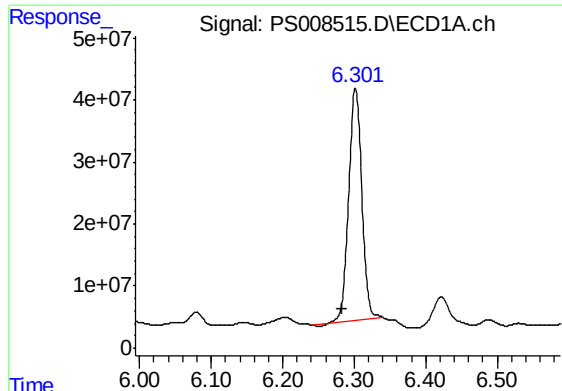

#4 2,4-DCAA


R.T.: 6.302 min
Delta R.T.: 0.019 min
Response: 478883874
Conc: 271.21 ng/ml

Instrument :
ECD_S
ClientSampleId :
93OAK-AVE-COMP

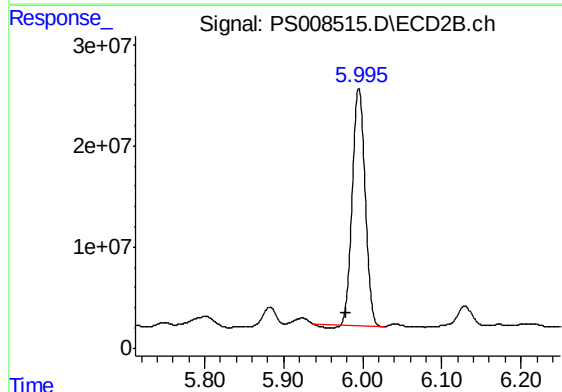


#4 2,4-DCAA

R.T.: 5.995 min
Delta R.T.: 0.016 min
Response: 260028441
Conc: 274.45 ng/ml

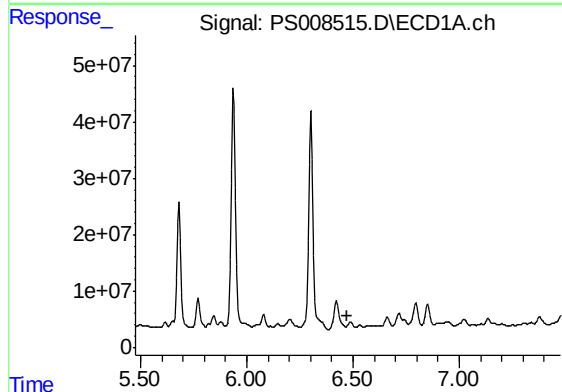


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 6.476 min
Response: 0
Conc: N.D.

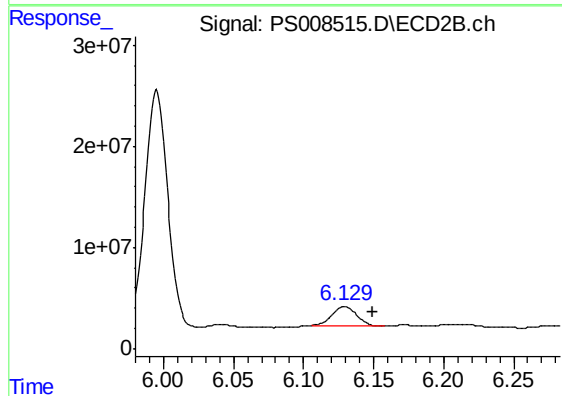

#5 DICAMBA


R.T.: 6.129 min
Delta R.T.: -0.021 min
Response: 23102665
Conc: 5.78 ng/ml

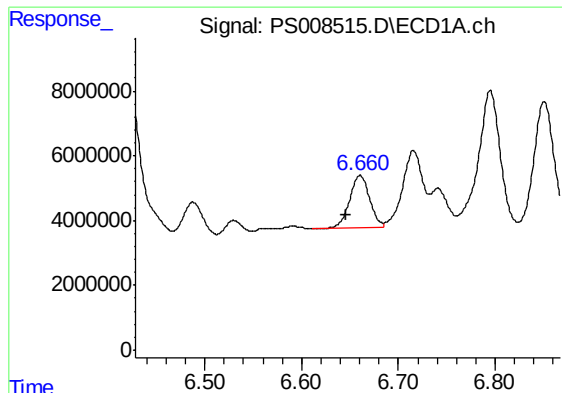

#6 MCPP


R.T.: 6.661 min
Delta R.T.: 0.015 min
Response: 23554966
Conc: 4.62 ug/ml

Instrument :
ECD_S
ClientSampleId :
93OAK-AVE-COMP

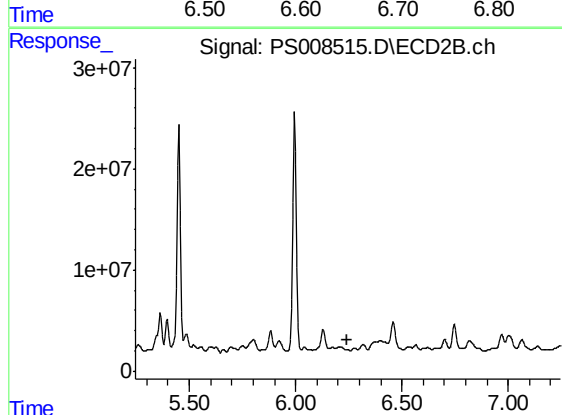


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 6.246 min
Response: 0
Conc: N.D.

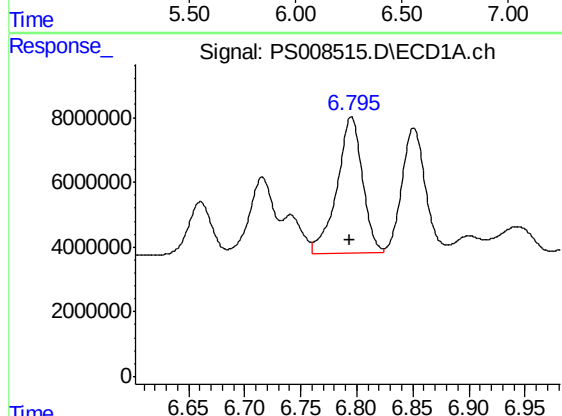


#7 MCPA

R.T.: 6.795 min
Delta R.T.: 0.000 min
Response: 66765665
Conc: 9.14 ug/ml

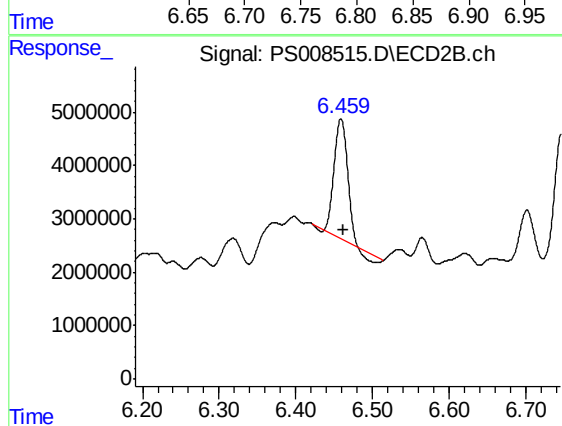

#7 MCPA


R.T.: 6.459 min
Delta R.T.: -0.003 min
Response: 24666175
Conc: 5.78 ug/ml

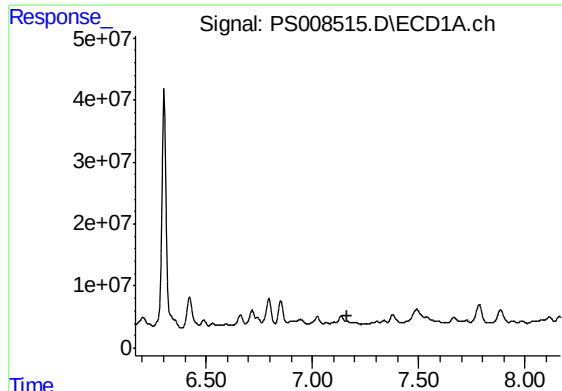

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.167 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
93OAK-AVE-COMP

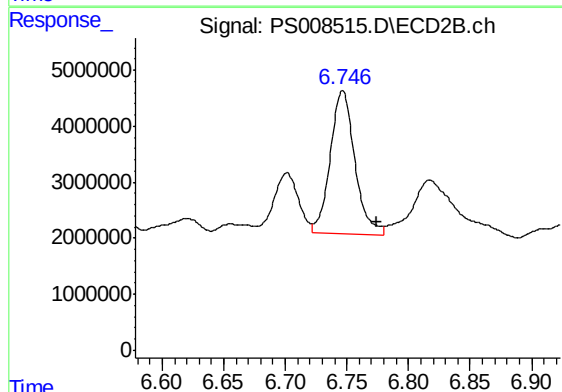


#8 DICHLORPROP

R.T.: 6.747 min
Delta R.T.: -0.028 min
Response: 35593677
Conc: 36.84 ng/ml

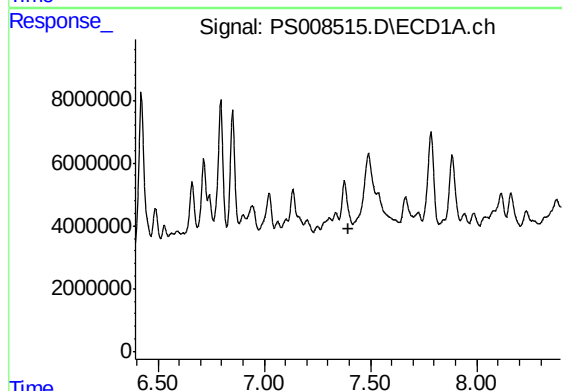


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 7.394 min
Response: 0
Conc: N.D.

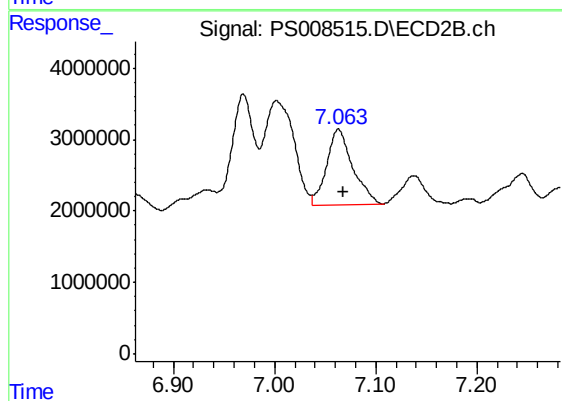

#9 2,4-D


R.T.: 7.063 min
Delta R.T.: -0.005 min
Response: 19118153
Conc: 16.31 ng/ml

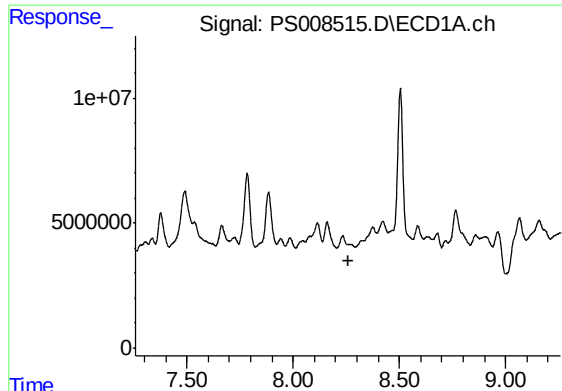

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 8.258 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
93OAK-AVE-COMP

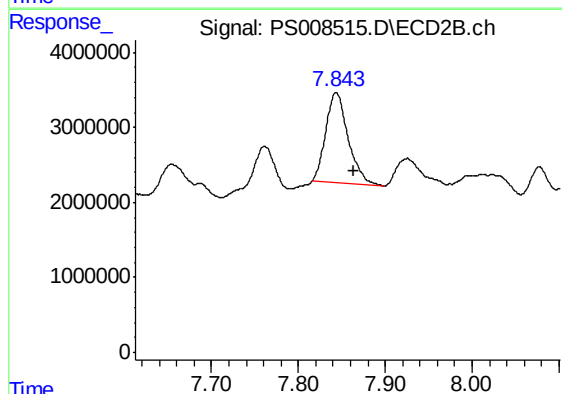


#11 2,4,5-TP (SILVEX)

R.T.: 7.844 min
Delta R.T.: -0.020 min
Response: 21584093
Conc: 4.13 ng/ml

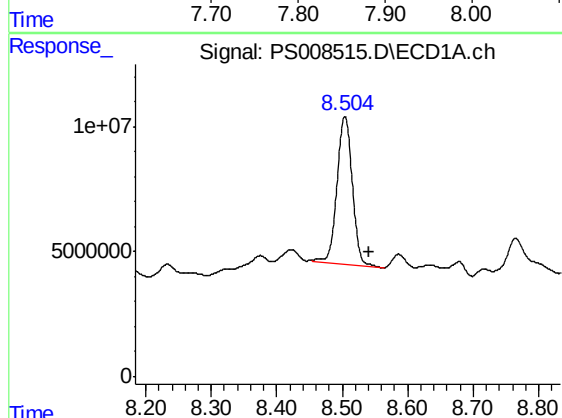


#12 2,4,5-T

R.T.: 8.504 min
Delta R.T.: -0.037 min
Response: 95998010
Conc: 10.40 ng/ml

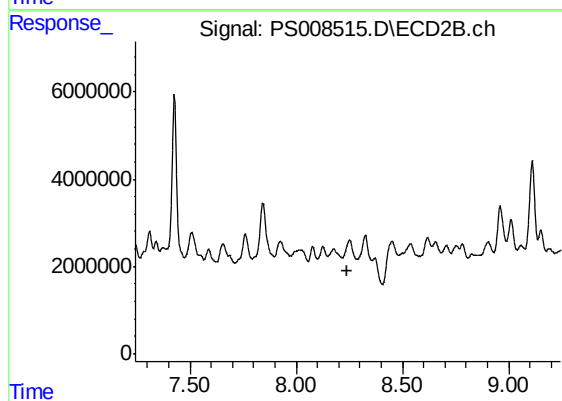

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 8.243 min
Response: 0
Conc: N.D.

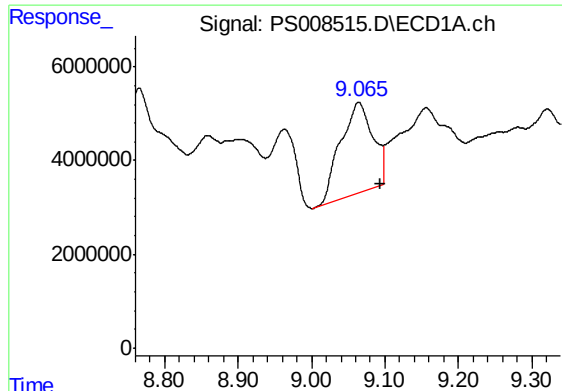

#13 2,4-DB


R.T.: 9.064 min
Delta R.T.: -0.030 min
Response: 58919149
Conc: 42.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
93OAK-AVE-COMP

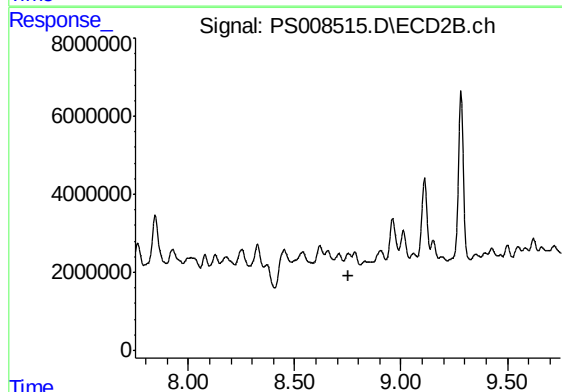


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 8.751 min
Response: 0
Conc: N.D.

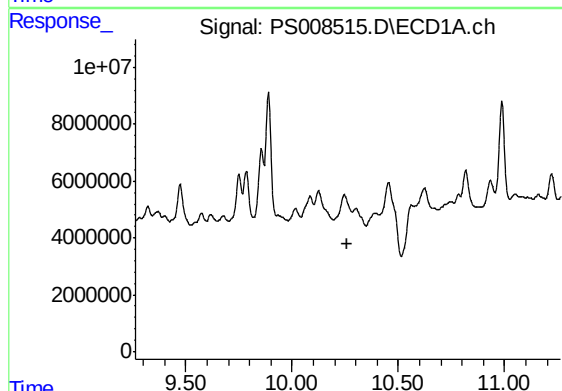


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 10.263 min
Response: 0
Conc: N.D.

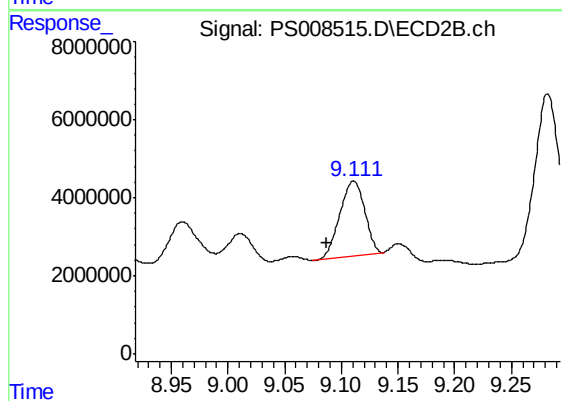

#14 DINOSEB


R.T.: 9.111 min
Delta R.T.: 0.023 min
Response: 29145358
Conc: 7.72 ng/ml

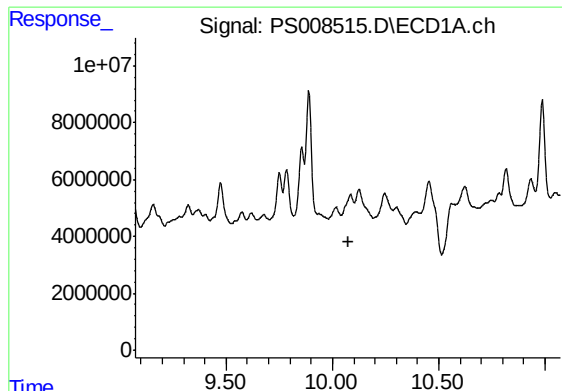

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 10.073 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
93OAK-AVE-COMP

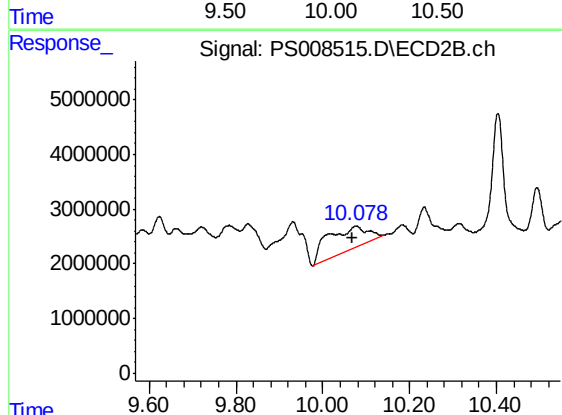


#15 Picloram

R.T.: 10.077 min
Delta R.T.: 0.009 min
Response: 28177539
Conc: 3.79 ng/ml

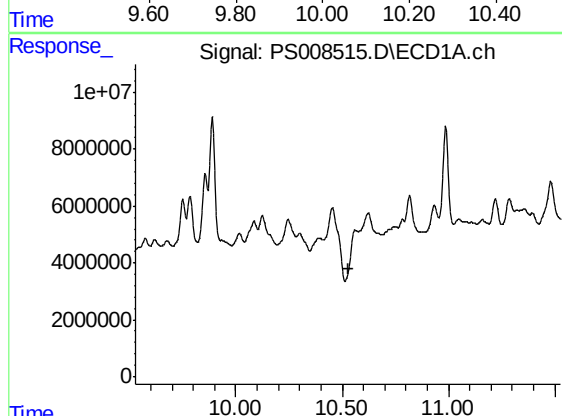

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.527 min
Response: 0
Conc: N.D.

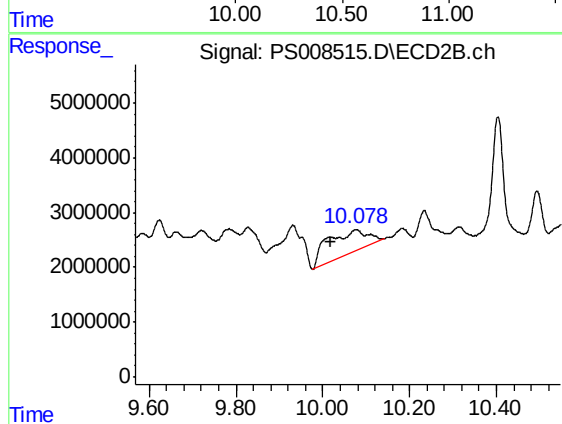

#16 DCPA

R.T.: 10.077 min
Delta R.T.: 0.058 min
Response: 28177539
Conc: 4.32 ng/ml