

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012220\
 Data File : PS008519.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jan 2020 02:56
 Operator : DD\AJ
 Sample : L1210-06
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 Q012-WC1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 22 03:47:30 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 08 11:00:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.287	5.981	428.8E6	210.4E6	242.821	222.087
Target Compounds							
2) T	3,5-DICHL...	0.000	5.168	0	110.1E6	N.D.	78.786
6) T	MCP	6.702	0.000	26217575	0	5.144	N.D. #
7) T	MCPA	6.782	6.445	32192123	36916767	4.405	8.646 #
8) T	DICHLORPROP	0.000	6.801	0	19825794	N.D.	20.520
9) T	2,4-D	0.000	7.048	0	14656162	N.D.	12.503
10) T	Pentachlo...	7.712	7.501	18064216	21975675	<MDL	1.627 #
12) T	2,4,5-T	8.489	8.309	70687004	29771080	7.661	5.630 #
13) T	2,4-DB	9.049	0.000	50628084	0	36.522	N.D. #
14) T	DINOSEB	0.000	9.097	0	22982660	N.D.	6.084
15) T	Picloram	0.000	10.059	0	22670897	N.D.	3.052
16) T	DCPA	0.000	10.059	0	22670897	N.D.	3.479



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012220\
Data File : PS008519.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jan 2020 02:56
Operator : DD\AJ
Sample : L1210-06
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
Q012-WC1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 22 03:47:30 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
Quant Title : 8080.M
QLast Update : Wed Jan 08 11:00:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

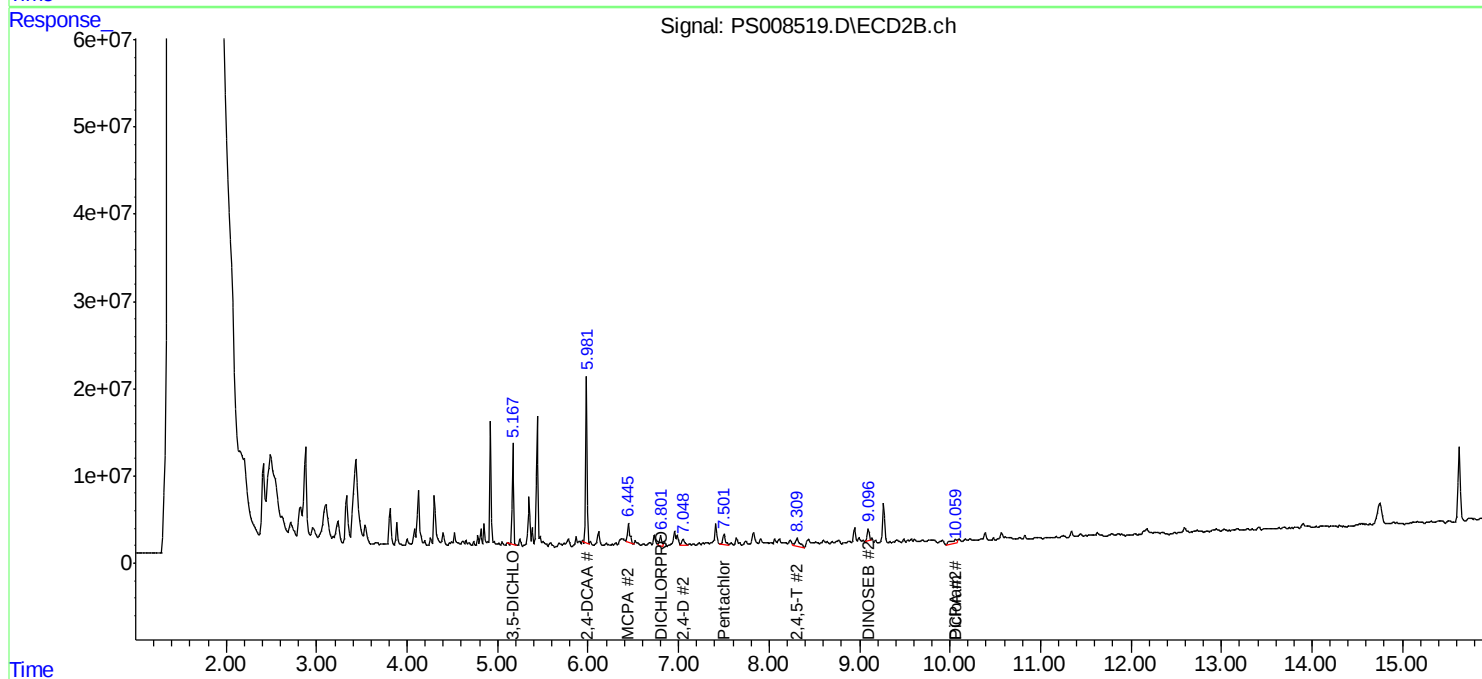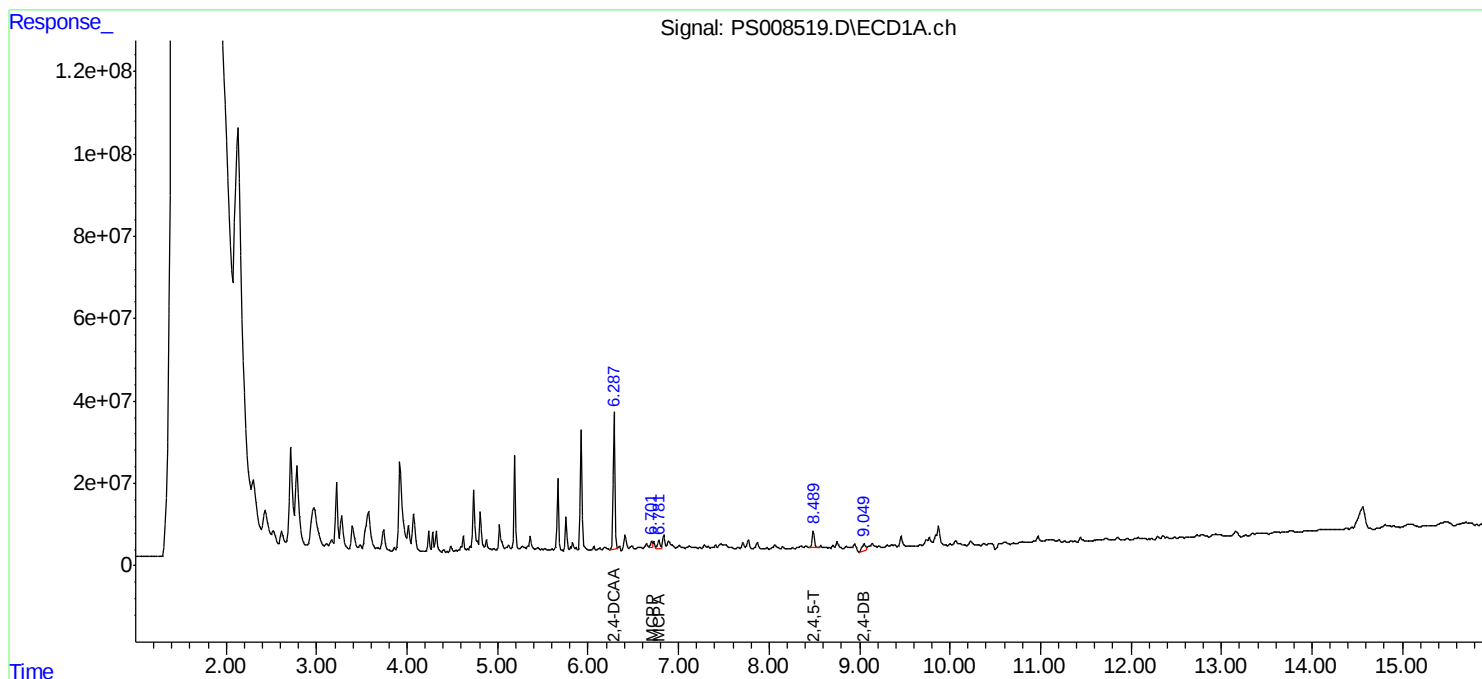


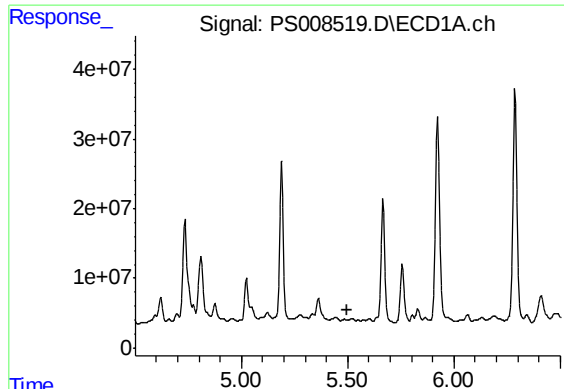

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 5.501 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
Q012-WC1

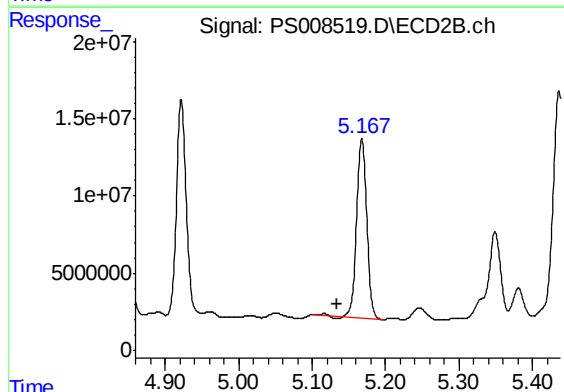


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.168 min
Delta R.T.: 0.034 min
Response: 110078191
Conc: 78.79 ng/ml

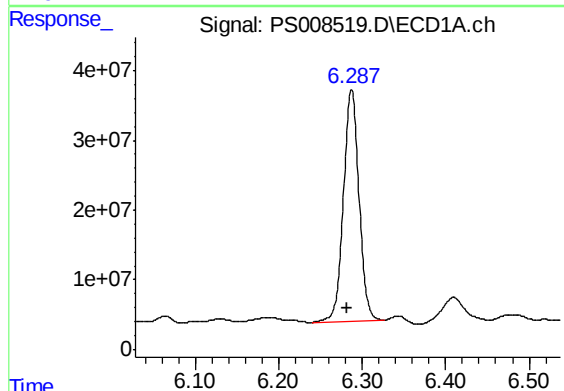


#4 2,4-DCAA

R.T.: 6.287 min
Delta R.T.: 0.005 min
Response: 428750222
Conc: 242.82 ng/ml

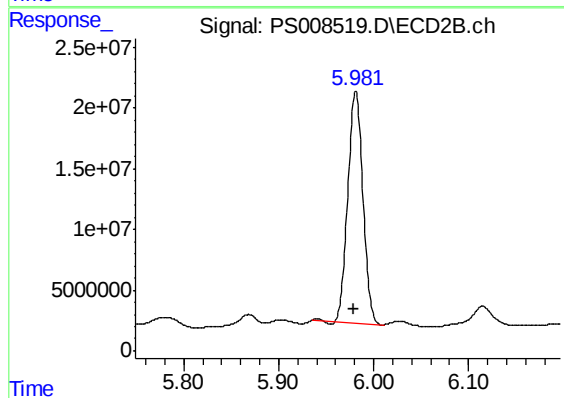

#4 2,4-DCAA


R.T.: 5.981 min
Delta R.T.: 0.002 min
Response: 210419134
Conc: 222.09 ng/ml

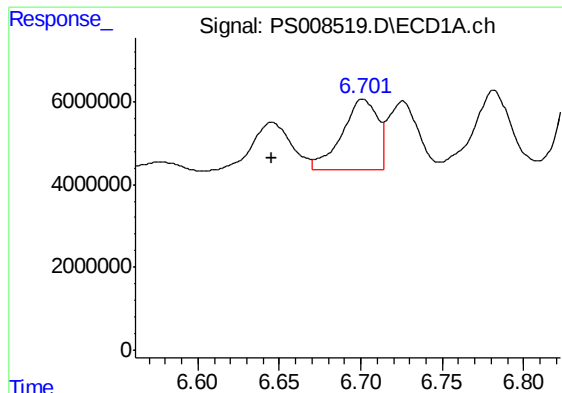

#6 MCPP


R.T.: 6.702 min
Delta R.T.: 0.056 min
Response: 26217575
Conc: 5.14 ug/ml

Instrument :
ECD_S
ClientSampleId :
Q012-WC1

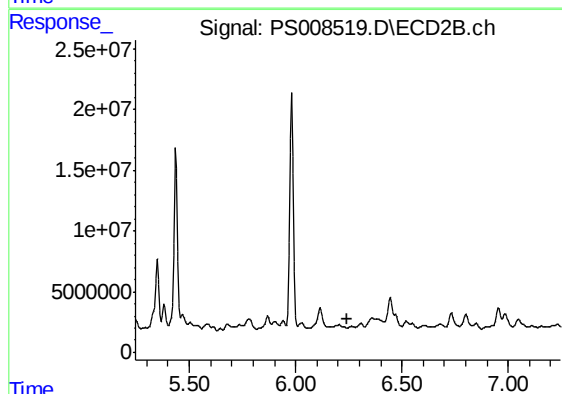


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 6.246 min
Response: 0
Conc: N.D.

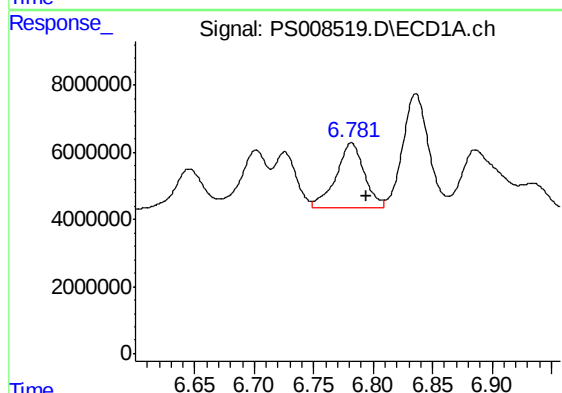


#7 MCPA

R.T.: 6.782 min
Delta R.T.: -0.013 min
Response: 32192123
Conc: 4.41 ug/ml

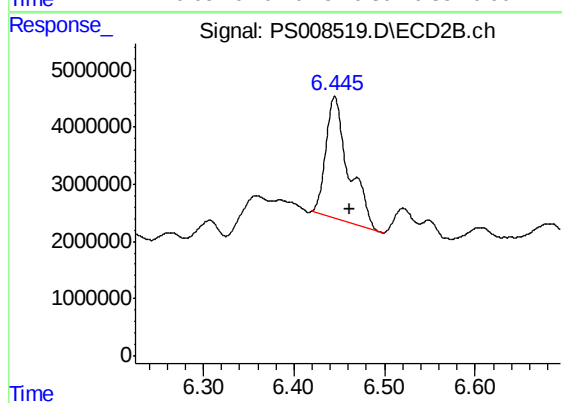

#7 MCPA


R.T.: 6.445 min
Delta R.T.: -0.017 min
Response: 36916767
Conc: 8.65 ug/ml

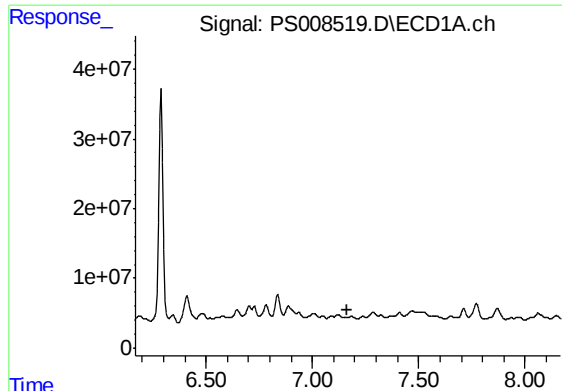

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 7.167 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
Q012-WC1

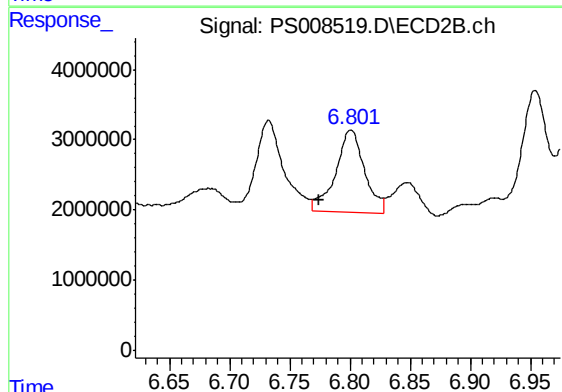


#8 DICHLORPROP

R.T.: 6.801 min
Delta R.T.: 0.026 min
Response: 19825794
Conc: 20.52 ng/ml

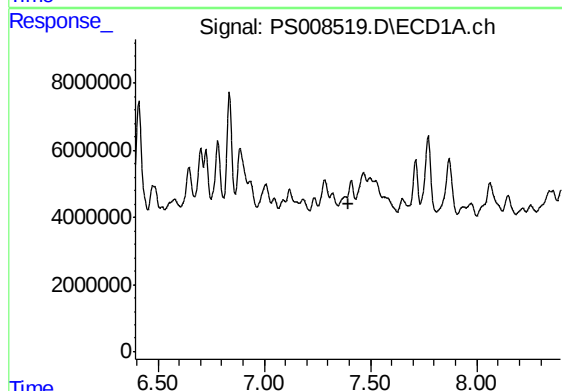


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.394 min
Response: 0
Conc: N.D.

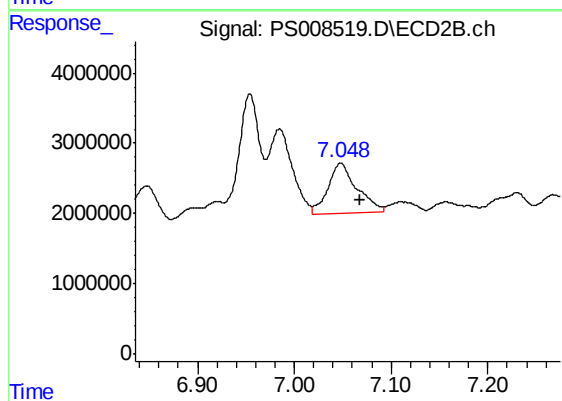

#9 2,4-D


R.T.: 7.048 min
Delta R.T.: -0.021 min
Response: 14656162
Conc: 12.50 ng/ml

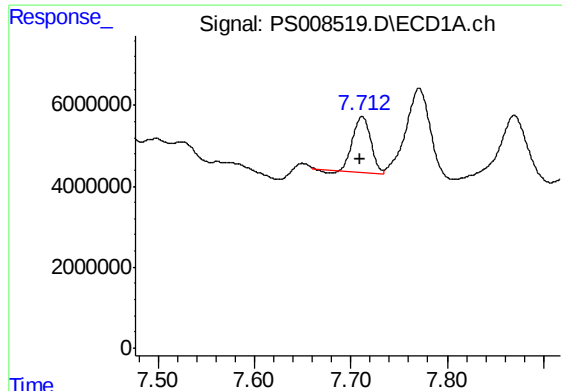

#10 Pentachlorophenol


R.T.: 7.712 min
Delta R.T.: 0.002 min
Response: 18064216
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
Q012-WC1

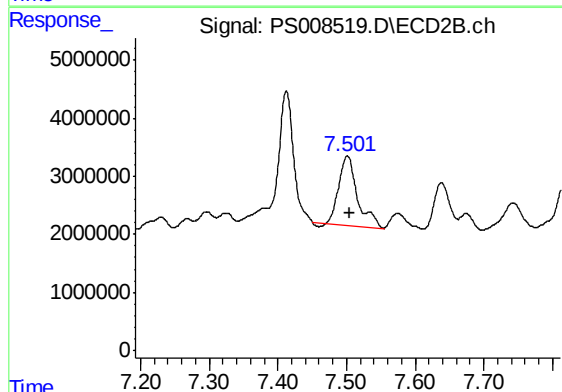


#10 Pentachlorophenol

R.T.: 7.501 min
Delta R.T.: -0.004 min
Response: 21975675
Conc: 1.63 ng/ml

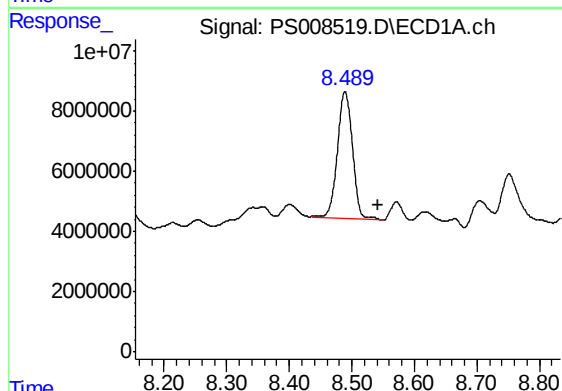


#12 2,4,5-T

R.T.: 8.489 min
Delta R.T.: -0.052 min
Response: 70687004
Conc: 7.66 ng/ml

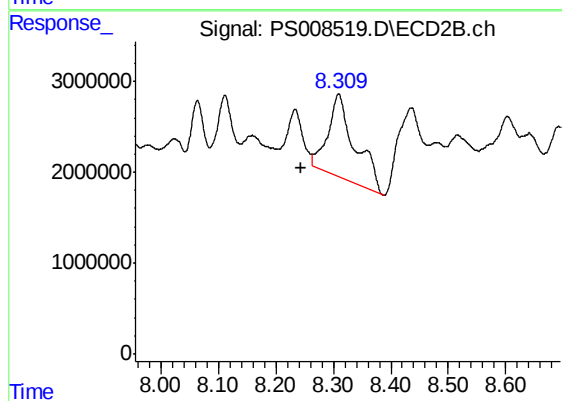

#12 2,4,5-T


R.T.: 8.309 min
Delta R.T.: 0.066 min
Response: 29771080
Conc: 5.63 ng/ml

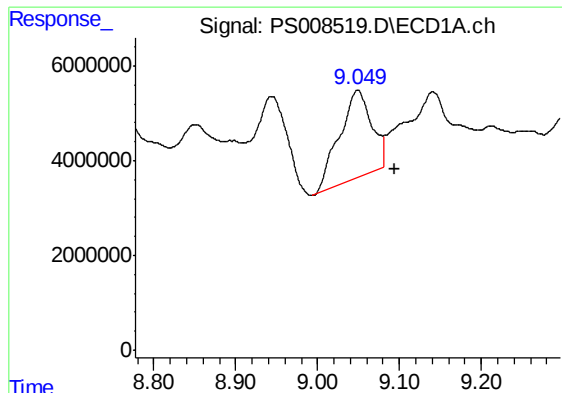

#13 2,4-DB


R.T.: 9.049 min
Delta R.T.: -0.046 min
Response: 50628084
Conc: 36.52 ng/ml

Instrument :
ECD_S
ClientSampleId :
Q012-WC1

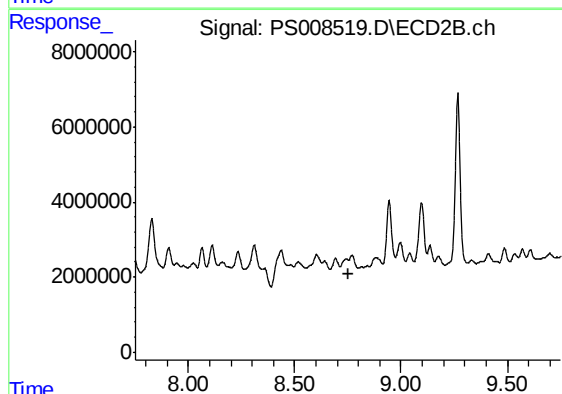


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 8.751 min
Response: 0
Conc: N.D.

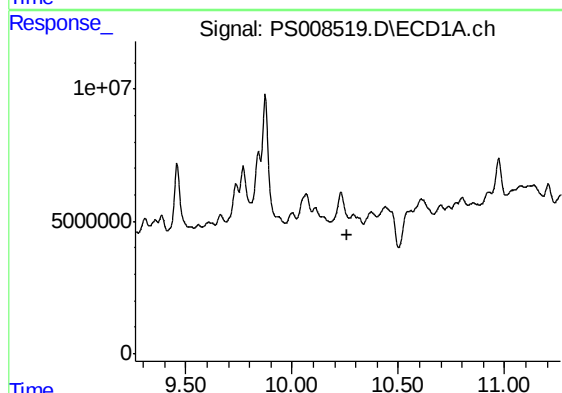


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 10.263 min
Response: 0
Conc: N.D.

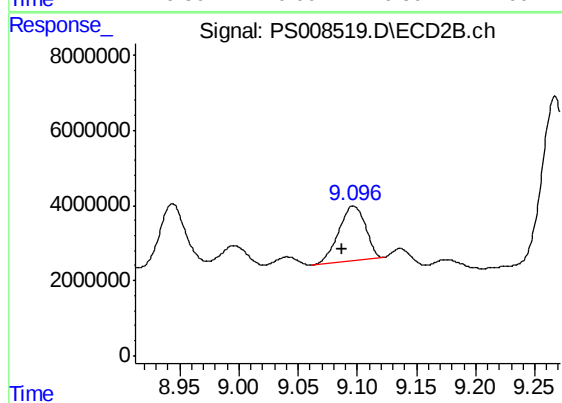

#14 DINOSEB


R.T.: 9.097 min
Delta R.T.: 0.009 min
Response: 22982660
Conc: 6.08 ng/ml

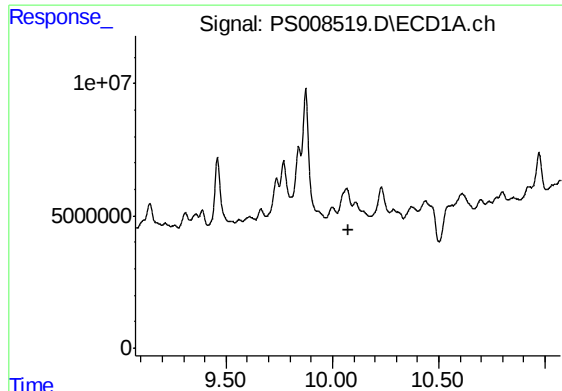

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 10.073 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
Q012-WC1

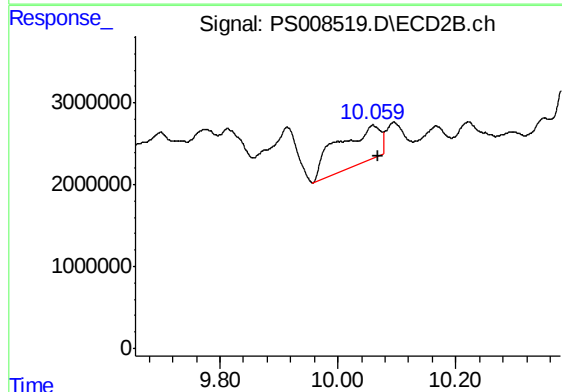


#15 Picloram

R.T.: 10.059 min
Delta R.T.: -0.008 min
Response: 22670897
Conc: 3.05 ng/ml

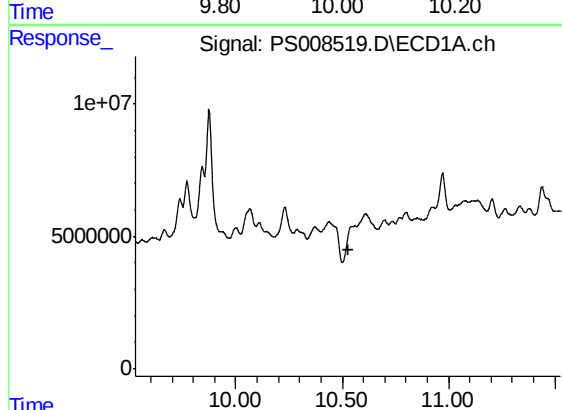

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.527 min
Response: 0
Conc: N.D.

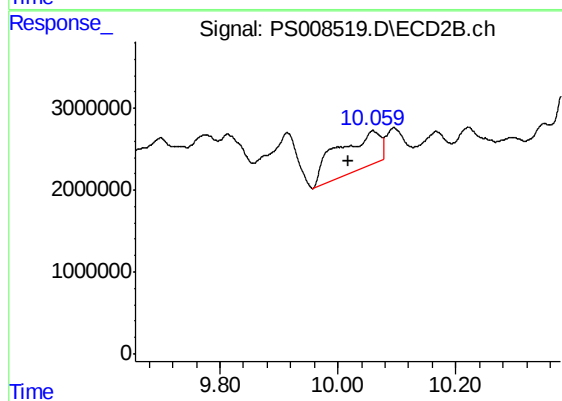

#16 DCPA

R.T.: 10.059 min
Delta R.T.: 0.040 min
Response: 22670897
Conc: 3.48 ng/ml