

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012224\
 Data File : PS025612.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jan 2024 22:46
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 23 00:35:38 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS011124.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 11 16:45:24 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	6.350	6.759	785.1E6	415.7E6	527.125	541.460
Target Compounds						
1) T Dalapon	0.000	2.552	0	306267	N.D.	<MDL
5) T DICAMBA	0.000	6.956	0	358795	N.D.	<MDL
6) T MCPP	0.000	6.956f	0	358795	N.D.	<MDL
7) T MCPA	0.000	7.237	0	2982139	N.D.	<MDL
8) T DICHLORPROP	0.000	7.550	0	3258680	N.D.	3.770
11) T 2,4,5-TP ...	0.000	8.548f	0	105761	N.D.	<MDL
12) T 2,4,5-T	0.000	8.982	0	4990	N.D.	<MDL
14) T DINOSEB	0.000	9.793	0	213480	N.D.	<MDL
15) T Picloram	0.000	10.785	0	149019	N.D.	<MDL
16) T DCPA	0.000	10.708	0	461202	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012224\
Data File : PS025612.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jan 2024 22:46
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 23 00:35:38 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS011124.M
Quant Title : 8080.M
QLast Update : Thu Jan 11 16:45:24 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

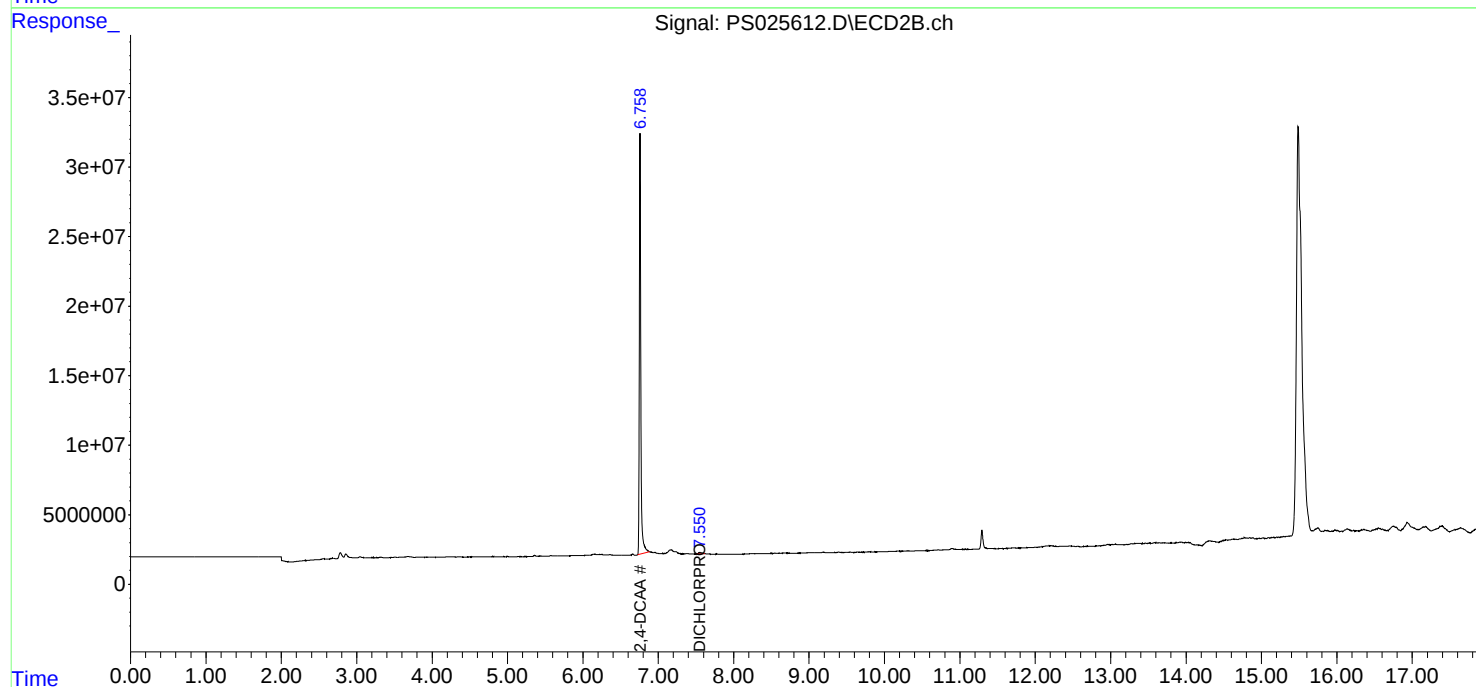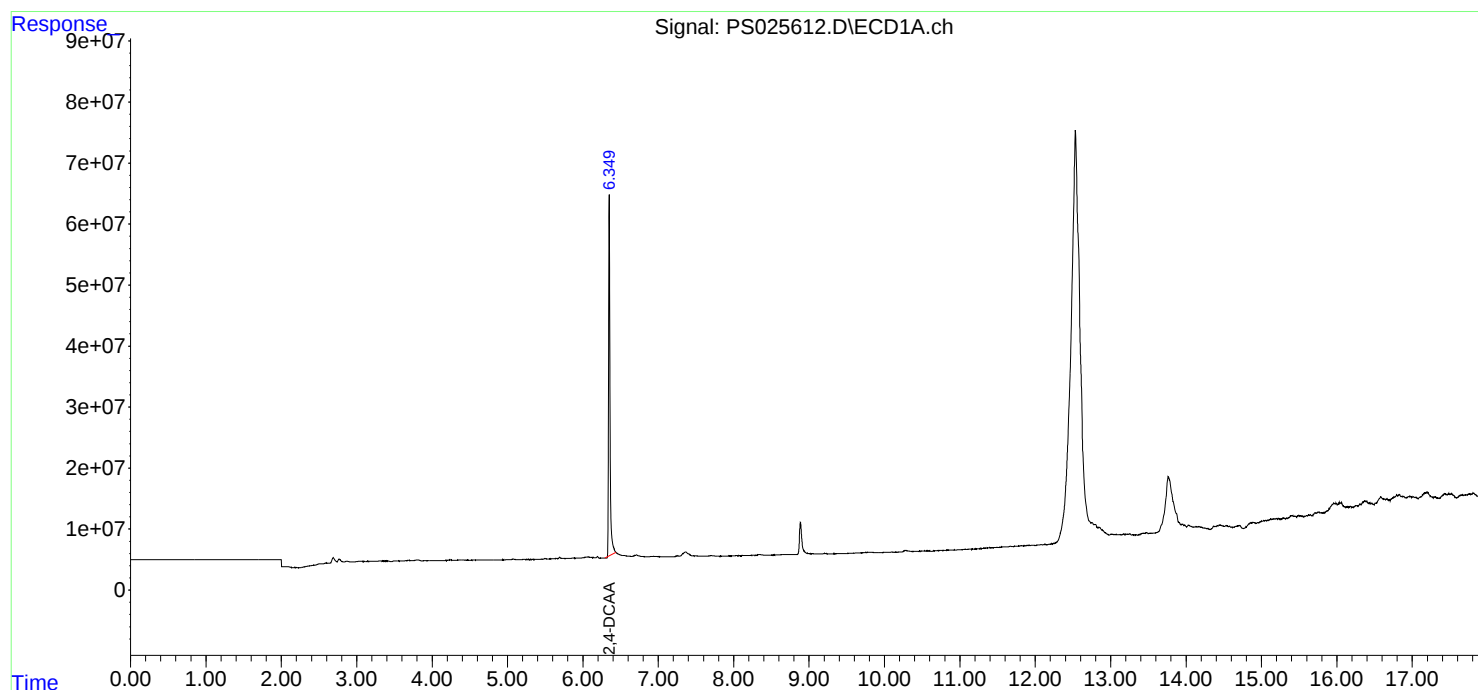


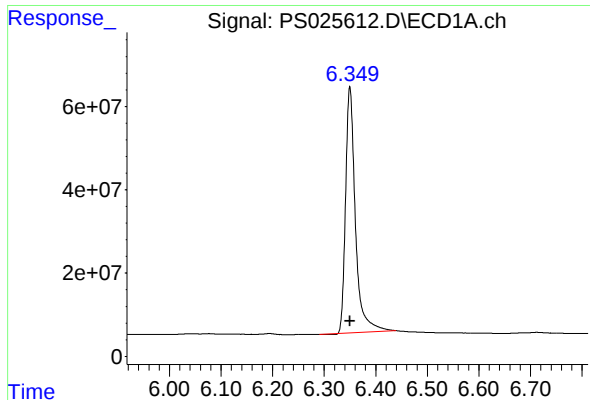

#4 2,4-DCAA


R.T.: 6.350 min
Delta R.T.: 0.000 min
Response: 785133965
Conc: 527.13 ng/ml

Instrument :
ECD_S
ClientSampleId :

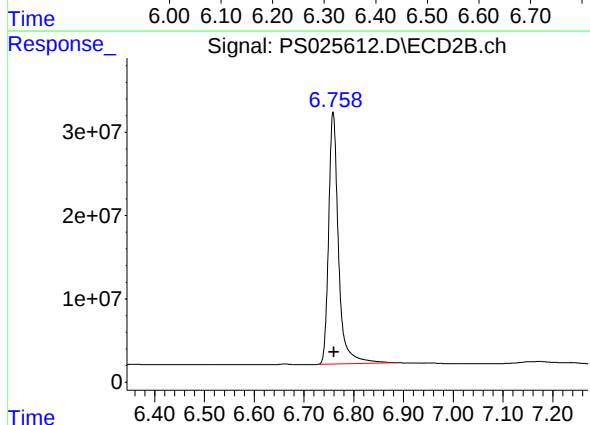


#4 2,4-DCAA

R.T.: 6.759 min
Delta R.T.: -0.002 min
Response: 415732939
Conc: 541.46 ng/ml

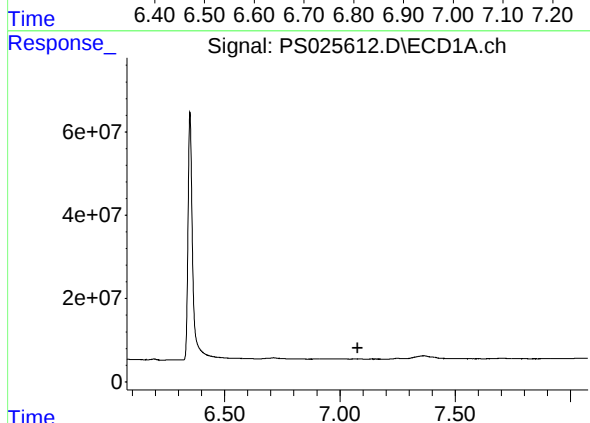

#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.077 min
Response: 0
Conc: N.D.

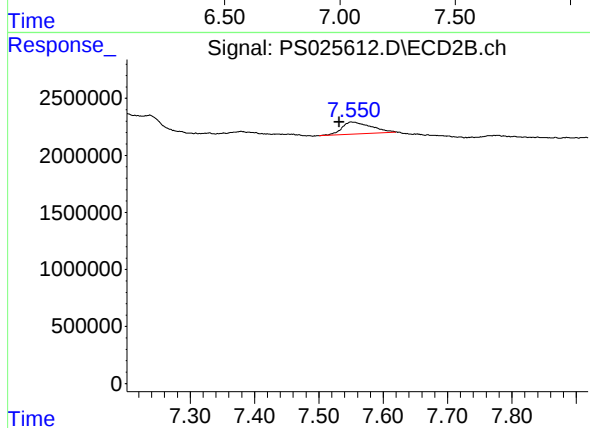

#8 DICHLORPROP

R.T.: 7.550 min
Delta R.T.: 0.019 min
Response: 3258680
Conc: 3.77 ng/ml