

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012225\
 Data File : PS028950.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jan 2025 18:10
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 23 08:54:44 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS011425.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 14 12:25:39 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.194	7.673	1335.4E6	541.0E6	479.667	484.805
Target Compounds							
1) T	Dalapon	2.598	2.712f	475202	14616536	<MDL	7.164 #
2) T	3,5-DICHL...	6.354	0.000	3343901	0	<MDL	N.D. #
3) T	4-Nitroph...	6.990	0.000	5823389	0	3.286	N.D. #
5) T	DICAMBA	0.000	7.873	0	3836255	N.D.	<MDL
6) T	MCPD	7.521f	7.966	435643	2914197	<MDL	<MDL #
7) T	MCPA	7.733	8.208	909026	5903060	<MDL	1.390 #
8) T	DICHLORPROP	8.102	8.630f	310037	6998469	<MDL	4.979 #
10) T	Pentachlo...	8.610	0.000	2877983	0	<MDL	N.D. #
12) T	2,4,5-T	9.484	10.230	-98304	4258955	N.D.	<MDL
13) T	2,4-DB	10.070	0.000	744821	0	<MDL	N.D. #
14) T	DINOSEB	11.239	0.000	6331912	0	<MDL	N.D. #
15) T	Picloram	11.076	12.261	55207561	9275048	1.750	<MDL #
16) T	DCPA	11.534	12.261f	9685324	9275048	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012225\
Data File : PS028950.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jan 2025 18:10
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 23 08:54:44 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS011425.M
Quant Title : 8080.M
QLast Update : Tue Jan 14 12:25:39 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

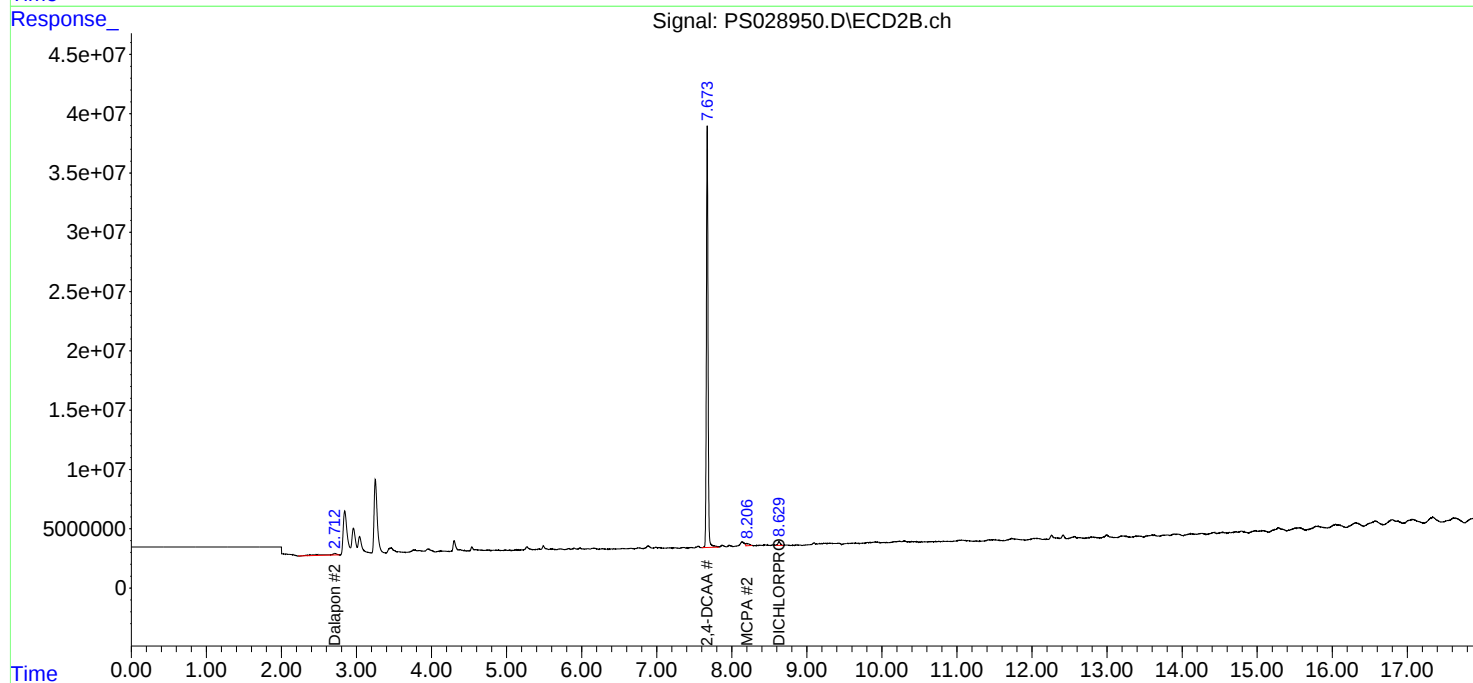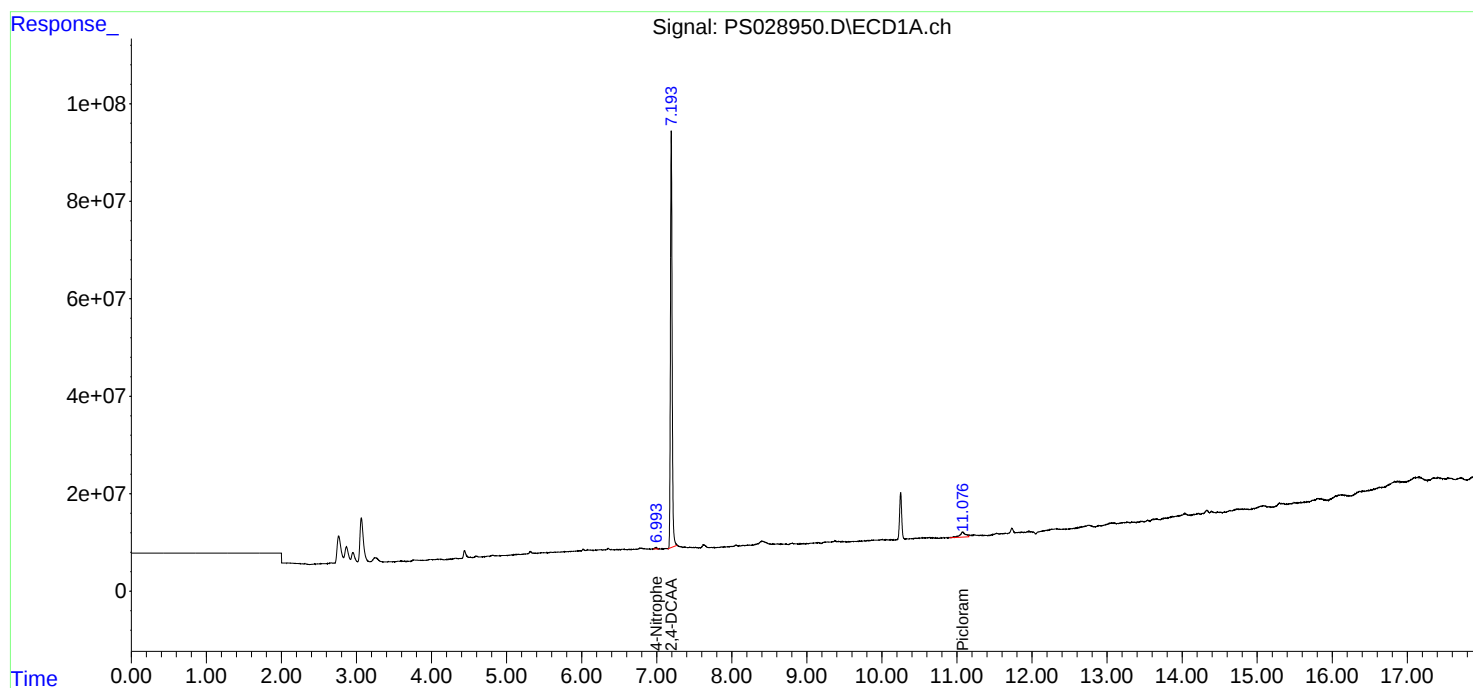


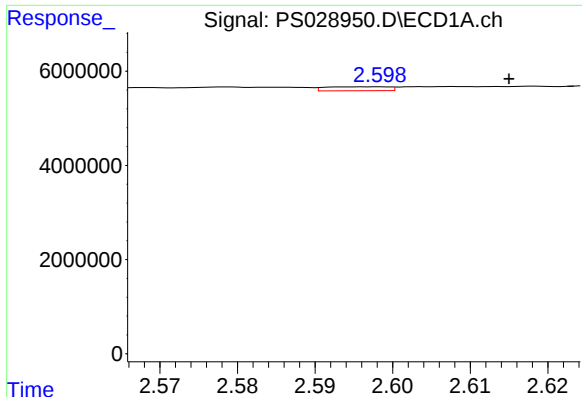

#1 Dalapon


R.T.: 2.598 min
Delta R.T.: -0.017 min
Response: 475202
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

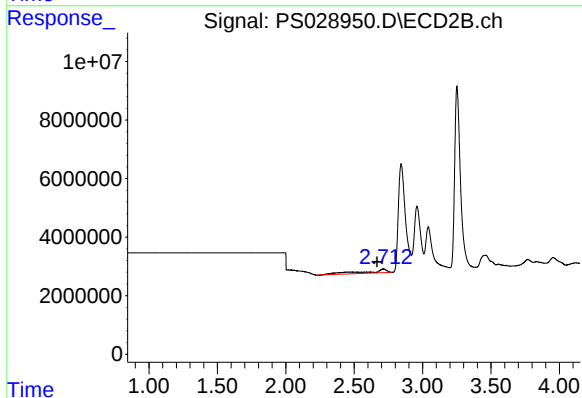


#1 Dalapon

R.T.: 2.712 min
Delta R.T.: 0.045 min
Response: 14616536
Conc: 7.16 ng/ml

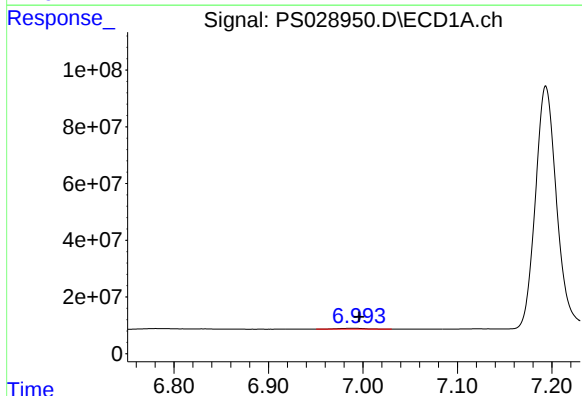


#3 4-Nitrophenol

R.T.: 6.990 min
Delta R.T.: -0.006 min
Response: 5823389
Conc: 3.29 ng/ml

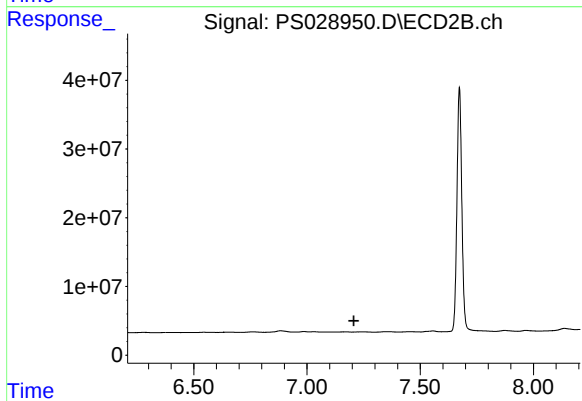

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.207 min
Response: 0
Conc: N.D.

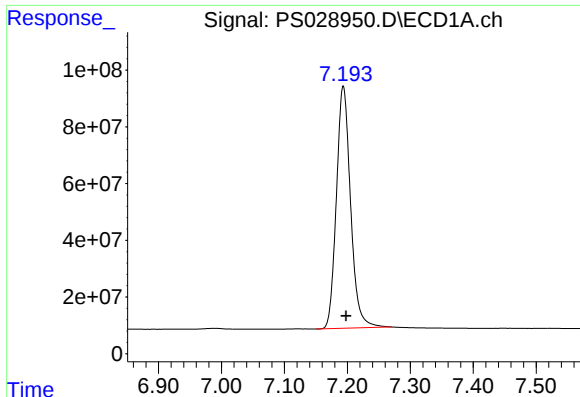

#4 2,4-DCAA


R.T.: 7.194 min
Delta R.T.: -0.004 min
Response: 1335397709
Conc: 479.67 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

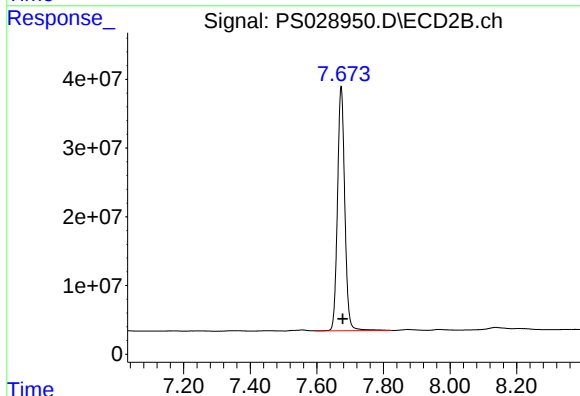


#4 2,4-DCAA

R.T.: 7.673 min
Delta R.T.: -0.005 min
Response: 540951550
Conc: 484.80 ng/ml

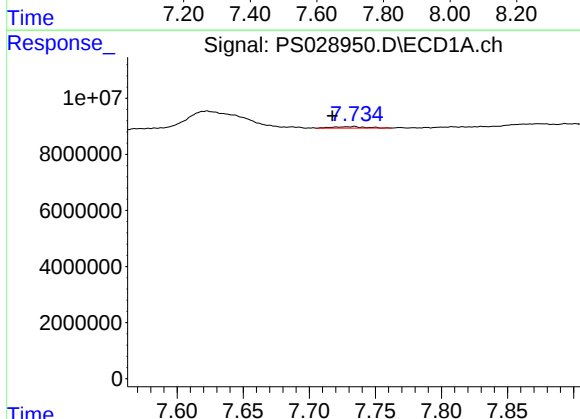


#7 MCPA

R.T.: 7.733 min
Delta R.T.: 0.016 min
Response: 909026
Conc: N.D.

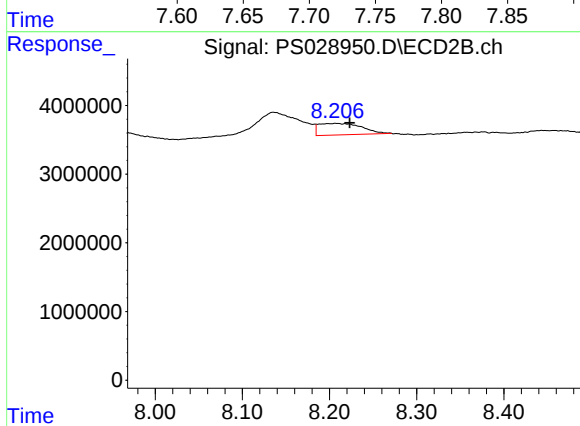

#7 MCPA


R.T.: 8.208 min
Delta R.T.: -0.016 min
Response: 5903060
Conc: 1.39 ug/ml

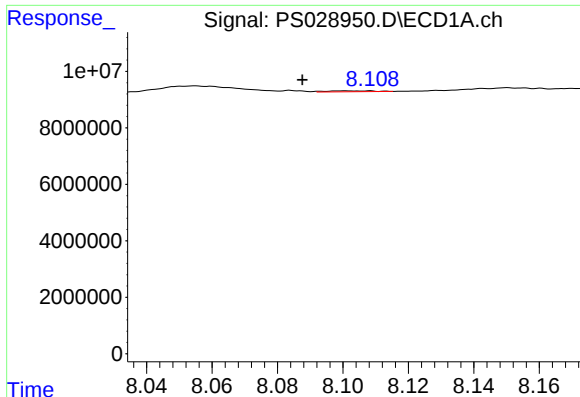

#8 DICHLORPROP


R.T.: 8.102 min
Delta R.T.: 0.014 min
Response: 310037
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

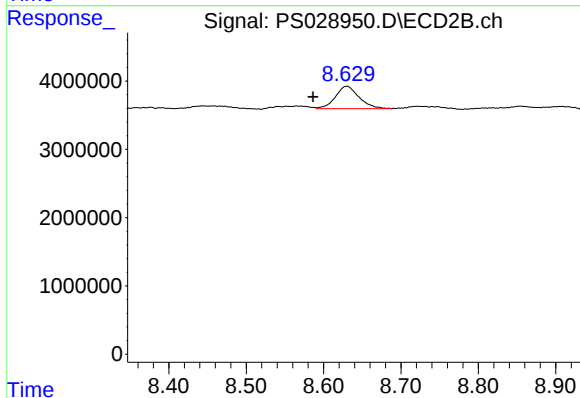


#8 DICHLORPROP

R.T.: 8.630 min
Delta R.T.: 0.044 min
Response: 6998469
Conc: 4.98 ng/ml

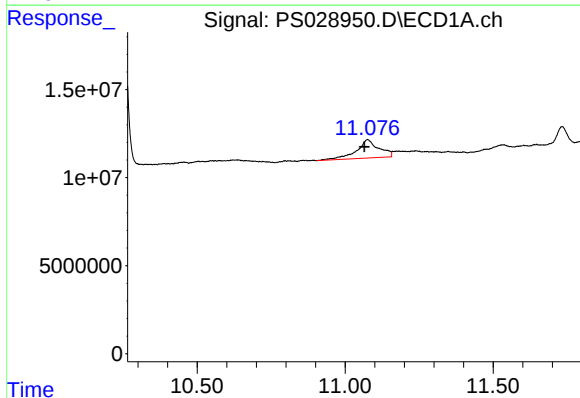

#15 Picloram

R.T.: 11.076 min
Delta R.T.: 0.011 min
Response: 55207561
Conc: 1.75 ng/ml

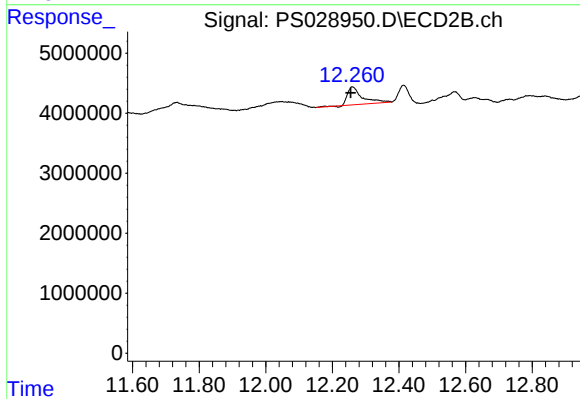

#15 Picloram

R.T.: 12.261 min
Delta R.T.: 0.005 min
Response: 9275048
Conc: N.D.