

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012323\
 Data File : PS021838.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jan 2023 09:40
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 23 20:51:45 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010923.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 10 10:34:52 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.381	6.809	1557.6E6	1105.7E6	559.574	615.418
Target Compounds							
1) T	Dalapon	2.474	0.000	302196	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.810f	0.000	517559	0	<MDL	N.D. #
3) T	4-Nitroph...	6.228	0.000	5288214	0	3.628	N.D. #
5) T	DICAMBA	0.000	6.992	0	25766032	N.D.	3.030
6) T	MCPD	0.000	7.049	0	28262171	N.D.	4.262
7) T	MCPA	6.762	0.000	5270505	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.626	0	6326615	N.D.	2.965
9) T	2,4-D	7.300	0.000	26386983	0	6.794	N.D. #
10) T	Pentachlo...	7.546	0.000	1692507	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.090	8.650	1931410	6843941	<MDL	<MDL #
12) T	2,4,5-T	8.312	0.000	16767542	0	<MDL	N.D. #
13) T	2,4-DB	8.838	9.497f	628476	15254883	<MDL	10.182 #
15) T	Picloram	0.000	10.903f	0	30545987	N.D.	1.725
16) T	DCPA	10.155	0.000	522861	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012323\
Data File : PS021838.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jan 2023 09:40
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 23 20:51:45 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010923.M
Quant Title : 8080.M
QLast Update : Tue Jan 10 10:34:52 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

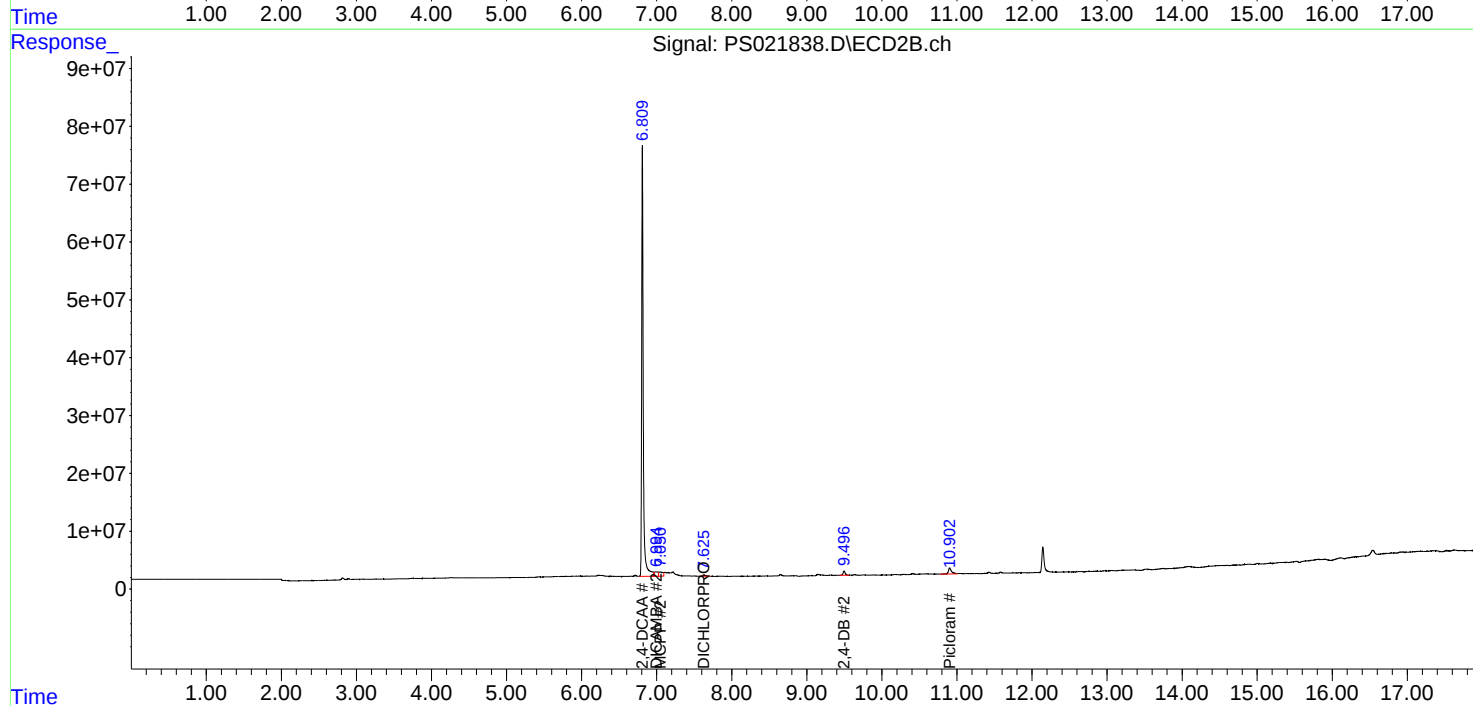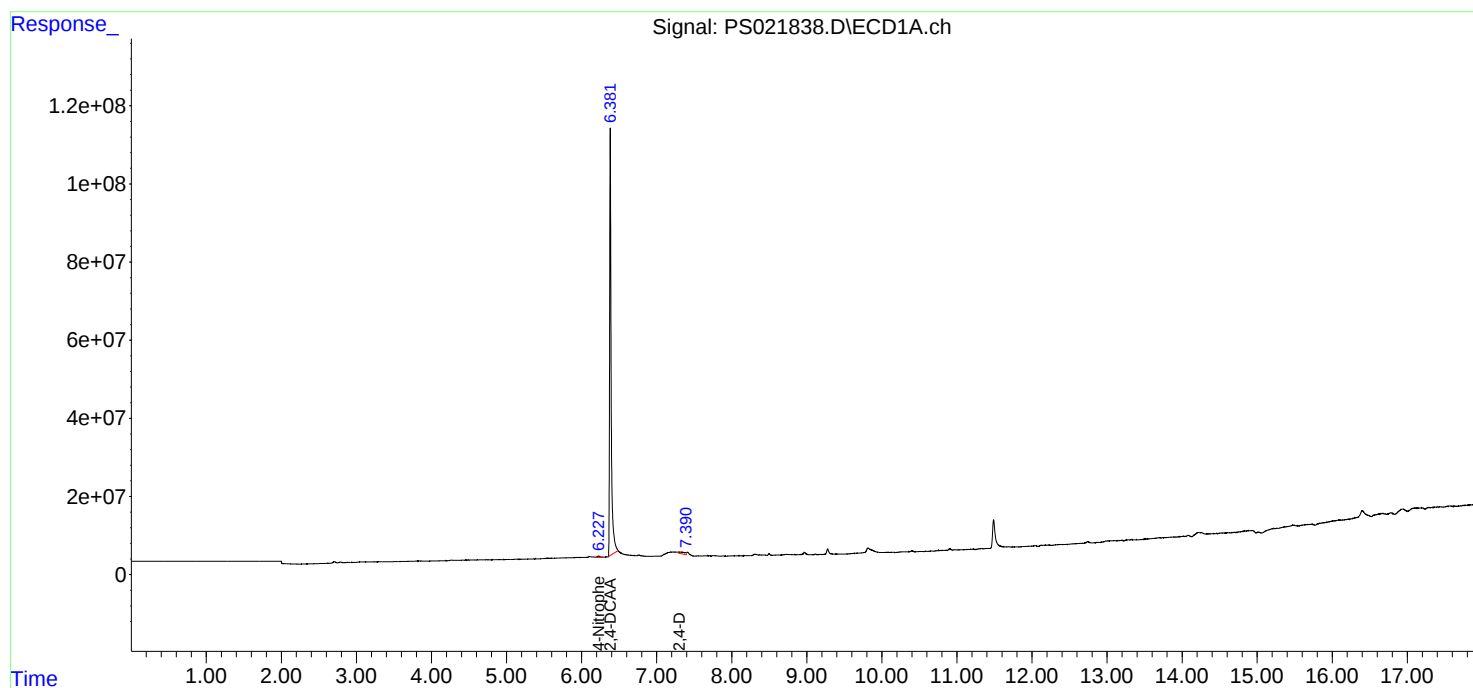


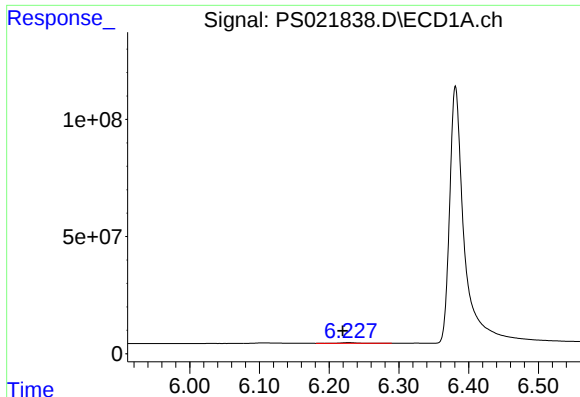

#3 4-Nitrophenol


R.T.: 6.228 min
Delta R.T.: 0.008 min
Response: 5288214
Conc: 3.63 ng/ml

Instrument :
ECD_S
ClientSampleId :

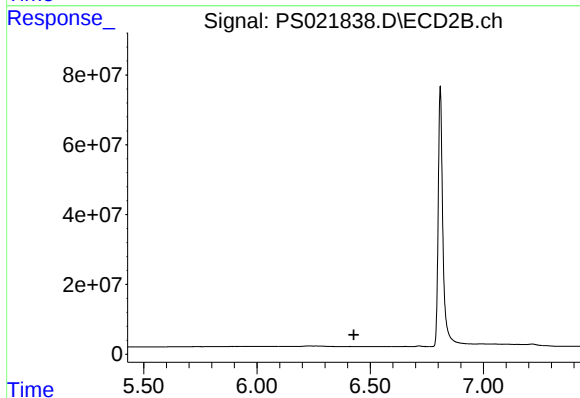


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.428 min
Response: 0
Conc: N.D.

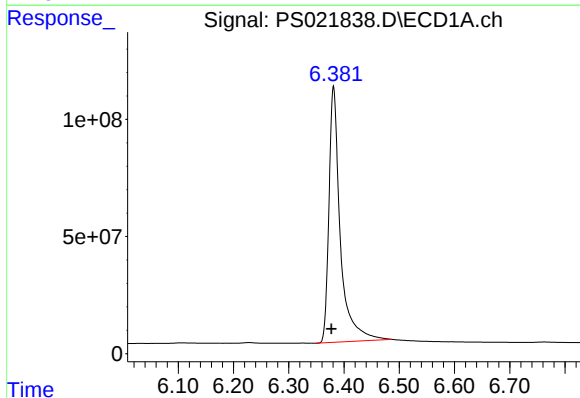


#4 2,4-DCAA

R.T.: 6.381 min
Delta R.T.: 0.004 min
Response: 1557612033
Conc: 559.57 ng/ml

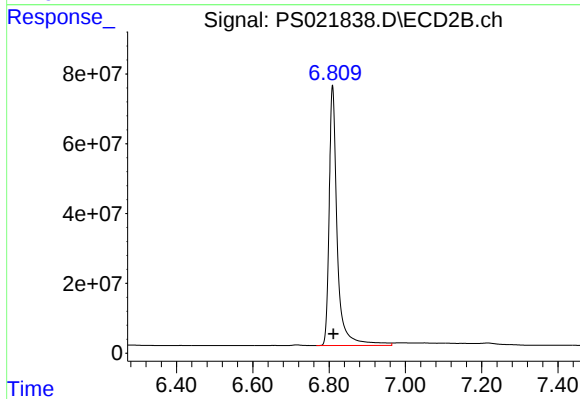

#4 2,4-DCAA


R.T.: 6.809 min
Delta R.T.: -0.002 min
Response: 1105714263
Conc: 615.42 ng/ml

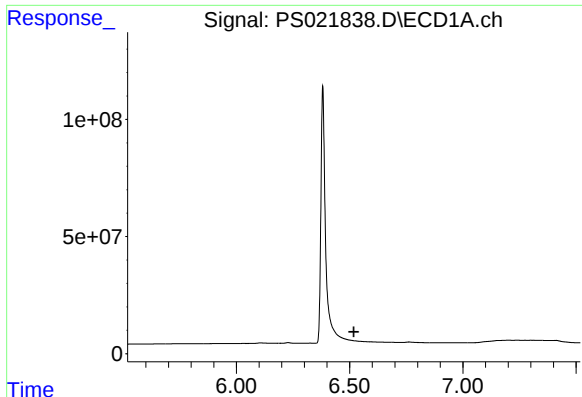

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 6.518 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

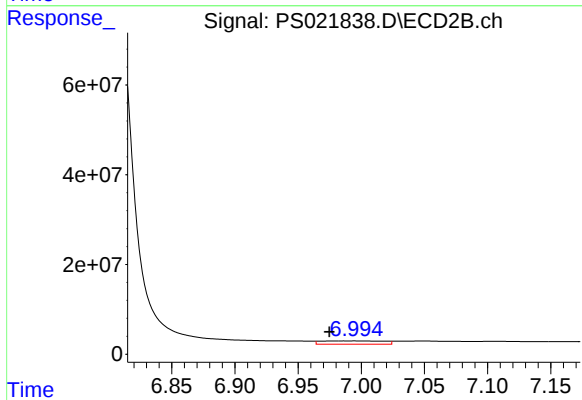


#5 DICAMBA

R.T.: 6.992 min
Delta R.T.: 0.017 min
Response: 25766032
Conc: 3.03 ng/ml

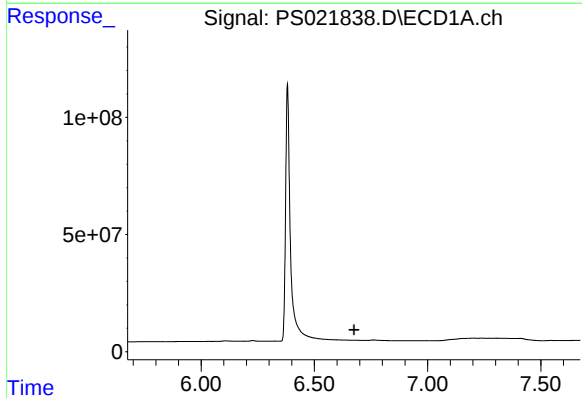


#6 MCP

R.T.: 0.000 min
Exp R.T.: 6.675 min
Response: 0
Conc: N.D.

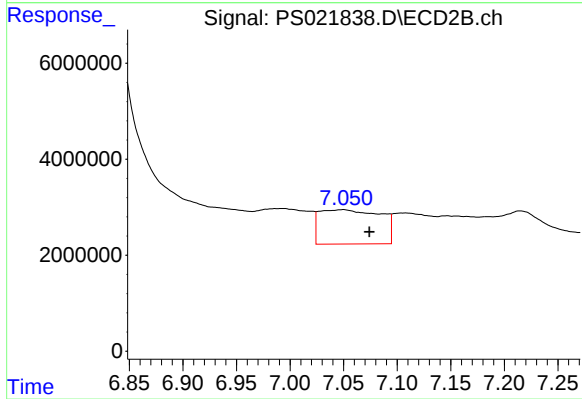

#6 MCP


R.T.: 7.049 min
Delta R.T.: -0.025 min
Response: 28262171
Conc: 4.26 ug/ml

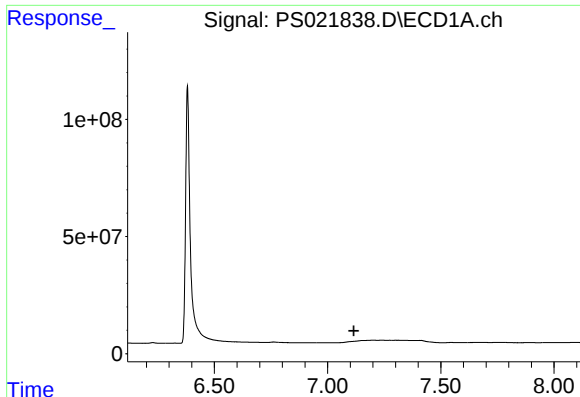

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.117 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

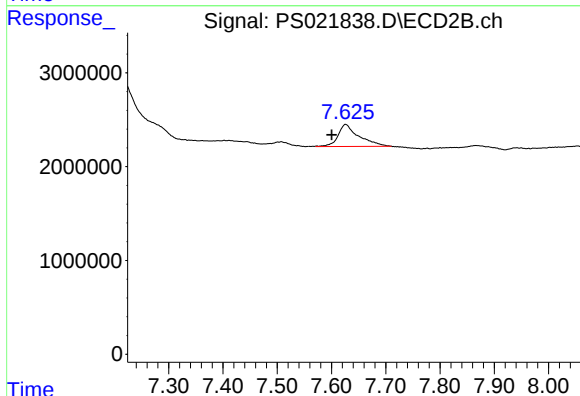


#8 DICHLORPROP

R.T.: 7.626 min
Delta R.T.: 0.026 min
Response: 6326615
Conc: 2.97 ng/ml

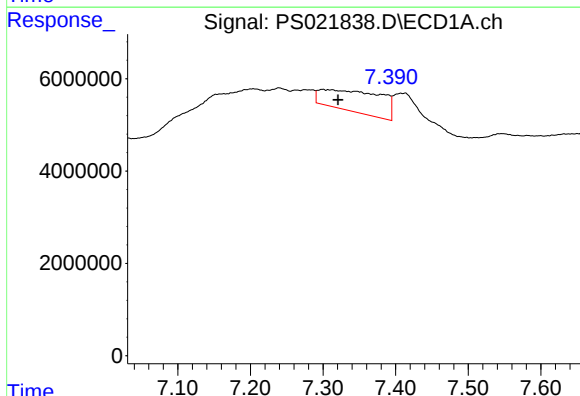


#9 2,4-D

R.T.: 7.300 min
Delta R.T.: -0.021 min
Response: 26386983
Conc: 6.79 ng/ml

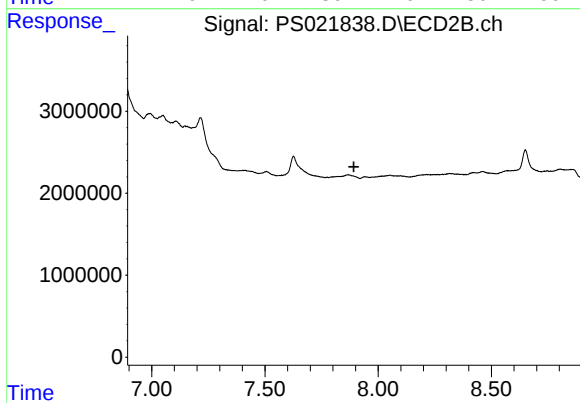

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.893 min
Response: 0
Conc: N.D.

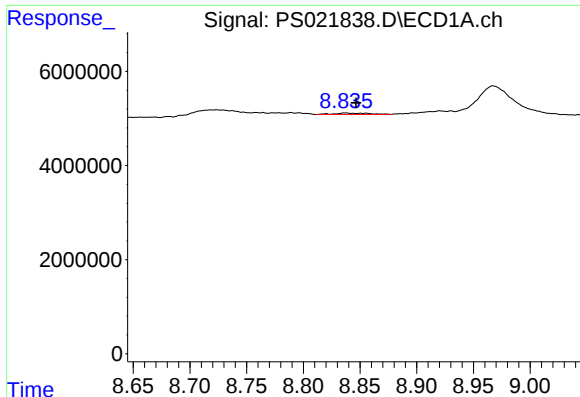

#13 2,4-DB


R.T.: 8.838 min
Delta R.T.: -0.009 min
Response: 628476
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

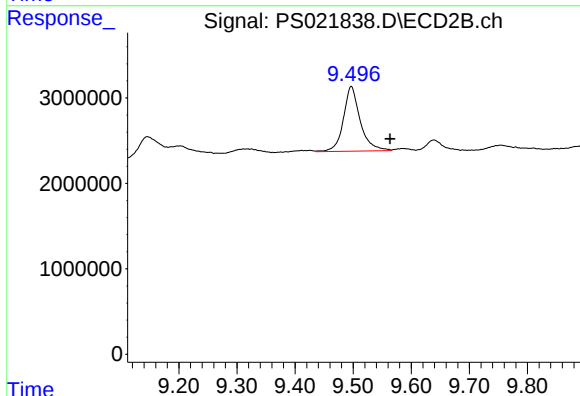


#13 2,4-DB

R.T.: 9.497 min
Delta R.T.: -0.067 min
Response: 15254883
Conc: 10.18 ng/ml

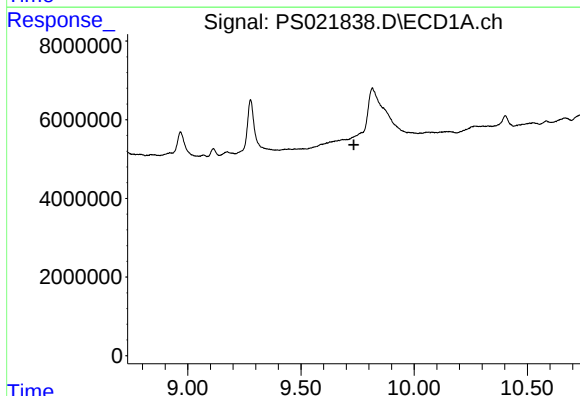

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.734 min
Response: 0
Conc: N.D.

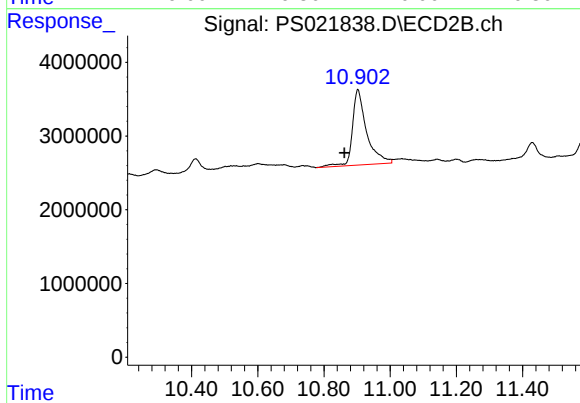

#15 Picloram

R.T.: 10.903 min
Delta R.T.: 0.040 min
Response: 30545987
Conc: 1.72 ng/ml