

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012324\
 Data File : PS025623.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jan 2024 09:14
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 23 23:59:22 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS011124.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 11 16:45:24 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

1) T	Dalapon	0.000	2.553	0	2753076	N.D.	2.343
2) T	3,5-DICHL...	5.693	0.000	254.7E6	0	111.306	N.D. #
5) T	DICAMBA	0.000	6.956	0	912.9E6	N.D.	274.326
6) T	MCPD	6.707f	6.956f	3927442	912.9E6	<MDL	393.536 #
7) T	MCPA	6.707f	0.000	3927442	0	<MDL	N.D. #
8) T	DICHLORPROP	7.072	7.559	972632	3970866	<MDL	4.594 #
9) T	2,4-D	7.236	0.000	3151.4E6	0	1711.459	N.D. #
10) T	Pentachlo...	0.000	8.233	0	1172556	N.D.	<MDL
13) T	2,4-DB	0.000	9.458	0	515534	N.D.	<MDL
14) T	DINOSEB	0.000	9.800	0	18455769	N.D.	5.871
15) T	Picloram	9.646	10.770	230.5E6	22455313	22.275	4.223 #
16) T	DCPA	0.000	10.724	0	13662487	N.D.	2.350



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012324\
Data File : PS025623.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jan 2024 09:14
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 23 23:59:22 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS011124.M
Quant Title : 8080.M
QLast Update : Thu Jan 11 16:45:24 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

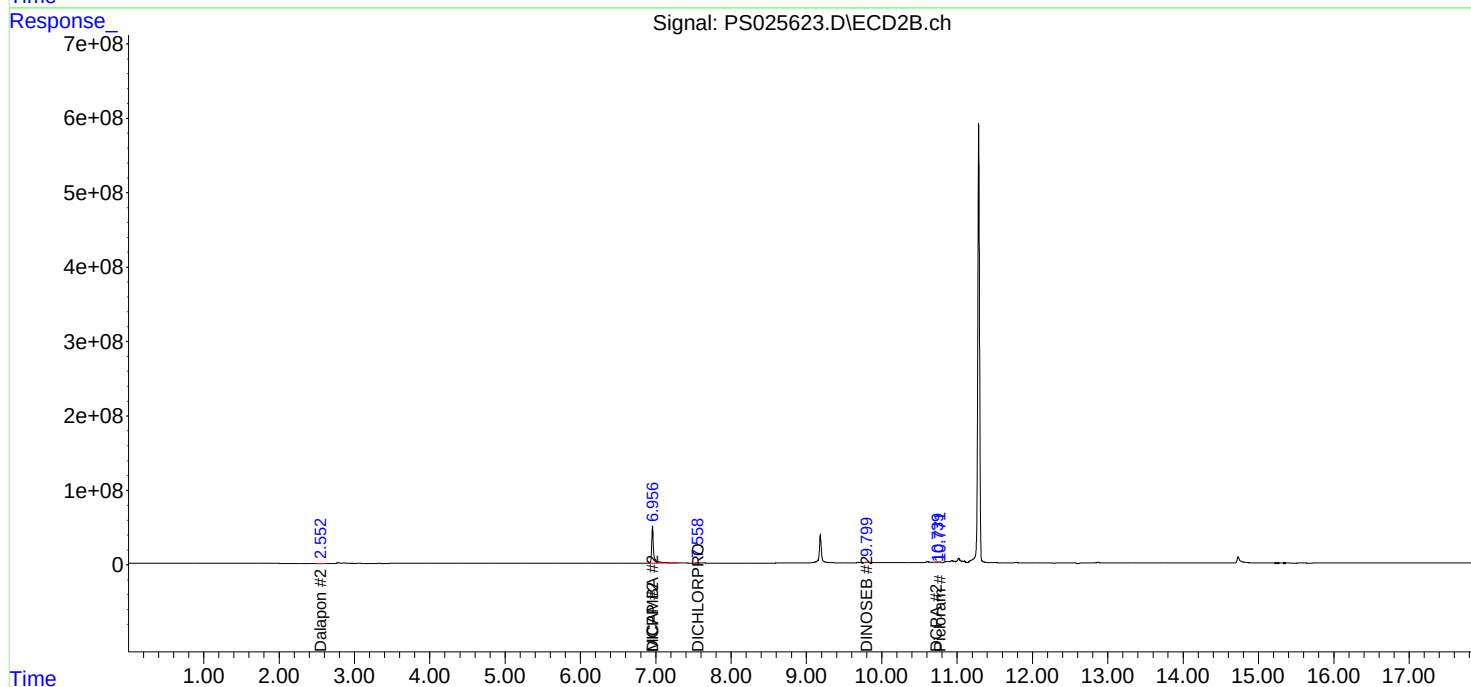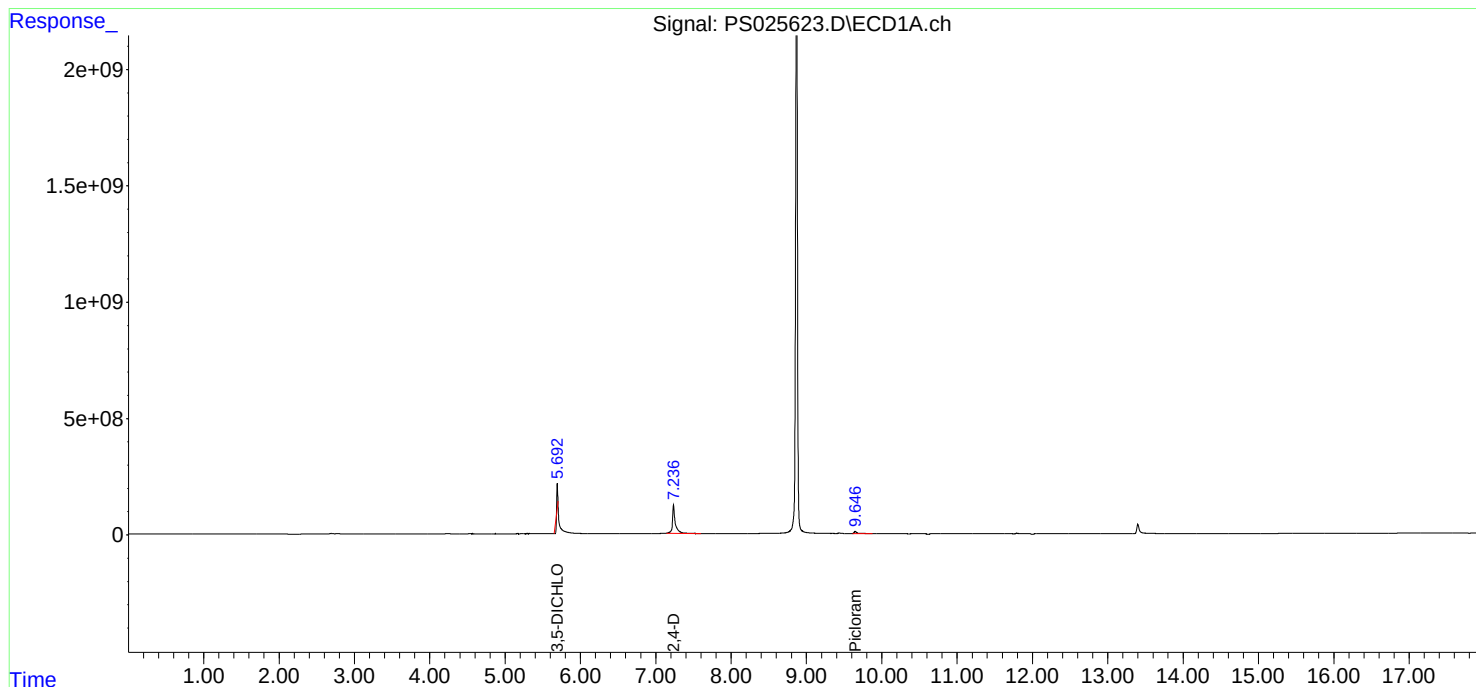


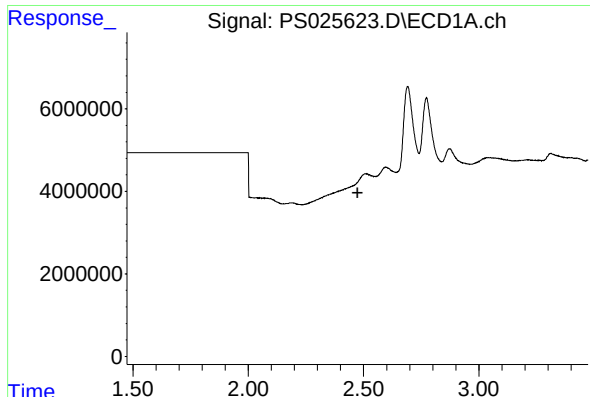

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.474 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

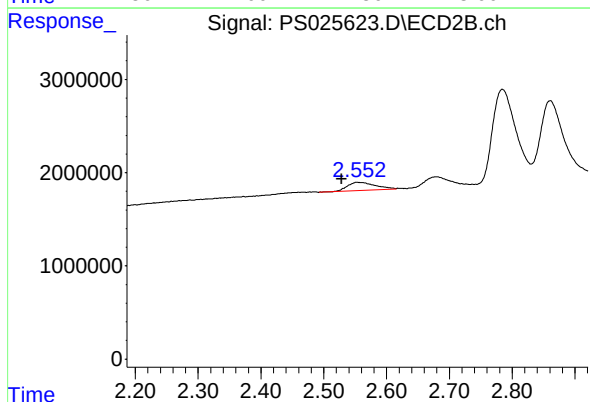


#1 Dalapon

R.T.: 2.553 min
Delta R.T.: 0.024 min
Response: 2753076
Conc: 2.34 ng/ml

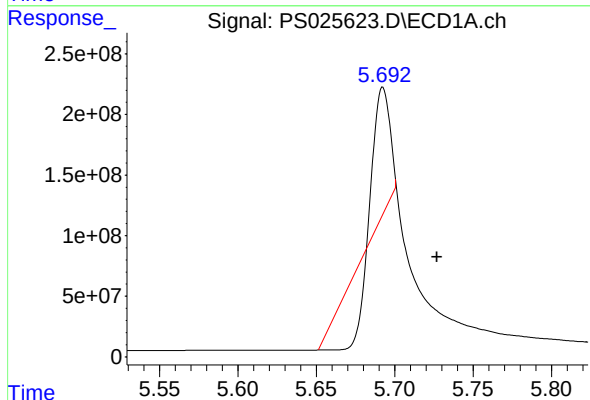


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.693 min
Delta R.T.: -0.034 min
Response: 254715247
Conc: 111.31 ng/ml

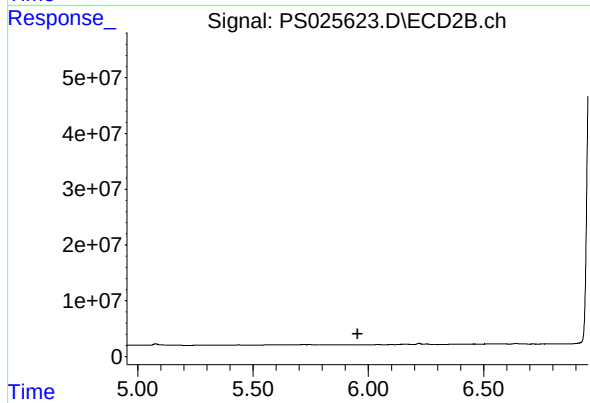

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 5.953 min
Response: 0
Conc: N.D.

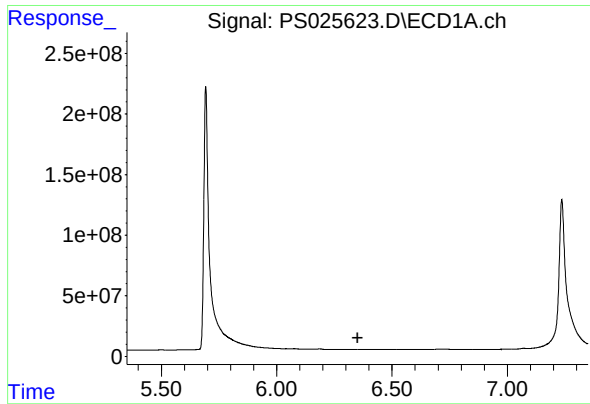

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 6.350 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

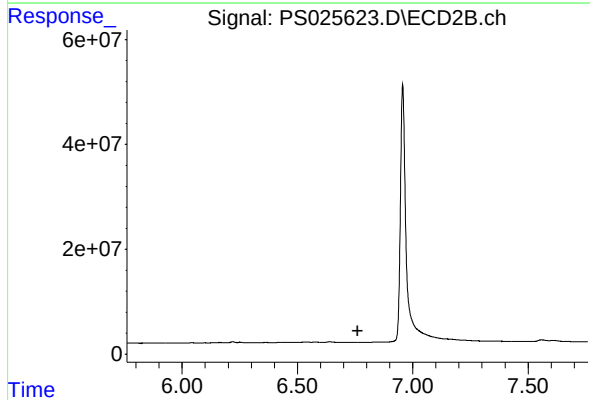


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.761 min
Response: 0
Conc: N.D.

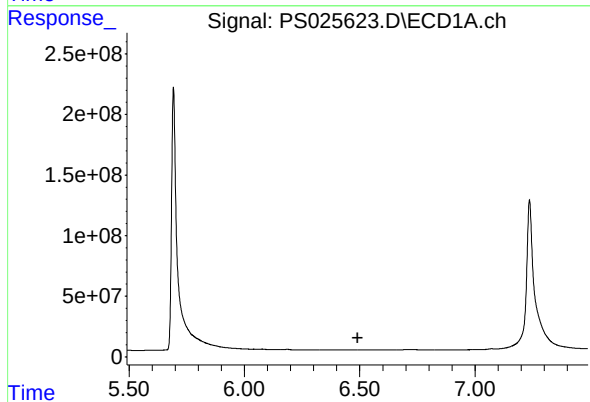


#5 DICAMBA

R.T.: 0.000 min
Exp R.T.: 6.491 min
Response: 0
Conc: N.D.

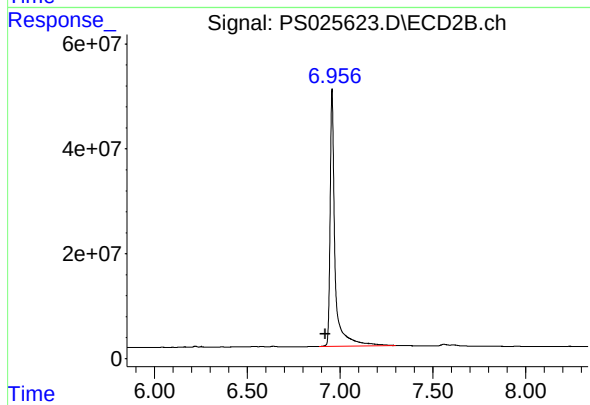

#5 DICAMBA


R.T.: 6.956 min
Delta R.T.: 0.037 min
Response: 912933847
Conc: 274.33 ng/ml

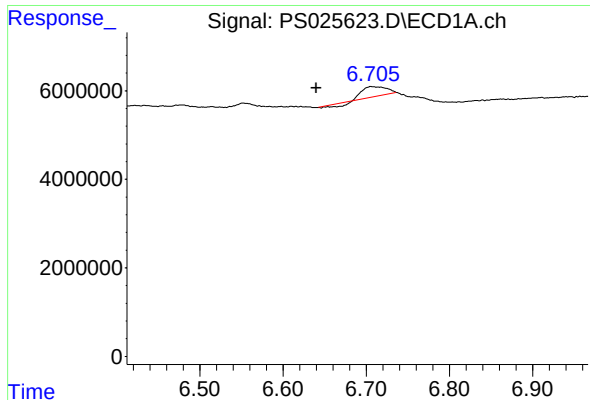

#6 MCPP


R.T.: 6.707 min
Delta R.T.: 0.067 min
Response: 3927442
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

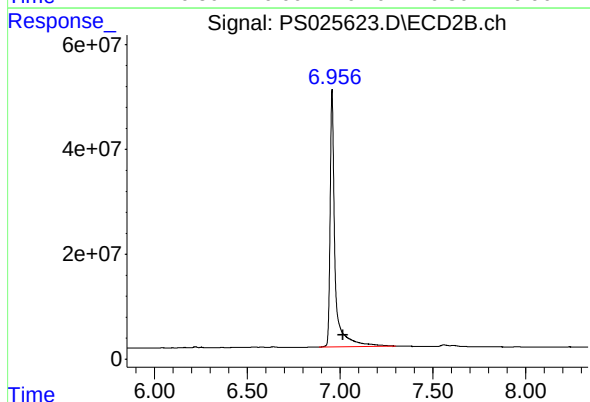


#6 MCPP

R.T.: 6.956 min
Delta R.T.: -0.060 min
Response: 912933847
Conc: 393.54 ug/ml

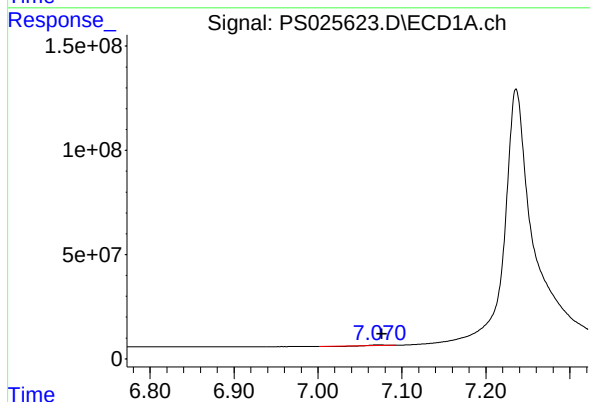


#8 DICHLORPROP

R.T.: 7.072 min
Delta R.T.: -0.005 min
Response: 972632
Conc: N.D.

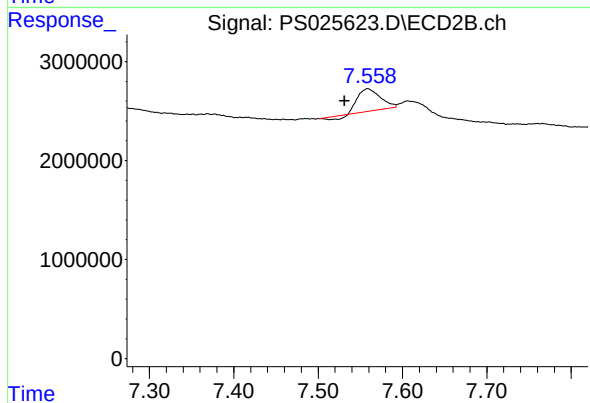

#8 DICHLORPROP


R.T.: 7.559 min
Delta R.T.: 0.027 min
Response: 3970866
Conc: 4.59 ng/ml

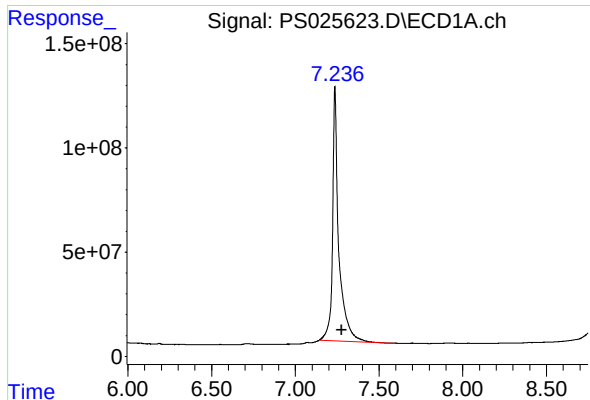

#9 2,4-D


R.T.: 7.236 min
Delta R.T.: -0.039 min
Response: 3151397447
Conc: 1711.46 ng/ml

Instrument :
ECD_S
ClientSampleId :

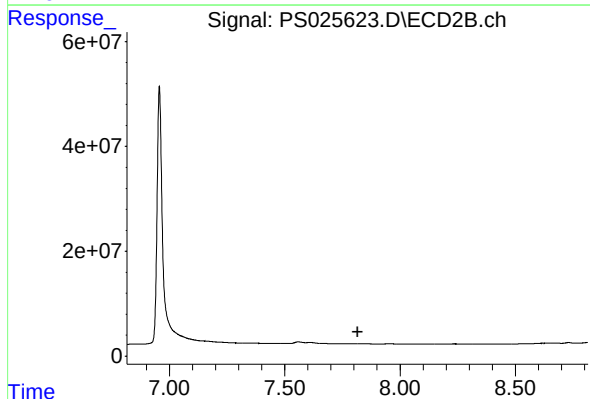


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.815 min
Response: 0
Conc: N.D.

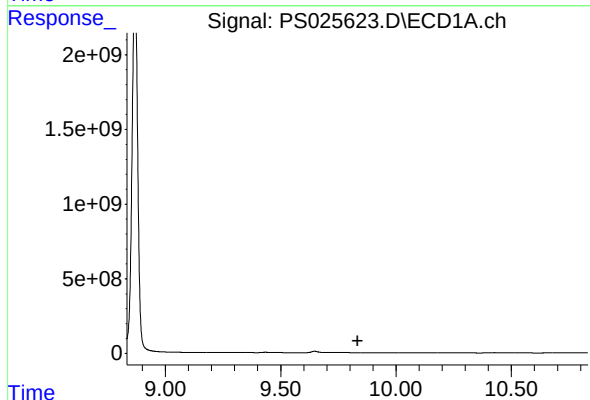


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.833 min
Response: 0
Conc: N.D.

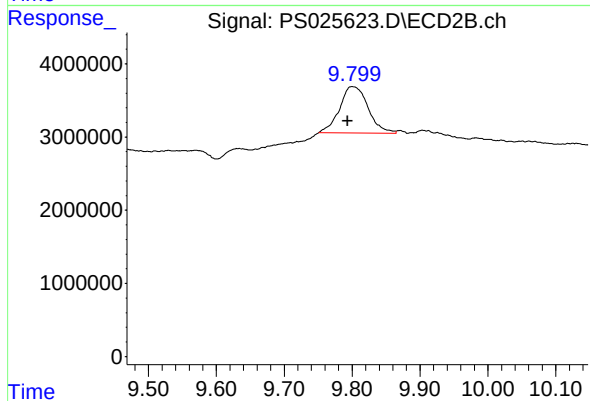

#14 DINOSEB


R.T.: 9.800 min
Delta R.T.: 0.007 min
Response: 18455769
Conc: 5.87 ng/ml

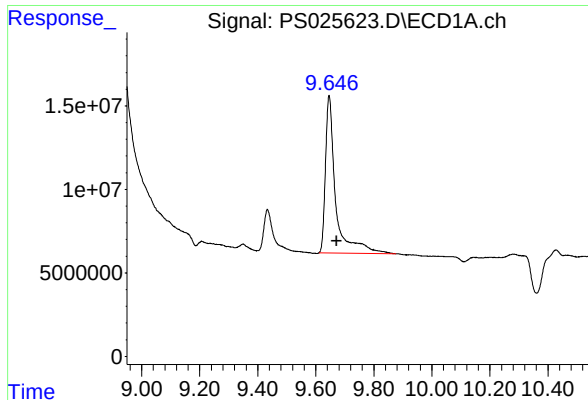

#15 Picloram


R.T.: 9.646 min
Delta R.T.: -0.026 min
Response: 230458176
Conc: 22.27 ng/ml

Instrument :
ECD_S
ClientSampleId :

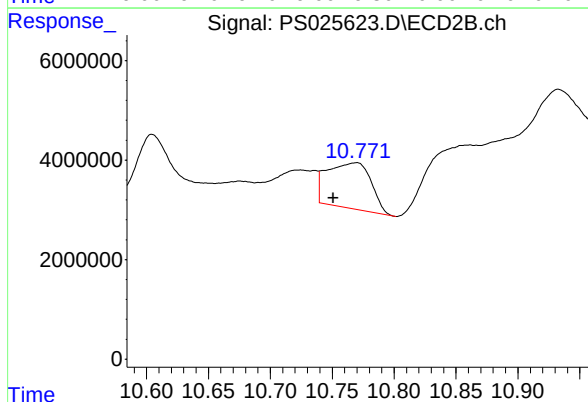


#15 Picloram

R.T.: 10.770 min
Delta R.T.: 0.019 min
Response: 22455313
Conc: 4.22 ng/ml

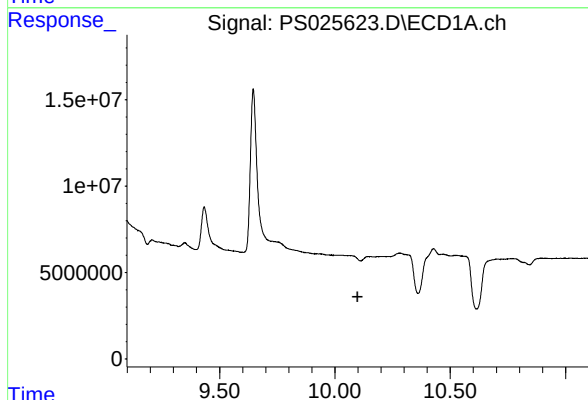

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.098 min
Response: 0
Conc: N.D.

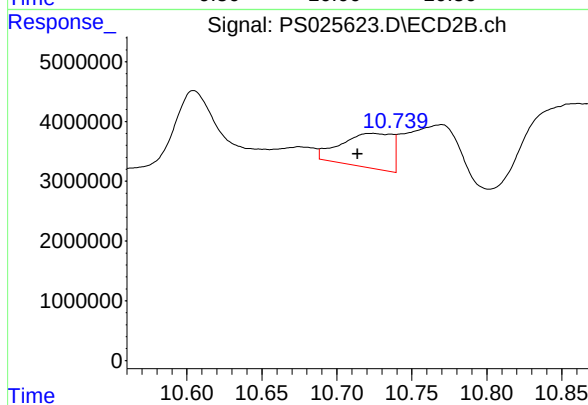

#16 DCPA

R.T.: 10.724 min
Delta R.T.: 0.010 min
Response: 13662487
Conc: 2.35 ng/ml