

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012420\
 Data File : PS008531.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jan 2020 20:41
 Operator : DD\AJ
 Sample : L1007-18
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 JC-03-012320-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 25 03:22:57 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 08 11:00:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.287	5.965	814.1E6	419.5E6	461.060	442.741
Target Compounds							
1) T	Dalapon	2.521	2.188	112.8E6	56168357	44.003	44.306
2) T	3,5-DICHL...	0.000	5.152	0	129.7E6	N.D.	92.826
5) T	DICAMBA	6.474	6.100	-1987366	2255695	N.D.	<MDL
6) T	MCPD	6.595	0.000	8541371	0	1.676	N.D. #
7) T	MCPA	6.728	6.437	91634452	11206427	12.540	2.625 #
8) T	DICHLORPROP	0.000	6.785	0	27722906	N.D.	28.694
10) T	Pentachlo...	7.712	7.485	21806589	19176888	<MDL	1.420 #
12) T	2,4,5-T	8.489	8.226	102.0E6	8895594	11.051	1.682 #
13) T	2,4-DB	9.049	0.000	17074342	0	12.317	N.D. #
14) T	DINOSEB	0.000	9.118	0	53131747	N.D.	14.065
15) T	Picloram	10.068	10.050	60109253	20241444	4.816	2.725 #
16) T	DCPA	0.000	10.002	0	13877409	N.D.	2.130



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012420\
Data File : PS008531.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jan 2020 20:41
Operator : DD\AJ
Sample : L1007-18
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
JC-03-012320-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 25 03:22:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
Quant Title : 8080.M
QLast Update : Wed Jan 08 11:00:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

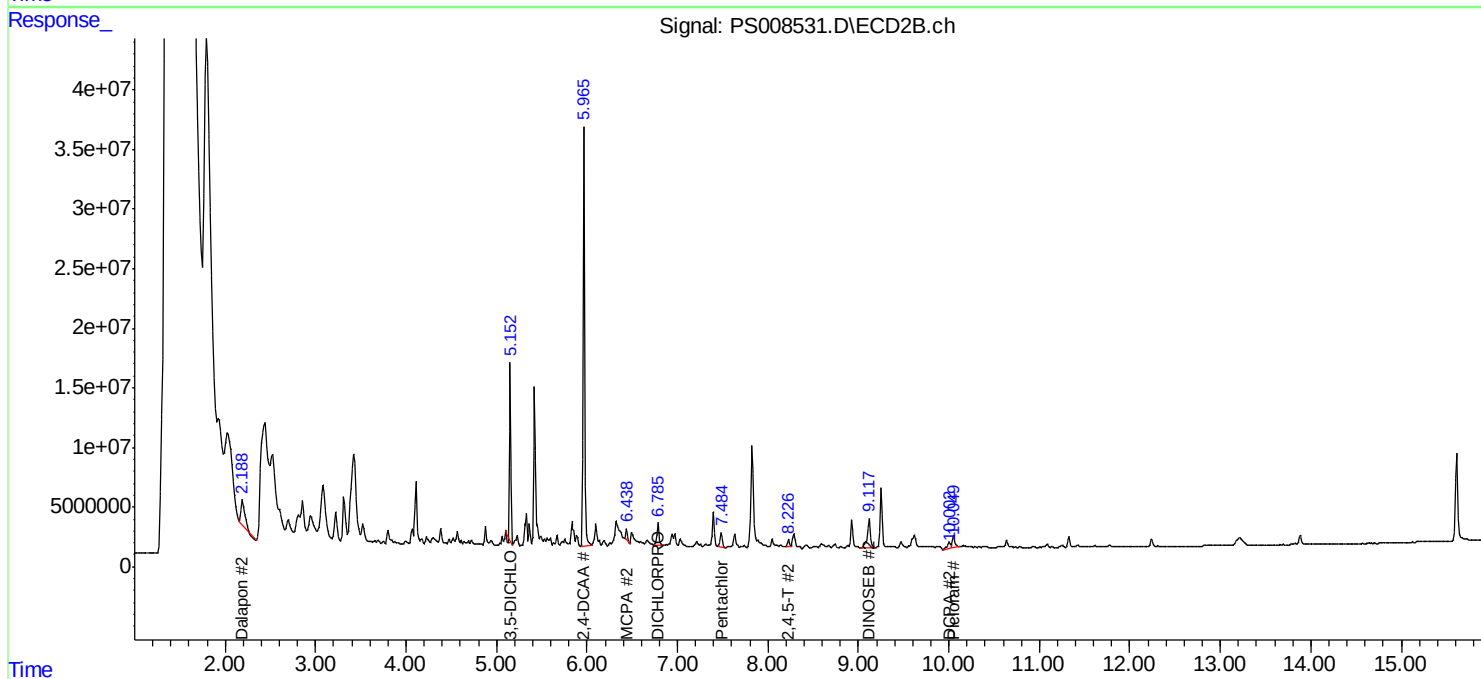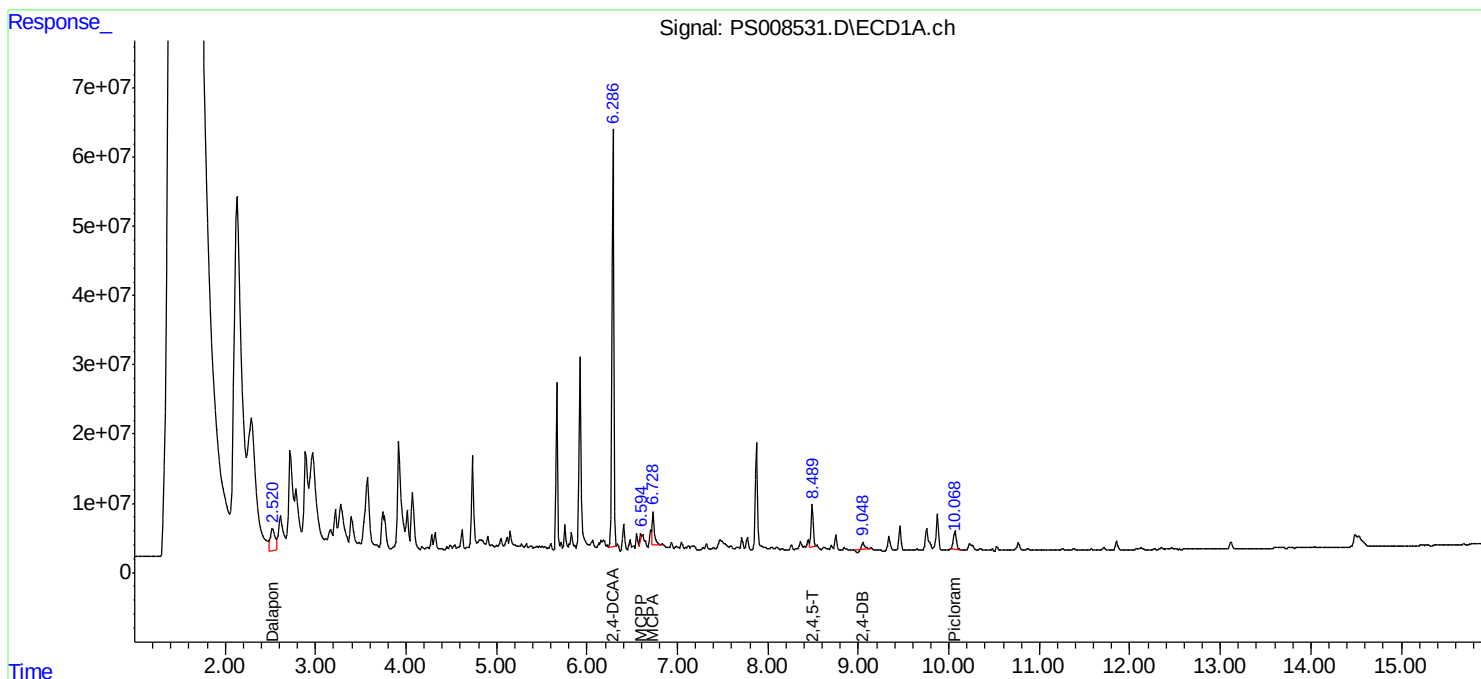


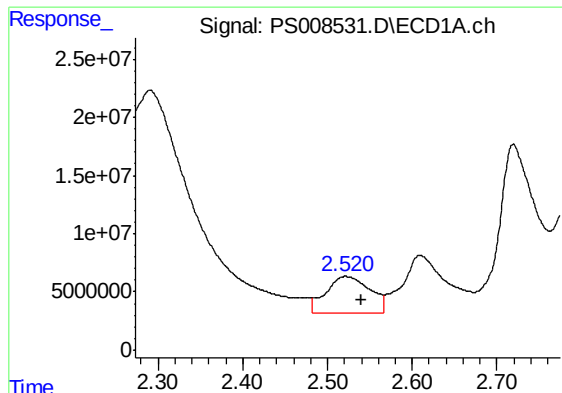

#1 Dalapon


R.T.: 2.521 min
Delta R.T.: -0.019 min
Response: 112816522
Conc: 44.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
JC-03-012320-B

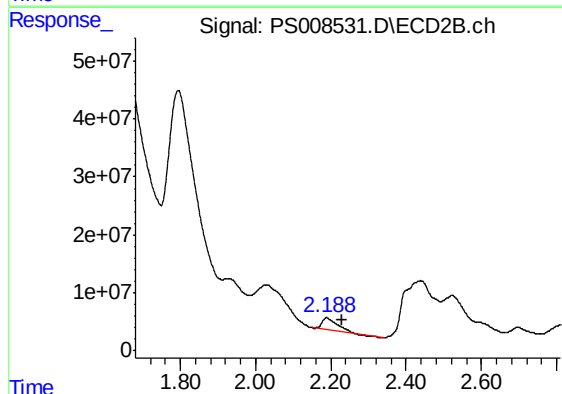


#1 Dalapon

R.T.: 2.188 min
Delta R.T.: -0.043 min
Response: 56168357
Conc: 44.31 ng/ml

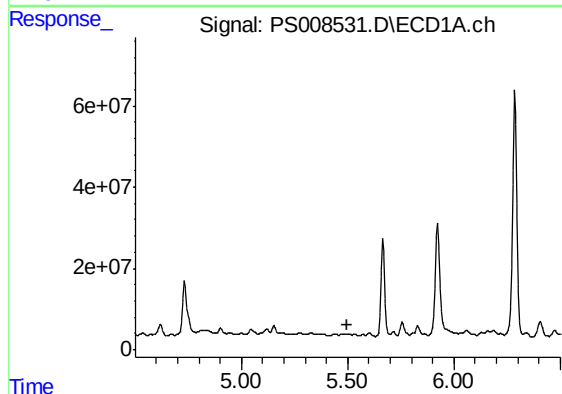


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.501 min
Response: 0
Conc: N.D.

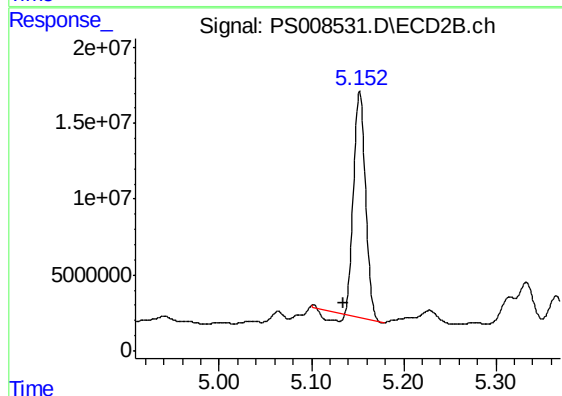

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.152 min
Delta R.T.: 0.018 min
Response: 129694345
Conc: 92.83 ng/ml

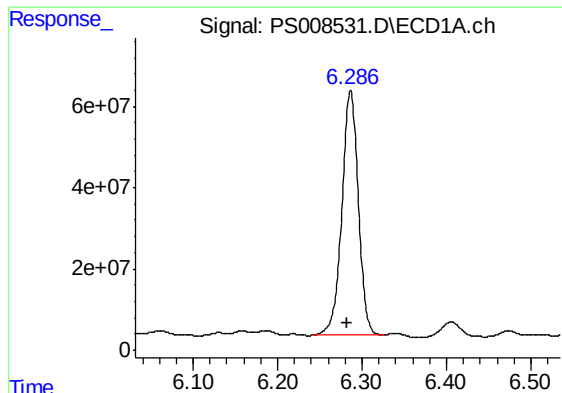

#4 2,4-DCAA


R.T.: 6.287 min
Delta R.T.: 0.004 min
Response: 814096157
Conc: 461.06 ng/ml

Instrument :
ECD_S
ClientSampleId :
JC-03-012320-B

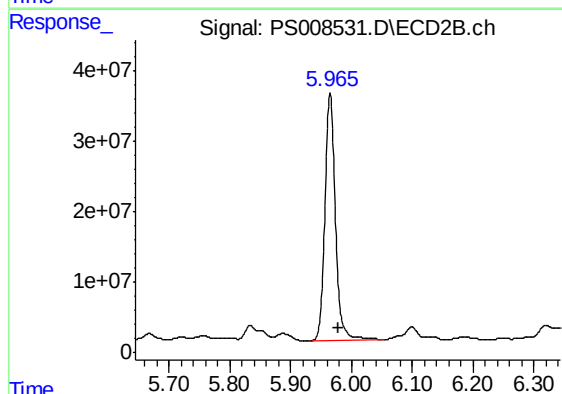


#4 2,4-DCAA

R.T.: 5.965 min
Delta R.T.: -0.014 min
Response: 419480844
Conc: 442.74 ng/ml

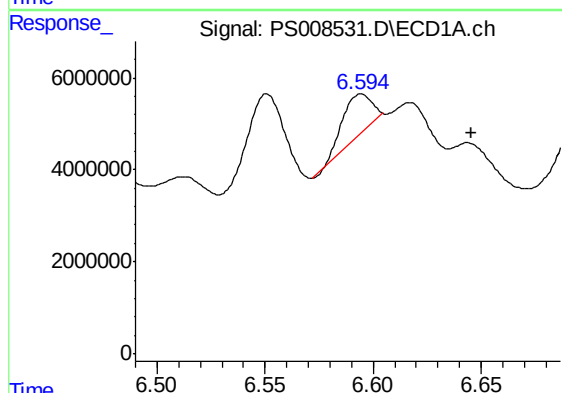


#6 MCP

R.T.: 6.595 min
Delta R.T.: -0.051 min
Response: 8541371
Conc: 1.68 ug/ml

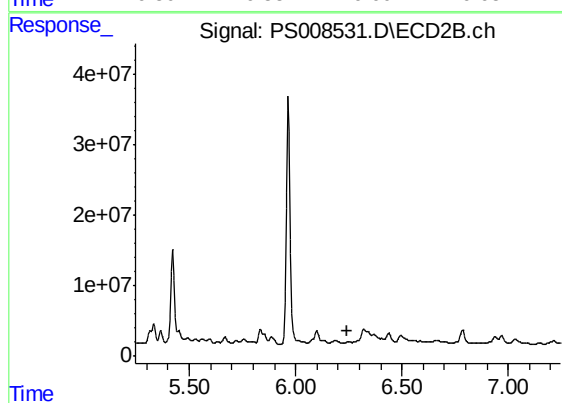

#6 MCP


R.T.: 0.000 min
Exp R.T.: 6.246 min
Response: 0
Conc: N.D.

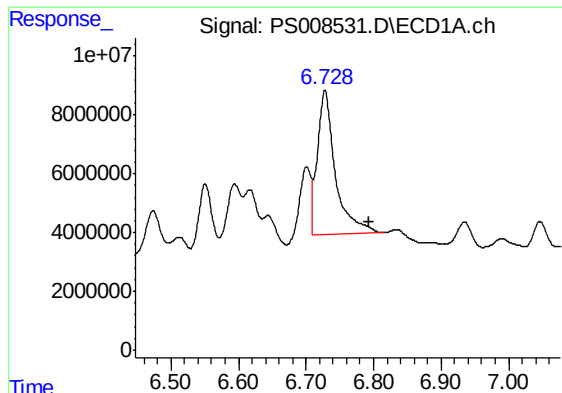

#7 MCPA


R.T.: 6.728 min
Delta R.T.: -0.066 min
Response: 91634452
Conc: 12.54 ug/ml

Instrument :
ECD_S
ClientSampleId :
JC-03-012320-B

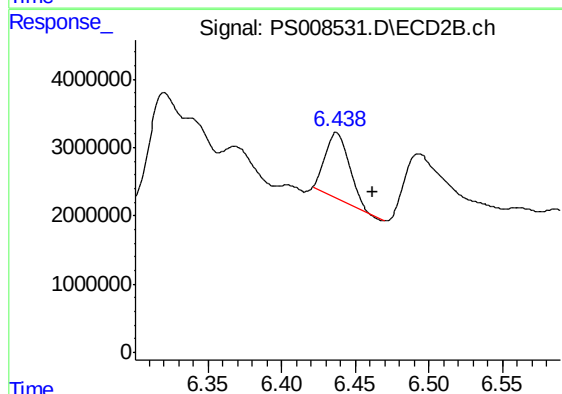


#7 MCPA

R.T.: 6.437 min
Delta R.T.: -0.024 min
Response: 11206427
Conc: 2.62 ug/ml

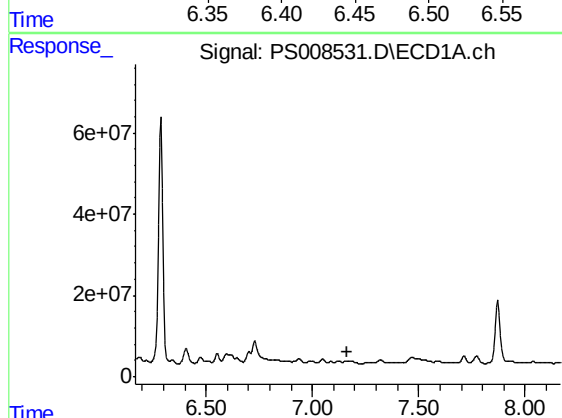


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 7.167 min
Response: 0
Conc: N.D.

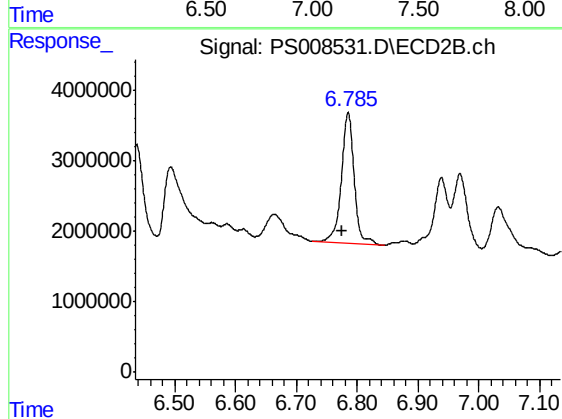

#8 DICHLORPROP


R.T.: 6.785 min
Delta R.T.: 0.010 min
Response: 27722906
Conc: 28.69 ng/ml

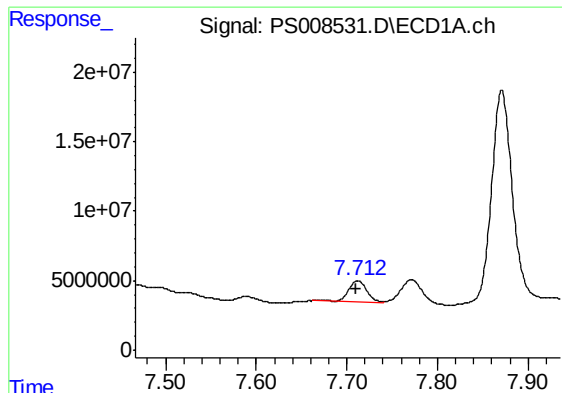

#10 Pentachlorophenol


R.T.: 7.712 min
Delta R.T.: 0.002 min
Response: 21806589
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
JC-03-012320-B

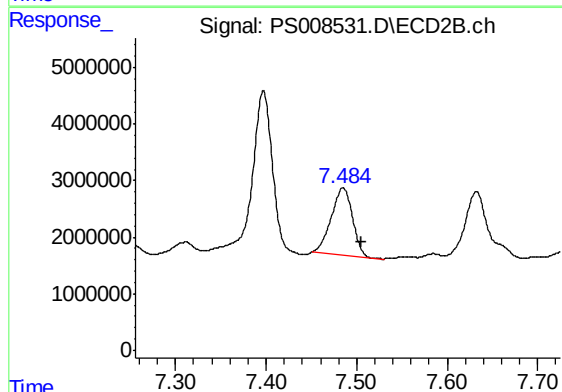


#10 Pentachlorophenol

R.T.: 7.485 min
Delta R.T.: -0.020 min
Response: 19176888
Conc: 1.42 ng/ml

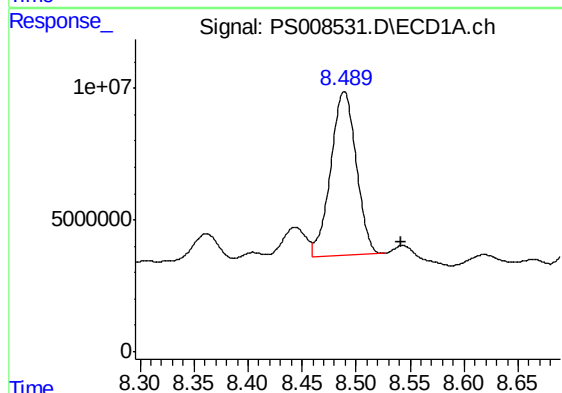


#12 2,4,5-T

R.T.: 8.489 min
Delta R.T.: -0.052 min
Response: 101959929
Conc: 11.05 ng/ml

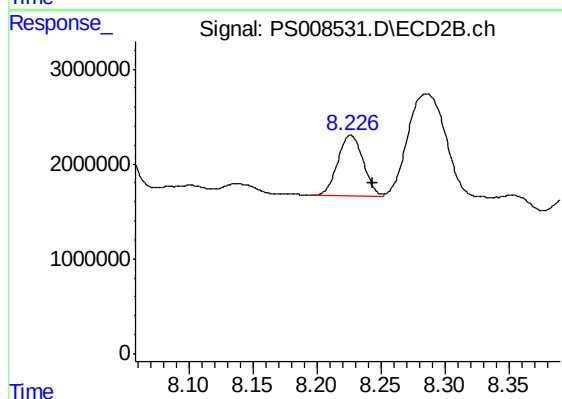

#12 2,4,5-T


R.T.: 8.226 min
Delta R.T.: -0.017 min
Response: 8895594
Conc: 1.68 ng/ml

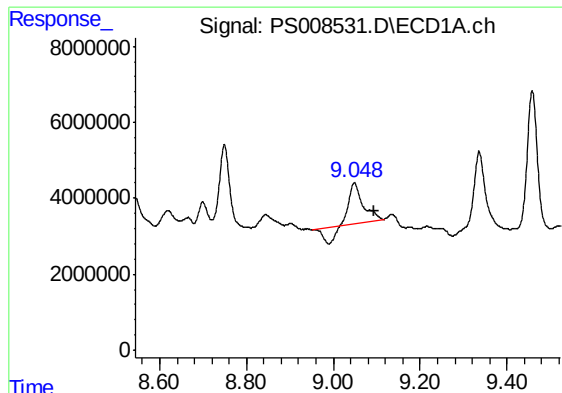

#13 2,4-DB


R.T.: 9.049 min
Delta R.T.: -0.046 min
Response: 17074342
Conc: 12.32 ng/ml

Instrument :
ECD_S
ClientSampleId :
JC-03-012320-B

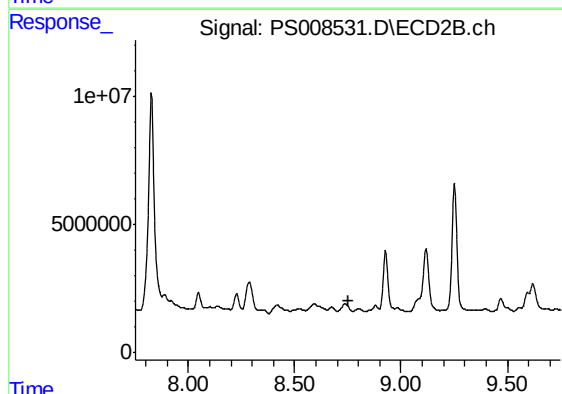


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 8.751 min
Response: 0
Conc: N.D.

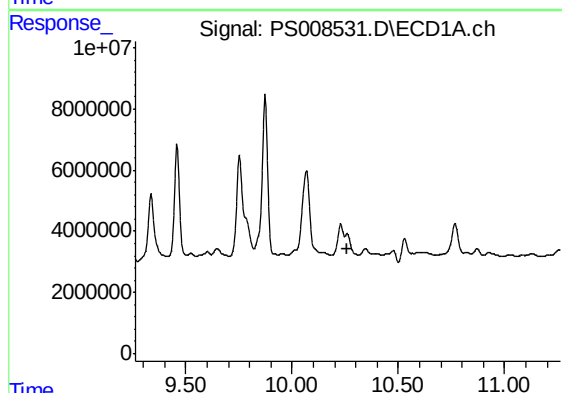


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 10.263 min
Response: 0
Conc: N.D.

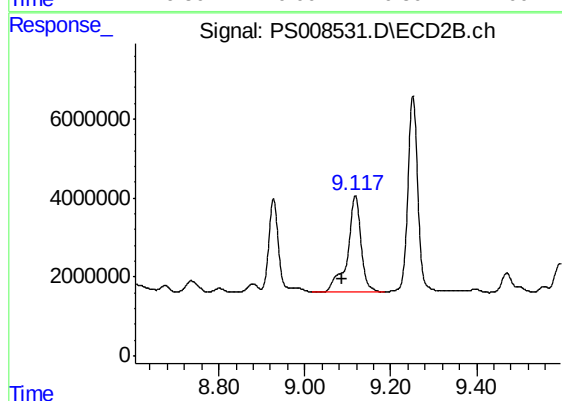

#14 DINOSEB


R.T.: 9.118 min
Delta R.T.: 0.030 min
Response: 53131747
Conc: 14.06 ng/ml

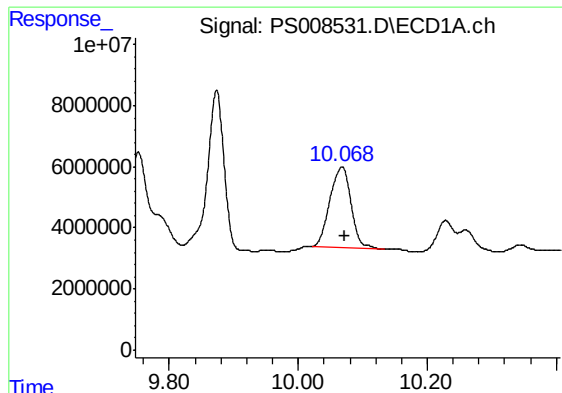

#15 Picloram


R.T.: 10.068 min
Delta R.T.: -0.005 min
Response: 60109253
Conc: 4.82 ng/ml

Instrument :
ECD_S
ClientSampleId :
JC-03-012320-B

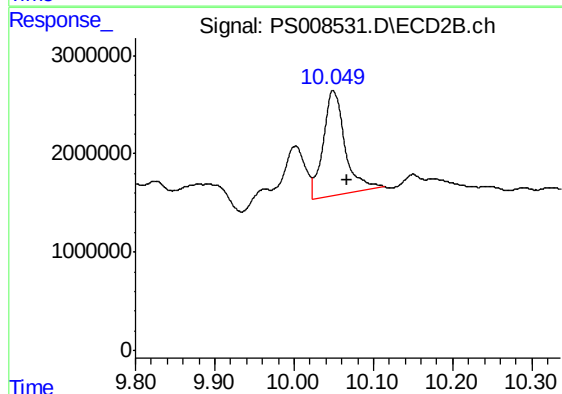


#15 Picloram

R.T.: 10.050 min
Delta R.T.: -0.018 min
Response: 20241444
Conc: 2.72 ng/ml

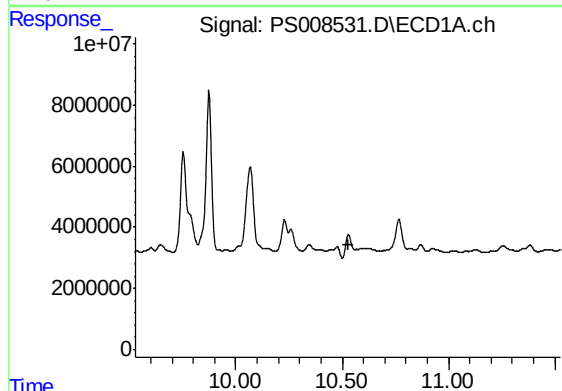

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.527 min
Response: 0
Conc: N.D.

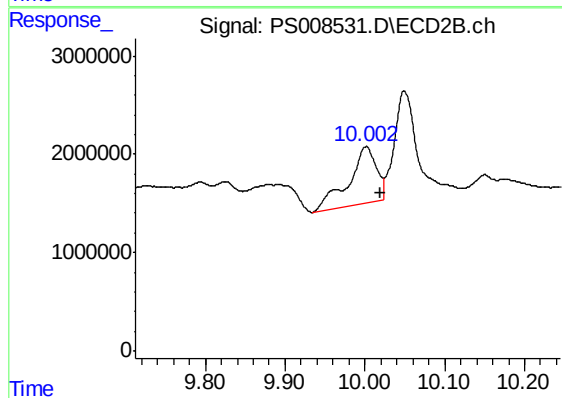

#16 DCPA

R.T.: 10.002 min
Delta R.T.: -0.018 min
Response: 13877409
Conc: 2.13 ng/ml