

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012420\
 Data File : PS008533.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jan 2020 21:25
 Operator : DD\AJ
 Sample : L1016-14
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 SU-04-012320

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 25 03:23:24 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 08 11:00:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.271	5.966	549.8E6	302.6E6	311.371	319.430
Target Compounds							
1) T	Dalapon	2.506	2.191	133.6E6	57304385	52.113	45.202
2) T	3,5-DICHL...	0.000	5.153	0	124.7E6	N.D.	89.262
5) T	DICAMBA	6.535	0.000	29283769	0	4.261	N.D. #
6) T	MCPD	6.713	0.000	180.3E6	0	35.383	N.D. #
7) T	MCPA	0.000	6.437	0	8246876	N.D.	1.931
8) T	DICHLORPROP	0.000	6.786	0	20517175	N.D.	21.236
9) T	2,4-D	7.453	7.033	53661375	10507064	29.499	8.963 #
10) T	Pentachlo...	7.755	0.000	31633876	0	1.301	N.D. #
12) T	2,4,5-T	8.473	8.294	143.0E6	11263393	15.494	2.130 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012420\
Data File : PS008533.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jan 2020 21:25
Operator : DD\AJ
Sample : L1016-14
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
SU-04-012320

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 25 03:23:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
Quant Title : 8080.M
QLast Update : Wed Jan 08 11:00:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

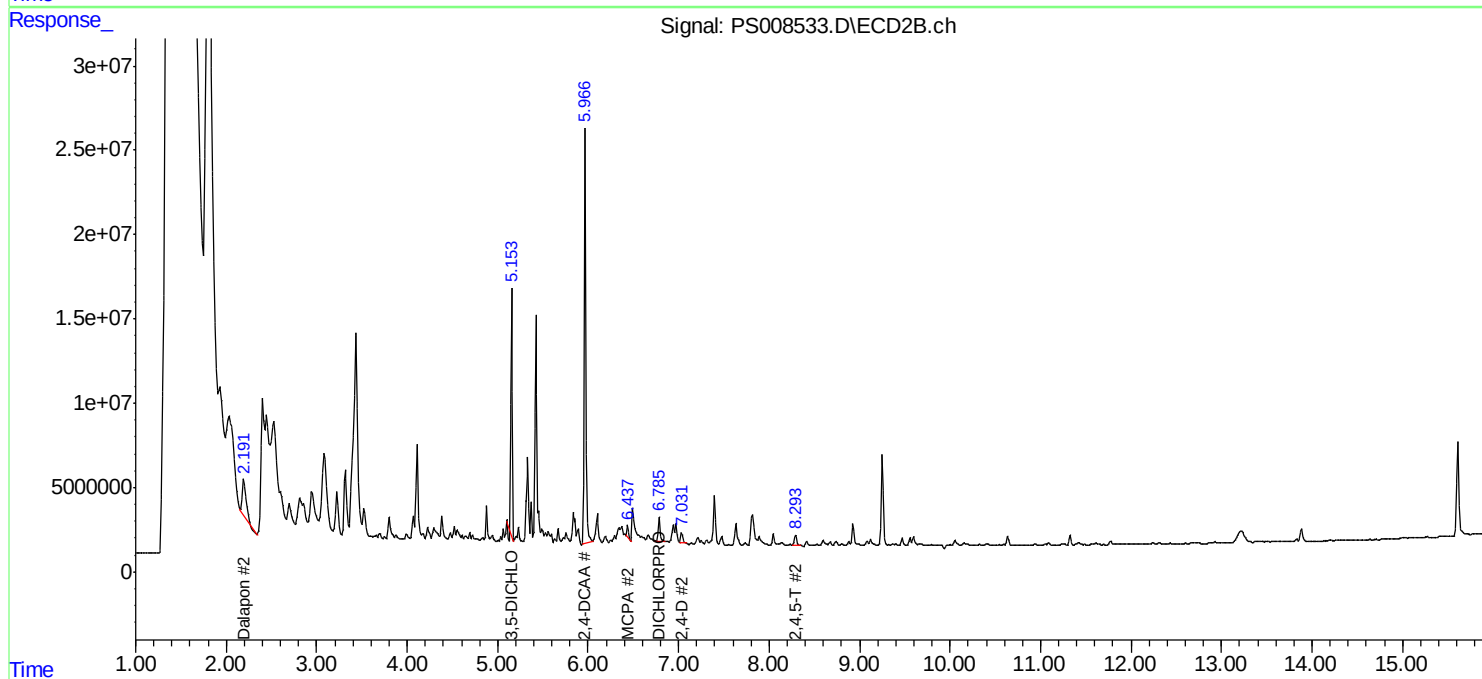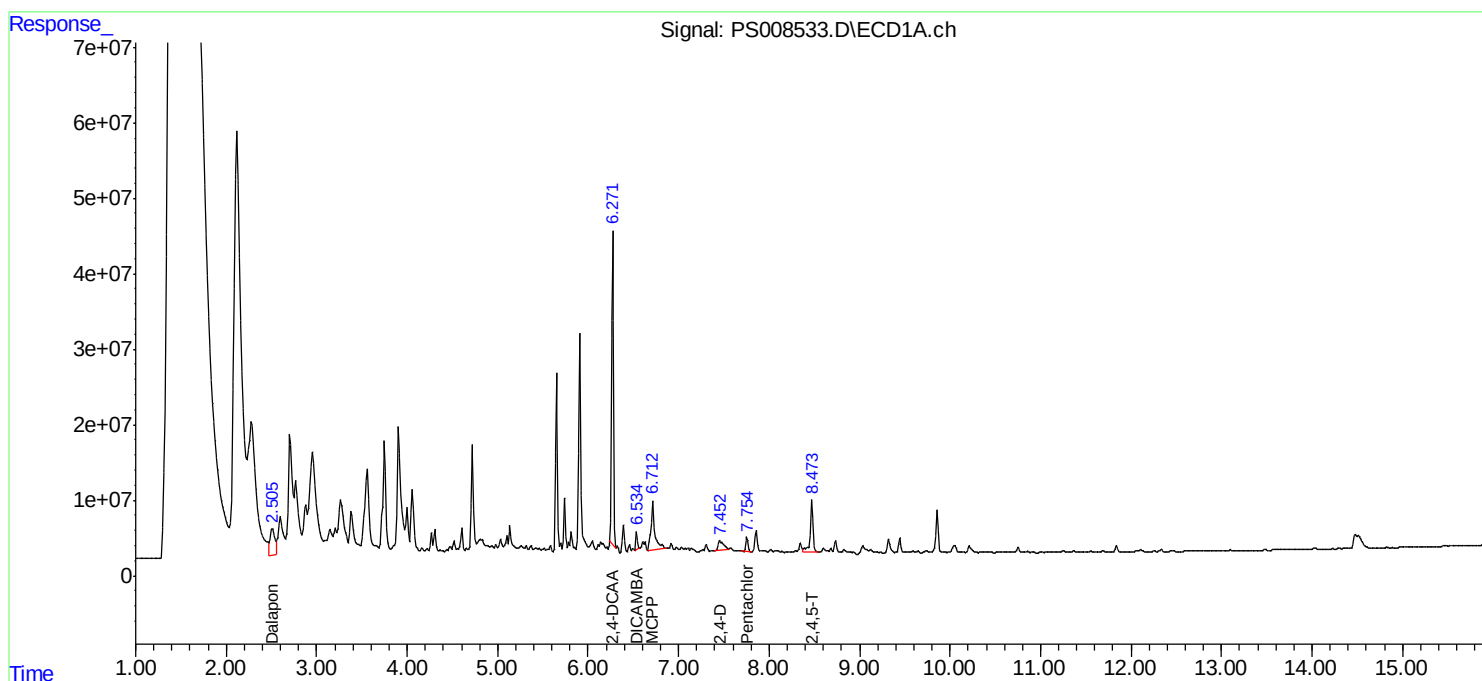


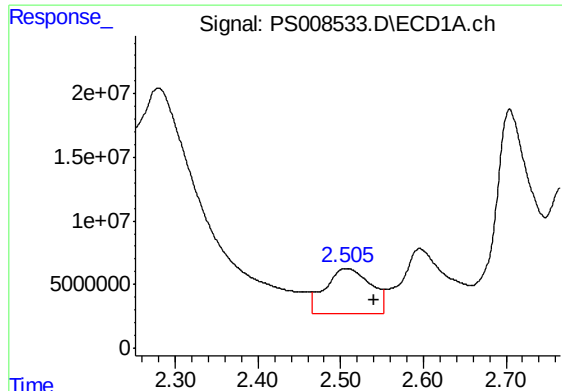

#1 Dalapon


R.T.: 2.506 min
Delta R.T.: -0.034 min
Response: 133609681
Conc: 52.11 ng/ml

Instrument :
ECD_S
ClientSampleId :
SU-04-012320

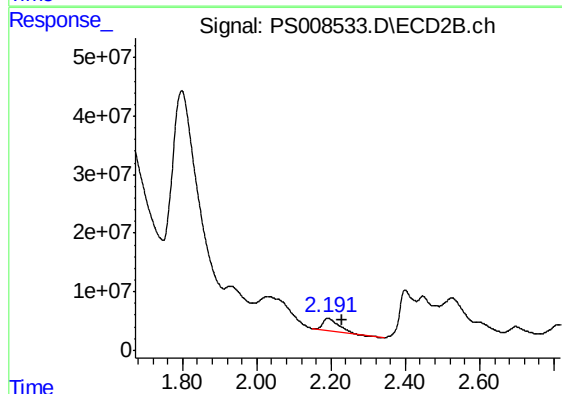


#1 Dalapon

R.T.: 2.191 min
Delta R.T.: -0.040 min
Response: 57304385
Conc: 45.20 ng/ml

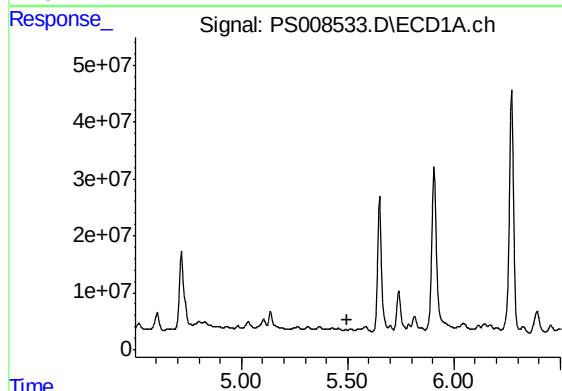


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.501 min
Response: 0
Conc: N.D.

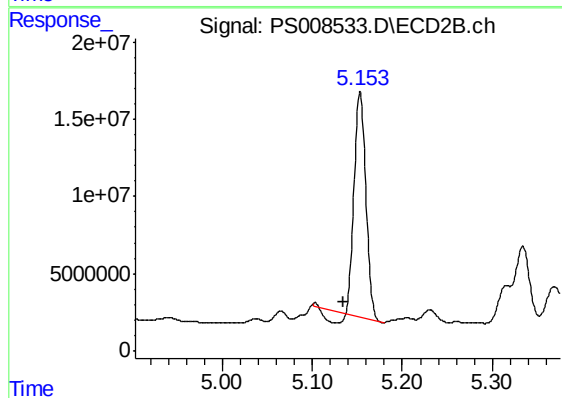

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.153 min
Delta R.T.: 0.019 min
Response: 124715362
Conc: 89.26 ng/ml

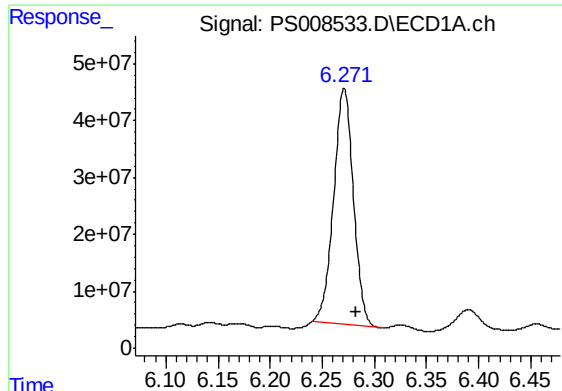

#4 2,4-DCAA


R.T.: 6.271 min
Delta R.T.: -0.012 min
Response: 549788580
Conc: 311.37 ng/ml

Instrument :
ECD_S
ClientSampleId :
SU-04-012320

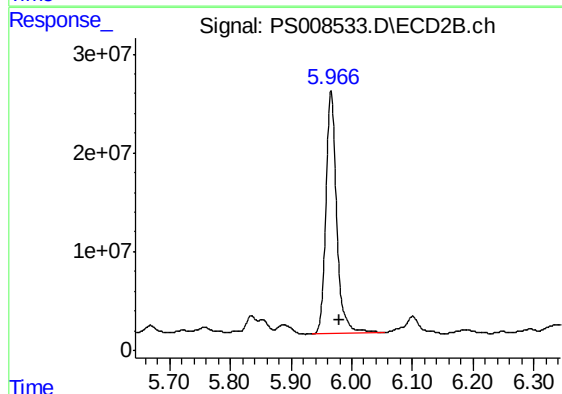


#4 2,4-DCAA

R.T.: 5.966 min
Delta R.T.: -0.013 min
Response: 302647964
Conc: 319.43 ng/ml

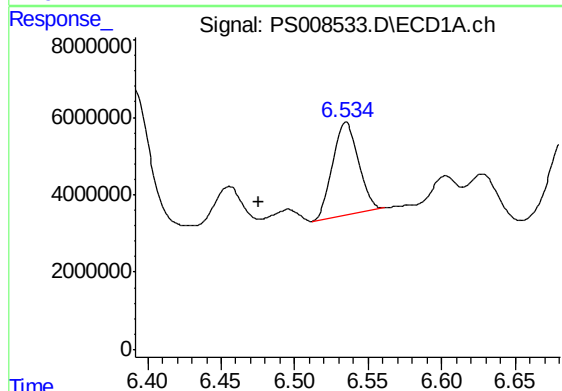


#5 DICAMBA

R.T.: 6.535 min
Delta R.T.: 0.059 min
Response: 29283769
Conc: 4.26 ng/ml

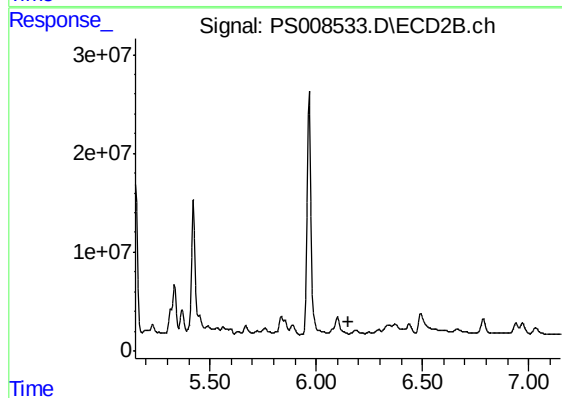

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 6.150 min
Response: 0
Conc: N.D.

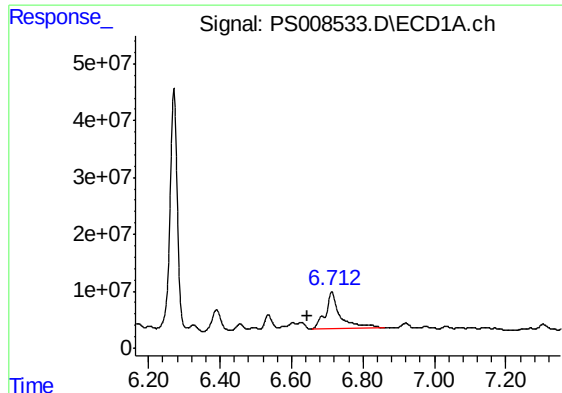

#6 MCPP


R.T.: 6.713 min
Delta R.T.: 0.067 min
Response: 180342344
Conc: 35.38 ug/ml

Instrument :
ECD_S
ClientSampleId :
SU-04-012320

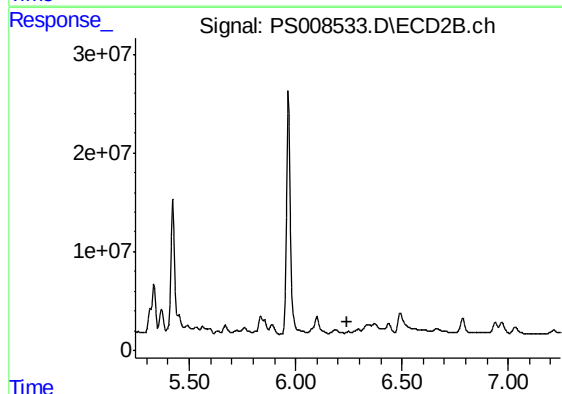


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 6.246 min
Response: 0
Conc: N.D.

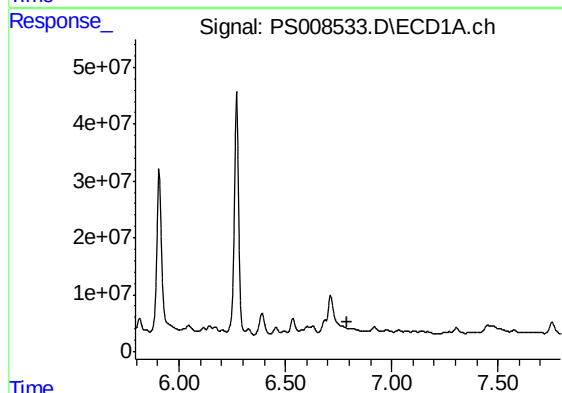


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 6.794 min
Response: 0
Conc: N.D.

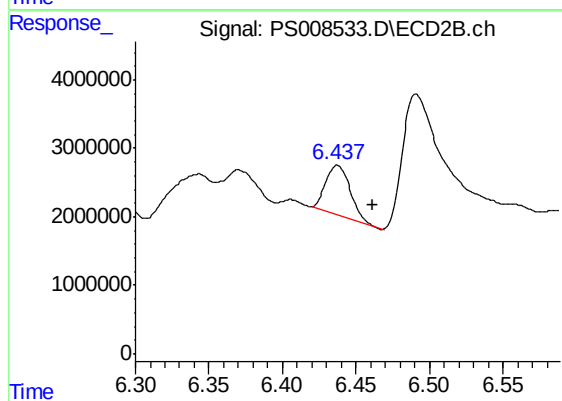

#7 MCPA


R.T.: 6.437 min
Delta R.T.: -0.024 min
Response: 8246876
Conc: 1.93 ug/ml

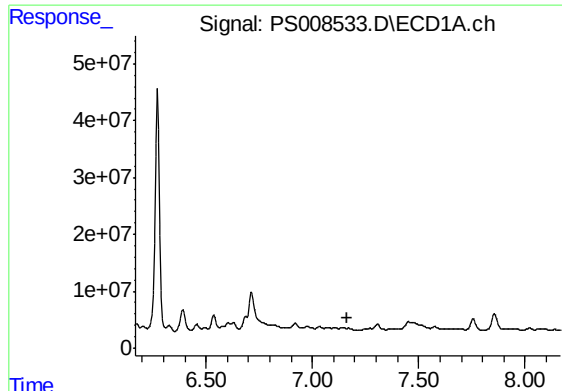

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.167 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SU-04-012320

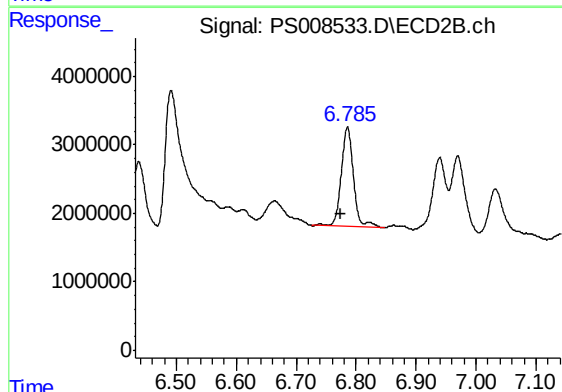


#8 DICHLORPROP

R.T.: 6.786 min
Delta R.T.: 0.011 min
Response: 20517175
Conc: 21.24 ng/ml

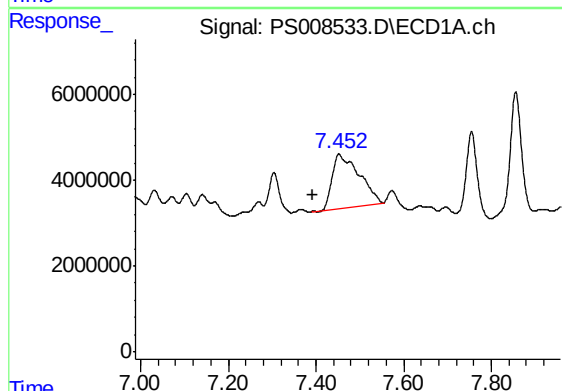


#9 2,4-D

R.T.: 7.453 min
Delta R.T.: 0.059 min
Response: 53661375
Conc: 29.50 ng/ml

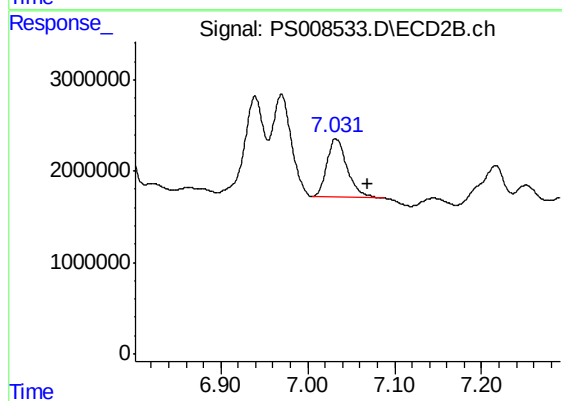

#9 2,4-D


R.T.: 7.033 min
Delta R.T.: -0.036 min
Response: 10507064
Conc: 8.96 ng/ml

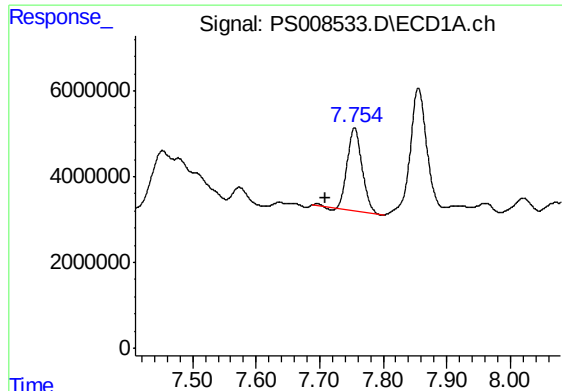

#10 Pentachlorophenol


R.T.: 7.755 min
Delta R.T.: 0.045 min
Response: 31633876
Conc: 1.30 ng/ml

Instrument :
ECD_S
ClientSampleId :
SU-04-012320

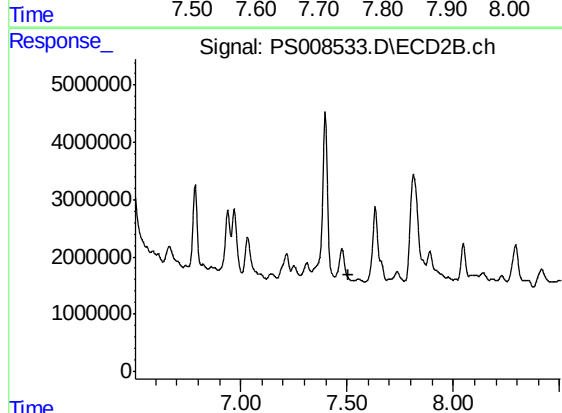


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 7.505 min
Response: 0
Conc: N.D.

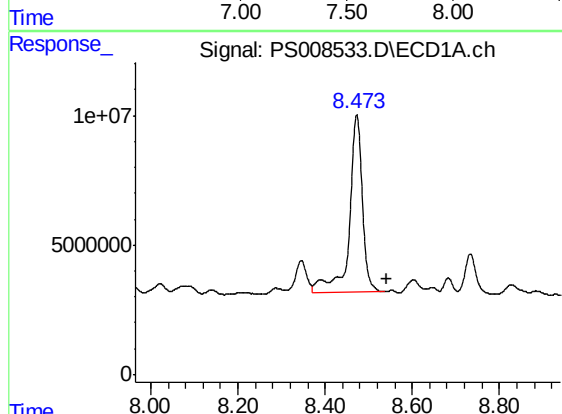

#12 2,4,5-T

R.T.: 8.473 min
Delta R.T.: -0.068 min
Response: 142956747
Conc: 15.49 ng/ml

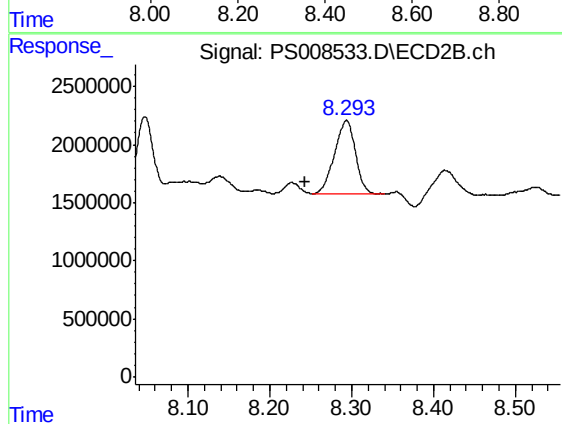

#12 2,4,5-T

R.T.: 8.294 min
Delta R.T.: 0.050 min
Response: 11263393
Conc: 2.13 ng/ml