

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012420\
 Data File : PS008539.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jan 2020 23:36
 Operator : DD\AJ
 Sample : L1247-14
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-7-6-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 25 03:24:50 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 08 11:00:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.272	5.966	790.8E6	429.0E6	447.872	452.773
Target Compounds							
1) T	Dalapon	2.506	2.191	151.7E6	92049591	59.167	72.609
2) T	3,5-DICHL...	0.000	5.153	0	142.5E6	N.D.	102.024
5) T	DICAMBA	6.536	6.100	36229947	-872584	5.272	N.D. #
6) T	MCPD	6.686	0.000	30784501	0	6.040	N.D. #
7) T	MCPA	0.000	6.438	0	10618213	N.D.	2.487
8) T	DICHLORPROP	0.000	6.785	0	24265554	N.D.	25.116
9) T	2,4-D	7.454	7.033	9942662	10916856	5.466	9.313 #
10) T	Pentachlo...	7.756	0.000	34377139	0	1.414	N.D. #
12) T	2,4,5-T	8.474	8.294	113.4E6	20742937	12.290	3.923 #
13) T	2,4-DB	9.034	0.000	31240980	0	22.536	N.D. #
14) T	DINOSEB	0.000	9.119	0	65761244	N.D.	17.408
15) T	Picloram	10.048	0.000	48533680	0	3.888	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012420\
Data File : PS008539.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jan 2020 23:36
Operator : DD\AJ
Sample : L1247-14
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-7-6-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 25 03:24:50 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
Quant Title : 8080.M
QLast Update : Wed Jan 08 11:00:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

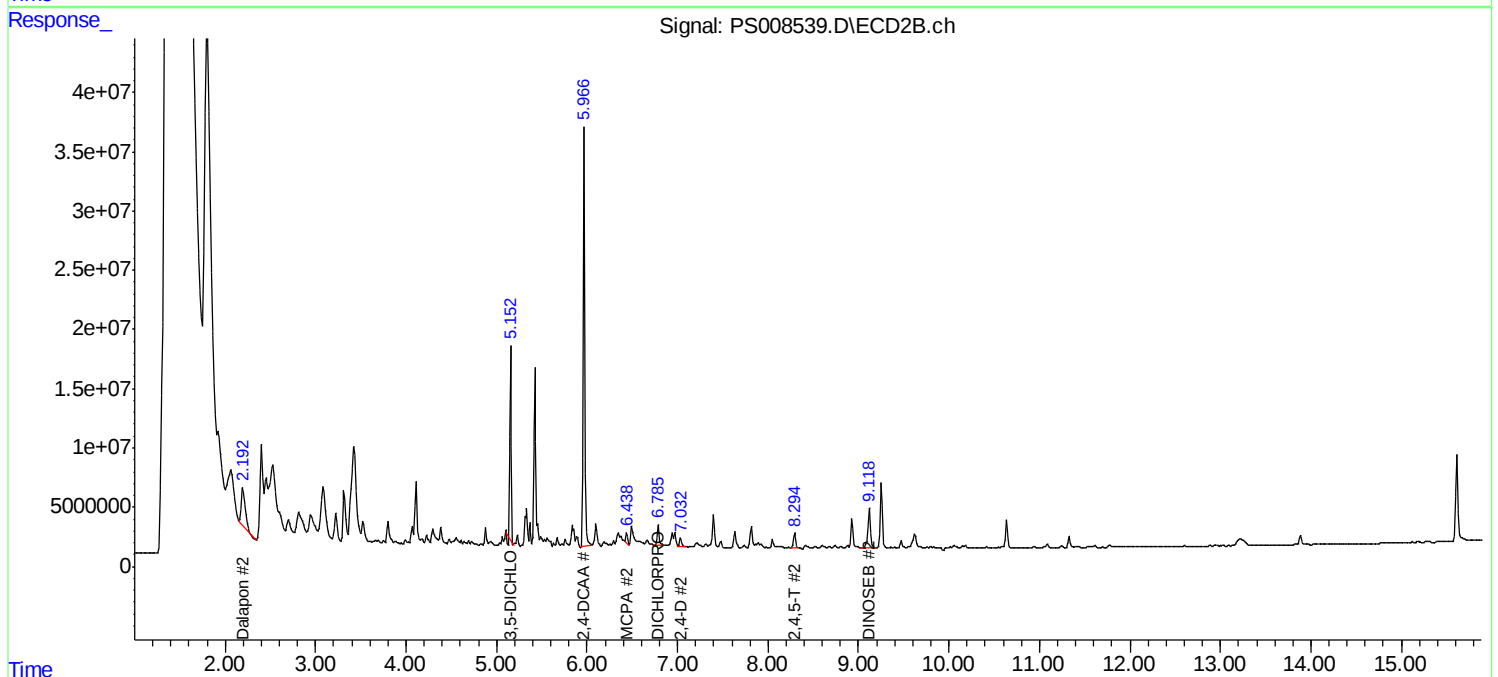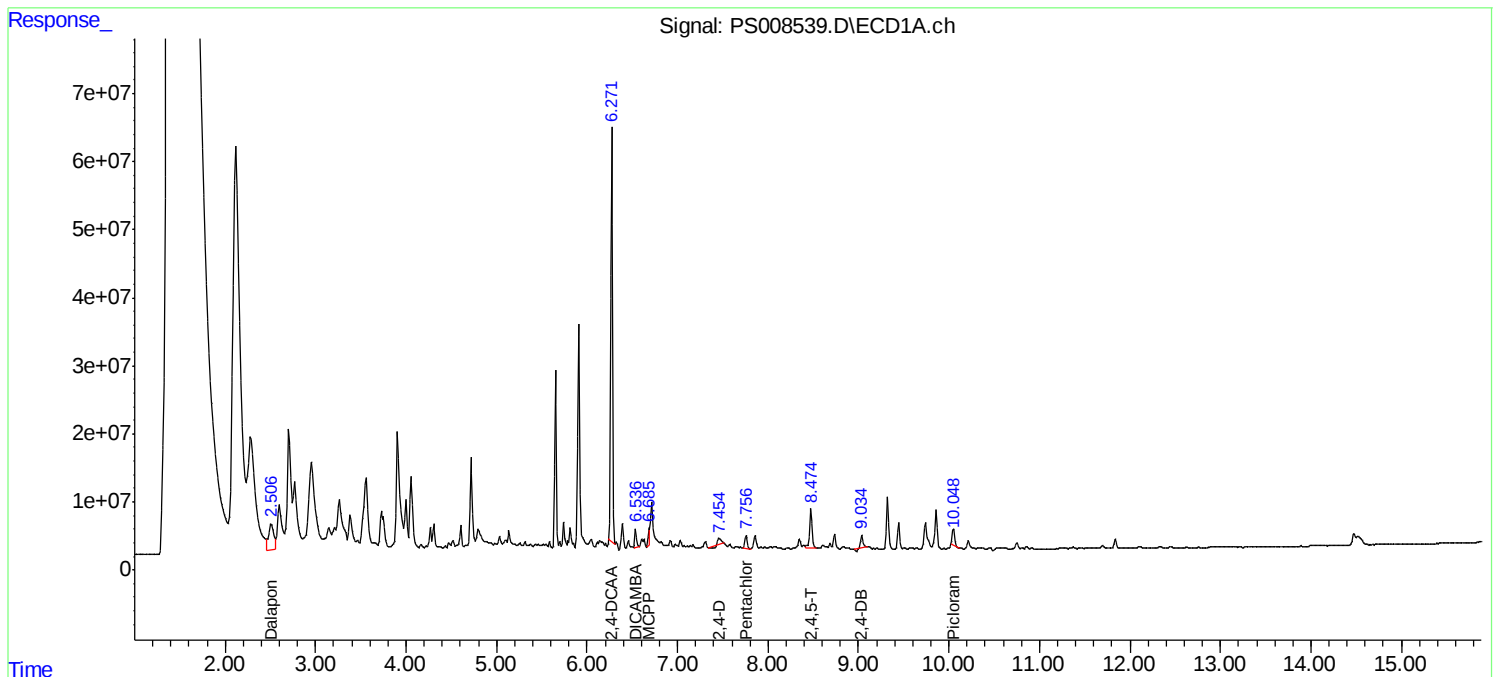


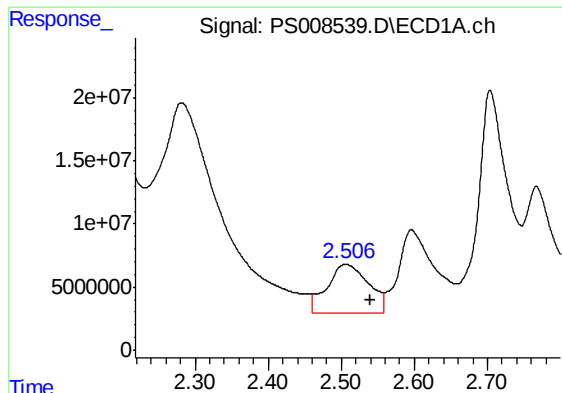

#1 Dalapon


R.T.: 2.506 min
Delta R.T.: -0.034 min
Response: 151694754
Conc: 59.17 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-7-6-COMP

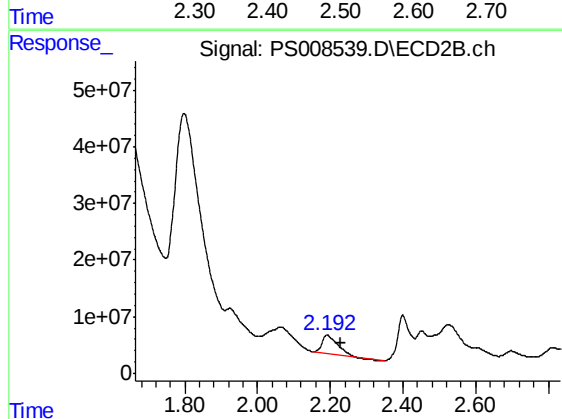


#1 Dalapon

R.T.: 2.191 min
Delta R.T.: -0.040 min
Response: 92049591
Conc: 72.61 ng/ml

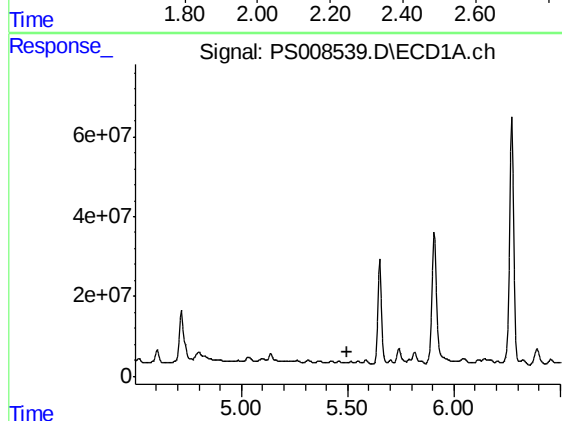


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.501 min
Response: 0
Conc: N.D.

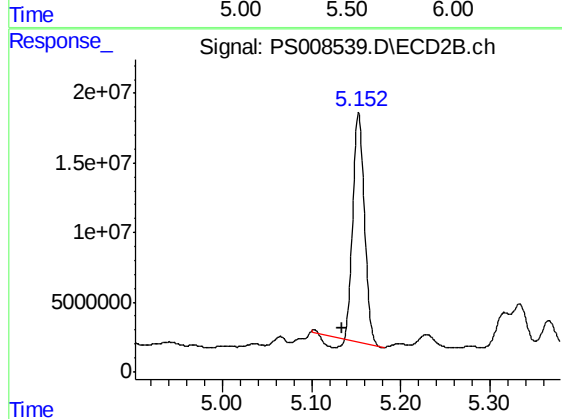

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.153 min
Delta R.T.: 0.019 min
Response: 142545067
Conc: 102.02 ng/ml

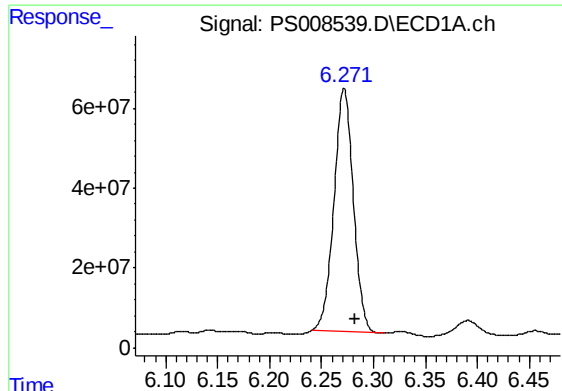

#4 2,4-DCAA


R.T.: 6.272 min
Delta R.T.: -0.011 min
Response: 790809555
Conc: 447.87 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-7-6-COMP

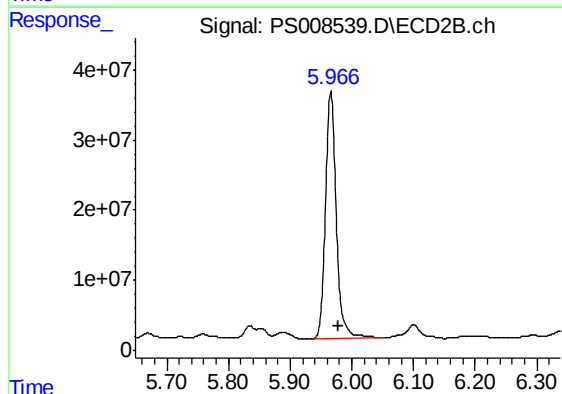


#4 2,4-DCAA

R.T.: 5.966 min
Delta R.T.: -0.013 min
Response: 428986063
Conc: 452.77 ng/ml

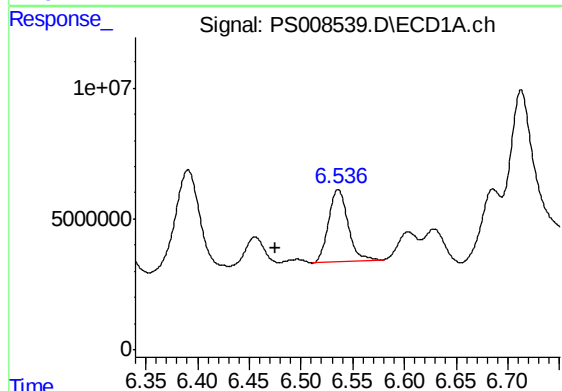


#5 DICAMBA

R.T.: 6.536 min
Delta R.T.: 0.060 min
Response: 36229947
Conc: 5.27 ng/ml

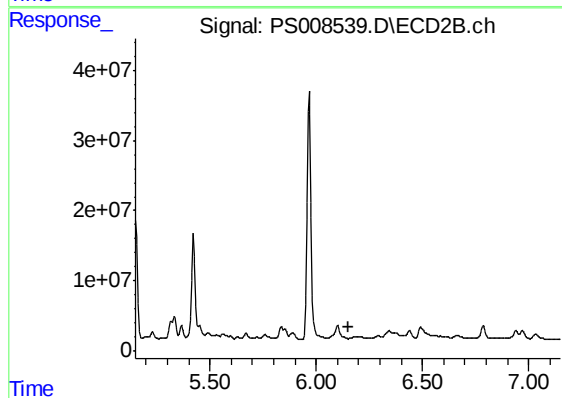

#5 DICAMBA


R.T.: 6.100 min
Delta R.T.: -0.050 min
Response: -872584
Conc: N.D.

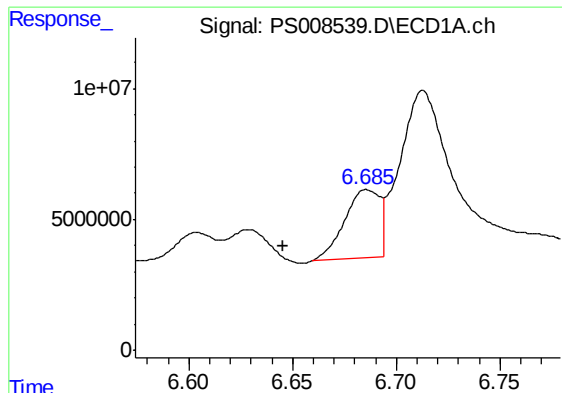

#6 MCPP


R.T.: 6.686 min
Delta R.T.: 0.040 min
Response: 30784501
Conc: 6.04 ug/ml

Instrument :
ECD_S
ClientSampleId :
TP-7-6-COMP

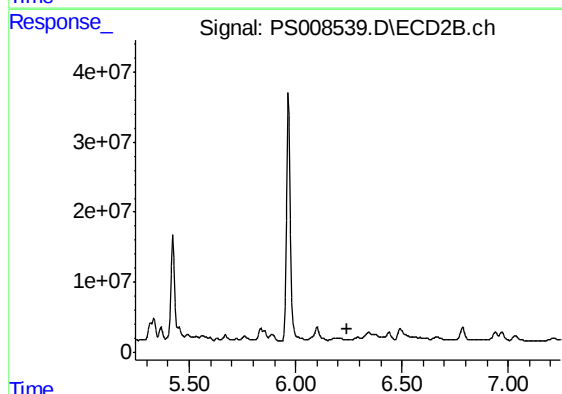


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 6.246 min
Response: 0
Conc: N.D.

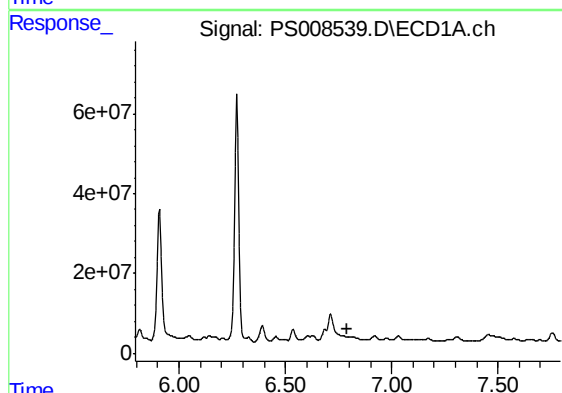


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 6.794 min
Response: 0
Conc: N.D.

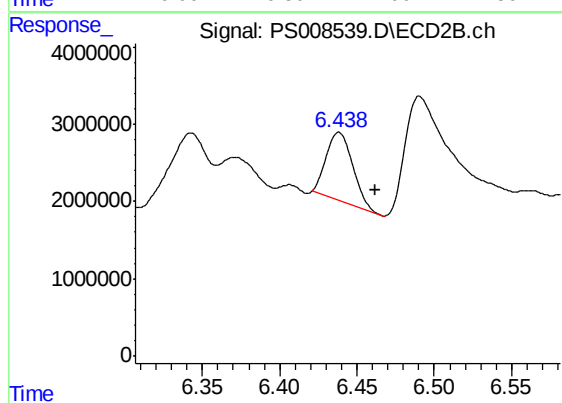

#7 MCPA


R.T.: 6.438 min
Delta R.T.: -0.023 min
Response: 10618213
Conc: 2.49 ug/ml

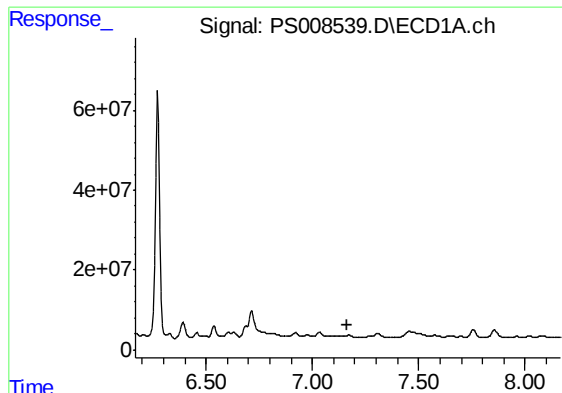

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.167 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-7-6-COMP

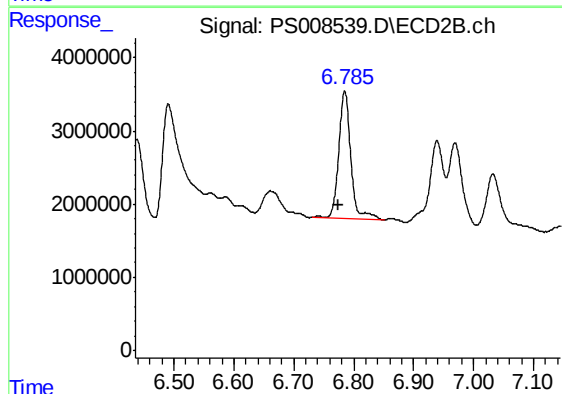


#8 DICHLORPROP

R.T.: 6.785 min
Delta R.T.: 0.010 min
Response: 2426554
Conc: 25.12 ng/ml

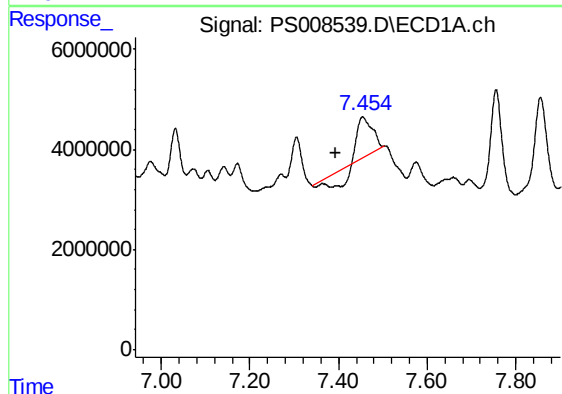


#9 2,4-D

R.T.: 7.454 min
Delta R.T.: 0.060 min
Response: 9942662
Conc: 5.47 ng/ml

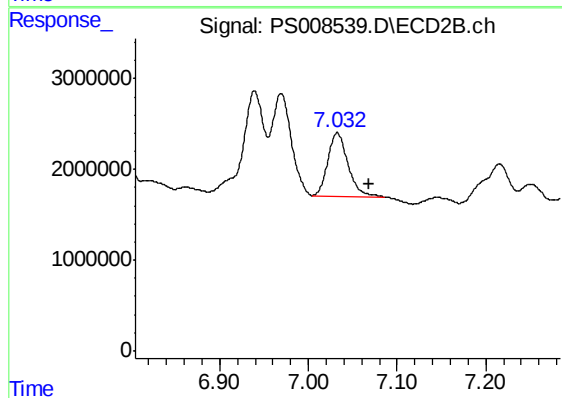

#9 2,4-D


R.T.: 7.033 min
Delta R.T.: -0.036 min
Response: 10916856
Conc: 9.31 ng/ml

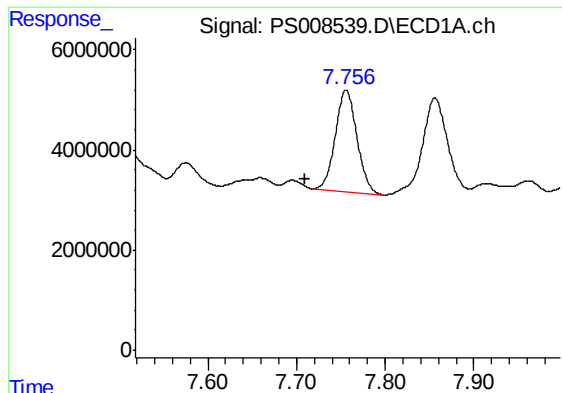

#10 Pentachlorophenol


R.T.: 7.756 min
Delta R.T.: 0.046 min
Response: 34377139
Conc: 1.41 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-7-6-COMP

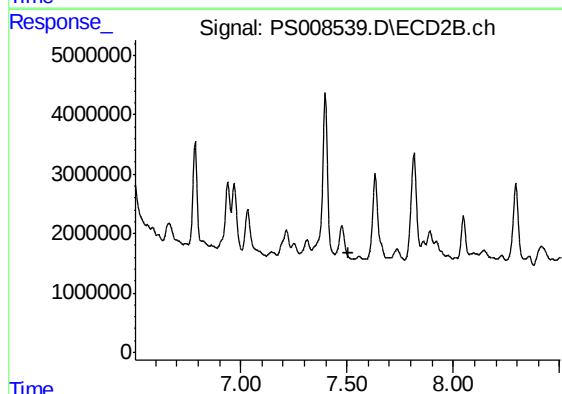


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 7.505 min
Response: 0
Conc: N.D.

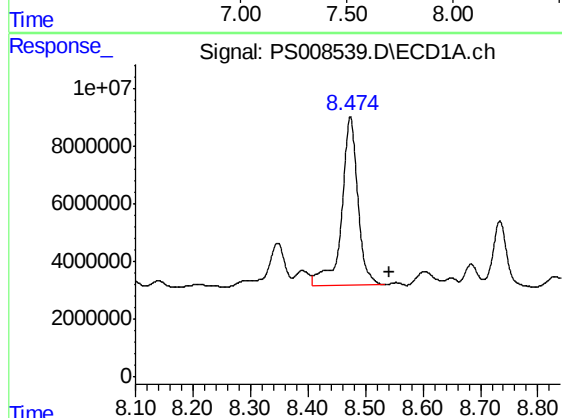


#12 2,4,5-T

R.T.: 8.474 min
Delta R.T.: -0.067 min
Response: 113393245
Conc: 12.29 ng/ml

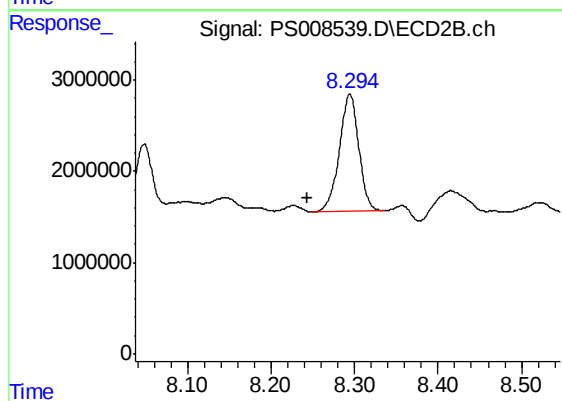

#12 2,4,5-T


R.T.: 8.294 min
Delta R.T.: 0.051 min
Response: 20742937
Conc: 3.92 ng/ml

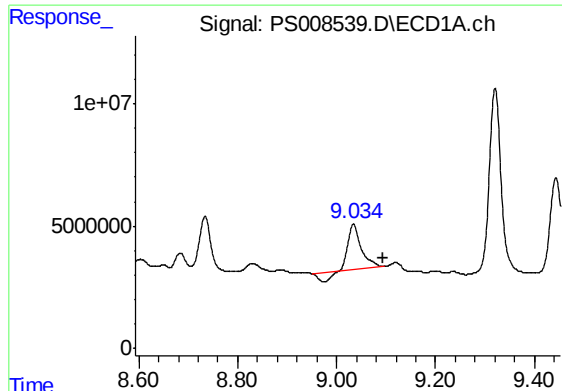

#13 2,4-DB


R.T.: 9.034 min
Delta R.T.: -0.061 min
Response: 31240980
Conc: 22.54 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-7-6-COMP

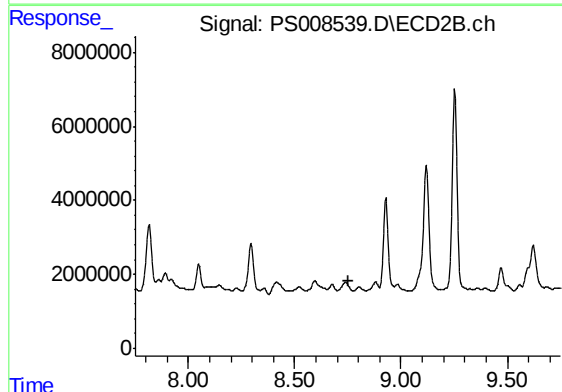


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 8.751 min
Response: 0
Conc: N.D.

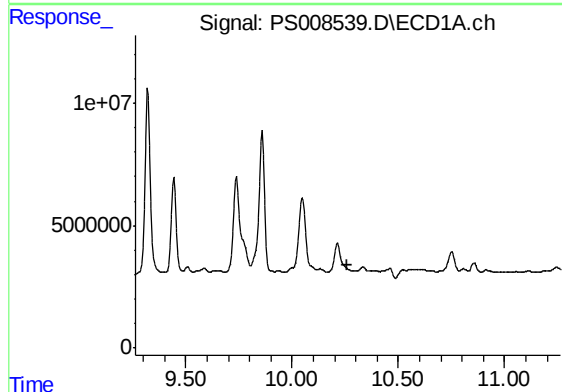


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 10.263 min
Response: 0
Conc: N.D.

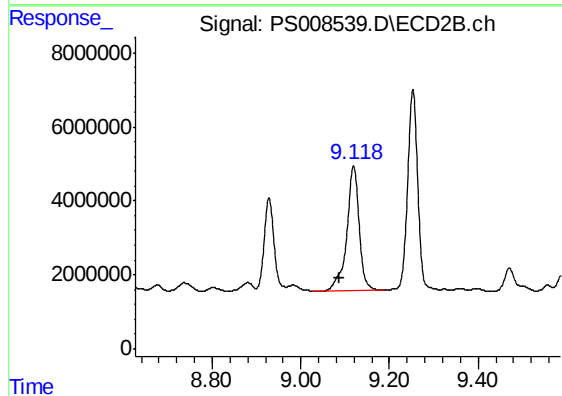

#14 DINOSEB


R.T.: 9.119 min
Delta R.T.: 0.031 min
Response: 65761244
Conc: 17.41 ng/ml

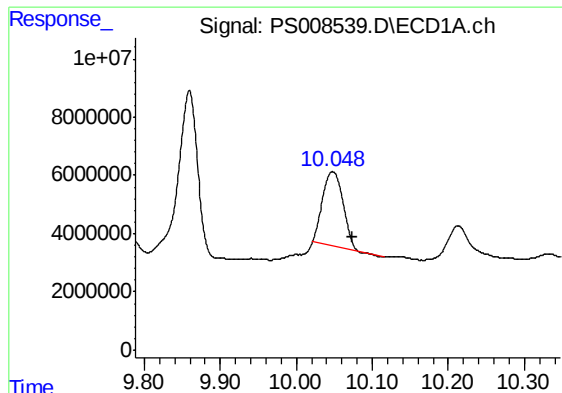

#15 Picloram

R.T.: 10.048 min
Delta R.T.: -0.025 min
Response: 48533680
Conc: 3.89 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-7-6-COMP

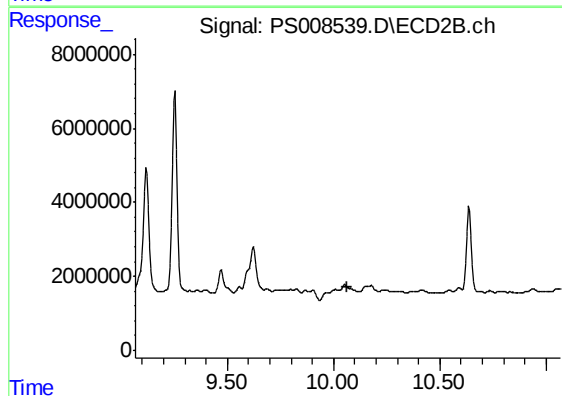

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.068 min
Response: 0
Conc: N.D.