

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012422\
 Data File : PS018102.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jan 2022 08:54
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 24 20:56:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 06 10:21:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

2) T	3,5-DICHL...	6.314	0.000	84518276	0	39.288	N.D.	#
5) T	DICAMBA	0.000	6.847f	0	46385625	N.D.	17.643	
6) T	MCPD	0.000	6.847f	0	46385625	N.D.	21.565	
7) T	MCPA	7.479f	0.000	5310774	0	<MDL	N.D.	#
9) T	2,4-D	8.196f	0.000	180.9E6	0	99.345	N.D.	#
11) T	2,4,5-TP ...	0.000	8.431f	0	16023065	N.D.	4.495	
12) T	2,4,5-T	9.279	0.000	16139374	0	1.821	N.D.	#
13) T	2,4-DB	9.819	0.000	6873893	0	4.158	N.D.	#
15) T	Picloram	10.799	10.657	59776572	22238633	5.008	4.756	
16) T	DCPA	0.000	10.657f	0	22238633	N.D.	5.037	



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012422\
Data File : PS018102.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jan 2022 08:54
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 24 20:56:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
Quant Title : 8080.M
QLast Update : Thu Jan 06 10:21:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

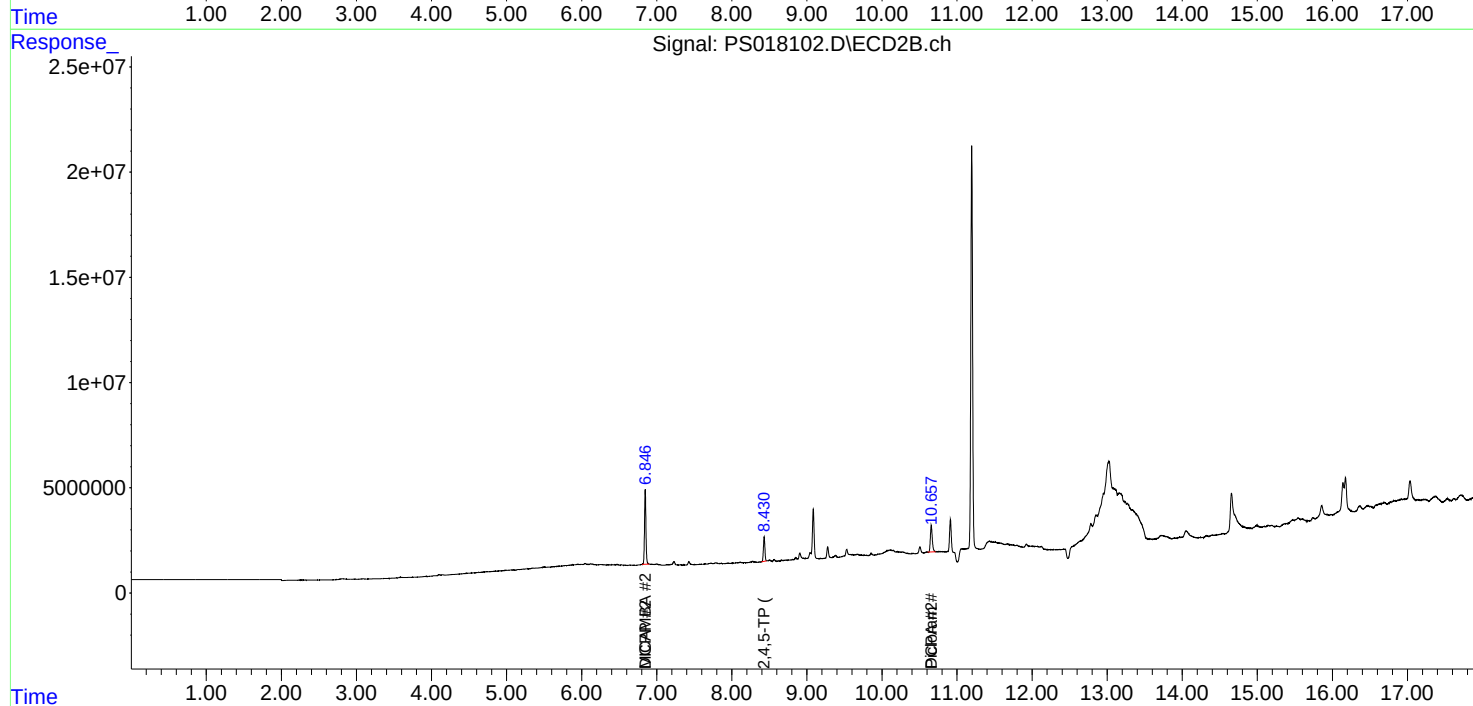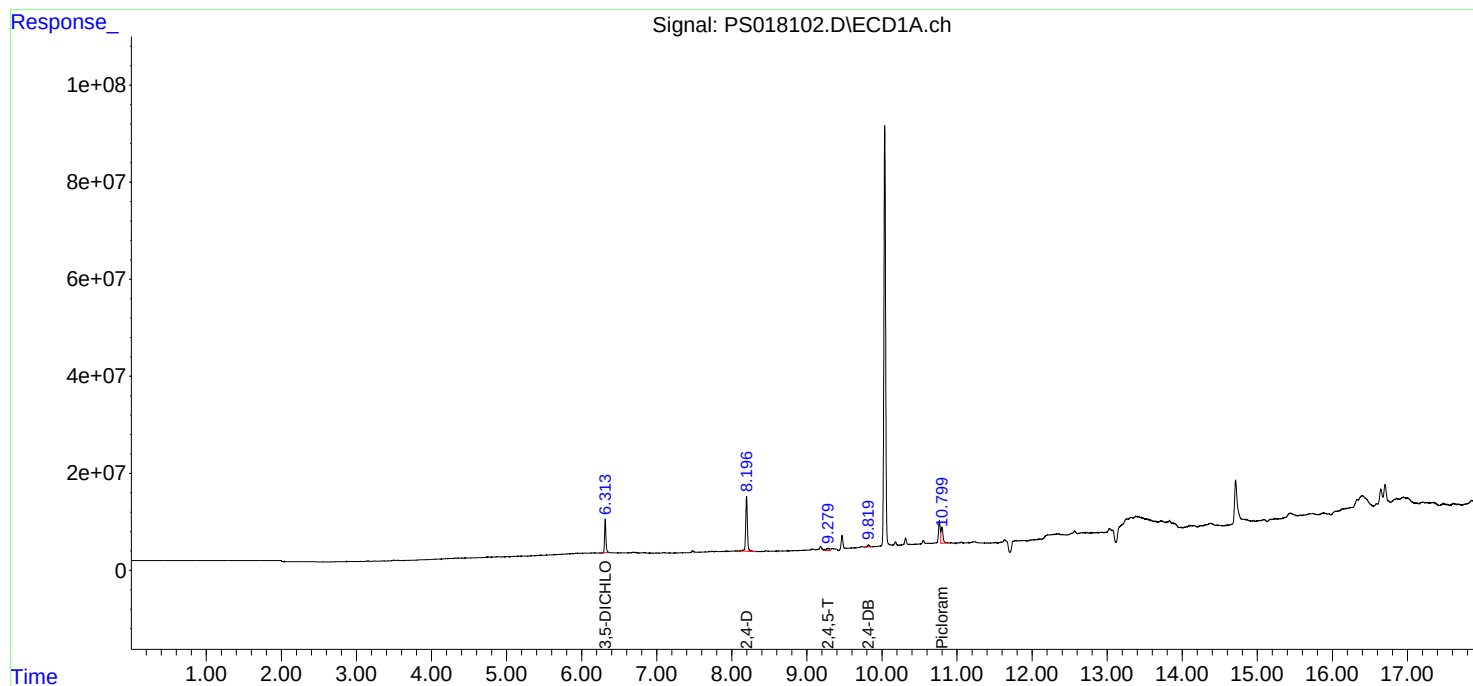


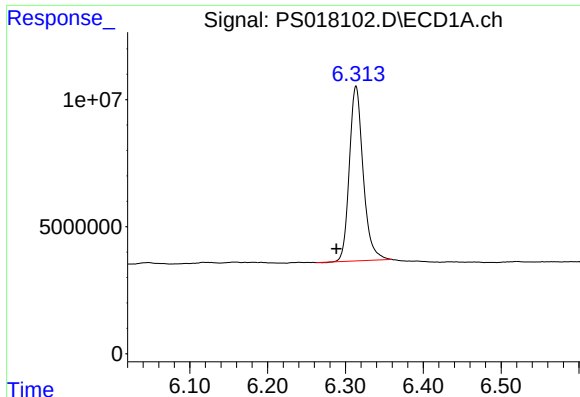

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.314 min
Delta R.T.: 0.025 min
Response: 84518276
Conc: 39.29 ng/ml

Instrument :
ECD_S
ClientSampleId :

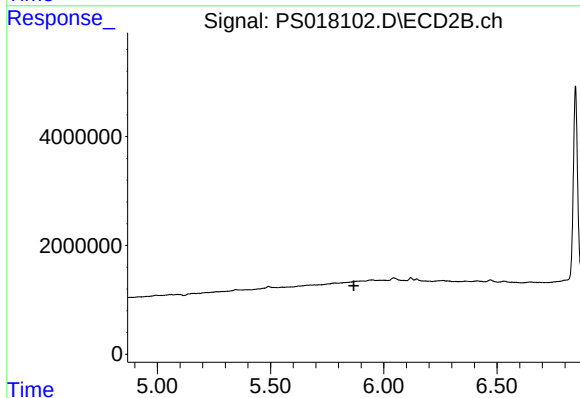


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.868 min
Response: 0
Conc: N.D.

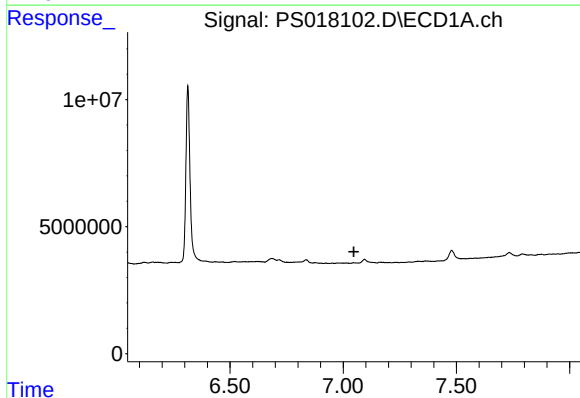


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.047 min
Response: 0
Conc: N.D.

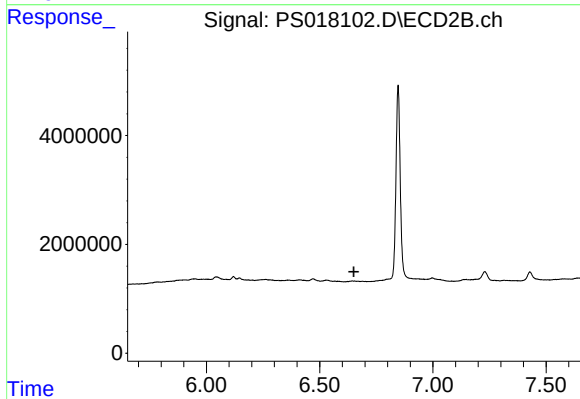

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.651 min
Response: 0
Conc: N.D.

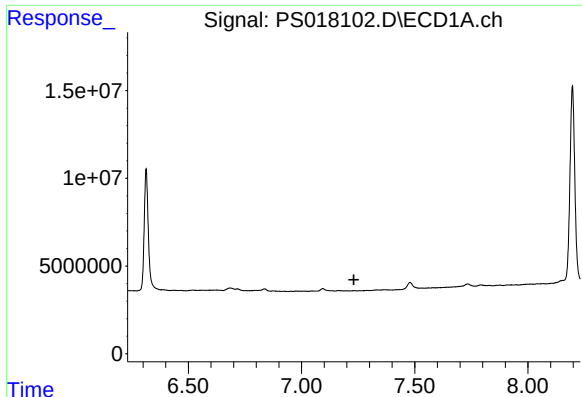

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.231 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

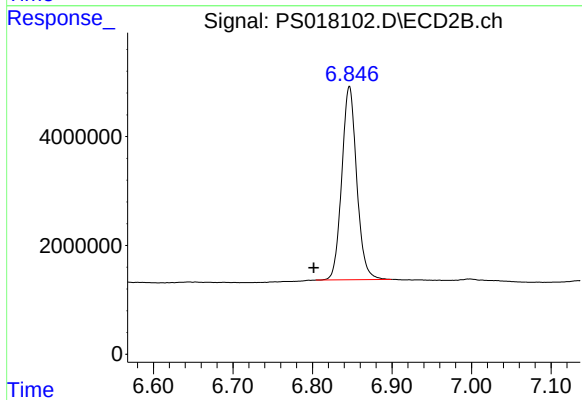


#5 DICAMBA

R.T.: 6.847 min
Delta R.T.: 0.045 min
Response: 46385625
Conc: 17.64 ng/ml

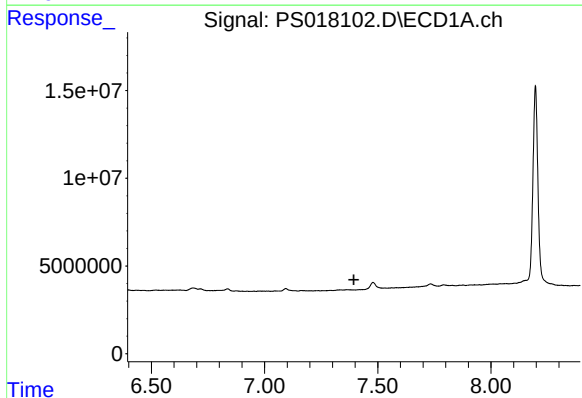


#6 MCP

R.T.: 0.000 min
Exp R.T.: 7.395 min
Response: 0
Conc: N.D.

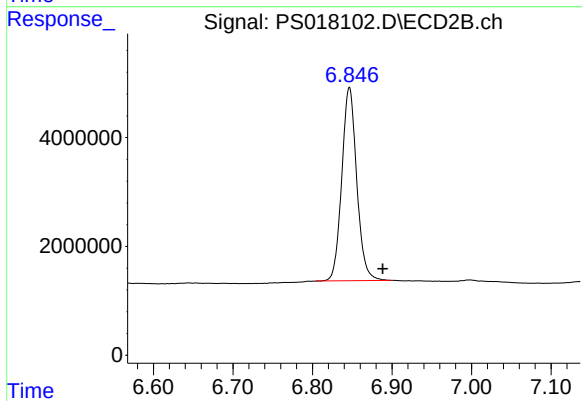

#6 MCP


R.T.: 6.847 min
Delta R.T.: -0.042 min
Response: 46385625
Conc: 21.57 ug/ml

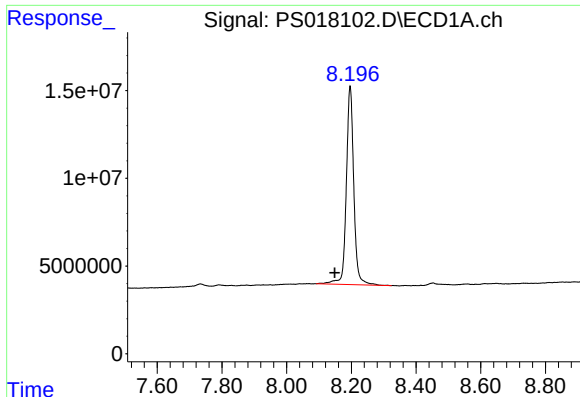

#9 2,4-D


R.T.: 8.196 min
Delta R.T.: 0.047 min
Response: 180900998
Conc: 99.35 ng/ml

Instrument :
ECD_S
ClientSampleId :

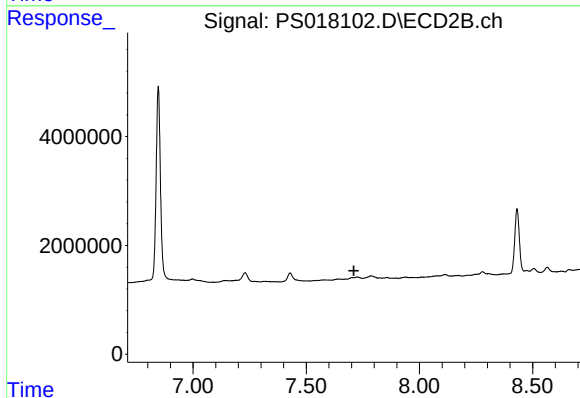


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.710 min
Response: 0
Conc: N.D.

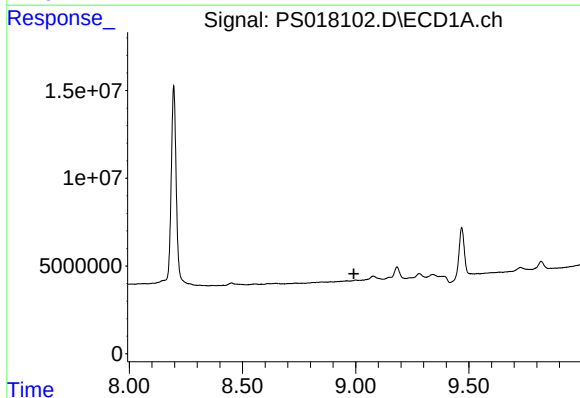


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 8.992 min
Response: 0
Conc: N.D.

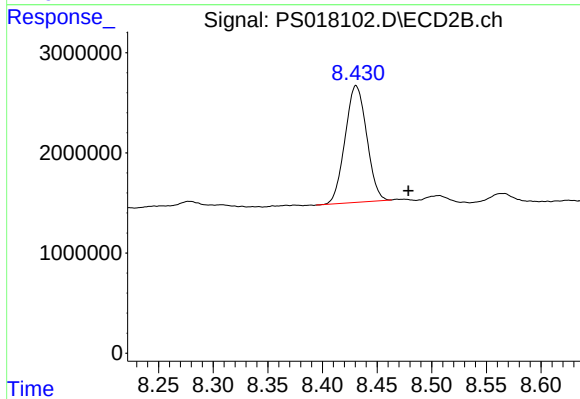

#11 2,4,5-TP (SILVEX)


R.T.: 8.431 min
Delta R.T.: -0.048 min
Response: 16023065
Conc: 4.49 ng/ml

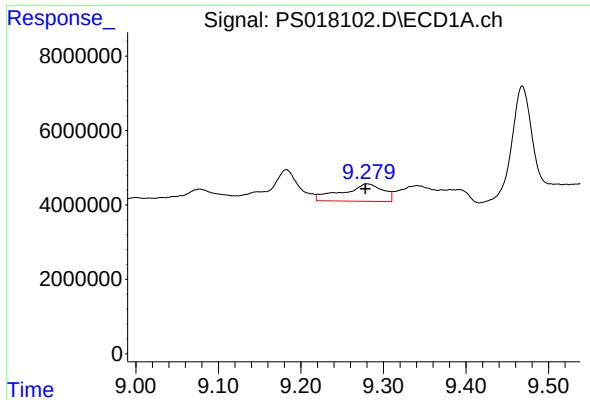

#12 2,4,5-T


R.T.: 9.279 min
Delta R.T.: 0.001 min
Response: 16139374
Conc: 1.82 ng/ml

Instrument :
ECD_S
ClientSampleId :

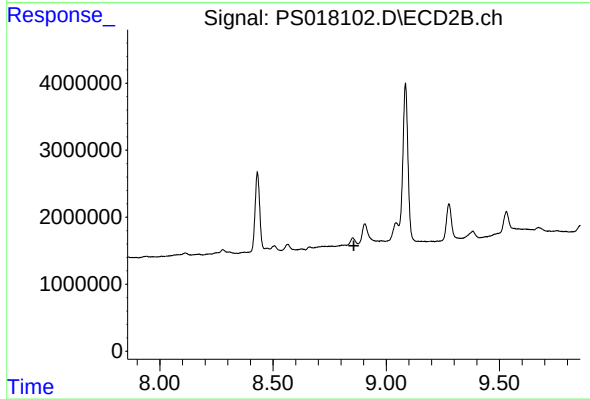


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 8.857 min
Response: 0
Conc: N.D.

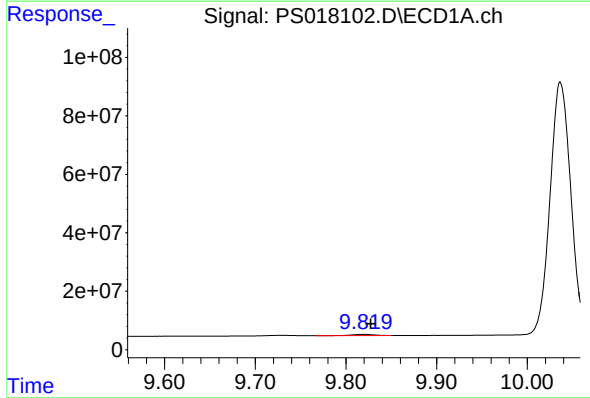


#13 2,4-DB

R.T.: 9.819 min
Delta R.T.: -0.008 min
Response: 6873893
Conc: 4.16 ng/ml

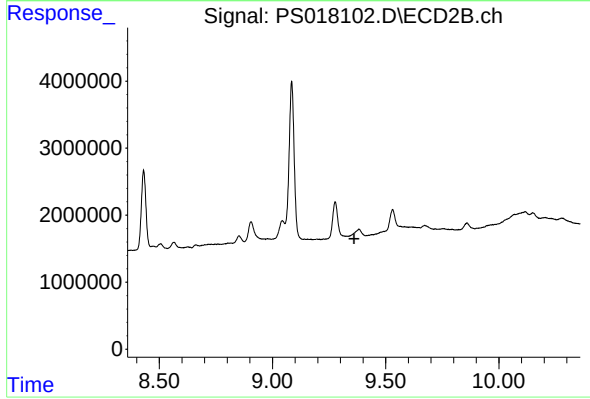

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.360 min
Response: 0
Conc: N.D.

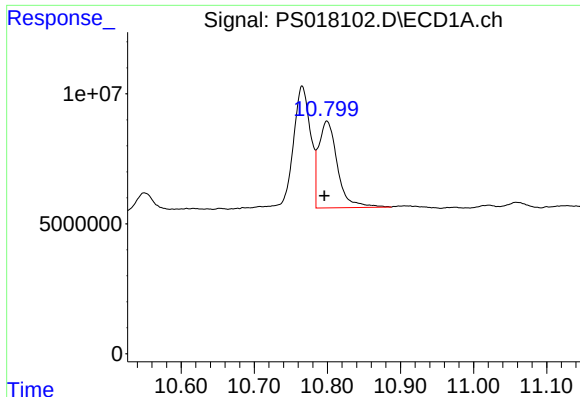

#15 Picloram


R.T.: 10.799 min
Delta R.T.: 0.003 min
Response: 59776572
Conc: 5.01 ng/ml

Instrument :
ECD_S
ClientSampleId :

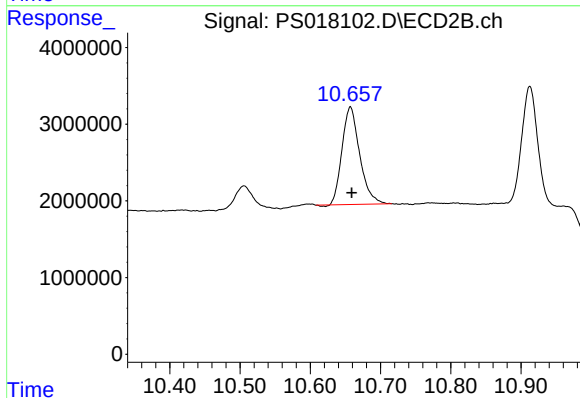


#15 Picloram

R.T.: 10.657 min
Delta R.T.: -0.002 min
Response: 22238633
Conc: 4.76 ng/ml

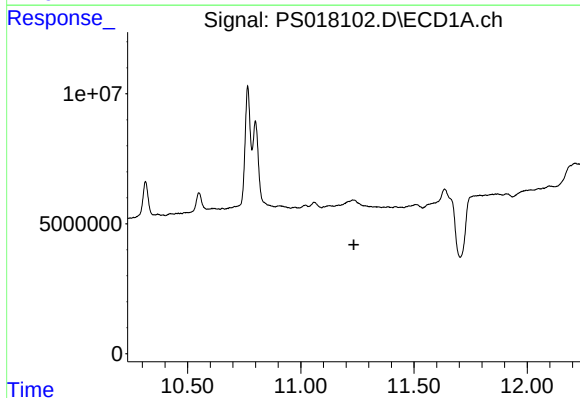

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.234 min
Response: 0
Conc: N.D.

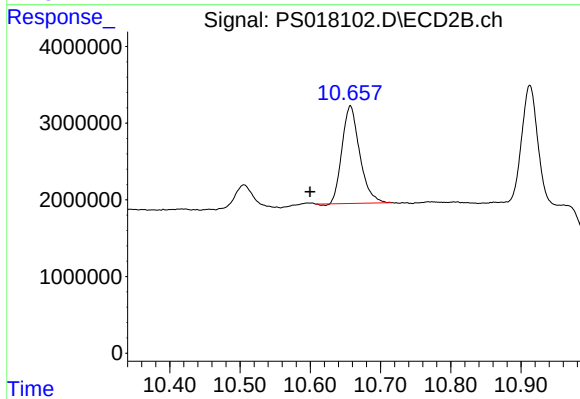

#16 DCPA

R.T.: 10.657 min
Delta R.T.: 0.057 min
Response: 22238633
Conc: 5.04 ng/ml