

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012422\
 Data File : PS018105.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jan 2022 12:02
 Operator : AJ\MA
 Sample : PB142176BSD
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 24 20:57:49 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 06 10:21:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.048	6.646	750.4E6	294.8E6	519.110	508.024
Target Compounds							
1) T	Dalapon	2.909	2.415	1100.7E6	330.4E6	448.670	432.016
2) T	3,5-DICHL...	6.288	5.861	1007.2E6	421.3E6	468.183	476.191
3) T	4-Nitroph...	6.877	6.282	429.7E6	162.5E6	531.999	530.017
5) T	DICAMBA	7.234	6.799	2938.5E6	1232.1E6	470.578	468.652
6) T	MCPD	7.403	6.892	212.6E6	95818025	45.534	44.547
7) T	MCPA	7.549	7.100	305.5E6	136.3E6	45.784	45.674
8) T	DICHLORPROP	7.921	7.410	751.3E6	307.5E6	477.602	460.661
9) T	2,4-D	8.149	7.700	892.7E6	363.8E6	490.266	494.348
10) T	Pentachlo...	8.447	8.112	10441.8E6	4131.1E6	494.261	490.490
11) T	2,4,5-TP ...	8.997	8.475	4071.0E6	1709.0E6	481.084	479.432
12) T	2,4,5-T	9.280	8.852	4303.7E6	1632.9E6	485.513	499.216
13) T	2,4-DB	9.828	9.355	860.9E6	208.2E6	520.809	470.515
14) T	DINOSEB	10.974	9.675	3075.8E6	1148.1E6	468.378	460.165
15) T	Picloram	10.799	10.657	5685.8E6	2204.4E6	476.363	471.409
16) T	DCPA	11.243	10.602	5268.2E6	2115.0E6	487.577	479.003



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012422\
Data File : PS018105.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jan 2022 12:02
Operator : AJ\MA
Sample : PB142176BSD
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 24 20:57:49 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
Quant Title : 8080.M
QLast Update : Thu Jan 06 10:21:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

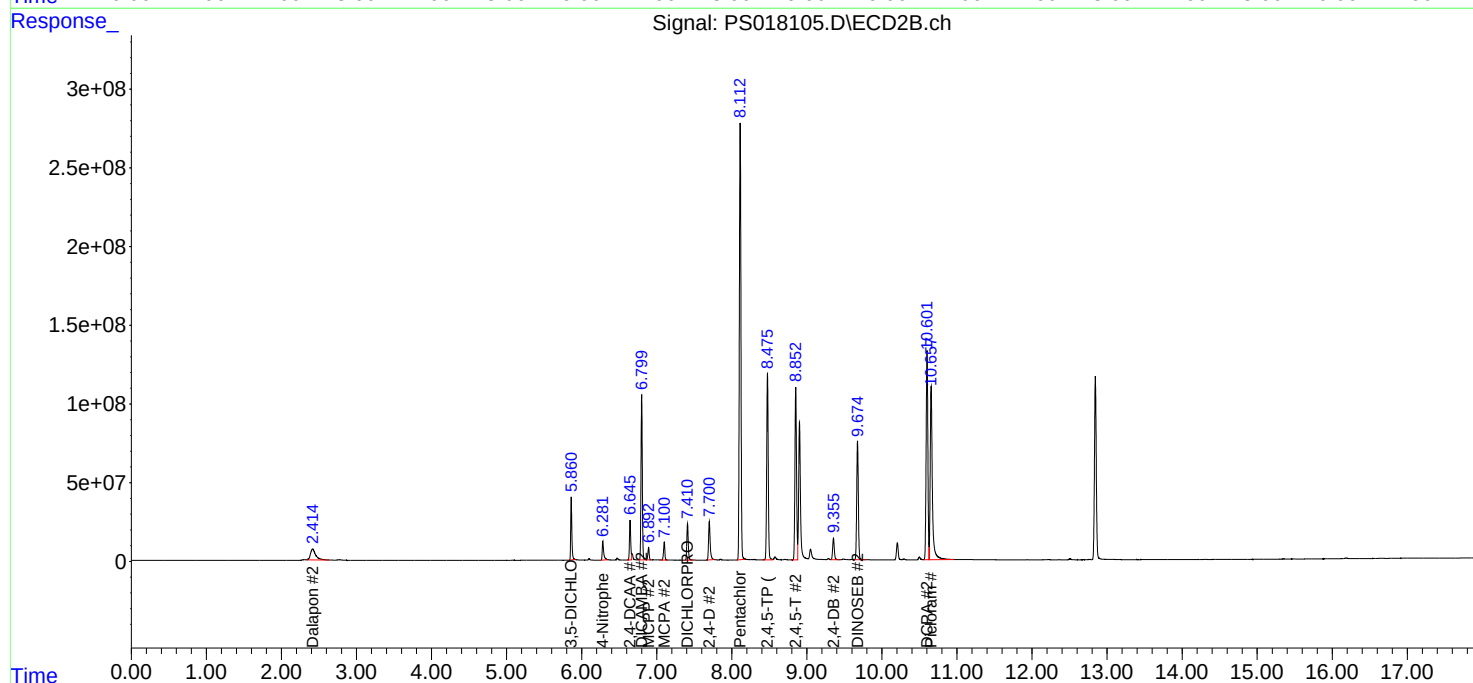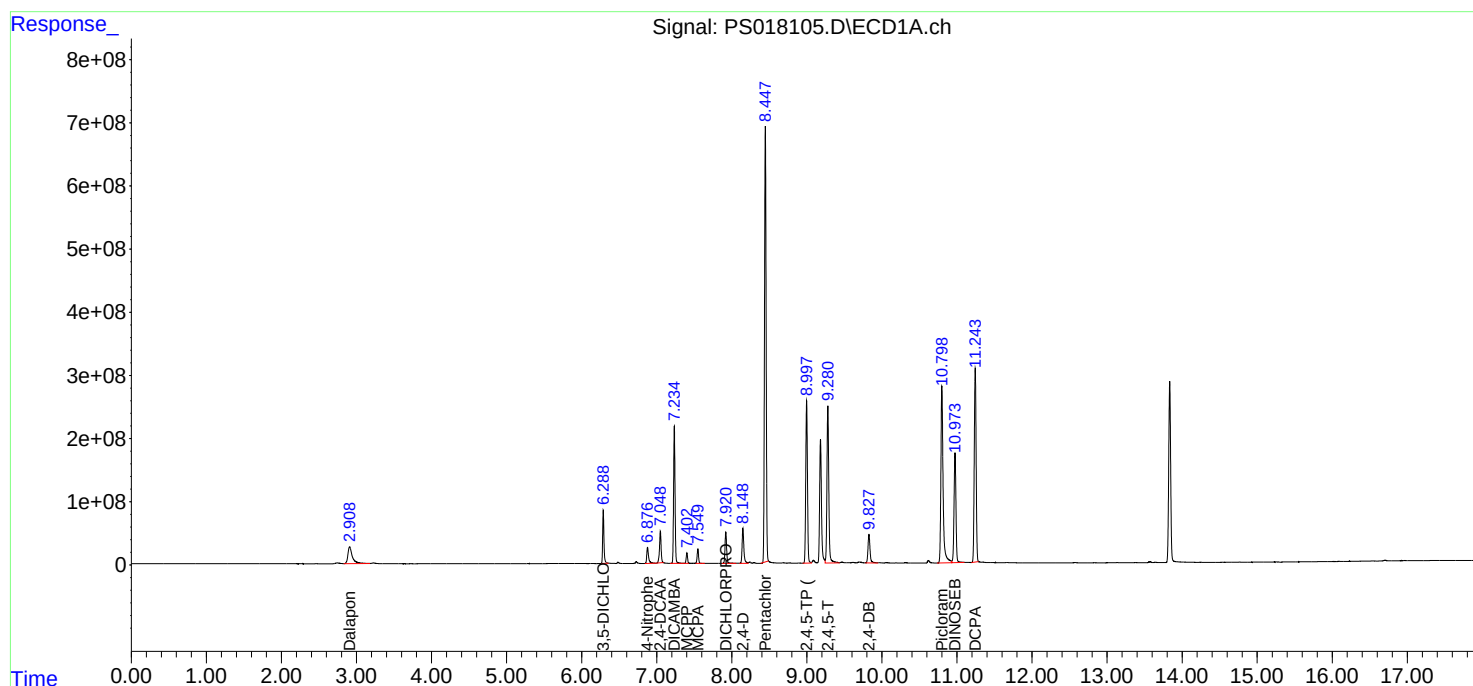


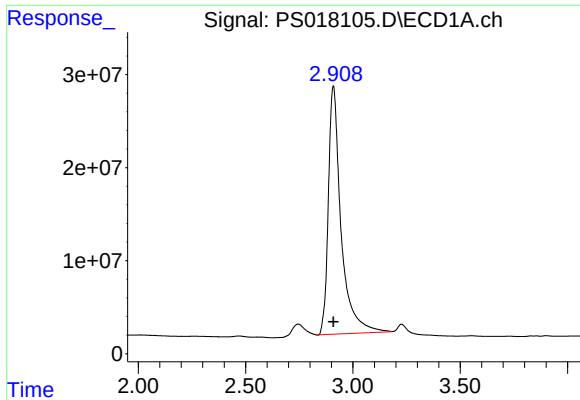

#1 Dalapon


R.T.: 2.909 min
Delta R.T.: 0.000 min
Response: 1100687209
Conc: 448.67 ng/ml

Instrument :
ECD_S
ClientSampleId :

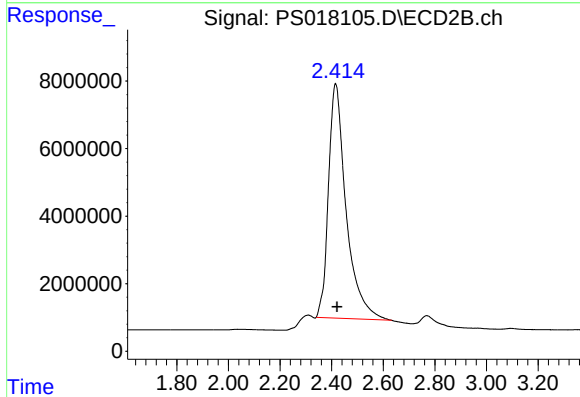


#1 Dalapon

R.T.: 2.415 min
Delta R.T.: -0.006 min
Response: 330357677
Conc: 432.02 ng/ml

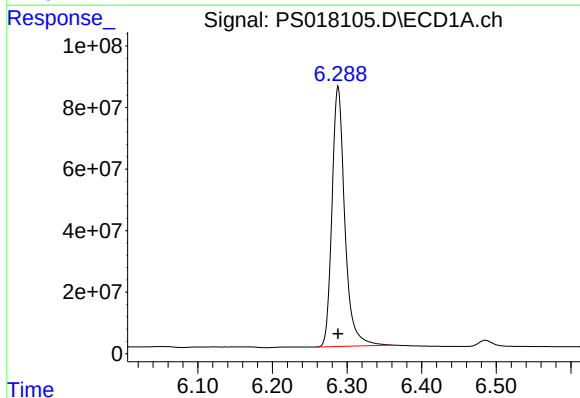


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.288 min
Delta R.T.: 0.000 min
Response: 1007174460
Conc: 468.18 ng/ml

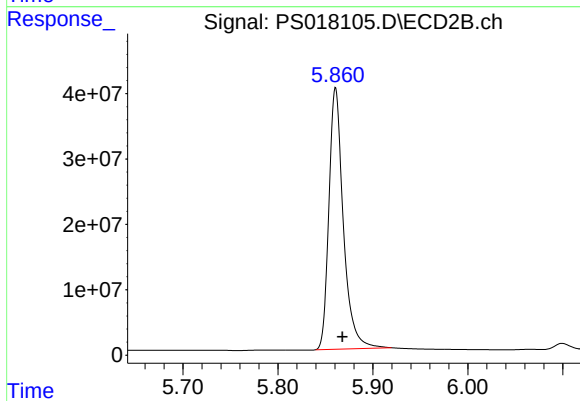

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.861 min
Delta R.T.: -0.007 min
Response: 421252675
Conc: 476.19 ng/ml

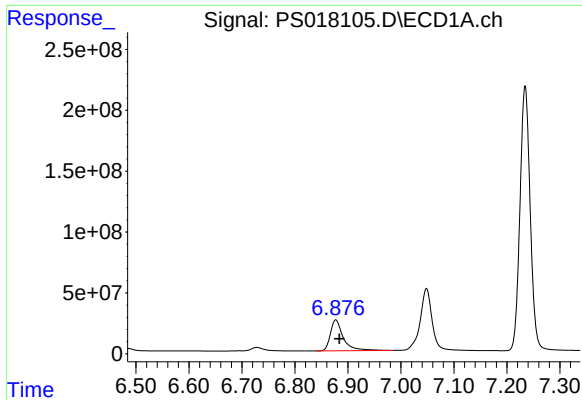

#3 4-Nitrophenol


R.T.: 6.877 min
Delta R.T.: -0.007 min
Response: 429687196
Conc: 532.00 ng/ml

Instrument :
ECD_S
ClientSampleId :

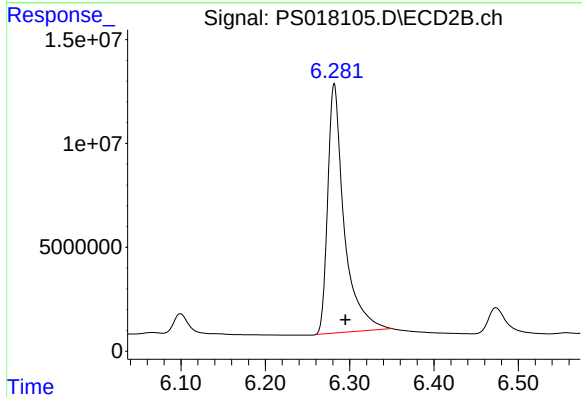


#3 4-Nitrophenol

R.T.: 6.282 min
Delta R.T.: -0.013 min
Response: 162461979
Conc: 530.02 ng/ml

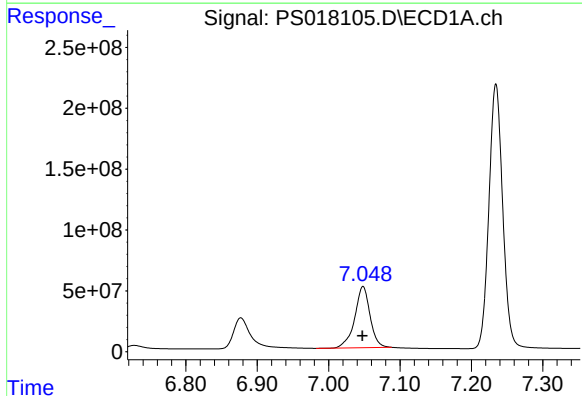


#4 2,4-DCAA

R.T.: 7.048 min
Delta R.T.: 0.000 min
Response: 750367847
Conc: 519.11 ng/ml

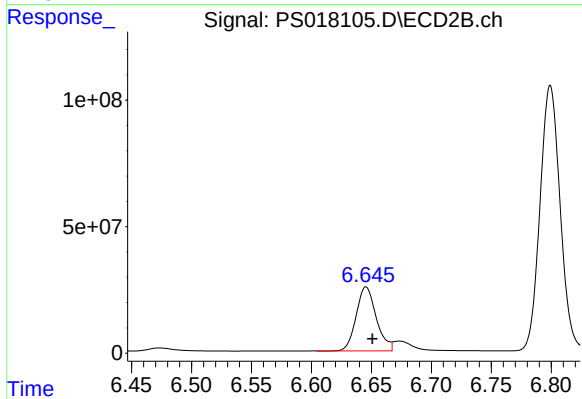

#4 2,4-DCAA


R.T.: 6.646 min
Delta R.T.: -0.005 min
Response: 294780340
Conc: 508.02 ng/ml

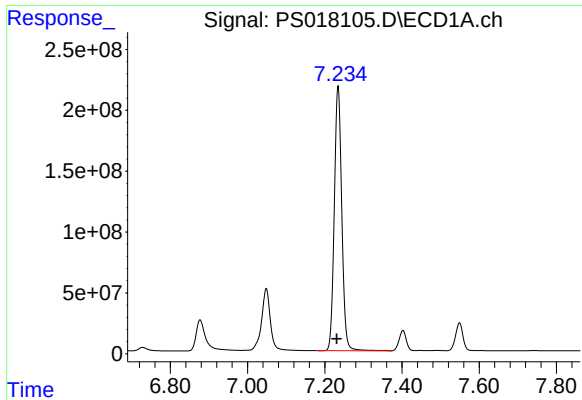

#5 DICAMBA


R.T.: 7.234 min
Delta R.T.: 0.003 min
Response: 2938487270
Conc: 470.58 ng/ml

Instrument :
ECD_S
ClientSampleId :

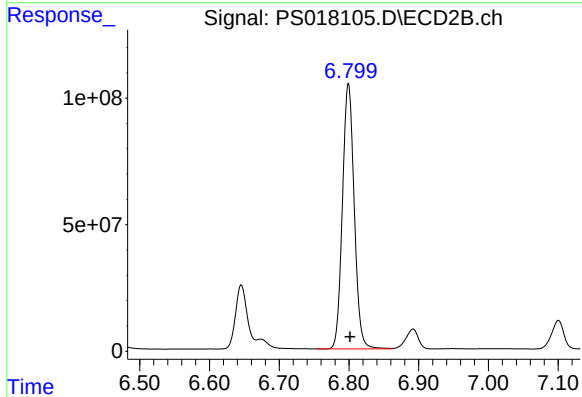


#5 DICAMBA

R.T.: 6.799 min
Delta R.T.: -0.002 min
Response: 1232111570
Conc: 468.65 ng/ml

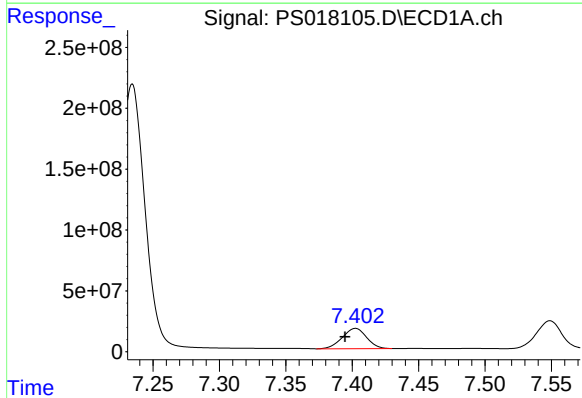


#6 MCP

R.T.: 7.403 min
Delta R.T.: 0.008 min
Response: 212597987
Conc: 45.53 ug/ml

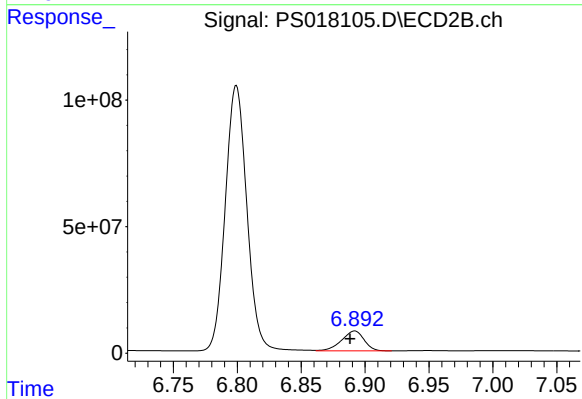

#6 MCP


R.T.: 6.892 min
Delta R.T.: 0.004 min
Response: 95818025
Conc: 44.55 ug/ml

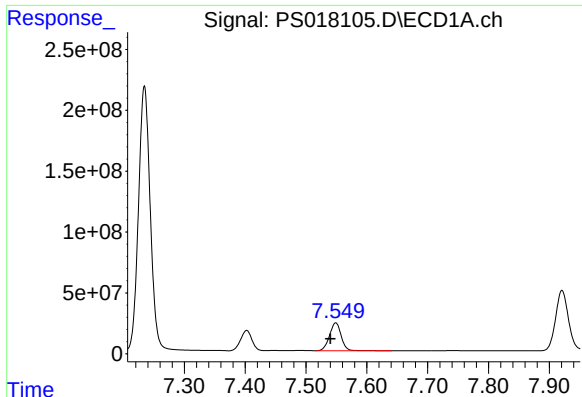

#7 MCPA


R.T.: 7.549 min
Delta R.T.: 0.009 min
Response: 305457348
Conc: 45.78 ug/ml

Instrument :
ECD_S
ClientSampleId :

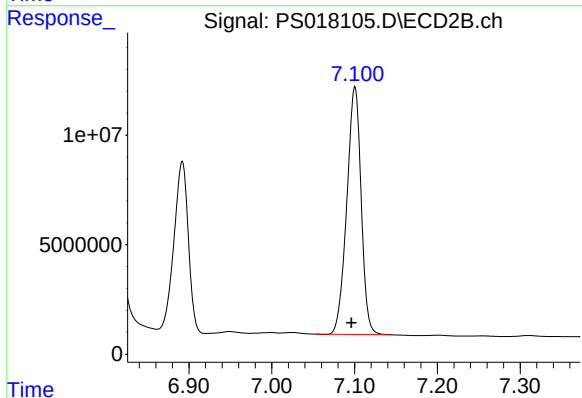


#7 MCPA

R.T.: 7.100 min
Delta R.T.: 0.004 min
Response: 136287339
Conc: 45.67 ug/ml

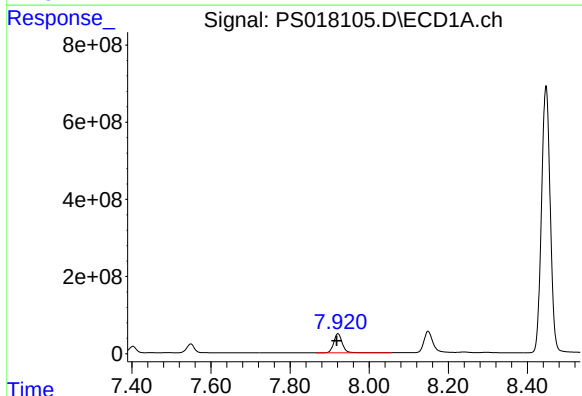


#8 DICHLORPROP

R.T.: 7.921 min
Delta R.T.: 0.003 min
Response: 751290588
Conc: 477.60 ng/ml

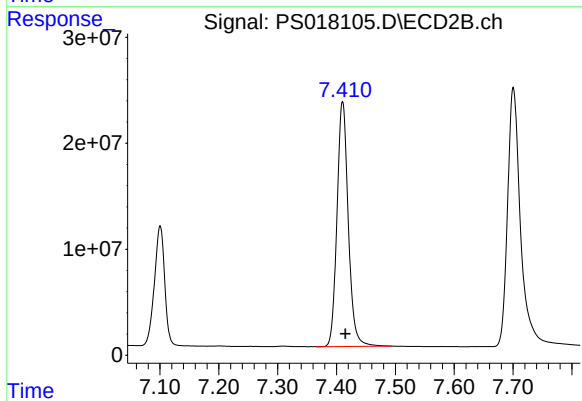

#8 DICHLORPROP


R.T.: 7.410 min
Delta R.T.: -0.005 min
Response: 307456110
Conc: 460.66 ng/ml

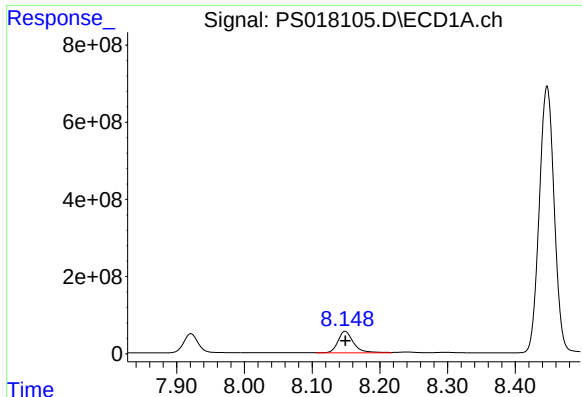

#9 2,4-D


R.T.: 8.149 min
Delta R.T.: 0.000 min
Response: 892743400
Conc: 490.27 ng/ml

Instrument :
ECD_S
ClientSampleId :

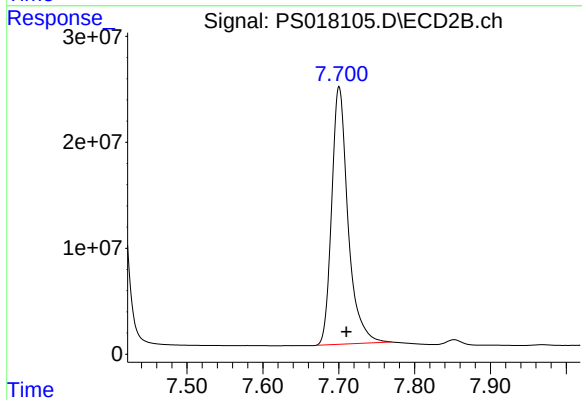


#9 2,4-D

R.T.: 7.700 min
Delta R.T.: -0.010 min
Response: 363813406
Conc: 494.35 ng/ml

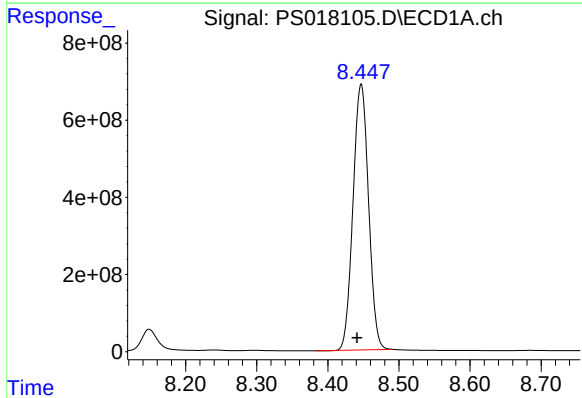


#10 Pentachlorophenol

R.T.: 8.447 min
Delta R.T.: 0.006 min
Response: 10441793631
Conc: 494.26 ng/ml

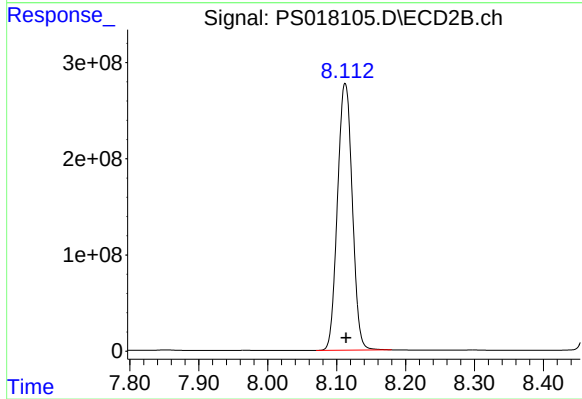

#10 Pentachlorophenol


R.T.: 8.112 min
Delta R.T.: -0.001 min
Response: 4131083952
Conc: 490.49 ng/ml

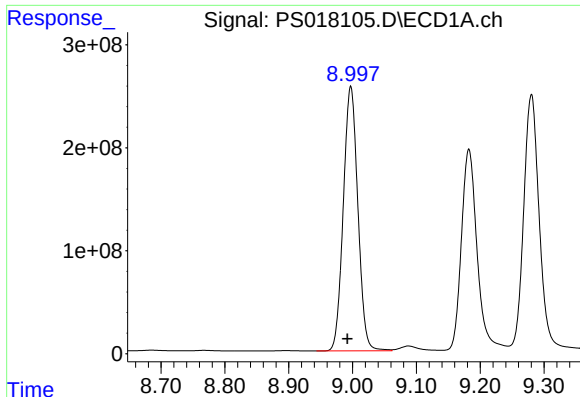

#11 2,4,5-TP (SILVEX)


R.T.: 8.997 min
Delta R.T.: 0.005 min
Response: 4070998827
Conc: 481.08 ng/ml

Instrument :
ECD_S
ClientSampleId :

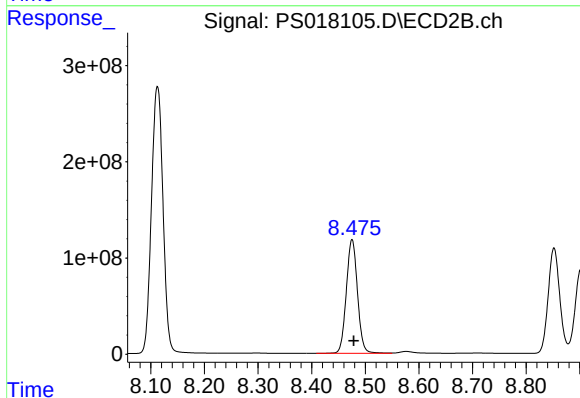


#11 2,4,5-TP (SILVEX)

R.T.: 8.475 min
Delta R.T.: -0.003 min
Response: 1709029447
Conc: 479.43 ng/ml

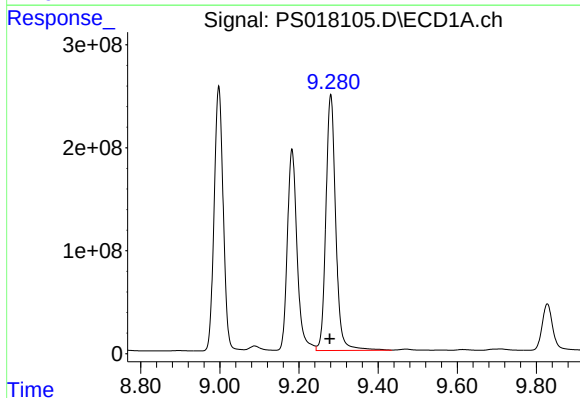


#12 2,4,5-T

R.T.: 9.280 min
Delta R.T.: 0.002 min
Response: 4303651170
Conc: 485.51 ng/ml

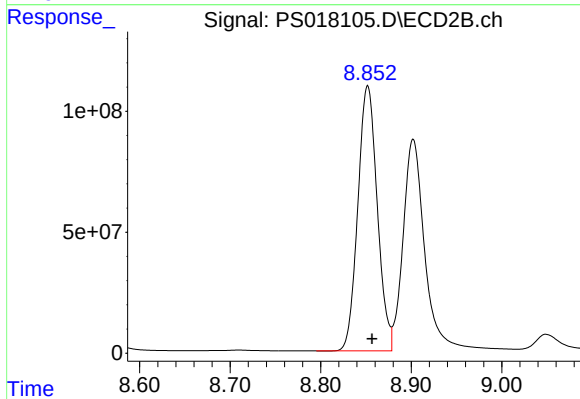

#12 2,4,5-T


R.T.: 8.852 min
Delta R.T.: -0.005 min
Response: 1632943981
Conc: 499.22 ng/ml

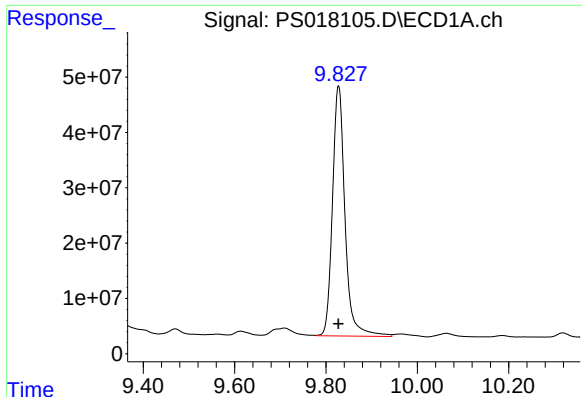

#13 2,4-DB


R.T.: 9.828 min
Delta R.T.: 0.000 min
Response: 860914190
Conc: 520.81 ng/ml

Instrument :
ECD_S
ClientSampleId :

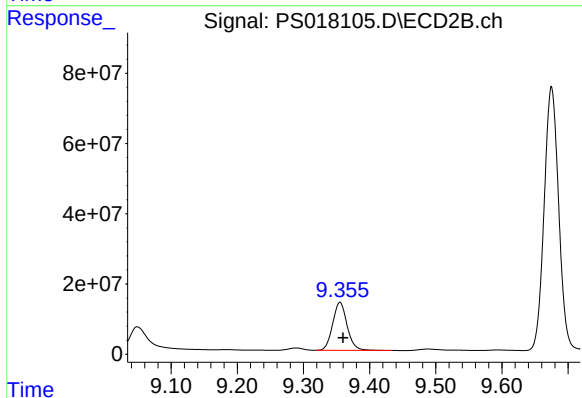


#13 2,4-DB

R.T.: 9.355 min
Delta R.T.: -0.005 min
Response: 208182799
Conc: 470.52 ng/ml

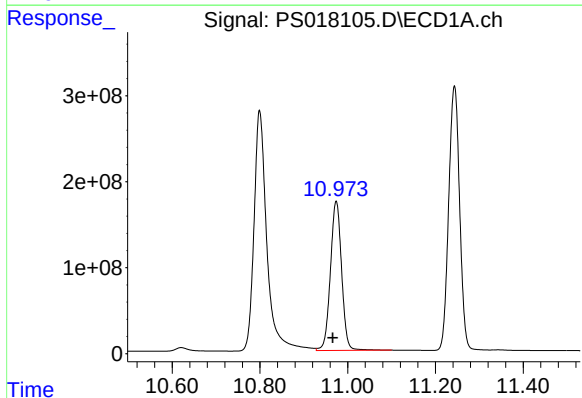


#14 DINOSEB

R.T.: 10.974 min
Delta R.T.: 0.008 min
Response: 3075811040
Conc: 468.38 ng/ml

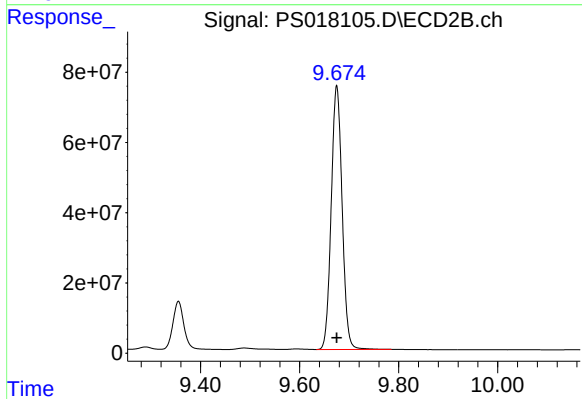

#14 DINOSEB


R.T.: 9.675 min
Delta R.T.: 0.000 min
Response: 1148118594
Conc: 460.16 ng/ml

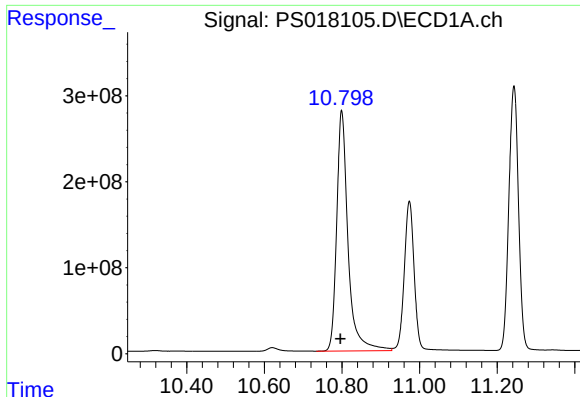

#15 Picloram


R.T.: 10.799 min
Delta R.T.: 0.003 min
Response: 5685828135
Conc: 476.36 ng/ml

Instrument :
ECD_S
ClientSampleId :

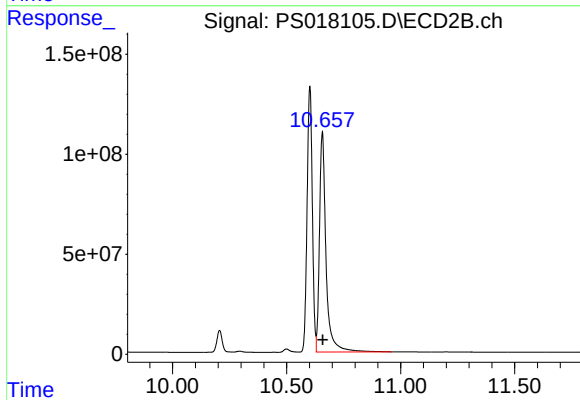


#15 Picloram

R.T.: 10.657 min
Delta R.T.: -0.002 min
Response: 2204378302
Conc: 471.41 ng/ml

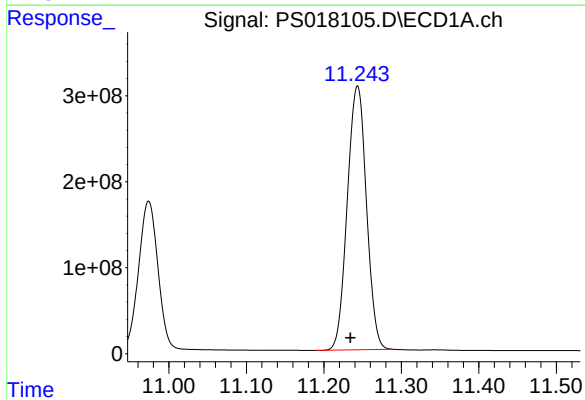

#16 DCPA

R.T.: 11.243 min
Delta R.T.: 0.009 min
Response: 5268163321
Conc: 487.58 ng/ml

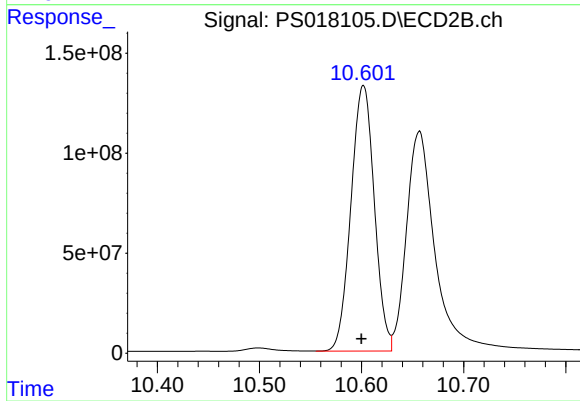

#16 DCPA

R.T.: 10.602 min
Delta R.T.: 0.002 min
Response: 2115030046
Conc: 479.00 ng/ml