

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012422\
 Data File : PS018115.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jan 2022 21:08
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 24 21:18:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 06 10:21:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.045	6.646	682.6E6	302.8E6	472.240	521.796
Target Compounds							
7) T	MCPA	7.489f	0.000	10944631	0	1.640	N.D. #
9) T	2,4-D	8.201f	0.000	1283763	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.050f	8.435f	33965906	19191907	4.014	5.384 #
14) T	DINOSEB	10.911f	0.000	10413910	0	1.586	N.D. #
15) T	Picloram	10.807	10.678	33639118	26753214	2.818	5.721 #
16) T	DCPA	11.228	0.000	6087984	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012422\
Data File : PS018115.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jan 2022 21:08
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 24 21:18:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
Quant Title : 8080.M
QLast Update : Thu Jan 06 10:21:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

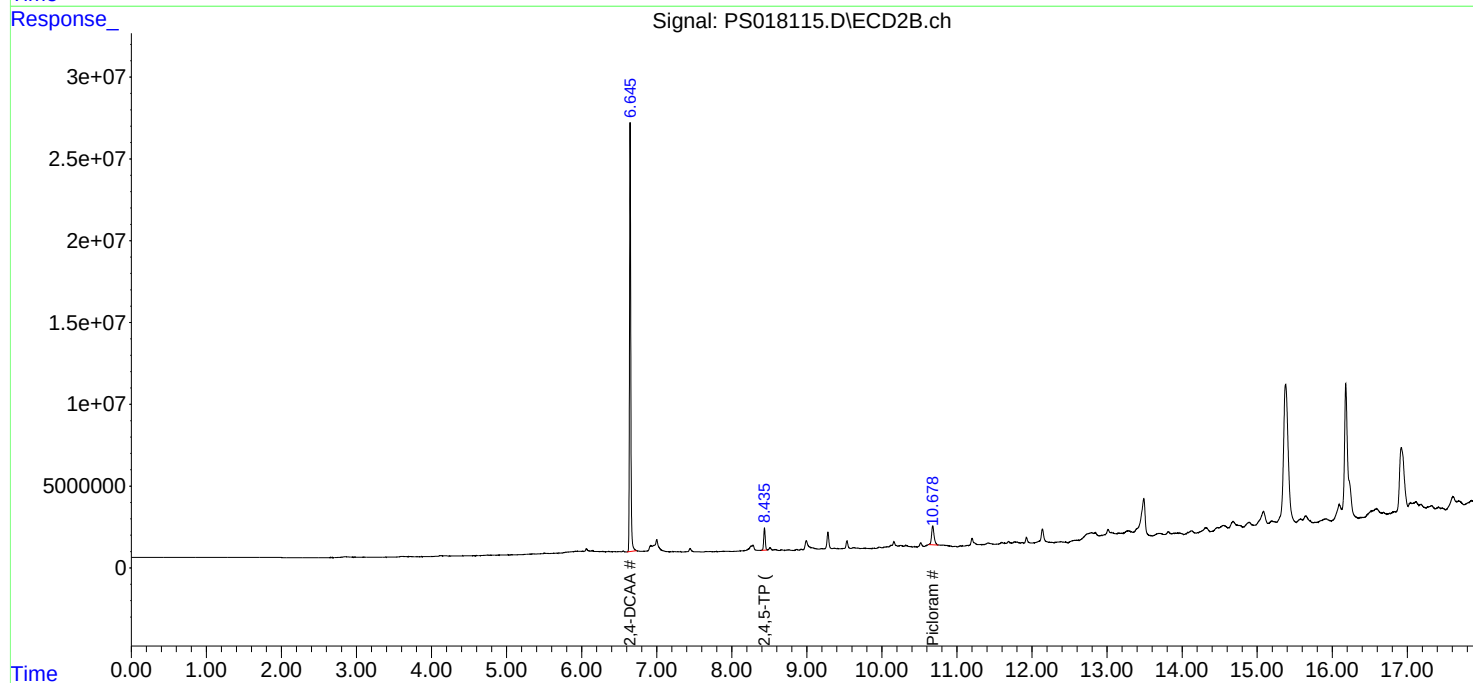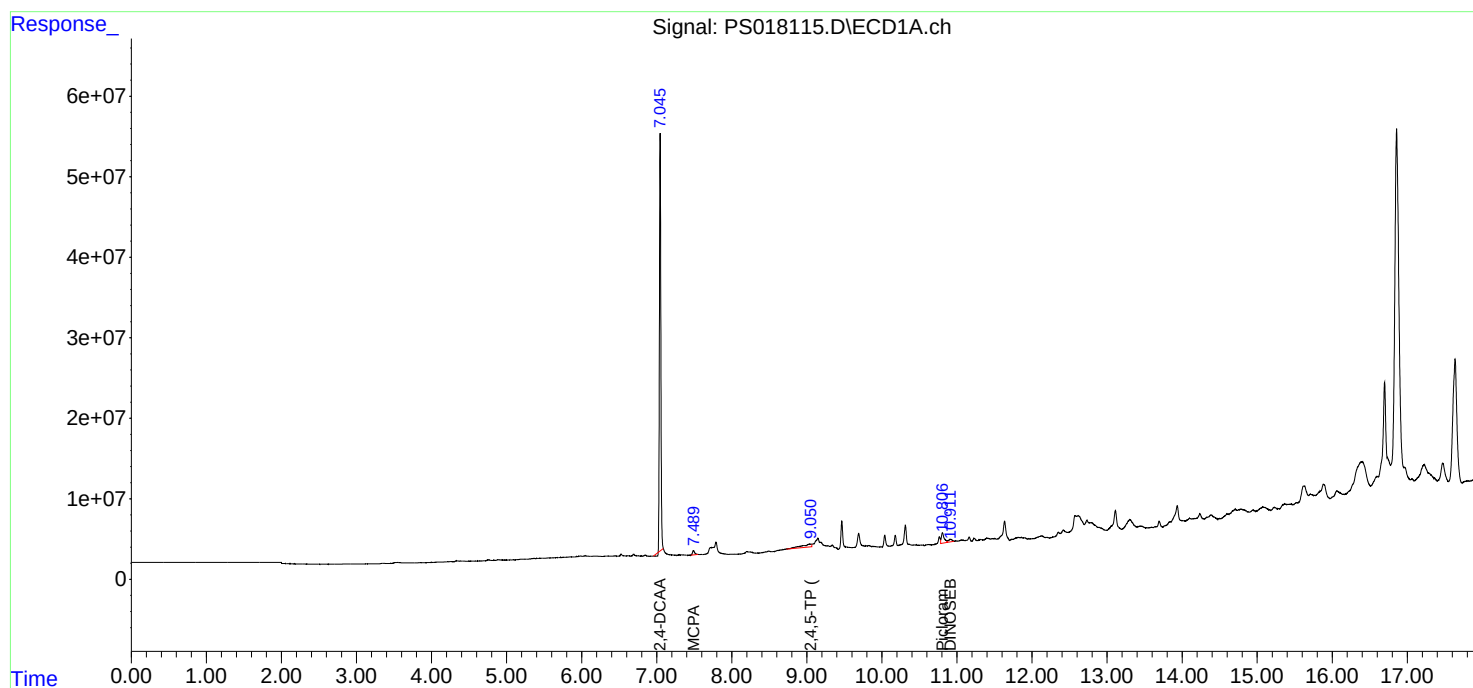


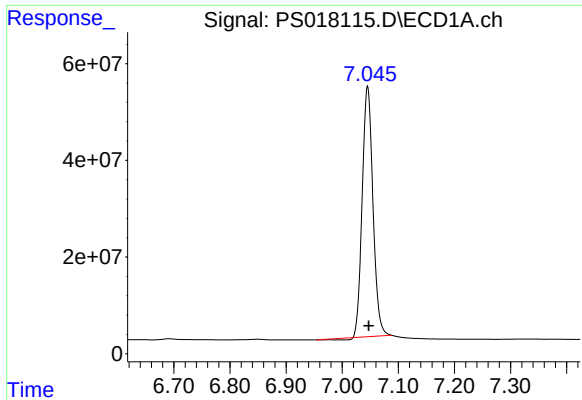

#4 2,4-DCAA


R.T.: 7.045 min
Delta R.T.: -0.002 min
Response: 682616461
Conc: 472.24 ng/ml

Instrument :
ECD_S
ClientSampleId :

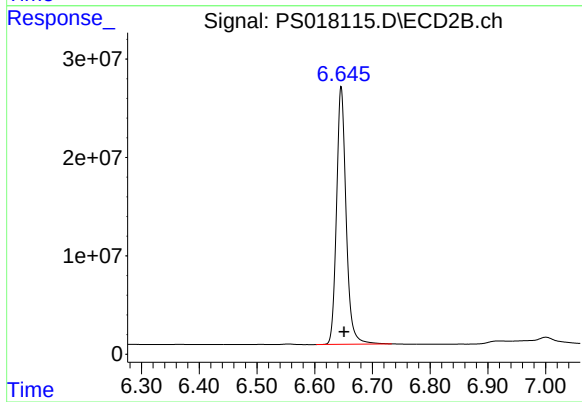


#4 2,4-DCAA

R.T.: 6.646 min
Delta R.T.: -0.005 min
Response: 302771542
Conc: 521.80 ng/ml

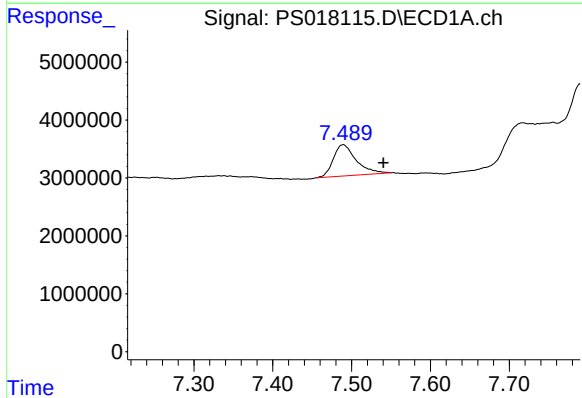


#7 MCPA

R.T.: 7.489 min
Delta R.T.: -0.051 min
Response: 10944631
Conc: 1.64 ug/ml

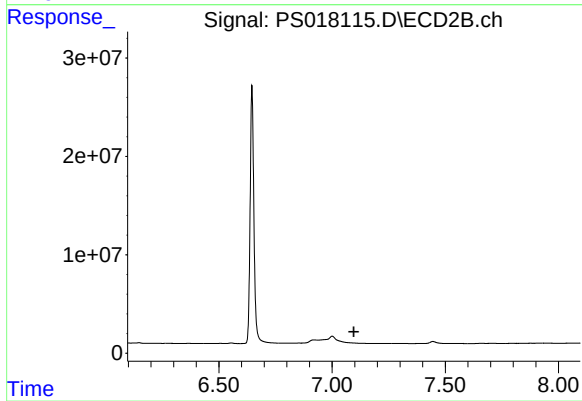

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 7.096 min
Response: 0
Conc: N.D.

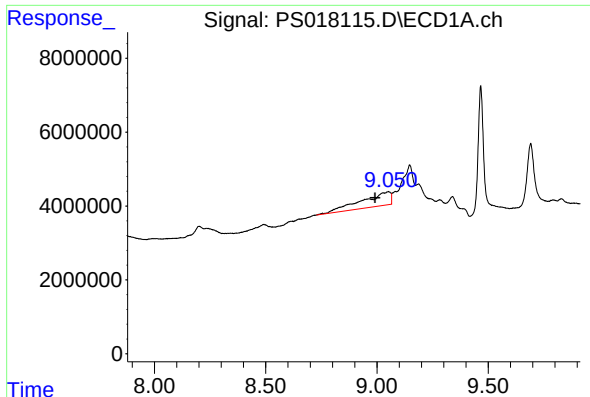

#11 2,4,5-TP (SILVEX)


R.T.: 9.050 min
Delta R.T.: 0.058 min
Response: 33965906
Conc: 4.01 ng/ml

Instrument :
ECD_S
ClientSampleId :

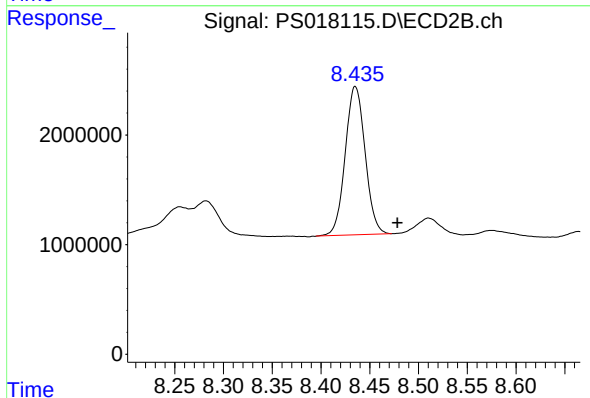


#11 2,4,5-TP (SILVEX)

R.T.: 8.435 min
Delta R.T.: -0.043 min
Response: 19191907
Conc: 5.38 ng/ml

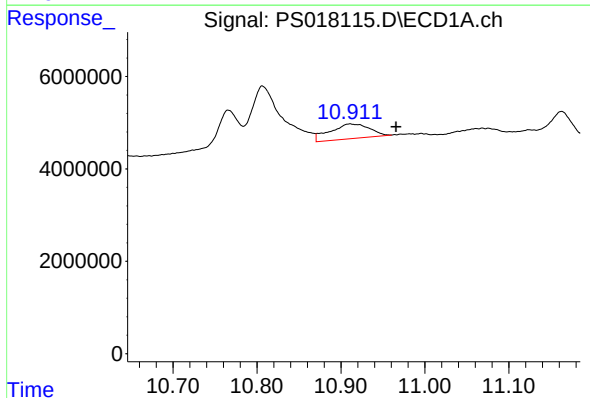


#14 DINOSEB

R.T.: 10.911 min
Delta R.T.: -0.055 min
Response: 10413910
Conc: 1.59 ng/ml

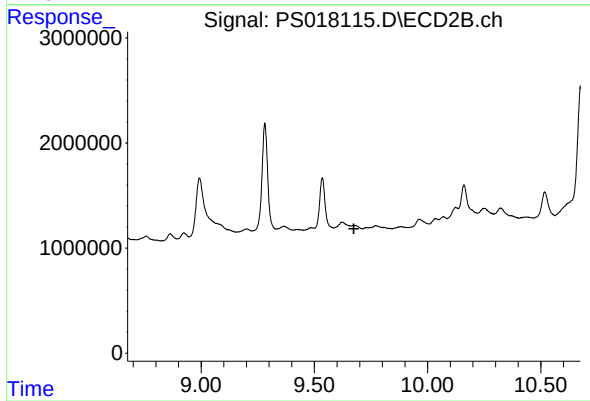

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 9.675 min
Response: 0
Conc: N.D.

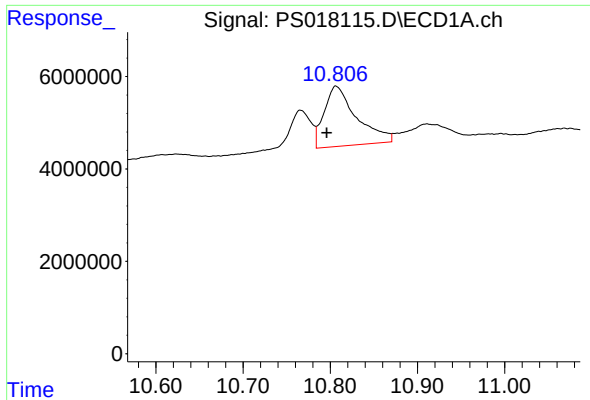

#15 Picloram

R.T.: 10.807 min
Delta R.T.: 0.011 min
Response: 33639118
Conc: 2.82 ng/ml

Instrument :
ECD_S
ClientSampleId :

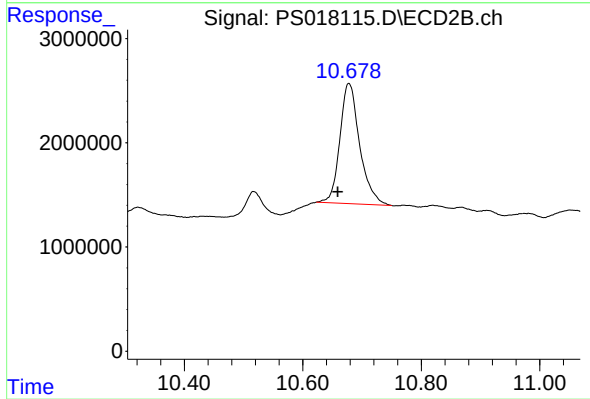

#15 Picloram

R.T.: 10.678 min
Delta R.T.: 0.019 min
Response: 26753214
Conc: 5.72 ng/ml