

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012523\
 Data File : PS021870.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jan 2023 09:29
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 25 20:43:24 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010923.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 10 10:34:52 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
4) S	2,4-DCAA	6.360	6.848	26924266	4180540	9.673	2.327 #
Target Compounds							
1) T	Dalapon	2.505	0.000	1266397	0	<MDL	N.D. #
3) T	4-Nitroph...	6.213	6.387f	10691562	783039	7.335	<MDL #
5) T	DICAMBA	6.524	7.023f	544497	3405.4E6	<MDL	400.504 #
6) T	MCP	6.734f	7.023f	29322306	3405.4E6	3.060	513.510 #
7) T	MCPA	6.734f	0.000	29322306	0	2.270	N.D. #
9) T	2,4-D	7.284	7.869	6670.2E6	1458622	1717.443	<MDL #
10) T	Pentachlo...	7.543	8.318	2069190	3211389	<MDL	<MDL #
11) T	2,4,5-TP ...	8.101	8.687	47942029	9064169	2.602	<MDL #
12) T	2,4,5-T	8.285f	0.000	11023626	0	<MDL	N.D. #
13) T	2,4-DB	0.000	9.624f	0	11844508	N.D.	7.906
14) T	DINOSEB	9.841f	9.912	80197845	2622751	4.886	<MDL #
15) T	Picloram	9.713	10.886	1498.0E6	1175783	52.805	<MDL #
16) T	DCPA	10.224f	10.831	-9299973	75282400	N.D.	5.401


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012523\
Data File : PS021870.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jan 2023 09:29
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 25 20:43:24 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010923.M
Quant Title : 8080.M
QLast Update : Tue Jan 10 10:34:52 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

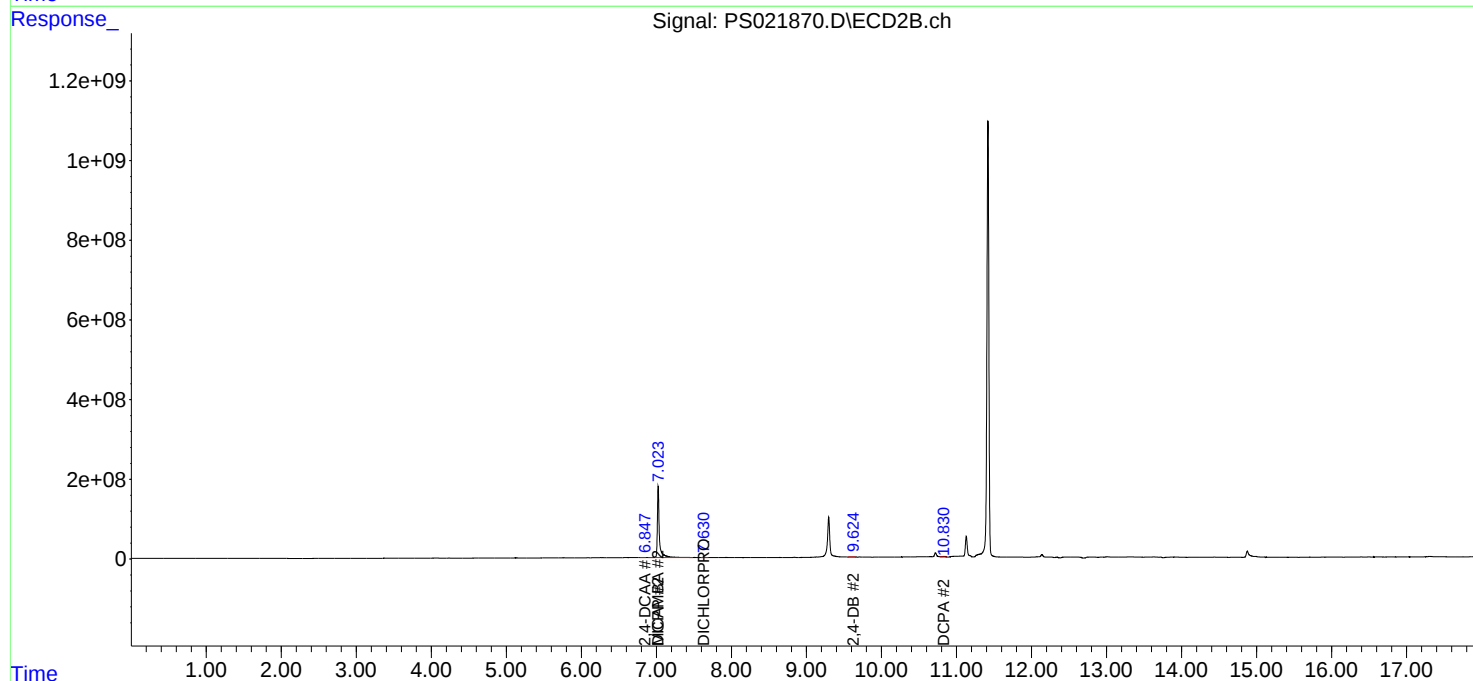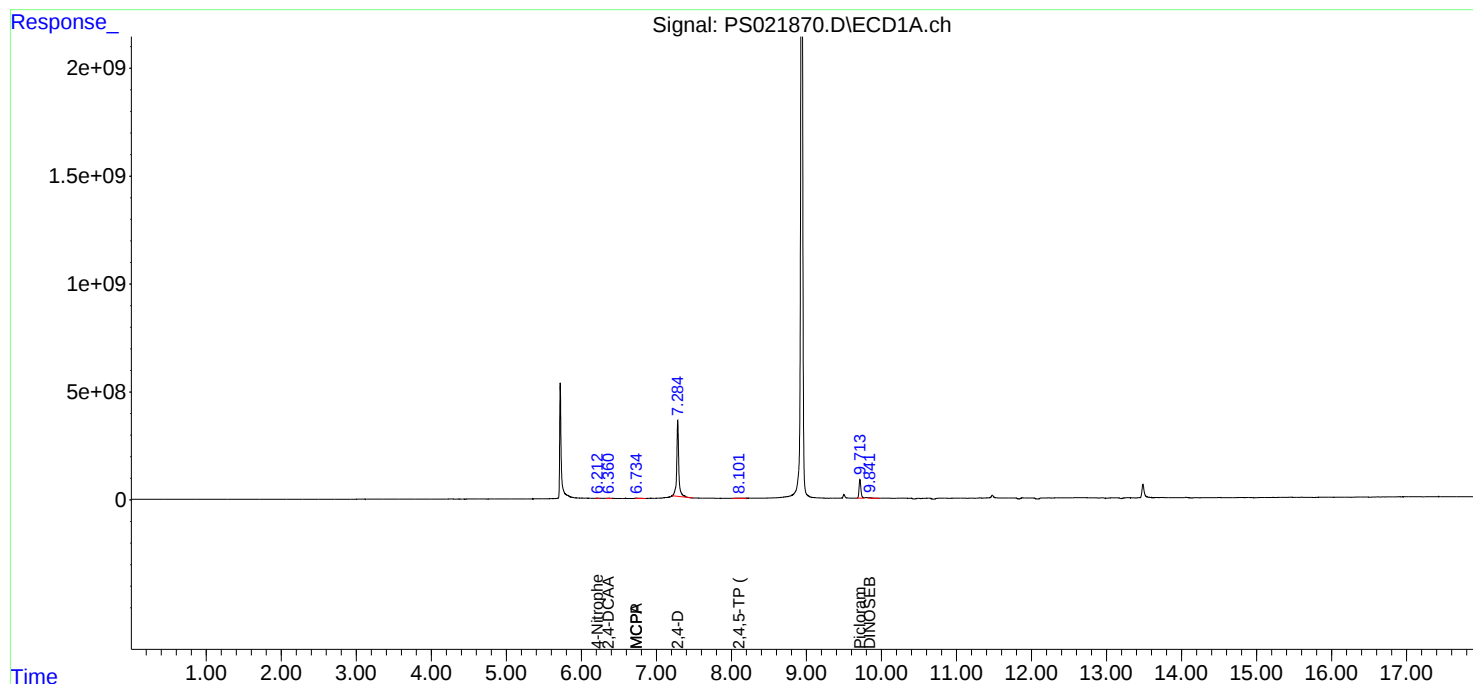

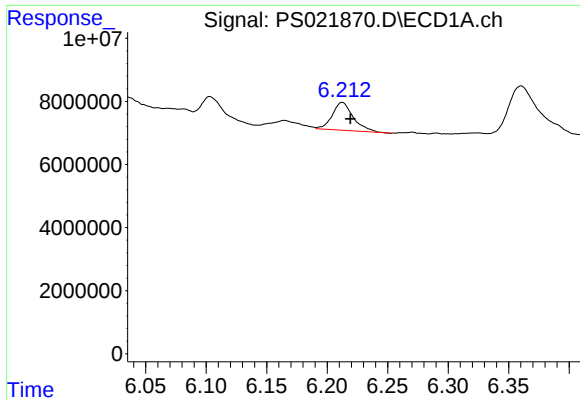


#3 4-Nitrophenol

R.T.: 6.213 min
Delta R.T.: -0.007 min
Response: 10691562
Conc: 7.33 ng/ml

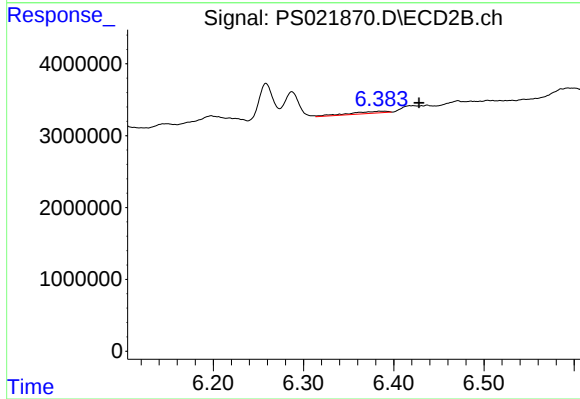


#3 4-Nitrophenol

R.T.: 6.387 min
Delta R.T.: -0.041 min
Response: 783039
Conc: N.D.

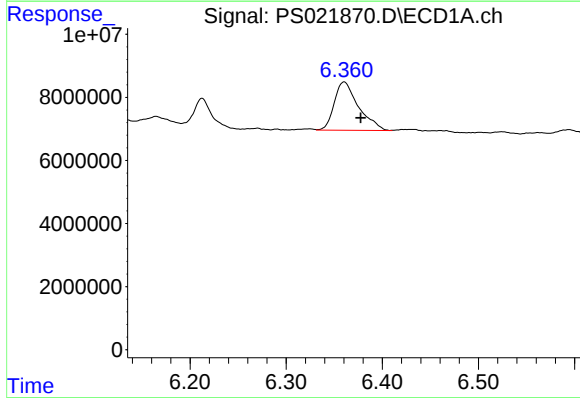


#4 2,4-DCAA

R.T.: 6.360 min
Delta R.T.: -0.017 min
Response: 26924266
Conc: 9.67 ng/ml

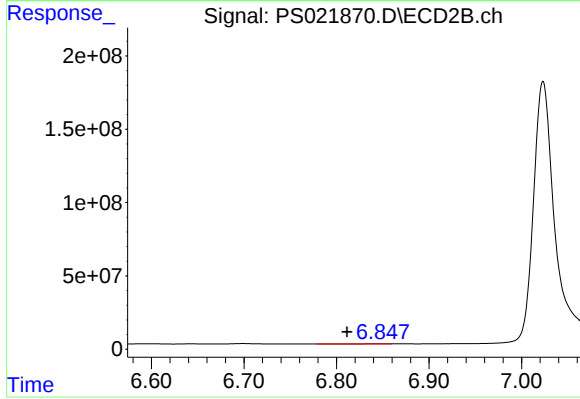


#4 2,4-DCAA

R.T.: 6.848 min
Delta R.T.: 0.036 min
Response: 4180540
Conc: 2.33 ng/ml

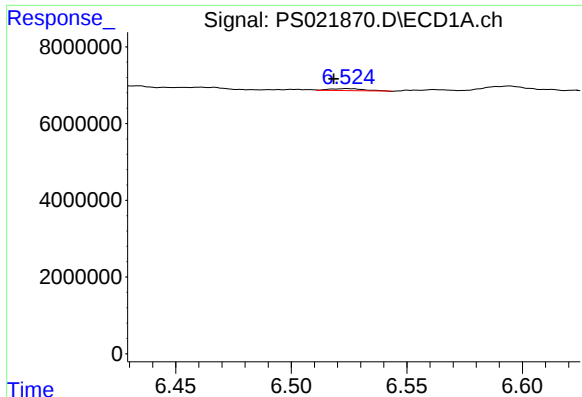


#5 DICAMBA

R.T.: 6.524 min
Delta R.T.: 0.006 min
Response: 544497
Conc: N.D.

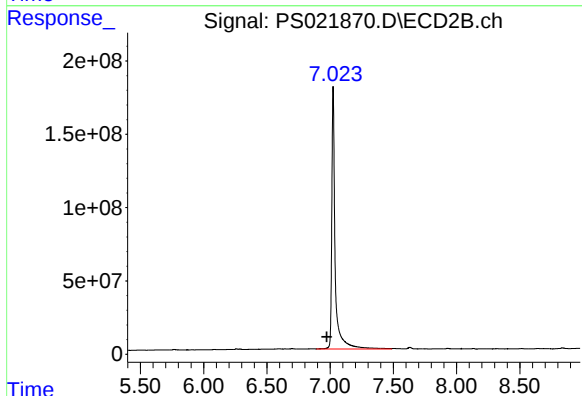


#5 DICAMBA

R.T.: 7.023 min
Delta R.T.: 0.049 min
Response: 3405382817
Conc: 400.50 ng/ml

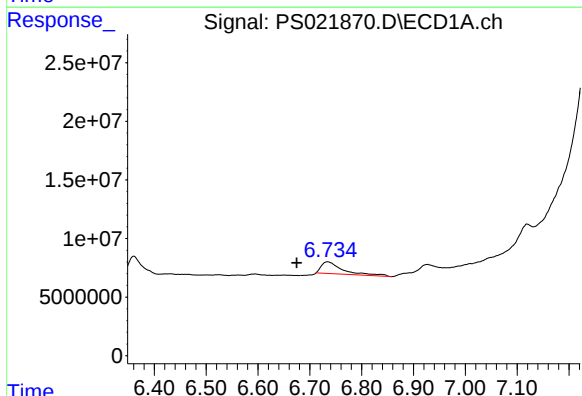


#6 MCP

R.T.: 6.734 min
Delta R.T.: 0.059 min
Response: 29322306
Conc: 3.06 ug/ml

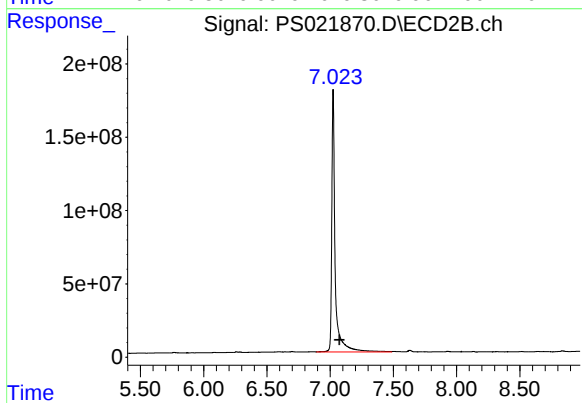


#6 MCP

R.T.: 7.023 min
Delta R.T.: -0.051 min
Response: 3405382817
Conc: 513.51 ug/ml

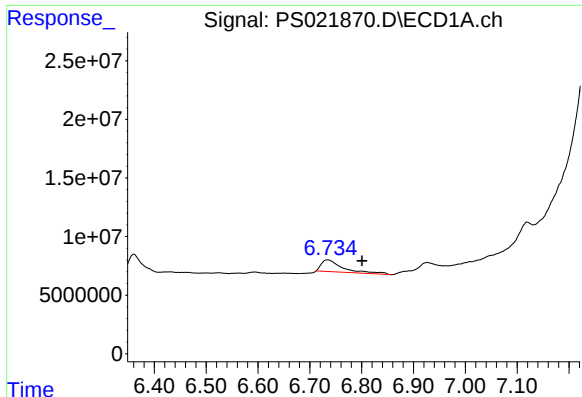


#7 MCPA

R.T.: 6.734 min
Delta R.T.: -0.067 min
Response: 29322306
Conc: 2.27 ug/ml

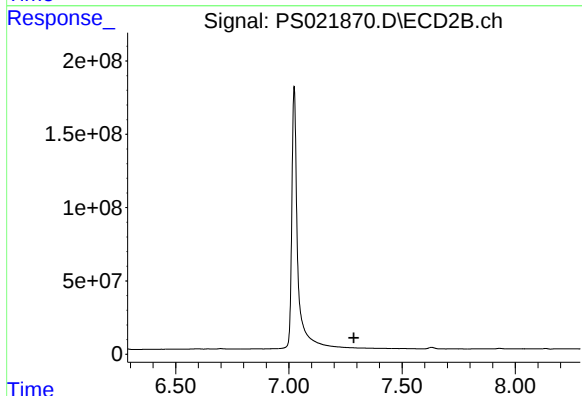


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 7.287 min
Response: 0
Conc: N.D.

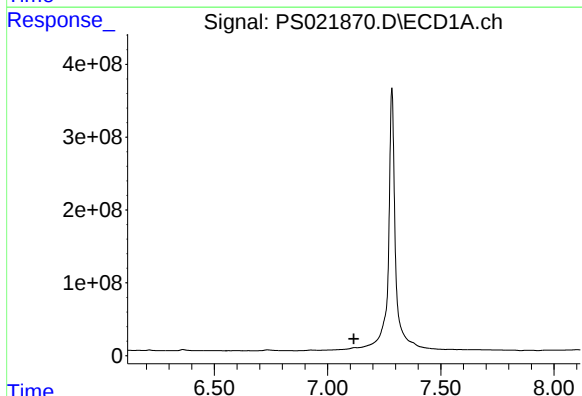


#8 DICHLORPROP

R.T.: 7.120 min
Delta R.T.: 0.003 min
Response: -42822869
Conc: N.D.

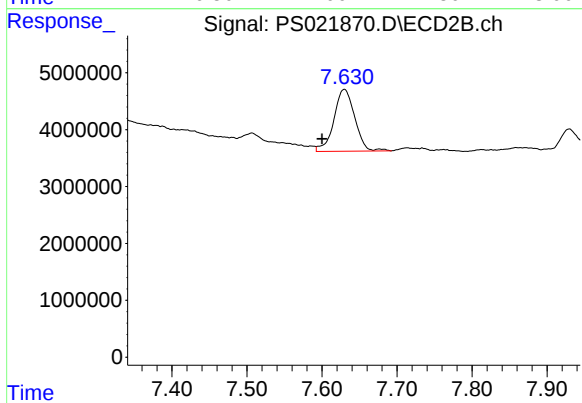


#8 DICHLORPROP

R.T.: 7.630 min
Delta R.T.: 0.029 min
Response: 21001561
Conc: 9.84 ng/ml

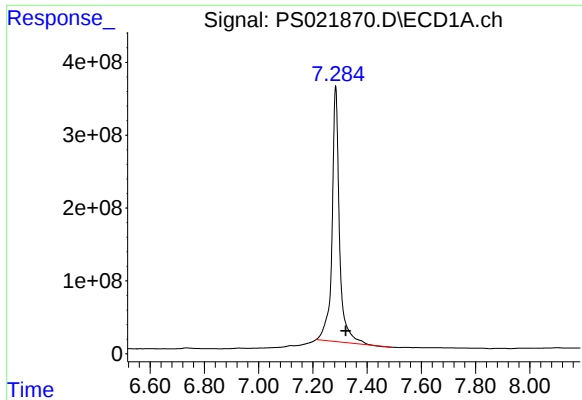


#9 2,4-D

R.T.: 7.284 min
Delta R.T.: -0.037 min
Response: 6670208241
Conc: 1717.44 ng/ml

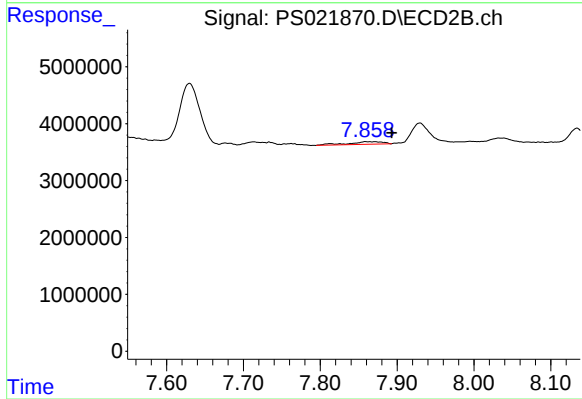


#9 2,4-D

R.T.: 7.869 min
Delta R.T.: -0.024 min
Response: 1458622
Conc: N.D.

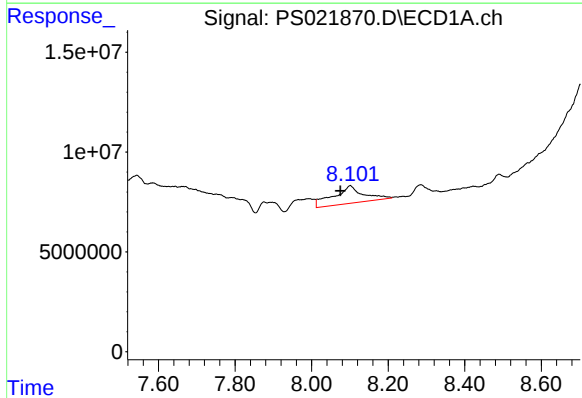


#11 2,4,5-TP (SILVEX)

R.T.: 8.101 min
Delta R.T.: 0.026 min
Response: 47942029
Conc: 2.60 ng/ml

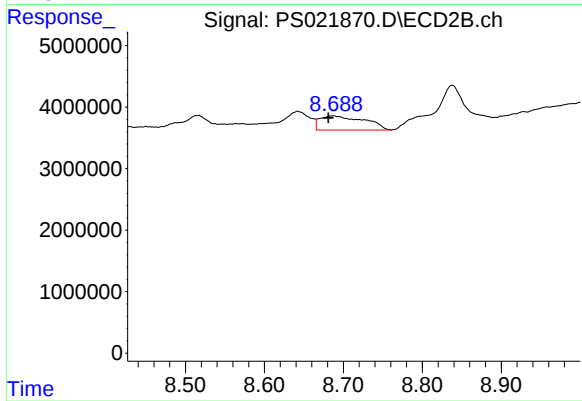


#11 2,4,5-TP (SILVEX)

R.T.: 8.687 min
Delta R.T.: 0.006 min
Response: 9064169
Conc: N.D.

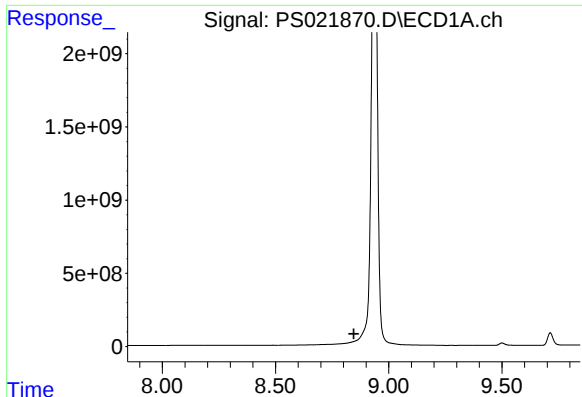


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 8.846 min
Response: 0
Conc: N.D.

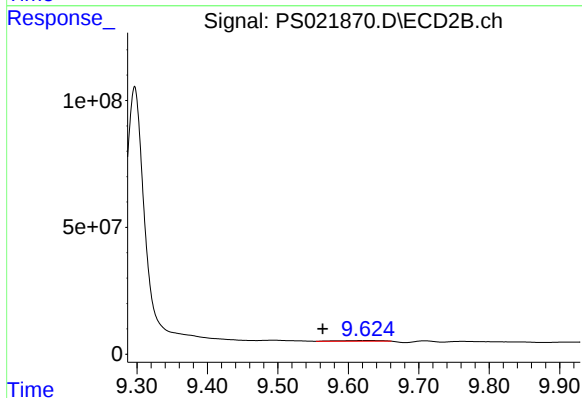


#13 2,4-DB

R.T.: 9.624 min
Delta R.T.: 0.060 min
Response: 11844508
Conc: 7.91 ng/ml

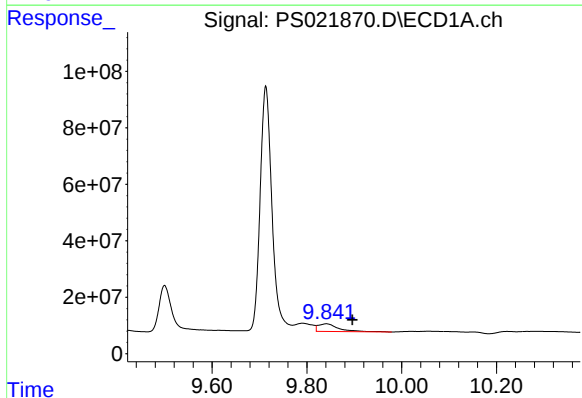


#14 DINOSEB

R.T.: 9.841 min
Delta R.T.: -0.055 min
Response: 80197845
Conc: 4.89 ng/ml

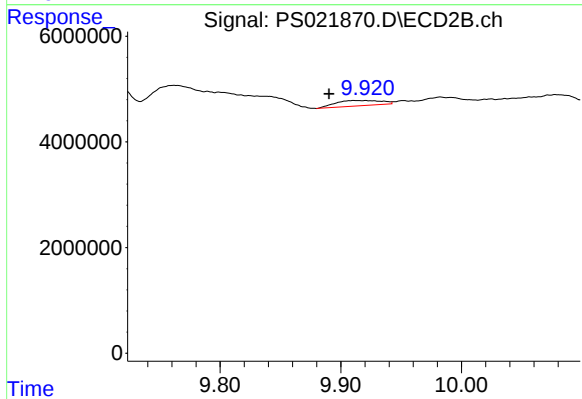


#14 DINOSEB

R.T.: 9.912 min
Delta R.T.: 0.022 min
Response: 2622751
Conc: N.D.

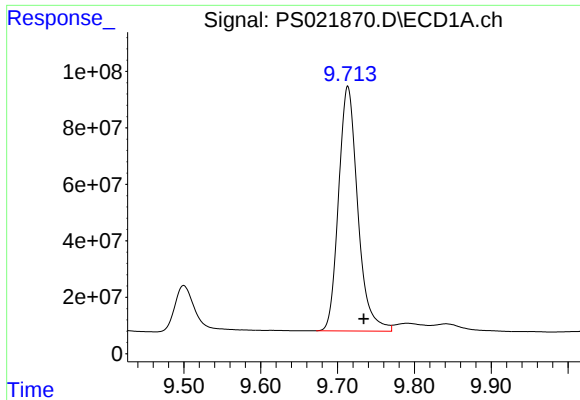


#15 Picloram

R.T.: 9.713 min
Delta R.T.: -0.021 min
Response: 1497955613
Conc: 52.81 ng/ml

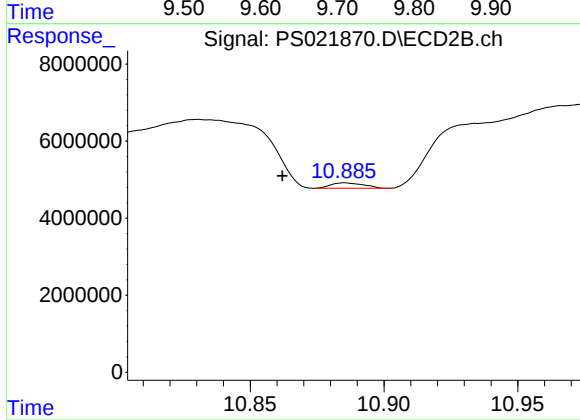


#15 Picloram

R.T.: 10.886 min
Delta R.T.: 0.024 min
Response: 1175783
Conc: N.D.

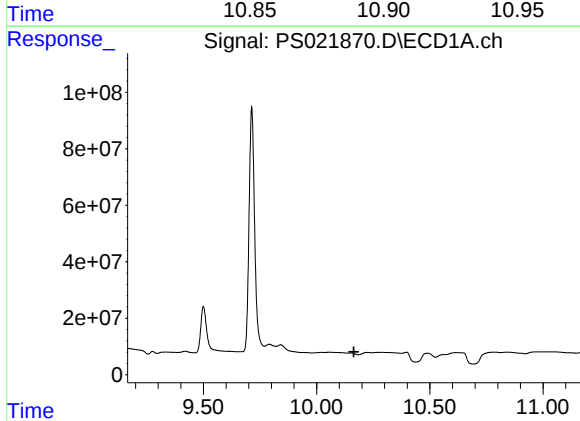

#16 DCPA

R.T.: 10.224 min
Delta R.T.: 0.059 min
Response: -9299973
Conc: N.D.

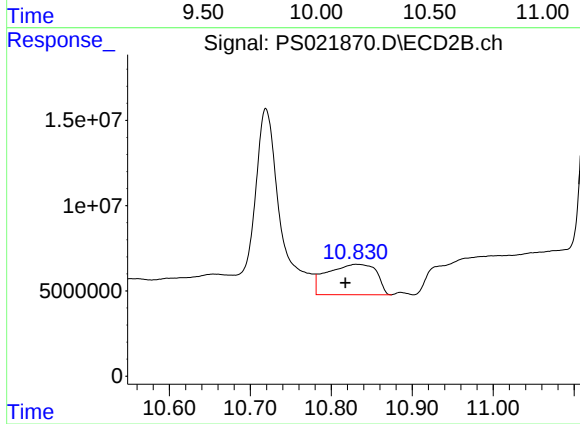

#16 DCPA

R.T.: 10.831 min
Delta R.T.: 0.014 min
Response: 75282400
Conc: 5.40 ng/ml