

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012622\
 Data File : PS018117.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jan 2022 08:35
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 26 13:00:27 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 06 10:21:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
11) T	2,4,5-TP ...	0.000	8.436f	0	6087956	N.D. 1.708
12) T	2,4,5-T	9.282	8.919f	4156319	11574195	<MDL 3.538 #
13) T	2,4-DB	9.827	0.000	11546144	0	6.985 N.D. #
14) T	DINOSEB	10.973	0.000	2068432	0	<MDL N.D. #
15) T	Picloram	10.808	10.668	137.4E6	34611014	11.512 7.402 #
16) T	DCPA	11.240	10.668f	7716512	34611014	<MDL 7.839 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012622\
Data File : PS018117.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jan 2022 08:35
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 26 13:00:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
Quant Title : 8080.M
QLast Update : Thu Jan 06 10:21:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

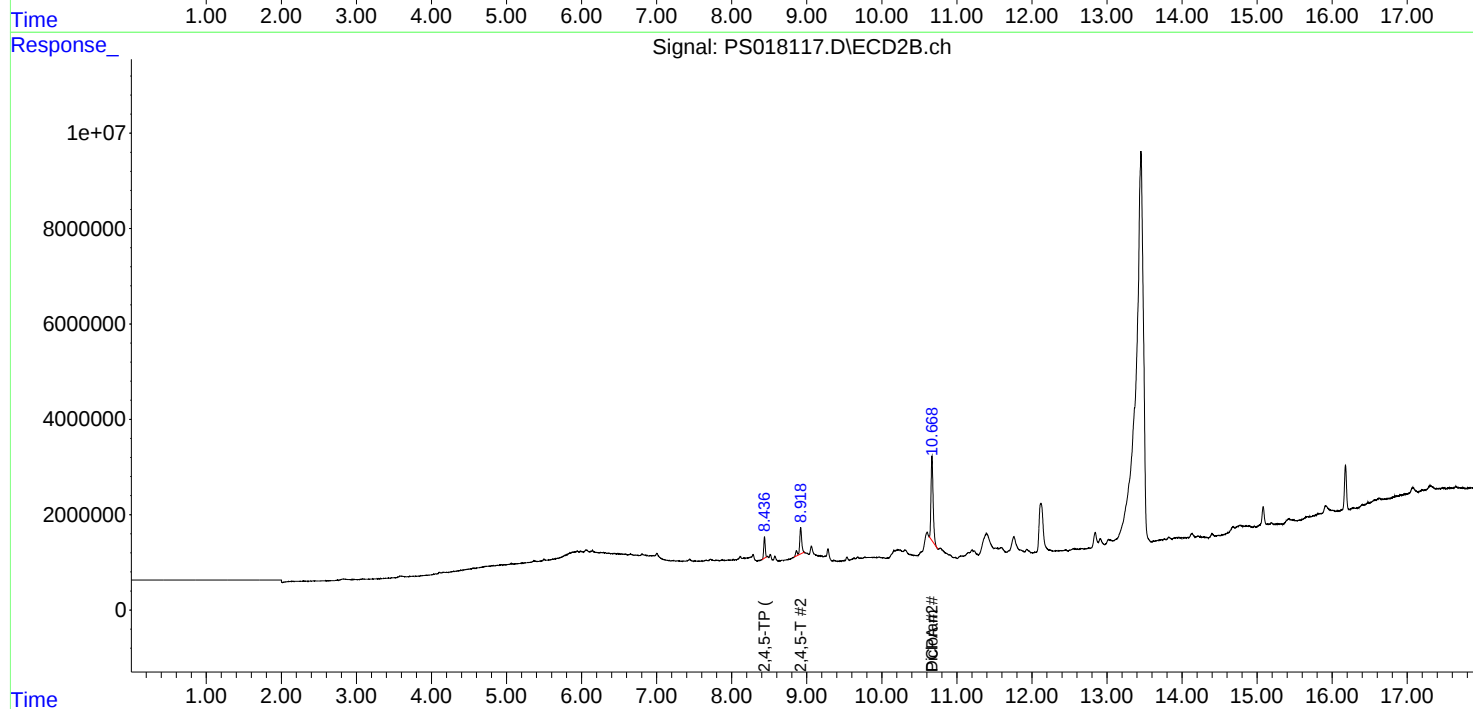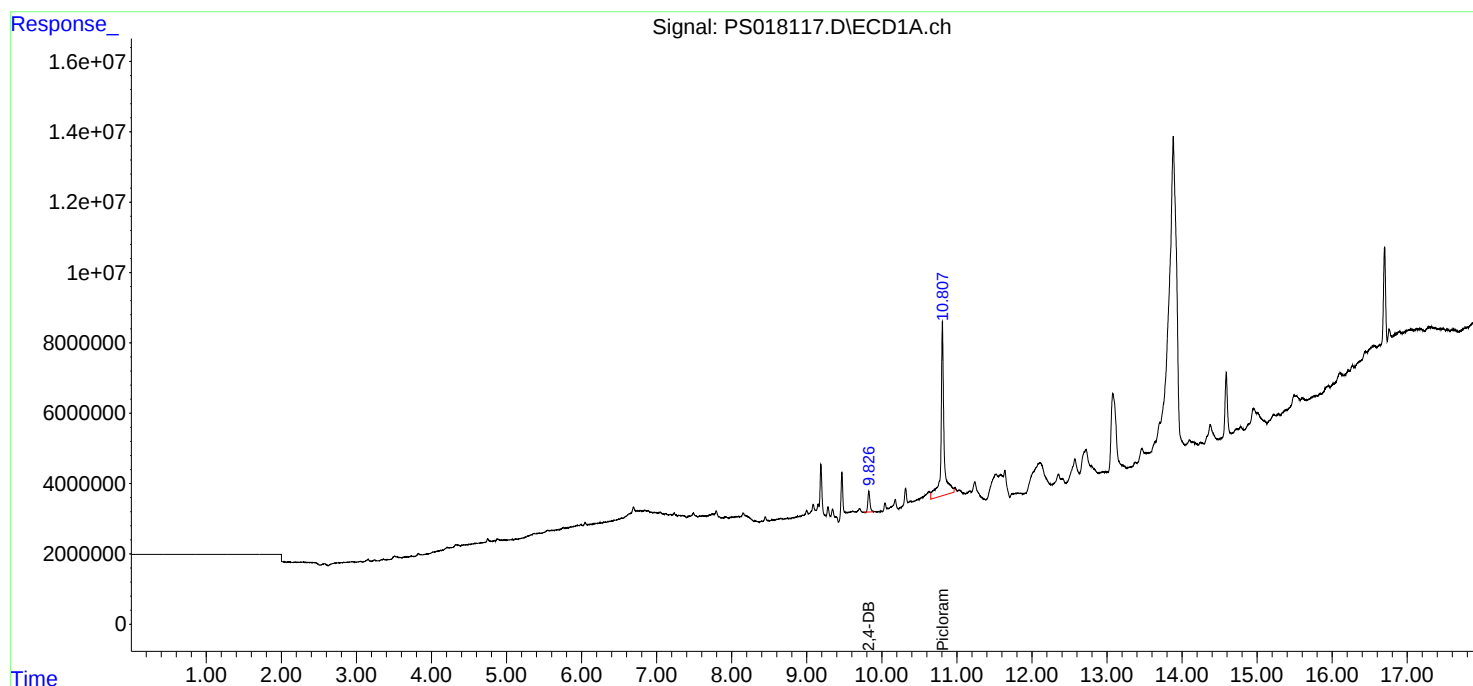


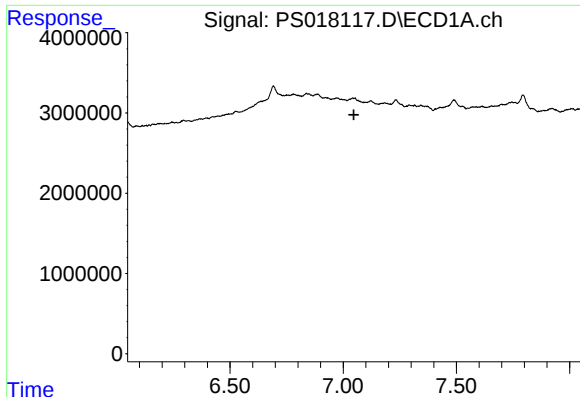

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 7.047 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

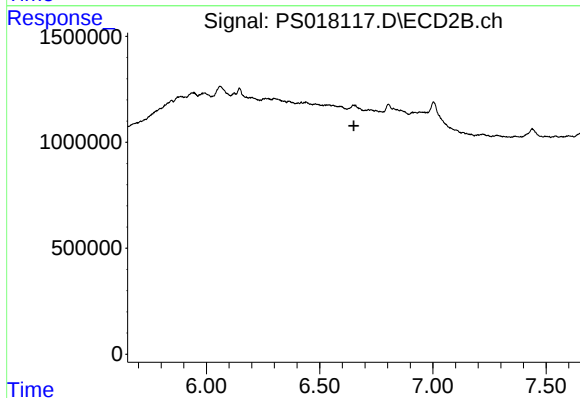


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.651 min
Response: 0
Conc: N.D.

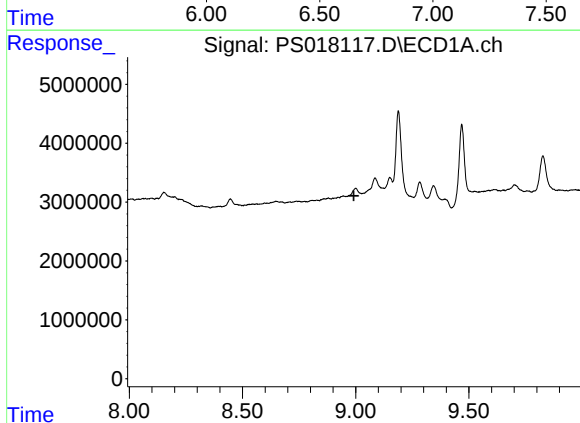


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 8.992 min
Response: 0
Conc: N.D.

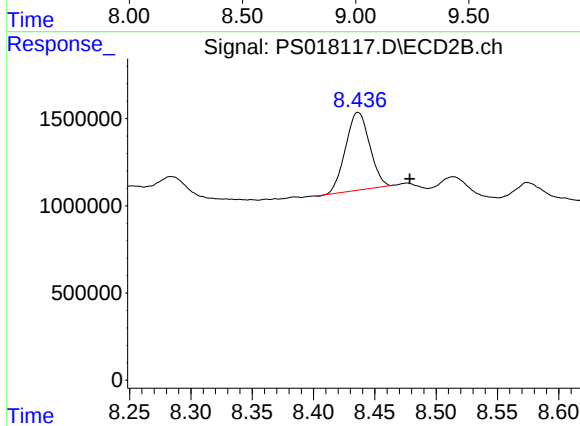

#11 2,4,5-TP (SILVEX)


R.T.: 8.436 min
Delta R.T.: -0.042 min
Response: 6087956
Conc: 1.71 ng/ml

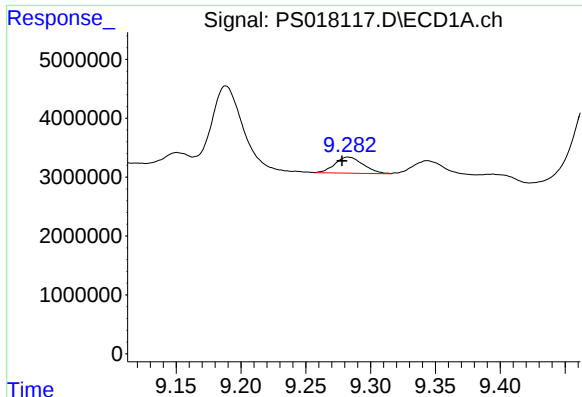

#12 2,4,5-T


R.T.: 9.282 min
Delta R.T.: 0.004 min
Response: 4156319
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

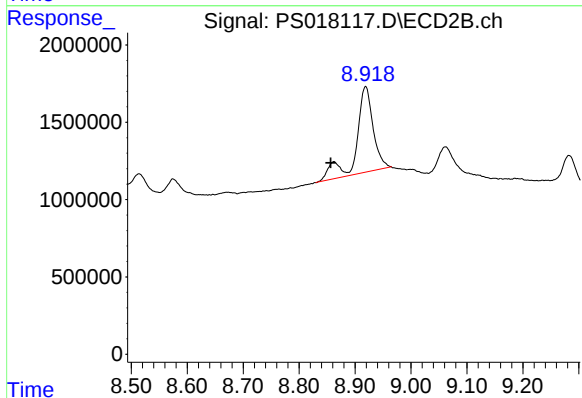


#12 2,4,5-T

R.T.: 8.919 min
Delta R.T.: 0.062 min
Response: 11574195
Conc: 3.54 ng/ml

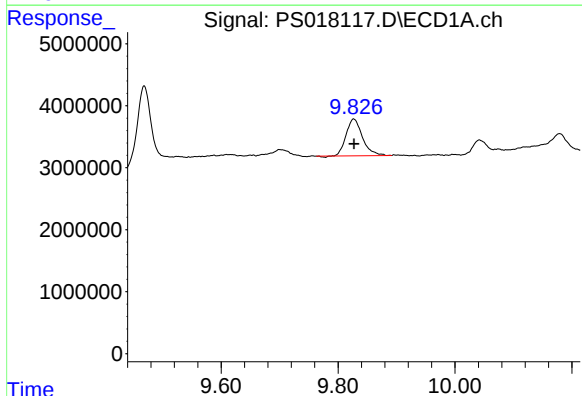


#13 2,4-DB

R.T.: 9.827 min
Delta R.T.: 0.000 min
Response: 11546144
Conc: 6.98 ng/ml

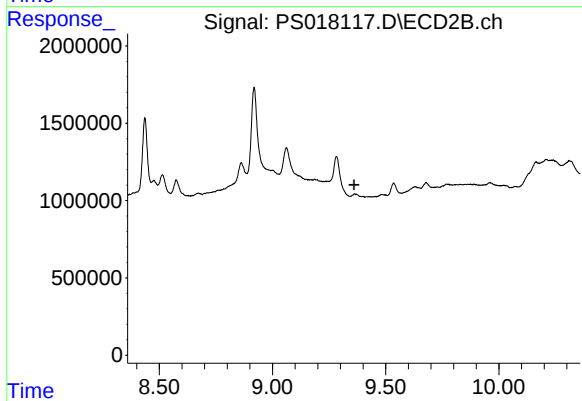

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.360 min
Response: 0
Conc: N.D.

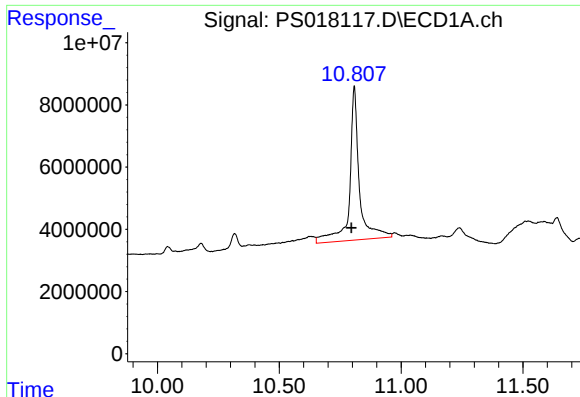

#15 Picloram


R.T.: 10.808 min
Delta R.T.: 0.012 min
Response: 137405423
Conc: 11.51 ng/ml

Instrument :
ECD_S
ClientSampleId :

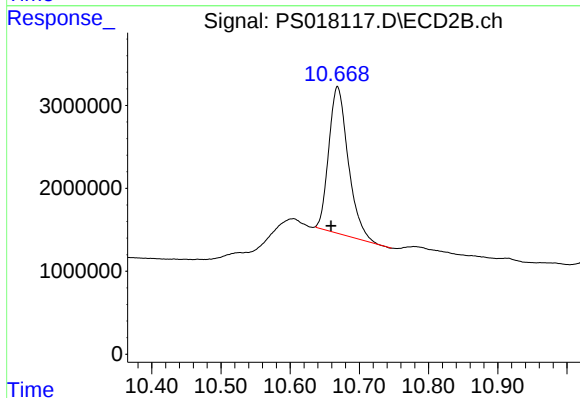


#15 Picloram

R.T.: 10.668 min
Delta R.T.: 0.009 min
Response: 34611014
Conc: 7.40 ng/ml

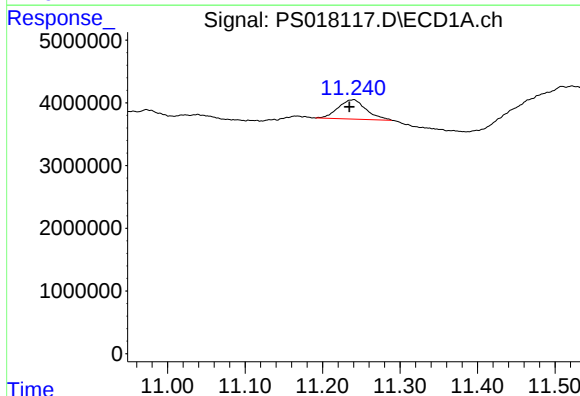

#16 DCPA

R.T.: 11.240 min
Delta R.T.: 0.006 min
Response: 7716512
Conc: N.D.

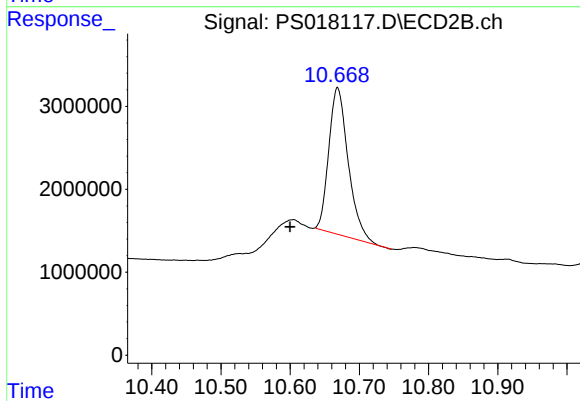

#16 DCPA

R.T.: 10.668 min
Delta R.T.: 0.069 min
Response: 34611014
Conc: 7.84 ng/ml