

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012622\
 Data File : PS018118.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jan 2022 09:02
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 26 13:00:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 06 10:21:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.047	6.648	620.1E6	291.3E6	428.966	501.946
Target Compounds							
9) T	2,4-D	8.208f	0.000	12322960	0	6.767	N.D. #
11) T	2,4,5-TP ...	0.000	8.445	0	13418550	N.D.	3.764
12) T	2,4,5-T	9.303	0.000	7541350	0	<MDL	N.D. #
13) T	2,4-DB	9.844	0.000	3278274	0	1.983	N.D. #
15) T	Picloram	10.777	10.701f	4276768	11950346	<MDL	2.556 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012622\
Data File : PS018118.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jan 2022 09:02
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 26 13:00:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
Quant Title : 8080.M
QLast Update : Thu Jan 06 10:21:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

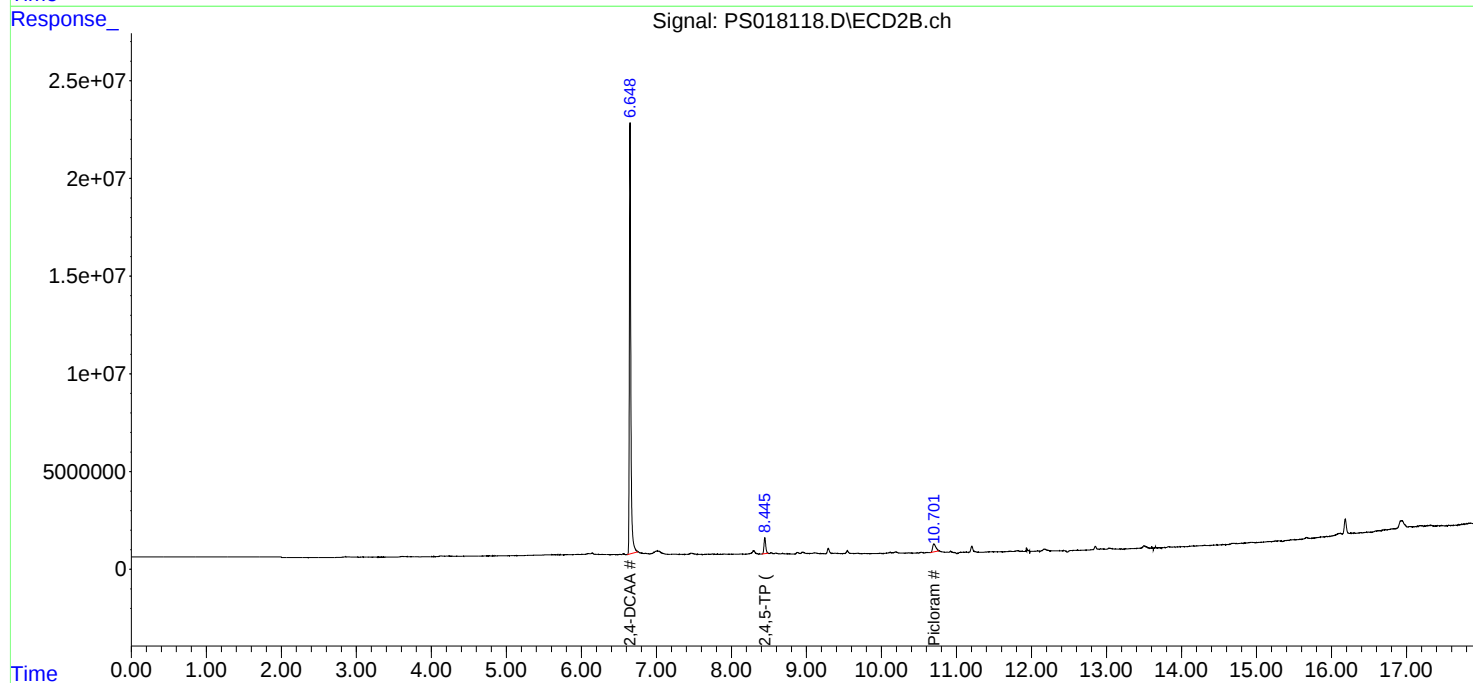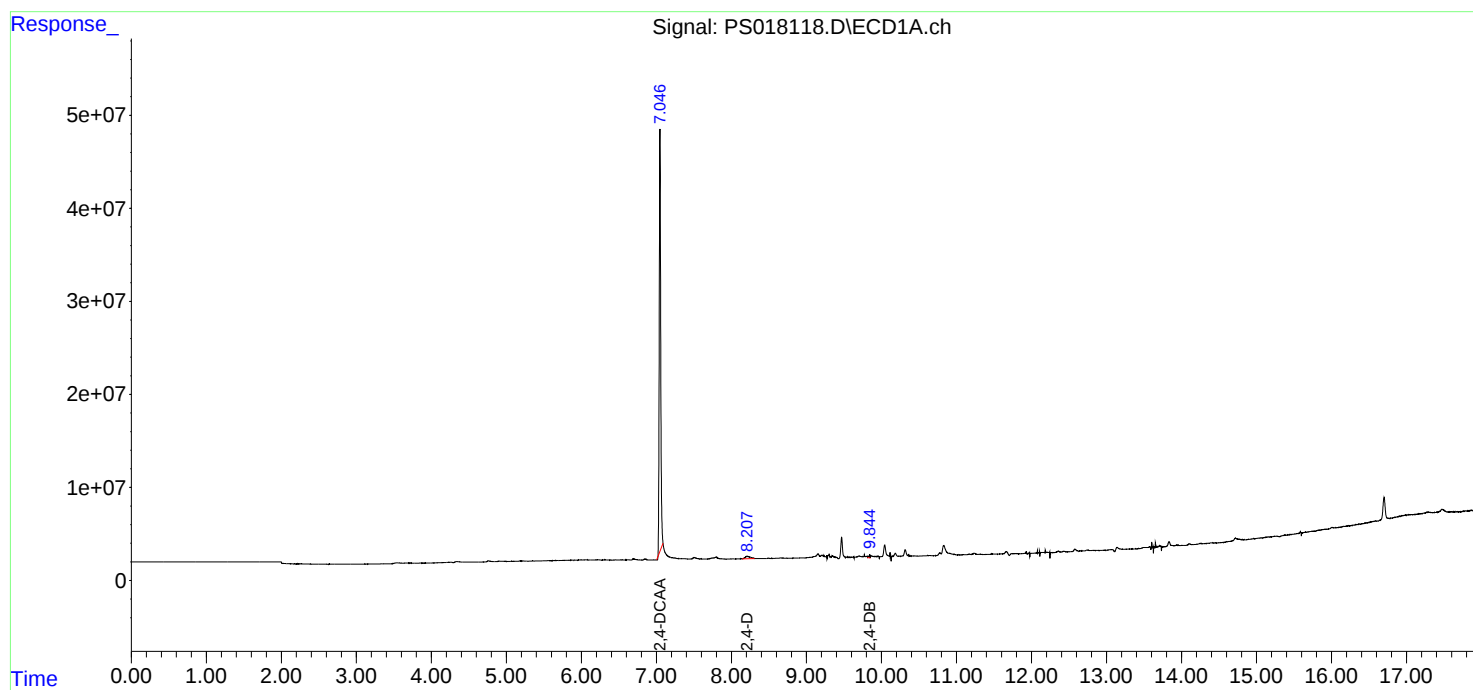


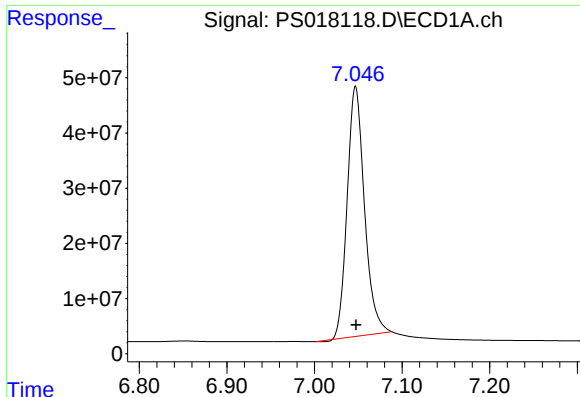

#4 2,4-DCAA


R.T.: 7.047 min
Delta R.T.: 0.000 min
Response: 620064399
Conc: 428.97 ng/ml

Instrument :
ECD_S
ClientSampleId :

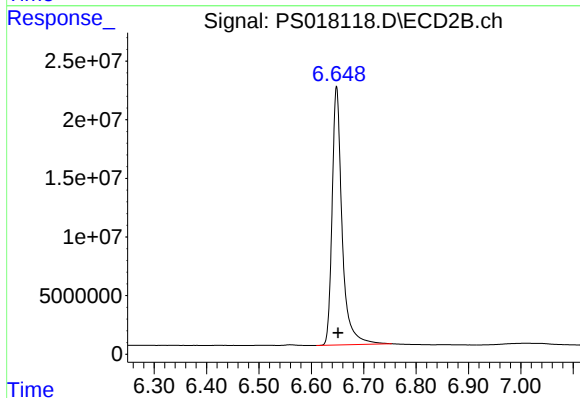


#4 2,4-DCAA

R.T.: 6.648 min
Delta R.T.: -0.003 min
Response: 291253666
Conc: 501.95 ng/ml

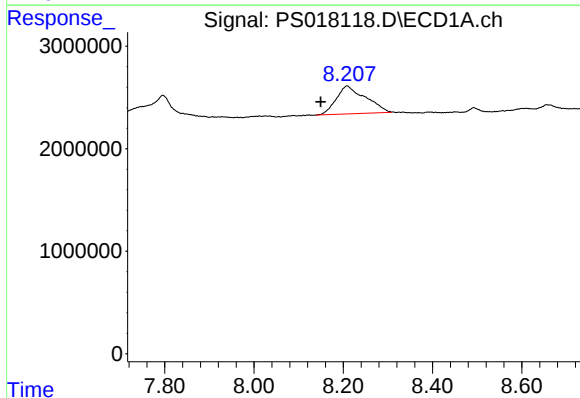


#9 2,4-D

R.T.: 8.208 min
Delta R.T.: 0.059 min
Response: 12322960
Conc: 6.77 ng/ml

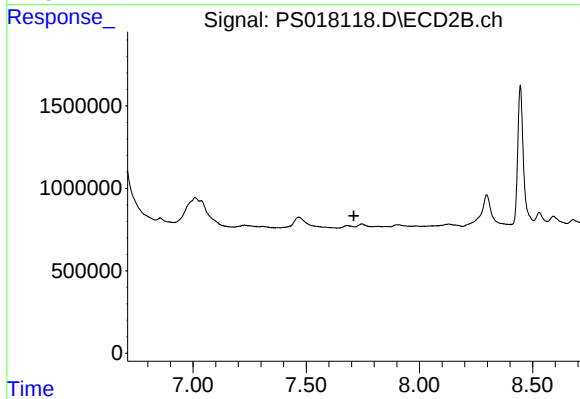

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.710 min
Response: 0
Conc: N.D.

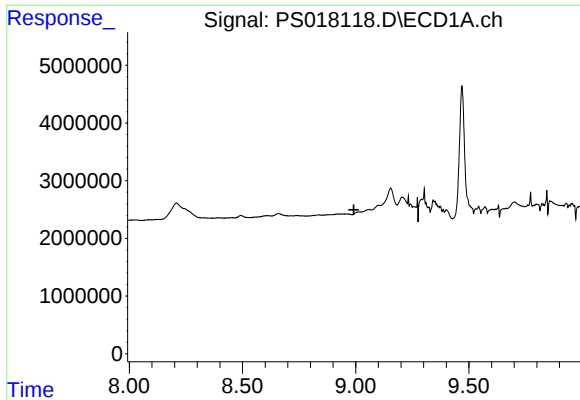

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 8.992 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

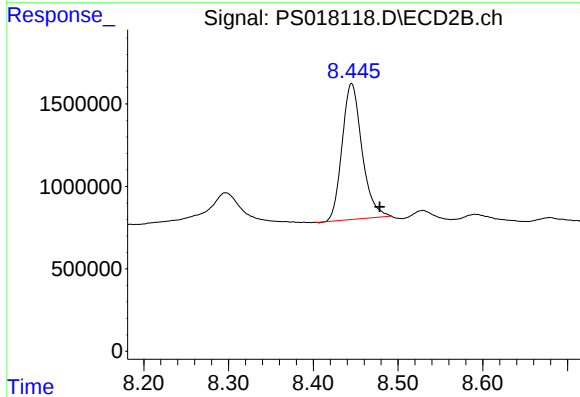


#11 2,4,5-TP (SILVEX)

R.T.: 8.445 min
Delta R.T.: -0.033 min
Response: 13418550
Conc: 3.76 ng/ml

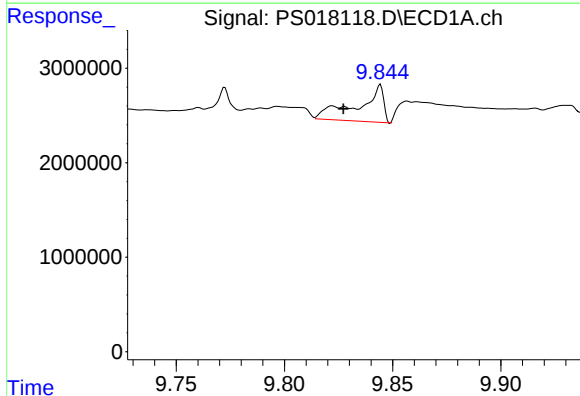


#13 2,4-DB

R.T.: 9.844 min
Delta R.T.: 0.017 min
Response: 3278274
Conc: 1.98 ng/ml

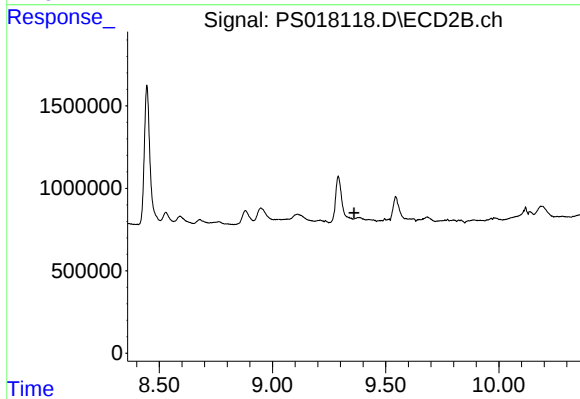

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 9.360 min
Response: 0
Conc: N.D.

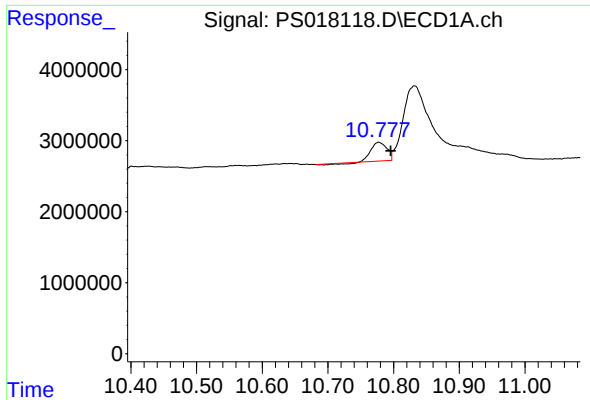

#15 Picloram

R.T.: 10.777 min
Delta R.T.: -0.019 min
Response: 4276768
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

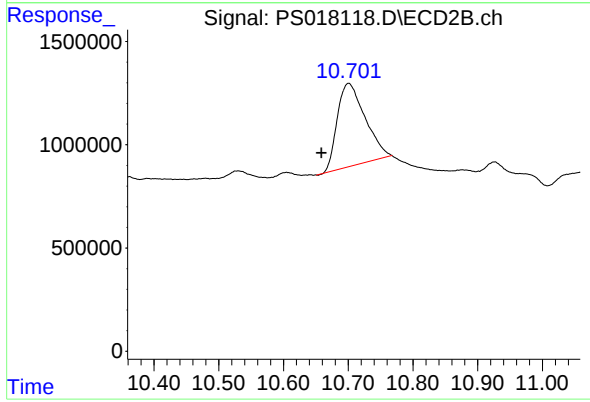

#15 Picloram

R.T.: 10.701 min
Delta R.T.: 0.042 min
Response: 11950346
Conc: 2.56 ng/ml