

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012622\
 Data File : PS018138.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jan 2022 18:37
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 26 23:57:17 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 06 10:21:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.043	6.646	673.4E6	294.9E6	465.836	508.316
Target Compounds							
7) T	MCPA	7.484f	0.000	14213072	0	2.130	N.D. #
9) T	2,4-D	8.195f	0.000	399372	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.052f	8.508	50147061	6981359	5.926	1.958 #
12) T	2,4,5-T	9.275	0.000	11849432	0	1.337	N.D. #
13) T	2,4-DB	9.794	0.000	8597844	0	5.201	N.D. #
14) T	DINOSEB	10.966	9.679	1020037	14935181	<MDL	5.986 #
15) T	Picloram	10.762	10.677	243.9E6	53655798	20.430	11.474 #
16) T	DCPA	11.224	0.000	14106240	0	1.306	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012622\
Data File : PS018138.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jan 2022 18:37
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 26 23:57:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
Quant Title : 8080.M
QLast Update : Thu Jan 06 10:21:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

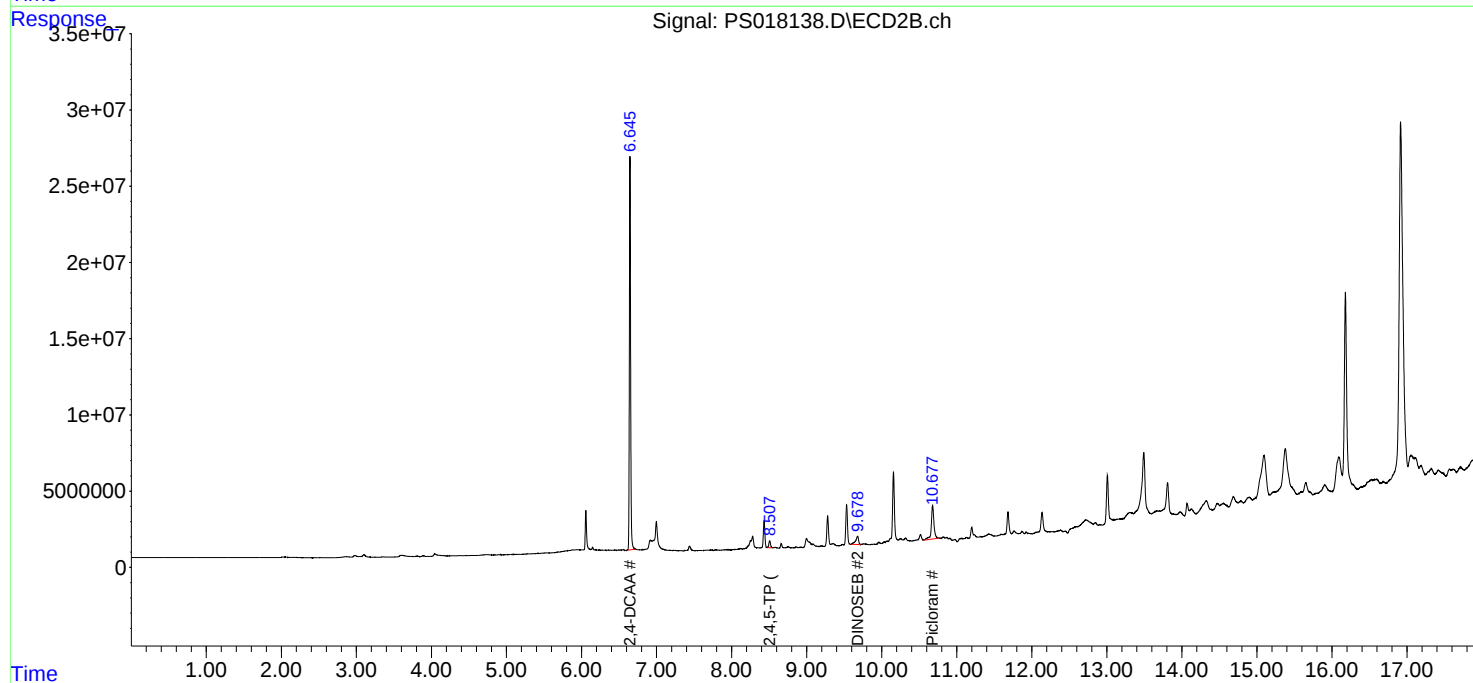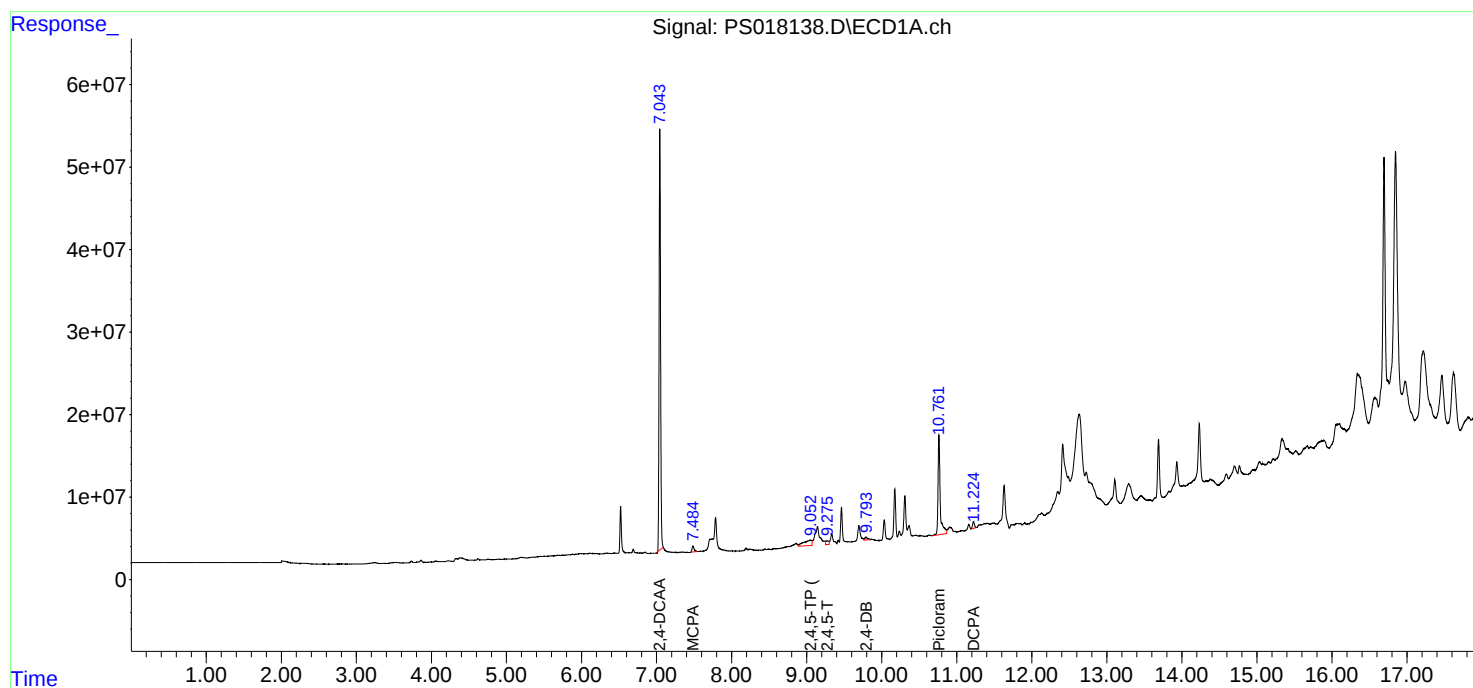


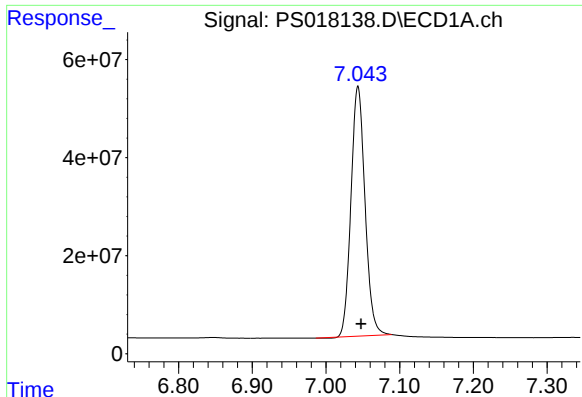

#4 2,4-DCAA


R.T.: 7.043 min
Delta R.T.: -0.004 min
Response: 673360072
Conc: 465.84 ng/ml

Instrument :
ECD_S
ClientSampleId :

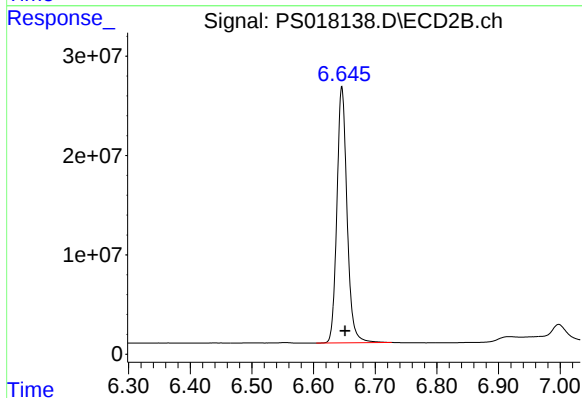


#4 2,4-DCAA

R.T.: 6.646 min
Delta R.T.: -0.005 min
Response: 294949523
Conc: 508.32 ng/ml

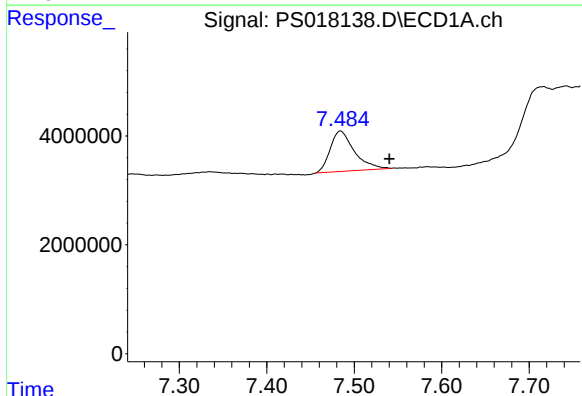


#7 MCPA

R.T.: 7.484 min
Delta R.T.: -0.056 min
Response: 14213072
Conc: 2.13 ug/ml

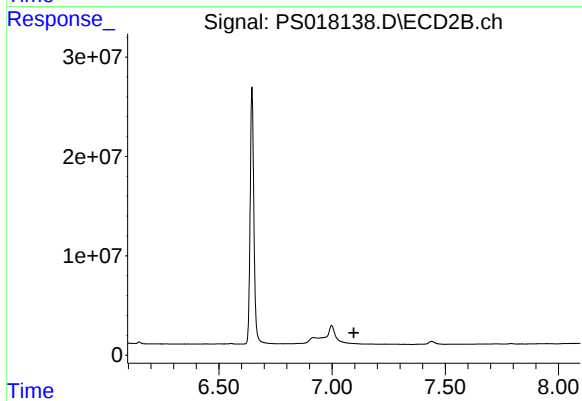

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 7.096 min
Response: 0
Conc: N.D.

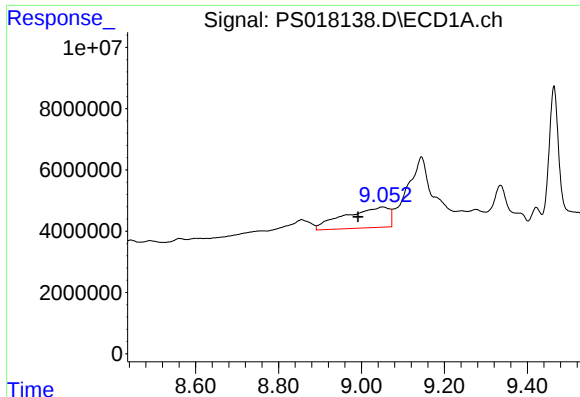

#11 2,4,5-TP (SILVEX)


R.T.: 9.052 min
Delta R.T.: 0.060 min
Response: 50147061
Conc: 5.93 ng/ml

Instrument :
ECD_S
ClientSampleId :

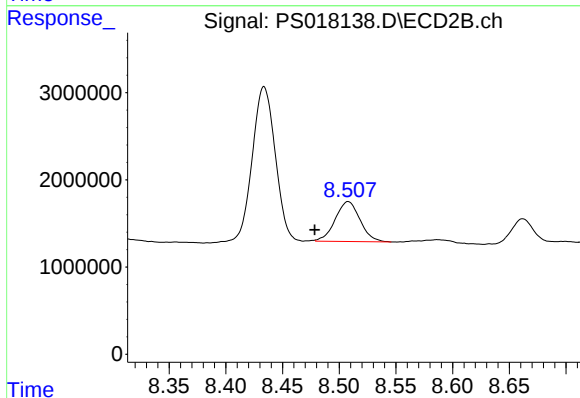


#11 2,4,5-TP (SILVEX)

R.T.: 8.508 min
Delta R.T.: 0.029 min
Response: 6981359
Conc: 1.96 ng/ml

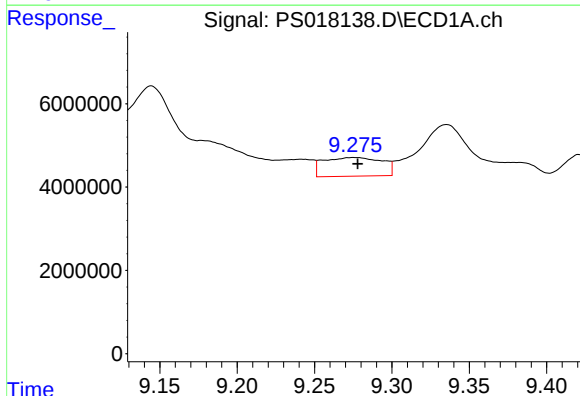


#12 2,4,5-T

R.T.: 9.275 min
Delta R.T.: -0.003 min
Response: 11849432
Conc: 1.34 ng/ml

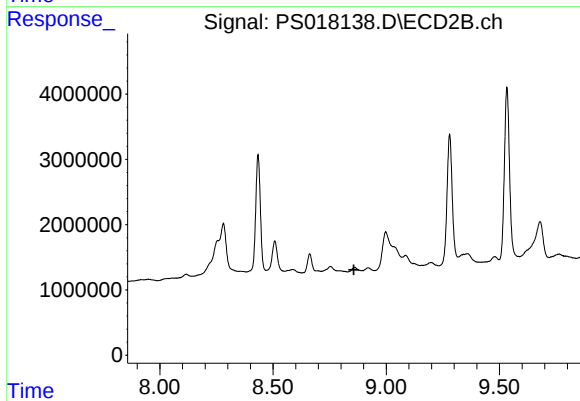

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 8.857 min
Response: 0
Conc: N.D.

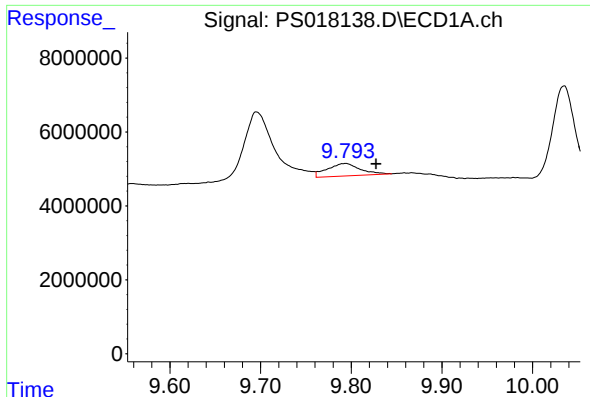

#13 2,4-DB


R.T.: 9.794 min
Delta R.T.: -0.033 min
Response: 8597844
Conc: 5.20 ng/ml

Instrument :
ECD_S
ClientSampleId :

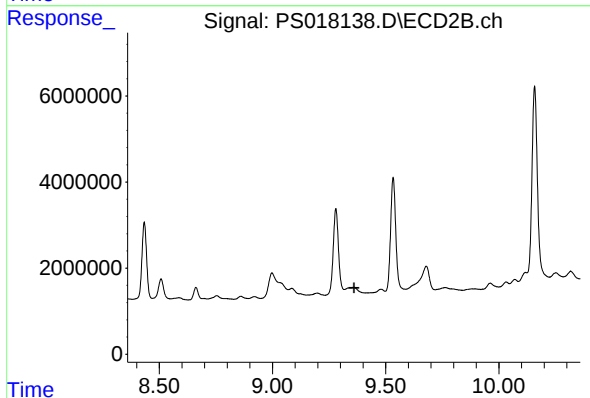


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.360 min
Response: 0
Conc: N.D.

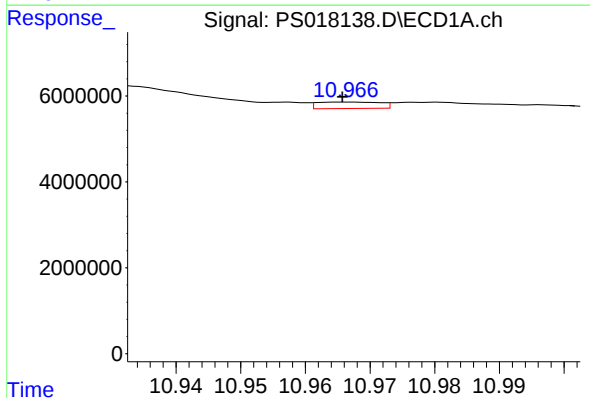


#14 DINOSEB

R.T.: 10.966 min
Delta R.T.: 0.000 min
Response: 1020037
Conc: N.D.

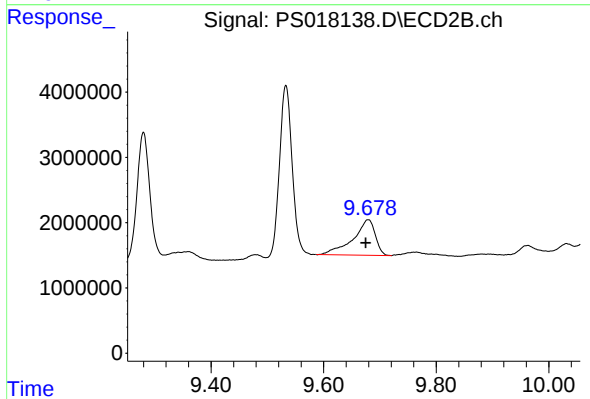

#14 DINOSEB


R.T.: 9.679 min
Delta R.T.: 0.004 min
Response: 14935181
Conc: 5.99 ng/ml

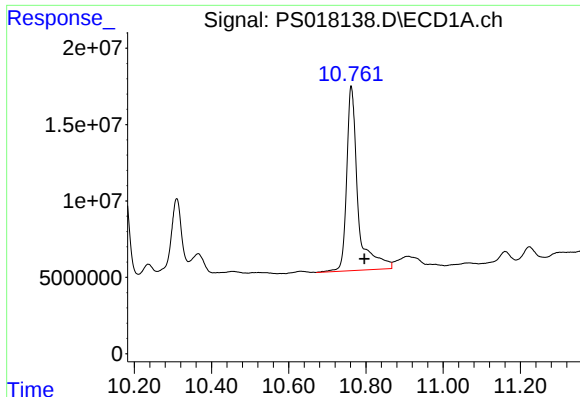

#15 Picloram


R.T.: 10.762 min
Delta R.T.: -0.034 min
Response: 243854371
Conc: 20.43 ng/ml

Instrument :
ECD_S
ClientSampleId :

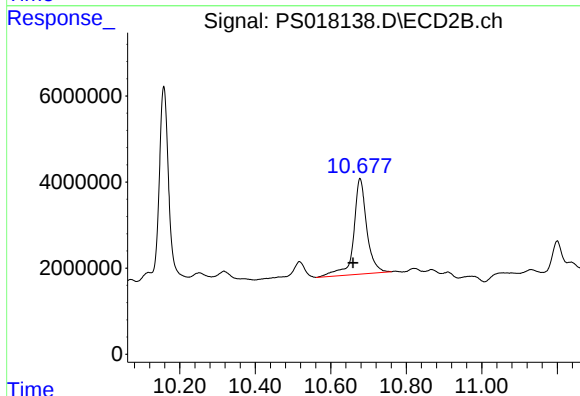


#15 Picloram

R.T.: 10.677 min
Delta R.T.: 0.018 min
Response: 53655798
Conc: 11.47 ng/ml

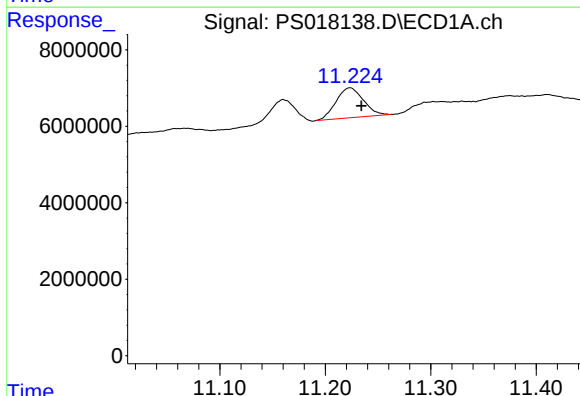

#16 DCPA

R.T.: 11.224 min
Delta R.T.: -0.011 min
Response: 14106240
Conc: 1.31 ng/ml

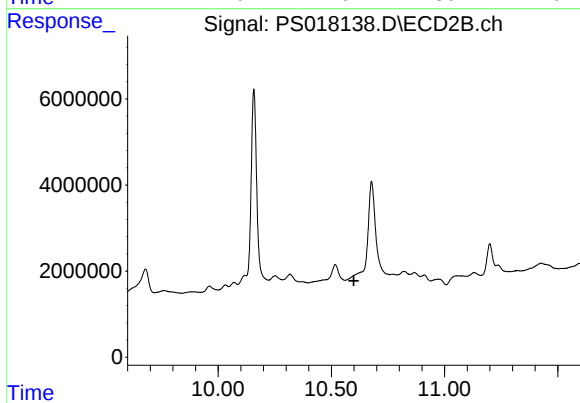

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.600 min
Response: 0
Conc: N.D.