

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012720\
 Data File : PS008554.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jan 2020 13:26
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 28 04:46:15 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 08 11:00:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.273	5.967	914.6E6	488.9E6	517.974	515.988
Target Compounds							
9) T	2,4-D	7.459	0.000	41853447	0	23.008	N.D. #
12) T	2,4,5-T	0.000	8.281	0	15593591	N.D.	2.949
15) T	Picloram	10.062	10.052	80930937	55405608	6.484	7.458
16) T	DCPA	0.000	10.052	0	55405608	N.D.	8.502



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012720\
Data File : PS008554.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jan 2020 13:26
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 28 04:46:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
Quant Title : 8080.M
QLast Update : Wed Jan 08 11:00:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

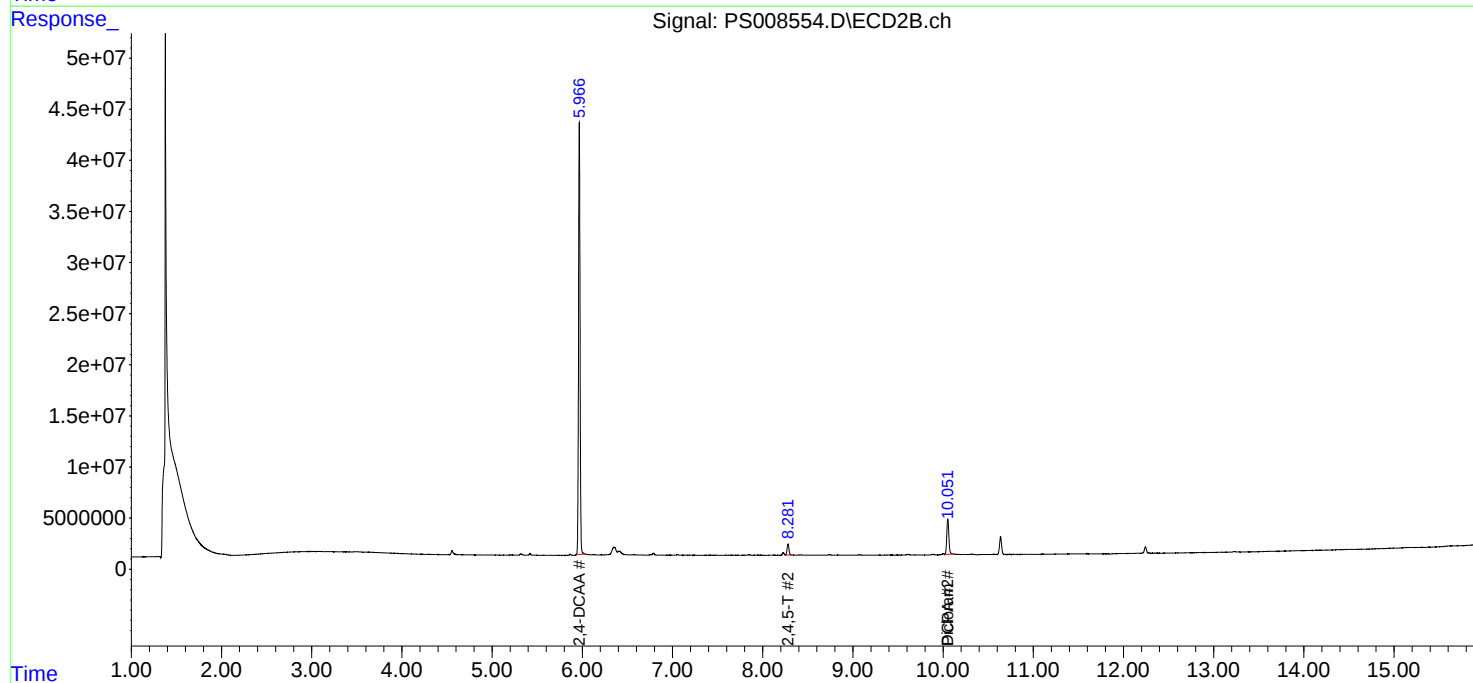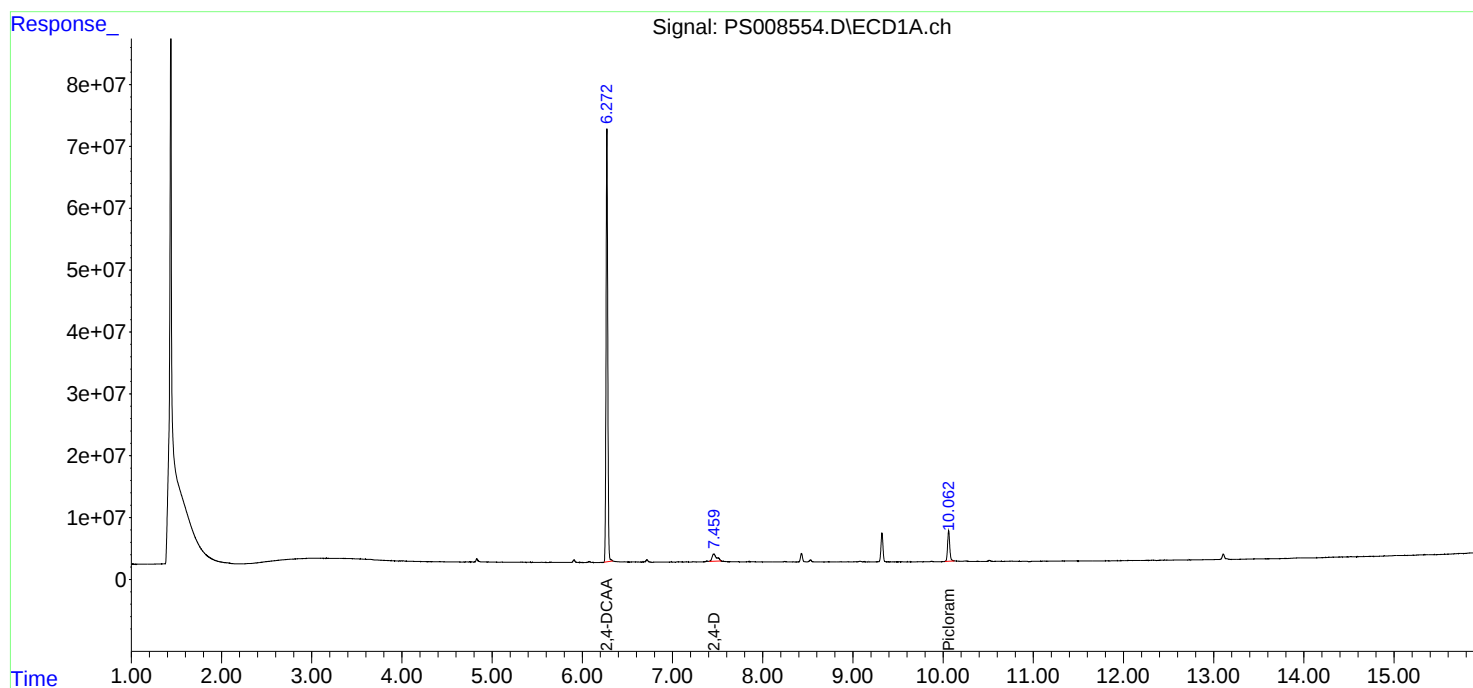


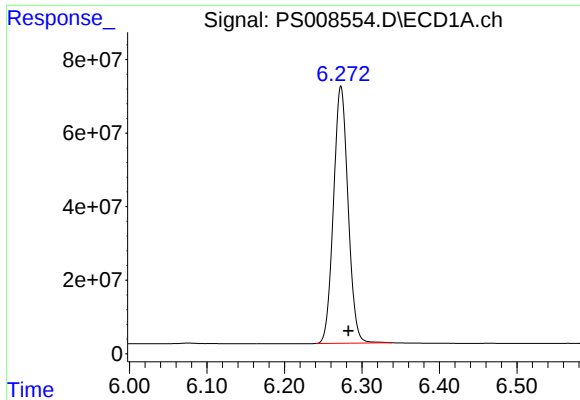

#4 2,4-DCAA


R.T.: 6.273 min
Delta R.T.: -0.010 min
Response: 914588107
Conc: 517.97 ng/ml

Instrument :
ECD_S
ClientSampleId :

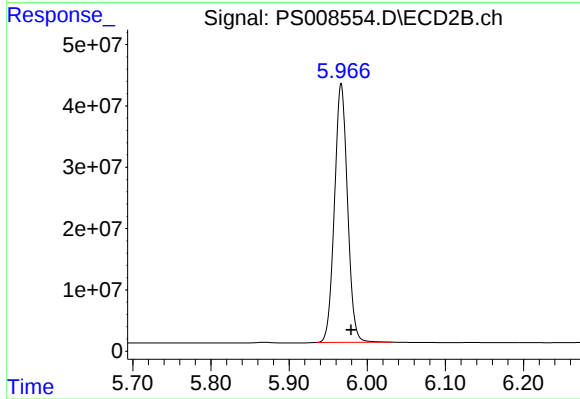


#4 2,4-DCAA

R.T.: 5.967 min
Delta R.T.: -0.013 min
Response: 488879191
Conc: 515.99 ng/ml

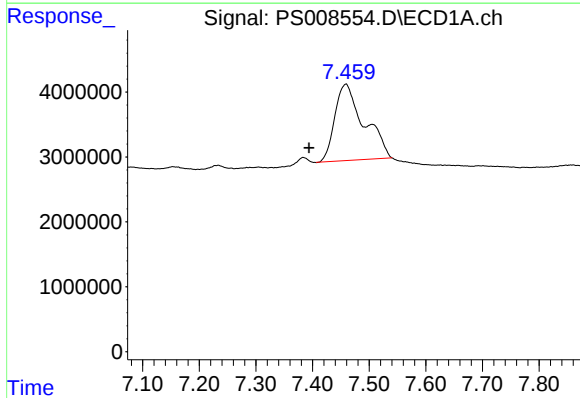


#9 2,4-D

R.T.: 7.459 min
Delta R.T.: 0.065 min
Response: 41853447
Conc: 23.01 ng/ml

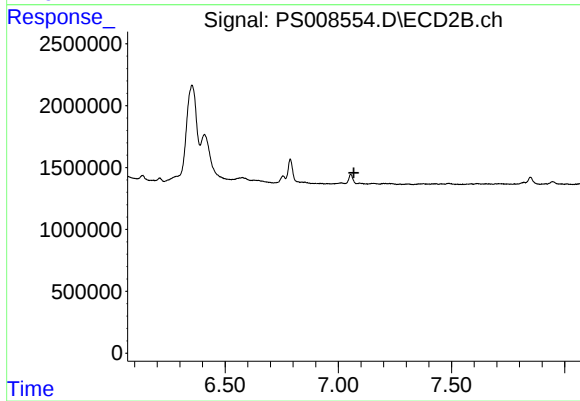

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.069 min
Response: 0
Conc: N.D.

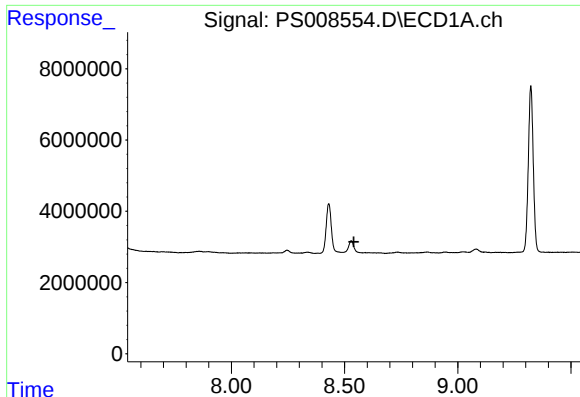

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 8.541 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

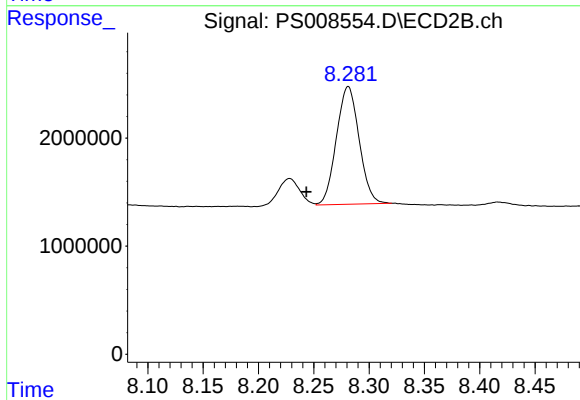


#12 2,4,5-T

R.T.: 8.281 min
Delta R.T.: 0.038 min
Response: 15593591
Conc: 2.95 ng/ml

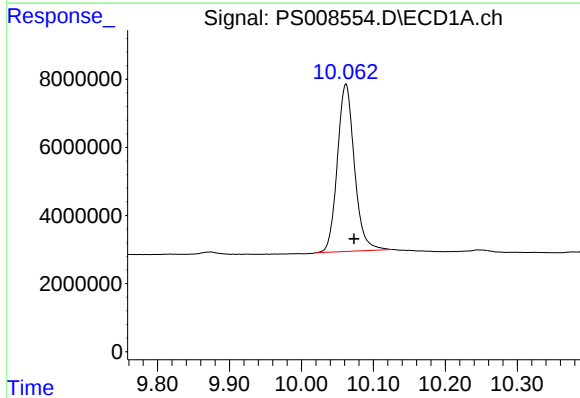


#15 Picloram

R.T.: 10.062 min
Delta R.T.: -0.011 min
Response: 80930937
Conc: 6.48 ng/ml

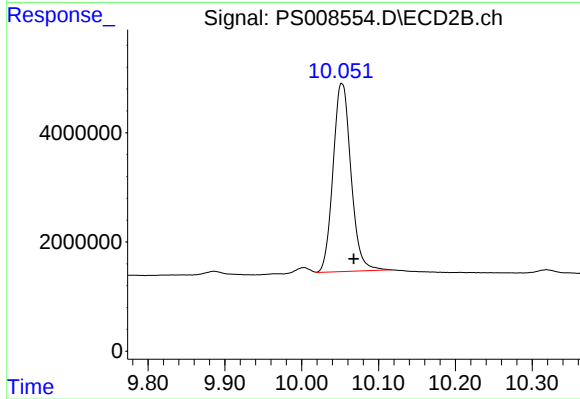

#15 Picloram


R.T.: 10.052 min
Delta R.T.: -0.016 min
Response: 55405608
Conc: 7.46 ng/ml

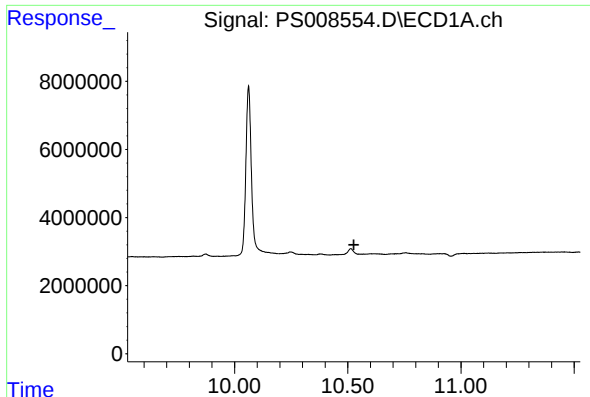

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.527 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

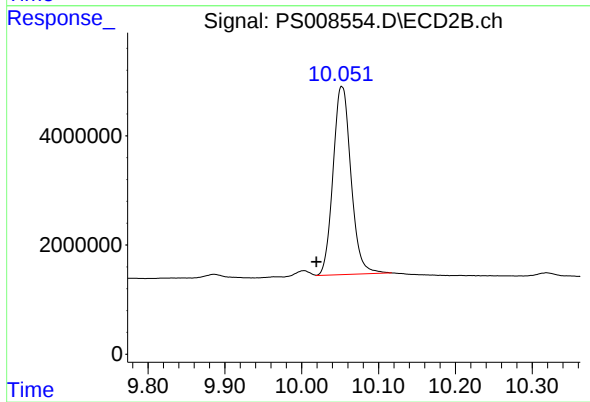

#16 DCPA

R.T.: 10.052 min
Delta R.T.: 0.033 min
Response: 55405608
Conc: 8.50 ng/ml