

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012720\
 Data File : PS008572.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jan 2020 21:32
 Operator : DD\AJ
 Sample : PB126364BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 28 04:52:48 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 08 11:00:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.277	5.971	955.8E6	492.6E6	541.322	519.883
Target Compounds							
1) T	Dalapon	2.510	2.190	42991645	20538101	16.768	16.201
2) T	3,5-DICHL...	0.000	5.158	0	77197010	N.D.	55.252
7) T	MCPA	6.772	6.436	65833987	23214243	9.009	5.437 #
8) T	DICHLORPROP	0.000	6.792	0	26915191	N.D.	27.858
10) T	Pentachlo...	7.762	0.000	34293009	0	1.411	N.D. #
12) T	2,4,5-T	8.480	0.000	86531906	0	9.379	N.D. #
13) T	2,4-DB	9.041	0.000	2778026	0	2.004	N.D. #
14) T	DINOSEB	0.000	9.088	0	8603014	N.D.	2.277
15) T	Picloram	0.000	10.055	0	33435435	N.D.	4.501
16) T	DCPA	10.590	10.055	-10269020	33435435	N.D.	5.131



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012720\
Data File : PS008572.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jan 2020 21:32
Operator : DD\AJ
Sample : PB126364BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 28 04:52:48 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
Quant Title : 8080.M
QLast Update : Wed Jan 08 11:00:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

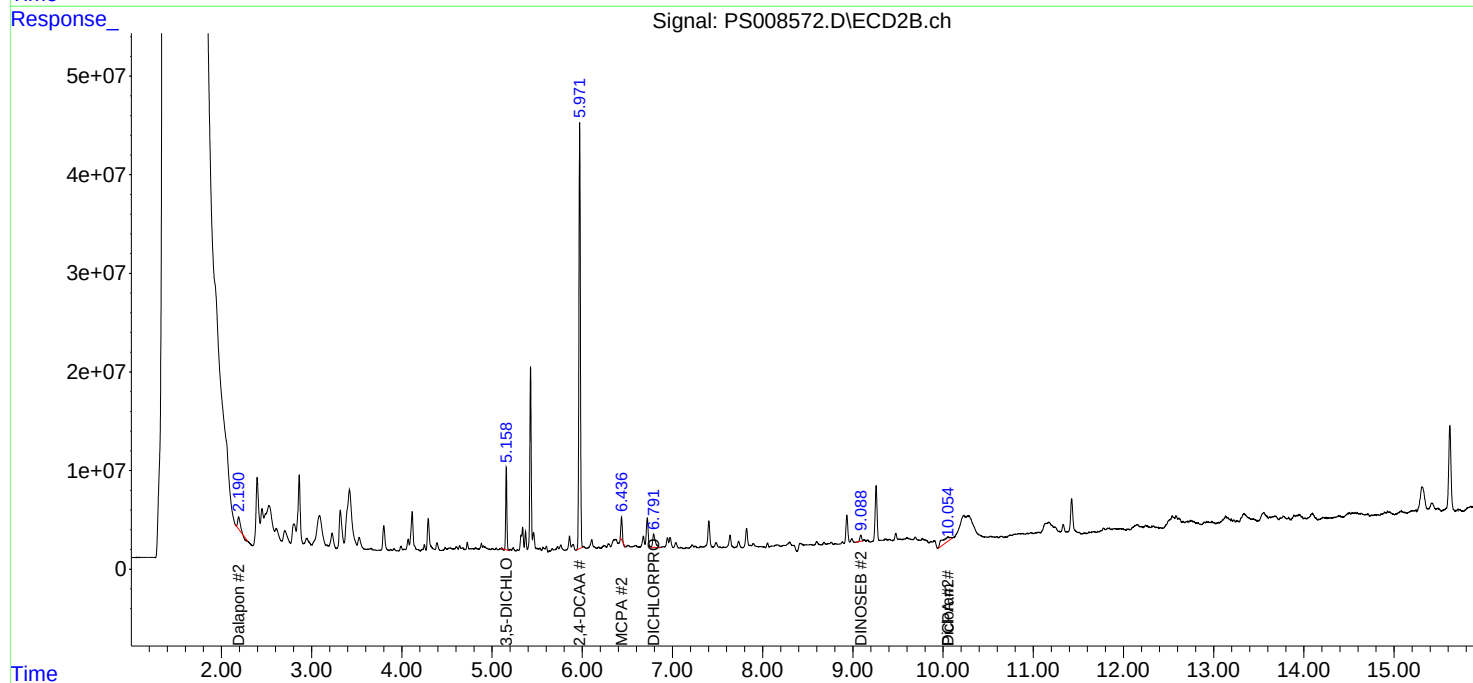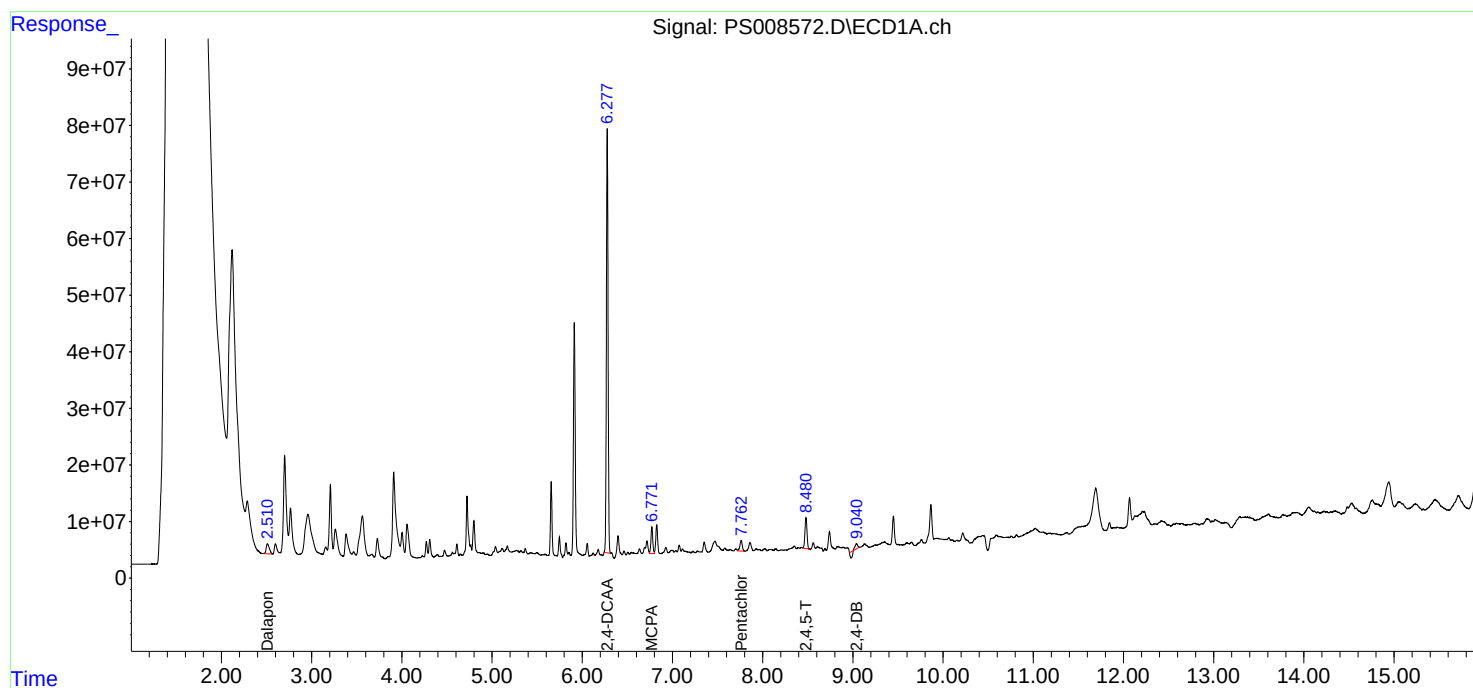


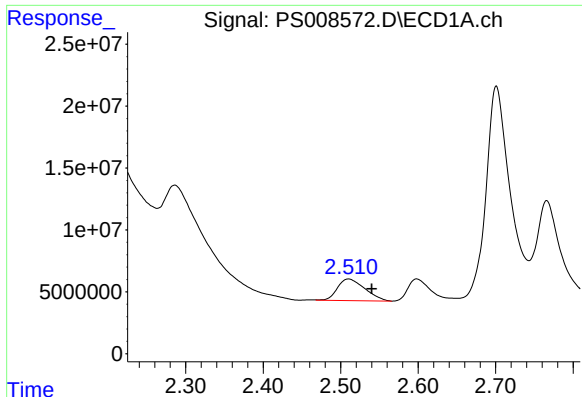

#1 Dalapon


R.T.: 2.510 min
Delta R.T.: -0.030 min
Response: 42991645
Conc: 16.77 ng/ml

Instrument :
ECD_S
ClientSampleId :

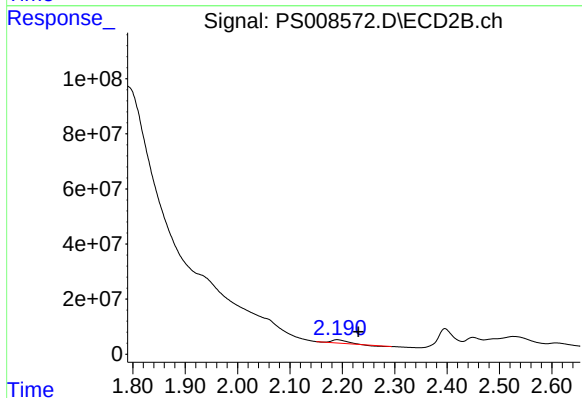


#1 Dalapon

R.T.: 2.190 min
Delta R.T.: -0.041 min
Response: 20538101
Conc: 16.20 ng/ml

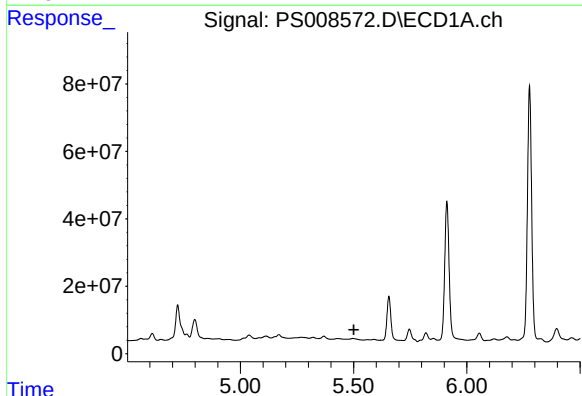


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.501 min
Response: 0
Conc: N.D.

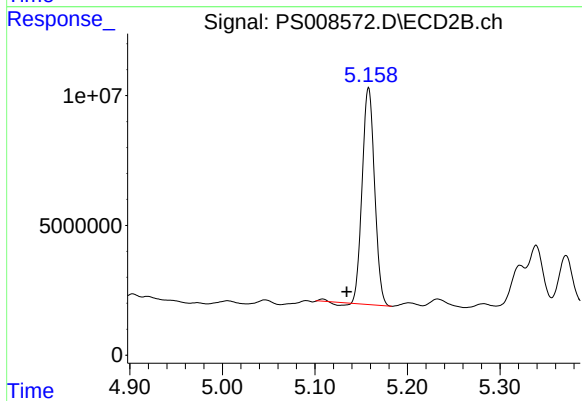

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.158 min
Delta R.T.: 0.024 min
Response: 77197010
Conc: 55.25 ng/ml

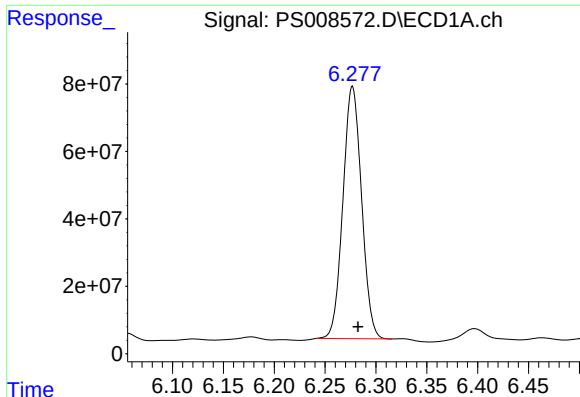

#4 2,4-DCAA


R.T.: 6.277 min
Delta R.T.: -0.006 min
Response: 955814863
Conc: 541.32 ng/ml

Instrument :
ECD_S
ClientSampleId :

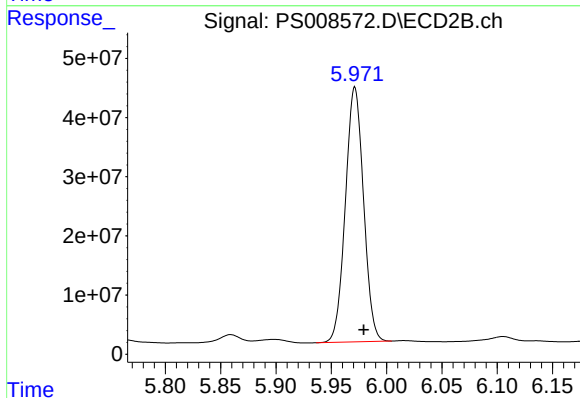


#4 2,4-DCAA

R.T.: 5.971 min
Delta R.T.: -0.008 min
Response: 492569905
Conc: 519.88 ng/ml

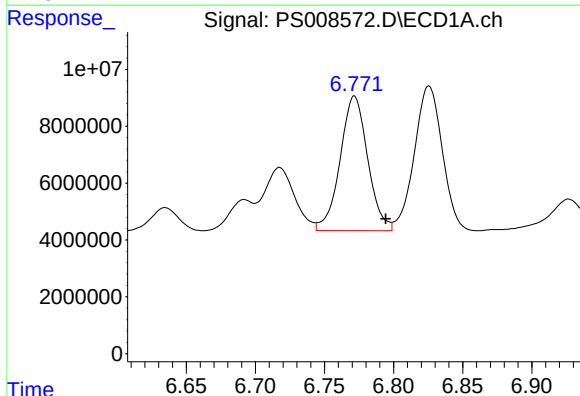


#7 MCPA

R.T.: 6.772 min
Delta R.T.: -0.023 min
Response: 65833987
Conc: 9.01 ug/ml

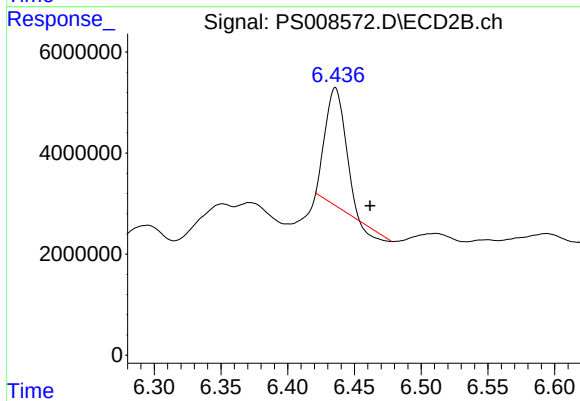

#7 MCPA


R.T.: 6.436 min
Delta R.T.: -0.026 min
Response: 23214243
Conc: 5.44 ug/ml

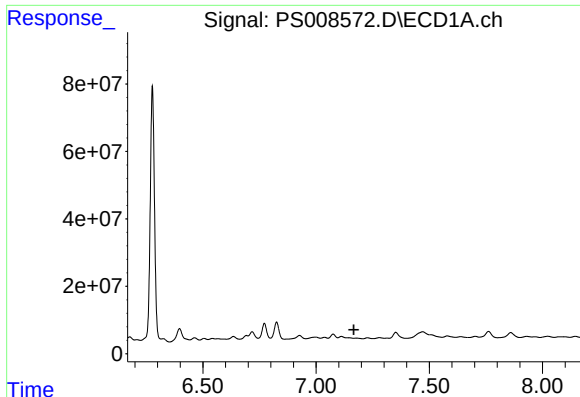

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.167 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

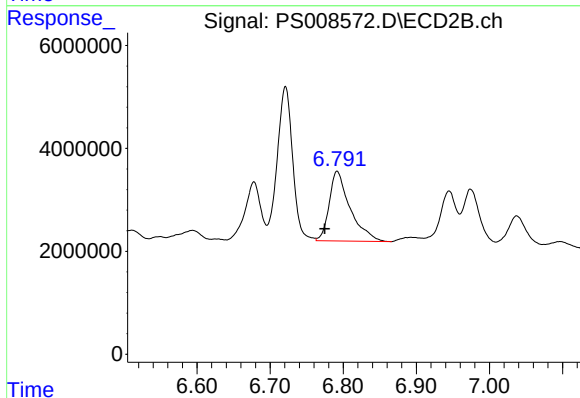


#8 DICHLORPROP

R.T.: 6.792 min
Delta R.T.: 0.017 min
Response: 26915191
Conc: 27.86 ng/ml

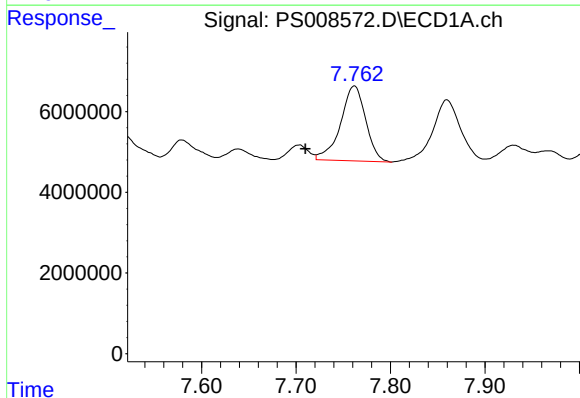


#10 Pentachlorophenol

R.T.: 7.762 min
Delta R.T.: 0.052 min
Response: 34293009
Conc: 1.41 ng/ml

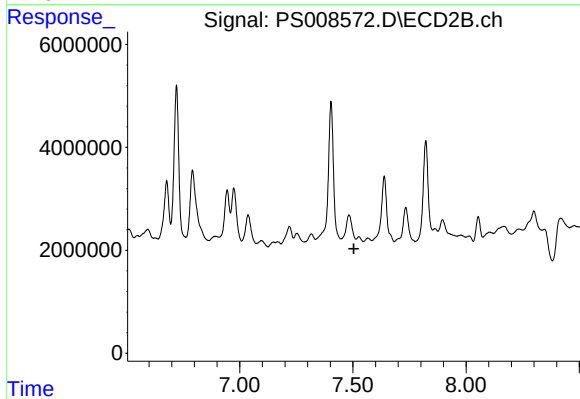

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 7.505 min
Response: 0
Conc: N.D.

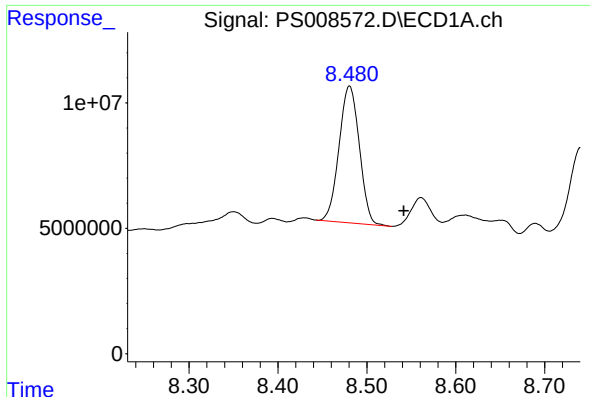

#12 2,4,5-T


R.T.: 8.480 min
Delta R.T.: -0.061 min
Response: 86531906
Conc: 9.38 ng/ml

Instrument :
ECD_S
ClientSampleId :

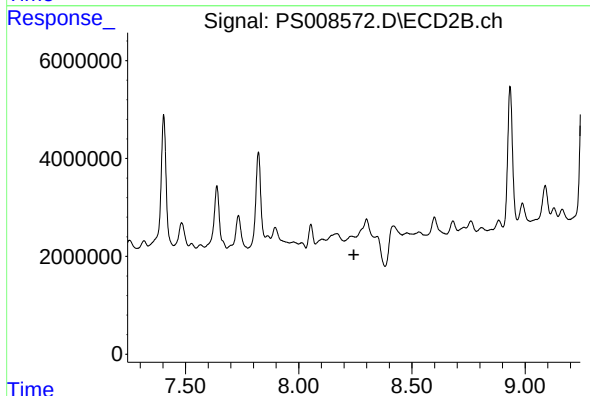


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 8.243 min
Response: 0
Conc: N.D.

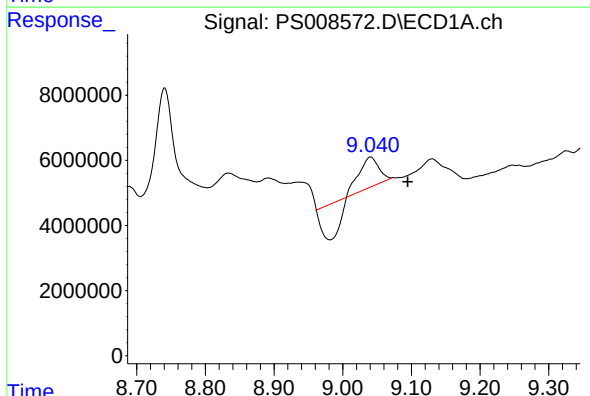


#13 2,4-DB

R.T.: 9.041 min
Delta R.T.: -0.054 min
Response: 2778026
Conc: 2.00 ng/ml

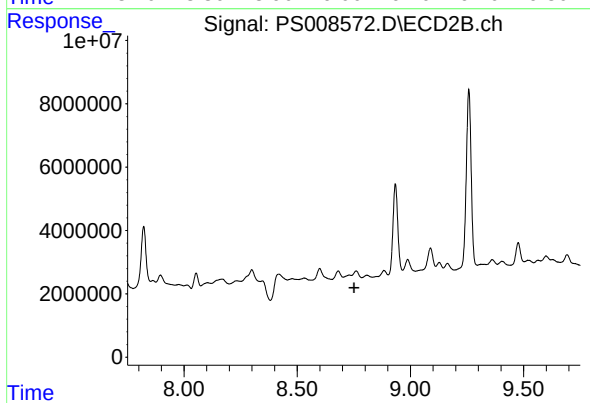

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 8.751 min
Response: 0
Conc: N.D.

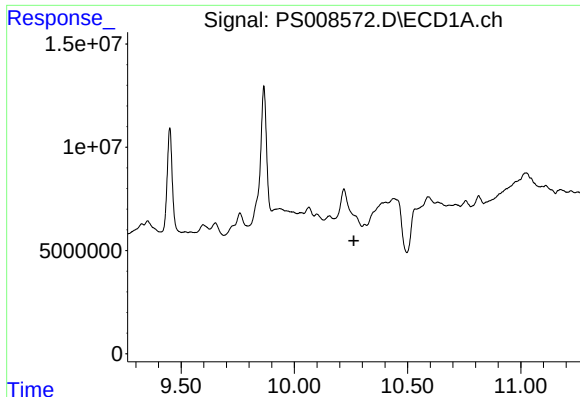

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 10.263 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

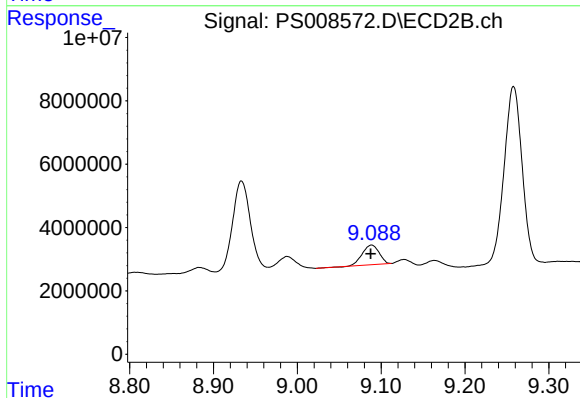


#14 DINOSEB

R.T.: 9.088 min
Delta R.T.: 0.000 min
Response: 8603014
Conc: 2.28 ng/ml

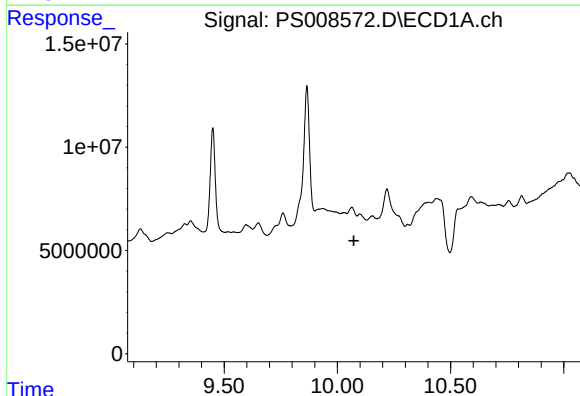


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 10.073 min
Response: 0
Conc: N.D.

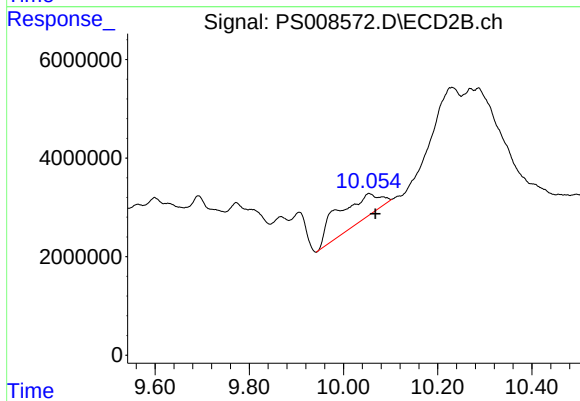

#15 Picloram


R.T.: 10.055 min
Delta R.T.: -0.013 min
Response: 33435435
Conc: 4.50 ng/ml

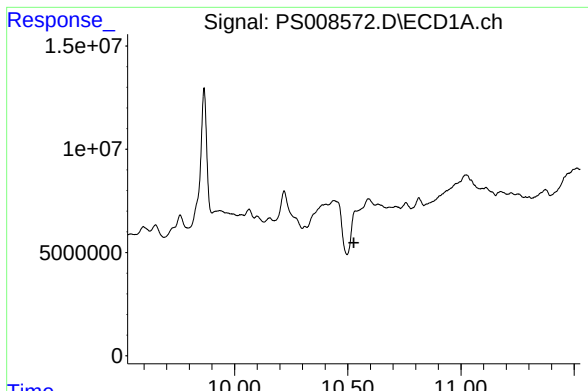

#16 DCPA

R.T.: 10.590 min
Delta R.T.: 0.063 min
Response: -10269020
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

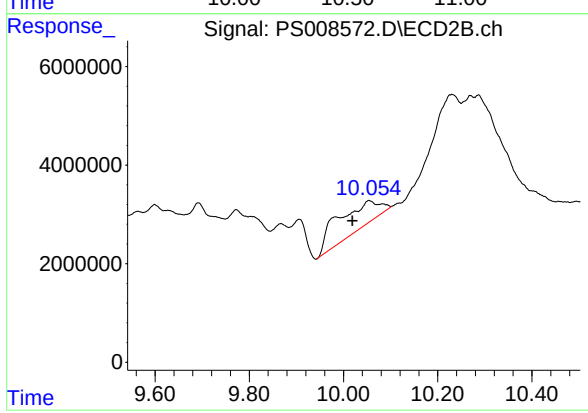

#16 DCPA

R.T.: 10.055 min
Delta R.T.: 0.035 min
Response: 33435435
Conc: 5.13 ng/ml