

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012720\
 Data File : PS008576.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jan 2020 23:00
 Operator : DD\AJ
 Sample : L1265-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 28 04:54:15 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 08 11:00:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.273	5.968	958.4E6	501.2E6	542.772	529.026
Target Compounds							
1) T	Dalapon	2.506	2.188	57458682	43835903	22.411	34.578 #
2) T	3,5-DICHL...	0.000	5.155	0	56515748	N.D.	40.450
6) T	MCP	6.712	0.000	56836577	0	11.151	N.D. #
7) T	MCPA	6.821	6.432	61002015	14129078	8.348	3.309 #
8) T	DICHLORPROP	0.000	6.787	0	24066991	N.D.	24.910
9) T	2,4-D	0.000	7.034	0	11727167	N.D.	10.004
10) T	Pentachlo...	7.756	0.000	31574079	0	1.299	N.D. #
12) T	2,4,5-T	8.478	0.000	87418483	0	9.475	N.D. #
14) T	DINOSEB	10.214	9.085	23899892	8463075	3.331	2.240 #
15) T	Picloram	10.121	10.001	174.0E6	42794477	13.942	5.760 #
16) T	DCPA	10.578	10.001	68206806	42794477	5.747	6.567



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012720\
Data File : PS008576.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jan 2020 23:00
Operator : DD\AJ
Sample : L1265-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 28 04:54:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
Quant Title : 8080.M
QLast Update : Wed Jan 08 11:00:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

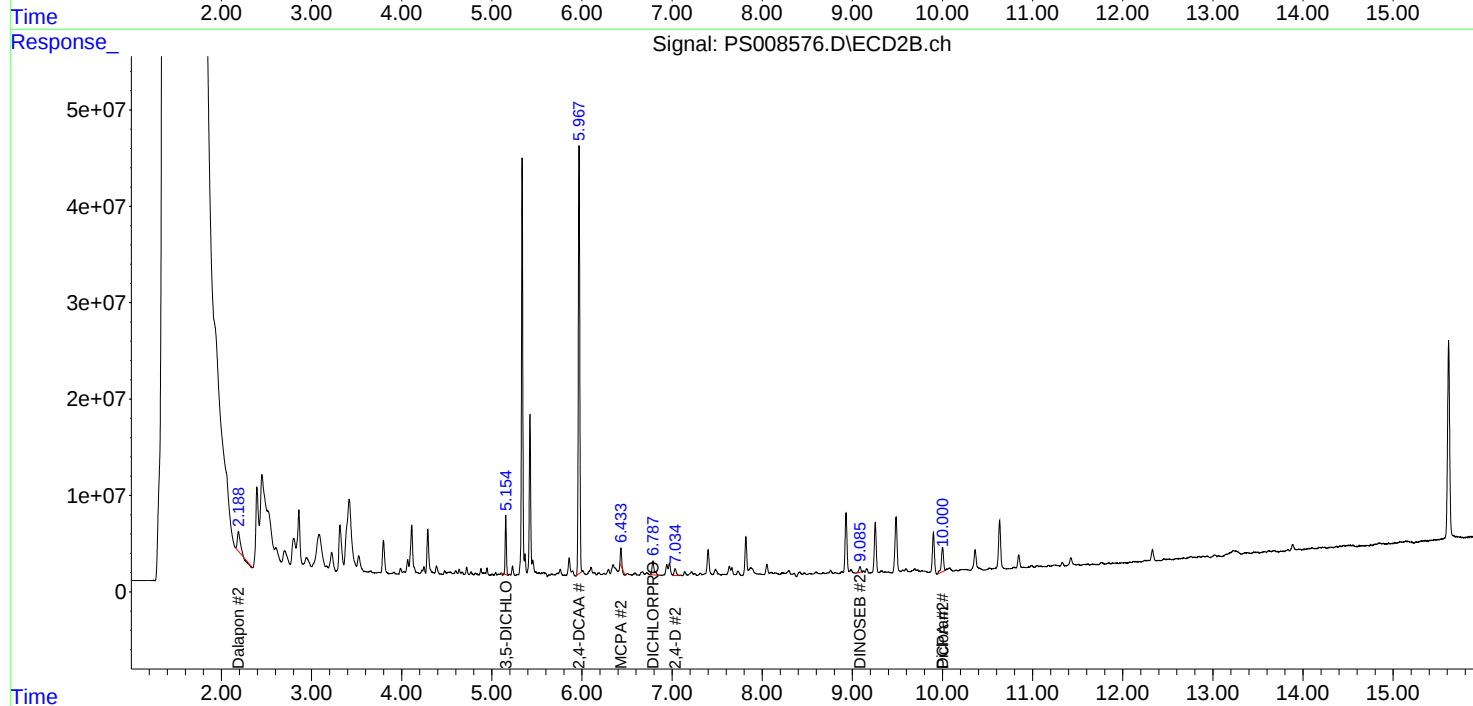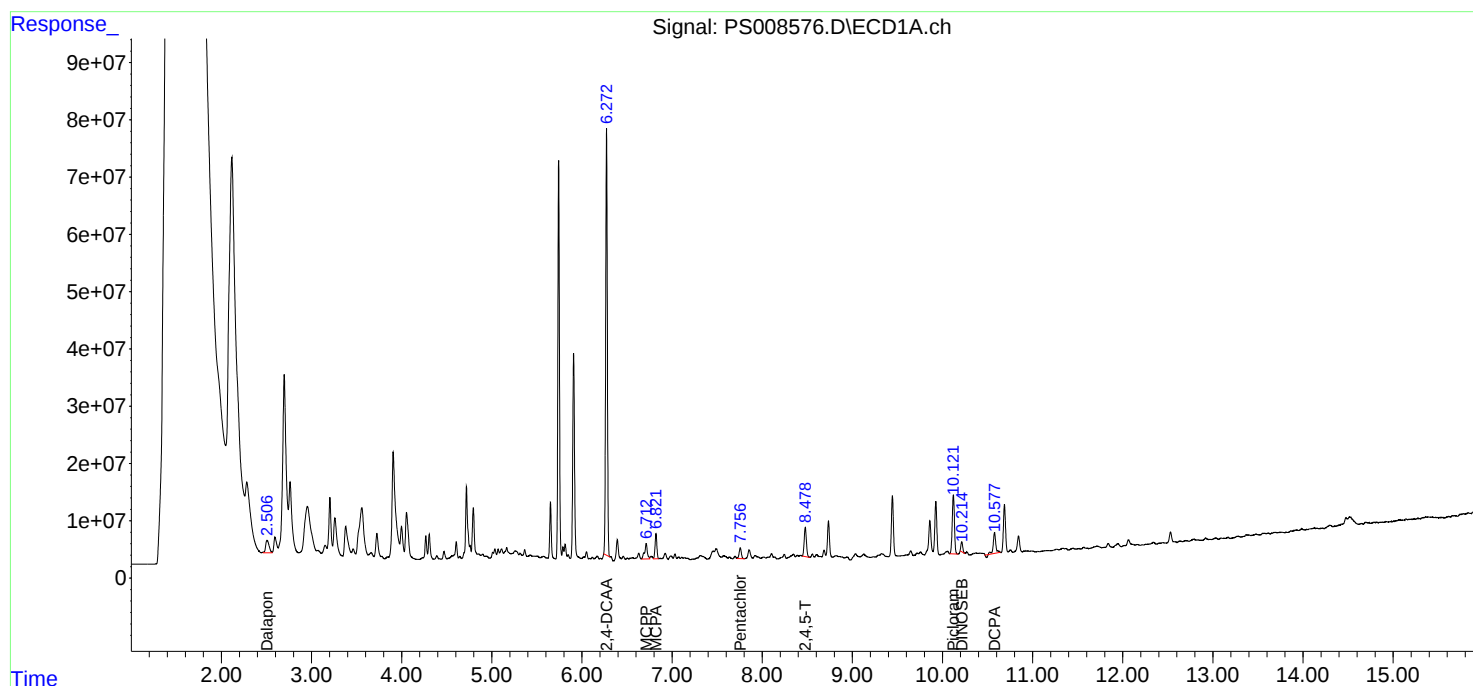


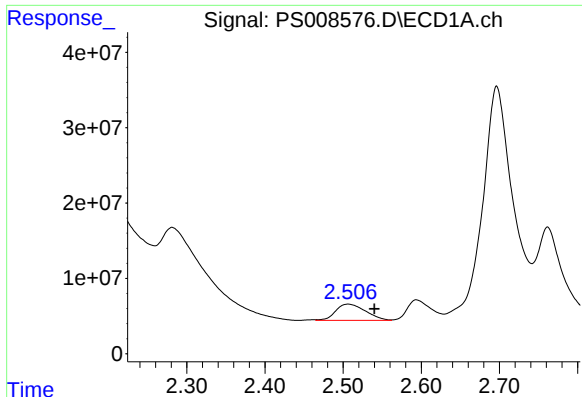

#1 Dalapon


R.T.: 2.506 min
Delta R.T.: -0.034 min
Response: 57458682
Conc: 22.41 ng/ml

Instrument :
ECD_S
ClientSampleId :

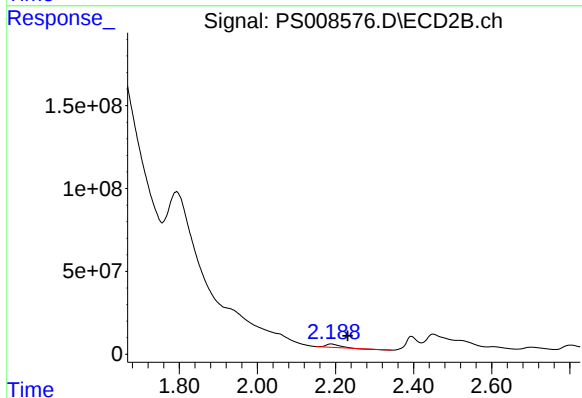


#1 Dalapon

R.T.: 2.188 min
Delta R.T.: -0.043 min
Response: 43835903
Conc: 34.58 ng/ml

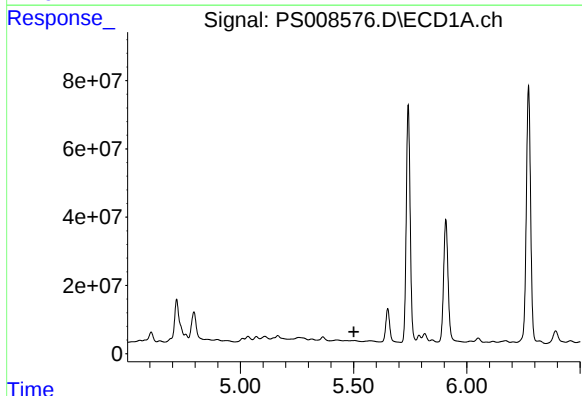


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.501 min
Response: 0
Conc: N.D.

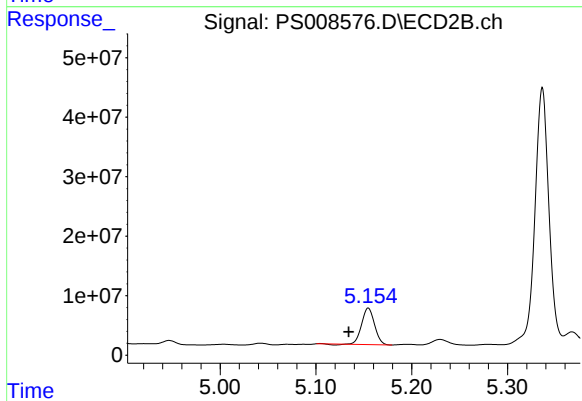

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.155 min
Delta R.T.: 0.020 min
Response: 56515748
Conc: 40.45 ng/ml

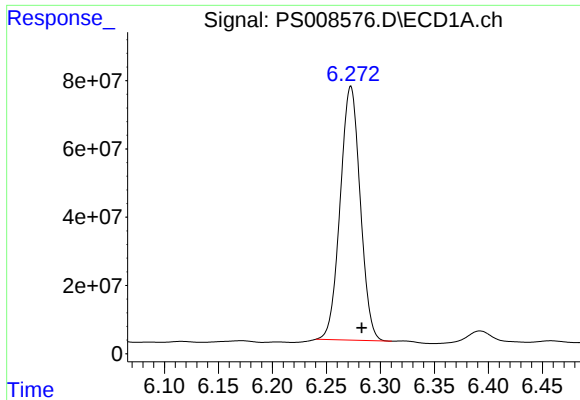

#4 2,4-DCAA


R.T.: 6.273 min
Delta R.T.: -0.010 min
Response: 958373697
Conc: 542.77 ng/ml

Instrument :
ECD_S
ClientSampleId :

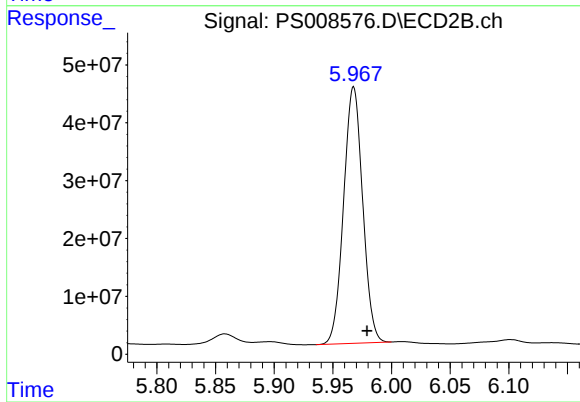


#4 2,4-DCAA

R.T.: 5.968 min
Delta R.T.: -0.011 min
Response: 501233014
Conc: 529.03 ng/ml

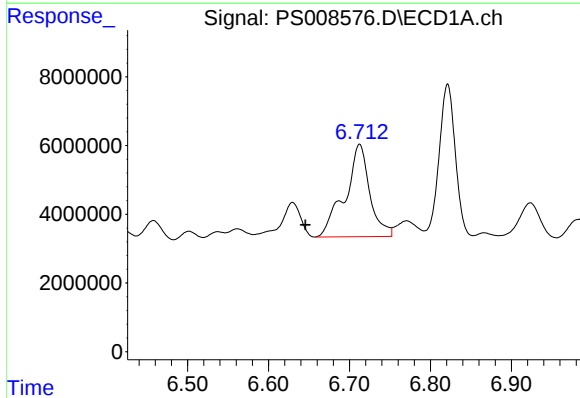


#6 MCP

R.T.: 6.712 min
Delta R.T.: 0.067 min
Response: 56836577
Conc: 11.15 ug/ml

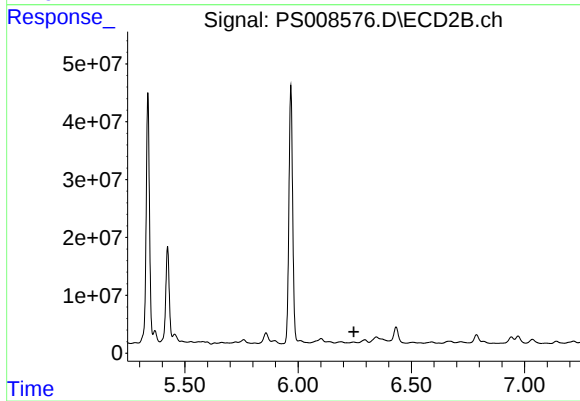

#6 MCP


R.T.: 0.000 min
Exp R.T.: 6.246 min
Response: 0
Conc: N.D.

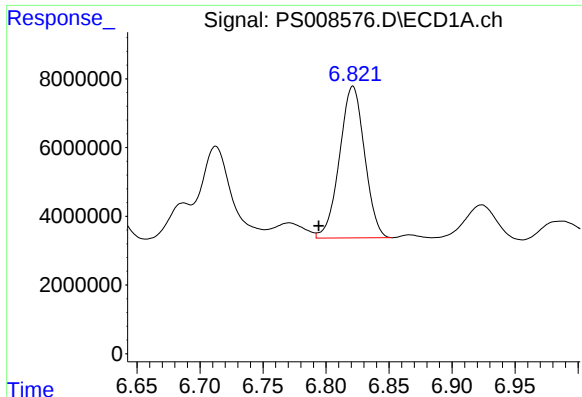

#7 MCPA


R.T.: 6.821 min
Delta R.T.: 0.027 min
Response: 61002015
Conc: 8.35 ug/ml

Instrument :
ECD_S
ClientSampleId :

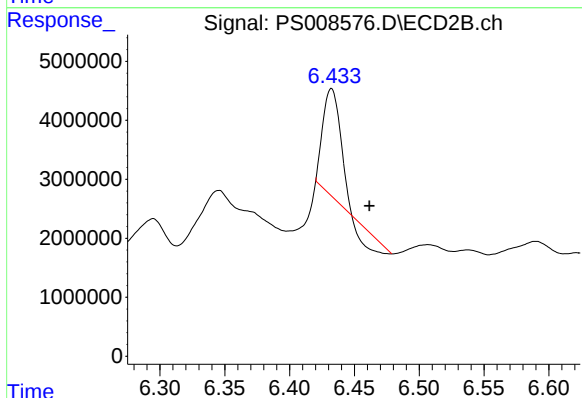


#7 MCPA

R.T.: 6.432 min
Delta R.T.: -0.029 min
Response: 14129078
Conc: 3.31 ug/ml

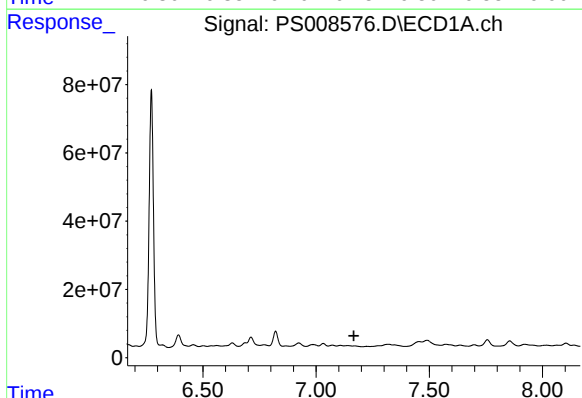


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 7.167 min
Response: 0
Conc: N.D.

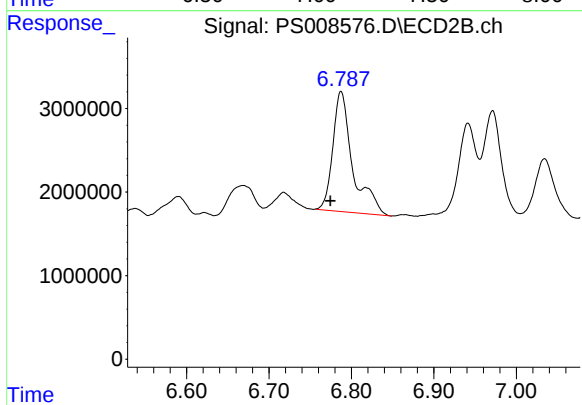

#8 DICHLORPROP


R.T.: 6.787 min
Delta R.T.: 0.013 min
Response: 24066991
Conc: 24.91 ng/ml

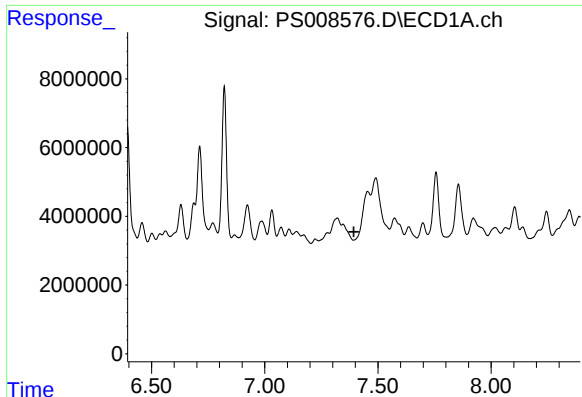

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.394 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

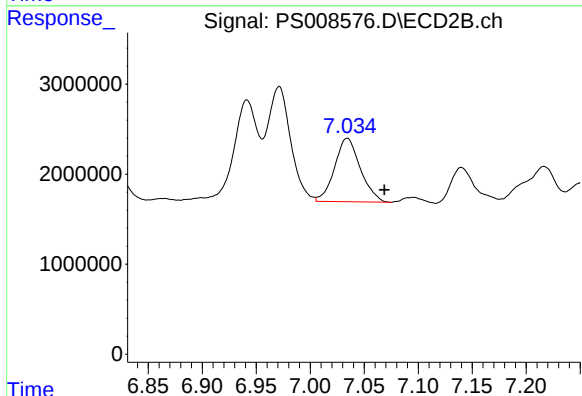


#9 2,4-D

R.T.: 7.034 min
Delta R.T.: -0.034 min
Response: 11727167
Conc: 10.00 ng/ml

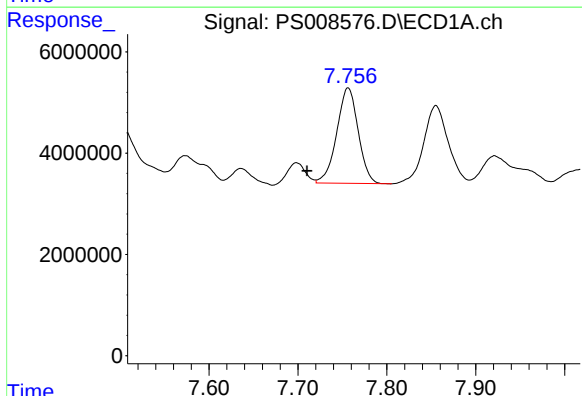


#10 Pentachlorophenol

R.T.: 7.756 min
Delta R.T.: 0.046 min
Response: 31574079
Conc: 1.30 ng/ml

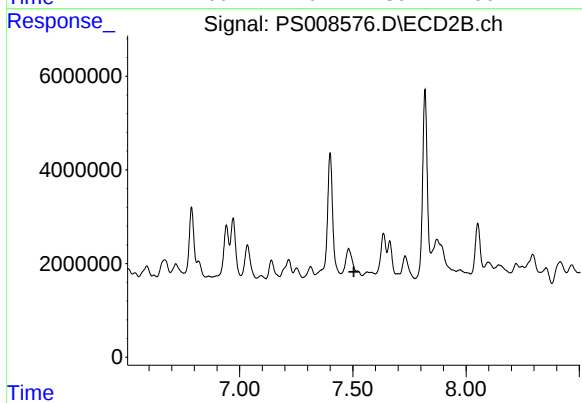

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 7.505 min
Response: 0
Conc: N.D.

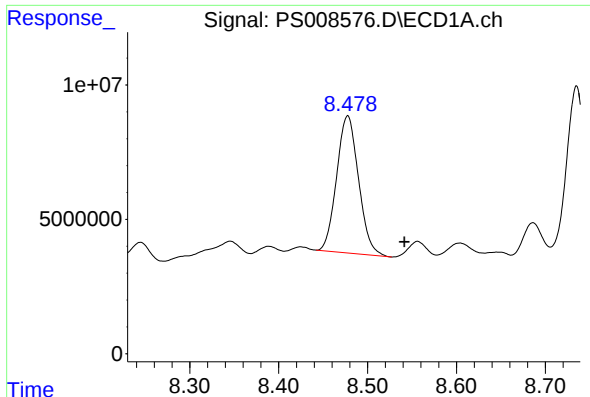

#12 2,4,5-T


R.T.: 8.478 min
Delta R.T.: -0.064 min
Response: 87418483
Conc: 9.47 ng/ml

Instrument :
ECD_S
ClientSampleId :

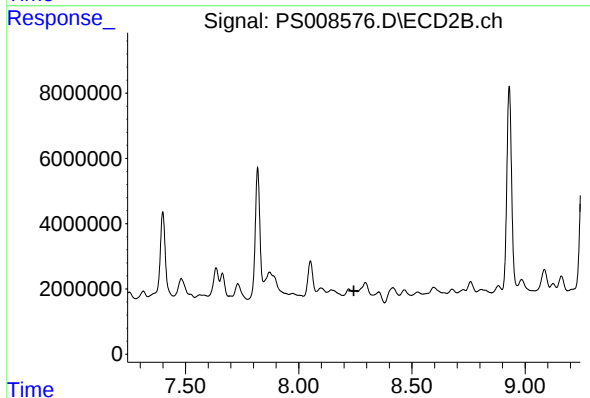


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 8.243 min
Response: 0
Conc: N.D.

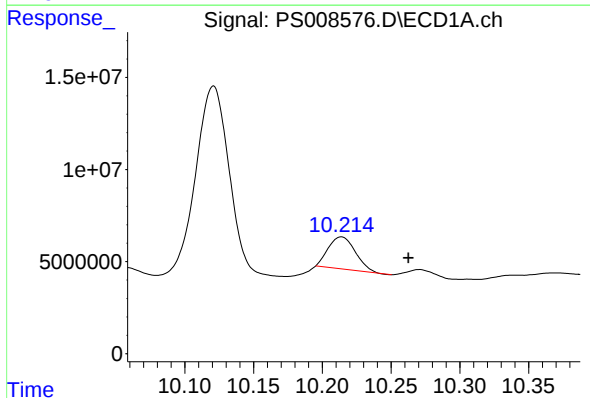


#14 DINOSEB

R.T.: 10.214 min
Delta R.T.: -0.049 min
Response: 23899892
Conc: 3.33 ng/ml

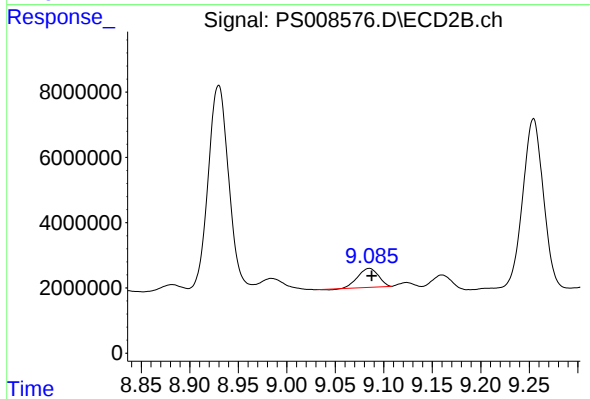

#14 DINOSEB


R.T.: 9.085 min
Delta R.T.: -0.003 min
Response: 8463075
Conc: 2.24 ng/ml

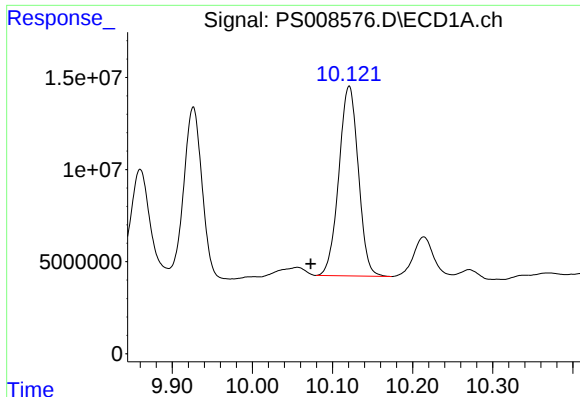

#15 Picloram


R.T.: 10.121 min
Delta R.T.: 0.048 min
Response: 174022852
Conc: 13.94 ng/ml

Instrument :
ECD_S
ClientSampleId :

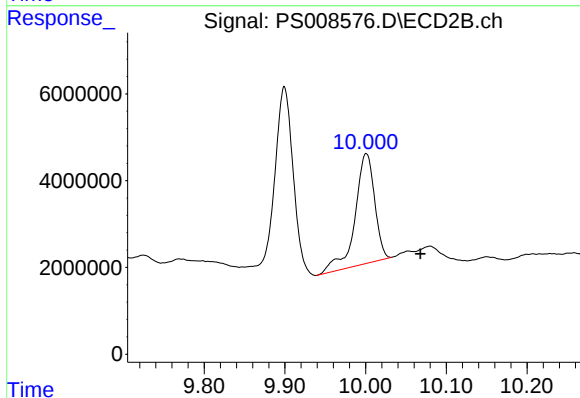


#15 Picloram

R.T.: 10.001 min
Delta R.T.: -0.067 min
Response: 42794477
Conc: 5.76 ng/ml

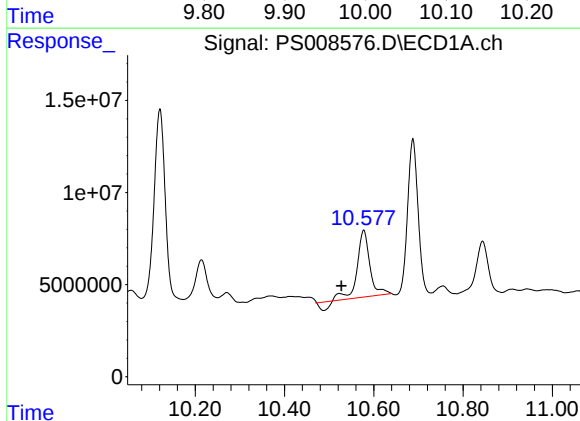

#16 DCPA

R.T.: 10.578 min
Delta R.T.: 0.050 min
Response: 68206806
Conc: 5.75 ng/ml

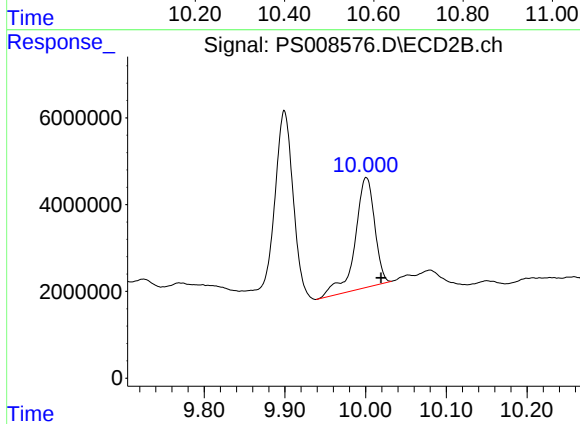

#16 DCPA

R.T.: 10.001 min
Delta R.T.: -0.018 min
Response: 42794477
Conc: 6.57 ng/ml