

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012720\
 Data File : PS008577.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jan 2020 23:22
 Operator : DD\AJ
 Sample : L1264-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 28 04:54:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
 Quant Title : 8080.M
 QLast Update : Wed Jan 08 11:00:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.268	5.964	1002.1E6	537.7E6	567.534	567.525
Target Compounds							
1) T	Dalapon	2.502	2.184	55583221	38640555	21.680	30.480 #
2) T	3,5-DICHL...	0.000	5.150	0	42170647	N.D.	30.183
5) T	DICAMBA	0.000	6.097	0	4719499	N.D.	1.180
6) T	MCP	6.708	0.000	56999285	0	11.183	N.D. #
7) T	MCPA	6.817	0.000	60403243	0	8.266	N.D. #
8) T	DICHLORPROP	0.000	6.783	0	25494453	N.D.	26.388
9) T	2,4-D	0.000	7.030	0	11319879	N.D.	9.657
10) T	Pentachlo...	7.752	0.000	29068538	0	1.196	N.D. #
12) T	2,4,5-T	8.473	0.000	90849519	0	9.847	N.D. #
13) T	2,4-DB	9.030	0.000	20426702	0	14.735	N.D. #
14) T	DINOSEB	10.211	9.081	19610209	12190998	2.733	3.227
15) T	Picloram	10.118	0.000	229.4E6	0	18.380	N.D. #
16) T	DCPA	10.574	9.996	71738534	48745191	6.045	7.480



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012720\
Data File : PS008577.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jan 2020 23:22
Operator : DD\AJ
Sample : L1264-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 28 04:54:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010820.M
Quant Title : 8080.M
QLast Update : Wed Jan 08 11:00:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

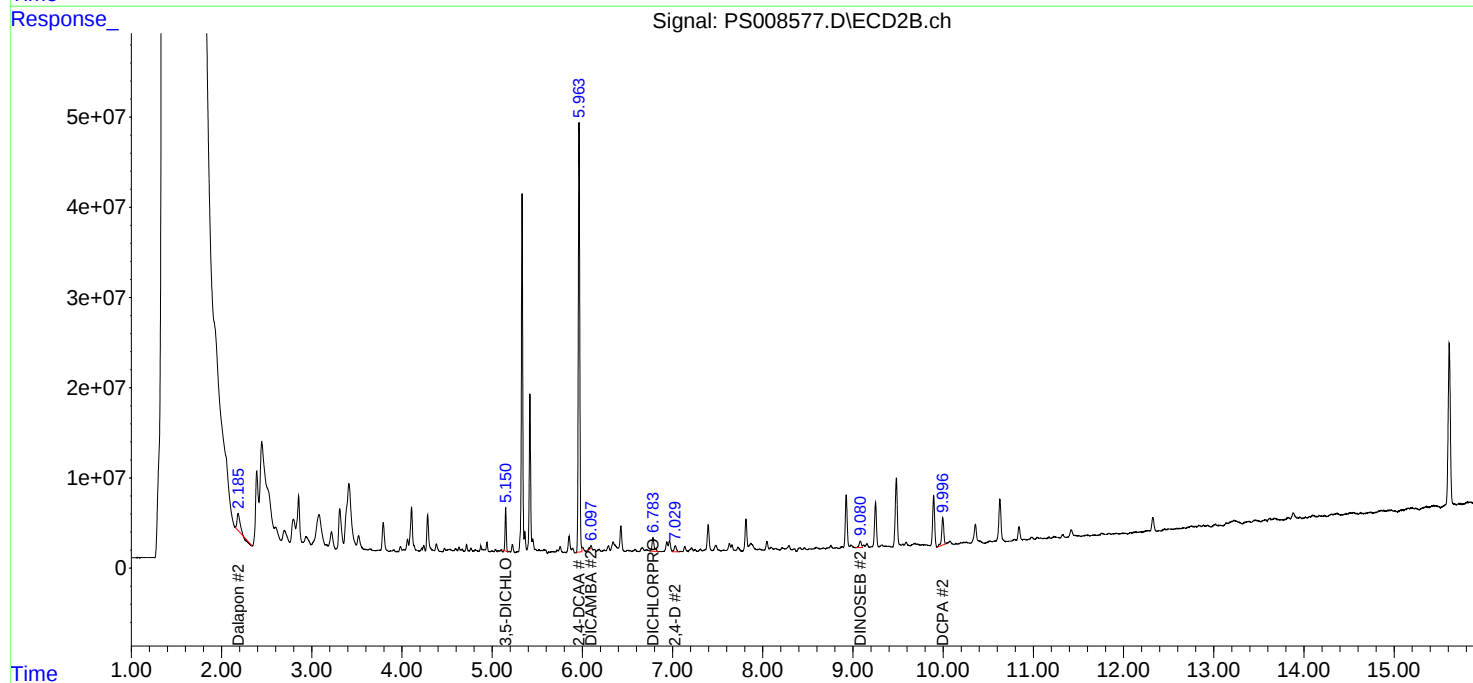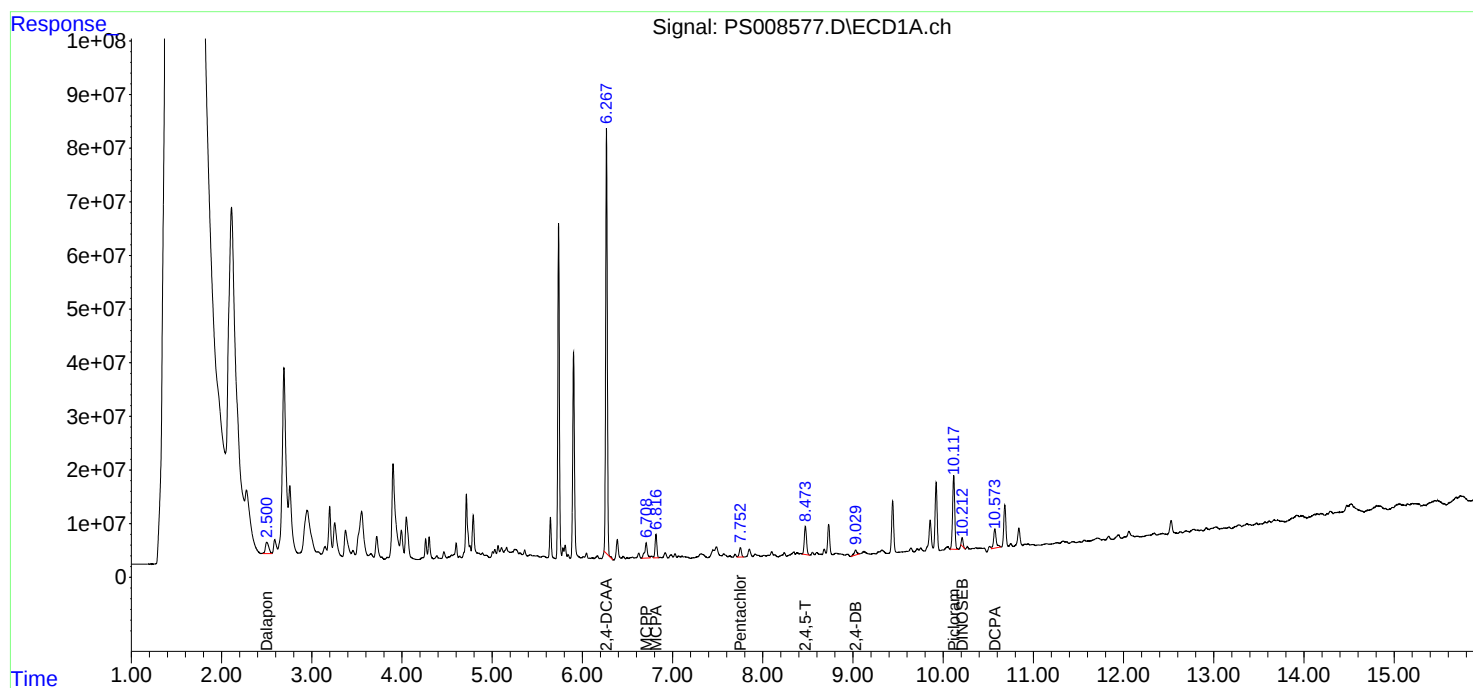


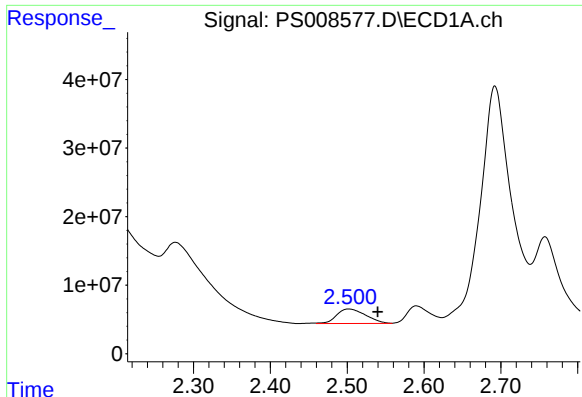

#1 Dalapon


R.T.: 2.502 min
Delta R.T.: -0.038 min
Response: 55583221
Conc: 21.68 ng/ml

Instrument :
ECD_S
ClientSampleId :

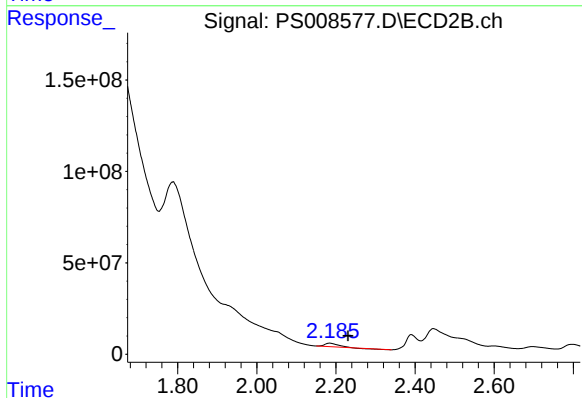


#1 Dalapon

R.T.: 2.184 min
Delta R.T.: -0.047 min
Response: 38640555
Conc: 30.48 ng/ml

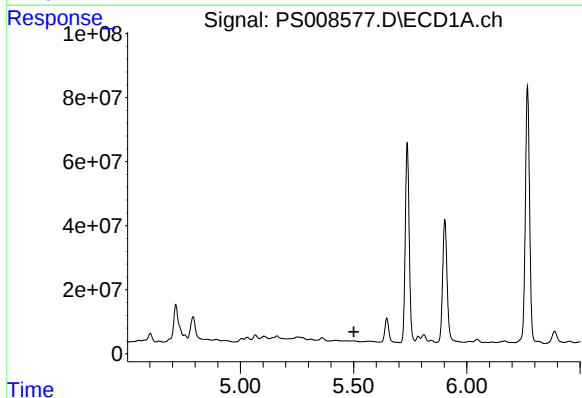


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.501 min
Response: 0
Conc: N.D.

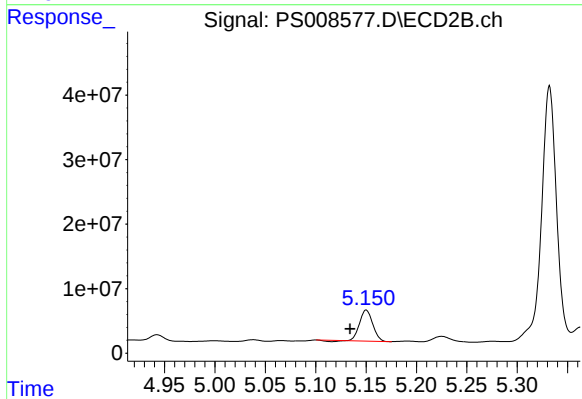

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.150 min
Delta R.T.: 0.016 min
Response: 42170647
Conc: 30.18 ng/ml

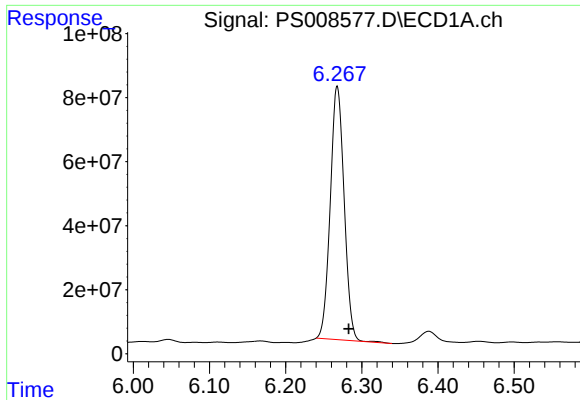

#4 2,4-DCAA


R.T.: 6.268 min
Delta R.T.: -0.015 min
Response: 1002096470
Conc: 567.53 ng/ml

Instrument :
ECD_S
ClientSampleId :

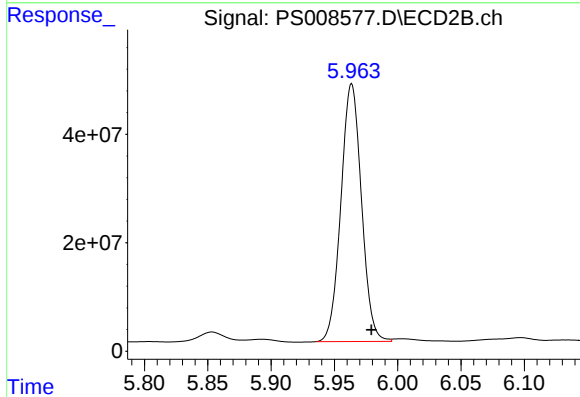


#4 2,4-DCAA

R.T.: 5.964 min
Delta R.T.: -0.016 min
Response: 537709118
Conc: 567.53 ng/ml

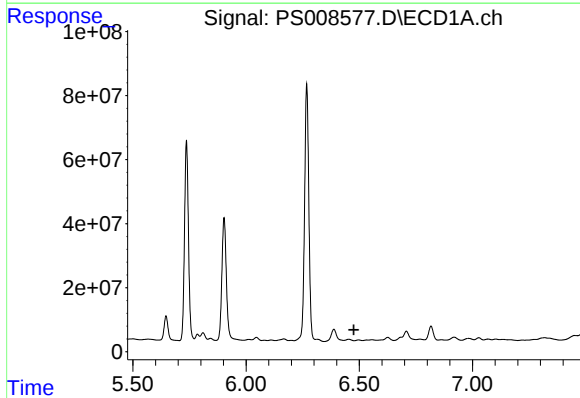


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 6.476 min
Response: 0
Conc: N.D.

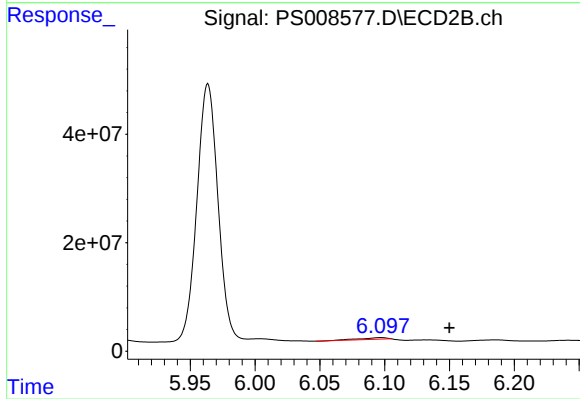

#5 DICAMBA


R.T.: 6.097 min
Delta R.T.: -0.053 min
Response: 4719499
Conc: 1.18 ng/ml

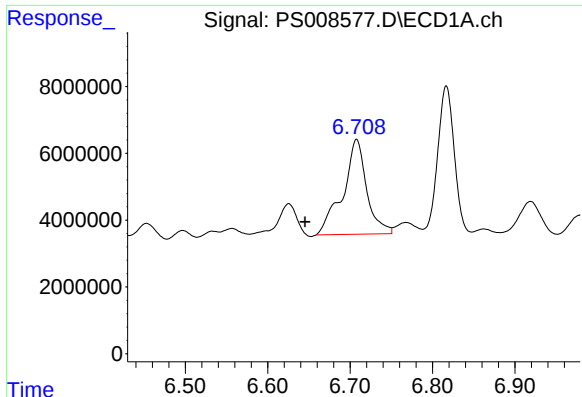

#6 MCPP


R.T.: 6.708 min
Delta R.T.: 0.062 min
Response: 56999285
Conc: 11.18 ug/ml

Instrument :
ECD_S
ClientSampleId :

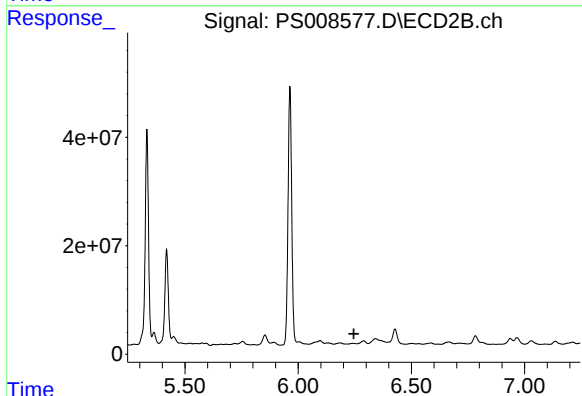


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 6.246 min
Response: 0
Conc: N.D.

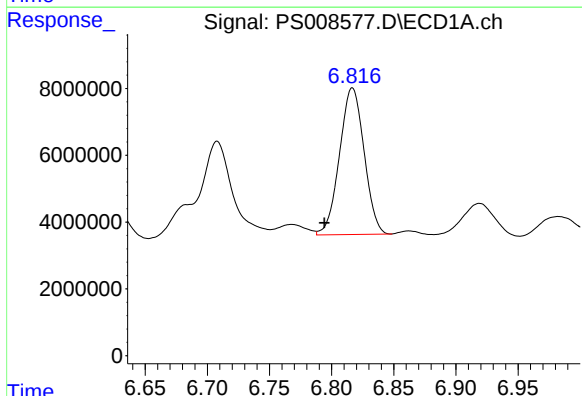


#7 MCPA

R.T.: 6.817 min
Delta R.T.: 0.022 min
Response: 60403243
Conc: 8.27 ug/ml

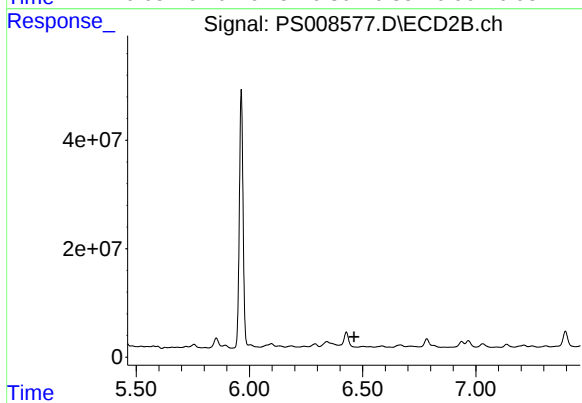

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 6.462 min
Response: 0
Conc: N.D.

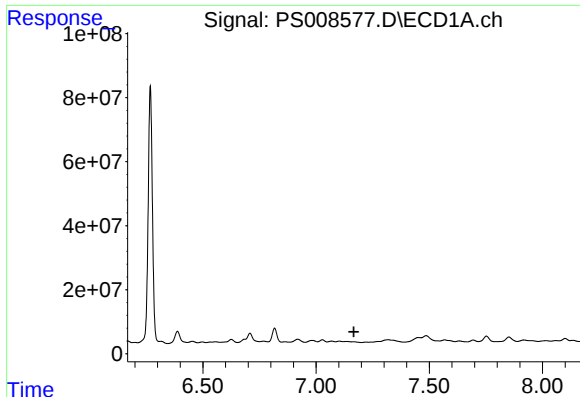

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.167 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

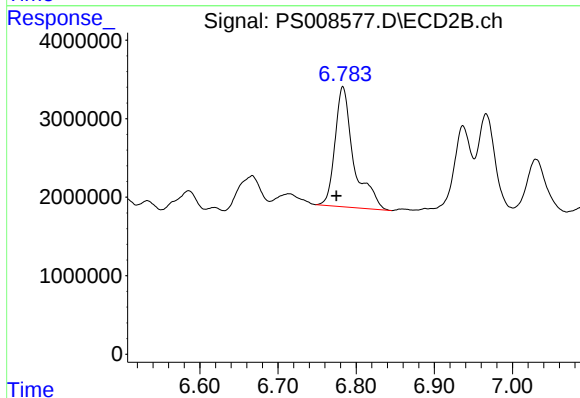


#8 DICHLORPROP

R.T.: 6.783 min
Delta R.T.: 0.008 min
Response: 25494453
Conc: 26.39 ng/ml

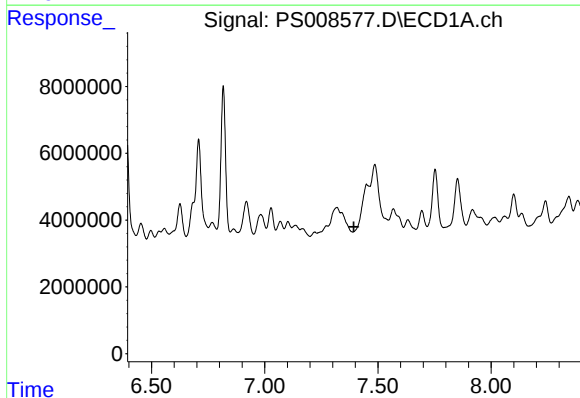


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 7.394 min
Response: 0
Conc: N.D.

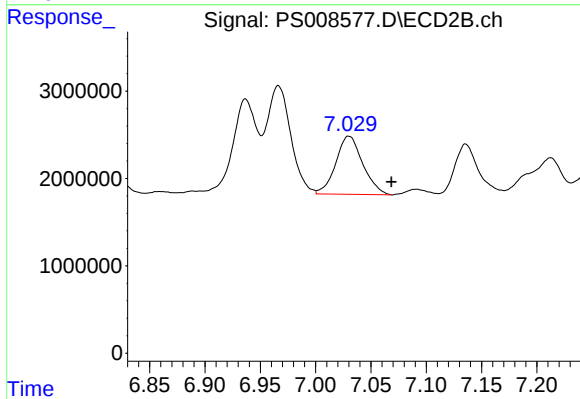

#9 2,4-D


R.T.: 7.030 min
Delta R.T.: -0.039 min
Response: 11319879
Conc: 9.66 ng/ml

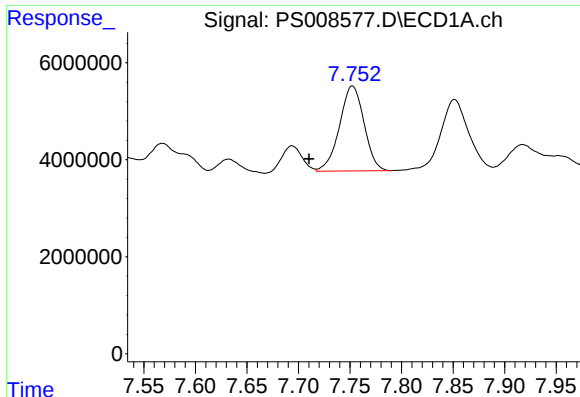

#10 Pentachlorophenol


R.T.: 7.752 min
Delta R.T.: 0.042 min
Response: 29068538
Conc: 1.20 ng/ml

Instrument :
ECD_S
ClientSampleId :

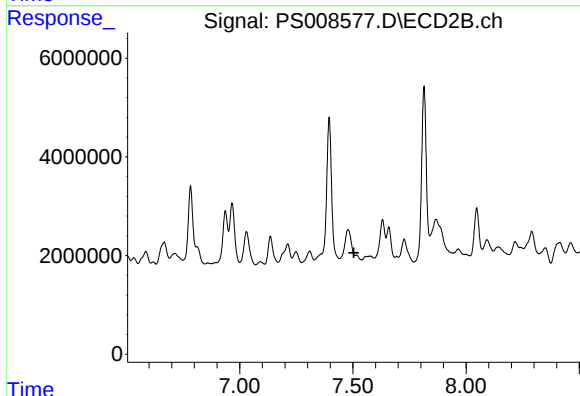


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 7.505 min
Response: 0
Conc: N.D.

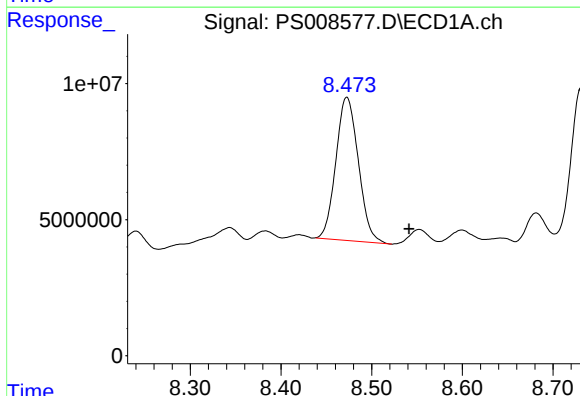


#12 2,4,5-T

R.T.: 8.473 min
Delta R.T.: -0.069 min
Response: 90849519
Conc: 9.85 ng/ml

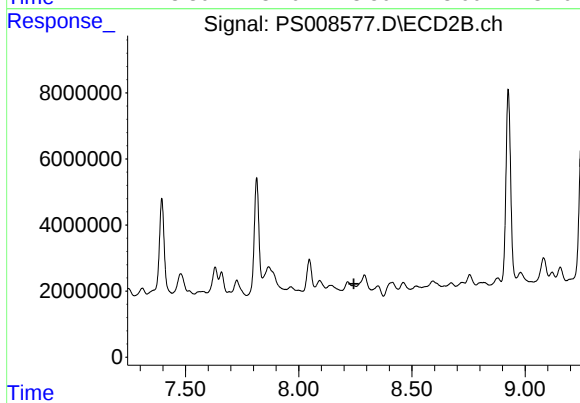

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 8.243 min
Response: 0
Conc: N.D.

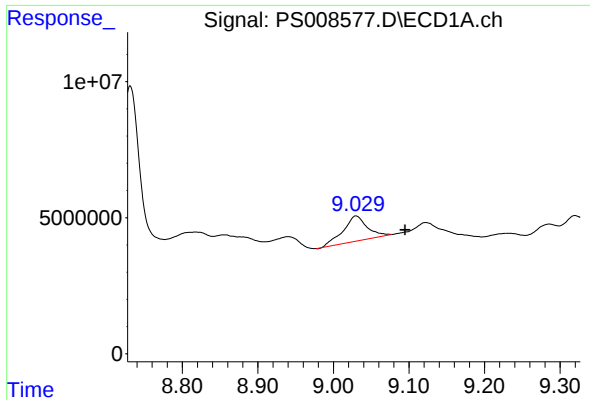

#13 2,4-DB


R.T.: 9.030 min
Delta R.T.: -0.065 min
Response: 20426702
Conc: 14.74 ng/ml

Instrument :
ECD_S
ClientSampleId :

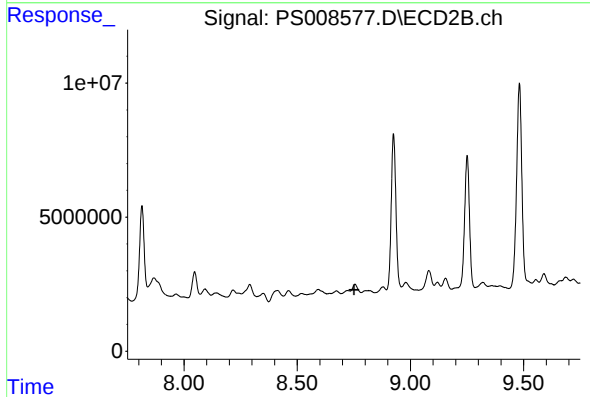


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 8.751 min
Response: 0
Conc: N.D.

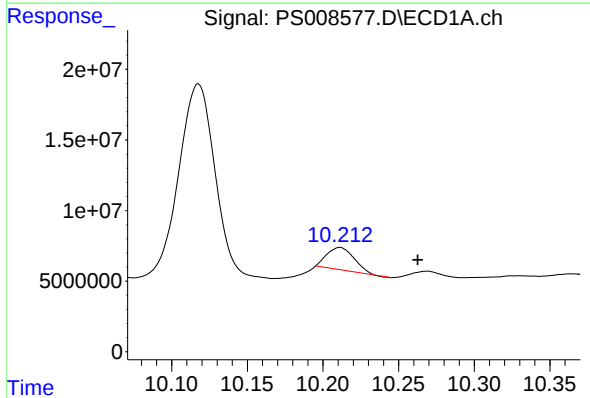


#14 DINOSEB

R.T.: 10.211 min
Delta R.T.: -0.051 min
Response: 19610209
Conc: 2.73 ng/ml

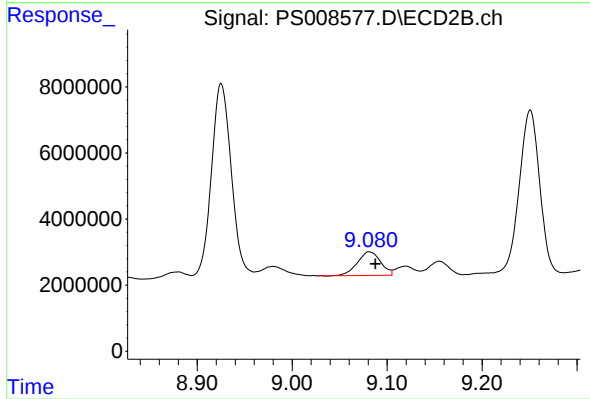

#14 DINOSEB


R.T.: 9.081 min
Delta R.T.: -0.007 min
Response: 12190998
Conc: 3.23 ng/ml

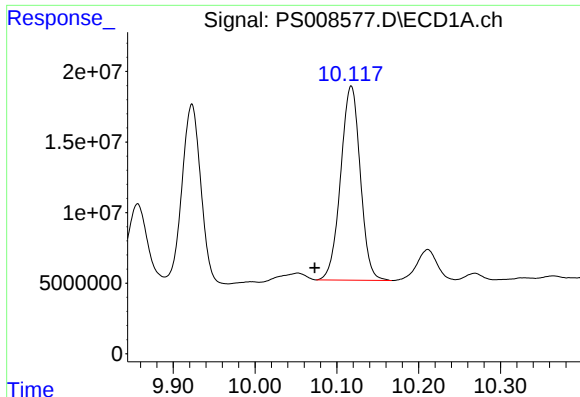

#15 Picloram


R.T.: 10.118 min
Delta R.T.: 0.045 min
Response: 229419289
Conc: 18.38 ng/ml

Instrument :
ECD_S
ClientSampleId :

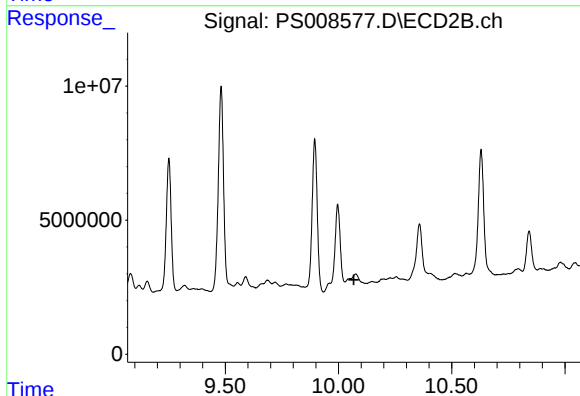


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.068 min
Response: 0
Conc: N.D.

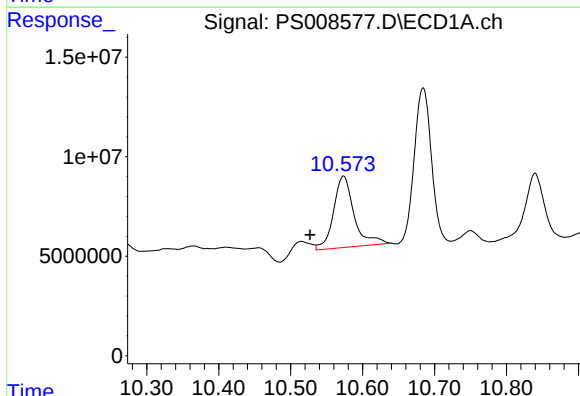

#16 DCPA

R.T.: 10.574 min
Delta R.T.: 0.046 min
Response: 71738534
Conc: 6.04 ng/ml

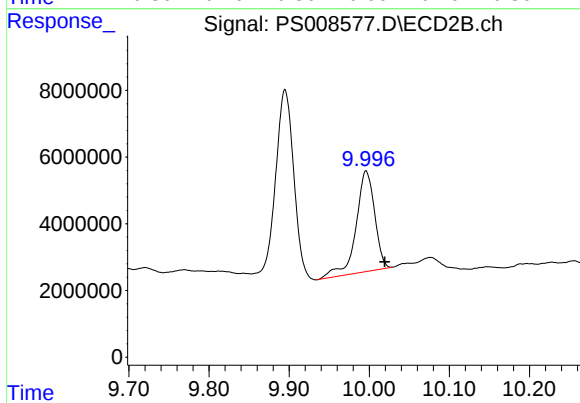

#16 DCPA

R.T.: 9.996 min
Delta R.T.: -0.023 min
Response: 48745191
Conc: 7.48 ng/ml