

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012721\
 Data File : PS013872.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jan 2021 18:35
 Operator : DD\AJ
 Sample : HSTDICC750
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 28 00:53:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012721.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 28 00:52:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.203	6.906	812.9E6	290.7E6	750.000	750.000
Target Compounds							
1) T	Dalapon	3.026	2.621	863.7E6	352.7E6	682.500	682.500
2) T	3,5-DICHL...	6.420	6.062	1046.5E6	424.8E6	697.500	697.500
3) T	4-Nitroph...	7.037	6.520	377.0E6	174.9E6	682.500	682.500
5) T	DICAMBA	7.392	7.072	3079.0E6	1181.3E6	705.000	705.000
6) T	MCPD	7.559	7.167	229.9E6	95708208	70.500	70.500
7) T	MCPA	7.709	7.381	322.4E6	135.8E6	69.750	69.750
8) T	DICHLORPROP	8.083	7.697	770.9E6	301.3E6	705.000	705.000
9) T	2,4-D	8.315	7.995	901.6E6	380.2E6	705.000	705.000
10) T	Pentachlo...	8.621	8.418	11488.8E6	4022.4E6	712.500	712.500
11) T	2,4,5-TP ...	9.170	8.780	4550.0E6	1665.6E6	712.500	712.500
12) T	2,4,5-T	9.457	9.161	4684.6E6	1633.7E6	712.500	712.500
13) T	2,4-DB	10.011	9.668	808.5E6	219.8E6	712.500	712.500
14) T	DINOSEB	11.162	9.995	3621.7E6	1179.7E6	705.000	705.000
15) T	Picloram	10.997	10.990	6338.5E6	2522.8E6	712.500	712.500
16) T	DCPA	11.427	10.921	5912.6E6	2194.2E6	720.000	720.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012721\
Data File : PS013872.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jan 2021 18:35
Operator : DD\AJ
Sample : HSTDICC750
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 28 00:53:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012721.M
Quant Title : 8080.M
QLast Update : Thu Jan 28 00:52:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

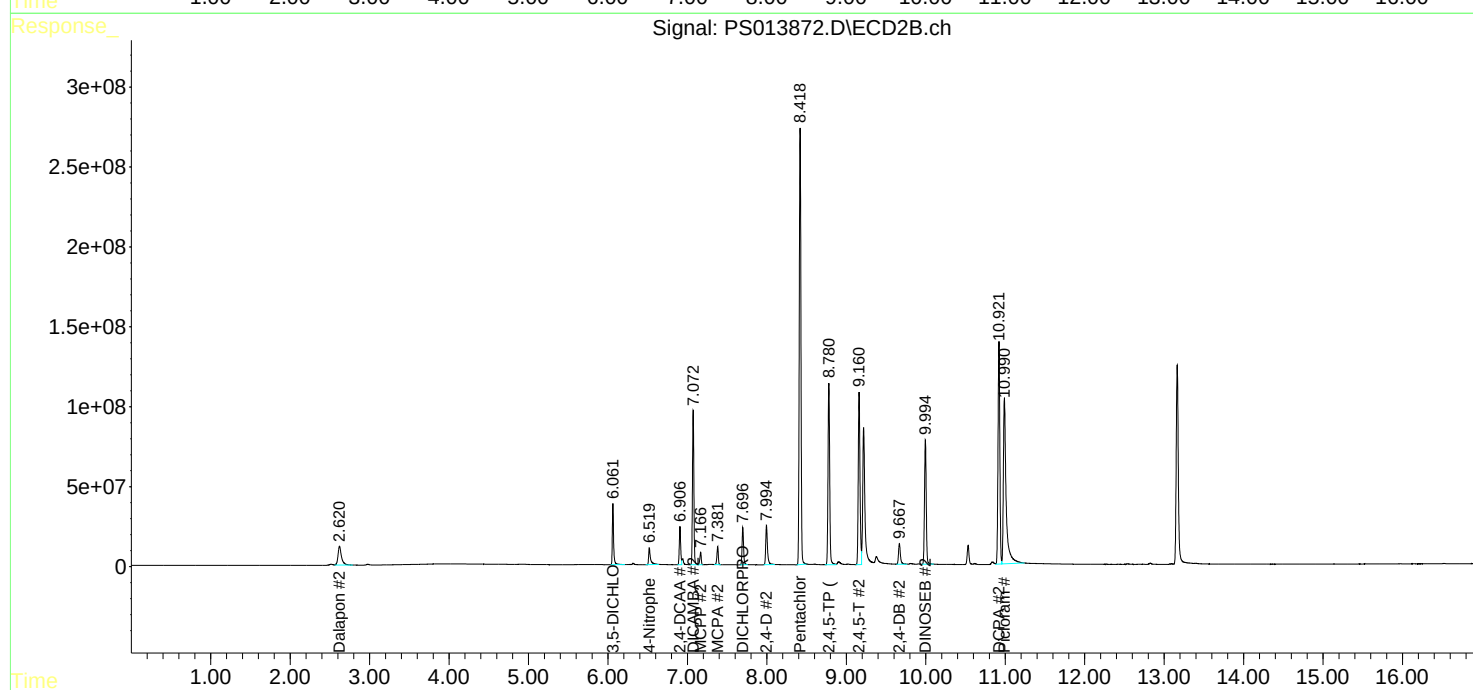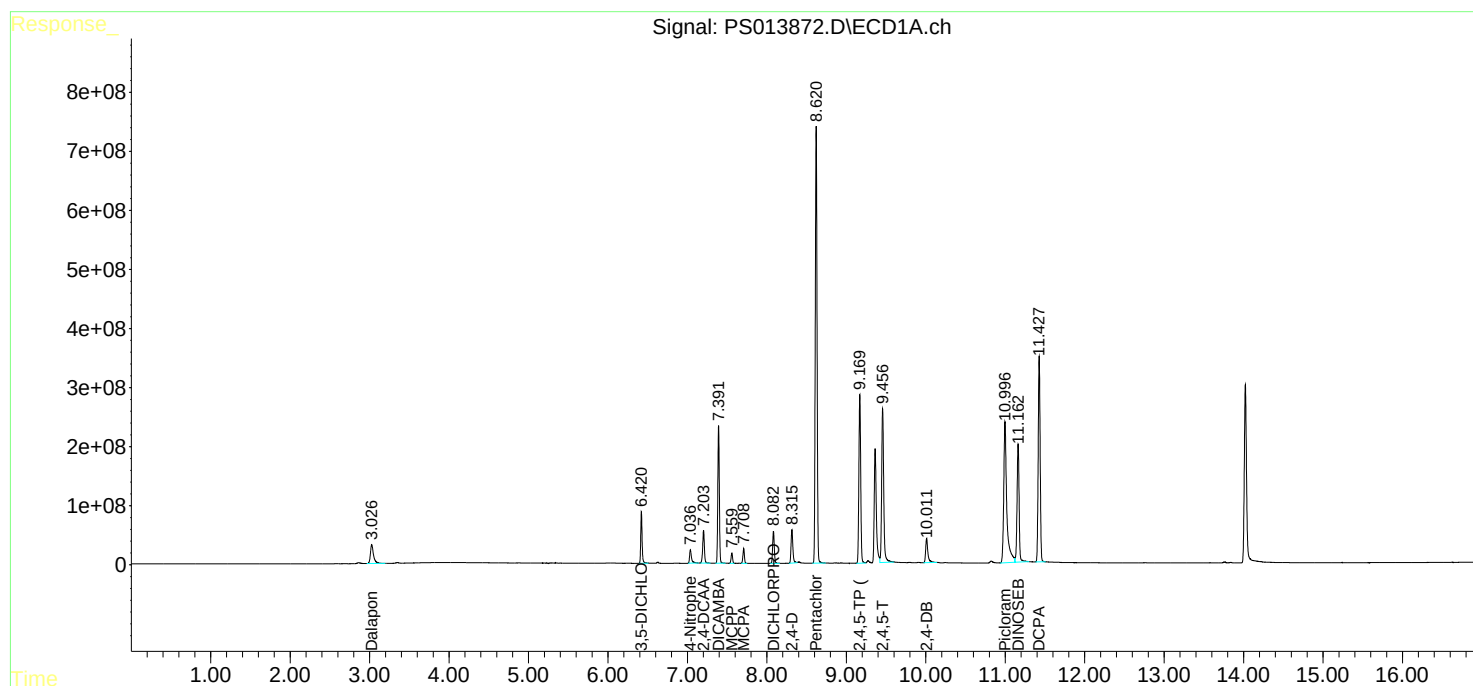


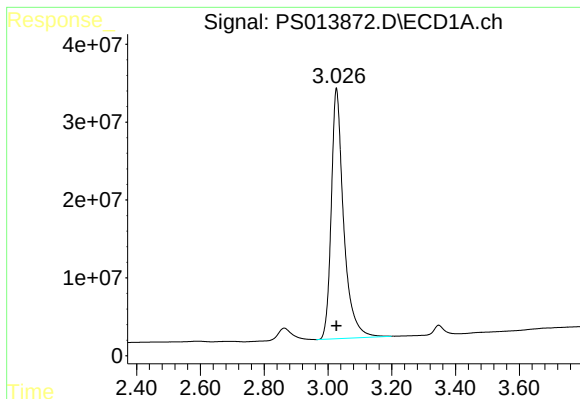

#1 Dalapon


R.T.: 3.026 min
Delta R.T.: 0.000 min
Response: 863720565
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

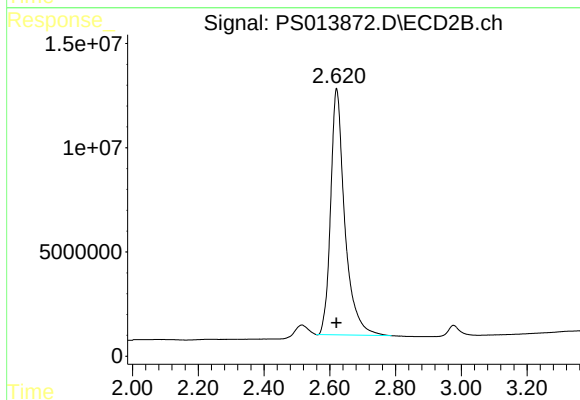


#1 Dalapon

R.T.: 2.621 min
Delta R.T.: 0.000 min
Response: 352741413
Conc: 682.50 ng/ml

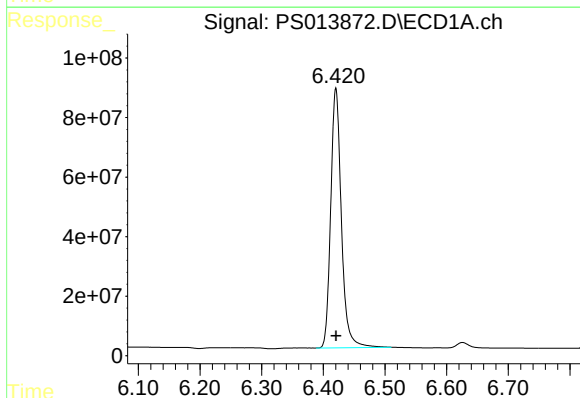


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.420 min
Delta R.T.: 0.000 min
Response: 1046503578
Conc: 697.50 ng/ml

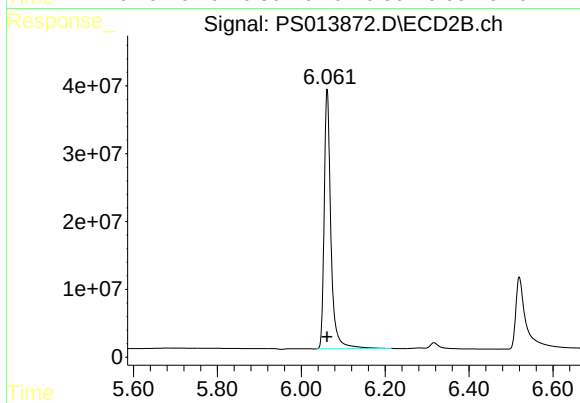

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.062 min
Delta R.T.: 0.000 min
Response: 424804959
Conc: 697.50 ng/ml

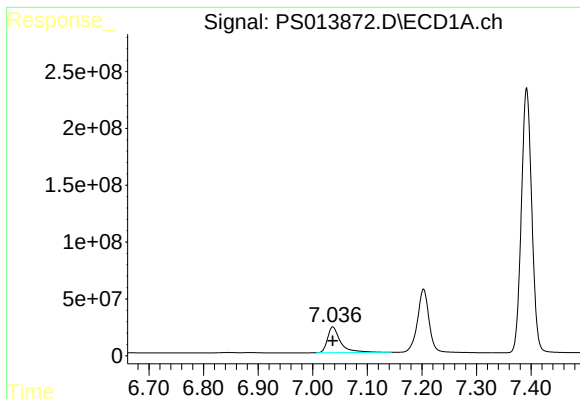

#3 4-Nitrophenol


R.T.: 7.037 min
Delta R.T.: 0.000 min
Response: 377019335
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

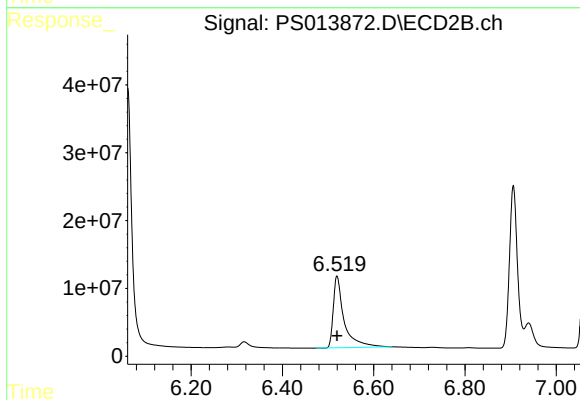


#3 4-Nitrophenol

R.T.: 6.520 min
Delta R.T.: 0.000 min
Response: 174945908
Conc: 682.50 ng/ml

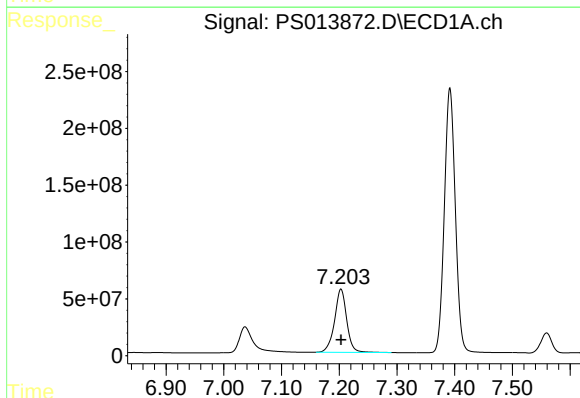


#4 2,4-DCAA

R.T.: 7.203 min
Delta R.T.: 0.000 min
Response: 812863858
Conc: 750.00 ng/ml

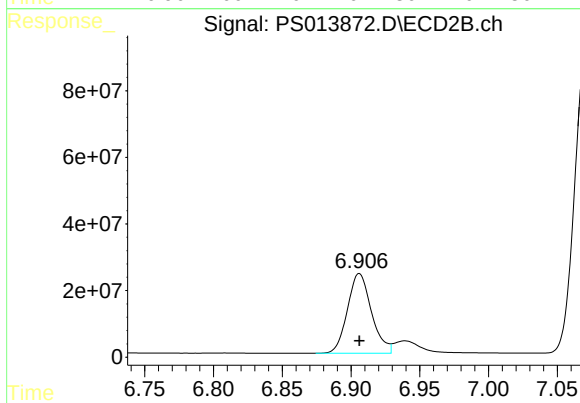

#4 2,4-DCAA


R.T.: 6.906 min
Delta R.T.: 0.000 min
Response: 290699065
Conc: 750.00 ng/ml

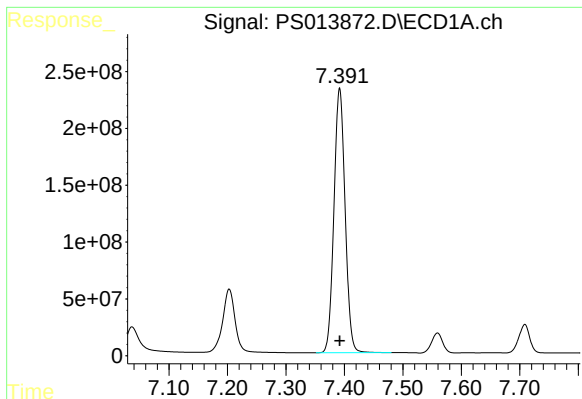

#5 DICAMBA


R.T.: 7.392 min
Delta R.T.: 0.000 min
Response: 3079049885
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

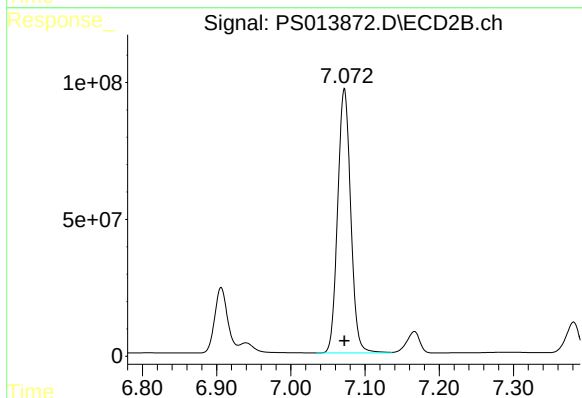


#5 DICAMBA

R.T.: 7.072 min
Delta R.T.: 0.000 min
Response: 1181346568
Conc: 705.00 ng/ml

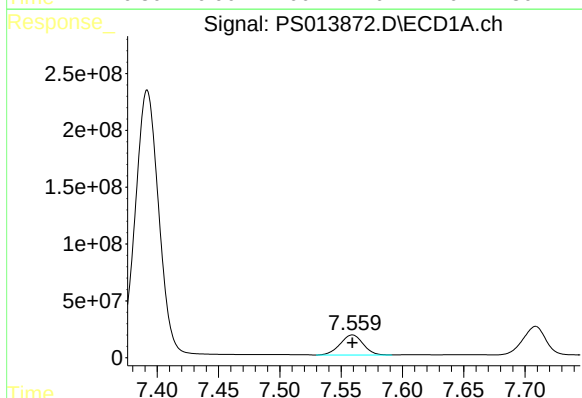


#6 MCP

R.T.: 7.559 min
Delta R.T.: 0.000 min
Response: 229850143
Conc: 70.50 ug/ml

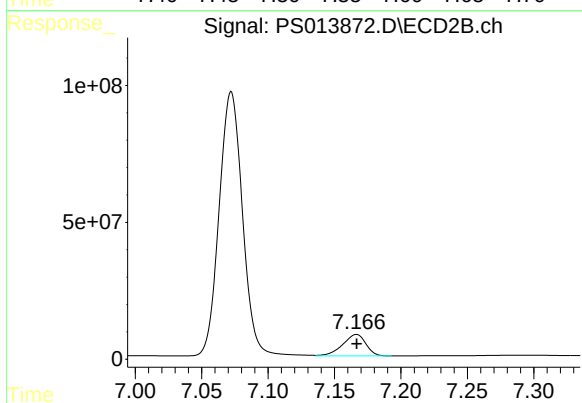

#6 MCP


R.T.: 7.167 min
Delta R.T.: 0.000 min
Response: 95708208
Conc: 70.50 ug/ml

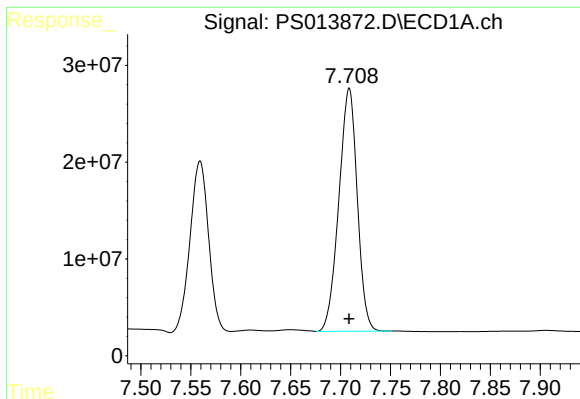

#7 MCPA


R.T.: 7.709 min
Delta R.T.: 0.000 min
Response: 322367105
Conc: 69.75 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

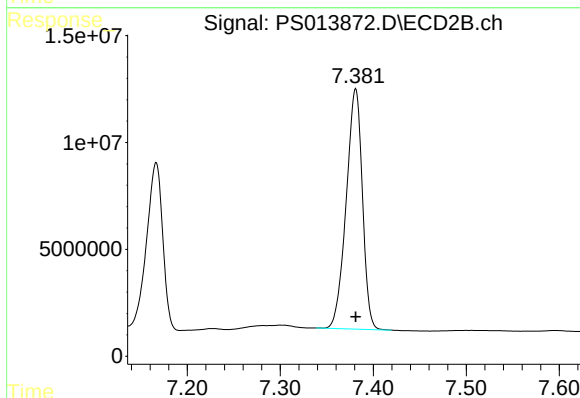


#7 MCPA

R.T.: 7.381 min
Delta R.T.: 0.000 min
Response: 135807103
Conc: 69.75 ug/ml

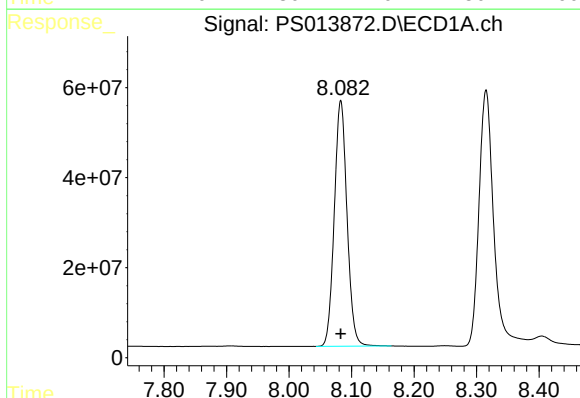


#8 DICHLORPROP

R.T.: 8.083 min
Delta R.T.: 0.000 min
Response: 770915917
Conc: 705.00 ng/ml

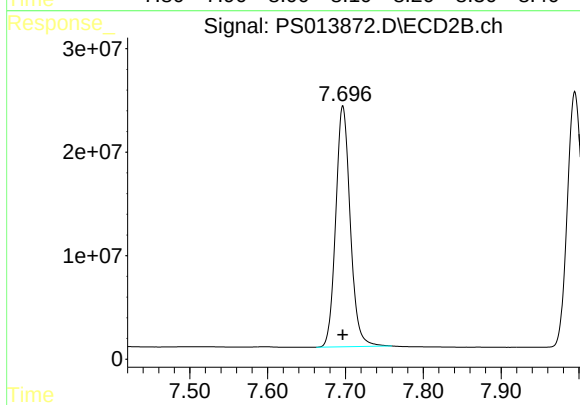

#8 DICHLORPROP


R.T.: 7.697 min
Delta R.T.: 0.000 min
Response: 301288156
Conc: 705.00 ng/ml

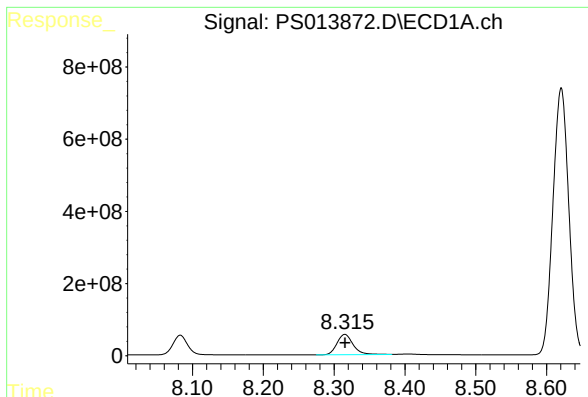

#9 2,4-D


R.T.: 8.315 min
Delta R.T.: 0.000 min
Response: 901594903
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

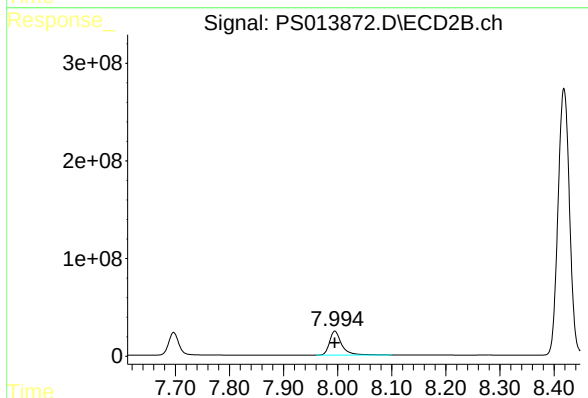


#9 2,4-D

R.T.: 7.995 min
Delta R.T.: 0.000 min
Response: 380203605
Conc: 705.00 ng/ml

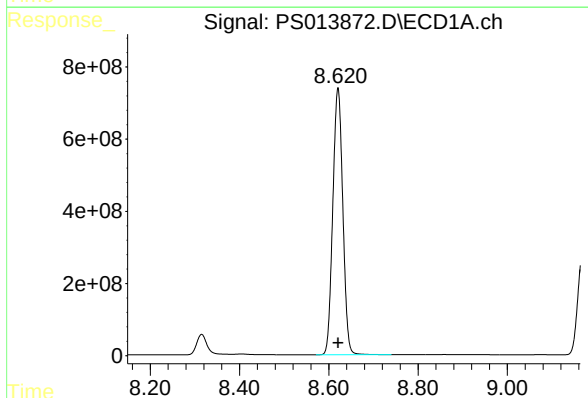


#10 Pentachlorophenol

R.T.: 8.621 min
Delta R.T.: 0.000 min
Response: 11488821472
Conc: 712.50 ng/ml

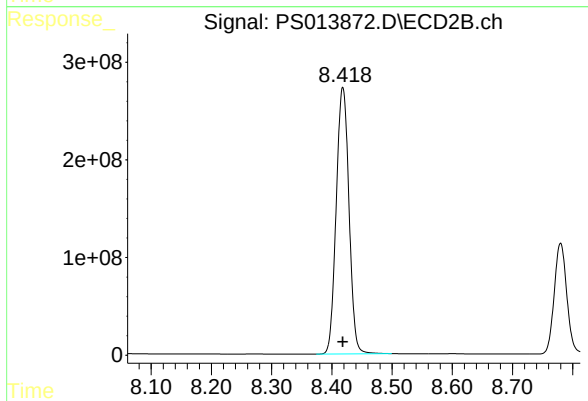

#10 Pentachlorophenol


R.T.: 8.418 min
Delta R.T.: 0.000 min
Response: 4022421898
Conc: 712.50 ng/ml

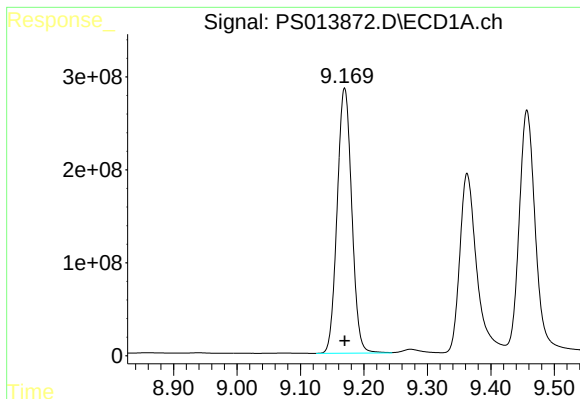

#11 2,4,5-TP (SILVEX)


R.T.: 9.170 min
Delta R.T.: 0.000 min
Response: 4549984468
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

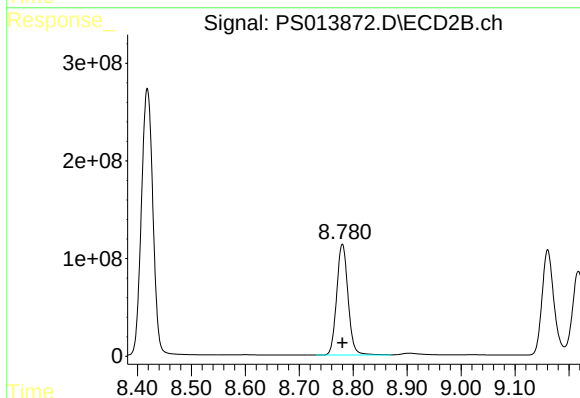


#11 2,4,5-TP (SILVEX)

R.T.: 8.780 min
Delta R.T.: 0.000 min
Response: 1665592732
Conc: 712.50 ng/ml

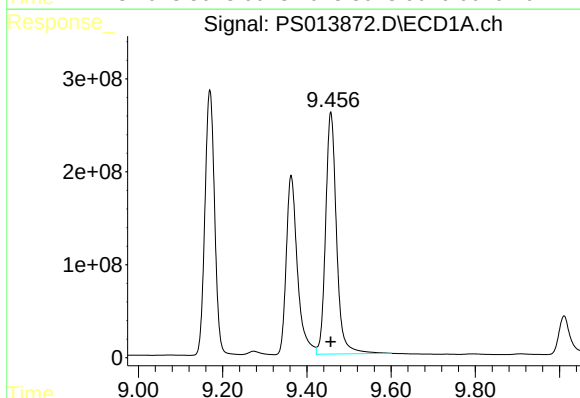


#12 2,4,5-T

R.T.: 9.457 min
Delta R.T.: 0.000 min
Response: 4684578497
Conc: 712.50 ng/ml

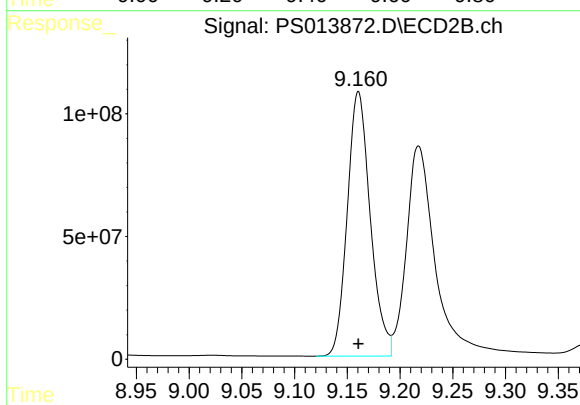

#12 2,4,5-T


R.T.: 9.161 min
Delta R.T.: 0.000 min
Response: 1633712183
Conc: 712.50 ng/ml

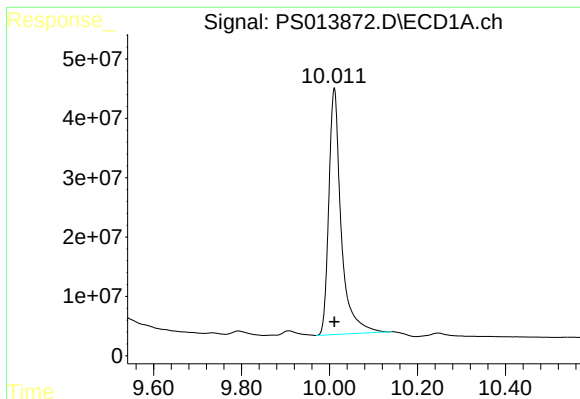

#13 2,4-DB


R.T.: 10.011 min
Delta R.T.: 0.000 min
Response: 808478737
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

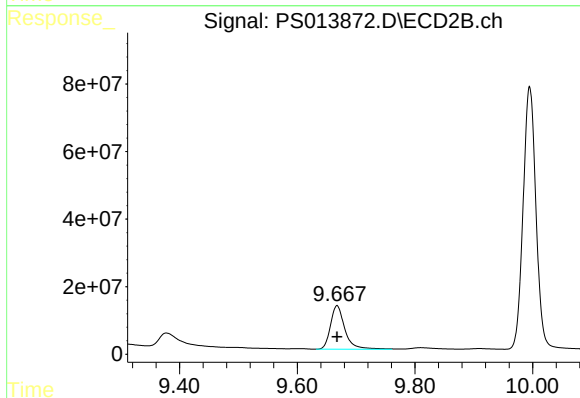


#13 2,4-DB

R.T.: 9.668 min
Delta R.T.: 0.000 min
Response: 219780674
Conc: 712.50 ng/ml

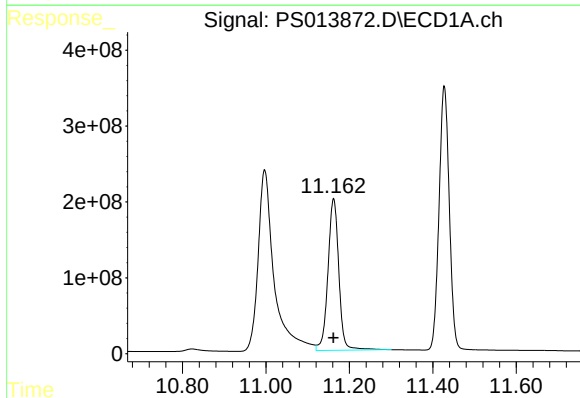


#14 DINOSEB

R.T.: 11.162 min
Delta R.T.: 0.000 min
Response: 3621684248
Conc: 705.00 ng/ml

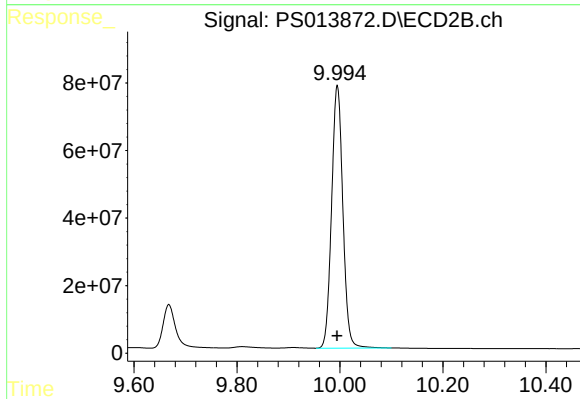

#14 DINOSEB


R.T.: 9.995 min
Delta R.T.: 0.000 min
Response: 1179717355
Conc: 705.00 ng/ml

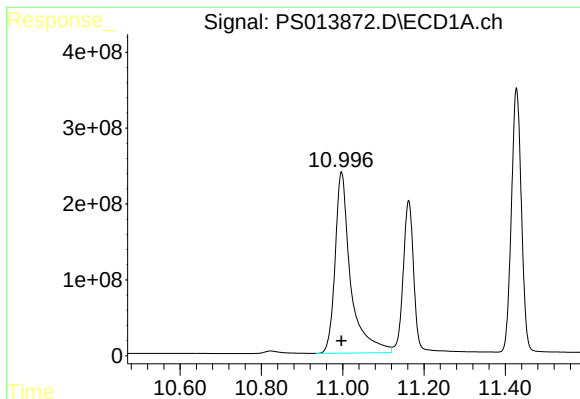

#15 Picloram


R.T.: 10.997 min
Delta R.T.: 0.000 min
Response: 6338504570
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

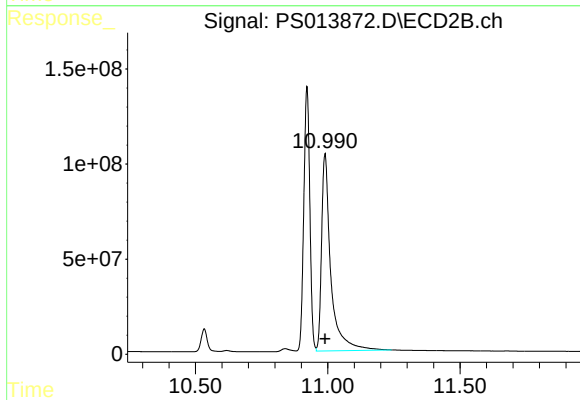


#15 Picloram

R.T.: 10.990 min
Delta R.T.: 0.000 min
Response: 2522770240
Conc: 712.50 ng/ml

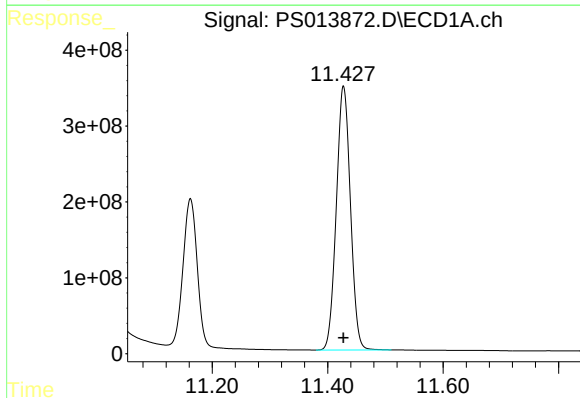

#16 DCPA

R.T.: 11.427 min
Delta R.T.: 0.000 min
Response: 5912610983
Conc: 720.00 ng/ml

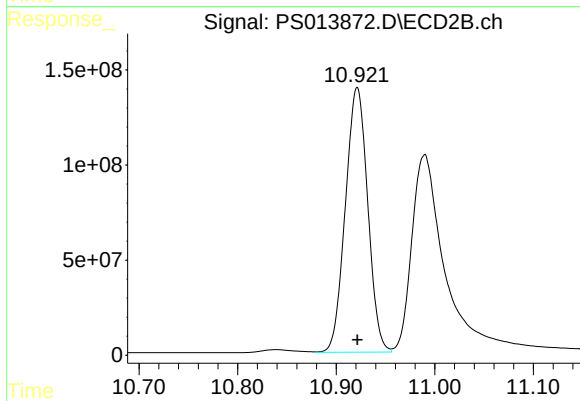

#16 DCPA

R.T.: 10.921 min
Delta R.T.: 0.000 min
Response: 2194188986
Conc: 720.00 ng/ml