

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012721\
 Data File : PS013877.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jan 2021 20:30
 Operator : DD\AJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDCCC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 28 01:03:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012721.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 28 01:00:30 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.204	6.906	830.2E6	297.8E6	771.656	772.123
Target Compounds							
1) T	Dalapon	3.027	2.621	868.8E6	356.4E6	696.136	693.184
2) T	3,5-DICHL...	6.421	6.062	1063.3E6	435.4E6	715.499	717.071
3) T	4-Nitroph...	7.038	6.520	378.4E6	176.0E6	696.454	699.726
5) T	DICAMBA	7.393	7.072	3141.0E6	1207.4E6	730.502	732.660
6) T	MCPD	7.560	7.167	234.9E6	98274517	74.449	73.170
7) T	MCPA	7.709	7.382	331.4E6	141.4E6	73.229	72.928
8) T	DICHLORPROP	8.084	7.697	785.7E6	309.0E6	722.863	726.234
9) T	2,4-D	8.316	7.995	914.0E6	387.3E6	744.372	726.498
10) T	Pentachlo...	8.622	8.419	11593.4E6	4099.7E6	732.075	735.937
11) T	2,4,5-TP ...	9.170	8.780	4620.2E6	1701.3E6	735.831	741.151
12) T	2,4,5-T	9.458	9.161	4710.1E6	1666.0E6	731.255	748.180
13) T	2,4-DB	10.011	9.667	824.6E6	220.6E6	746.996	737.833
14) T	DINOSEB	11.162	9.994	3557.7E6	1169.1E6	701.998	715.607
15) T	Picloram	10.996	10.989	6522.4E6	2589.7E6	768.142	758.841
16) T	DCPA	11.428	10.921	5971.4E6	2234.0E6	738.678	745.685



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012721\
Data File : PS013877.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jan 2021 20:30
Operator : DD\AJ
Sample : HSTDCCC750
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 28 01:03:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012721.M
Quant Title : 8080.M
QLast Update : Thu Jan 28 01:00:30 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

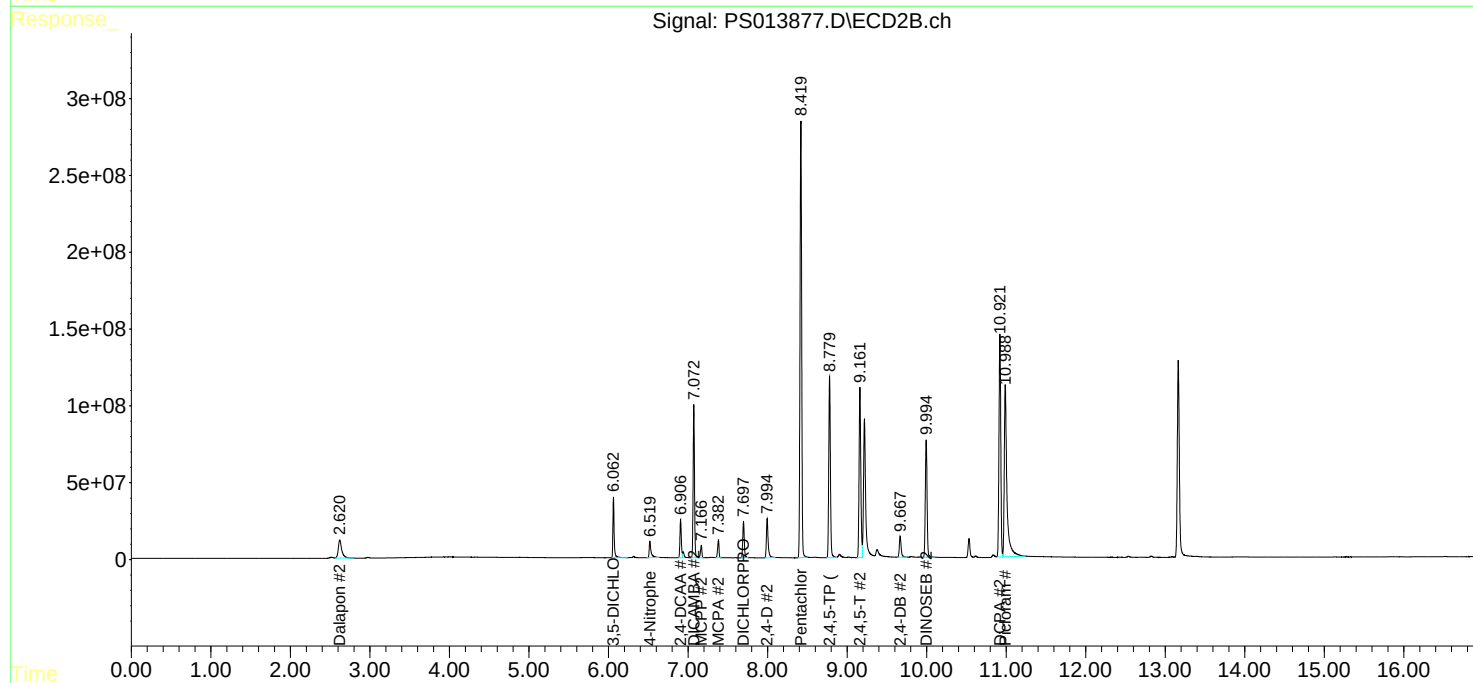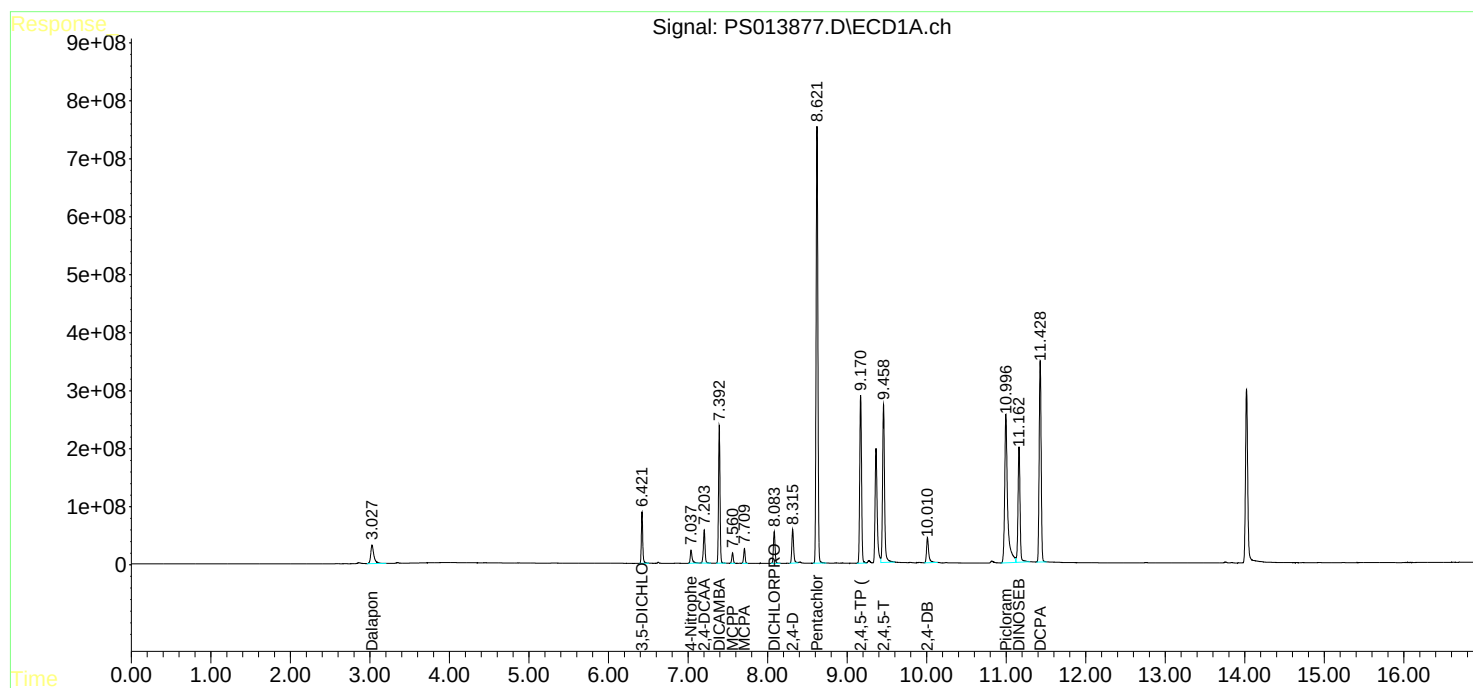


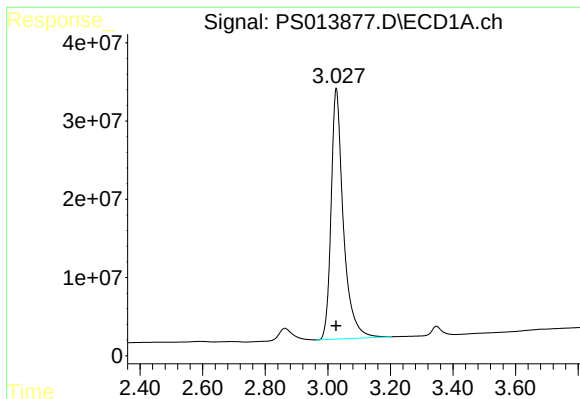

#1 Dalapon


R.T.: 3.027 min
Delta R.T.: 0.000 min
Response: 868831953
Conc: 696.14 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

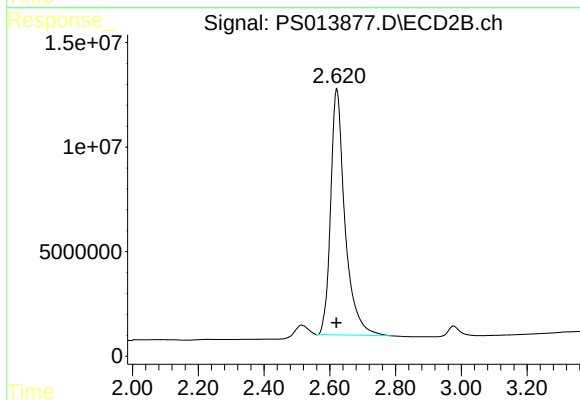


#1 Dalapon

R.T.: 2.621 min
Delta R.T.: 0.000 min
Response: 356408365
Conc: 693.18 ng/ml

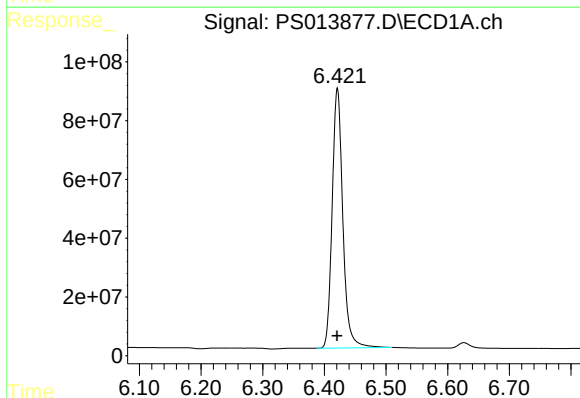


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.421 min
Delta R.T.: 0.000 min
Response: 1063258280
Conc: 715.50 ng/ml

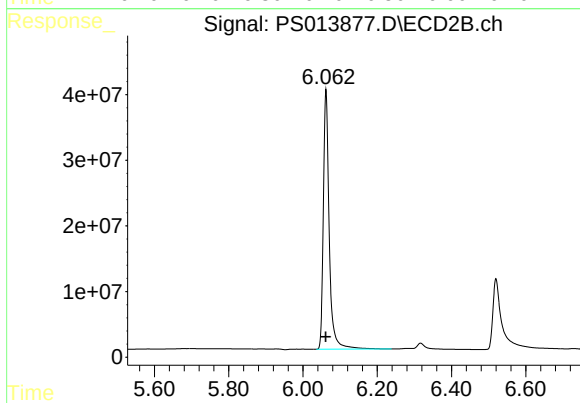

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.062 min
Delta R.T.: 0.000 min
Response: 435366302
Conc: 717.07 ng/ml

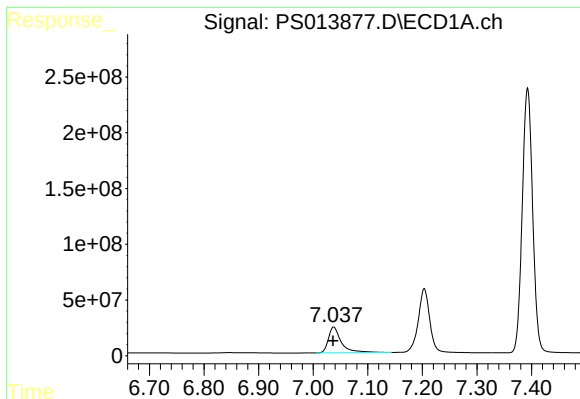

#3 4-Nitrophenol


R.T.: 7.038 min
Delta R.T.: 0.000 min
Response: 378441179
Conc: 696.45 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

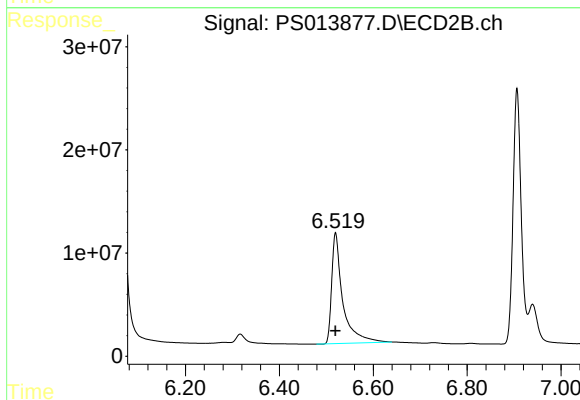


#3 4-Nitrophenol

R.T.: 6.520 min
Delta R.T.: 0.000 min
Response: 175963395
Conc: 699.73 ng/ml

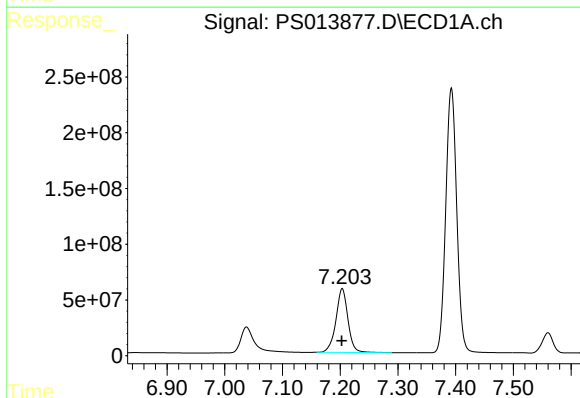


#4 2,4-DCAA

R.T.: 7.204 min
Delta R.T.: 0.000 min
Response: 830190459
Conc: 771.66 ng/ml

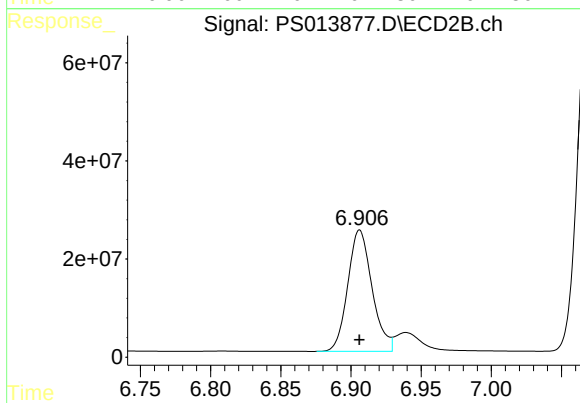

#4 2,4-DCAA


R.T.: 6.906 min
Delta R.T.: 0.000 min
Response: 297848776
Conc: 772.12 ng/ml

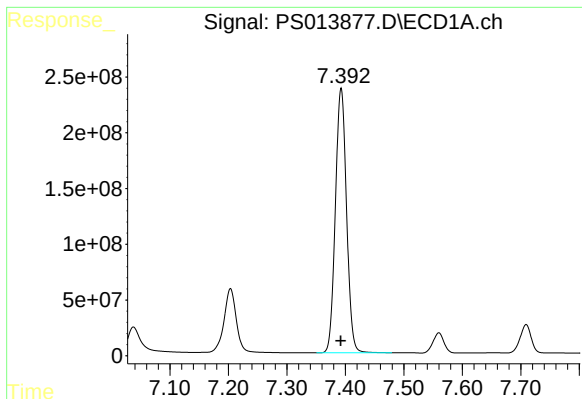

#5 DICAMBA


R.T.: 7.393 min
Delta R.T.: 0.000 min
Response: 3140988295
Conc: 730.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

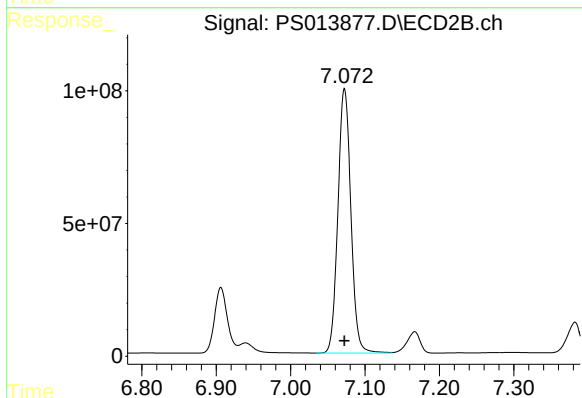


#5 DICAMBA

R.T.: 7.072 min
Delta R.T.: 0.000 min
Response: 1207387052
Conc: 732.66 ng/ml

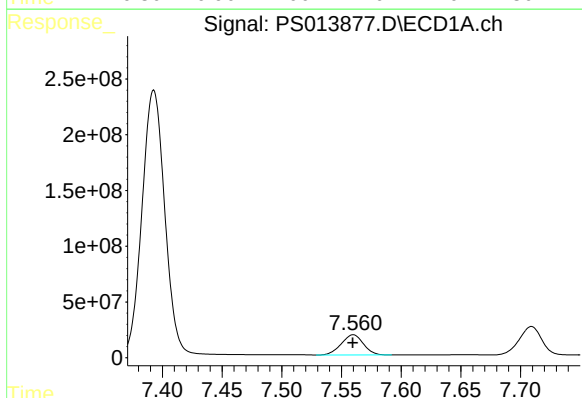


#6 MCP

R.T.: 7.560 min
Delta R.T.: 0.000 min
Response: 234933496
Conc: 74.45 ug/ml

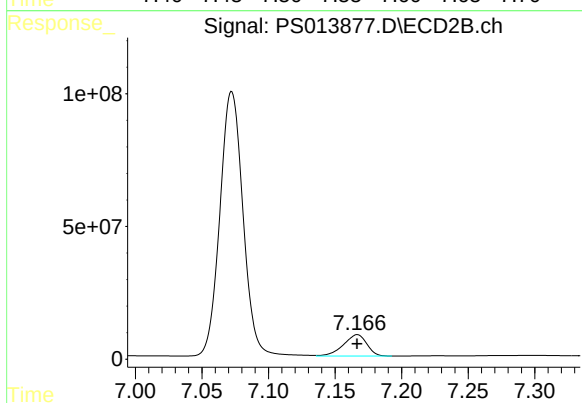

#6 MCP


R.T.: 7.167 min
Delta R.T.: 0.000 min
Response: 98274517
Conc: 73.17 ug/ml

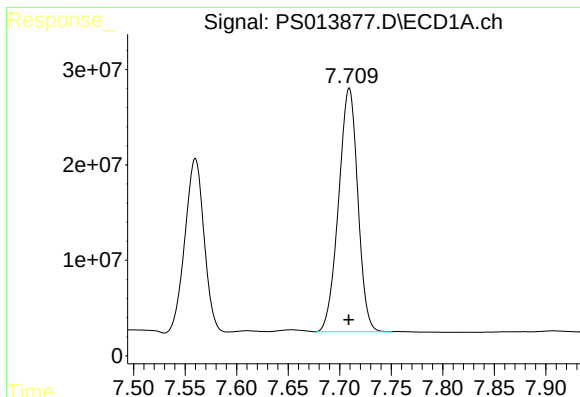

#7 MCPA


R.T.: 7.709 min
Delta R.T.: 0.000 min
Response: 331420657
Conc: 73.23 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

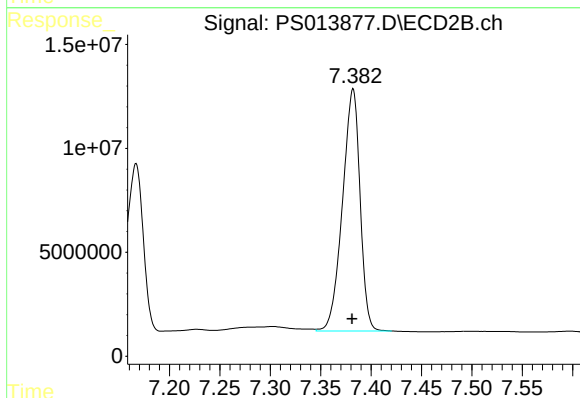


#7 MCPA

R.T.: 7.382 min
Delta R.T.: 0.001 min
Response: 141374459
Conc: 72.93 ug/ml

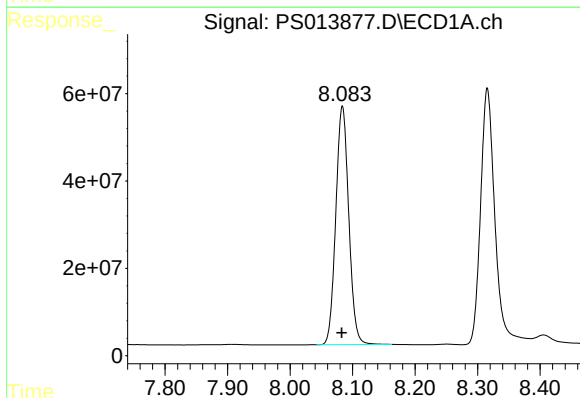


#8 DICHLORPROP

R.T.: 8.084 min
Delta R.T.: 0.000 min
Response: 785697735
Conc: 722.86 ng/ml

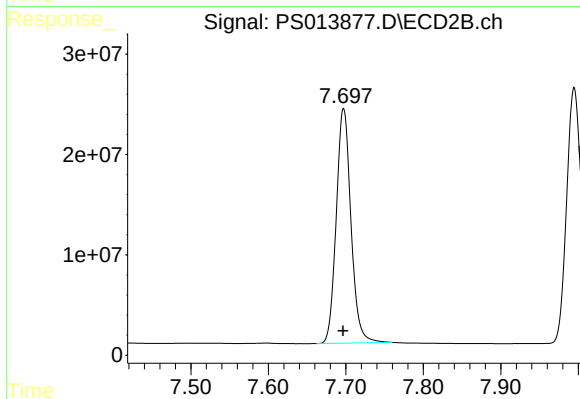

#8 DICHLORPROP


R.T.: 7.697 min
Delta R.T.: 0.000 min
Response: 308996880
Conc: 726.23 ng/ml

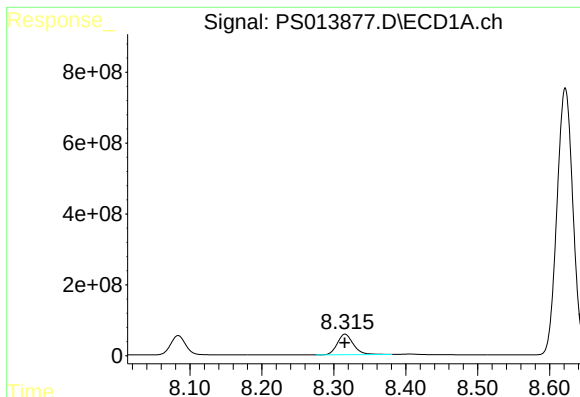

#9 2,4-D


R.T.: 8.316 min
Delta R.T.: 0.000 min
Response: 914003565
Conc: 744.37 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

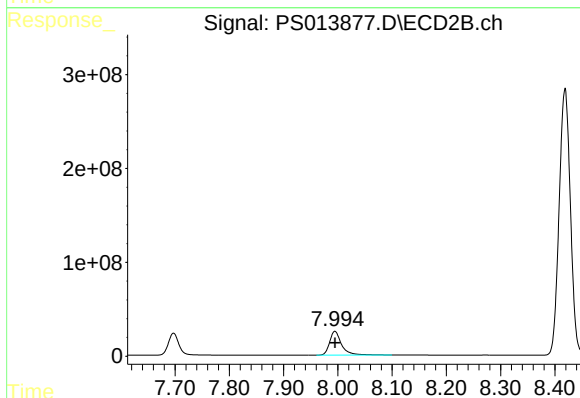


#9 2,4-D

R.T.: 7.995 min
Delta R.T.: 0.000 min
Response: 387258866
Conc: 726.50 ng/ml

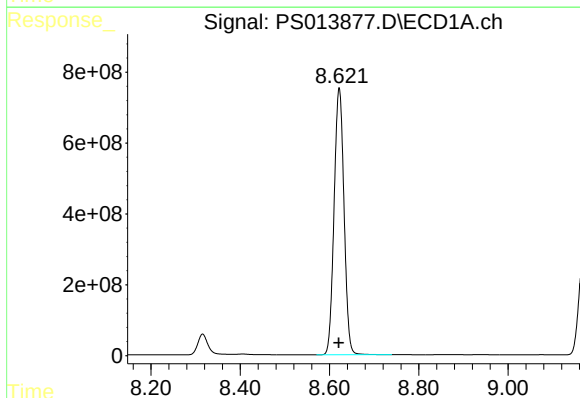


#10 Pentachlorophenol

R.T.: 8.622 min
Delta R.T.: 0.001 min
Response: 11593421698
Conc: 732.08 ng/ml

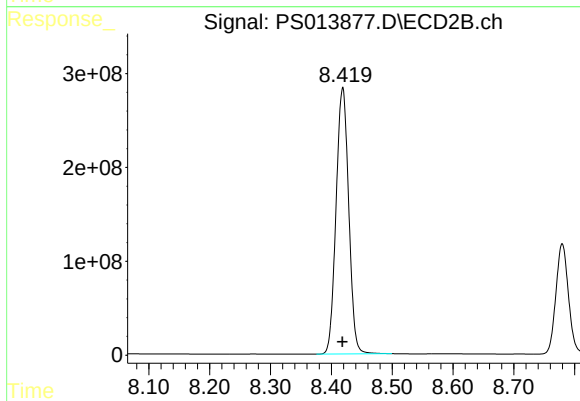

#10 Pentachlorophenol


R.T.: 8.419 min
Delta R.T.: 0.000 min
Response: 4099677561
Conc: 735.94 ng/ml

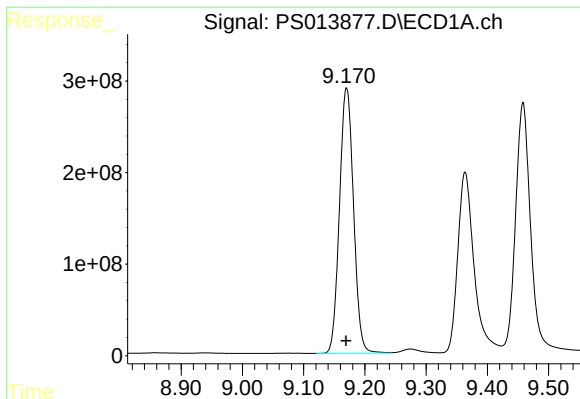

#11 2,4,5-TP (SILVEX)


R.T.: 9.170 min
Delta R.T.: 0.000 min
Response: 4620212319
Conc: 735.83 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

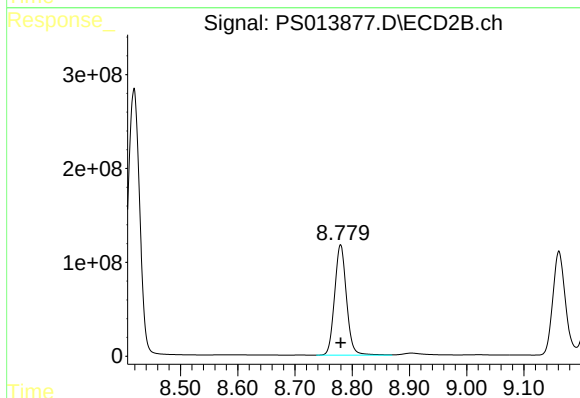


#11 2,4,5-TP (SILVEX)

R.T.: 8.780 min
Delta R.T.: 0.000 min
Response: 1701326269
Conc: 741.15 ng/ml

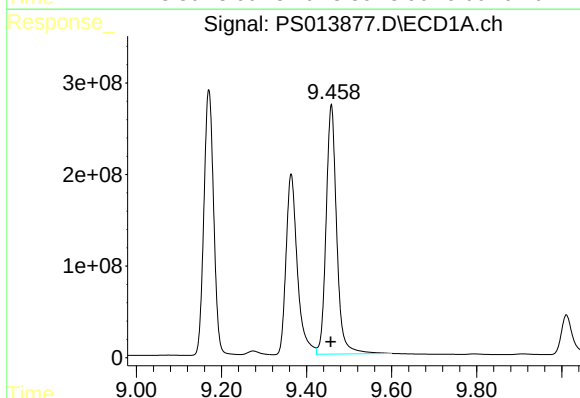


#12 2,4,5-T

R.T.: 9.458 min
Delta R.T.: 0.001 min
Response: 4710102947
Conc: 731.25 ng/ml

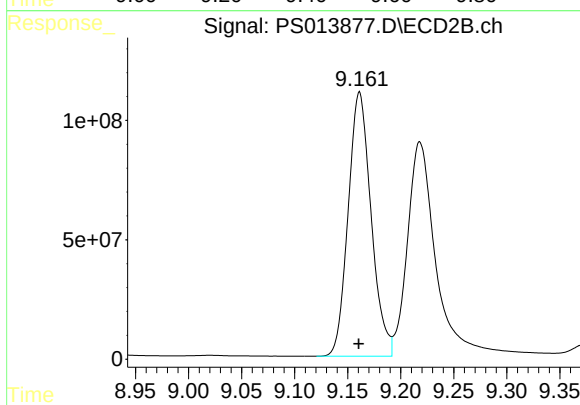

#12 2,4,5-T


R.T.: 9.161 min
Delta R.T.: 0.000 min
Response: 1666008760
Conc: 748.18 ng/ml

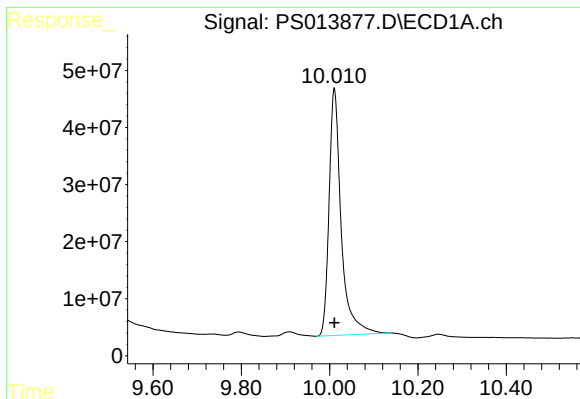

#13 2,4-DB


R.T.: 10.011 min
Delta R.T.: 0.000 min
Response: 824575943
Conc: 747.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

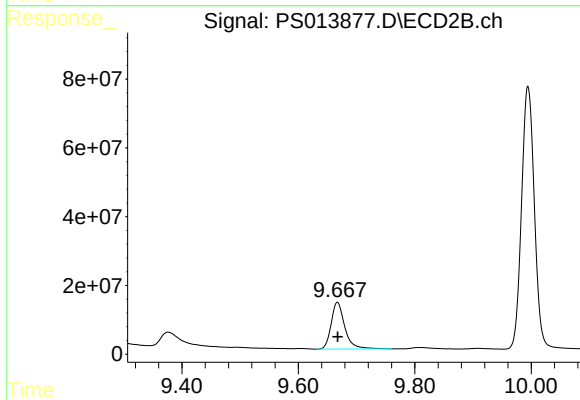


#13 2,4-DB

R.T.: 9.667 min
Delta R.T.: 0.000 min
Response: 220625152
Conc: 737.83 ng/ml

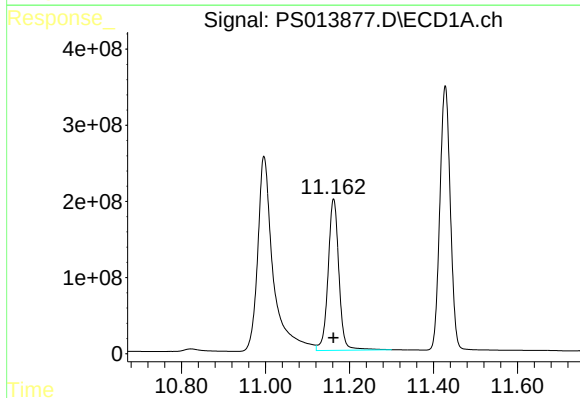


#14 DINOSEB

R.T.: 11.162 min
Delta R.T.: 0.000 min
Response: 3557731148
Conc: 702.00 ng/ml

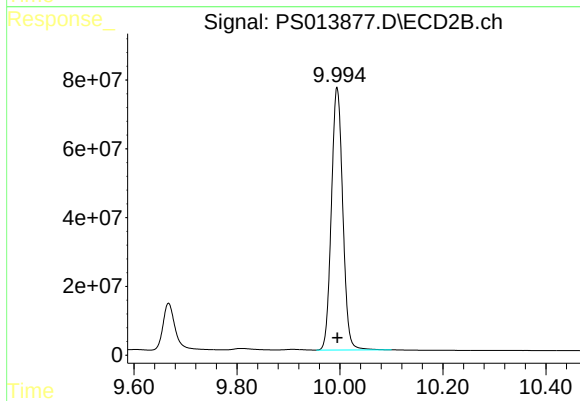

#14 DINOSEB


R.T.: 9.994 min
Delta R.T.: 0.000 min
Response: 1169094157
Conc: 715.61 ng/ml

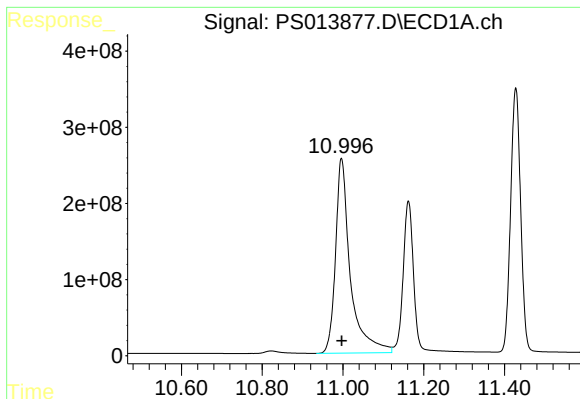

#15 Picloram


R.T.: 10.996 min
Delta R.T.: 0.000 min
Response: 6522400427
Conc: 768.14 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

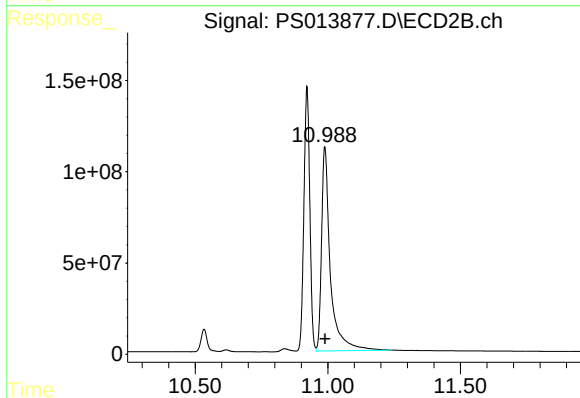


#15 Picloram

R.T.: 10.989 min
Delta R.T.: -0.001 min
Response: 2589657350
Conc: 758.84 ng/ml

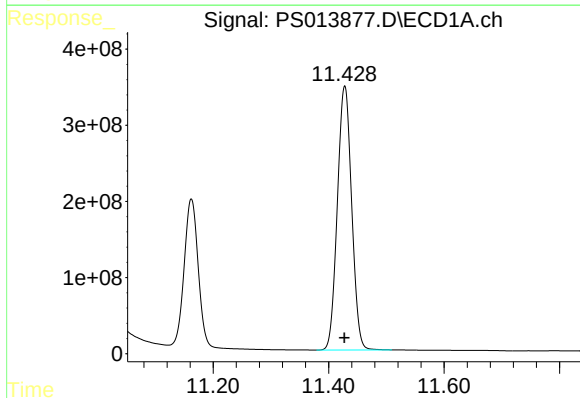

#16 DCPA

R.T.: 11.428 min
Delta R.T.: 0.000 min
Response: 5971377988
Conc: 738.68 ng/ml

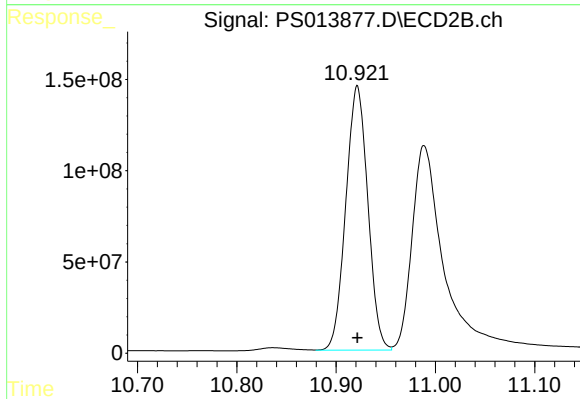

#16 DCPA

R.T.: 10.921 min
Delta R.T.: 0.000 min
Response: 2233988022
Conc: 745.68 ng/ml