

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012722\
 Data File : PS018140.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jan 2022 08:44
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 28 00:26:06 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 06 10:21:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
5) T	DICAMBA	7.232	0.000	8572780	0	1.373	N.D. #
8) T	DICHLORPROP	7.919	0.000	4074905	0	2.590	N.D. #
9) T	2,4-D	8.149	0.000	7703102	0	4.230	N.D. #
10) T	Pentachlo...	8.444	8.113	20551067	8205293	<MDL	<MDL #
11) T	2,4,5-TP ...	8.995	8.475	35779975	5256074	4.228	1.474 #
12) T	2,4,5-T	9.279	8.857	37226380	13486856	4.200	4.123
13) T	2,4-DB	9.822	0.000	28550545	0	17.272	N.D. #
14) T	DINOSEB	10.971	0.000	18524603	0	2.821	N.D. #
15) T	Picloram	10.801	10.662	436.5E6	137.1E6	36.573	29.318
16) T	DCPA	11.238	10.600	25637216	9802182	2.373	2.220



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS012722\
Data File : PS018140.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jan 2022 08:44
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 28 00:26:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS010522.M
Quant Title : 8080.M
QLast Update : Thu Jan 06 10:21:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

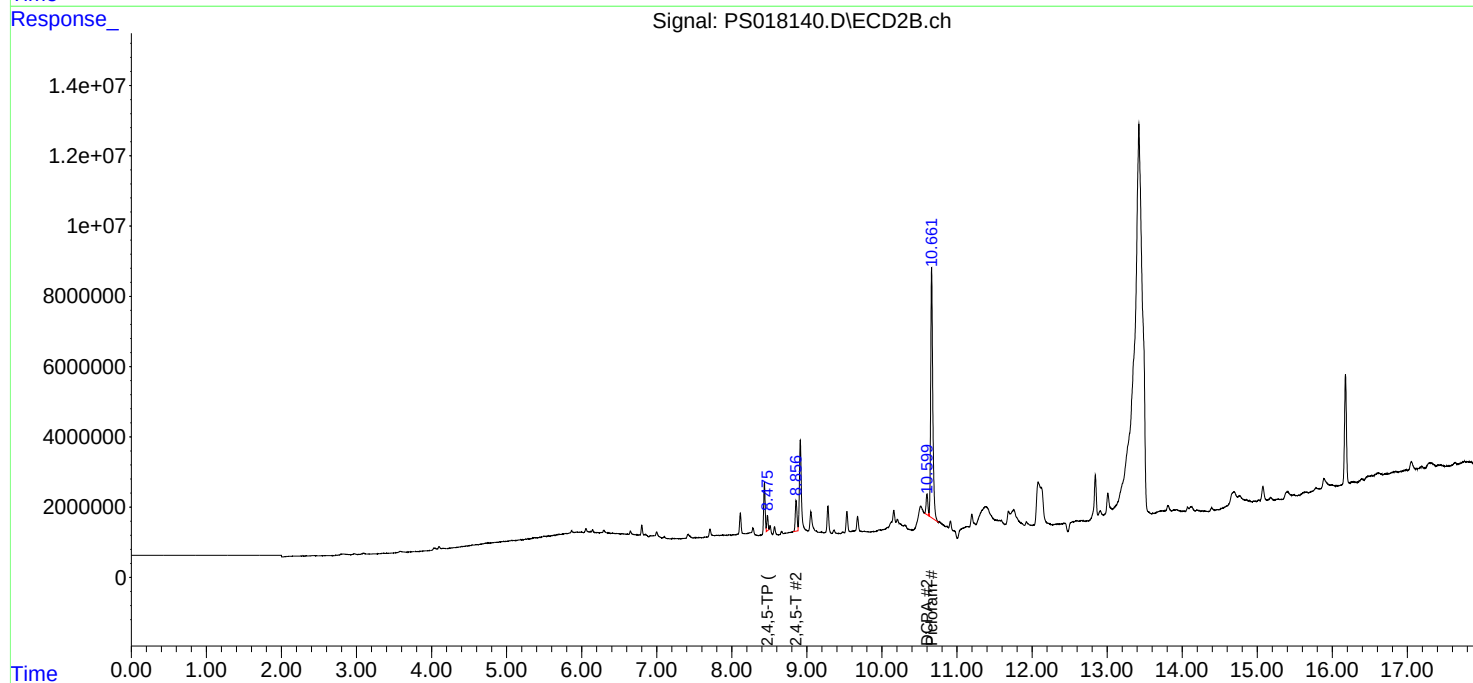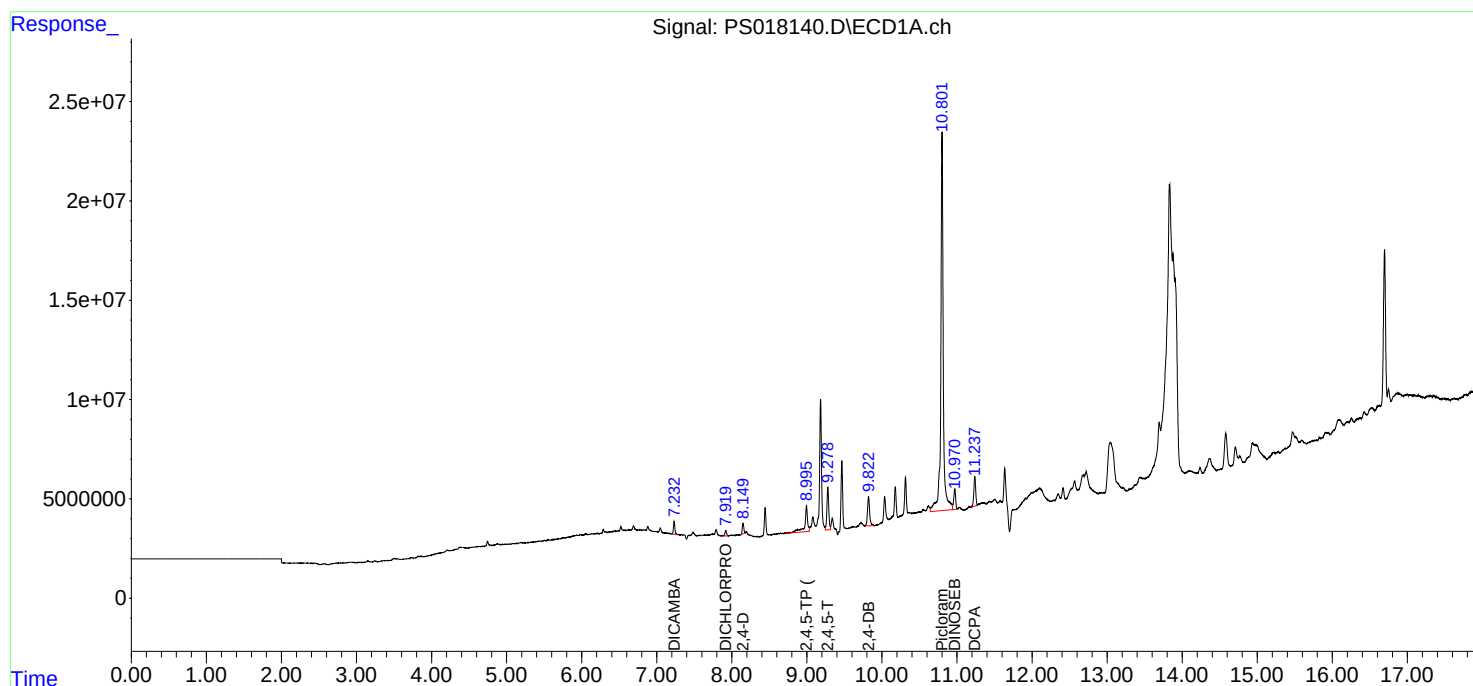


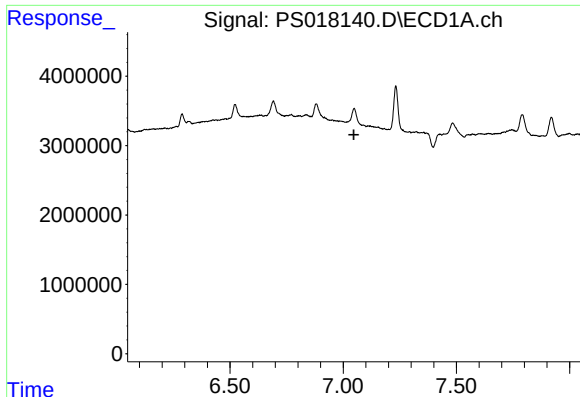

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 7.047 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

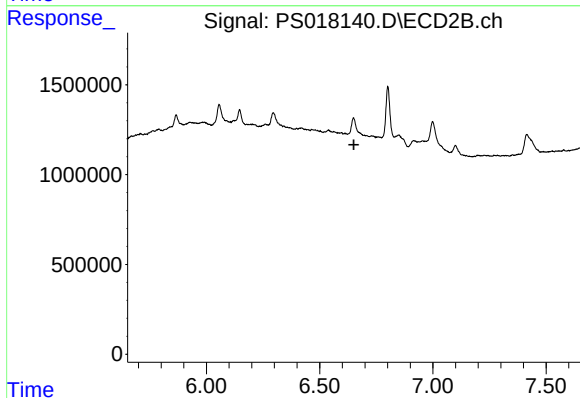


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.651 min
Response: 0
Conc: N.D.

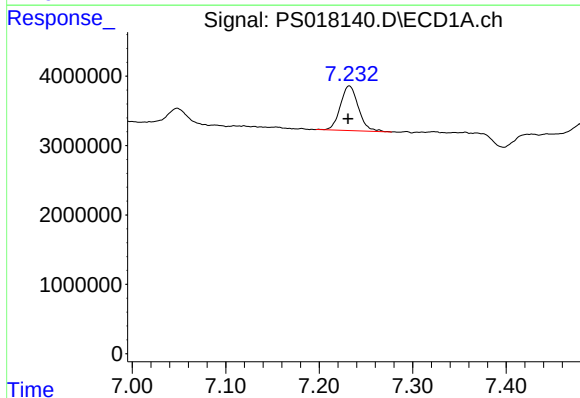


#5 DICAMBA

R.T.: 7.232 min
Delta R.T.: 0.001 min
Response: 8572780
Conc: 1.37 ng/ml

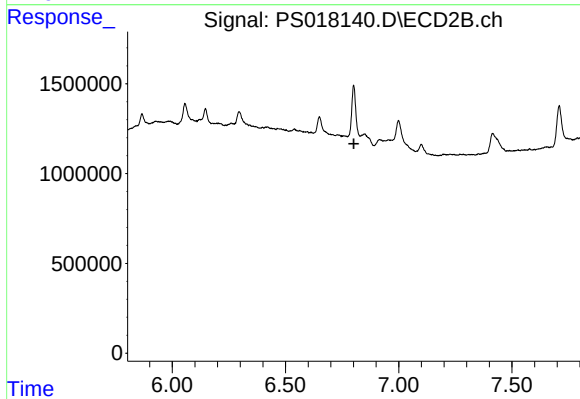

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 6.802 min
Response: 0
Conc: N.D.

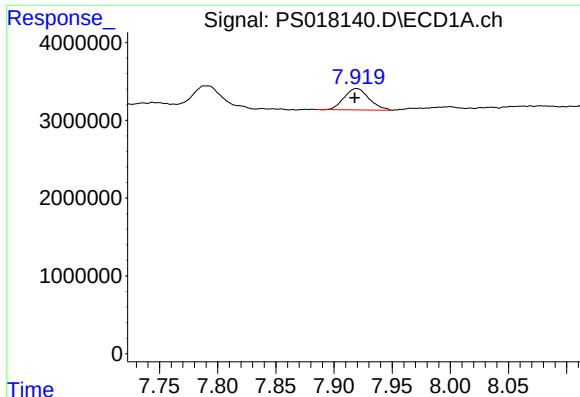

#8 DICHLORPROP


R.T.: 7.919 min
Delta R.T.: 0.001 min
Response: 4074905
Conc: 2.59 ng/ml

Instrument :
ECD_S
ClientSampleId :

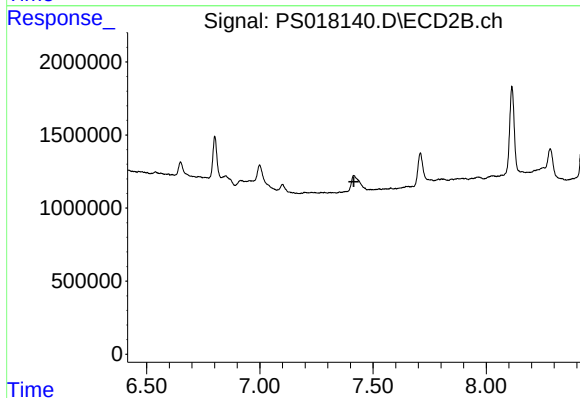


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 7.415 min
Response: 0
Conc: N.D.

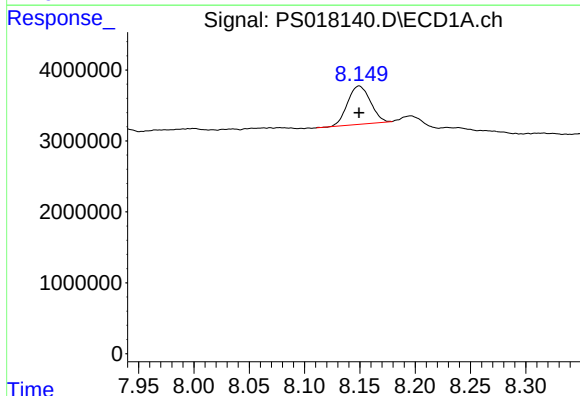


#9 2,4-D

R.T.: 8.149 min
Delta R.T.: 0.000 min
Response: 7703102
Conc: 4.23 ng/ml

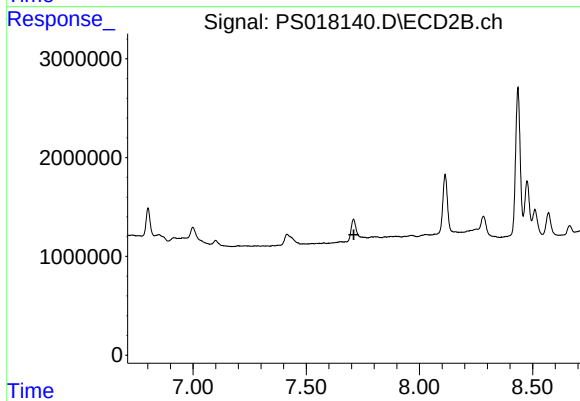

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.710 min
Response: 0
Conc: N.D.

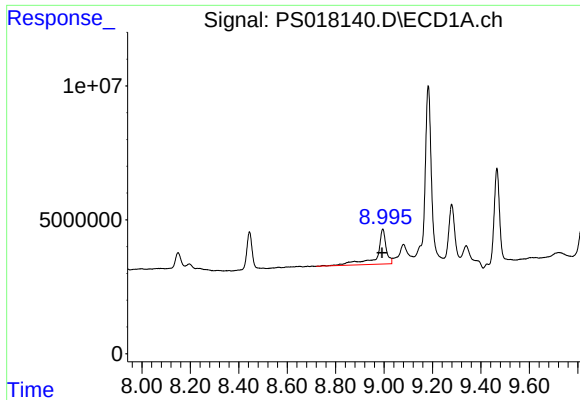

#11 2,4,5-TP (SILVEX)


R.T.: 8.995 min
Delta R.T.: 0.003 min
Response: 35779975
Conc: 4.23 ng/ml

Instrument :
ECD_S
ClientSampleId :

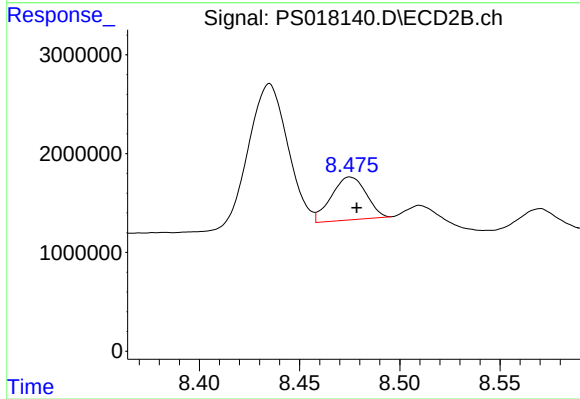


#11 2,4,5-TP (SILVEX)

R.T.: 8.475 min
Delta R.T.: -0.003 min
Response: 5256074
Conc: 1.47 ng/ml

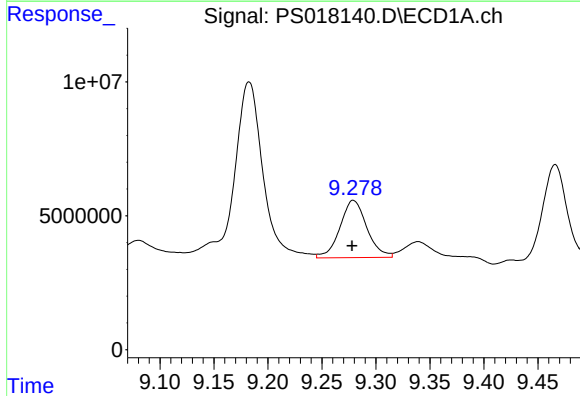


#12 2,4,5-T

R.T.: 9.279 min
Delta R.T.: 0.001 min
Response: 37226380
Conc: 4.20 ng/ml

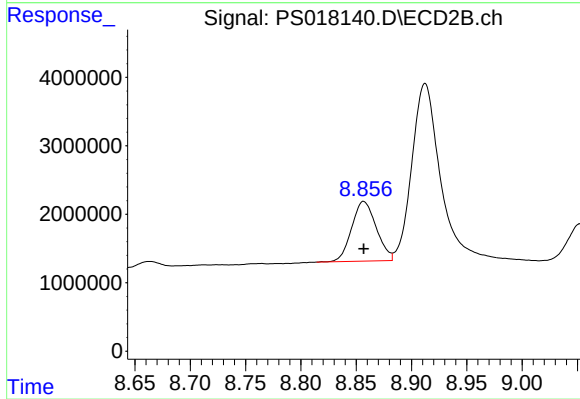

#12 2,4,5-T


R.T.: 8.857 min
Delta R.T.: 0.000 min
Response: 13486856
Conc: 4.12 ng/ml

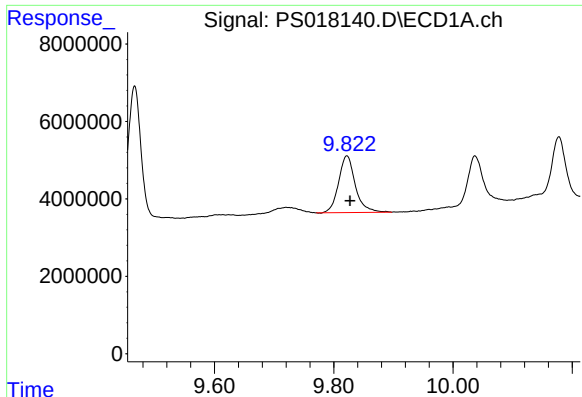

#13 2,4-DB


R.T.: 9.822 min
Delta R.T.: -0.005 min
Response: 28550545
Conc: 17.27 ng/ml

Instrument :
ECD_S
ClientSampleId :

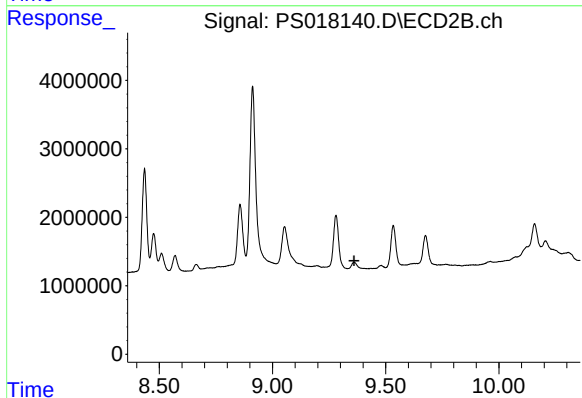


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.360 min
Response: 0
Conc: N.D.

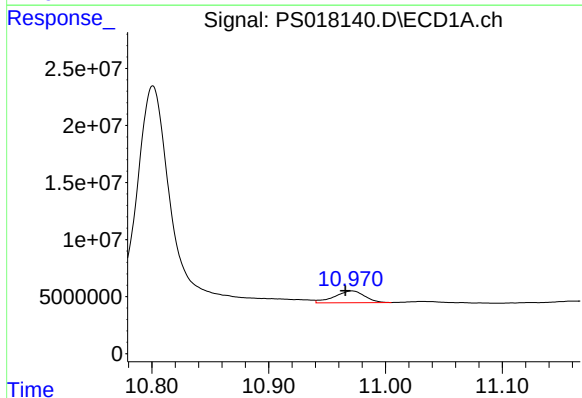


#14 DINOSEB

R.T.: 10.971 min
Delta R.T.: 0.005 min
Response: 18524603
Conc: 2.82 ng/ml

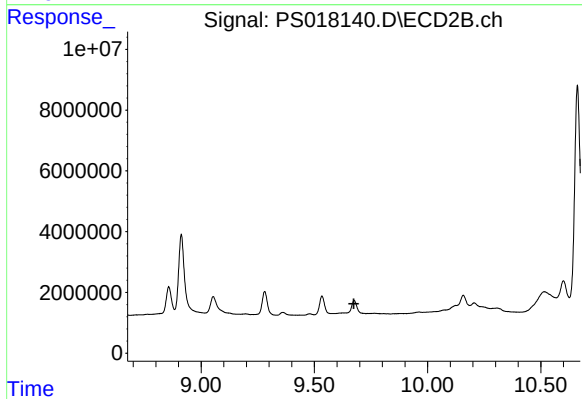

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.675 min
Response: 0
Conc: N.D.

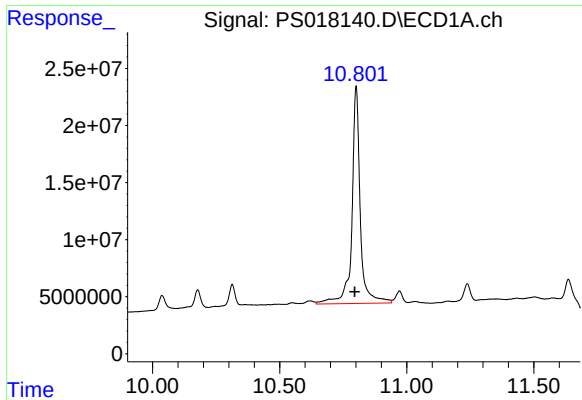

#15 Picloram


R.T.: 10.801 min
Delta R.T.: 0.005 min
Response: 436535298
Conc: 36.57 ng/ml

Instrument :
ECD_S
ClientSampleId :

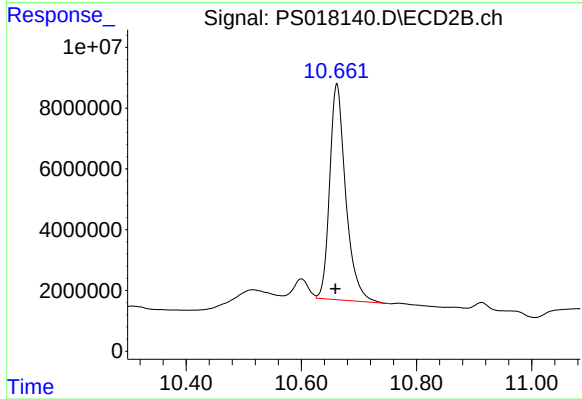


#15 Picloram

R.T.: 10.662 min
Delta R.T.: 0.003 min
Response: 137095856
Conc: 29.32 ng/ml

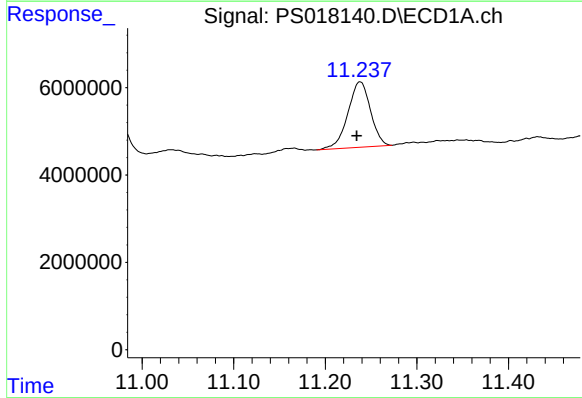

#16 DCPA

R.T.: 11.238 min
Delta R.T.: 0.004 min
Response: 25637216
Conc: 2.37 ng/ml

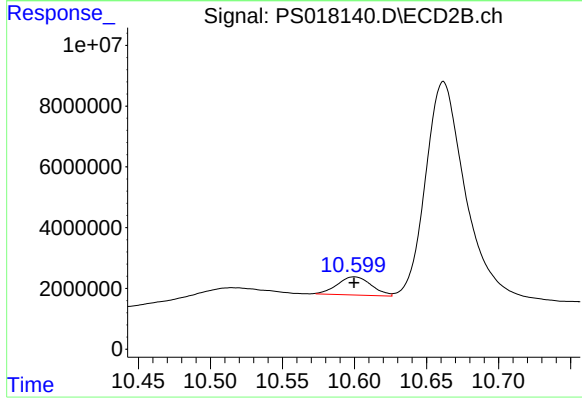

#16 DCPA

R.T.: 10.600 min
Delta R.T.: 0.000 min
Response: 9802182
Conc: 2.22 ng/ml